


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080918\
 Data File : VN050475.D
 Acq On : 9 Aug 2018 9:52
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
 Title : SW846 8260
 Last Update : Tue Aug 07 05:22:15 2018

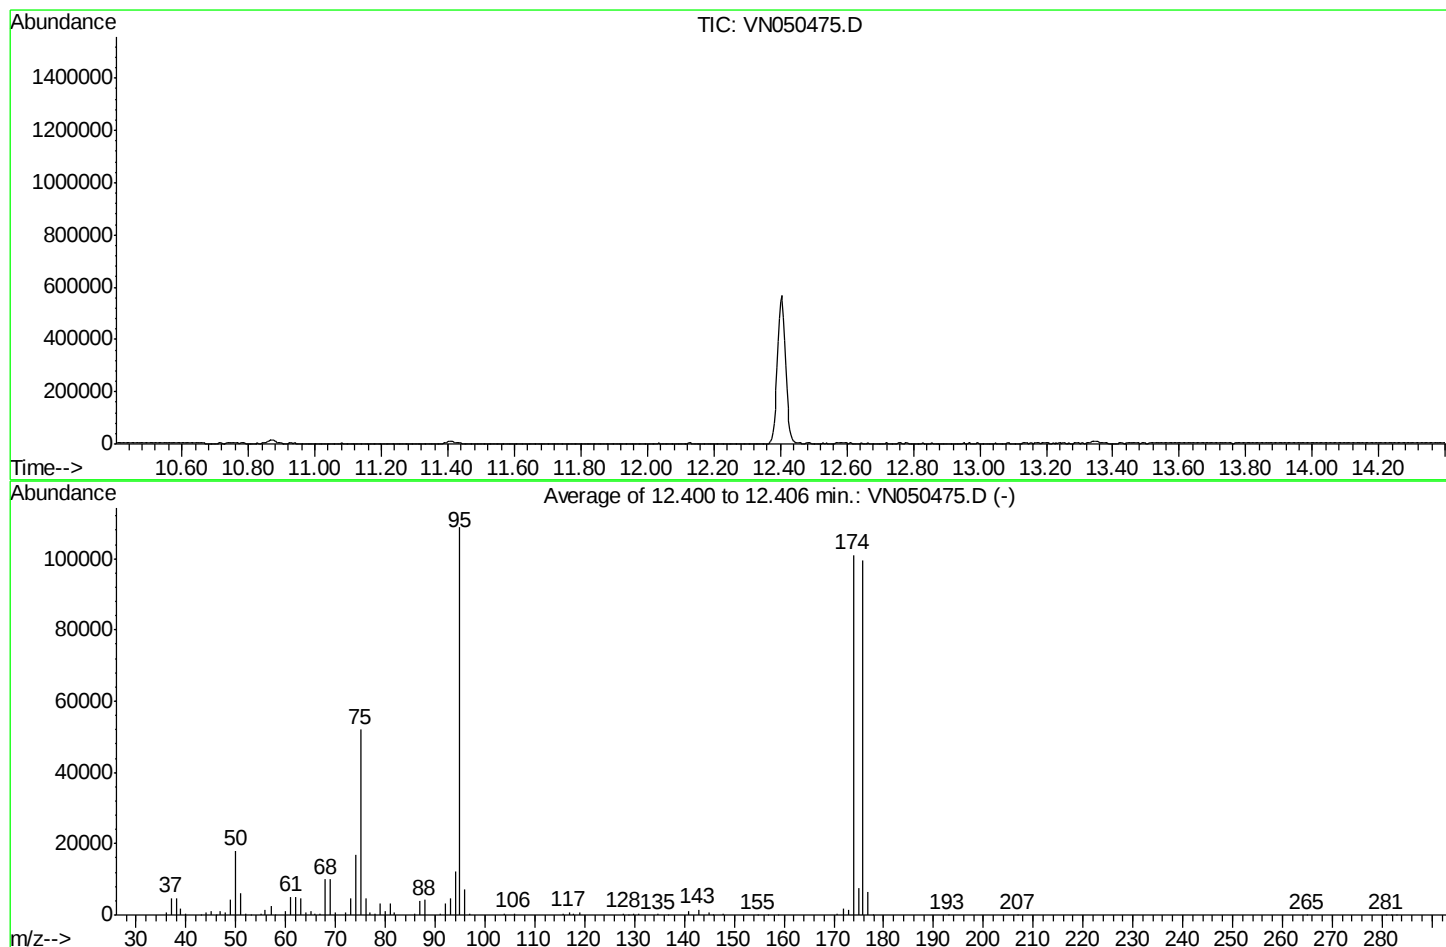

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	18133	PASS
75	95	30	60	47.8	52005	PASS
95	95	100	100	100.0	108797	PASS
96	95	5	9	6.6	7151	PASS
173	174	0.00	2	1.3	1306	PASS
174	95	50	100	92.9	101098	PASS
175	174	5	9	7.6	7720	PASS
176	174	95	101	98.3	99389	PASS
177	176	5	9	6.4	6395	PASS