


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080918\
 Data File : VN050498.D
 Acq On : 9 Aug 2018 20:49
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N072518W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jul 26 15:21:50 2018

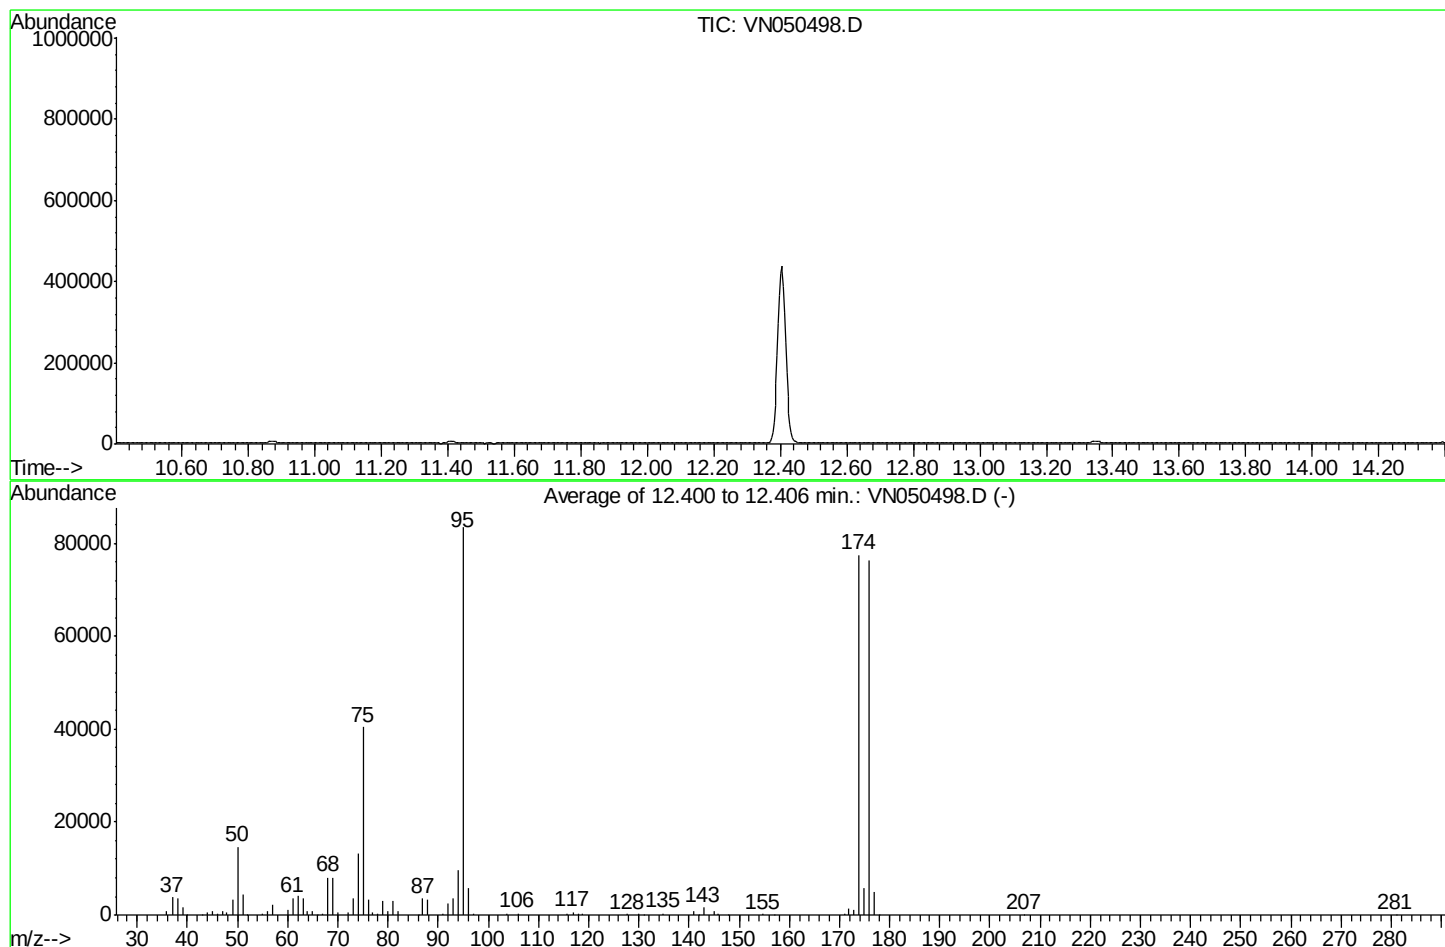

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3350

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	14696	PASS
75	95	30	60	48.5	40498	PASS
95	95	100	100	100.0	83434	PASS
96	95	5	9	7.0	5848	PASS
173	174	0.00	2	1.3	1036	PASS
174	95	50	100	92.9	77490	PASS
175	174	5	9	7.6	5927	PASS
176	174	95	101	98.5	76352	PASS
177	176	5	9	6.6	5022	PASS