


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080919\
 Data File : VN057134.D
 Acq On : 9 Aug 2019 9:30
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
 Title : SW846 8260
 Last Update : Thu Aug 08 06:49:25 2019

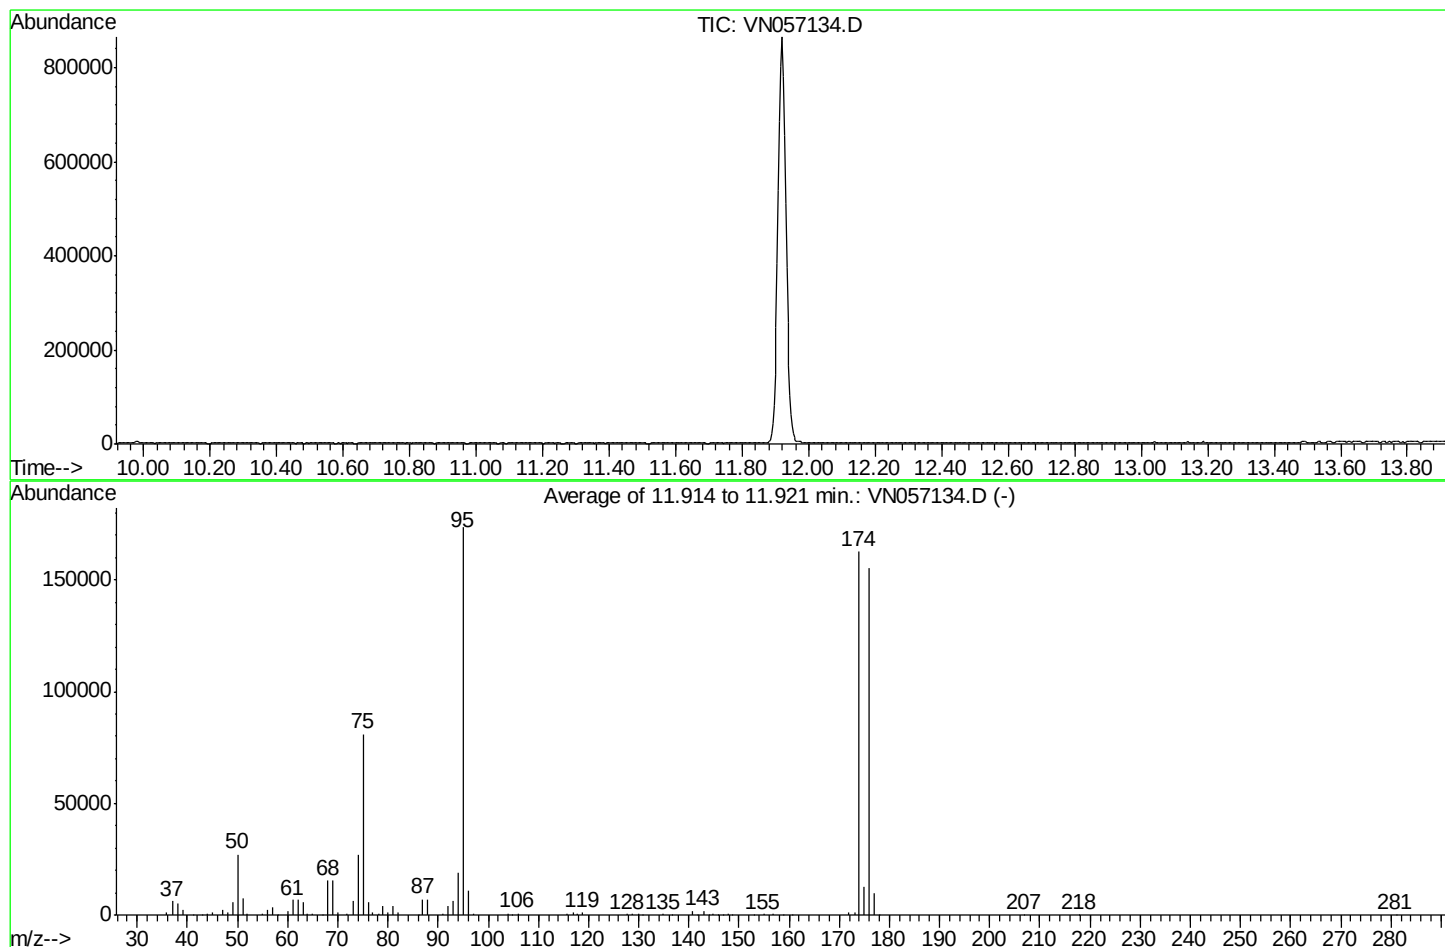

AutoFind: Scans 3154, 3155, 3156; Background Corrected with Scan 3140

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	27082	PASS
75	95	30	60	46.6	80853	PASS
95	95	100	100	100.0	173568	PASS
96	95	5	9	6.1	10643	PASS
173	174	0.00	2	0.8	1339	PASS
174	95	50	100	93.6	162538	PASS
175	174	5	9	7.6	12406	PASS
176	174	95	101	95.7	155520	PASS
177	176	5	9	6.2	9632	PASS