
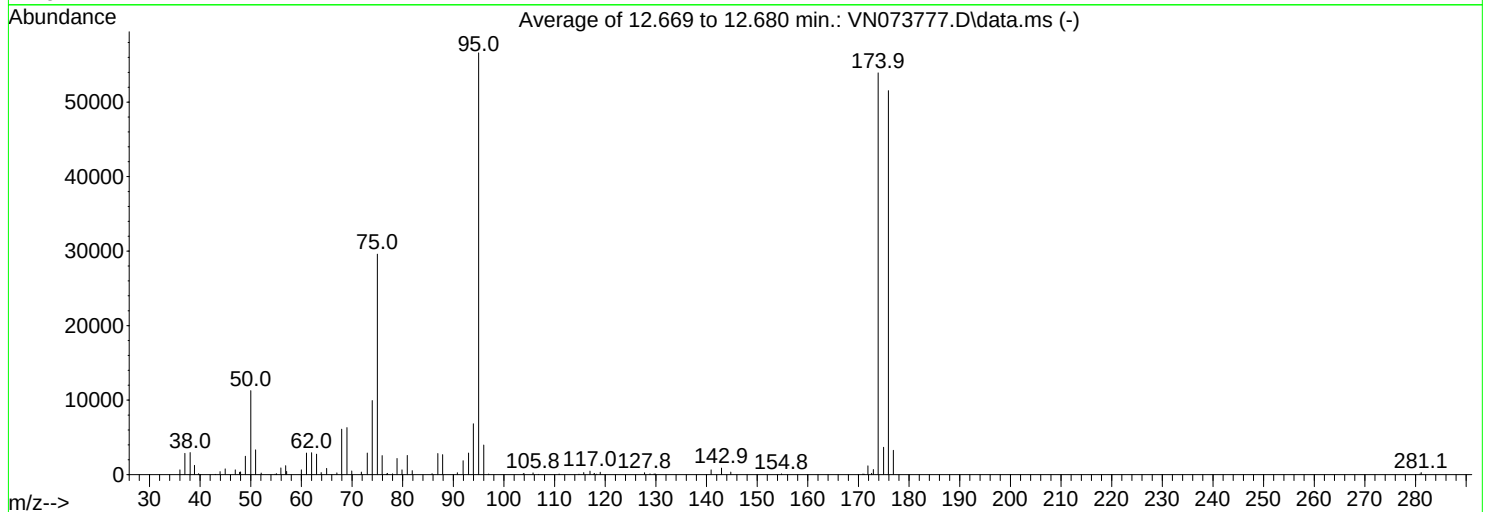


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN080922\  
Data File : VN073777.D  
Acq On : 09 Aug 2022 09:26  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N072822W.M  
Title : SW846 8260  
Last Update : Wed Aug 10 05:09:32 2022

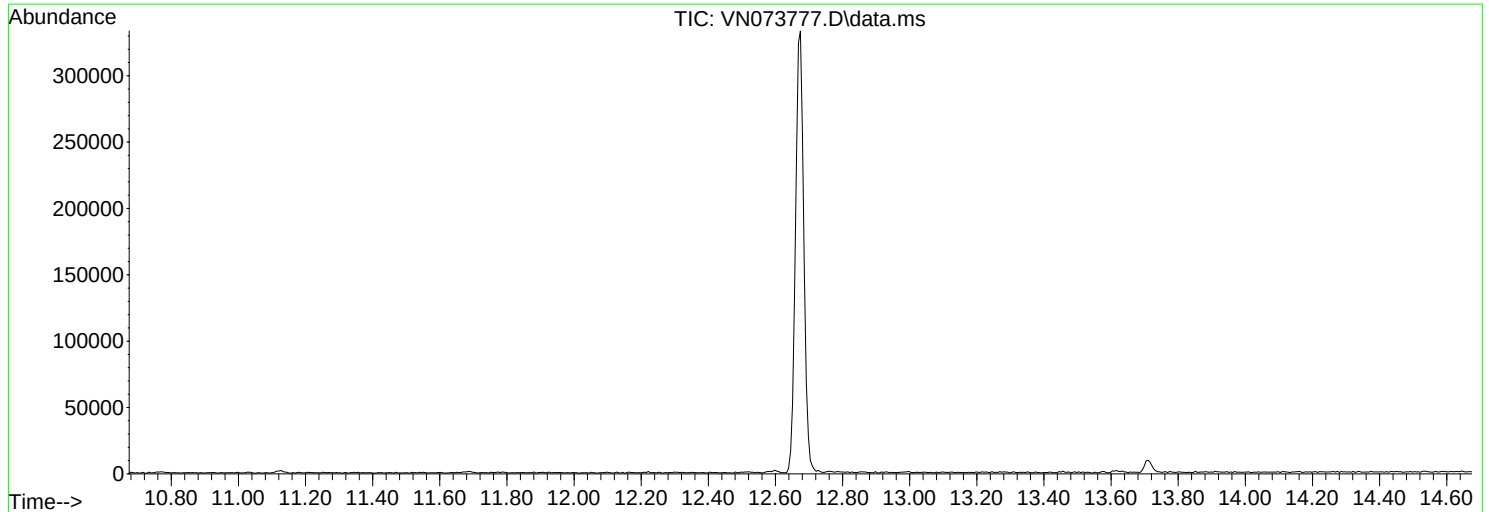

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.9         | 11277      | PASS                |
| 75             | 95              | 30              | 60              | 52.3         | 29605      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 56613      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 3966       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 696        | PASS                |
| 174            | 95              | 50              | 100             | 95.3         | 53931      | PASS                |
| 175            | 174             | 5               | 9               | 6.8          | 3679       | PASS                |
| 176            | 174             | 95              | 101             | 95.6         | 51544      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 3272       | PASS                |