


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN080923\  
 Data File : VN078811.D  
 Acq On : 09 Aug 2023 10:46  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N080823W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
 Last Update : Wed Aug 09 05:05:47 2023

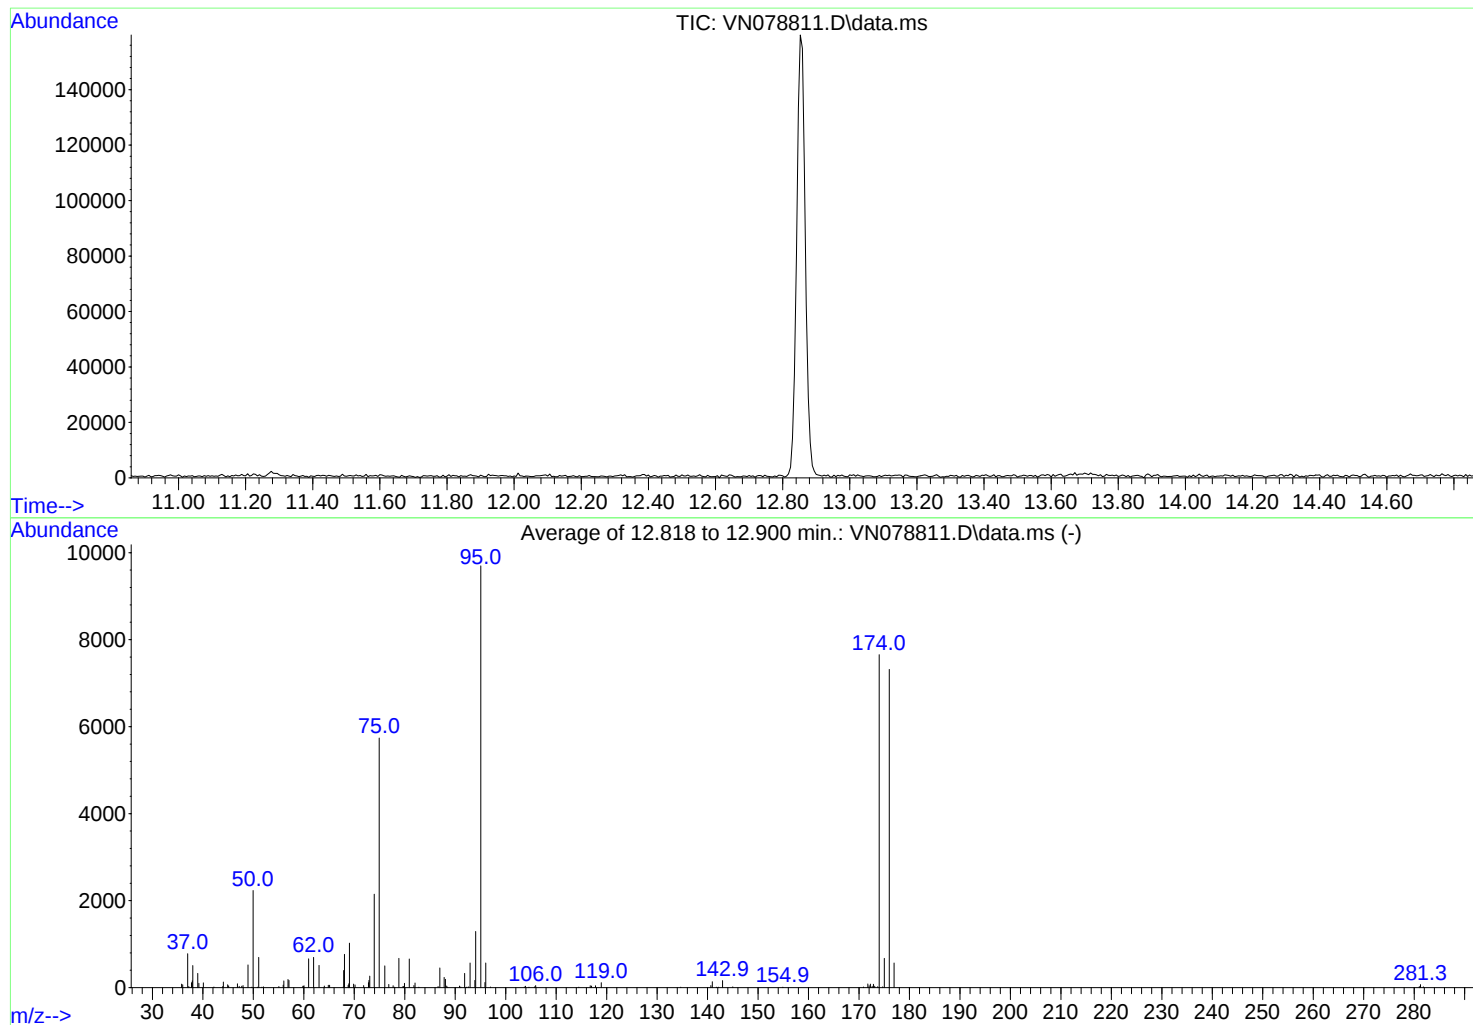

AutoFind: Averaged scan 1847 to 1861; Bkg corrected with scan 1846

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 23.0         | 2234       | PASS                |
| 75             | 95              | 30              | 60              | 59.2         | 5737       | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 9697       | PASS                |
| 96             | 95              | 5               | 9               | 5.8          | 566        | PASS                |
| 173            | 174             | 0.00            | 2               | 1.0          | 78         | PASS                |
| 174            | 95              | 50              | 100             | 78.9         | 7654       | PASS                |
| 175            | 174             | 5               | 9               | 8.8          | 673        | PASS                |
| 176            | 174             | 95              | 101             | 95.6         | 7317       | PASS                |
| 177            | 176             | 5               | 9               | 7.7          | 565        | PASS                |