
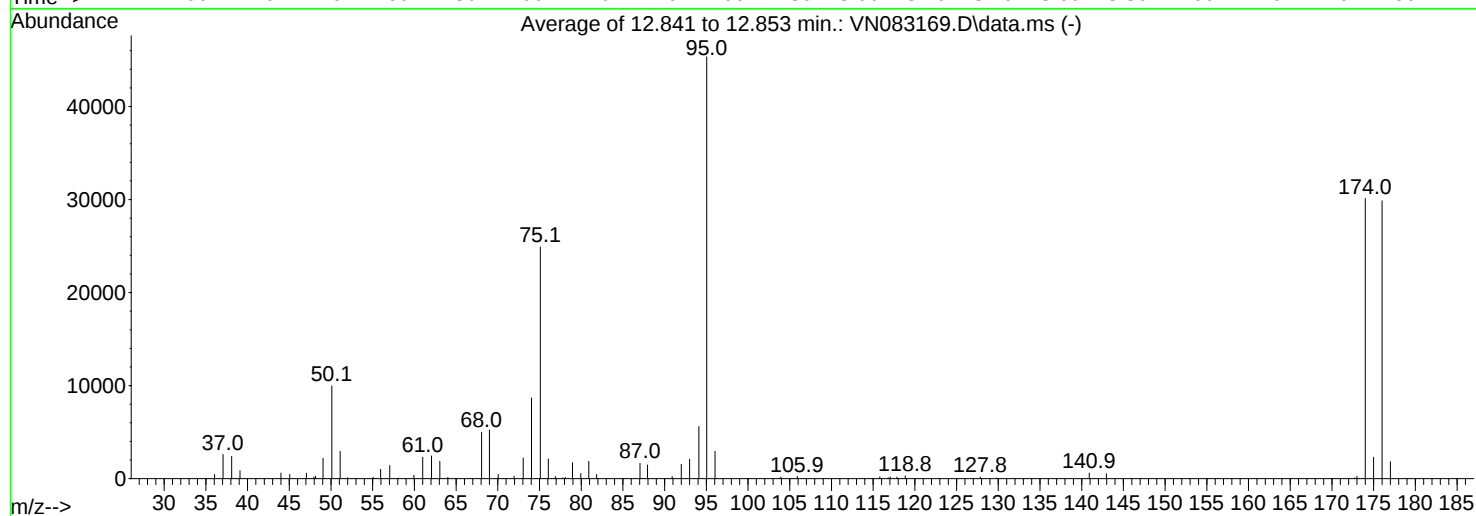


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080924\
Data File : VN083169.D
Acq On : 09 Aug 2024 09:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

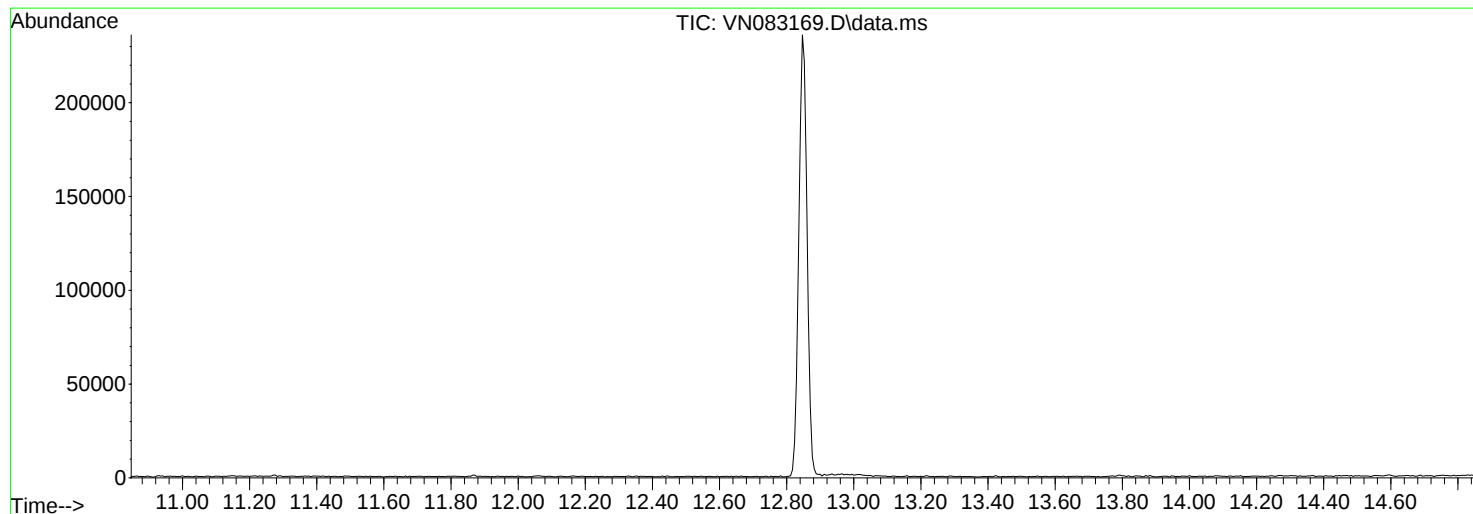

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	9950	PASS
75	95	30	60	54.9	24899	PASS
95	95	100	100	100.0	45336	PASS
96	95	5	9	6.5	2934	PASS
173	174	0.00	2	0.9	261	PASS
174	95	50	100	66.4	30109	PASS
175	174	5	9	7.6	2301	PASS
176	174	95	101	99.2	29869	PASS
177	176	5	9	6.1	1828	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	451	51.10	2920	68.05	4991	78.95	1711
37.05	2595	52.00	98	69.00	5226	79.95	551
38.10	2396	55.05	154	70.05	456	80.90	185
39.10	857	55.95	990	71.95	276	81.85	445
44.00	598	57.05	1406	73.05	2220	87.05	1657
45.05	448	58.10	52	74.05	8668	87.95	1456
47.05	567	59.95	383	75.10	24899	90.90	219
47.95	173	61.00	2311	76.05	2122	92.00	1553
48.15	251	62.05	2450	76.90	216	93.00	2086
49.05	2208	63.05	1850	77.80	87	94.10	5601
50.10	9950	64.00	139	78.10	144	95.05	45336

Average of 12.841 to 12.853 min.: VN083169.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2934	140.90	597				
103.80	50	142.95	523				
103.95	169	172.70	93				
105.90	234	173.00	261				
115.80	209	174.00	30109				
116.80	105	175.00	2301				
117.05	188	176.00	29869				
117.85	171	177.00	1828				
118.85	311						
127.85	166						
129.80	74						

Instrument :

MSVOA_N

ClientSampleId :

BFB