

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081018\
 Data File : VN050526.D
 Acq On : 10 Aug 2018 18:40
 Operator : MD\SY
 Sample : PB111921ZHE#05
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB111921ZHE#05

Quant Time: Aug 11 01:06:59 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 07 05:22:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	655469	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1092517	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	941745	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	372132	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	453644	51.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.60%	
35) Dibromofluoromethane	7.59	113	411676	46.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.92%	
50) Toluene-d8	10.09	98	1481394	44.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.90%	
62) 4-Bromofluorobenzene	12.40	95	433494	38.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	77.18%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.82	43	20930	7.66	ug/l	96
18) Methyl Acetate	4.33	43	16148	2.19	ug/l	96
20) Methylene Chloride	4.56	84	31341	2.45	ug/l	95
43) Isopropyl Acetate	8.17	43	319210	21.39	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN081018\
Data File : VN050526.D
Acq On : 10 Aug 2018 18:40
Operator : MD\SY
Sample : PB111921ZHE#05
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB111921ZHE#05

Quant Time: Aug 11 01:06:59 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 07 05:22:15 2018
Response via : Initial Calibration

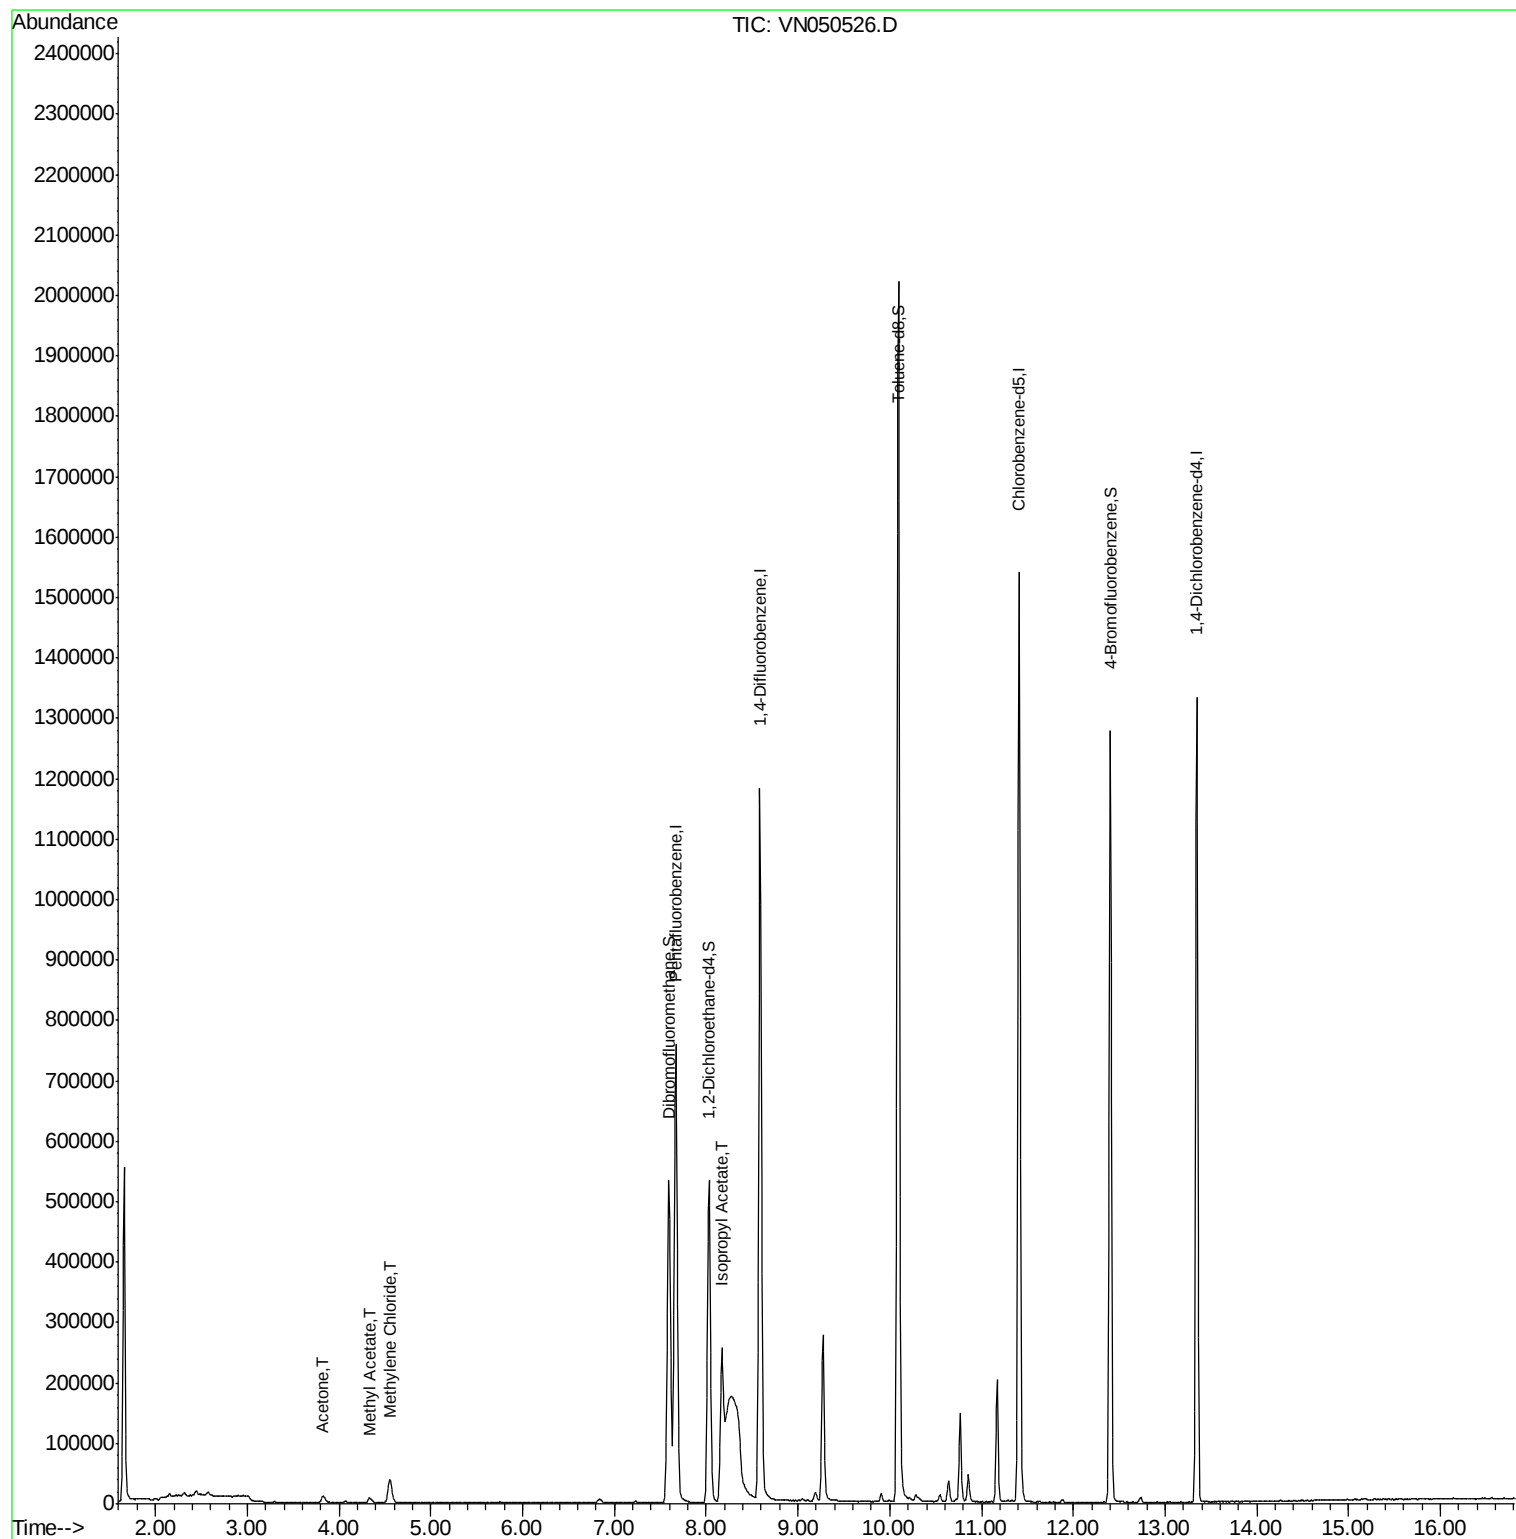

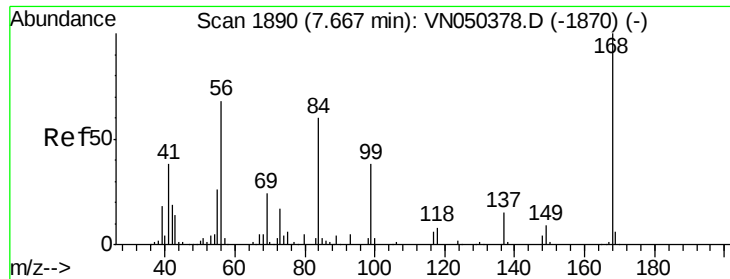

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050526.D

Acq: 10 Aug 2018 18:40

Instrument :

MSVOA_N

ClientSampleId :


PB111921ZHE#05

Tot Ion:168 Resp: 655469

Ion Ratio Lower Upper




168 100

99 51.6 40.0 60.0

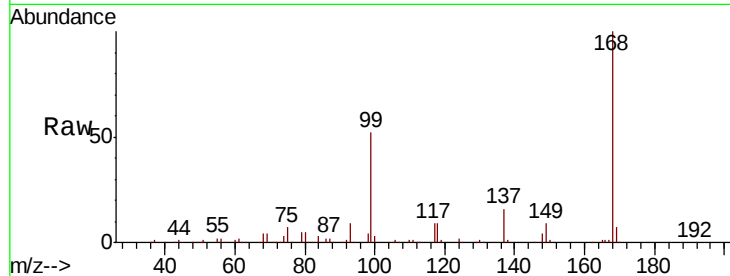

Abundance Ion 167.90 (167.60 to 168.60): VN050378.D (-1870) (-)

Ion 98.90 (98.60 to 99.60): VN050378.D (-1870) (-)

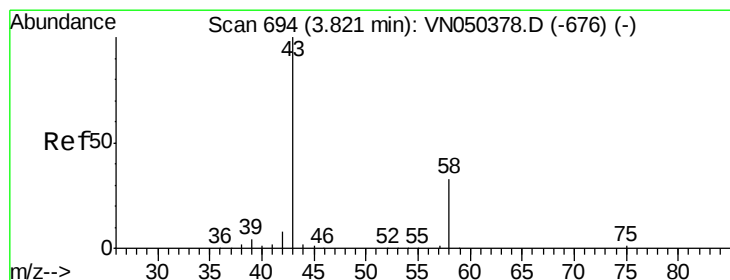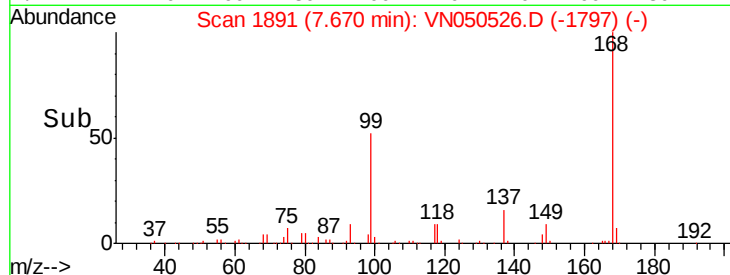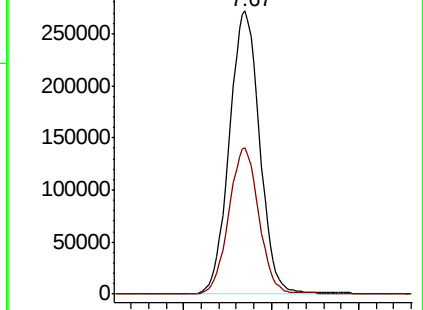

#16

Acetone

Concen: 7.66 ug/l

RT: 3.82 min Scan# 695

Delta R.T. 0.00 min

Lab File: VN050526.D


Acq: 10 Aug 2018 18:40

Tgt Ion: 43 Resp: 20930

Ion Ratio Lower Upper



43 100


58 34.8 25.8 38.8

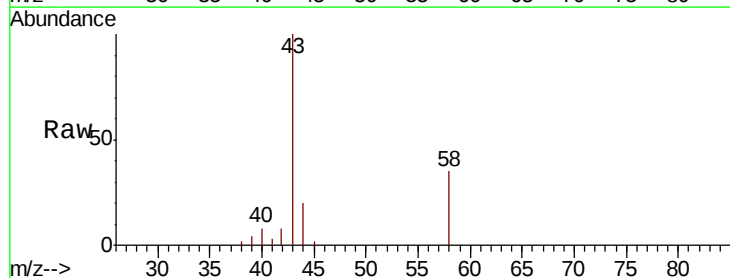

Abundance Ion 43.00 (42.70 to 43.70): VN050378.D (-676) (-)

Ion 58.00 (57.70 to 58.70): VN050378.D (-676) (-)



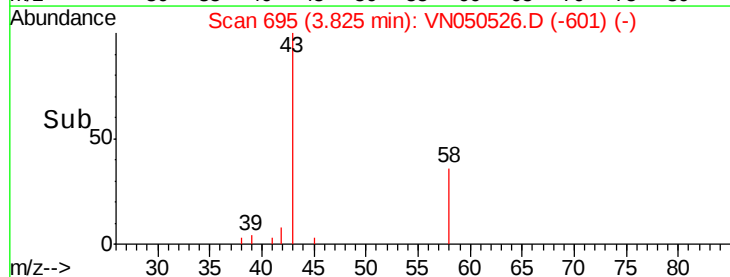
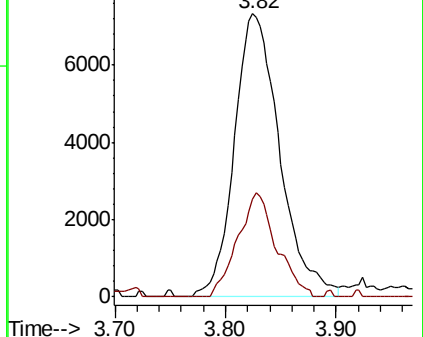


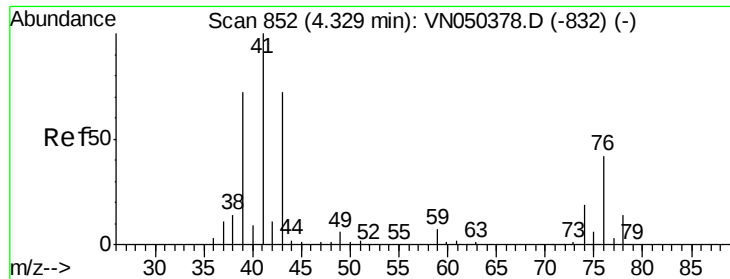

#18
Methyl Acetate
Concen: 2.19 ug/l
RT: 4.33 min Scan# 853
Delta R.T. 0.00 min
Lab File: VN050526.D
Acq: 10 Aug 2018 18:40




Instrument :
MSVOA_N
ClientSampleId :
PB111921ZHE#05


Tot Ion: 43 Resp: 16148
Ion Ratio Lower Upper
43 100
74 22.0 19.2 28.8

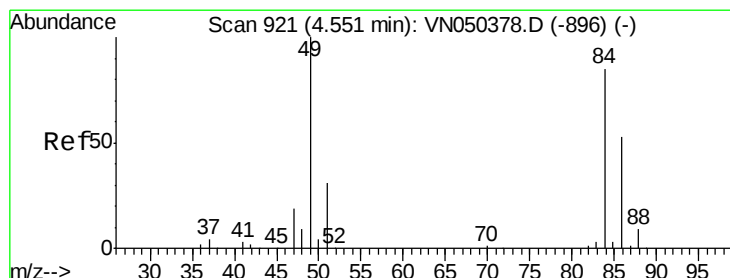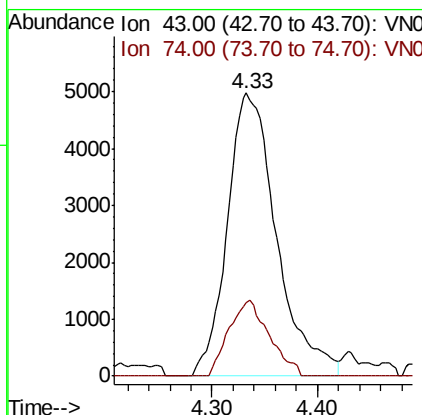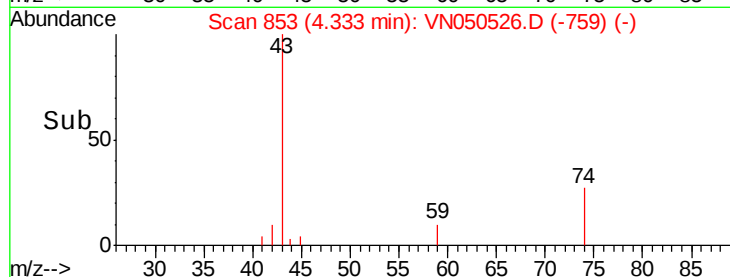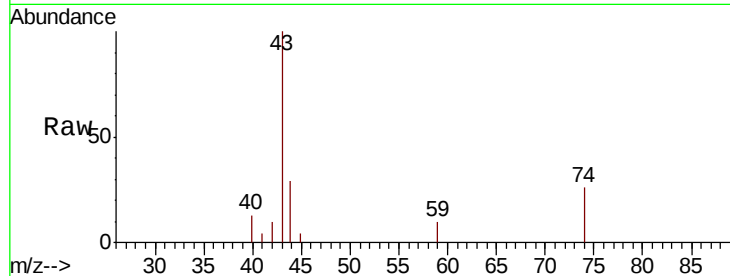

#20
Methylene Chloride
Concen: 2.45 ug/l
RT: 4.56 min Scan# 923
Delta R.T. 0.01 min
Lab File: VN050526.D
Acq: 10 Aug 2018 18:40

Tgt Ion: 84 Resp: 31341
Ion Ratio Lower Upper
84 100
49 112.7 94.8 142.2
51 32.8 28.3 42.5
86 61.4 51.0 76.6


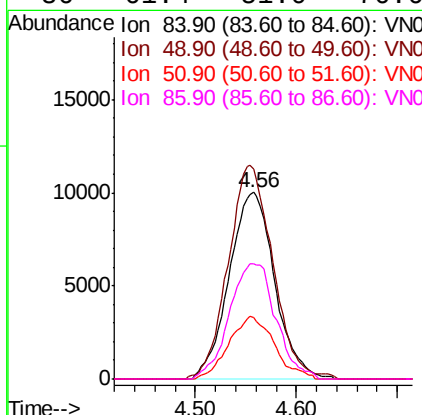
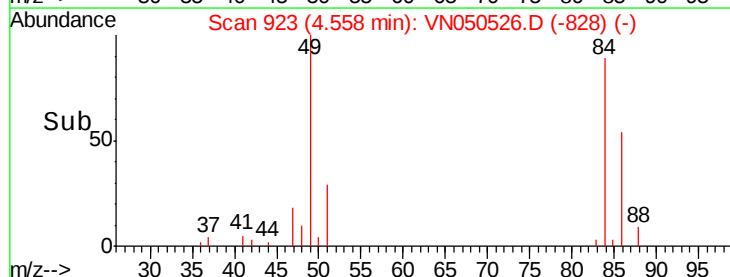
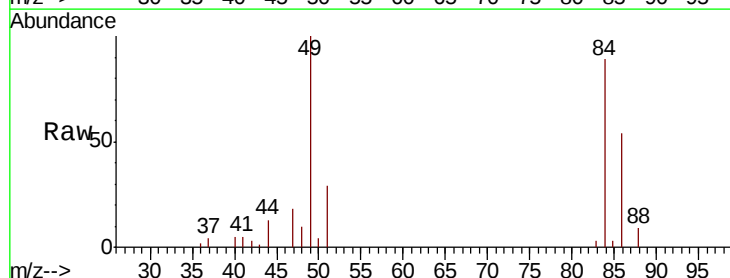


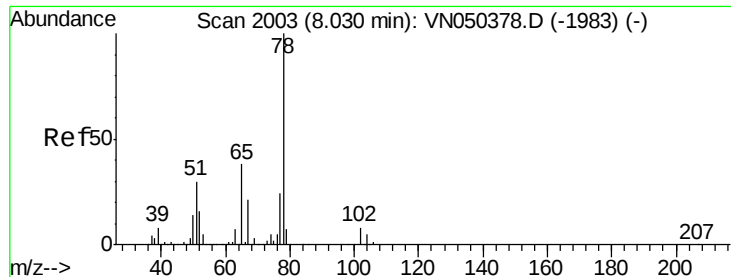

#33
 1,2-Dichloroethane-d4
 Concen: 51.80 ug/l
 RT: 8.03 min Scan# 2003
 Delta R.T. -0.00 min
 Lab File: VN050526.D
 Acq: 10 Aug 2018 18:40




Instrument :
 MSVOA_N
 ClientSampleId :
 PB111921ZHE#05

Tot Ion: 65 Resp: 453644
 Ion Ratio Lower Upper
 65 100
 67 54.0 0.0 108.4

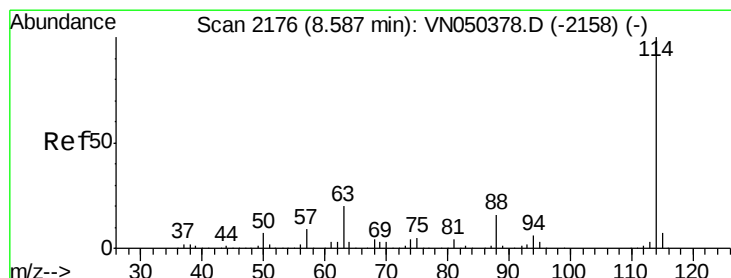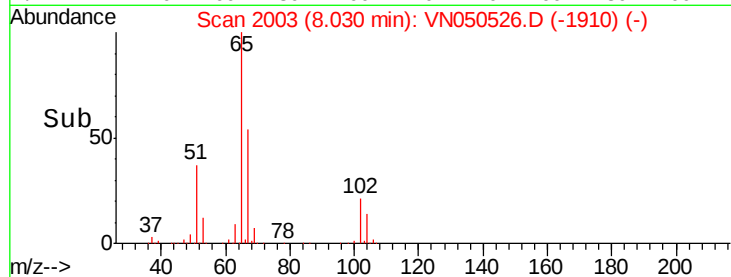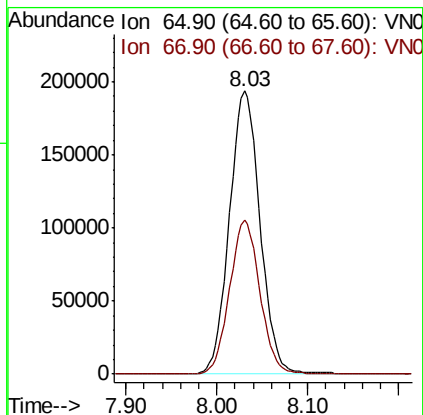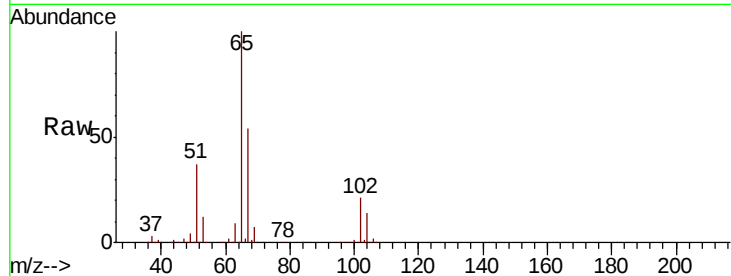

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN050526.D
 Acq: 10 Aug 2018 18:40

Tgt Ion: 114 Resp: 1092517
 Ion Ratio Lower Upper
 114 100
 63 19.6 0.0 40.0
 88 15.4 0.0 31.2


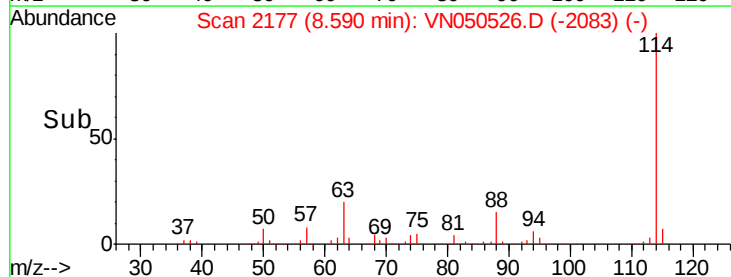
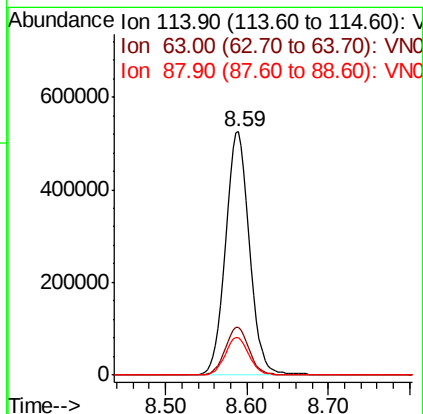
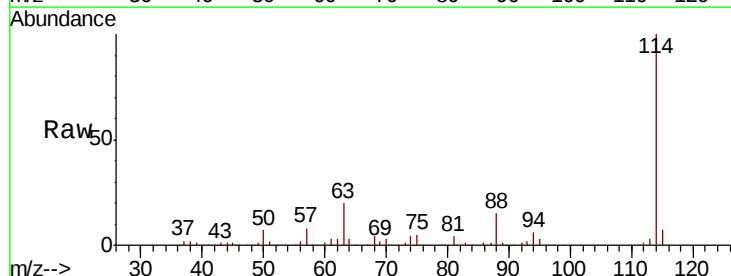




#35
 Dibromofluoromethane
 Concen: 46.96 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: VN050526.D
 Acq: 10 Aug 2018 18:40




Instrument :
 MSVOA_N
 ClientSampleId :
 PB111921ZHE#05


Tot Ion:113 Resp: 411676
 Ion Ratio Lower Upper
 113 100
 111 102.4 80.7 121.1
 192 22.2 17.8 26.6

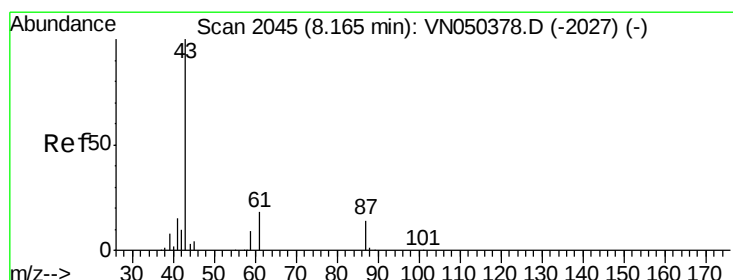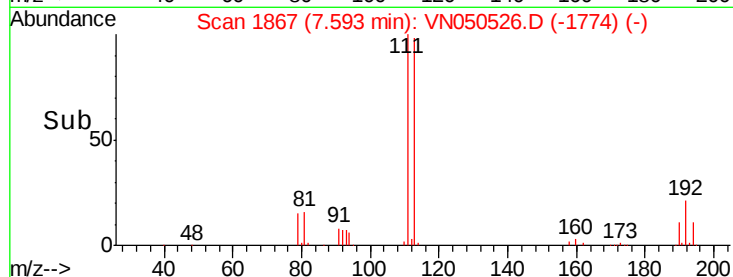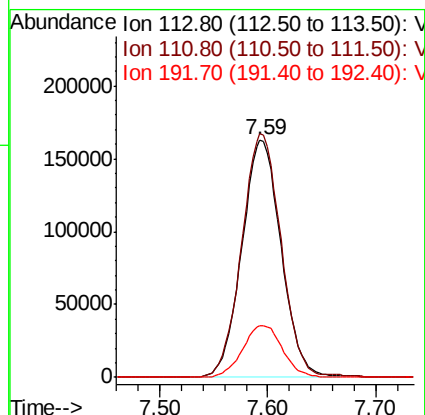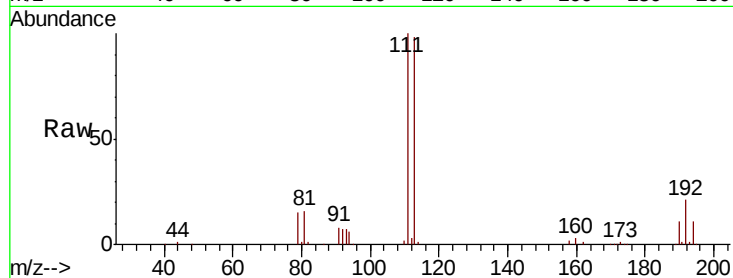

#43
 Isopropyl Acetate
 Concen: 21.39 ug/l
 RT: 8.17 min Scan# 2047
 Delta R.T. 0.01 min
 Lab File: VN050526.D
 Acq: 10 Aug 2018 18:40

Tgt Ion: 43 Resp: 319210
 Ion Ratio Lower Upper
 43 100
 61 17.1 15.8 23.6
 87 10.8 10.3 15.5


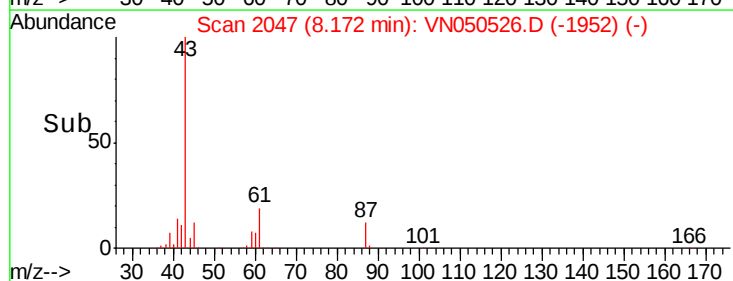
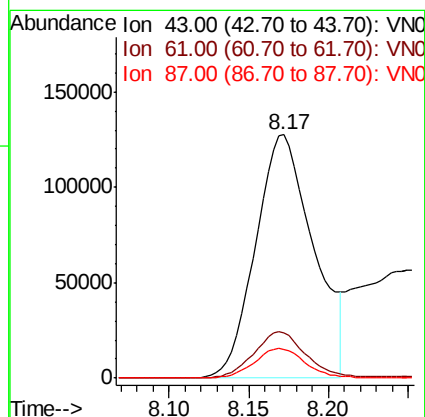
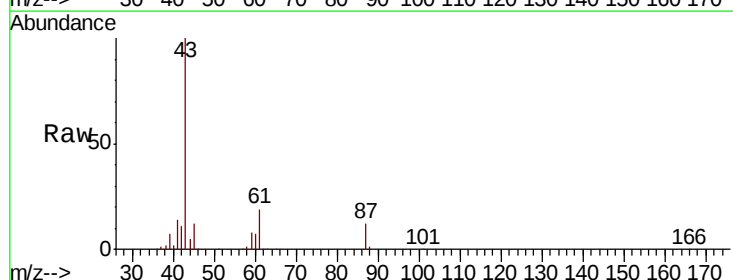


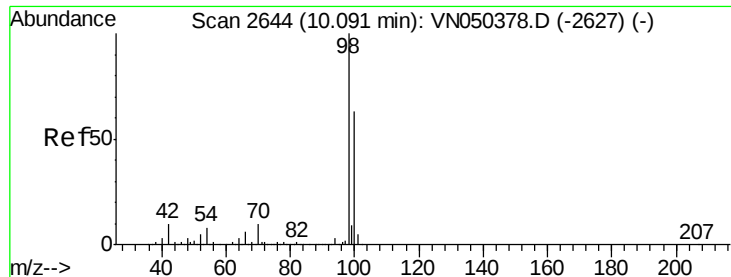

#50
Toluene-d8
Concen: 44.95 ug/l
RT: 10.09 min Scan# 2645
Delta R.T. 0.00 min
Lab File: VN050526.D
Acq: 10 Aug 2018 18:40




Instrument :
MSVOA_N
ClientSampleId :
PB111921ZHE#05


Tot Ion: 98 Resp: 1481394
Ion Ratio Lower Upper
98 100
100 63.5 50.7 76.1

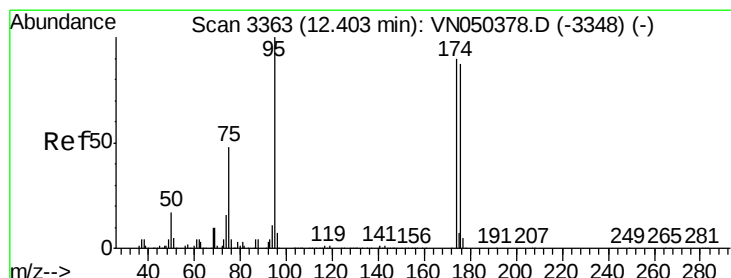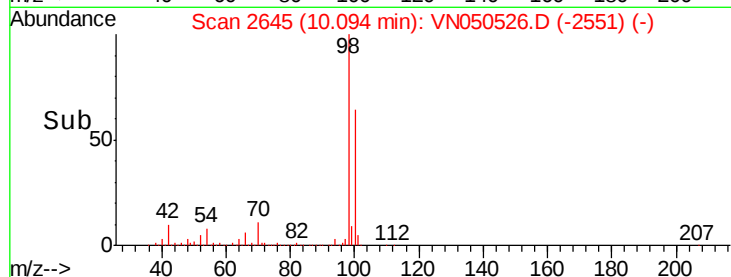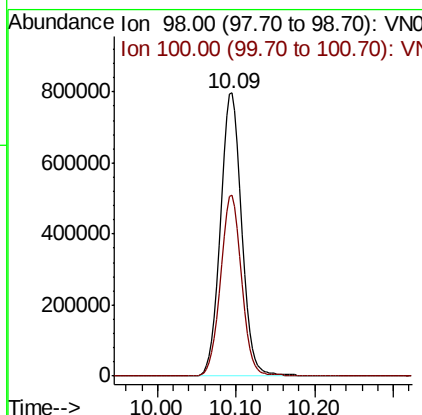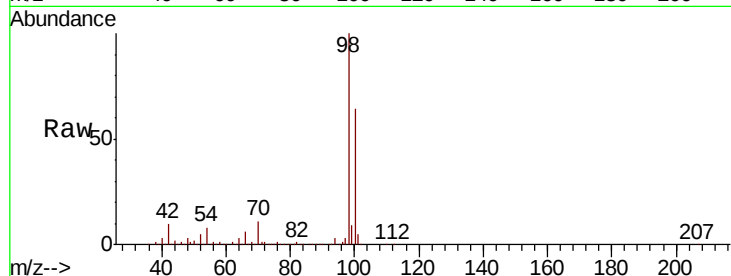

#62
4-Bromofluorobenzene
Concen: 38.59 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. -0.00 min
Lab File: VN050526.D
Acq: 10 Aug 2018 18:40

Tgt Ion: 95 Resp: 433494
Ion Ratio Lower Upper
95 100
174 91.0 0.0 178.2
176 86.8 0.0 173.4


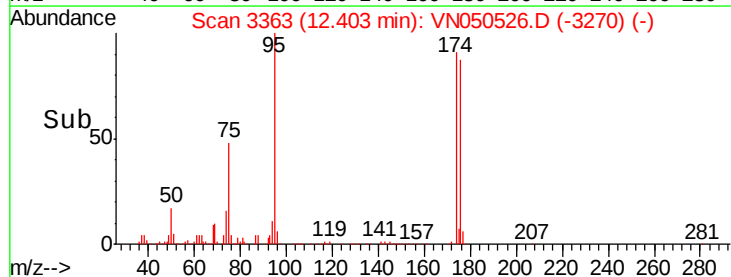
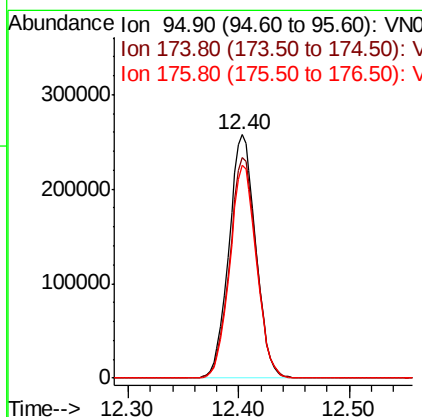
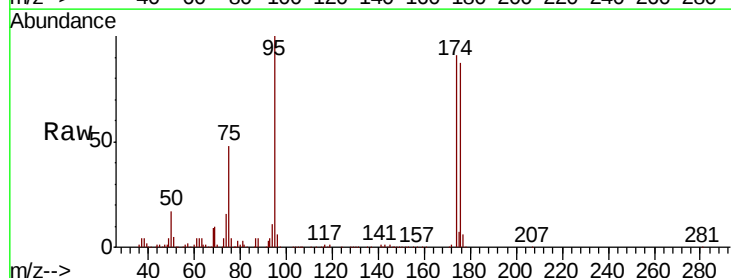


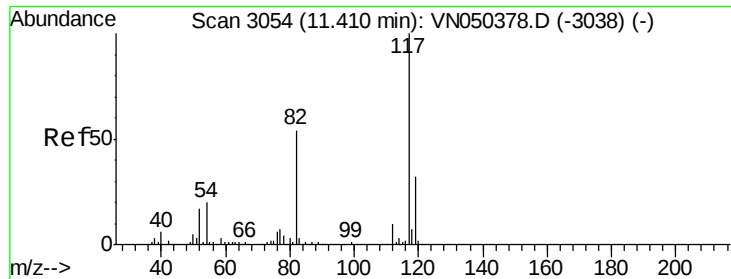

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. -0.00 min
Lab File: VN050526.D
Acq: 10 Aug 2018 18:40

Instrument :
MSVOA_N
ClientSampleId :
PB111921ZHE#05

Tot Ion:117 Resp: 941745
Ion Ratio Lower Upper
117 100
82 54.1 43.7 65.5
119 32.3 26.1 39.1

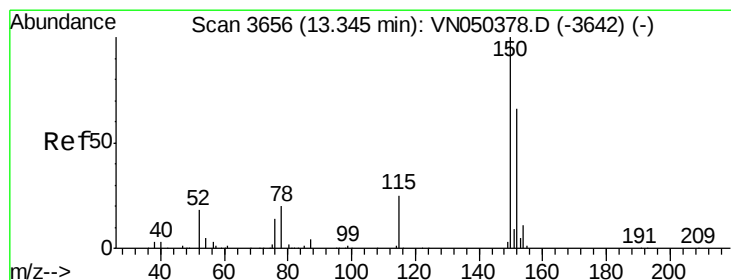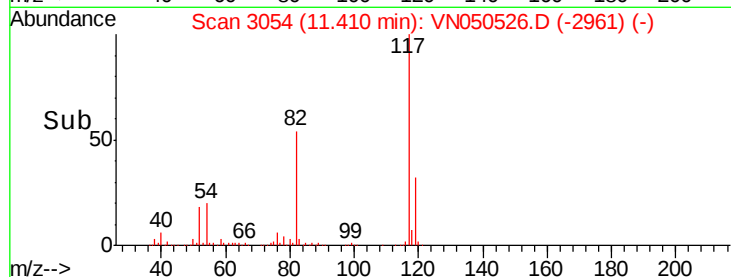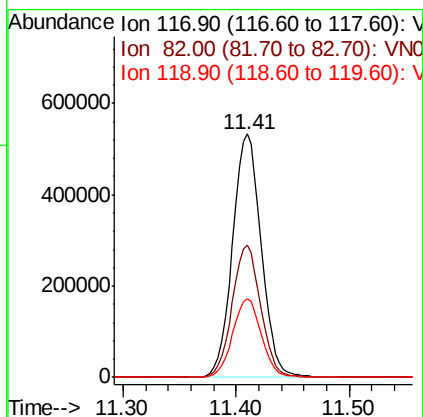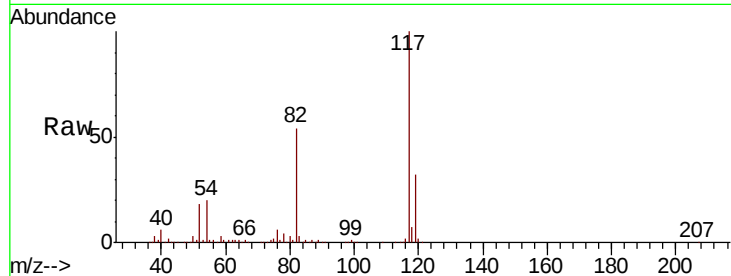

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3656
Delta R.T. -0.00 min
Lab File: VN050526.D
Acq: 10 Aug 2018 18:40

Tgt Ion:152 Resp: 372132
Ion Ratio Lower Upper
152 100
115 56.6 27.8 83.3
150 158.5 0.0 348.6

