


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081018\
 Data File : VN050506.D
 Acq On : 10 Aug 2018 9:09
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
 Title : SW846 8260
 Last Update : Tue Aug 07 05:22:15 2018

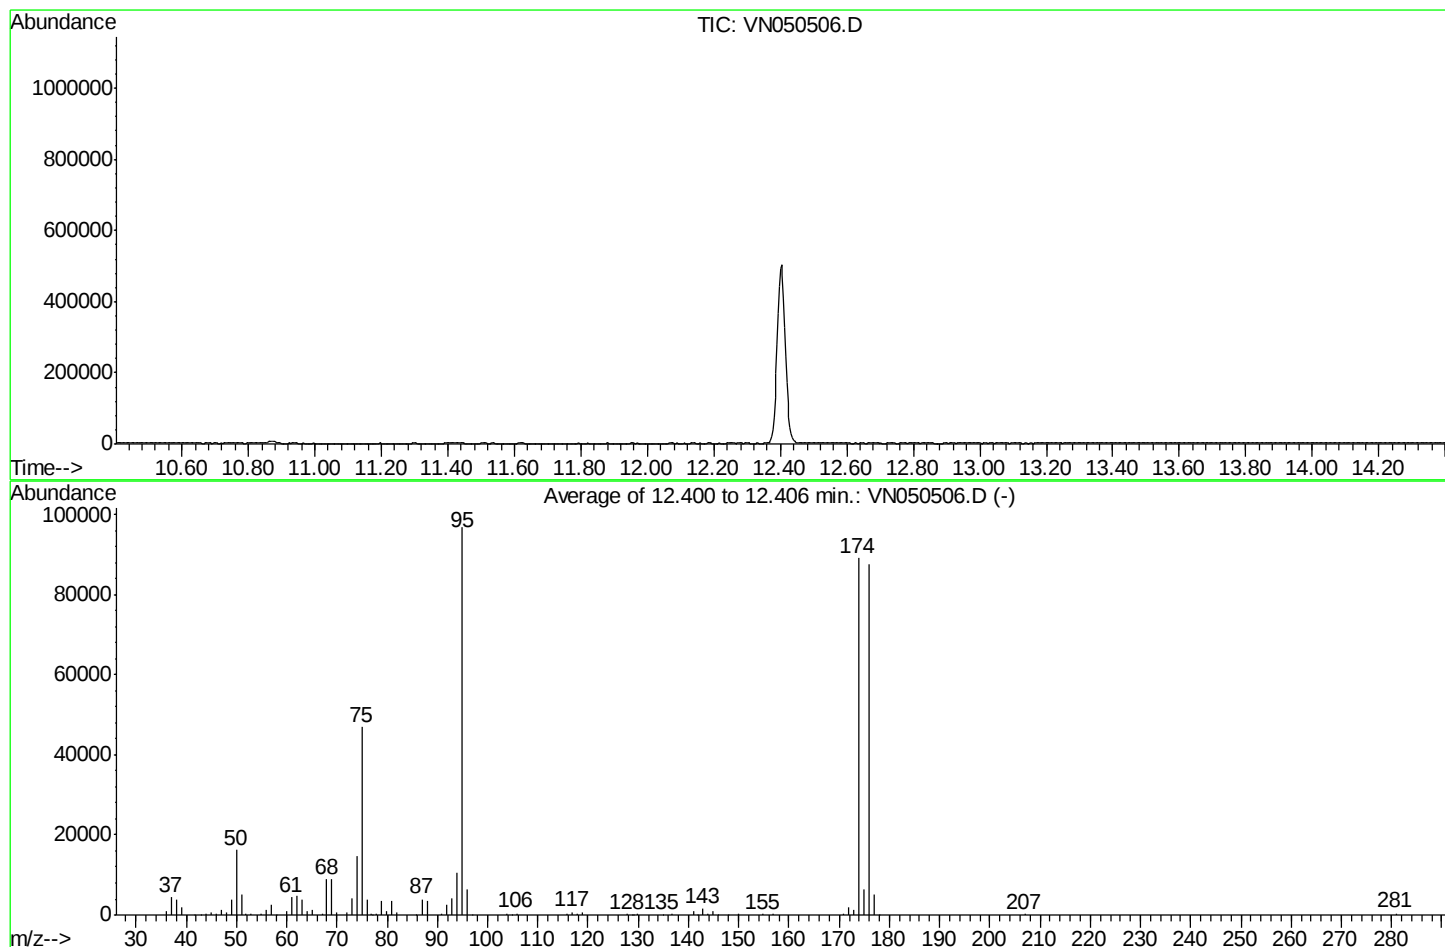

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	16211	PASS
75	95	30	60	48.5	46914	PASS
95	95	100	100	100.0	96816	PASS
96	95	5	9	6.7	6453	PASS
173	174	0.00	2	1.3	1133	PASS
174	95	50	100	92.1	89146	PASS
175	174	5	9	7.2	6453	PASS
176	174	95	101	98.2	87517	PASS
177	176	5	9	6.0	5213	PASS