


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081018\
Data File : VN050531.D
Acq On : 10 Aug 2018 20:44
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Title : SW846 8260
Last Update : Tue Aug 07 05:22:15 2018

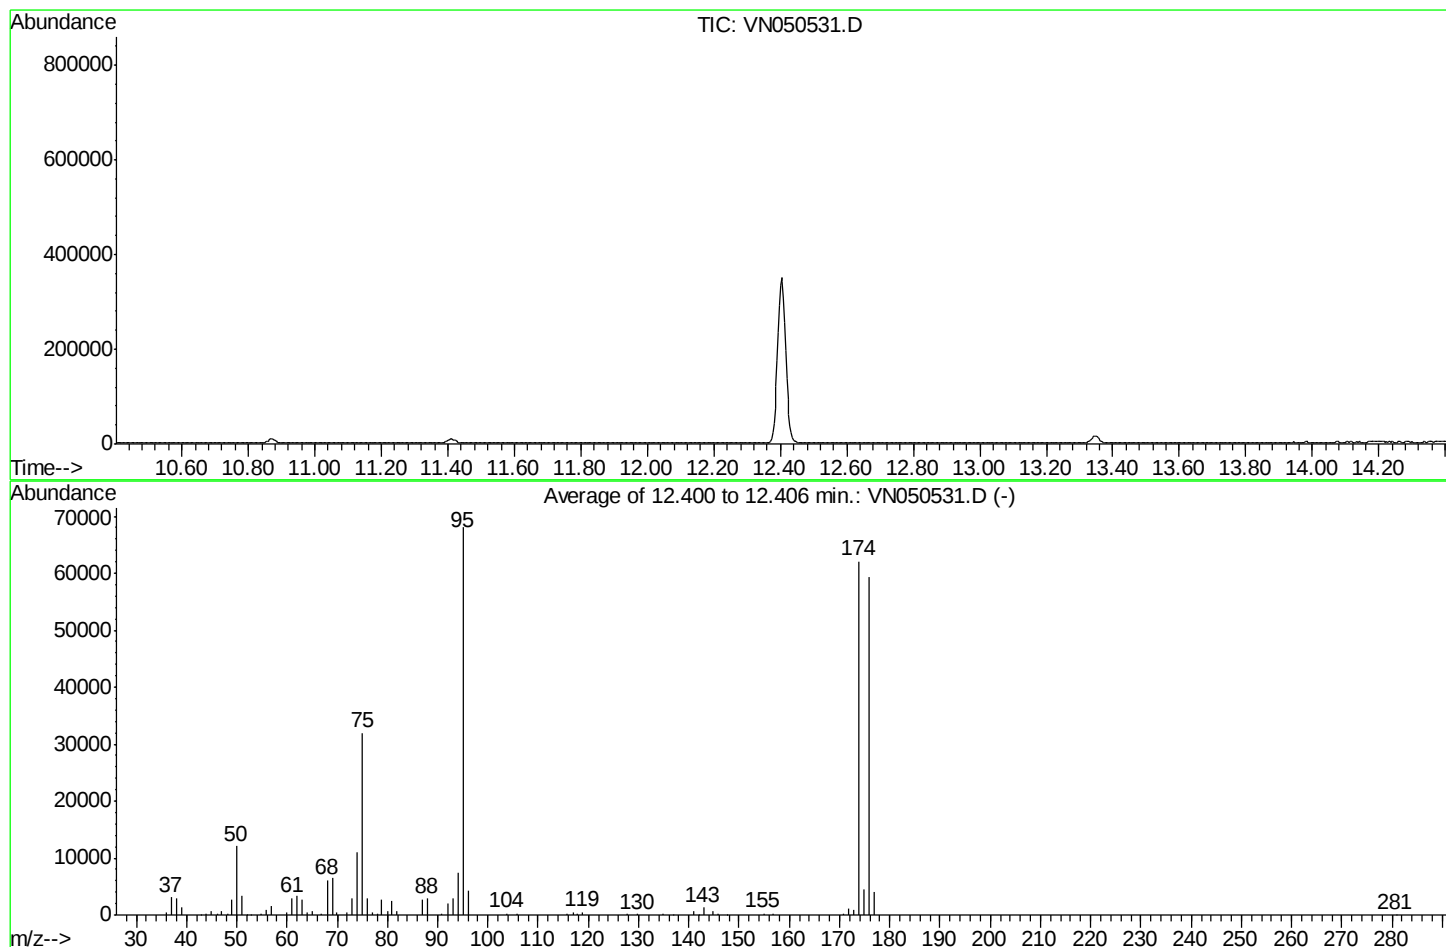

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12049	PASS
75	95	30	60	46.9	31912	PASS
95	95	100	100	100.0	68061	PASS
96	95	5	9	6.4	4360	PASS
173	174	0.00	2	1.5	910	PASS
174	95	50	100	91.2	62053	PASS
175	174	5	9	7.1	4415	PASS
176	174	95	101	95.6	59333	PASS
177	176	5	9	6.9	4077	PASS