


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081019\
 Data File : VN057163.D
 Acq On : 10 Aug 2019 9:17
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N081019W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sun Aug 11 03:53:25 2019

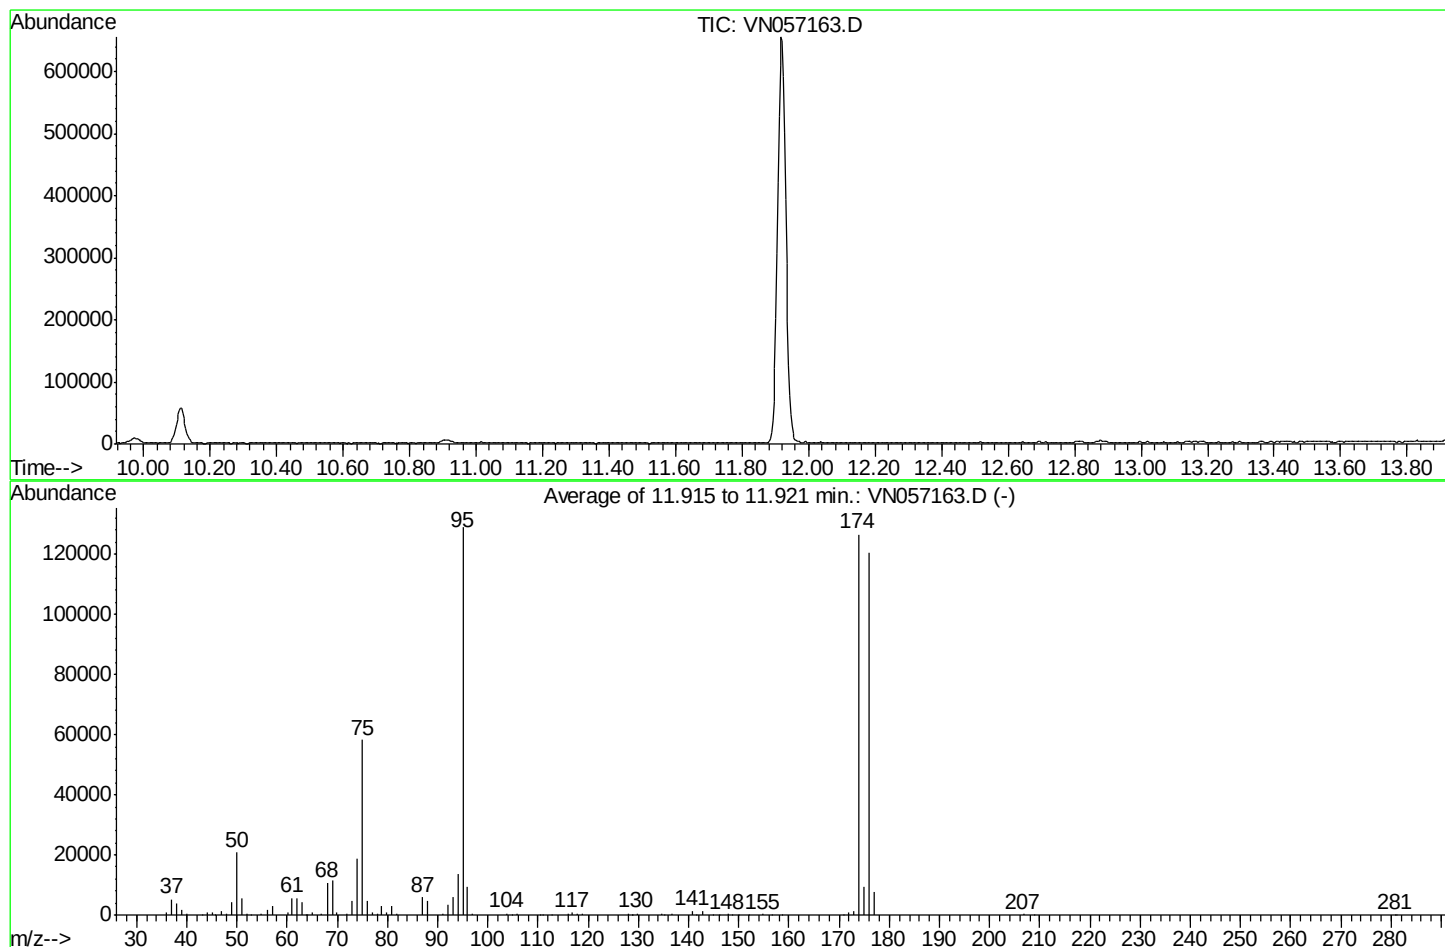

AutoFind: Scans 3154, 3155, 3156; Background Corrected with Scan 3142

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	20688	PASS
75	95	30	60	45.1	58152	PASS
95	95	100	100	100.0	128997	PASS
96	95	5	9	7.4	9523	PASS
173	174	0.00	2	1.2	1491	PASS
174	95	50	100	98.1	126528	PASS
175	174	5	9	7.5	9479	PASS
176	174	95	101	95.3	120640	PASS
177	176	5	9	6.5	7802	PASS