


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081020\  
Data File : VN062795.D  
Acq On : 10 Aug 2020 8:51  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N080520W.M  
Title : SW846 8260  
Last Update : Wed Aug 05 13:26:42 2020

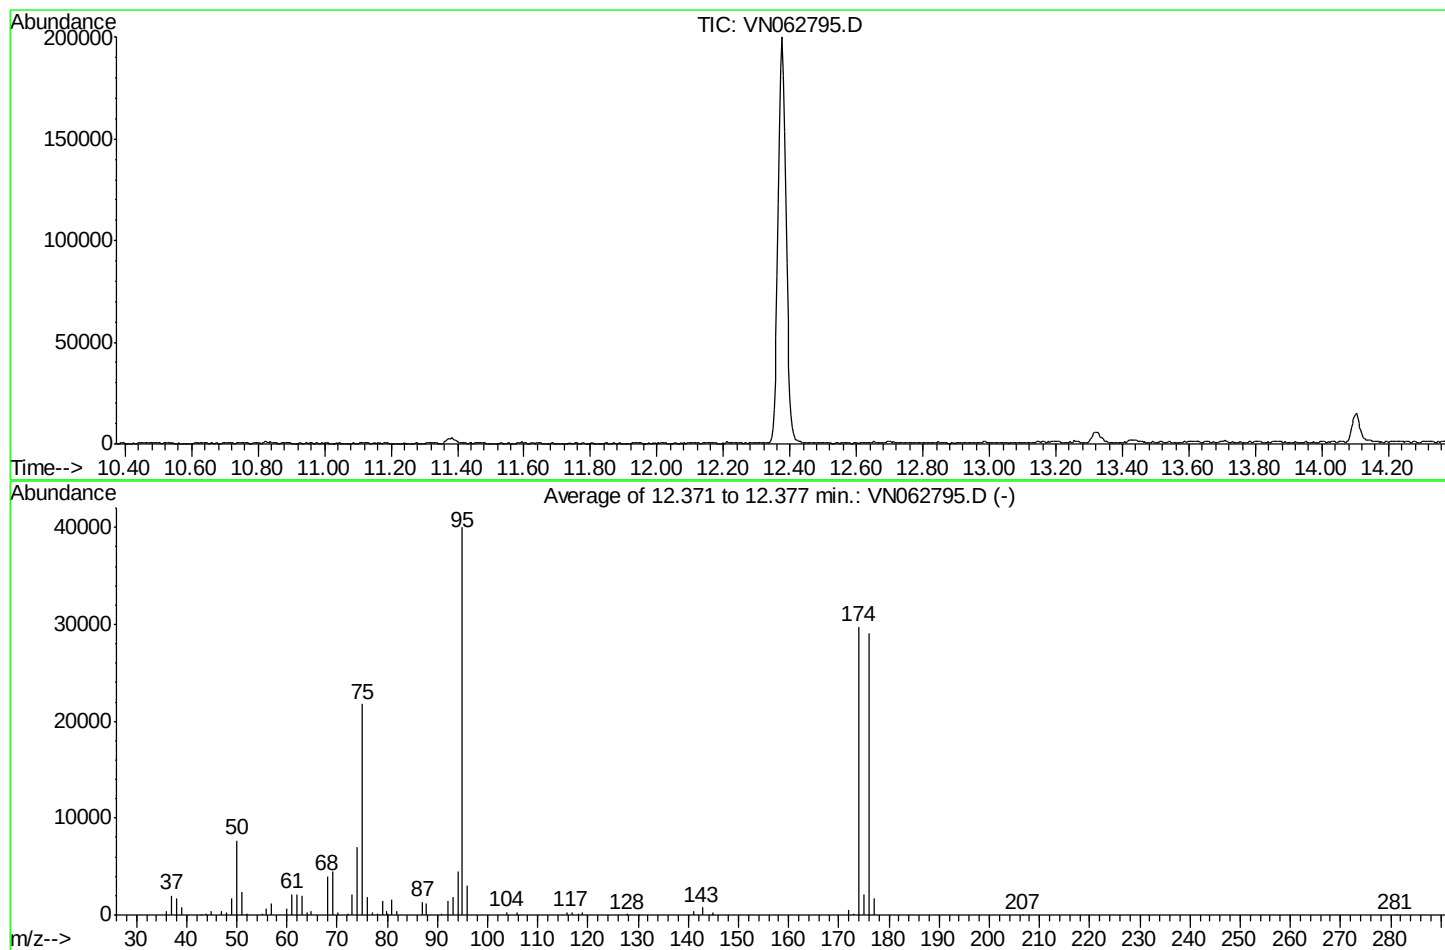

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3283

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.3      | 7733    | PASS             |
| 75          | 95           | 30           | 60           | 54.4      | 21752   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 40016   | PASS             |
| 96          | 95           | 5            | 9            | 7.6       | 3049    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.5       | 137     | PASS             |
| 174         | 95           | 50           | 100          | 74.4      | 29768   | PASS             |
| 175         | 174          | 5            | 9            | 7.2       | 2158    | PASS             |
| 176         | 174          | 95           | 101          | 97.6      | 29064   | PASS             |
| 177         | 176          | 5            | 9            | 5.8       | 1700    | PASS             |