


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081022\
Data File : VN073792.D
Acq On : 10 Aug 2022 10:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Title : SW846 8260
Last Update : Wed Aug 10 05:09:32 2022

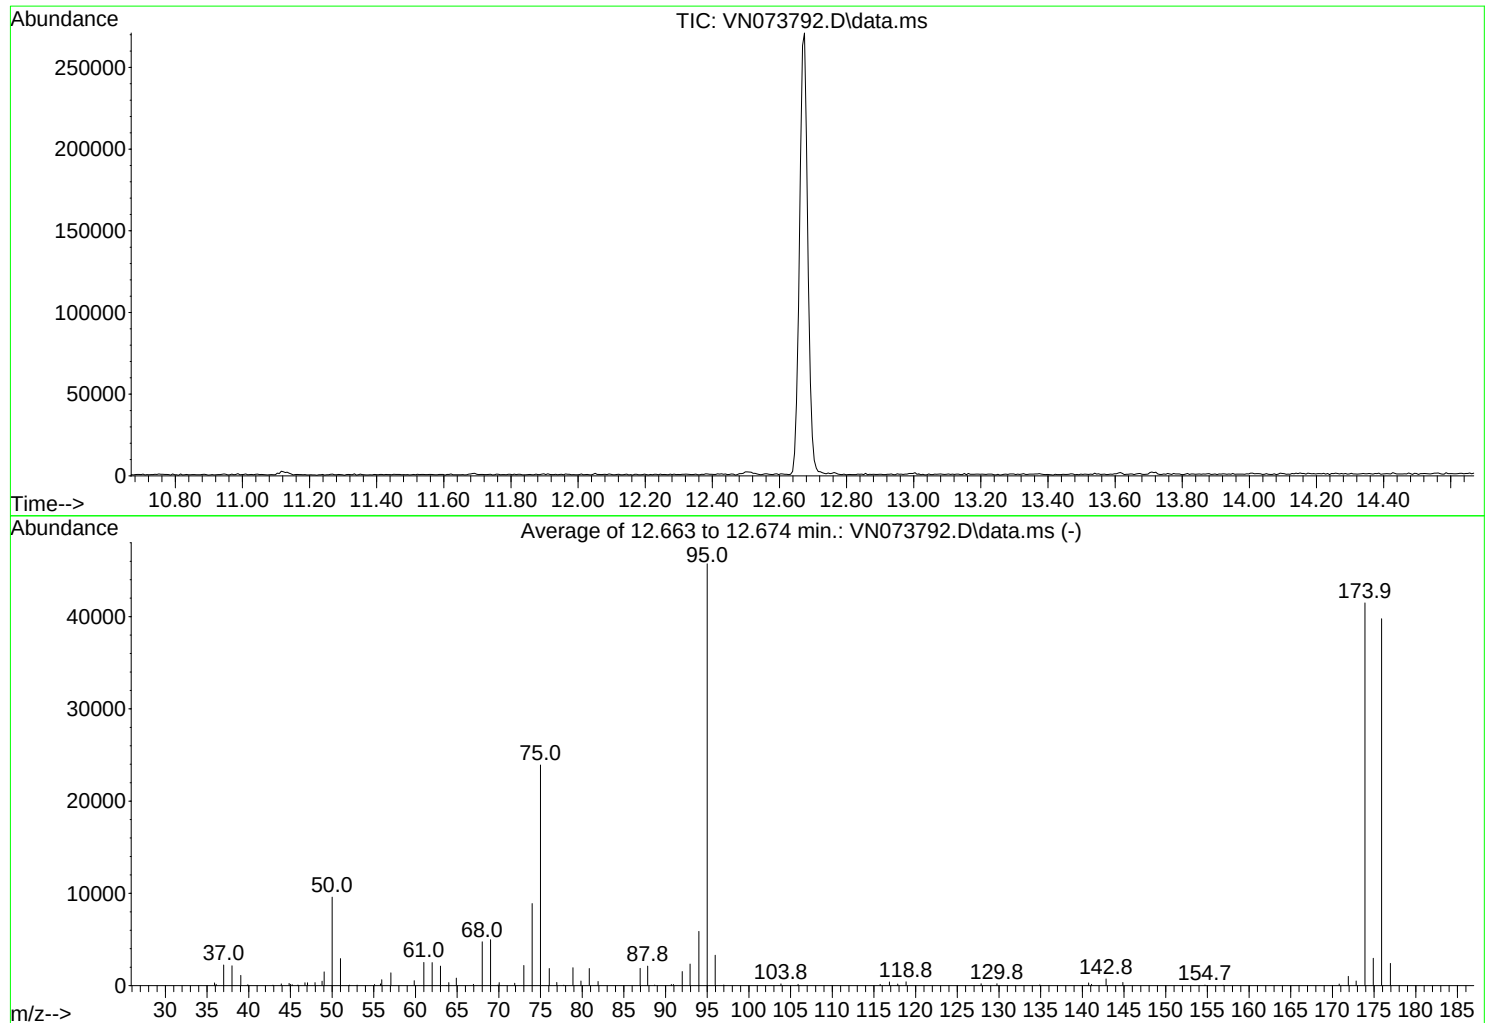

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	9591	PASS
75	95	30	60	52.3	23912	PASS
95	95	100	100	100.0	45720	PASS
96	95	5	9	7.2	3296	PASS
173	174	0.00	2	1.2	507	PASS
174	95	50	100	90.8	41493	PASS
175	174	5	9	7.2	2973	PASS
176	174	95	101	95.8	39768	PASS
177	176	5	9	6.1	2411	PASS