

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN081023\  
 Data File : VN078848.D  
 Acq On : 10 Aug 2023 19:34  
 Operator : JC\MD  
 Sample : 03905-02  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Aug 10 23:56:40 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N080723W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Aug 08 05:03:52 2023  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc   | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|--------|--------|----------|
| -----                         |                |      |                     |        |        |          |
| Internal Standards            |                |      |                     |        |        |          |
| 1) Pentafluorobenzene         | 8.230          | 168  | 172319              | 50.000 | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.112          | 114  | 333080              | 50.000 | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.871         | 117  | 310134              | 50.000 | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.794         | 152  | 86863               | 50.000 | ug/l   | 0.00     |
|                               |                |      |                     |        |        |          |
| System Monitoring Compounds   |                |      |                     |        |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.583          | 65   | 135028              | 52.269 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 104.540% |        |        |          |
| 35) Dibromofluoromethane      | 8.177          | 113  | 110234              | 49.008 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 98.020%  |        |        |          |
| 50) Toluene-d8                | 10.571         | 98   | 430133              | 51.964 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 103.920% |        |        |          |
| 62) 4-Bromofluorobenzene      | 12.859         | 95   | 115925              | 46.861 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 93.720%  |        |        |          |
|                               |                |      |                     |        |        |          |
| Target Compounds              |                |      |                     |        | Qvalue |          |
| 6) Chloroethane               | 3.106          | 64   | 466                 | 0.253  | ug/l # | 43       |
| 11) Tert butyl alcohol        | 5.530          | 59   | 1680                | 3.705  | ug/l # | 72       |
| 16) Acetone                   | 4.442          | 43   | 67232               | 67.641 | ug/l   | 94       |
| 18) Methyl Acetate            | 5.047          | 43   | 4593                | 1.029  | ug/l # | 63       |
| 20) Methylene Chloride        | 5.289          | 84   | 9104                | 3.698  | ug/l # | 67       |
| 25) 2-Butanone                | 7.489          | 43   | 31655               | 18.807 | ug/l # | 81       |
| 29) Tetrahydrofuran           | 7.847          | 42   | 339                 | 0.301  | ug/l # | 20       |
| 31) Cyclohexane               | 8.230          | 56   | 5130                | 1.352  | ug/l # | 51       |
| 36) 1,1-Dichloropropene       | 8.236          | 75   | 16216               | 4.647  | ug/l # | 50       |
| 37) Ethyl Acetate             | 7.571          | 43   | 36411               | 9.814  | ug/l # | 89       |
| 38) Carbon Tetrachloride      | 8.236          | 117  | 18813               | 5.230  | ug/l # | 16       |
| 42) 1,2-Dichloroethane        | 8.683          | 62   | 1254                | 0.331  | ug/l # | 73       |
| 43) Isopropyl Acetate         | 8.700          | 43   | 242509              | 38.768 | ug/l # | 70       |
| 48) Methyl methacrylate       | 9.671          | 41   | 5238                | 1.812  | ug/l # | 34       |
| 49) 1,4-Dioxane               | 9.735          | 88   | 228                 | 4.858  | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.453         | 43   | 114547              | 29.895 | ug/l # | 83       |
| 53) t-1,3-Dichloropropene     | 10.735         | 75   | 840                 | 0.219  | ug/l # | 52       |
| 54) cis-1,3-Dichloropropene   | 10.365         | 75   | 46172               | 11.097 | ug/l # | 71       |
| 56) Ethyl methacrylate        | 10.988         | 69   | 2330                | 0.627  | ug/l # | 1        |
| 57) 1,3-Dichloropropane       | 11.206         | 76   | 5598                | 1.257  | ug/l # | 42       |
| 59) 2-Hexanone                | 11.177         | 43   | 129925              | 47.888 | ug/l # | 19       |
| 71) Bromoform                 | 12.853         | 173  | 847                 | 0.444  | ug/l # | 1        |
| 74) N-amyl acetate            | 12.471         | 43   | 4151                | 1.070  | ug/l # | 36       |
| 76) 1,2,3-Trichloropropane    | 12.853         | 75   | 66290               | 28.227 | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853         | 75   | 66290               | 75.742 | ug/l # | 15       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN081023\  
Data File : VN078848.D  
Acq On : 10 Aug 2023 19:34  
Operator : JC\MD  
Sample : 03905-02  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Aug 10 23:56:40 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N080723W.M  
Quant Title : SW846 8260  
QLast Update : Tue Aug 08 05:03:52 2023  
Response via : Initial Calibration




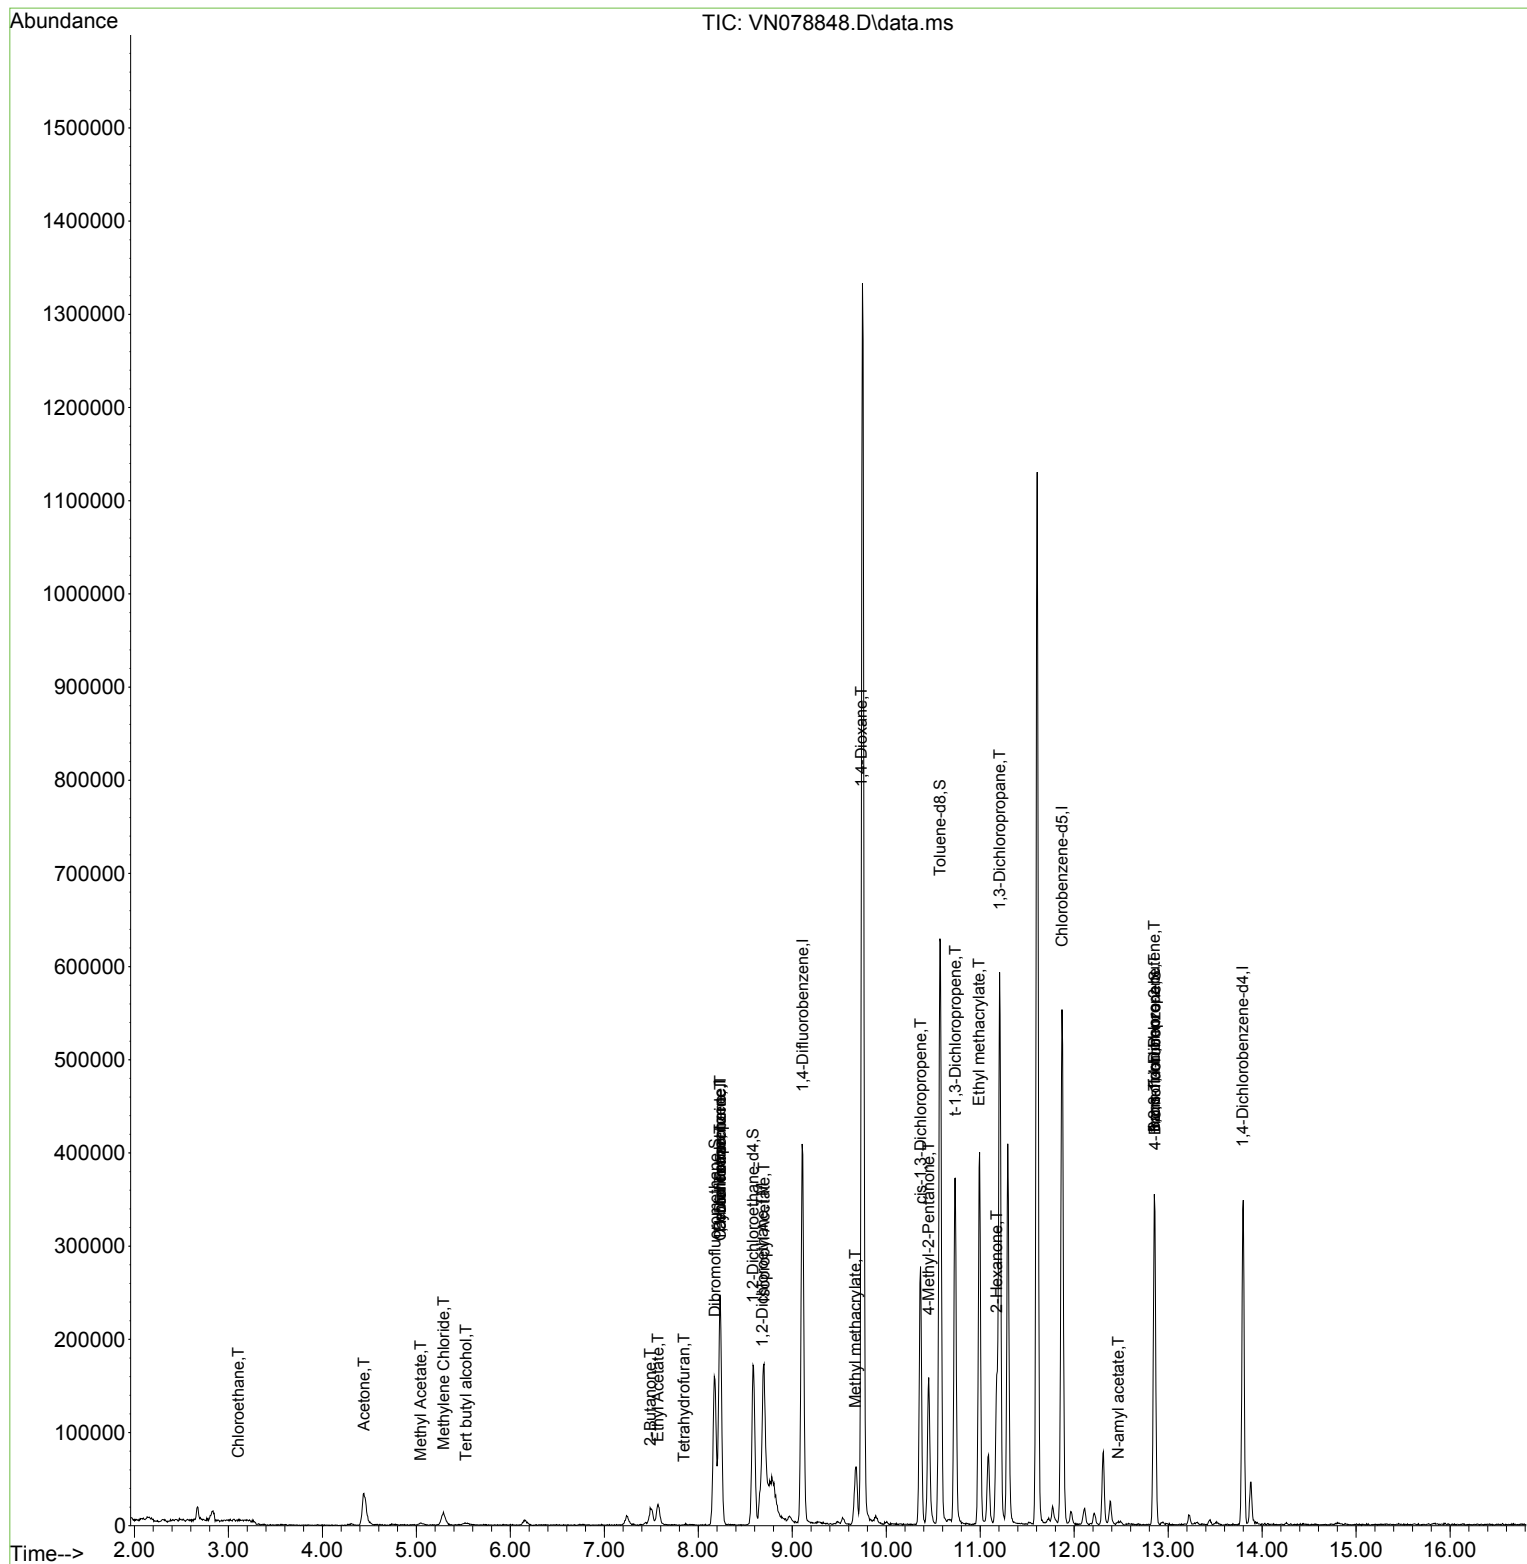




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.230 min Scan# 1067  
Delta R.T. -0.000 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:168 Resp: 172319  
Ion Ratio Lower Upper  
168 100  
99 58.4 53.0 79.6

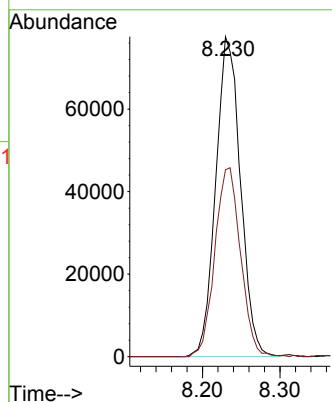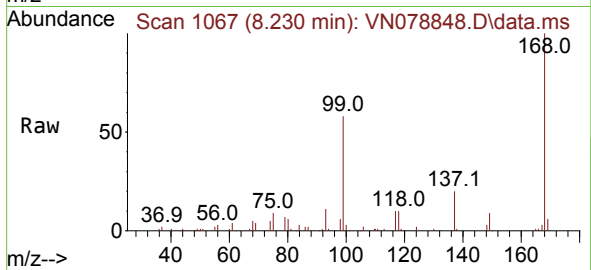

#6  
Chloroethane  
Concen: 0.253 ug/l  
RT: 3.106 min Scan# 196  
Delta R.T. -0.012 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Tgt Ion: 64 Resp: 466  
Ion Ratio Lower Upper  
64 100  
66 0.0 25.4 38.2#



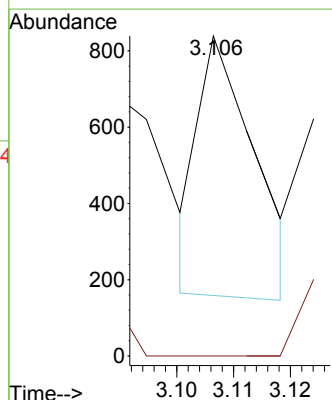
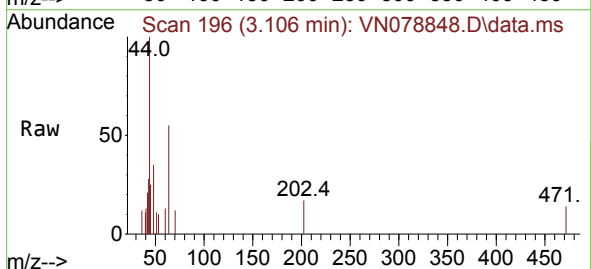




#11  
Tert butyl alcohol  
Concen: 3.705 ug/l  
RT: 5.530 min Scan# 610  
Delta R.T. -0.012 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 59 Resp: 1680  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.2 12.4#

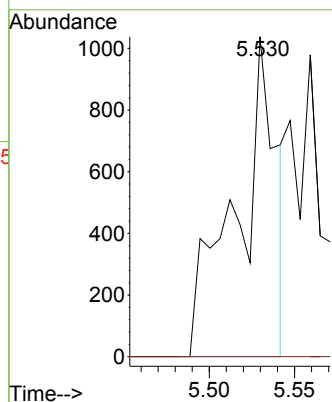

#16  
Acetone  
Concen: 67.641 ug/l  
RT: 4.442 min Scan# 423  
Delta R.T. -0.000 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34


Tgt Ion: 43 Resp: 67232  
Ion Ratio Lower Upper  
43 100  
58 31.7 28.0 42.0

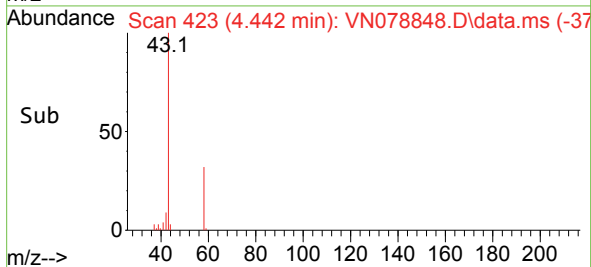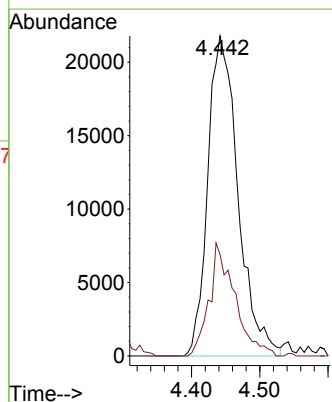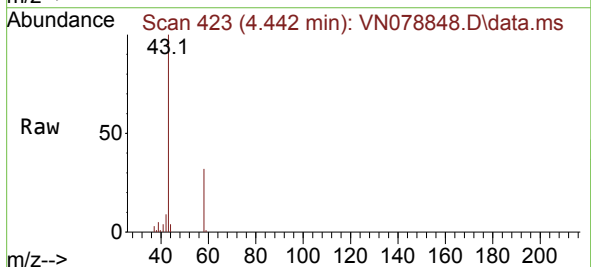






#18  
Methyl Acetate  
Concen: 1.029 ug/l  
RT: 5.047 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 43 Resp: 4593  
Ion Ratio Lower Upper  
43 100  
74 12.0 26.2 39.4#

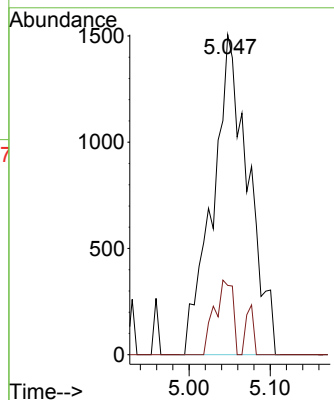

#20  
Methylene Chloride  
Concen: 3.698 ug/l  
RT: 5.289 min Scan# 567  
Delta R.T. -0.000 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34


Tgt Ion: 84 Resp: 9104  
Ion Ratio Lower Upper  
84 100  
49 162.1 79.7 119.5#  
51 33.3 25.2 37.8  
86 65.4 53.3 79.9

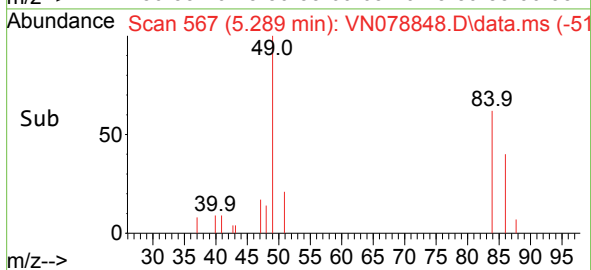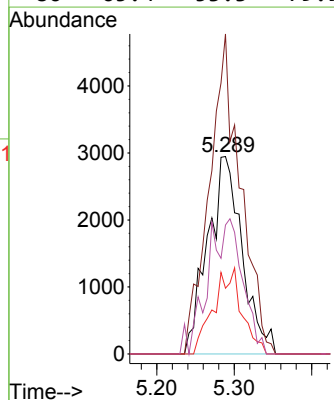






#25  
2-Butanone  
Concen: 18.807 ug/l  
RT: 7.489 min Scan# 941  
Delta R.T. -0.005 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34


Instrument :  
MSVOA\_N  
ClientSampleId :





Tgt Ion: 43 Resp: 31655  
Ion Ratio Lower Upper  
43 100  
72 26.5 30.2 45.2#

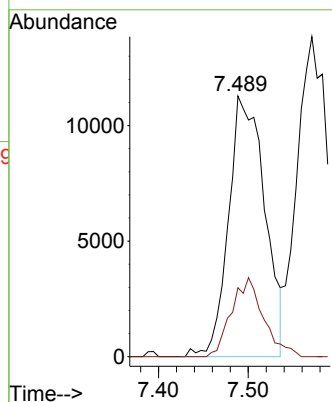


#29  
Tetrahydrofuran  
Concen: 0.301 ug/l  
RT: 7.847 min Scan# 1002  
Delta R.T. 0.000 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

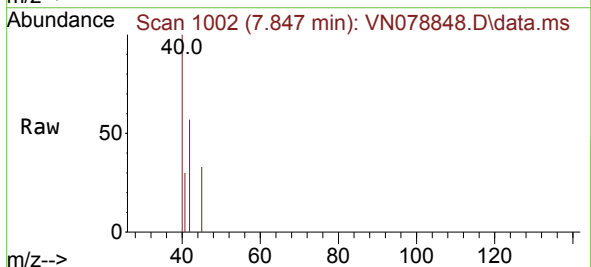


Tgt Ion: 42 Resp: 339  
Ion Ratio Lower Upper  
42 100  
72 0.0 49.8 74.6#  
71 0.0 47.4 71.2#

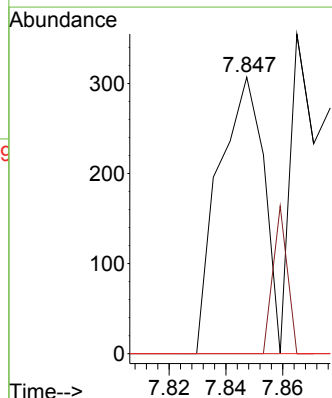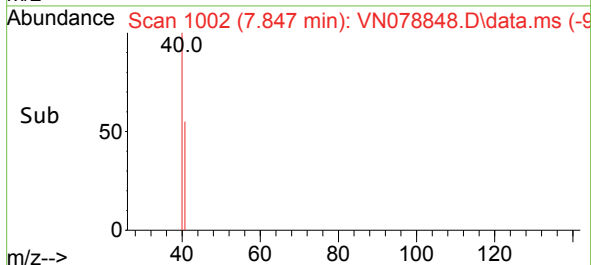






#31  
Cyclohexane  
Concen: 1.352 ug/l  
RT: 8.230 min Scan# 1067  
Delta R.T. -0.035 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 56 Resp: 5130  
Ion Ratio Lower Upper  
56 100  
69 133.2 26.8 40.2#  
84 109.6 81.8 122.6

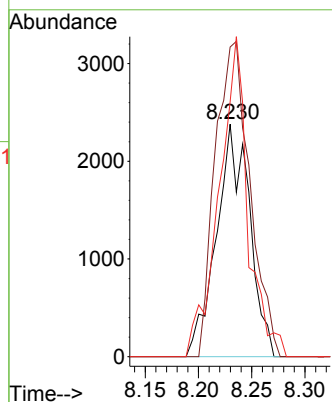

#33  
1,2-Dichloroethane-d4  
Concen: 52.269 ug/l  
RT: 8.583 min Scan# 1127  
Delta R.T. -0.006 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Tgt Ion: 65 Resp: 135028  
Ion Ratio Lower Upper  
65 100  
67 51.4 0.0 106.6


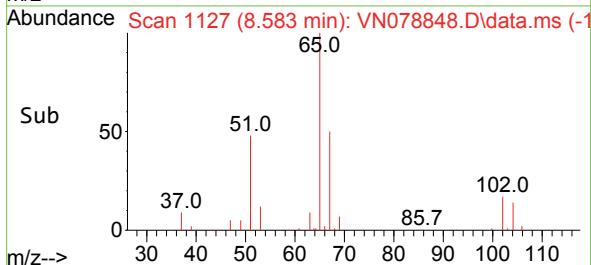
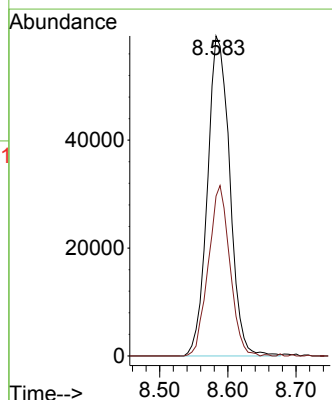
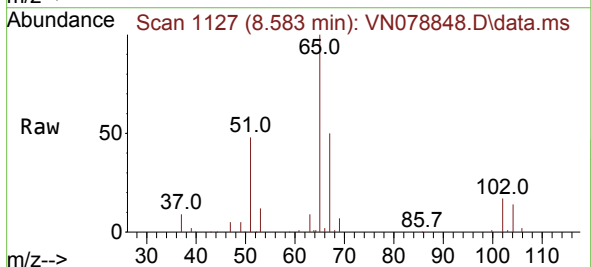




#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 9.112 min Scan# 11  
Delta R.T. 0.006 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:114 Resp: 333080  
Ion Ratio Lower Upper  
114 100  
63 22.1 0.0 36.4  
88 15.3 0.0 30.6

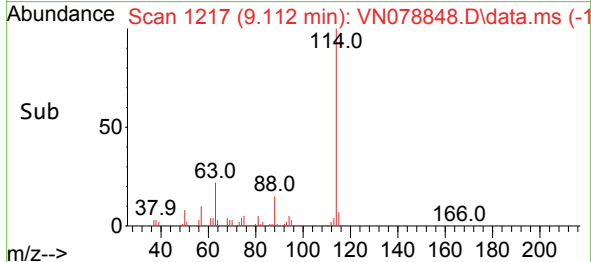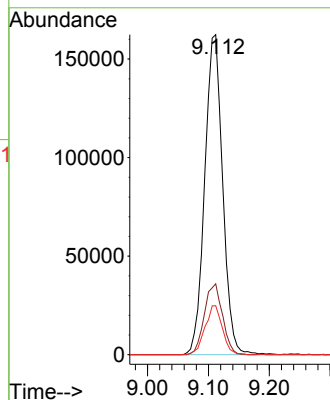

#35  
Dibromofluoromethane  
Concen: 49.008 ug/l  
RT: 8.177 min Scan# 1058  
Delta R.T. 0.006 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34


Tgt Ion:113 Resp: 110234  
Ion Ratio Lower Upper  
113 100  
111 104.1 82.6 123.8  
192 17.2 12.7 19.1

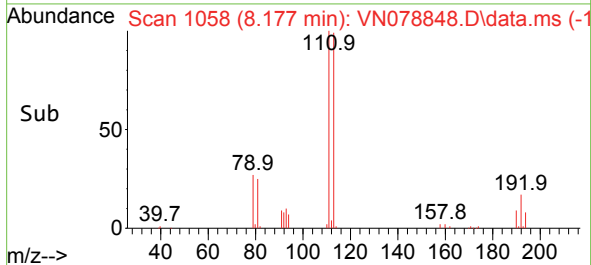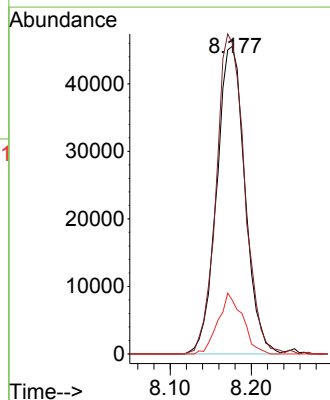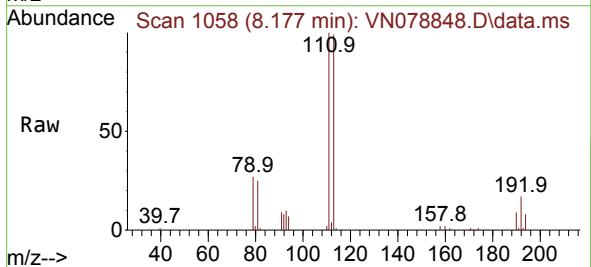






#36  
1,1-Dichloropropene  
Concen: 4.647 ug/l  
RT: 8.236 min Scan# 1068  
Delta R.T. -0.141 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 75 Resp: 16216  
Ion Ratio Lower Upper  
75 100  
110 11.4 19.1 57.3#  
77 0.0 25.0 37.4#

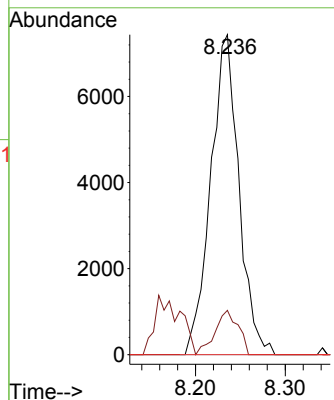

#37  
Ethyl Acetate  
Concen: 9.814 ug/l  
RT: 7.571 min Scan# 955  
Delta R.T. -0.000 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Tgt Ion: 43 Resp: 36411  
Ion Ratio Lower Upper  
43 100  
61 12.7 13.2 19.8#  
70 8.7 11.3 16.9#

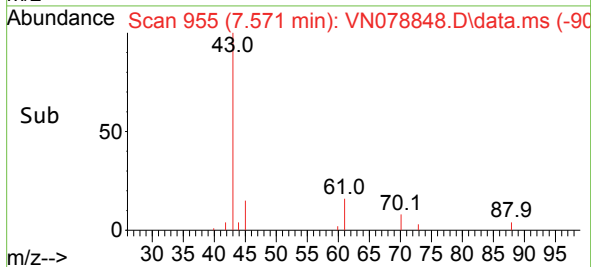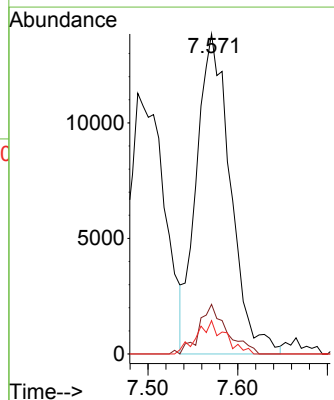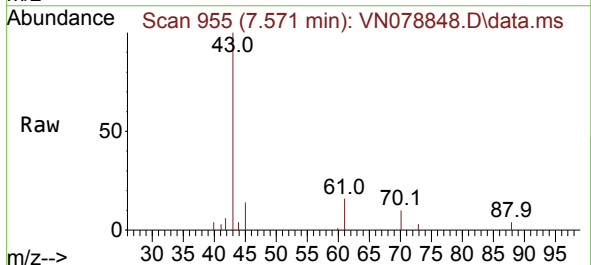



#38

Carbon Tetrachloride

Concen: 5.230 ug/l

RT: 8.236 min Scan# 110

Delta R.T. -0.135 min


Lab File: VN078848.D

Acq: 10 Aug 2023 19:34

Instrument :

MSVOA\_N

ClientSampleId :

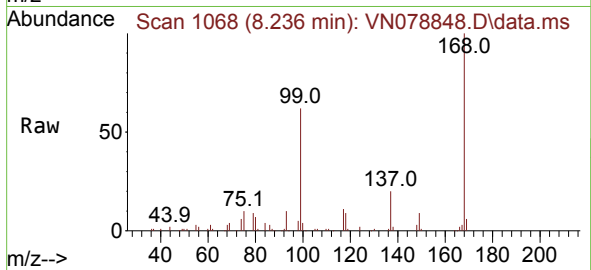




Tgt Ion:117 Resp: 18813

Ion Ratio Lower Upper

117 100

119 5.2 77.3 115.9#

121 0.0 23.3 34.9#

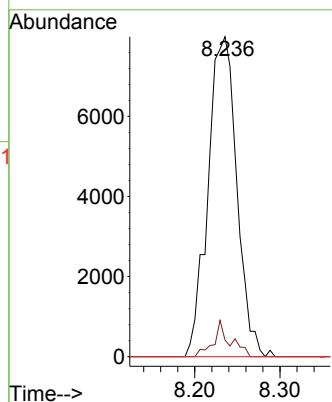

#42

1,2-Dichloroethane

Concen: 0.331 ug/l

RT: 8.683 min Scan# 1144

Delta R.T. 0.006 min

Lab File: VN078848.D




Acq: 10 Aug 2023 19:34


Tgt Ion: 62 Resp: 1254

Ion Ratio Lower Upper

62 100


98 0.0 0.0 19.8

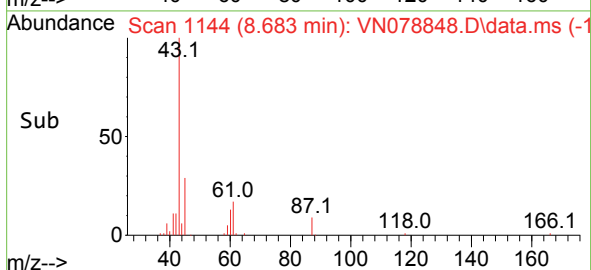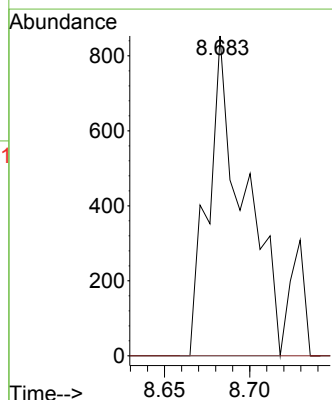






#43  
Isopropyl Acetate  
Concen: 38.768 ug/l  
RT: 8.700 min Scan# 1147  
Delta R.T. 0.006 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Instrument :  
MSVOA\_N  
ClientSampleId :



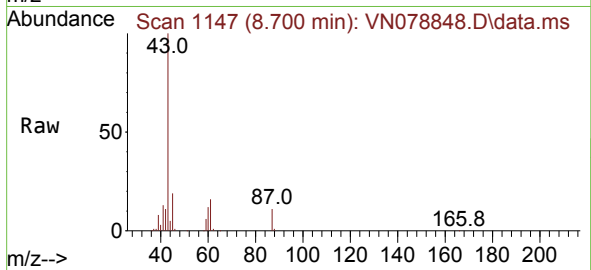



Tgt Ion: 43 Resp: 242509  
Ion Ratio Lower Upper  
43 100  
61 12.3 24.7 37.1#  
87 7.5 14.6 21.8#

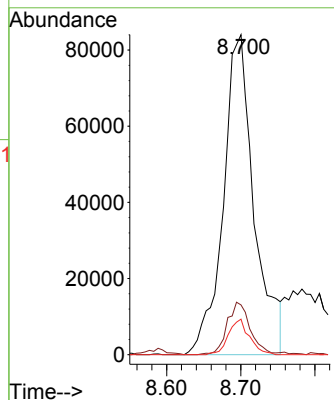

#48  
Methyl methacrylate  
Concen: 1.812 ug/l  
RT: 9.671 min Scan# 1312  
Delta R.T. -0.018 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Tgt Ion: 41 Resp: 5238  
Ion Ratio Lower Upper  
41 100  
69 0.0 90.4 135.6#  
39 70.0 54.6 81.8

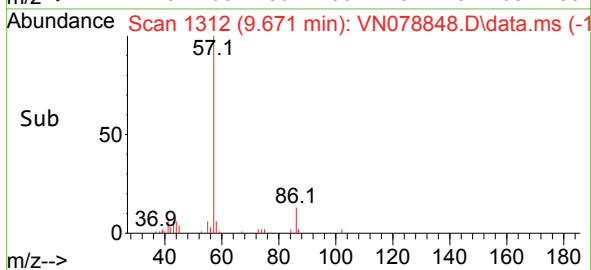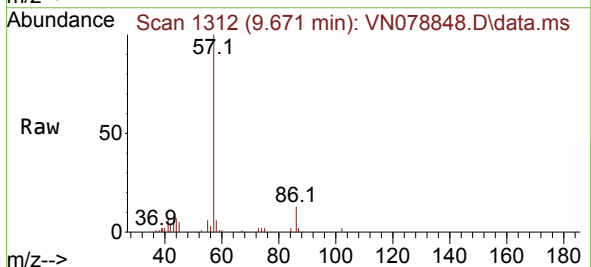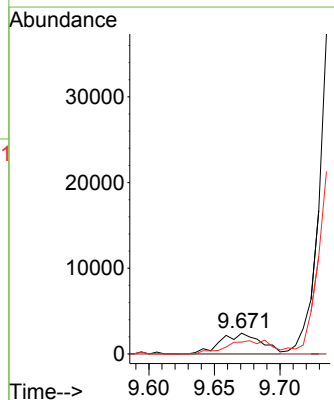



#49

1,4-Dioxane

Concen: 4.858 ug/l

RT: 9.735 min Scan# 1

Delta R.T. 0.035 min

Lab File: VN078848.D

Acq: 10 Aug 2023 19:34

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion: 88 Resp: 228

Ion Ratio Lower Upper

88 100

43 580412.7 17.0 25.6#

58 2612.3 47.0 70.4#

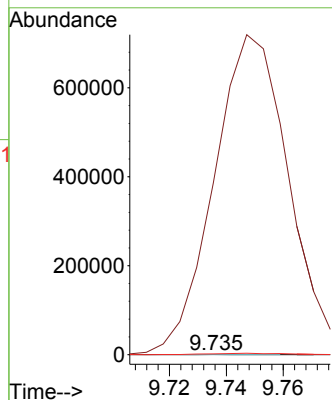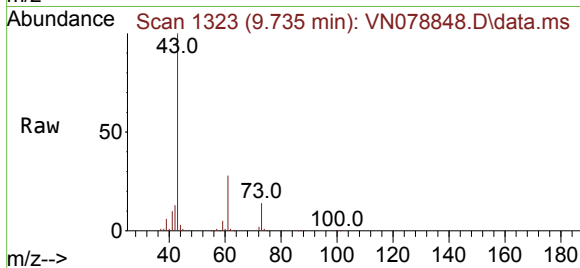

#50

Toluene-d8

Concen: 51.964 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN078848.D




Acq: 10 Aug 2023 19:34


Tgt Ion: 98 Resp: 430133

Ion Ratio Lower Upper

98 100

100 63.6 52.0 78.0



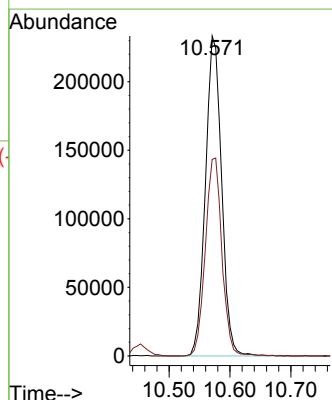
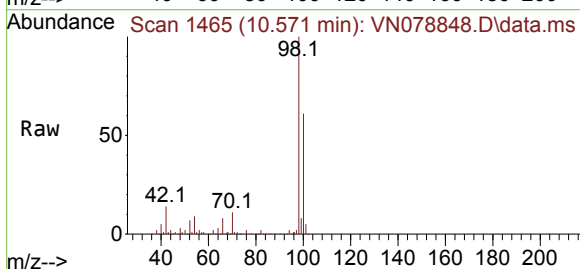


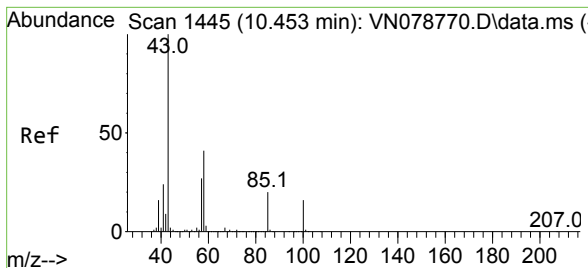

#51  
4-Methyl-2-Pentanone  
Concen: 29.895 ug/l  
RT: 10.453 min Scan# 1445  
Delta R.T. 0.000 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 114547  
Ion Ratio Lower Upper  
43 100  
58 34.7 36.6 54.8#

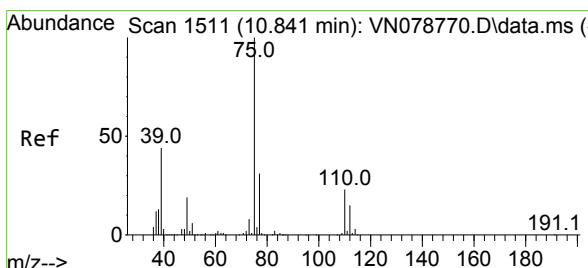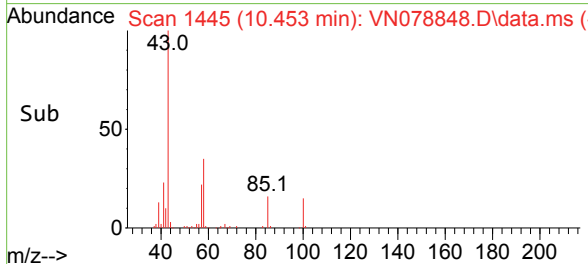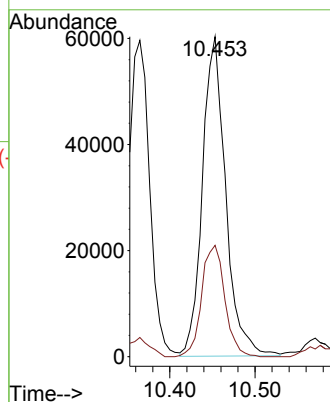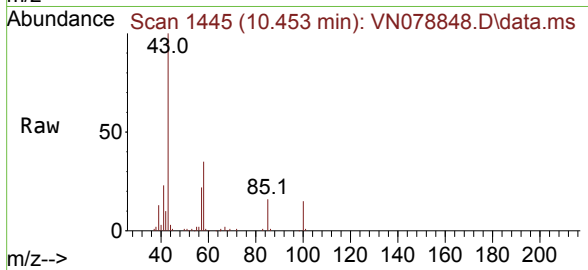

#53  
t-1,3-Dichloropropene  
Concen: 0.219 ug/l  
RT: 10.735 min Scan# 1493  
Delta R.T. -0.106 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Tgt Ion: 75 Resp: 840  
Ion Ratio Lower Upper  
75 100  
77 5.3 25.4 38.0#


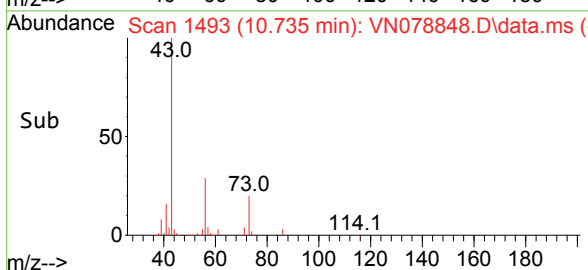
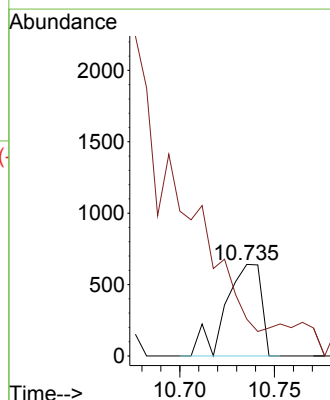
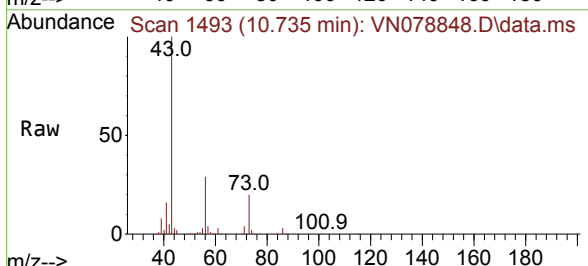


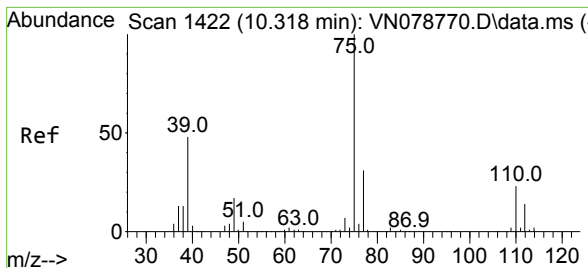

#54  
 cis-1,3-Dichloropropene  
 Concen: 11.097 ug/l  
 RT: 10.365 min Scan# 14  
 Delta R.T. 0.047 min  
 Lab File: VN078848.D  
 Acq: 10 Aug 2023 19:34




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion: 75 Resp: 46172  
 Ion Ratio Lower Upper  
 75 100  
 77 0.6 26.1 39.1#  
 39 42.9 31.6 47.4

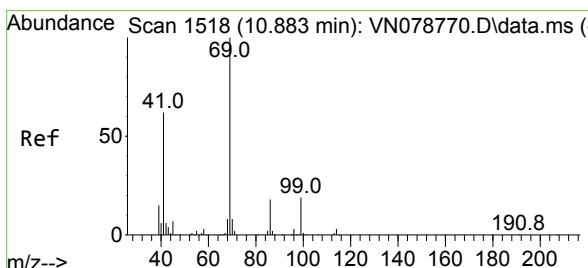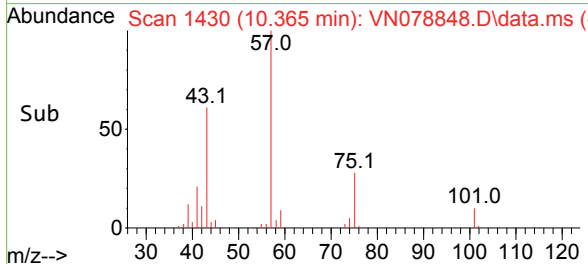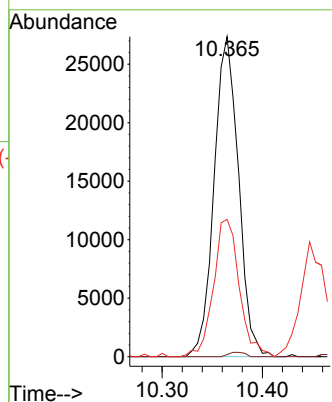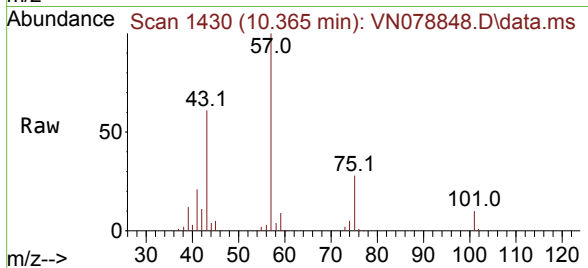

#56  
 Ethyl methacrylate  
 Concen: 0.627 ug/l  
 RT: 10.988 min Scan# 1536  
 Delta R.T. 0.106 min  
 Lab File: VN078848.D  
 Acq: 10 Aug 2023 19:34

Tgt Ion: 69 Resp: 2330  
 Ion Ratio Lower Upper  
 69 100  
 41 3359.4 39.6 59.4#  
 39 1596.4 28.6 43.0#

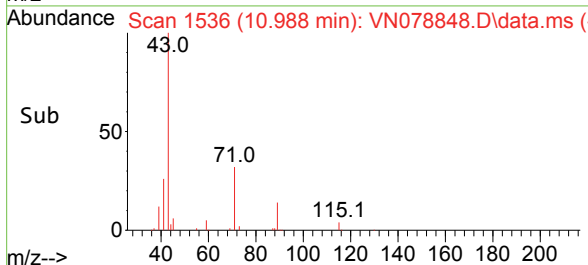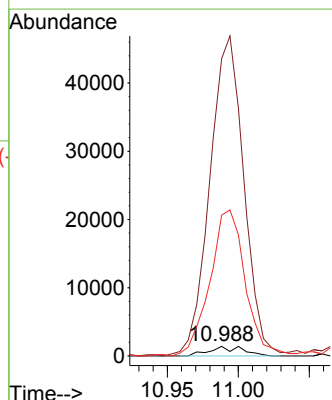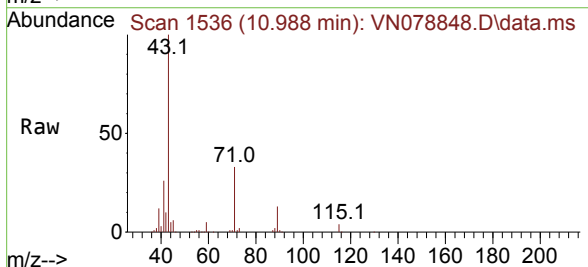

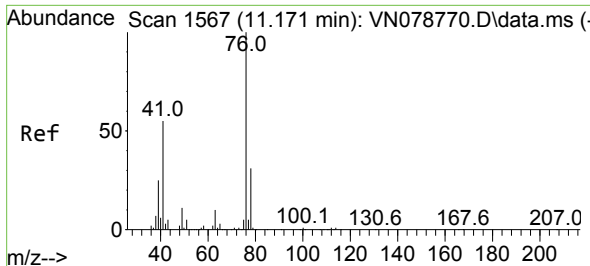

#57

1,3-Dichloropropane

Concen: 1.257 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.035 min


Lab File: VN078848.D

Acq: 10 Aug 2023 19:34

Instrument :

MSVOA\_N

ClientSampleId :



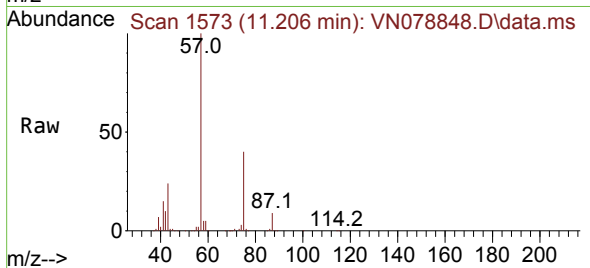


Tgt Ion: 76 Resp: 5598

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

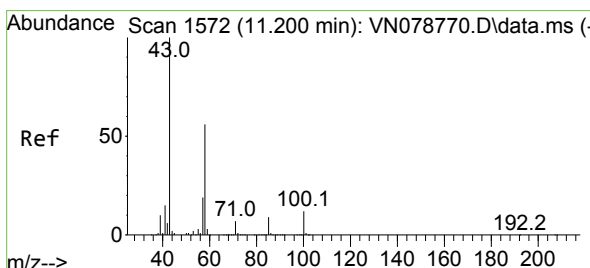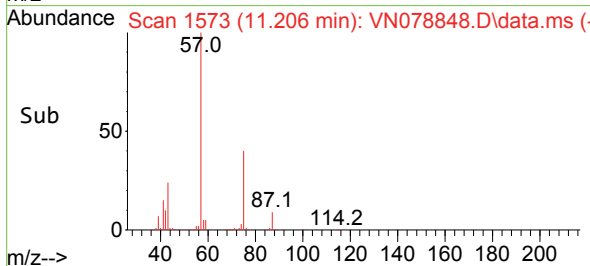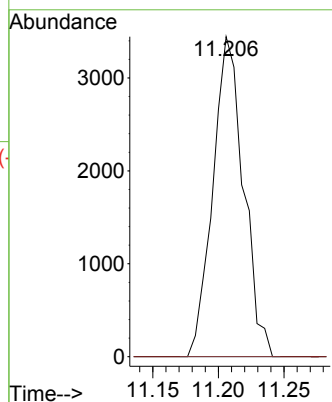

#59

2-Hexanone

Concen: 47.888 ug/l

RT: 11.177 min Scan# 1568

Delta R.T. -0.023 min

Lab File: VN078848.D




Acq: 10 Aug 2023 19:34


Tgt Ion: 43 Resp: 129925

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


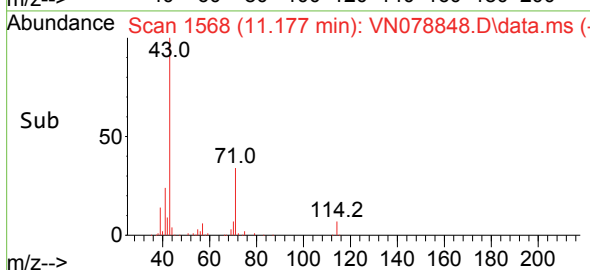
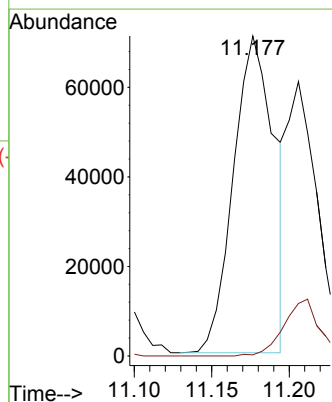
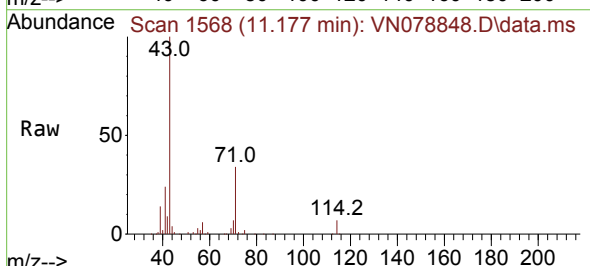


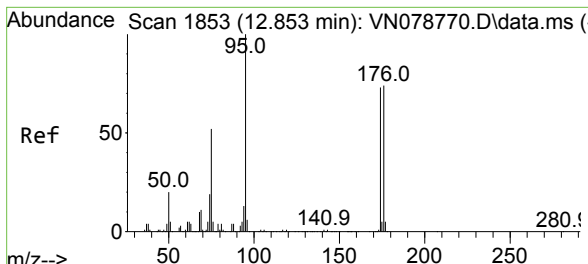

#62  
 4-Bromofluorobenzene  
 Concen: 46.861 ug/l  
 RT: 12.859 min Scan# 115925  
 Delta R.T. 0.006 min  
 Lab File: VN078848.D  
 Acq: 10 Aug 2023 19:34




Instrument :  
 MSVOA\_N  
 ClientSampleId :


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 95    | Resp: | 115925 |
| Ion      | Ratio | Lower | Upper  |
| 95       | 100   |       |        |
| 174      | 75.8  | 0.0   | 143.8  |
| 176      | 74.3  | 0.0   | 135.8  |

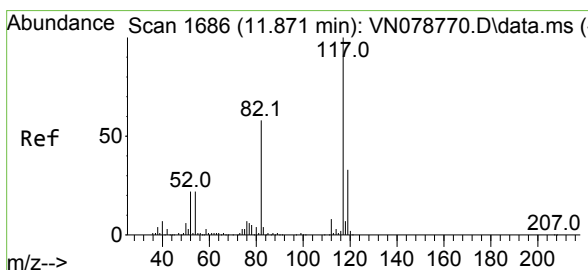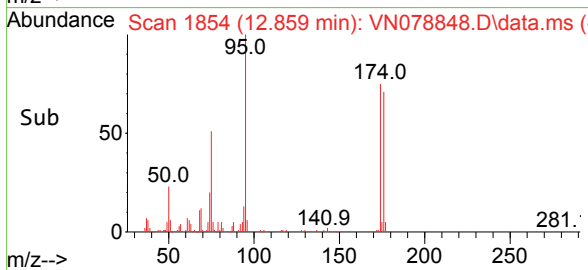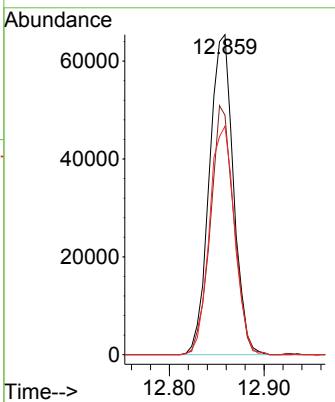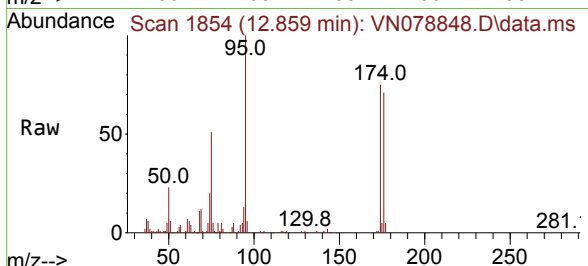

#63  
 Chlorobenzene-d5  
 Concen: 50.000 ug/l  
 RT: 11.871 min Scan# 1686  
 Delta R.T. -0.000 min  
 Lab File: VN078848.D  
 Acq: 10 Aug 2023 19:34

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 117   | Resp: | 310134 |
| Ion      | Ratio | Lower | Upper  |
| 117      | 100   |       |        |
| 82       | 58.3  | 44.0  | 66.0   |
| 119      | 31.9  | 25.6  | 38.4   |

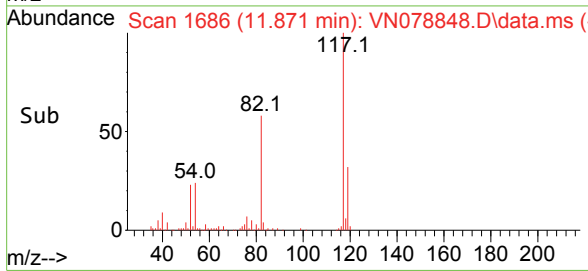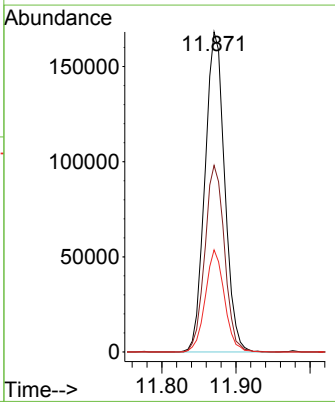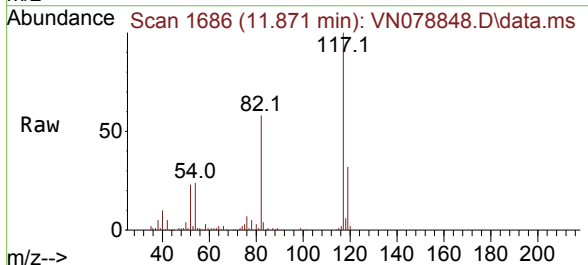

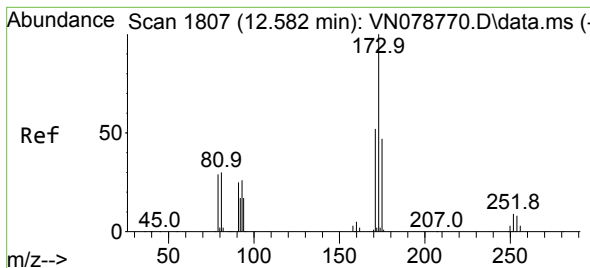

#71

Bromoform

Concen: 0.444 ug/l

RT: 12.853 min Scan# 11

Delta R.T. 0.270 min

Lab File: VN078848.D

Acq: 10 Aug 2023 19:34

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion:173 Resp: 847

Ion Ratio Lower Upper

173 100

175 638.3 24.3 73.0#

254 0.0 0.0 0.0

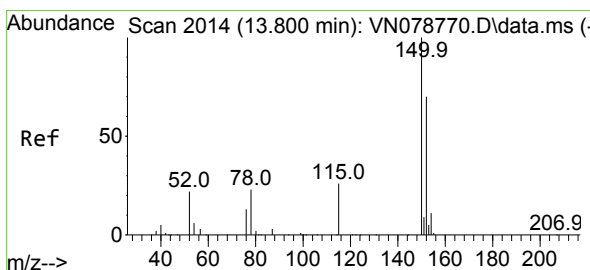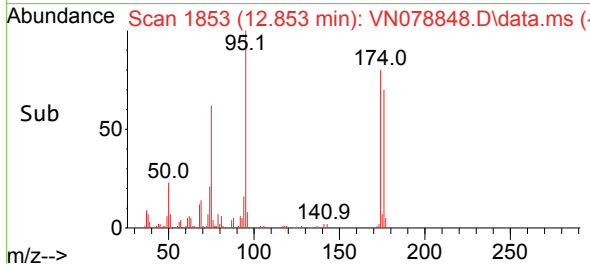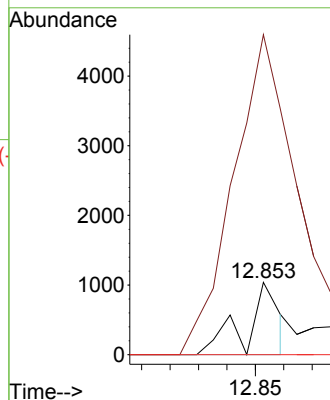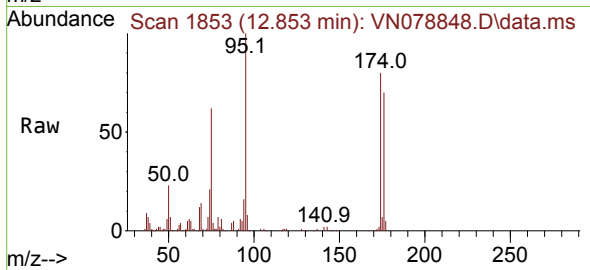

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.006 min

Lab File: VN078848.D

Acq: 10 Aug 2023 19:34




Tgt Ion:152 Resp: 86863


Ion Ratio Lower Upper

152 100

115 60.1 32.3 96.8


150 157.7 0.0 355.8

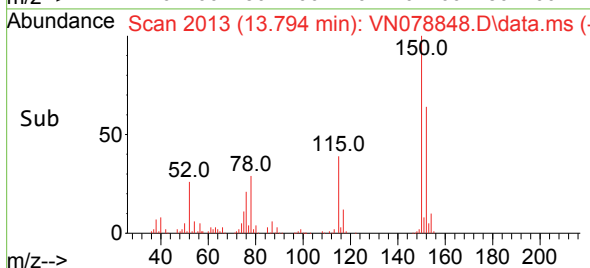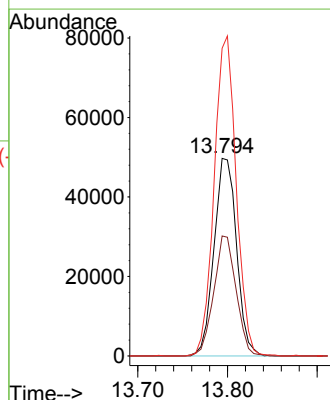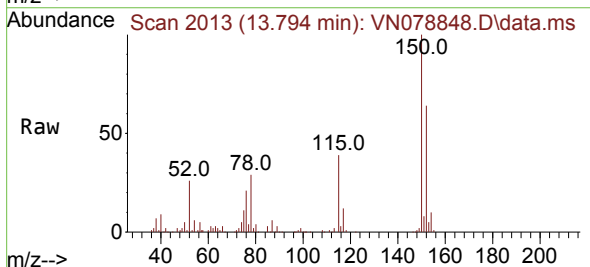






#74  
N-amy1 acetate  
Concen: 1.070 ug/l  
RT: 12.471 min Scan# 1788  
Delta R.T. -0.030 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34

Instrument :  
MSVOA\_N  
ClientSampleId :







|             |             |
|-------------|-------------|
| Tgt Ion: 43 | Resp: 4151  |
| Ion Ratio   | Lower Upper |
| 43 100      |             |
| 70 0.0      | 43.4 65.2#  |
| 55 0.0      | 21.4 32.0#  |
| 61 0.0      | 22.8 34.2#  |

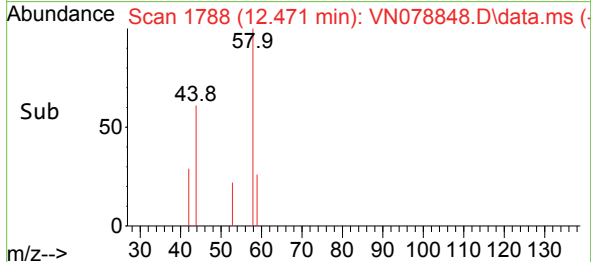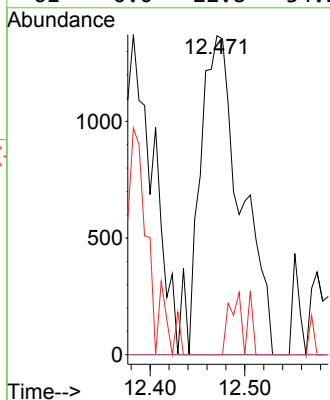

#76  
1,2,3-Trichloropropane  
Concen: 28.227 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. -0.147 min  
Lab File: VN078848.D  
Acq: 10 Aug 2023 19:34


|             |             |
|-------------|-------------|
| Tgt Ion: 75 | Resp: 66290 |
| Ion Ratio   | Lower Upper |
| 75 100      |             |
| 77 1.7      | 84.5 253.5# |

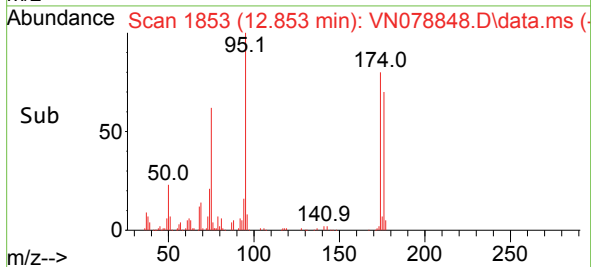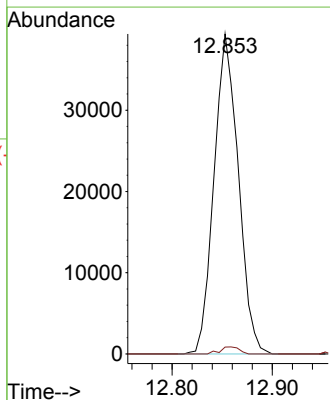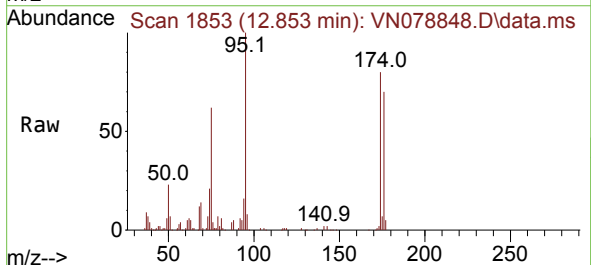

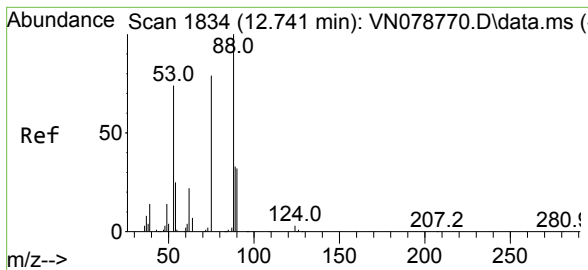

#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 75.742 ug/l  
 RT: 12.853 min Scan# 1853  
 Delta R.T. 0.112 min  
 Lab File: VN078848.D  
 Acq: 10 Aug 2023 19:34

Instrument :  
 MSVOA\_N  
 ClientSampleId :

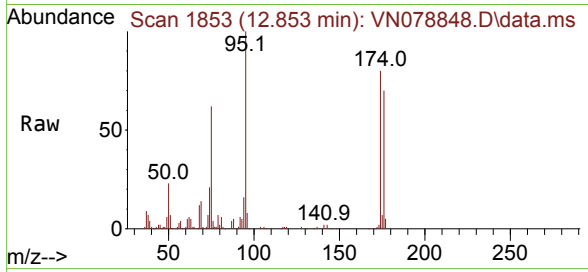

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 75    | Resp: | 66290  |
| Ion      | Ratio | Lower | Upper  |
| 75       | 100   |       |        |
| 53       | 0.1   | 67.4  | 101.2# |
| 89       | 0.1   | 38.8  | 58.2#  |

