
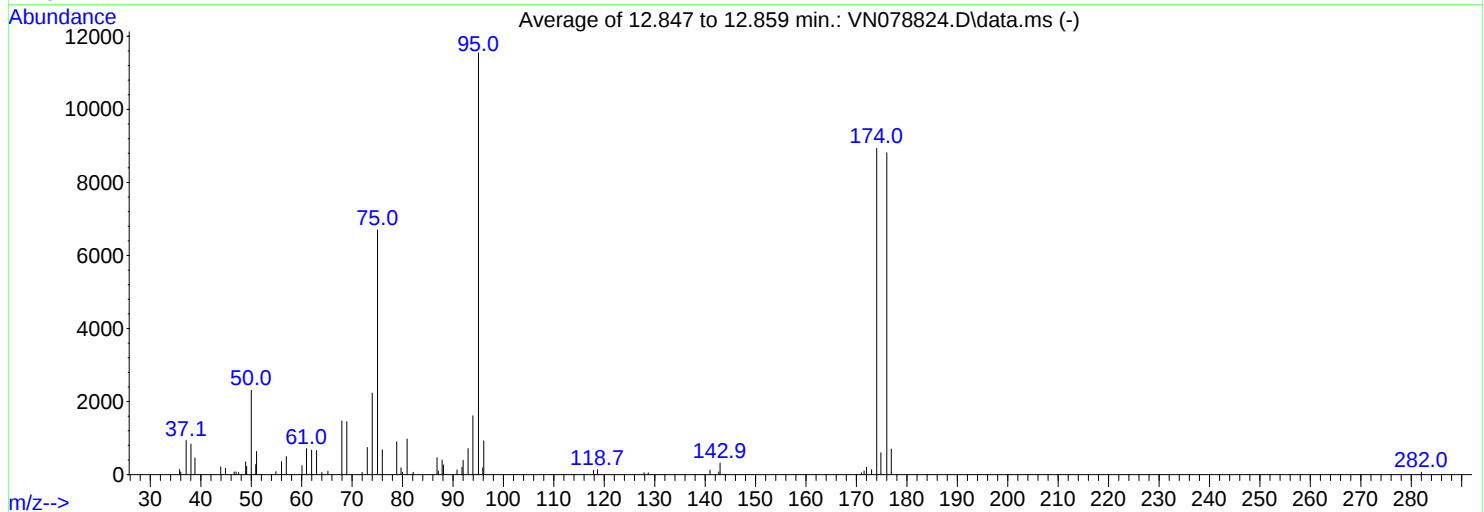


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081023\
 Data File : VN078824.D
 Acq On : 10 Aug 2023 09:15
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080723W.M
 Title : SW846 8260
 Last Update : Tue Aug 08 05:03:52 2023

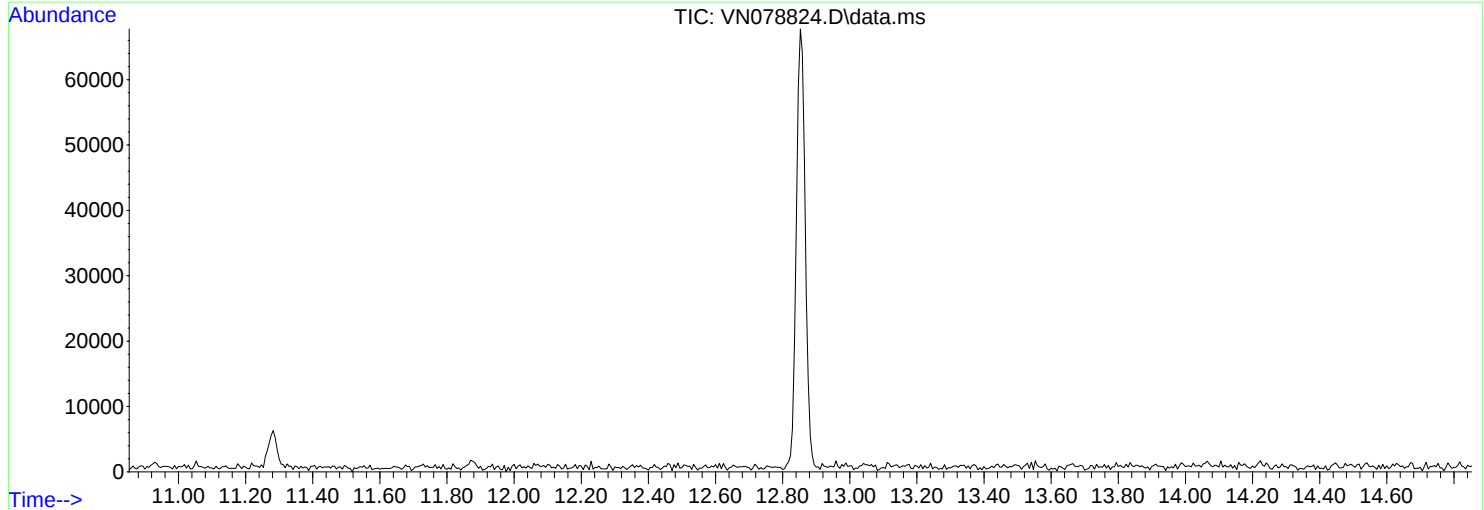

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	2314	PASS
75	95	30	60	58.0	6703	PASS
95	95	100	100	100.0	11547	PASS
96	95	5	9	8.0	926	PASS
173	174	0.00	2	1.5	136	PASS
174	95	50	100	77.4	8934	PASS
175	174	5	9	6.7	599	PASS
176	174	95	101	98.6	8813	PASS
177	176	5	9	7.9	699	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	142	49.10	222	64.00	63	80.00	61
36.00	70	50.00	2314	65.20	90	80.90	97
37.10	936	50.90	274	67.95	1474	82.10	6
38.05	838	51.05	635	68.95	1450	86.85	46
38.85	457	54.90	83	72.00	62	87.10	96
43.95	213	56.00	359	73.00	744	87.85	404
44.90	177	56.95	493	74.00	2234	88.10	266
46.60	74	60.05	251	75.05	6703	90.80	130
47.00	76	60.95	714	76.00	680	91.80	203
47.50	55	61.95	670	78.85	901	92.00	395
48.90	351	62.95	663	79.70	187	93.00	714

Average of 12.847 to 12.859 min.: VN078824.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.95	1612	171.00	53				
95.05	11547	171.50	100				
95.90	188	172.00	202				
96.10	926	173.00	136				
117.85	117	174.00	8934				
118.65	135	174.85	599				
127.90	53	176.00	8813				
128.70	52	176.90	699				
140.95	125	282.00	67				
142.70	75						
142.95	321						

Instrument :

MSVOA_N

ClientSampleId :

BFB