
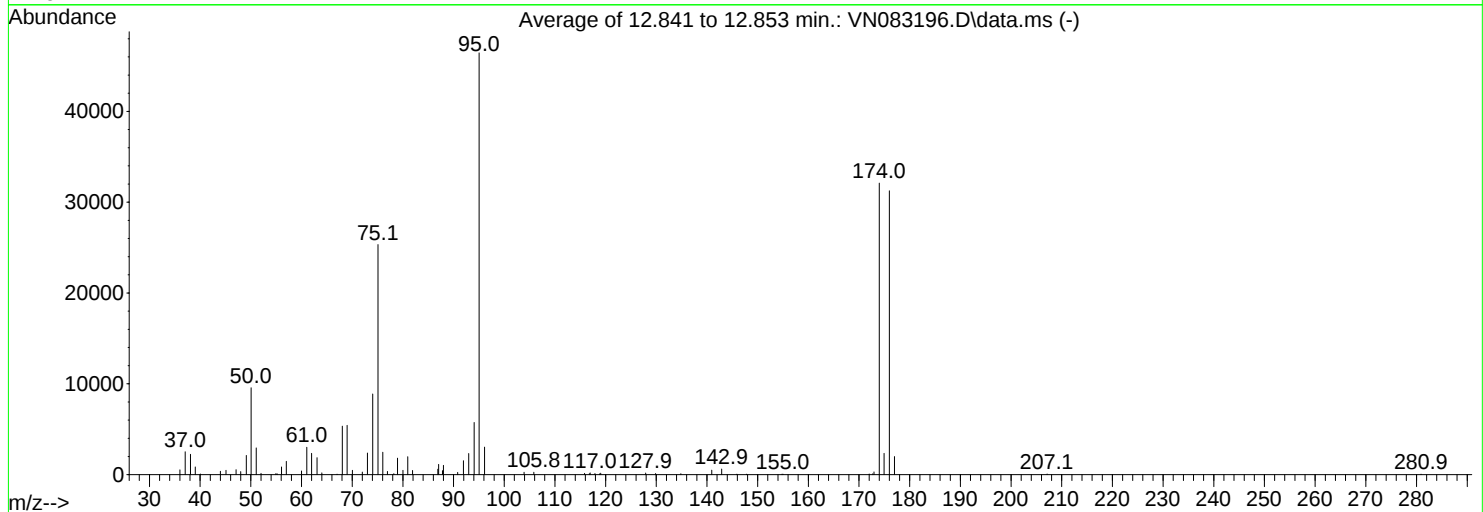


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081024\
Data File : VN083196.D
Acq On : 10 Aug 2024 09:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

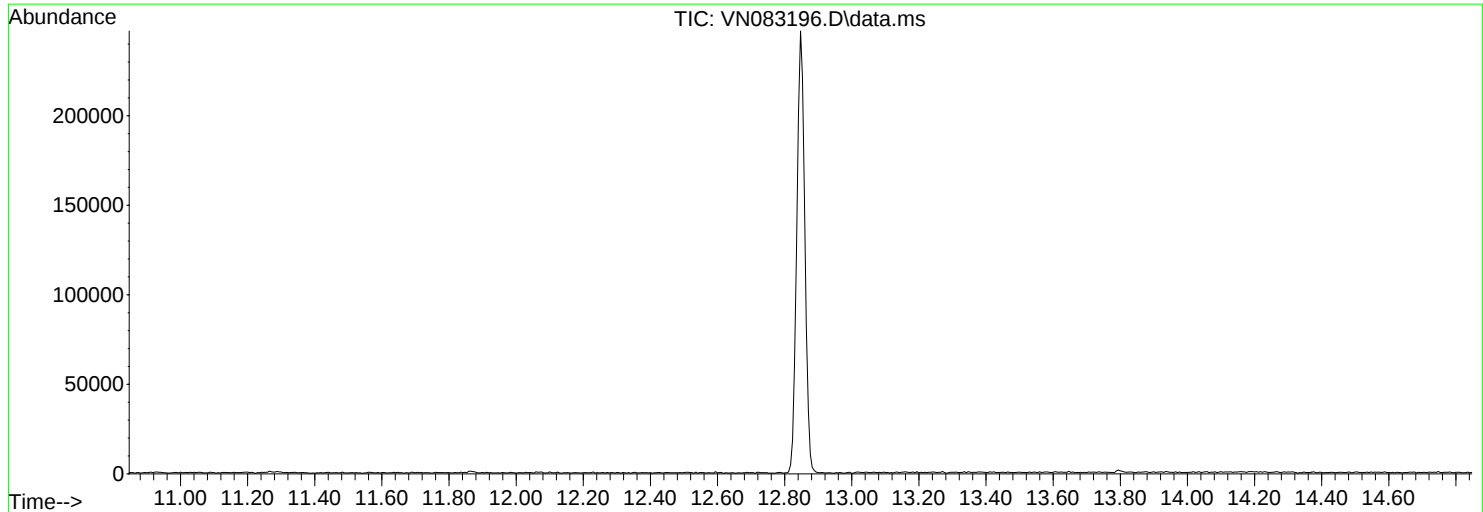

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	9568	PASS
75	95	30	60	54.6	25341	PASS
95	95	100	100	100.0	46448	PASS
96	95	5	9	6.5	3039	PASS
173	174	0.00	2	0.9	294	PASS
174	95	50	100	69.1	32104	PASS
175	174	5	9	7.3	2349	PASS
176	174	95	101	97.4	31261	PASS
177	176	5	9	6.4	1987	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	532	51.05	2947	67.00	56	78.95	180
37.05	2515	52.00	145	68.05	5338	80.00	48
38.10	2235	54.95	133	69.00	5435	80.95	197
39.05	855	55.20	81	70.05	479	81.90	46
40.05	79	56.05	843	72.00	289	86.90	607
44.00	369	57.00	1460	73.00	2380	87.05	1131
45.10	468	60.00	411	74.05	8877	87.80	437
47.10	538	61.05	3011	75.10	25341	88.00	1028
48.00	333	62.00	2343	76.05	2466	90.80	242
49.10	2109	63.05	1861	76.95	351	91.95	1540
50.05	9568	64.00	195	78.20	108	93.00	2320

Average of 12.841 to 12.853 min.: VN083196.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	5742	127.90	174	172.95	294		
95.05	46448	129.85	124	174.00	32104		
96.10	3039	134.85	112	174.95	2349		
103.90	263	140.95	488	176.00	31261		
105.85	266	142.90	617	177.00	1987		
115.85	149	145.90	57	207.10	65		
116.80	101	147.80	51	280.90	51		
116.95	194	154.80	54				
117.90	120	155.00	54				
118.80	92	172.00	73				
119.05	159	172.70	94				