

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081119\
 Data File : VN057195.D
 Acq On : 11 Aug 2019 18:18
 Operator : JC/SP
 Sample : K4245-08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-26

Quant Time: Aug 12 05:57:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:49:25 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	1319245	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.01	114	1869981	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.91	117	1537787	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.88	152	402845	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.44	65	621135	45.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.56%	
35) Dibromofluoromethane	6.99	113	561690	47.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.74%	
50) Toluene-d8	9.56	98	2168978	48.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.62%	
62) 4-Bromofluorobenzene	11.92	95	574274	39.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	79.40%	
Target Compounds						
					Qvalue	
8) Diethyl Ether	3.14	74	2701	0.371	ug/l	55
11) Tert butyl alcohol	4.23	59	1778	0.921	ug/l #	73
16) Acetone	3.48	43	37507	9.154	ug/l	98
18) Methyl Acetate	3.90	43	52692	3.708	ug/l	95
20) Methylene Chloride	4.10	84	23964	1.772	ug/l	95
25) 2-Butanone	6.22	43	2430	0.388	ug/l	93
31) Cyclohexane	7.05	56	19369	0.984	ug/l #	1
36) 1,1-Dichloropropene	7.05	75	79518	5.165	ug/l #	49
37) Ethyl Acetate	6.30	43	151	Below Cal	#	70
38) Carbon Tetrachloride	7.05	117	111721	6.963	ug/l #	16
43) Isopropyl Acetate	7.57	43	148055	6.836	ug/l #	64
48) Methyl methacrylate	8.62	41	20901	2.046	ug/l #	10
49) 1,4-Dioxane	8.71	88	465	2.235	ug/l #	1
51) 4-Methyl-2-Pentanone	9.45	43	8100	0.643	ug/l	94
54) cis-1,3-Dichloropropene	9.36	75	143339	7.637	ug/l #	62
57) 1,3-Dichloropropane	10.25	76	26728	1.362	ug/l #	42
59) 2-Hexanone	10.25	43	331292	38.833	ug/l #	49
71) Bromoform	11.92	173	2603	0.307	ug/l #	1
73) Isopropylbenzene	11.77	105	188	Below Cal	#	48
74) N-amyl acetate	11.39	43	27408	2.685	ug/l #	50
76) 1,2,3-Trichloropropane	11.92	75	258639	31.816	ug/l #	100
79) 2-Chlorotoluene	12.31	91	122	Below Cal		74
81) trans-1,4-Dichloro-2-buten	11.92	75	258639	94.401	ug/l #	14
83) tert-Butylbenzene	12.53	119	76	Below Cal	#	28
93) 1,2,4-Trichlorobenzene	14.45	180	327	5.980	ug/l #	57
95) Naphthalene	14.68	128	318	2.833	ug/l #	69
96) 1,2,3-Trichlorobenzene	14.83	180	210	5.752	ug/l #	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN081119\
Data File : VN057195.D
Acq On : 11 Aug 2019 18:18
Operator : JC/SP
Sample : K4245-08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMP-26

Quant Time: Aug 12 05:57:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:49:25 2019
Response via : Initial Calibration

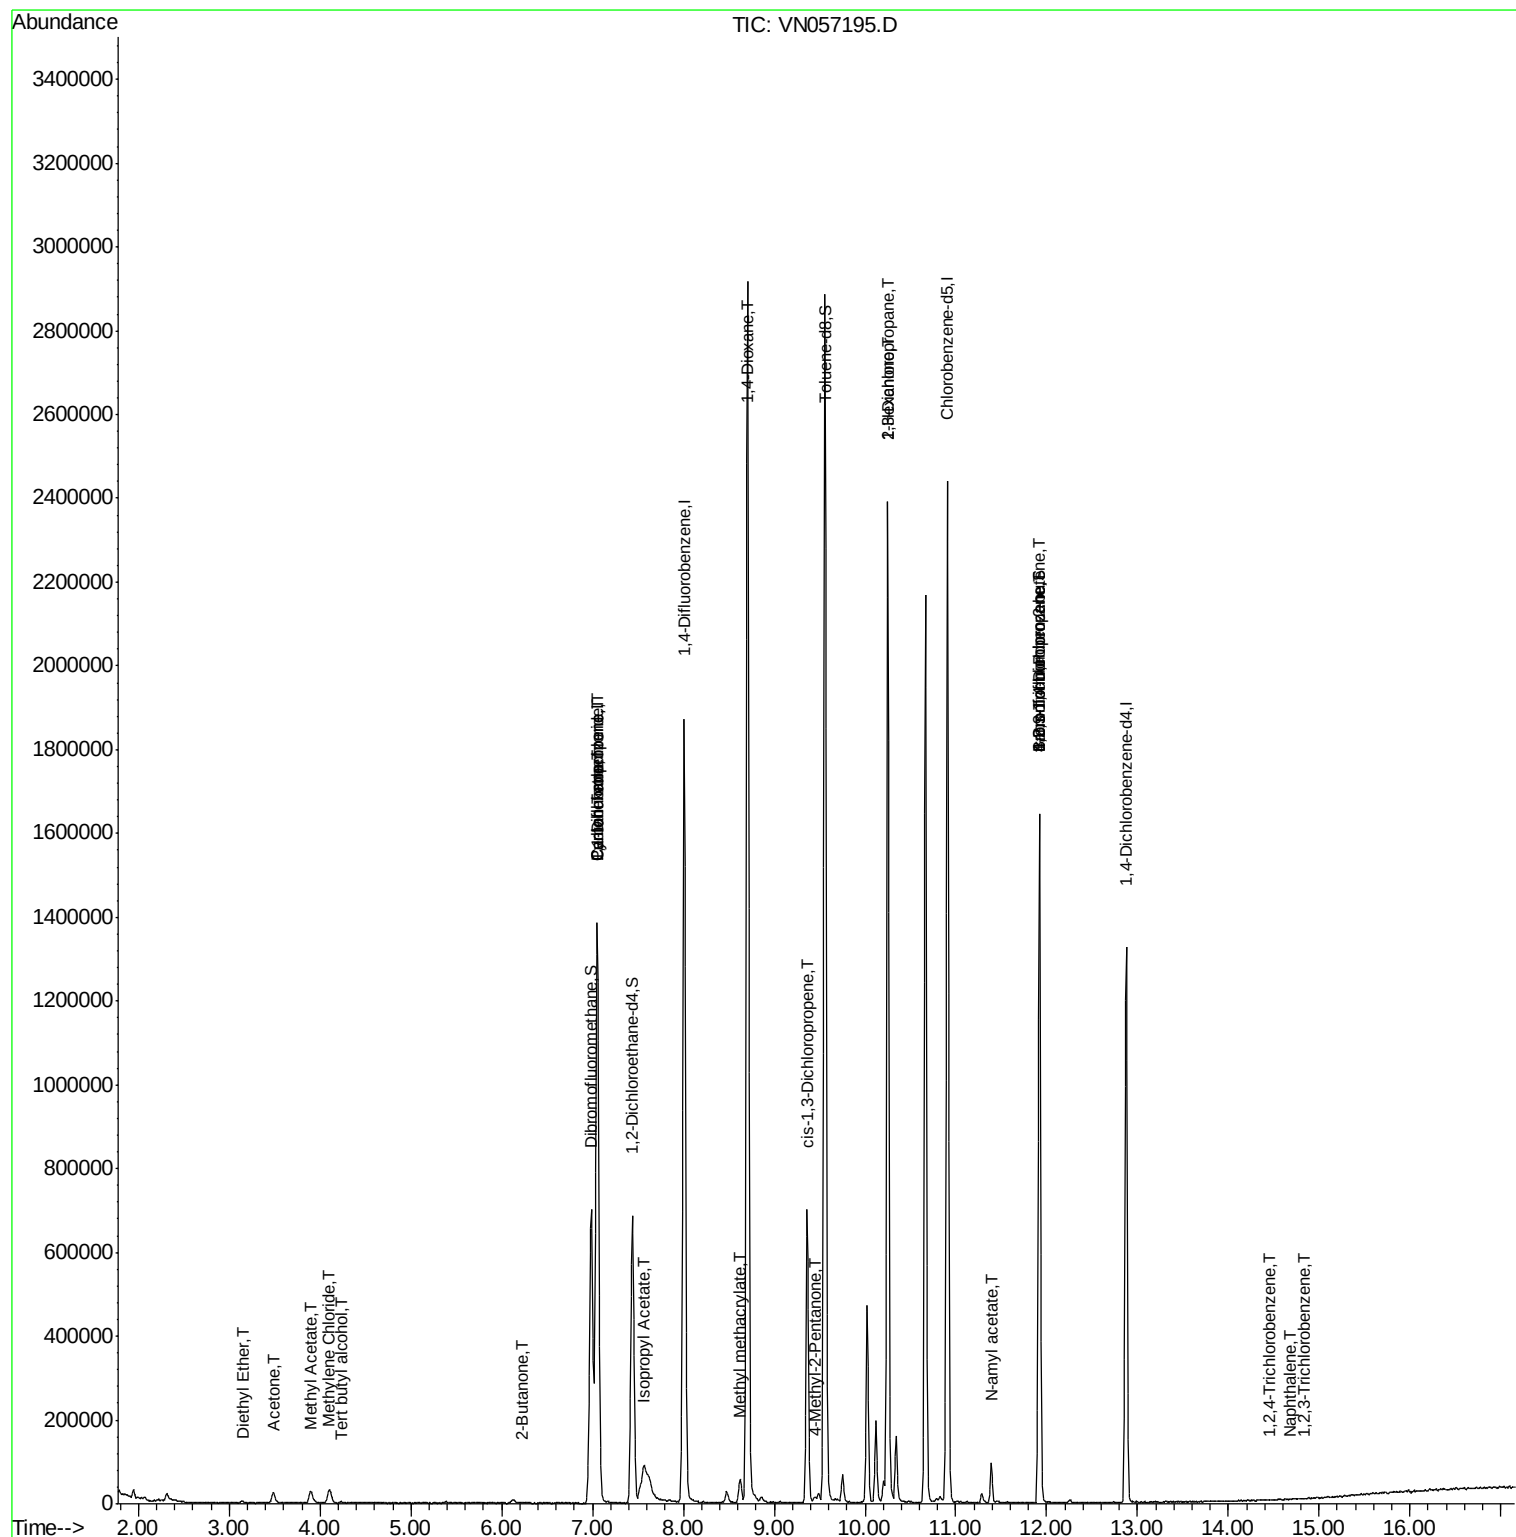

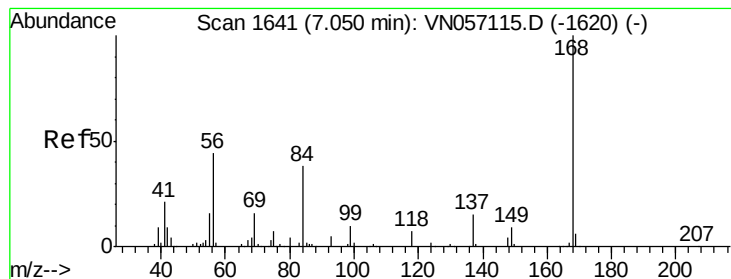

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 1642

Delta R.T. 0.00 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampleId :


COMP-26

Tgt Ion:168 Resp: 1319245

Ion Ratio Lower Upper

168 100

99 47.1 38.6 57.8

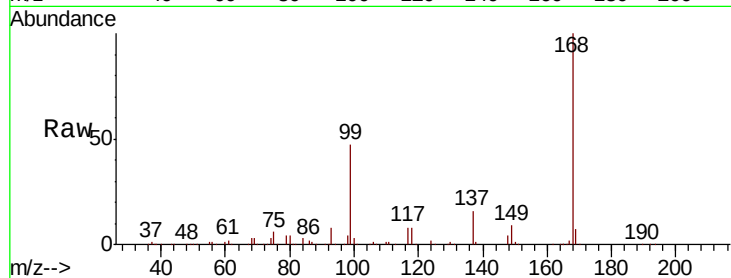

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.05

600000

500000

400000



300000

200000

100000

0

Time--> 6.90 7.00 7.10 7.20

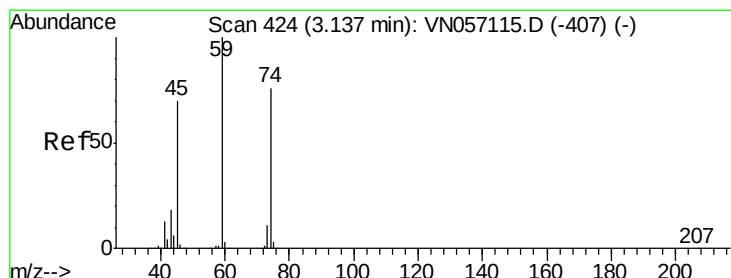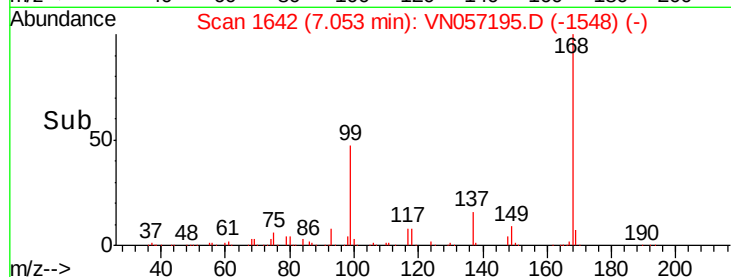

#8

Diethyl Ether

Concen: 0.371 ug/l

RT: 3.14 min Scan# 425

Delta R.T. 0.00 min

Lab File: VN057195.D


Acq: 11 Aug 2019 18:18

Tgt Ion: 74 Resp: 2701

Ion Ratio Lower Upper

74 100

45 49.8 46.3 138.8

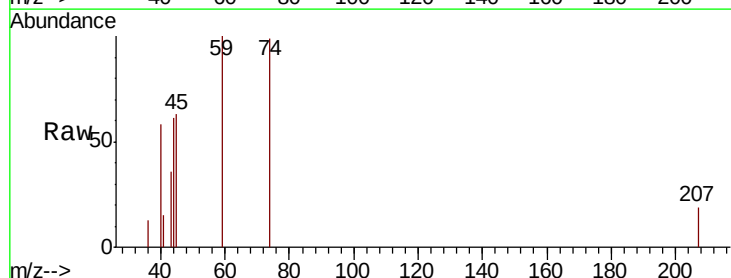

Abundance Ion 74.00 (73.70 to 74.70): VN

Ion 45.00 (44.70 to 45.70): VN

3.14


1500


1000

500

0

Time--> 3.10 3.15

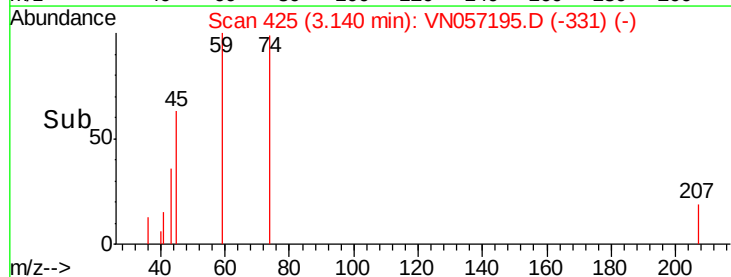

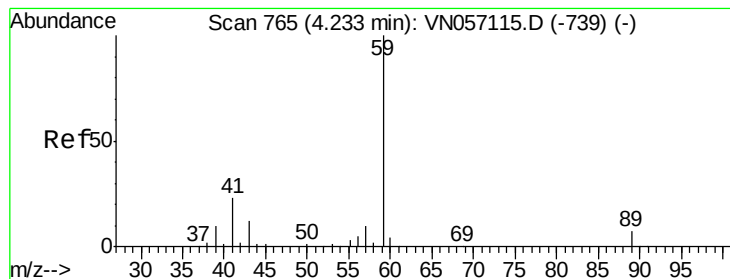

#11

Tert butyl alcohol

Concen: 0.921 ug/l

RT: 4.23 min Scan# 764

Delta R.T. -0.00 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampled :


COMP-26

Tgt Ion: 59 Resp: 1778

Ion Ratio Lower Upper




59 100

57 0.0 7.9 11.9#



Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

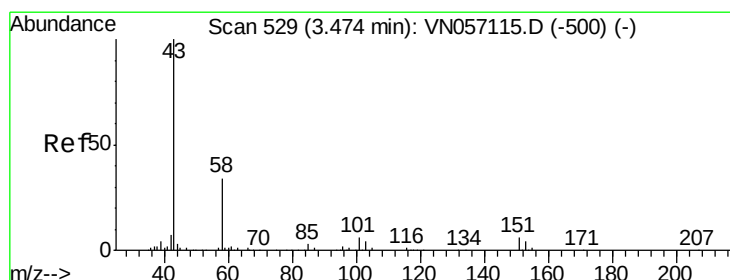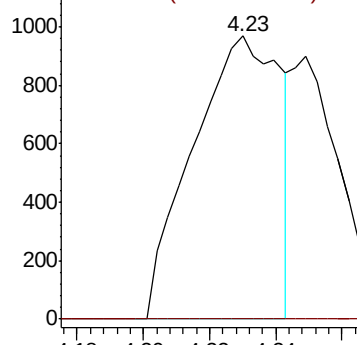

#16

Acetone

Concen: 9.154 ug/l

RT: 3.48 min Scan# 531

Delta R.T. 0.01 min

Lab File: VN057195.D


Acq: 11 Aug 2019 18:18

Tgt Ion: 43 Resp: 37507

Ion Ratio Lower Upper



43 100


58 35.3 27.4 41.2



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




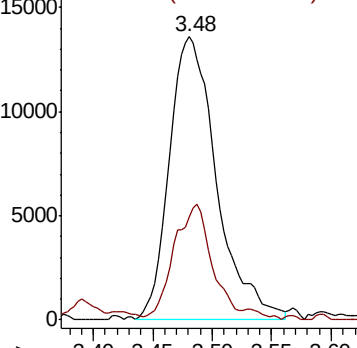


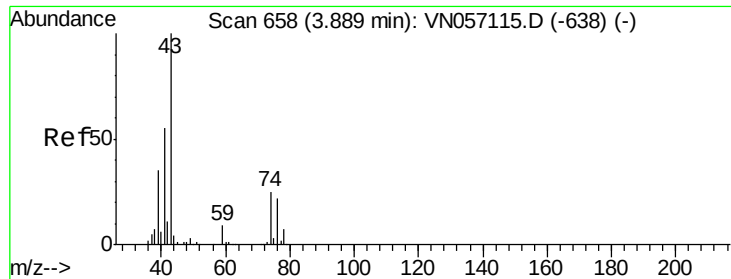

#18
Methyl Acetate
Concen: 3.708 ug/l
RT: 3.90 min Scan# 660
Delta R.T. 0.01 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18




Instrument :
MSVOA_N
ClientSampleId :
COMP-26


Tgt Ion: 43 Resp: 52692
Ion Ratio Lower Upper
43 100
74 22.7 20.2 30.4

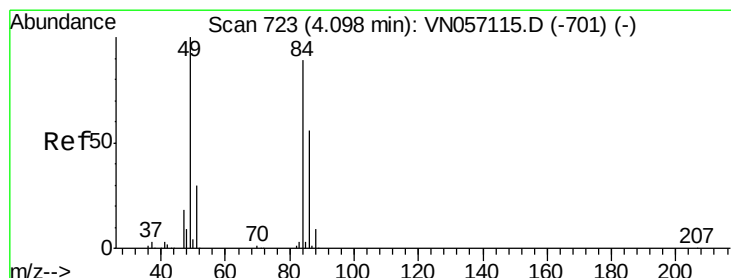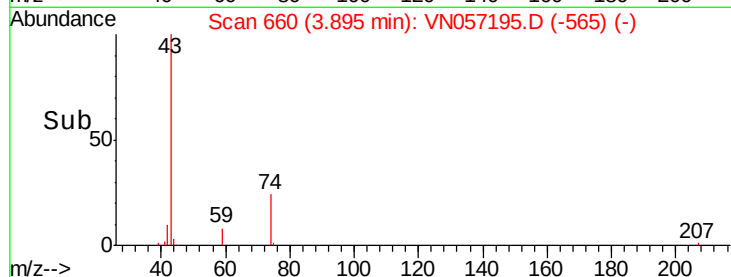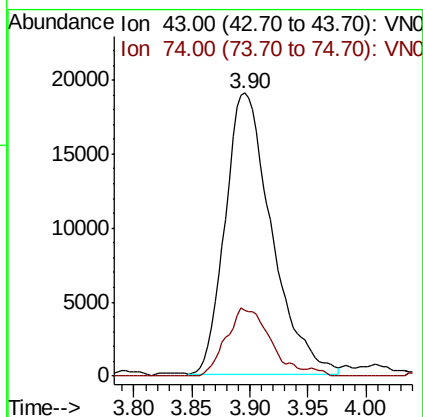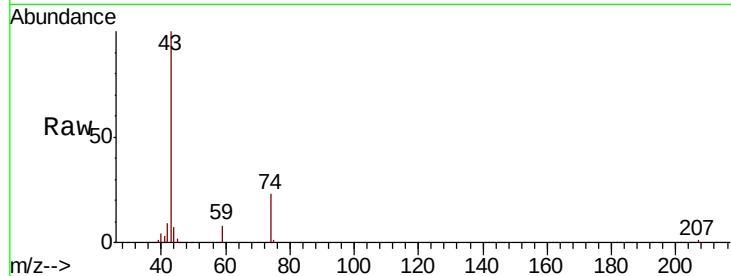

#20
Methylene Chloride
Concen: 1.772 ug/l
RT: 4.10 min Scan# 723
Delta R.T. -0.00 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18

Tgt Ion: 84 Resp: 23964
Ion Ratio Lower Upper
84 100
49 108.5 89.5 134.3
51 28.0 27.2 40.8
86 58.9 50.6 75.8


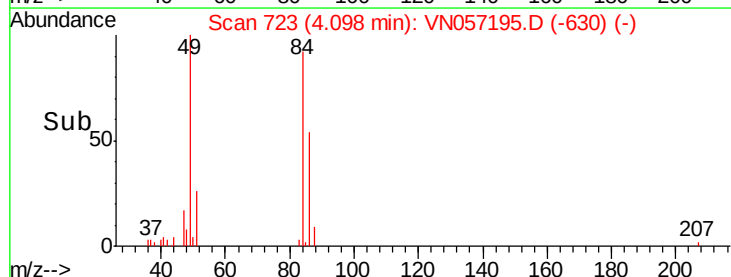
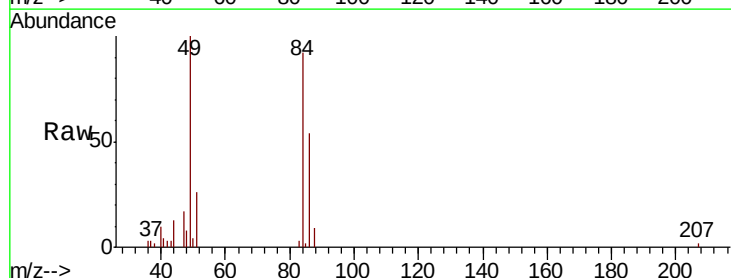
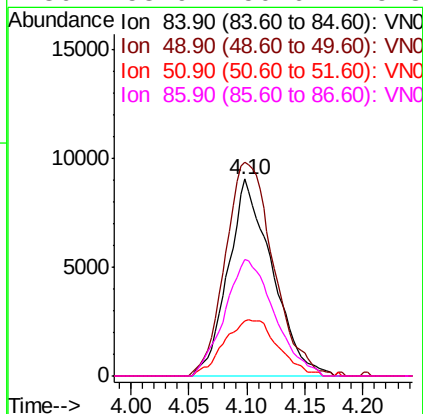




#25
2-Butanone
Concen: 0.388 ug/l
RT: 6.22 min Scan# 1382
Delta R.T. 0.02 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18




Instrument :
MSVOA_N
ClientSampleId :
COMP-26


Tgt Ion: 43 Resp: 2430
Ion Ratio Lower Upper
43 100
72 24.0 22.2 33.4

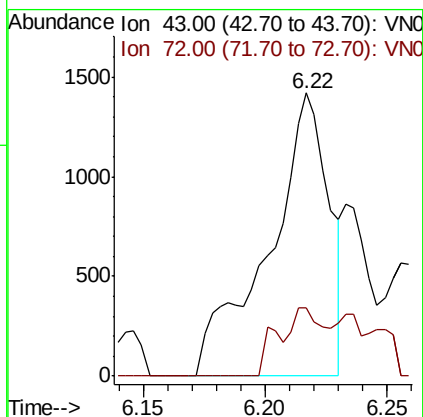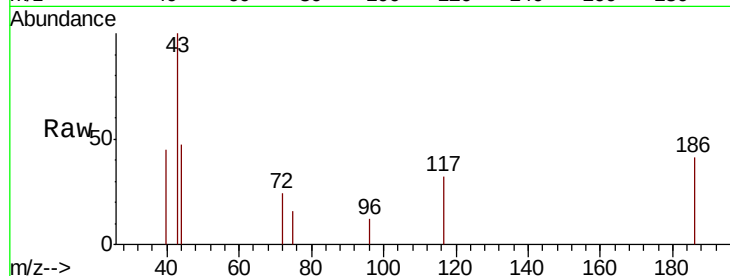

#31
Cyclohexane
Concen: 0.984 ug/l
RT: 7.05 min Scan# 1641
Delta R.T. -0.02 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18

Tgt Ion: 56 Resp: 19369
Ion Ratio Lower Upper
56 100
69 182.4 26.9 40.3#
84 162.5 71.9 107.9#



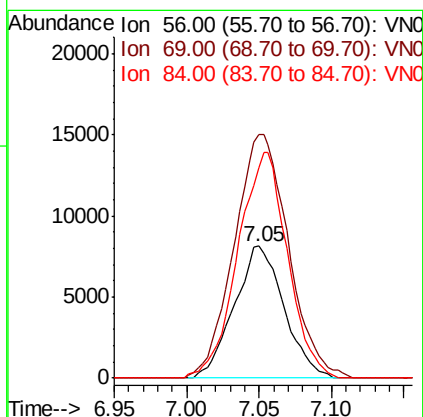



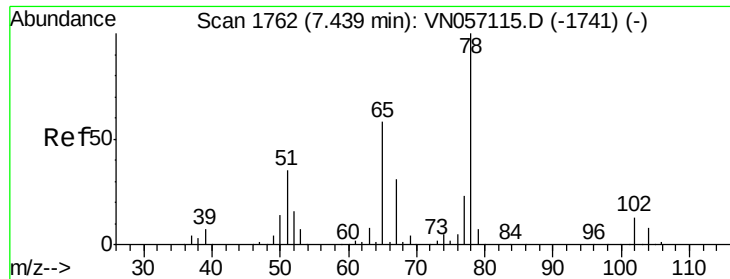

#33
 1,2-Dichloroethane-d4
 Concen: 45.781 ug/l
 RT: 7.44 min Scan# 1762
 Delta R.T. -0.00 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18




Instrument :
 MSVOA_N
 ClientSampled :
 COMP-26


Tgt Ion: 65 Resp: 621135
 Ion Ratio Lower Upper
 65 100
 67 54.3 0.0 108.2

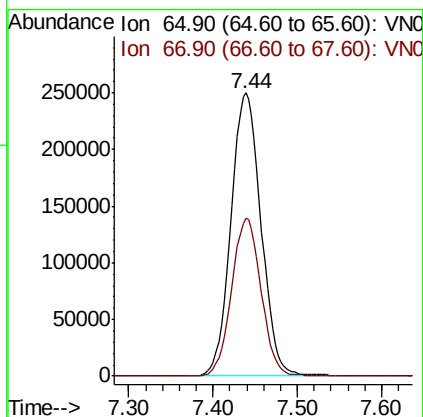

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.01 min Scan# 1939
 Delta R.T. -0.00 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18

Tgt Ion: 114 Resp: 1869981
 Ion Ratio Lower Upper
 114 100
 63 18.9 0.0 36.2
 88 14.9 0.0 30.0



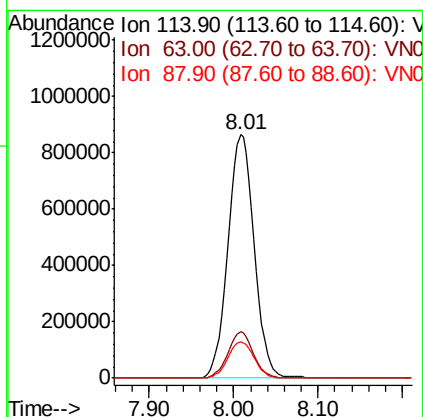



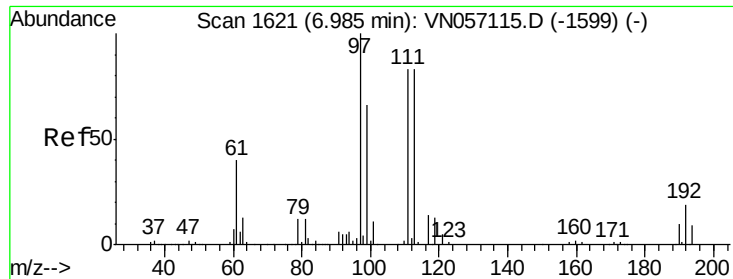

#35
 Dibromofluoromethane
 Concen: 47.867 ug/l
 RT: 6.99 min Scan# 1621
 Delta R.T. -0.00 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18




Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-26


Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.5	81.3	121.9
192	24.1	19.0	28.4

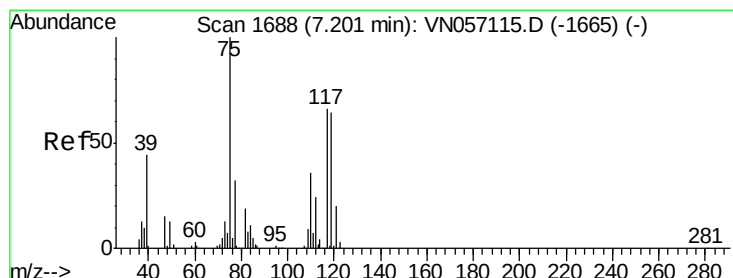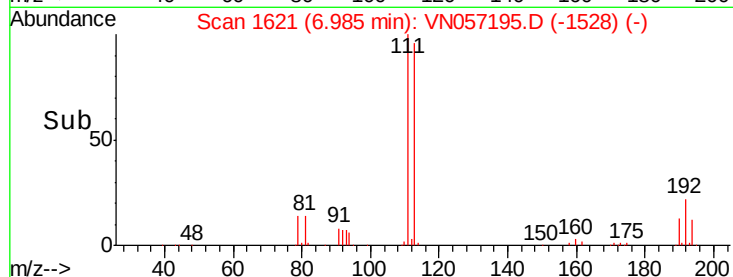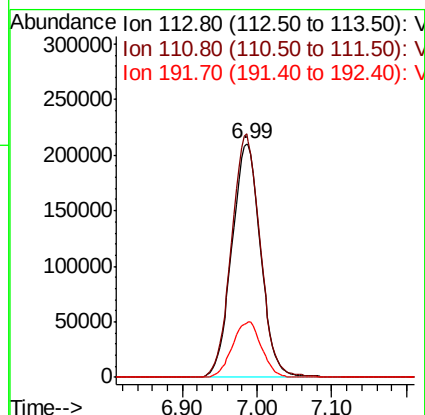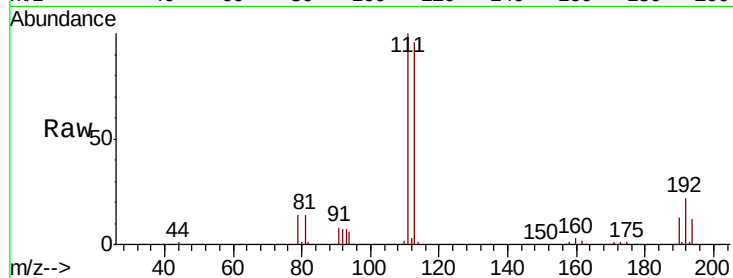

#36
 1,1-Dichloropropene
 Concen: 5.165 ug/l
 RT: 7.05 min Scan# 1641
 Delta R.T. -0.15 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.4	18.7	56.1#
77	0.0	25.0	37.4#


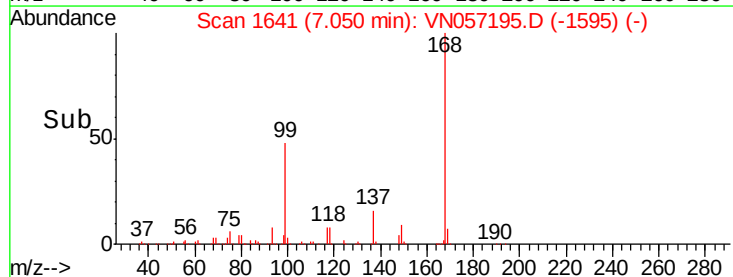
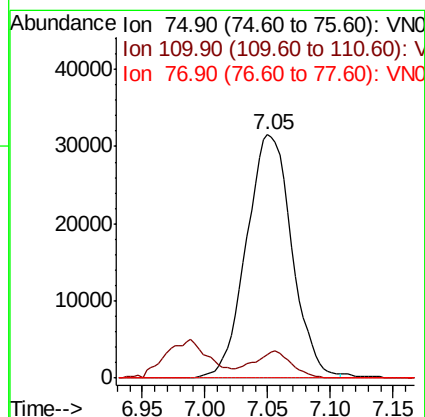
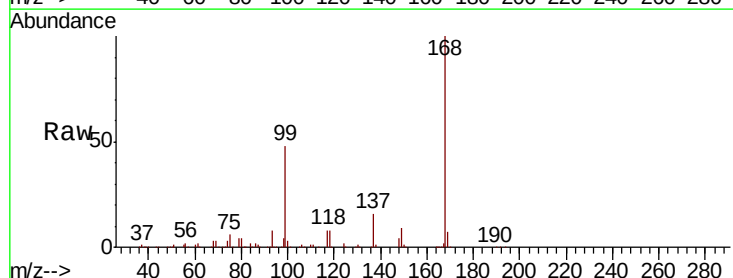


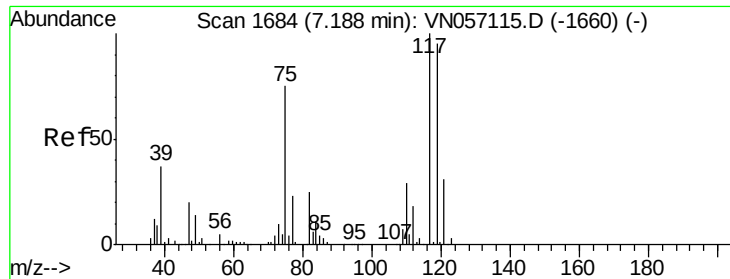

#38
Carbon Tetrachloride
Concen: 6.963 ug/l
RT: 7.05 min Scan# 1642
Delta R.T. -0.14 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18




Instrument :
MSVOA_N
ClientSampled :
COMP-26


Tgt Ion: 117 Resp: 111721
Ion Ratio Lower Upper
117 100
119 5.1 75.8 113.6#
121 0.0 24.4 36.6#

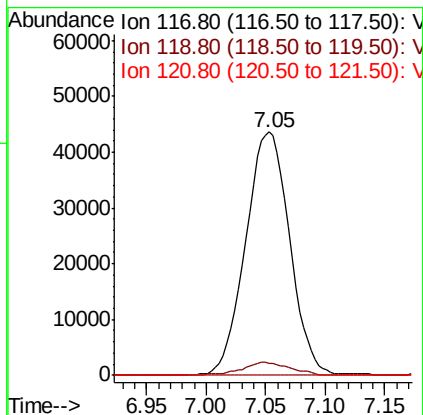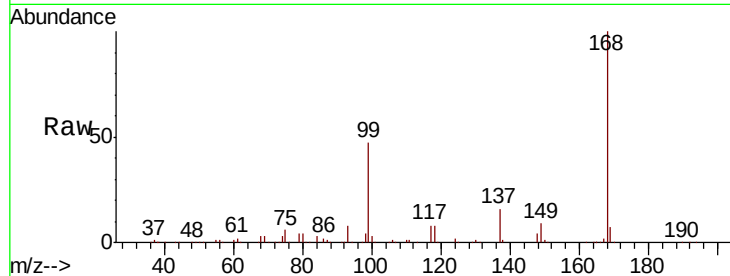

#43
Isopropyl Acetate
Concen: 6.836 ug/l
RT: 7.57 min Scan# 1802
Delta R.T. 0.01 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18

Tgt Ion: 43 Resp: 148055
Ion Ratio Lower Upper
43 100
61 7.4 24.2 36.2#
87 5.5 11.8 17.8#

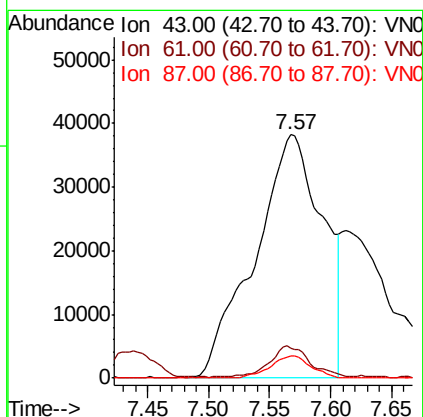







#48
Methyl methacrylate
Concen: 2.046 ug/l
RT: 8.62 min Scan# 2129
Delta R.T. -0.02 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18

Instrument :
MSVOA_N
ClientSampled :
COMP-26

Tgt Ion: 41 Resp: 20901
Ion Ratio Lower Upper
41 100
69 0.0 77.5 116.3#
39 0.0 39.8 59.6#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


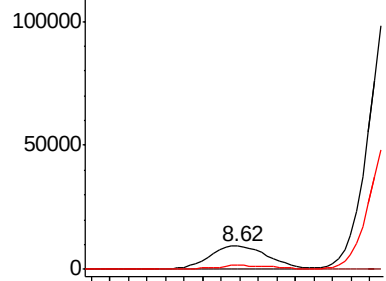



#49
1,4-Dioxane
Concen: 2.235 ug/l
RT: 8.71 min Scan# 2158
Delta R.T. 0.07 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18

Tgt Ion: 88 Resp: 465
Ion Ratio Lower Upper
88 100
43 630609.0 21.7 32.5#
58 2965.2 51.1 76.7#



Abundance Ion 88.00 (87.70 to 88.70): VN0
Ion 43.00 (42.70 to 43.70): VN0
Ion 58.00 (57.70 to 58.70): VN0

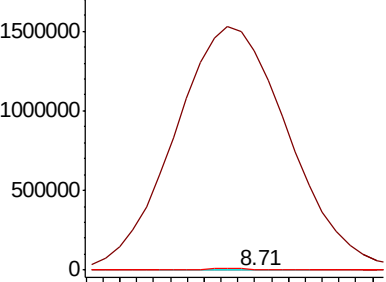



#50

Toluene-d8

Concen: 48.314 ug/l

RT: 9.56 min Scan# 2421

Delta R.T. -0.00 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampled :


COMP-26

Tgt Ion: 98 Resp: 2168978

Ion Ratio Lower Upper

98 100

100 64.7 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

9.56



1000000

500000

0

Time-->

9.50 9.60 9.70



#51

4-Methyl-2-Pentanone

Concen: 0.643 ug/l

RT: 9.45 min Scan# 2388

Delta R.T. 0.01 min

Lab File: VN057195.D


Acq: 11 Aug 2019 18:18

Tgt Ion: 43 Resp: 8100

Ion Ratio Lower Upper

43 100

58 45.1 33.2 49.8



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

12000

10000

8000

6000


4000


2000

0

Time-->

9.40 9.42 9.44 9.46






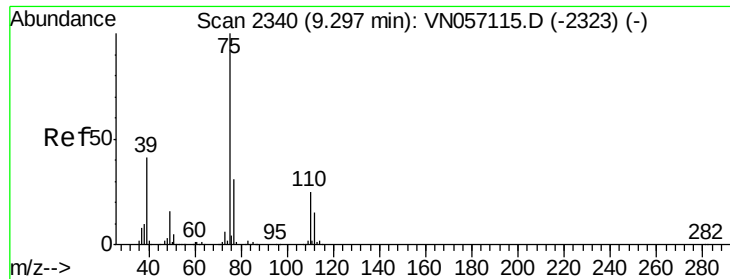


#54

cis-1,3-Dichloropropene
 Concen: 7.637 ug/l
 RT: 9.36 min Scan# 2361
 Delta R.T. 0.07 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18

Instrument :
 MSVOA_N
 ClientSampled :
 COMP-26




Tgt Ion	Ratio	Lower	Upper
75	100		
77	0.5	25.1	37.7#
39	25.6	32.5	48.7#

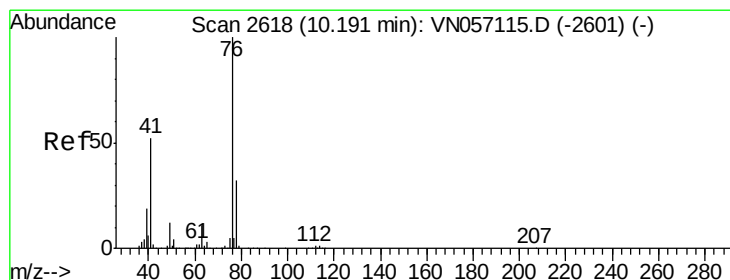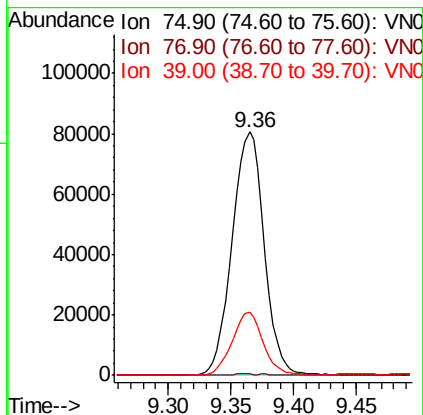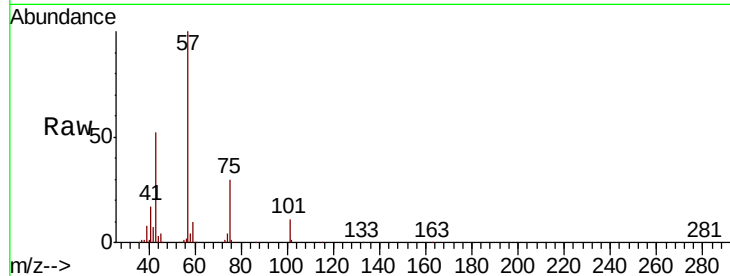


#57

1,3-Dichloropropane
 Concen: 1.362 ug/l
 RT: 10.25 min Scan# 2637
 Delta R.T. 0.06 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18

Tgt Ion	Ratio	Lower	Upper
76	100		
78	0.0	25.9	38.9#


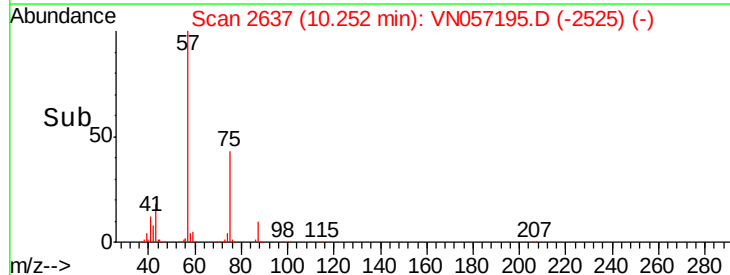
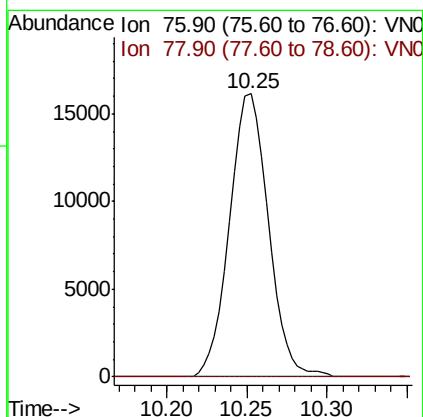





#59
2-Hexanone
Concen: 38.833 ug/l
RT: 10.25 min Scan# 2637
Delta R.T. 0.02 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18




Instrument :
MSVOA_N
ClientSampleId :
COMP-26


Tgt Ion: 43 Resp: 331292
Ion Ratio Lower Upper
43 100
58 20.5 29.2 87.6#

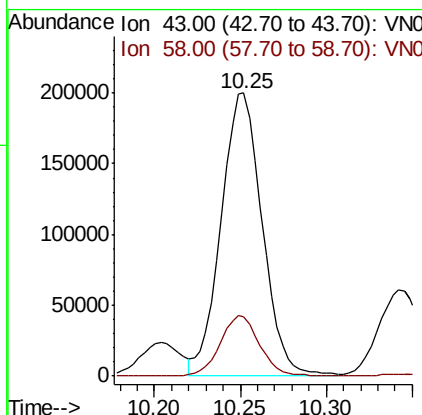

#62
4-Bromofluorobenzene
Concen: 39.700 ug/l
RT: 11.92 min Scan# 3156
Delta R.T. 0.00 min
Lab File: VN057195.D
Acq: 11 Aug 2019 18:18

Tgt Ion: 95 Resp: 574274
Ion Ratio Lower Upper
95 100
174 95.2 0.0 185.0
176 92.7 0.0 181.2

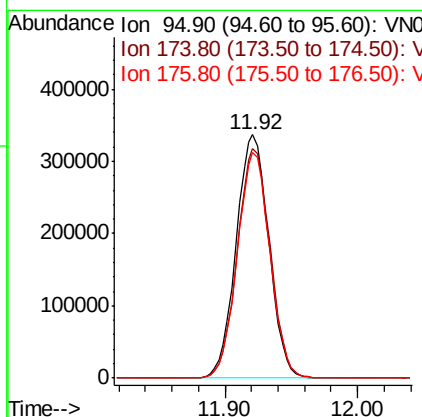


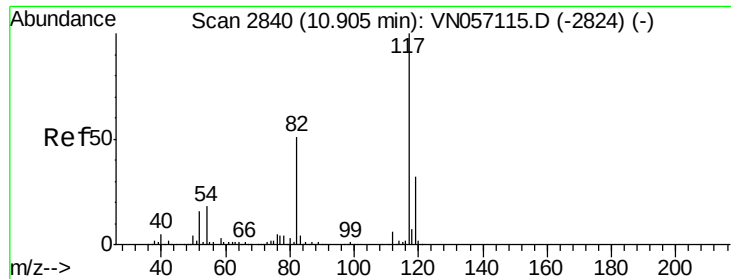




#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.91 min Scan# 2841
 Delta R.T. 0.00 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18

Instrument :
 MSVOA_N
 ClientSampled :
 COMP-26

Tgt Ion:117 Resp: 1537787
 Ion Ratio Lower Upper
 117 100
 82 52.0 40.8 61.2
 119 32.1 25.7 38.5

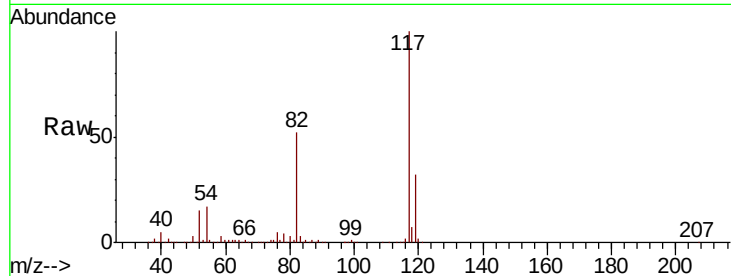


Abundance Ion 116.90 (116.60 to 117.60): V
 1200000 Ion 82.00 (81.70 to 82.70): VN
 1000000 Ion 118.90 (118.60 to 119.60): V

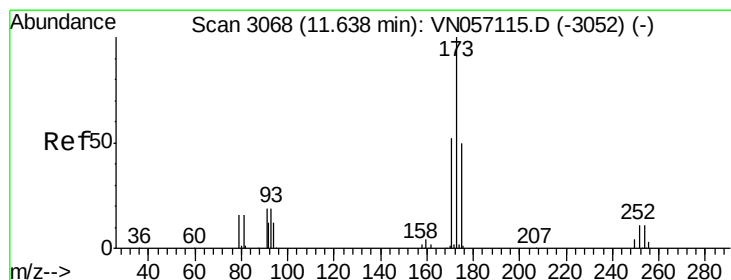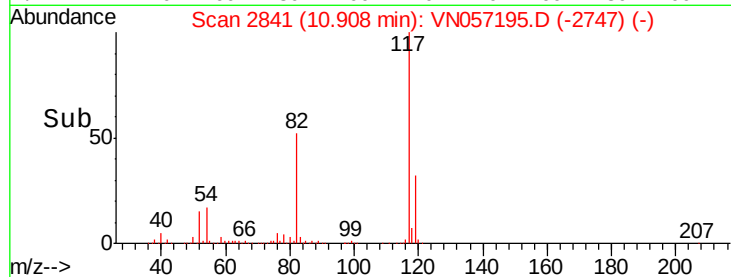
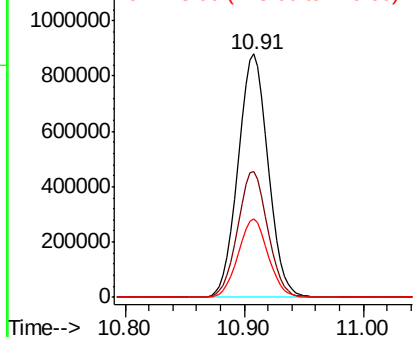



#71
 Bromoform
 Concen: 0.307 ug/l
 RT: 11.92 min Scan# 3155
 Delta R.T. 0.28 min
 Lab File: VN057195.D
 Acq: 11 Aug 2019 18:18

Tgt Ion:173 Resp: 2603
 Ion Ratio Lower Upper
 173 100
 175 990.4 24.6 73.8#
 254 0.0 0.1 0.1#

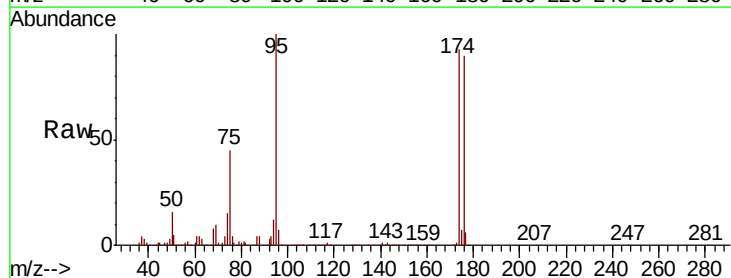

Abundance Ion 172.70 (172.40 to 173.40): V
 30000 Ion 174.70 (174.40 to 175.40): V
 25000 Ion 254.40 (254.10 to 255.10): V

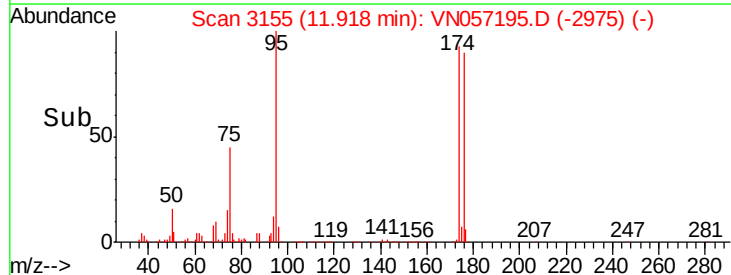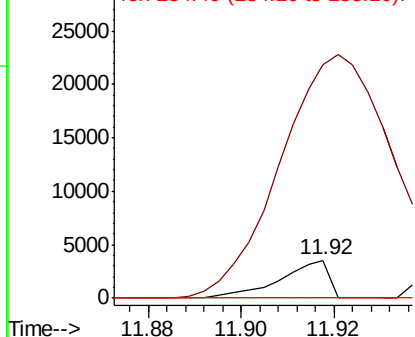



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.88 min Scan# 3453

Delta R.T. 0.00 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampled :

COMP-26


Tgt Ion:152 Resp: 402845

Ion Ratio Lower Upper

152 100

115 54.3 27.5 82.5




150 154.8 0.0 341.6



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

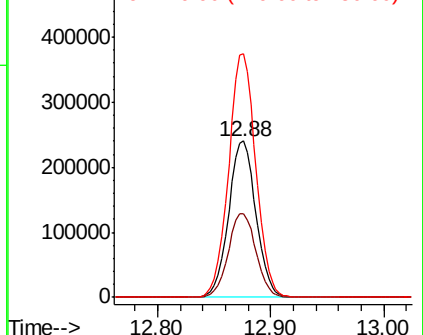

#73

Isopropylbenzene

Concen: Below Cal

RT: 11.77 min Scan# 3108

Delta R.T. 0.00 min

Lab File: VN057195.D


Acq: 11 Aug 2019 18:18

Tgt Ion:105 Resp: 188

Ion Ratio Lower Upper



105 100


120 0.0 13.7 41.0#



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

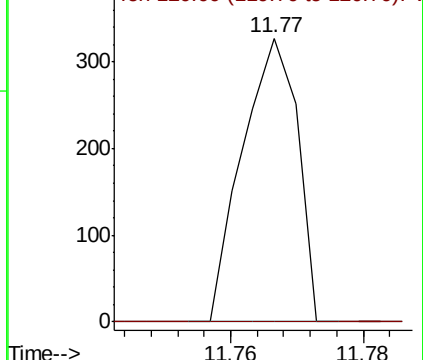



#74

N-ethyl acetate

Concen: 2.685 ug/l

RT: 11.39 min Scan# 2991

Delta R.T. -0.19 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampleId :

COMP-26

Tgt Ion: 43 Resp: 27408





Ion Ratio Lower Upper

43 100

70 1.4 36.8 55.2#

55 4.4 20.6 31.0#

61 12.4 21.0 31.4#

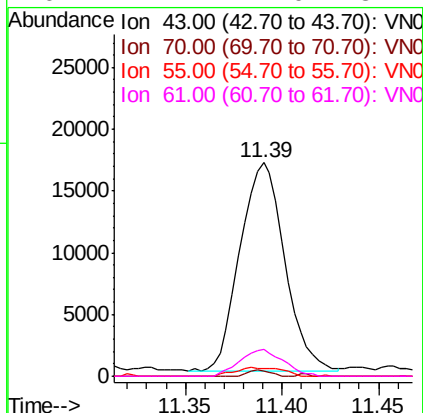

#76

1,2,3-Trichloropropane

Concen: 31.816 ug/l

RT: 11.92 min Scan# 3156

Delta R.T. -0.15 min

Lab File: VN057195.D




Acq: 11 Aug 2019 18:18


Tgt Ion: 75 Resp: 258639

Ion Ratio Lower Upper

75 100

77 1.2 0.0 0.0#

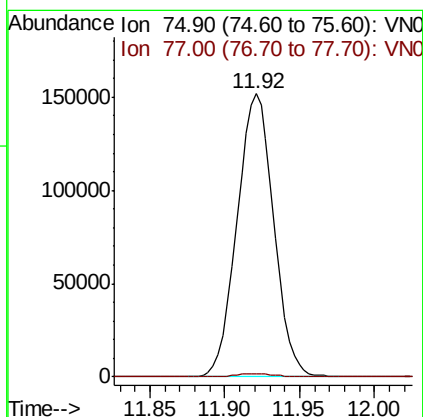



#79

2-Chlorotoluene

Concen: Below Cal

RT: 12.31 min Scan# 3276

Delta R.T. 0.11 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampled :


COMP-26

Tgt Ion: 91 Resp: 122

Ion Ratio Lower Upper




91 100

126 51.6 18.1 54.3

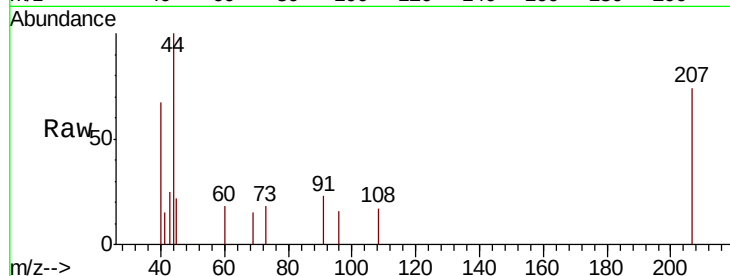

Abundance Ion 91.00 (90.70 to 91.70): VN0

Ion 125.90 (125.60 to 126.60): VN

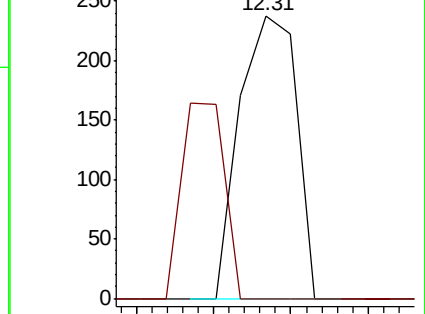

#81

trans-1,4-Dichloro-2-butene

Concen: 94.401 ug/l

RT: 11.92 min Scan# 3156

Delta R.T. 0.10 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18


Tgt Ion: 75 Resp: 258639

Ion Ratio Lower Upper

75 100

53 0.0 70.6 106.0#



89 0.0 36.4 54.6#




Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

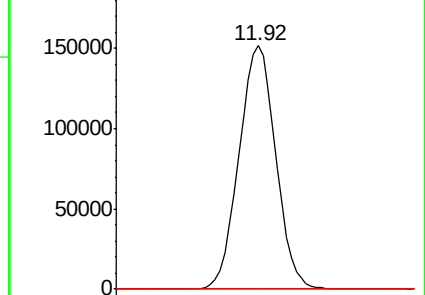



#83

tert-Butylbenzene

Concen: Below Cal

RT: 12.53 min Scan# 3345

Delta R.T. 0.01 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampled :

COMP-26


Tgt Ion:119 Resp: 76

Ion Ratio Lower Upper

119 100

91 0.0 31.4 94.2#


134 0.0 13.2 39.6#





Abundance Ion 119.00 (118.70 to 119.70): V

Ion 91.00 (90.70 to 91.70): V

Ion 134.00 (133.70 to 134.70): V

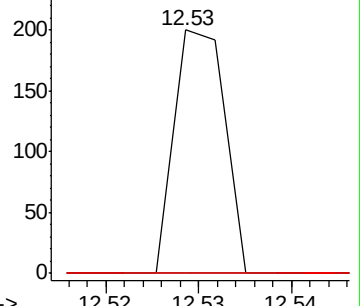

Time-->



#93

1,2,4-Trichlorobenzene

Concen: 5.980 ug/l

RT: 14.45 min Scan# 3942

Delta R.T. 0.00 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18


Tgt Ion:180 Resp: 327

Ion Ratio Lower Upper

180 100

182 56.9 47.5 142.6


145 0.0 14.1 42.2#




Abundance Ion 179.80 (179.50 to 180.50): V


Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V

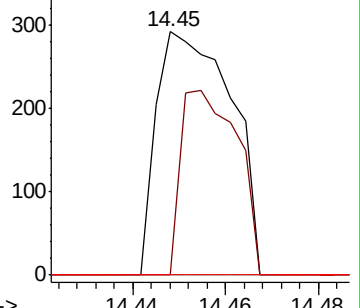

Time-->





#95

Naphthalene

Concen: 2.833 ug/l

RT: 14.68 min Scan# 4014

Delta R.T. 0.01 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18

Instrument :

MSVOA_N

ClientSampled :

COMP-26


Tgt Ion:128 Resp: 318

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.8 13.2#




Abundance Ion 128.00 (127.70 to 128.70): V


Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

14.68



Time-->



#96

1,2,3-Trichlorobenzene

Concen: 5.752 ug/l

RT: 14.83 min Scan# 4061

Delta R.T. -0.00 min

Lab File: VN057195.D

Acq: 11 Aug 2019 18:18


Tgt Ion:180 Resp: 210

Ion Ratio Lower Upper

180 100

182 0.0 48.3 144.8#

145 15.2 14.9 44.5




Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

14.83



Time-->