


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081119\
 Data File : VN057175.D
 Acq On : 11 Aug 2019 9:32
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
 Title : SW846 8260
 Last Update : Thu Aug 08 06:49:25 2019

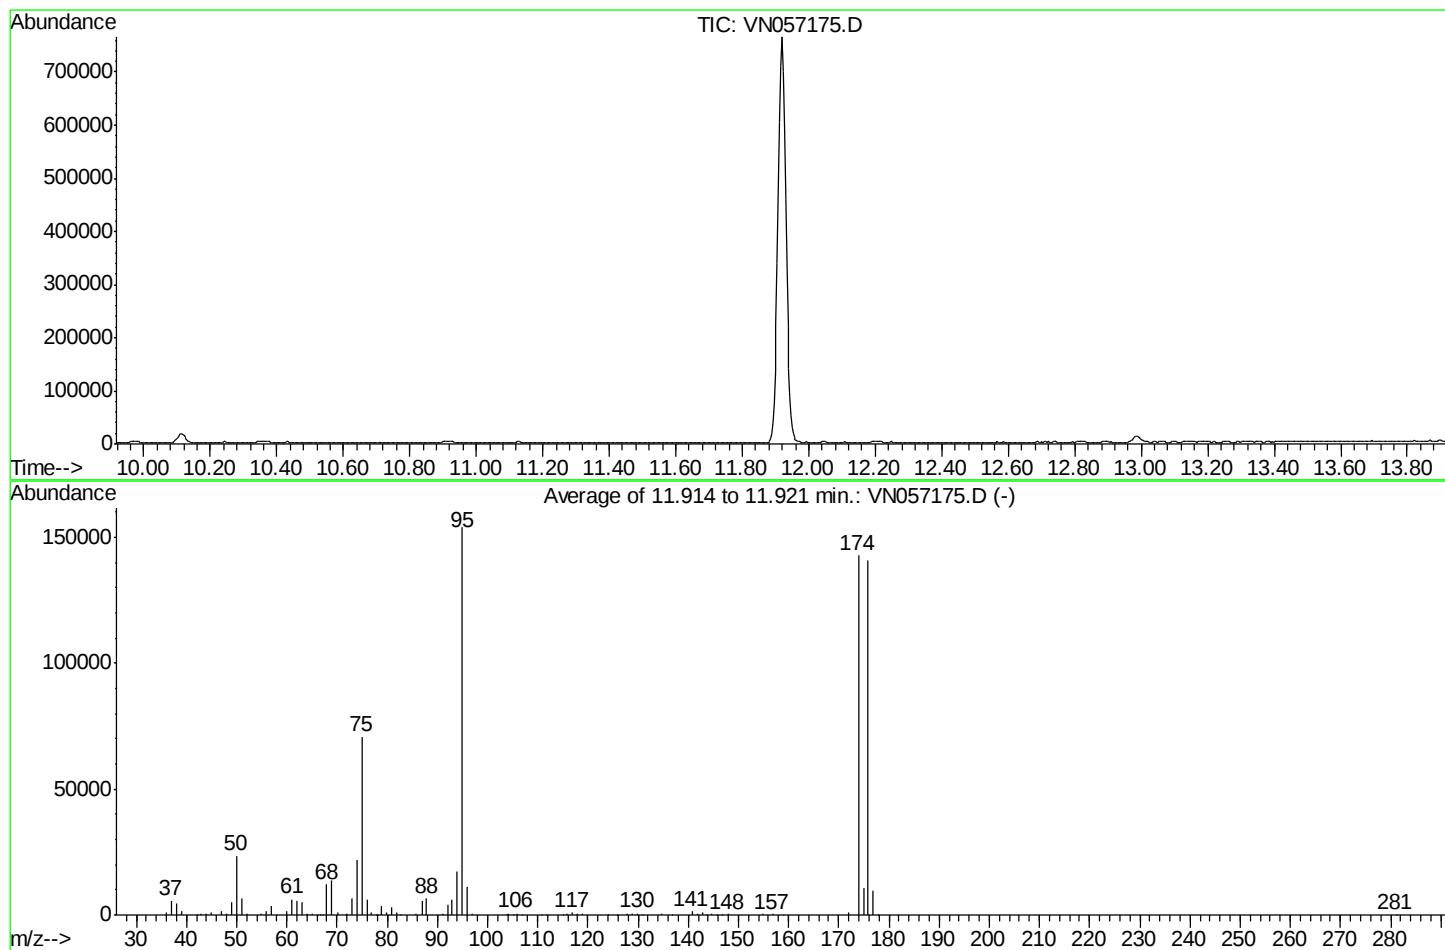

AutoFind: Scans 3154, 3155, 3156; Background Corrected with Scan 3139

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	23538	PASS
75	95	30	60	46.0	70784	PASS
95	95	100	100	100.0	153962	PASS
96	95	5	9	7.2	11148	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.8	142826	PASS
175	174	5	9	7.3	10460	PASS
176	174	95	101	98.7	140906	PASS
177	176	5	9	7.0	9855	PASS