

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081121\
 Data File : VN068072.D
 Acq On : 11 Aug 2021 14:55
 Operator : JC/MD
 Sample : PB138317ZHE#02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 12 07:12:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 29 15:02:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.085	168	295471	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	580133	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	605531	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	191484	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	232045	55.47	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 110.94%			
35) Dibromofluoromethane	8.024	113	175691	51.97	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 103.94%			
50) Toluene-d8	10.443	98	755973	48.57	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 97.14%			
62) 4-Bromofluorobenzene	12.733	95	241978	43.13	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 86.26%			
Target Compounds						Qvalue
16) Acetone	4.296	43	34067	22.32	ug/l	99
18) Methyl Acetate	4.859	43	2819	0.67	ug/l #	67
20) Methylene Chloride	5.092	84	17629	4.74	ug/l	86
23) Vinyl Acetate	6.608	43	129	8.81	ug/l #	75
25) 2-Butanone	7.348	43	2987	1.35	ug/l #	84
29) Tetrahydrofuran	7.705	42	2205	1.56	ug/l #	83
31) Cyclohexane	8.085	56	7943	1.29	ug/l #	47
36) 1,1-Dichloropropene	8.088	75	25869	4.82	ug/l #	45
38) Carbon Tetrachloride	8.088	117	32258	6.11	ug/l #	17
41) Methacrylonitrile	7.699	41	658	0.27	ug/l #	35
43) Isopropyl Acetate	8.566	43	42253	5.02	ug/l	93
45) 1,2-Dichloropropane	9.622	63	2833	0.72	ug/l #	44
48) Methyl methacrylate	9.553	41	9074	4.37	ug/l #	12
49) 1,4-Dioxane	9.625	88	272	4.06	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	9265	14.00	ug/l	92
53) t-1,3-Dichloropropene	10.647	75	51	2.84	ug/l #	1
54) cis-1,3-Dichloropropene	10.247	75	69089	11.52	ug/l #	60
56) Ethyl methacrylate	10.875	69	945	3.22	ug/l #	1
57) 1,3-Dichloropropane	11.095	76	46669	7.15	ug/l #	43
59) 2-Hexanone	11.095	43	654148	154.99	ug/l #	55
60) Dibromochloromethane	11.489	129	448	3.39	ug/l #	11
68) m/p-Xylenes	11.953	106	136	4.08	ug/l #	42
70) Styrene	12.299	104	307	2.65	ug/l #	42
71) Bromoform	12.717	173	213	4.08	ug/l #	29
74) N-amyl acetate	12.374	43	1156	0.21	ug/l #	47
76) 1,2,3-Trichloropropane	12.733	75	131532	34.20	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.061	105	10874	0.86	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.733	75	131532	91.66	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.265	180	339	2.58	ug/l #	48
95) Naphthalene	15.498	128	732	3.21	ug/l #	85
96) 1,2,3-Trichlorobenzene	15.689	180	150	2.42	ug/l #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081121\
Data File : VN068072.D
Acq On : 11 Aug 2021 14:55
Operator : JC/MD
Sample : PB138317ZHE#02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 12 07:12:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 29 15:02:35 2021
Response via : Initial Calibration




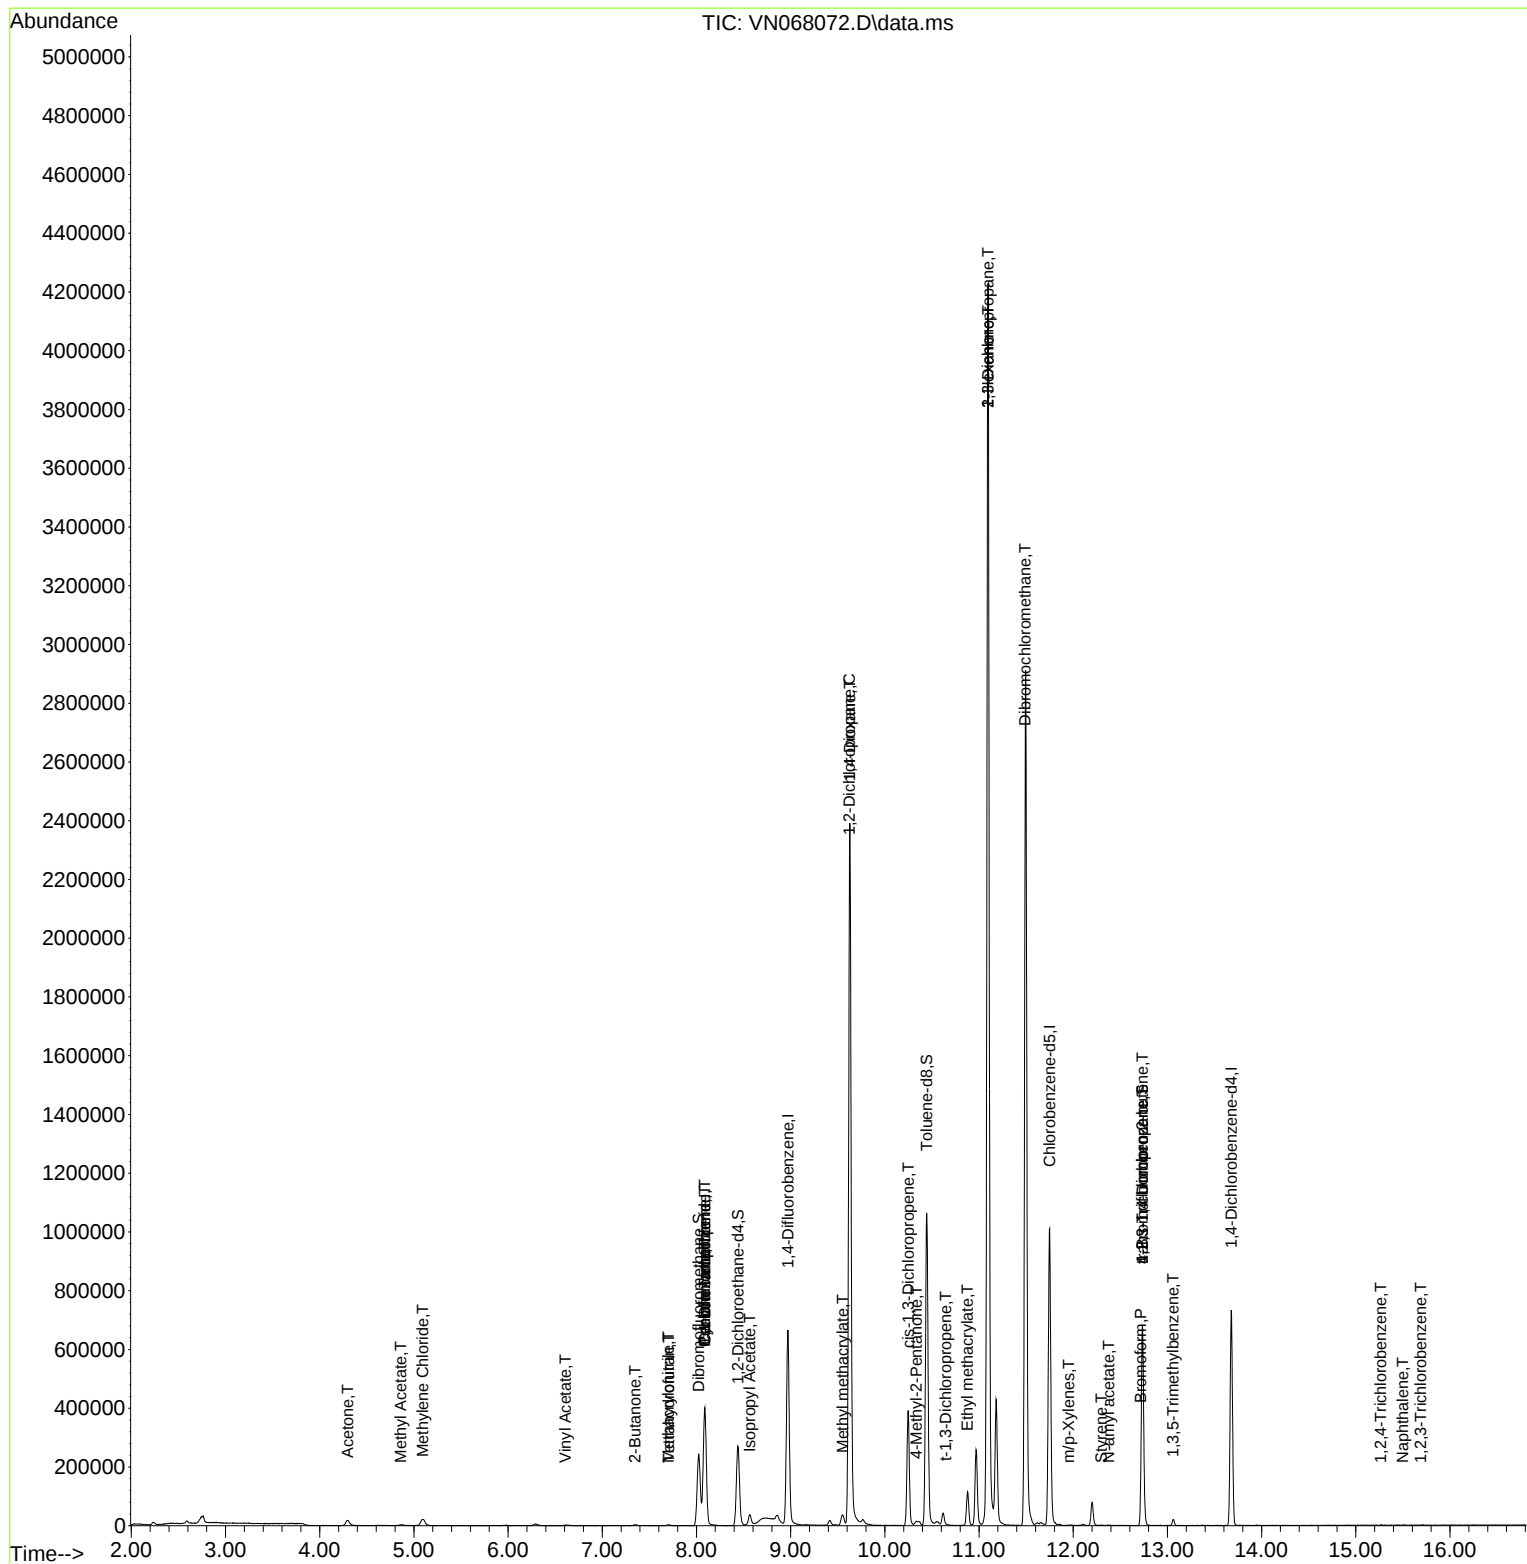




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.001 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 295471
Ion Ratio Lower Upper
168 100
99 65.6 62.9 94.3

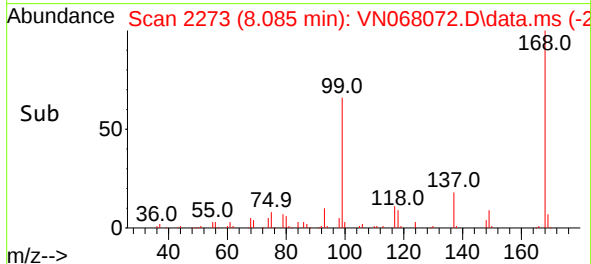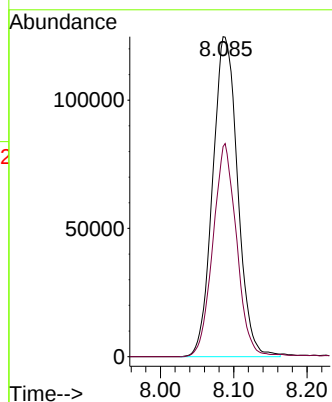

#16
Acetone
Concen: 22.32 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 43 Resp: 34067
Ion Ratio Lower Upper
43 100
58 27.2 21.2 31.8




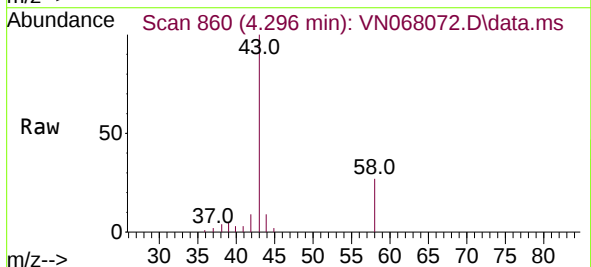


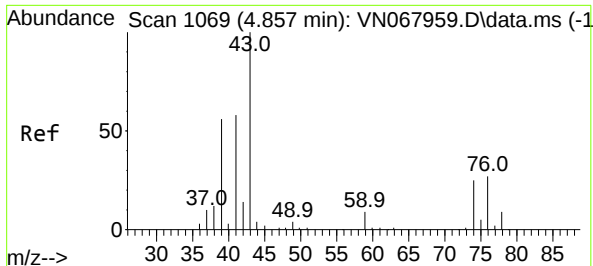

#18
Methyl Acetate
Concen: 0.67 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.002 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2819
Ion Ratio Lower Upper
43 100
74 37.2 17.4 26.0#

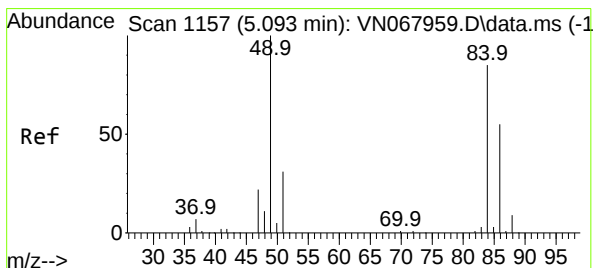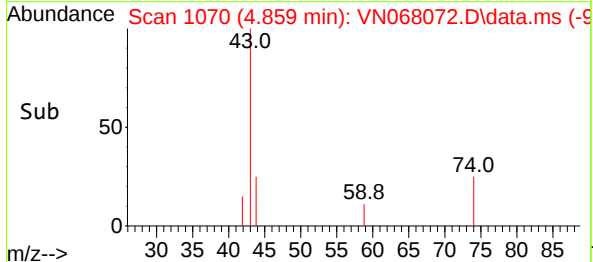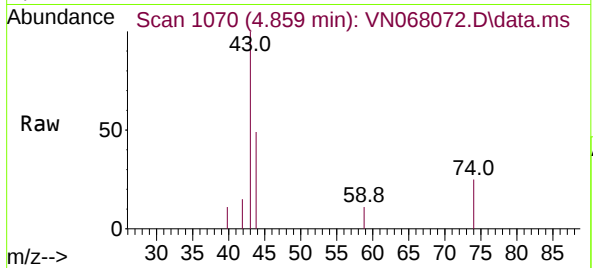

#20
Methylene Chloride
Concen: 4.74 ug/l
RT: 5.092 min Scan# 1157
Delta R.T. -0.001 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 84 Resp: 17629
Ion Ratio Lower Upper
84 100
49 112.8 110.9 166.3
51 36.3 32.6 49.0
86 63.8 51.6 77.4


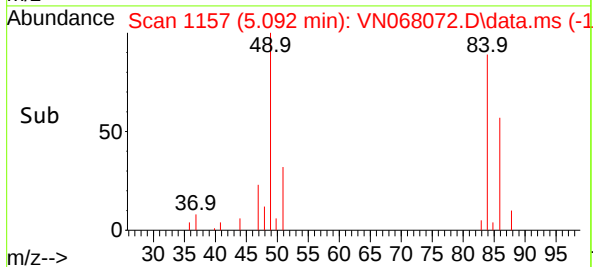

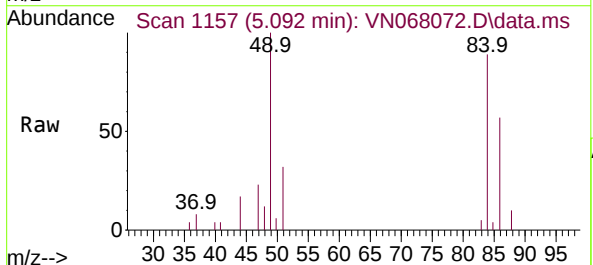


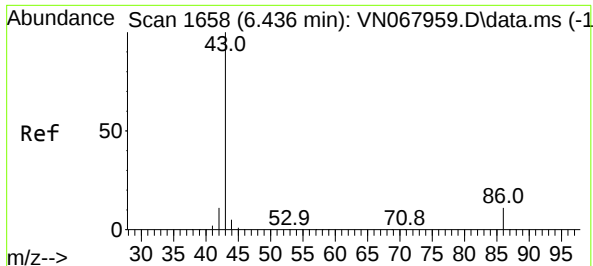

#23
 Vinyl Acetate
 Concen: 8.81 ug/l
 RT: 6.608 min Scan# 1722
 Delta R.T. 0.172 min
 Lab File: VN068072.D
 Acq: 11 Aug 2021 14:55




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 43 Resp: 129
 Ion Ratio Lower Upper
 43 100
 86 0.0 7.3 10.9#

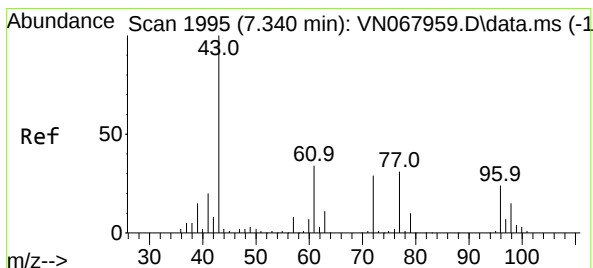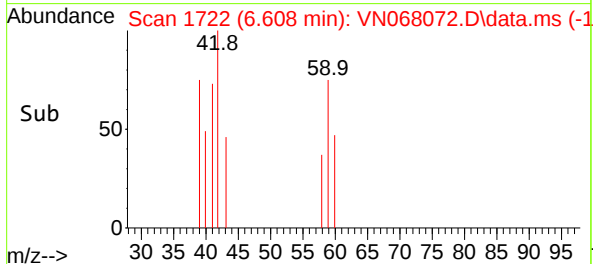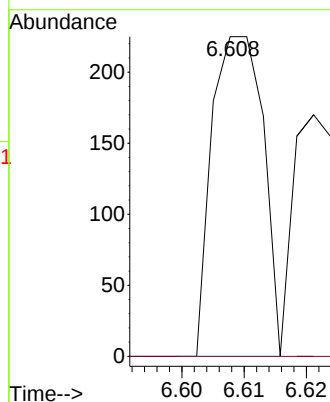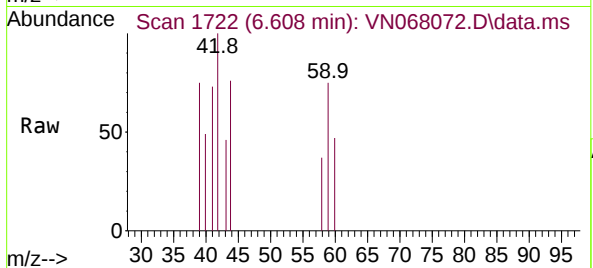

#25
 2-Butanone
 Concen: 1.35 ug/l
 RT: 7.348 min Scan# 1998
 Delta R.T. 0.008 min
 Lab File: VN068072.D
 Acq: 11 Aug 2021 14:55

Tgt Ion: 43 Resp: 2987
 Ion Ratio Lower Upper
 43 100
 72 32.8 19.7 29.5#

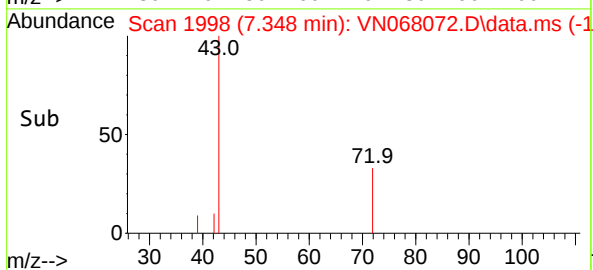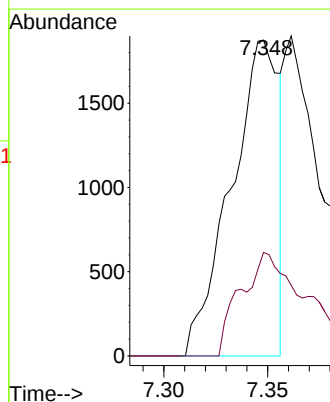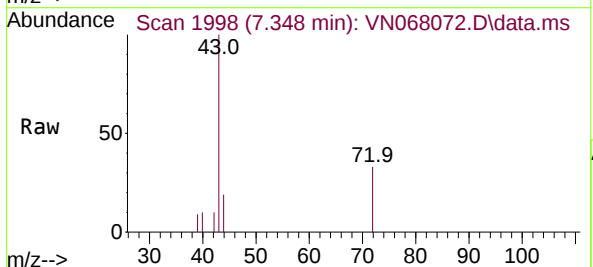

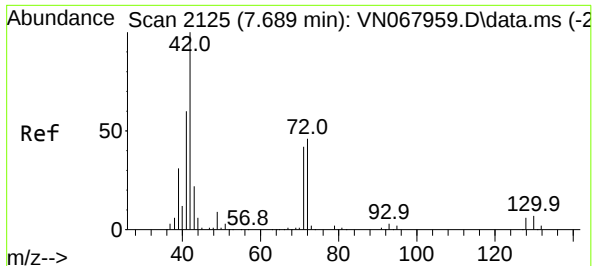

#29

Tetrahydrofuran

Concen: 1.56 ug/l

RT: 7.705 min Scan# 2131





Delta R.T. 0.016 min

Lab File: VN068072.D

Acq: 11 Aug 2021 14:55

Tgt Ion:	42	Resp:	2205
Ion	Ratio	Lower	Upper
42	100		
72	44.0	32.8	49.2
71	20.5	31.2	46.8

Instrument :
MSVOA_N
ClientSampleId :

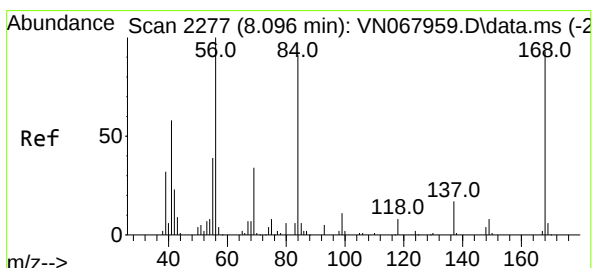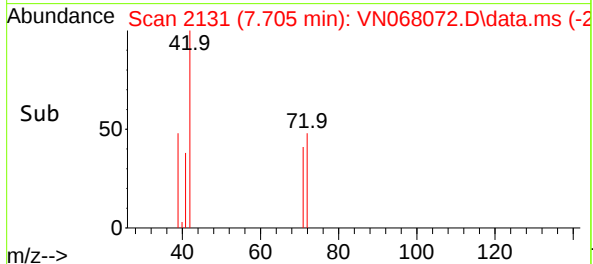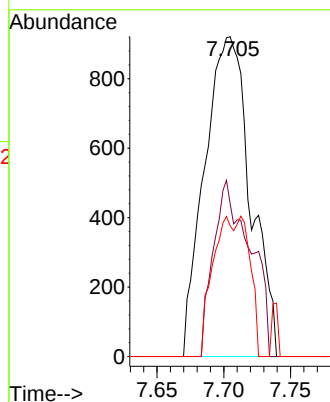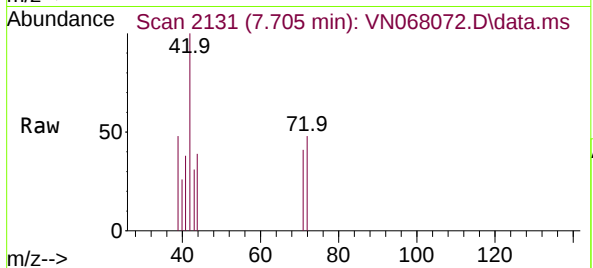

#31

Cyclohexane

Concen: 1.29 ug/l




RT: 8.085 min Scan# 2273


Delta R.T. -0.011 min

Lab File: VN068072.D

Acq: 11 Aug 2021 14:55

Tgt Ion:	56	Resp:	7943
Ion	Ratio	Lower	Upper
56	100		
69	121.6	27.3	40.9
84	91.2	64.9	97.3

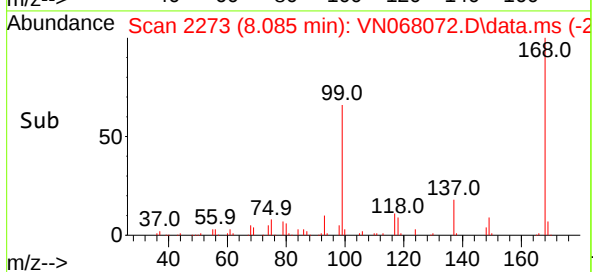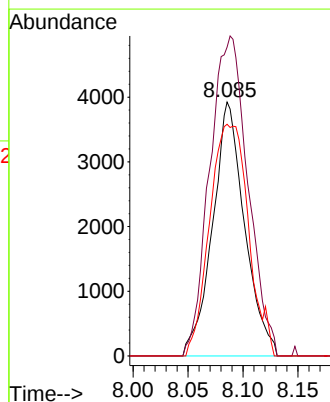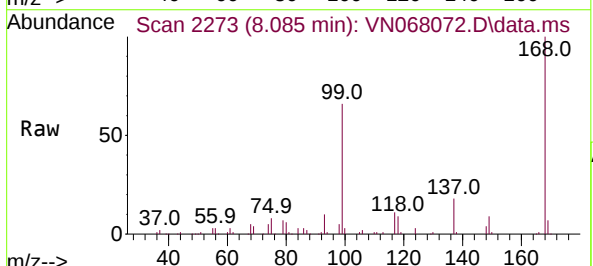



#33

1,2-Dichloroethane-d4

Concen: 55.47 ug/l

RT: 8.440 min Scan# 2405

Delta R.T. 0.003 min

Lab File: VN068072.D

Acq: 11 Aug 2021 14:55

Tgt Ion: 65 Resp: 232045





Ion Ratio Lower Upper

Ion	Ratio	Lower	Upper
65	100		
67	51.5	0.0	98.6

Instrument :

MSVOA_N

ClientSampled :

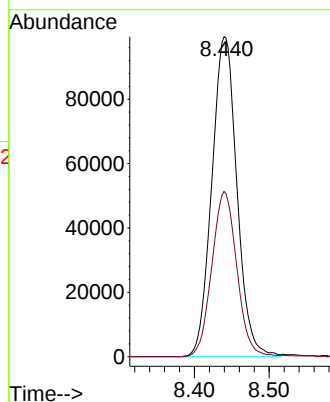

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. 0.003 min




Lab File: VN068072.D


Acq: 11 Aug 2021 14:55

Tgt Ion: 114 Resp: 580133

Ion Ratio Lower Upper

Ion	Ratio	Lower	Upper
114	100		
63	20.1	0.0	49.0
88	15.3	0.0	36.6



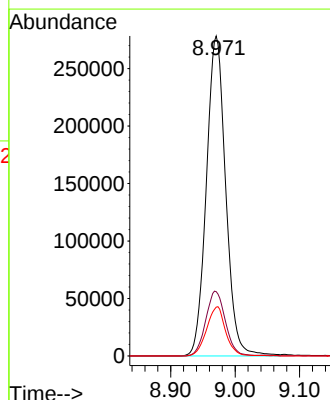





#35
Dibromofluoromethane
Concen: 51.97 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:113 Resp: 175691
Ion Ratio Lower Upper
113 100
111 104.8 83.8 125.8
192 15.8 13.4 20.0

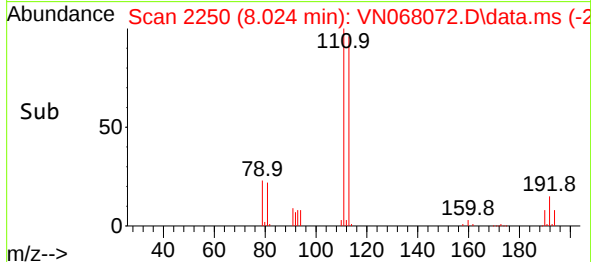

#36
1,1-Dichloropropene
Concen: 4.82 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55


Tgt Ion: 75 Resp: 25869
Ion Ratio Lower Upper
75 100
110 1.4 15.7 47.0#
77 0.0 24.6 37.0#

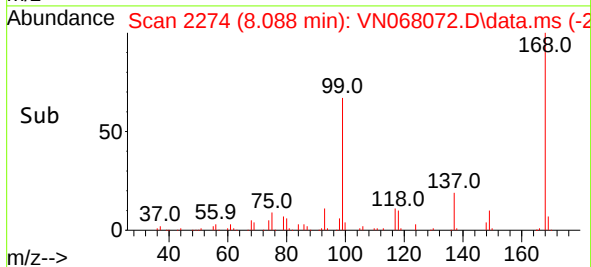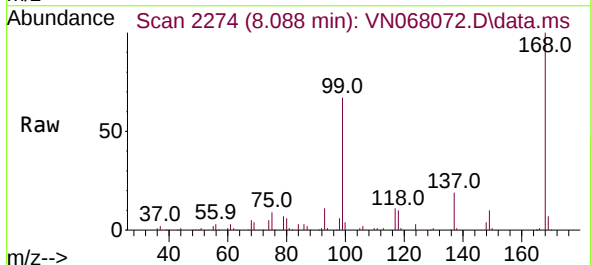



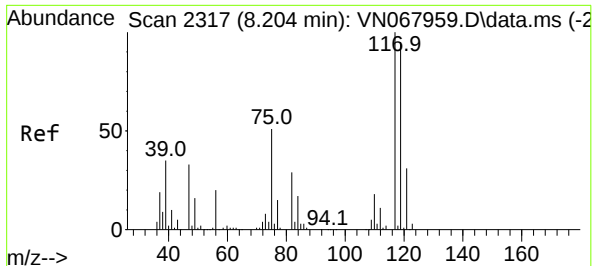


#38
Carbon Tetrachloride
Concen: 6.11 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.116 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Instrument :
MSVOA_N
ClientSampled :



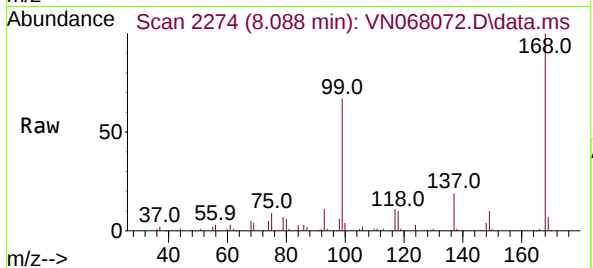



Tgt Ion: 117 Resp: 32258
Ion Ratio Lower Upper
117 100
119 5.2 75.4 113.2#
121 0.0 23.5 35.3#

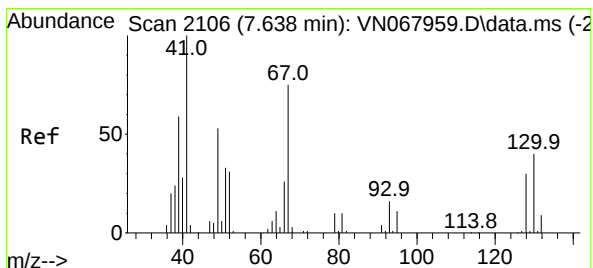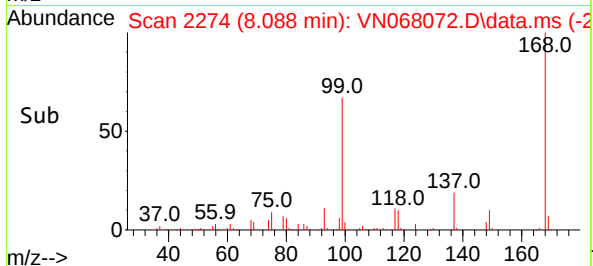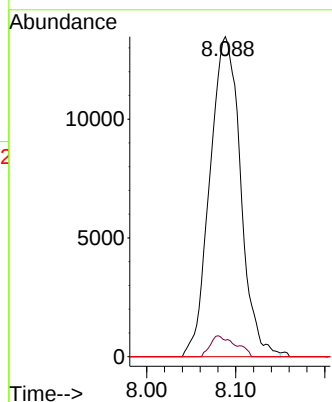

#41
Methacrylonitrile
Concen: 0.27 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.061 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 41 Resp: 658
Ion Ratio Lower Upper
41 100
39 27.8 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#


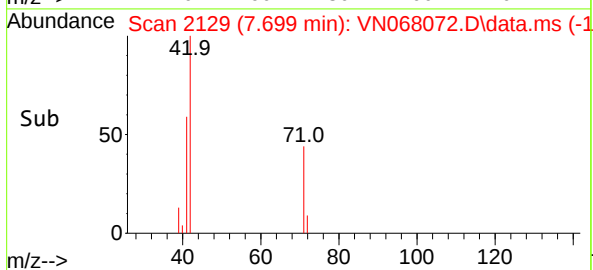

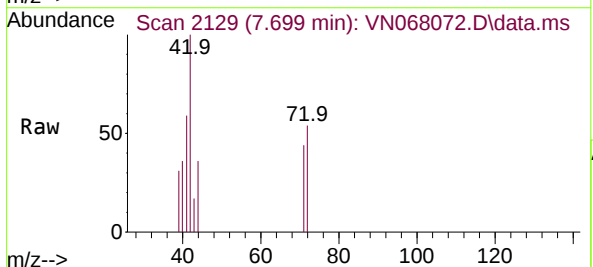




#43
Isopropyl Acetate
Concen: 5.02 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 42253
Ion Ratio Lower Upper
43 100
61 19.1 19.0 28.4
87 13.0 9.5 14.3

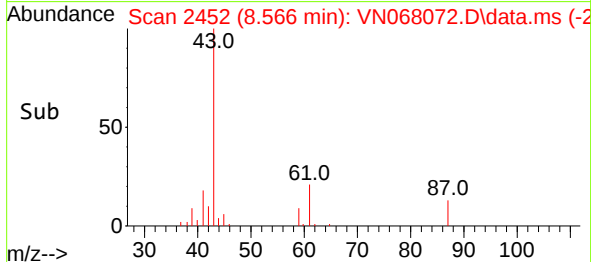

#45
1,2-Dichloropropane
Concen: 0.72 ug/l
RT: 9.622 min Scan# 2846
Delta R.T. 0.131 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 63 Resp: 2833
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#


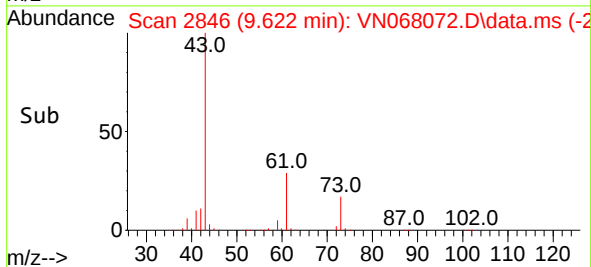

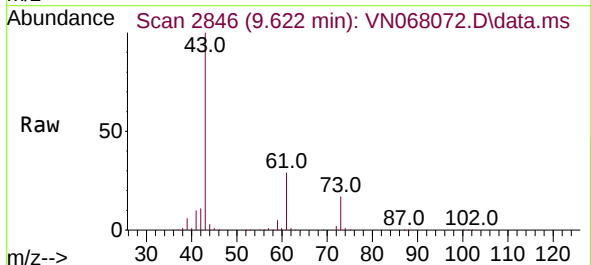




#48
Methyl methacrylate
Concen: 4.37 ug/l
RT: 9.553 min Scan# 2820
Delta R.T. -0.010 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 41 Resp: 9074
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

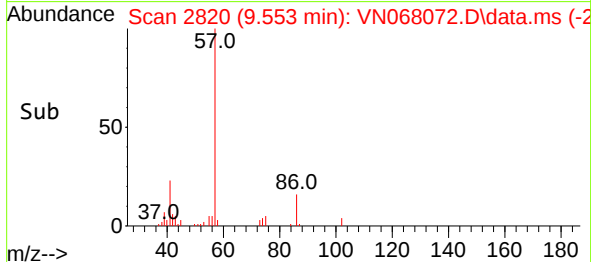

#49
1,4-Dioxane
Concen: 4.06 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.053 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 88 Resp: 272
Ion Ratio Lower Upper
88 100
43 852022.1 28.8 43.2#
58 4031.3 60.4 90.6#


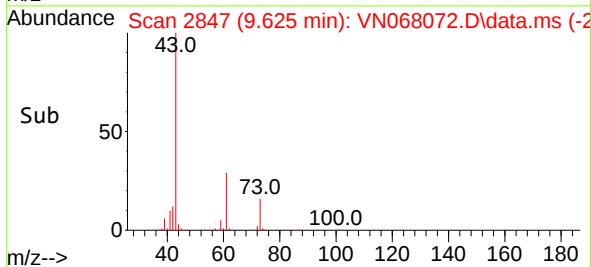

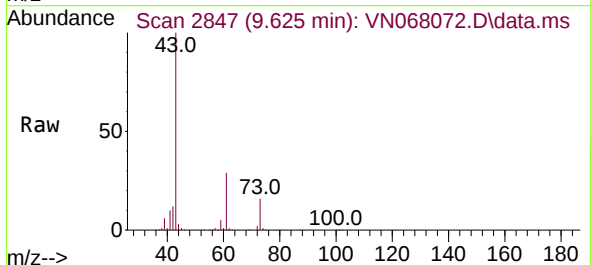




#50
Toluene-d8
Concen: 48.57 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 755973
Ion Ratio Lower Upper
98 100
100 64.2 51.7 77.5

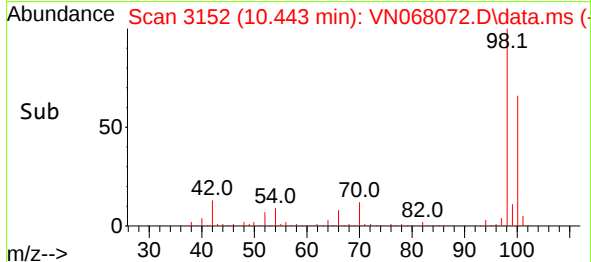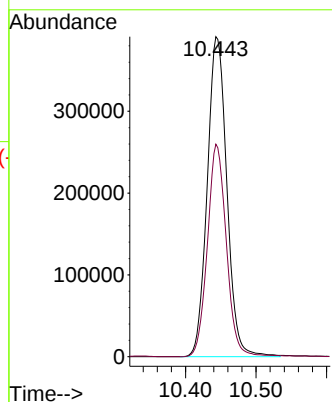

#51
4-Methyl-2-Pentanone
Concen: 14.00 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 43 Resp: 9265
Ion Ratio Lower Upper
43 100
58 40.7 28.6 43.0


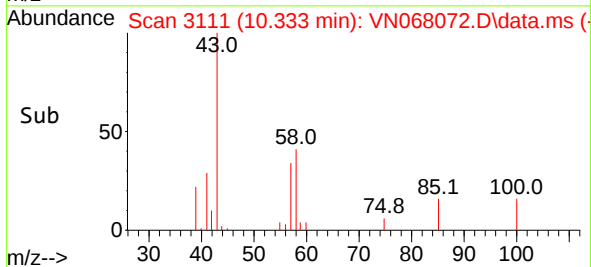
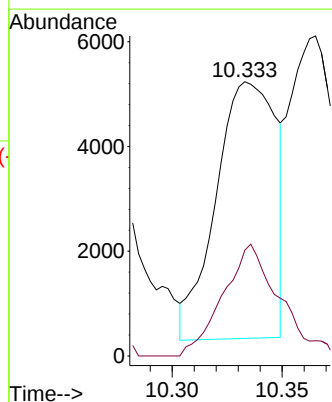
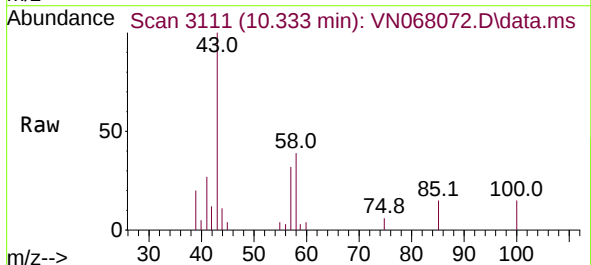




#53
t-1,3-Dichloropropene
Concen: 2.84 ug/l
RT: 10.647 min Scan# 3228
Delta R.T. -0.075 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 51
Ion Ratio Lower Upper
75 100
77 201.2 25.1 37.7#

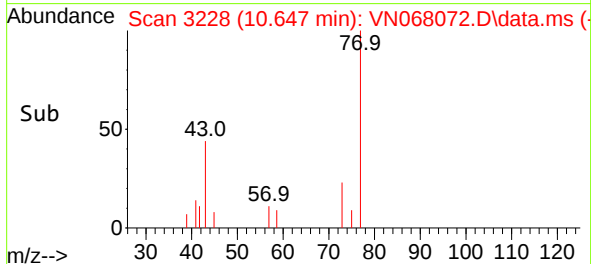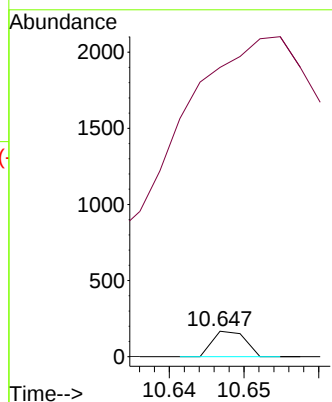

#54
cis-1,3-Dichloropropene
Concen: 11.52 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 75 Resp: 69089
Ion Ratio Lower Upper
75 100
77 0.7 24.6 37.0#
39 37.4 50.7 76.1#




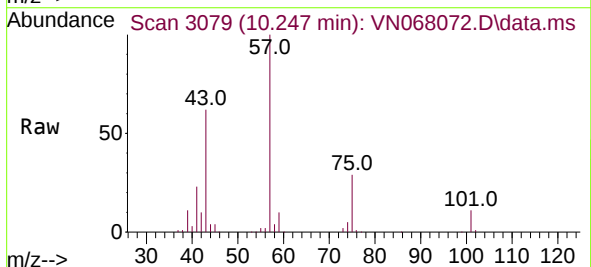


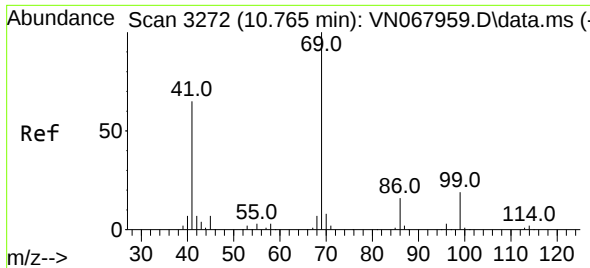

#56
Ethyl methacrylate
Concen: 3.22 ug/l
RT: 10.875 min Scan# 3313
Delta R.T. 0.110 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 69 Resp: 945
Ion Ratio Lower Upper
69 100
41 2575.6 58.6 88.0#
39 1292.1 38.3 57.5#

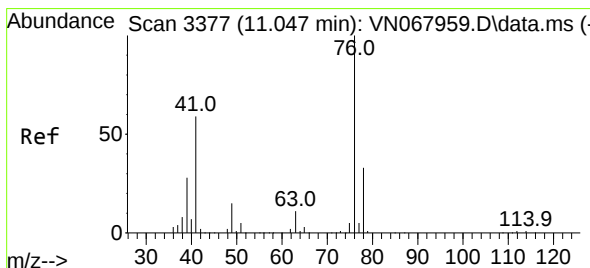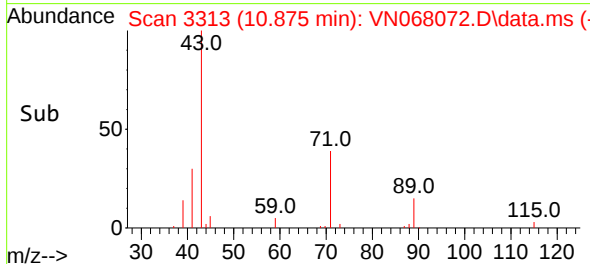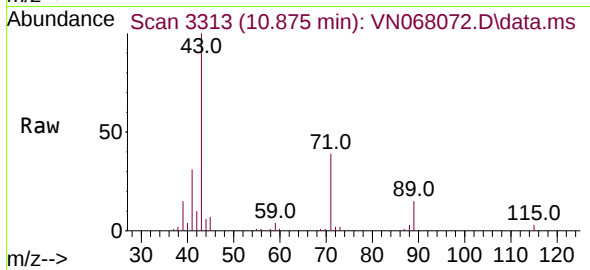

#57
1,3-Dichloropropane
Concen: 7.15 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 76 Resp: 46669
Ion Ratio Lower Upper
76 100
78 0.3 25.7 38.5#


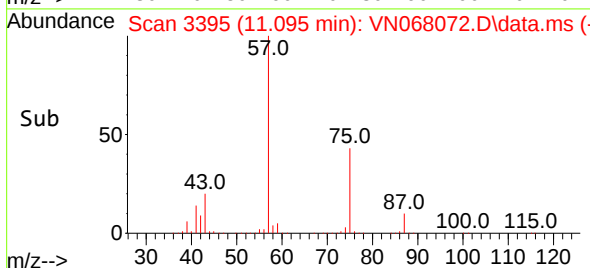
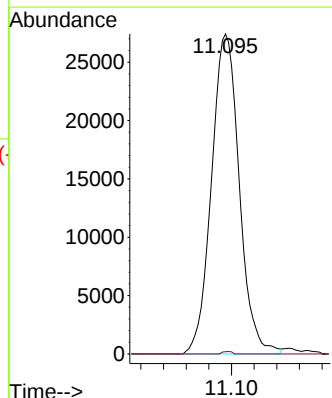
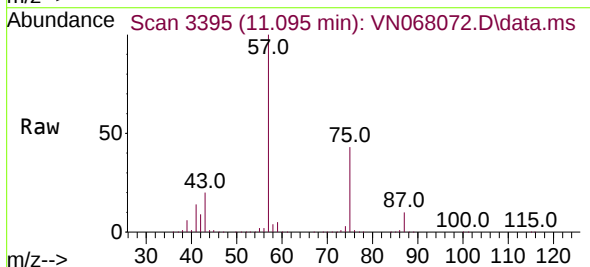




#59
2-Hexanone
Concen: 154.99 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 654148
Ion Ratio Lower Upper
43 100
58 18.4 24.7 74.1#

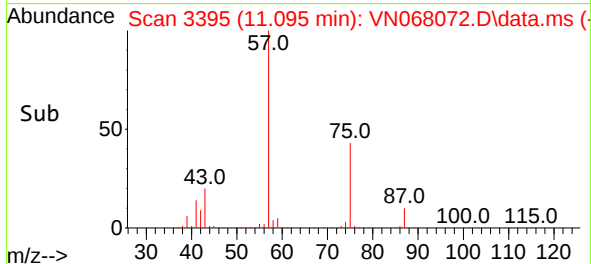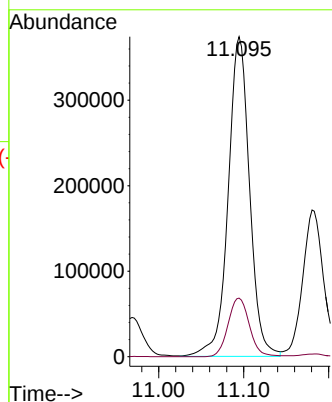

#60
Dibromochloromethane
Concen: 3.39 ug/l
RT: 11.489 min Scan# 3542
Delta R.T. 0.249 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion:129 Resp: 448
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#




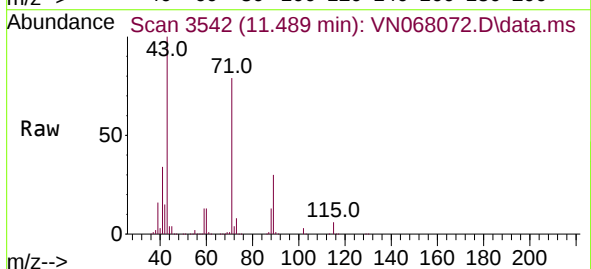


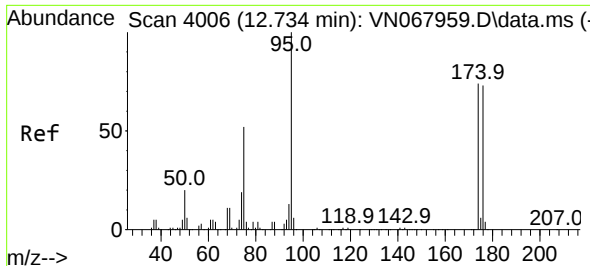

#62
4-Bromofluorobenzene
Concen: 43.13 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 95 Resp: 241978
Ion Ratio Lower Upper
95 100
174 72.9 0.0 122.0
176 68.8 0.0 117.6

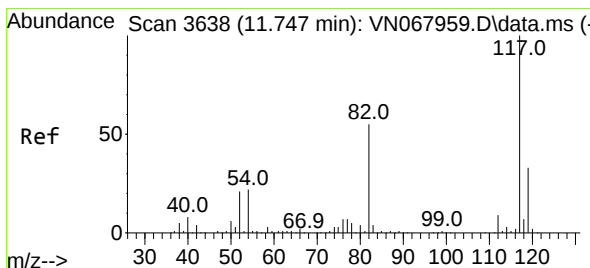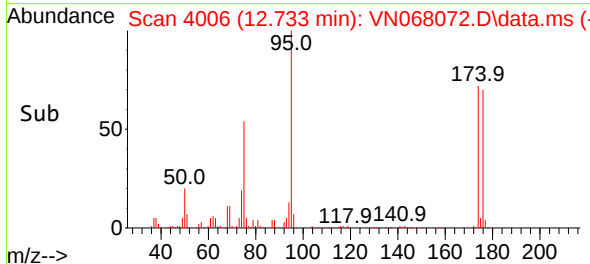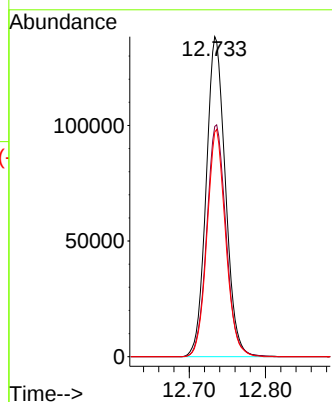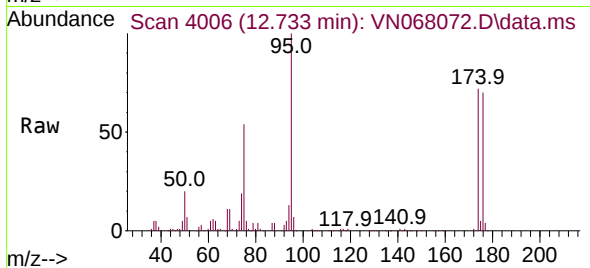

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.002 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion: 117 Resp: 605531
Ion Ratio Lower Upper
117 100
82 54.2 53.1 79.7
119 31.4 25.5 38.3


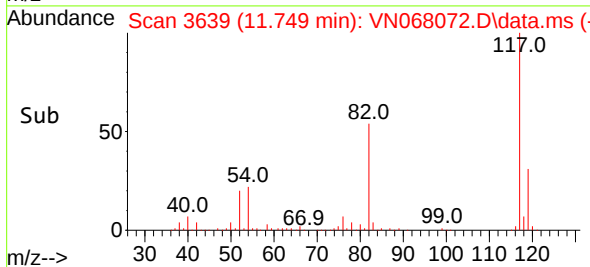

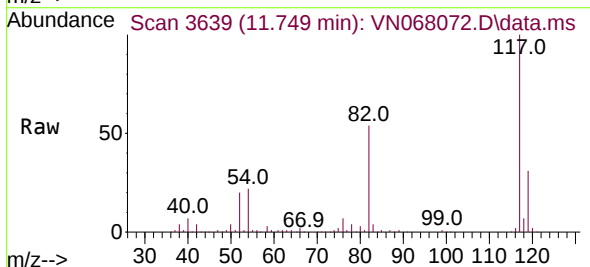




#68
m/p-Xylenes
Concen: 4.08 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. -0.003 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 136
Ion Ratio Lower Upper
106 100
91 319.9 180.6 270.8#

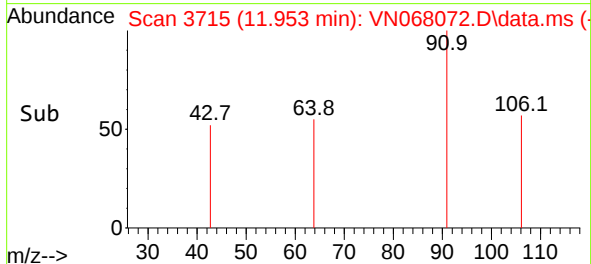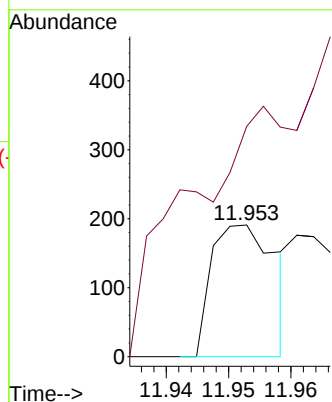

#70
Styrene
Concen: 2.65 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.003 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Tgt Ion:104 Resp: 307
Ion Ratio Lower Upper
104 100
78 29.3 48.2 72.2#
103 0.0 44.5 66.7#



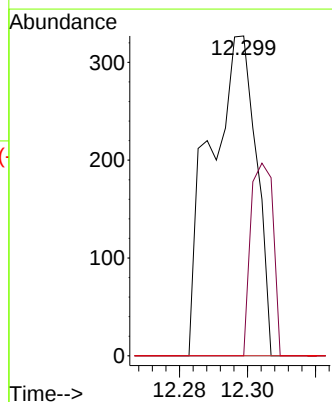
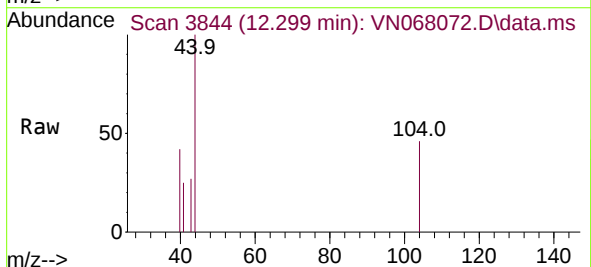


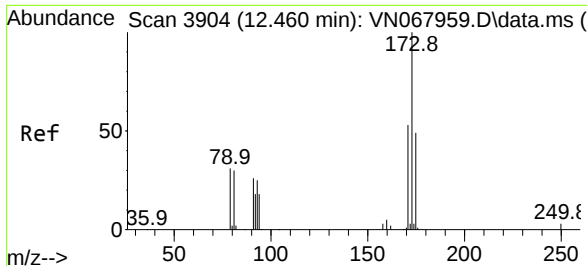

#71
Bromoform
Concen: 4.08 ug/l
RT: 12.717 min Scan# 4000
Delta R.T. 0.257 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 213
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0

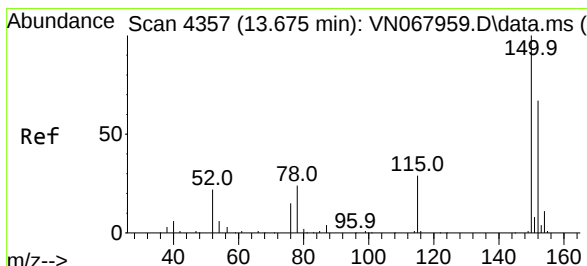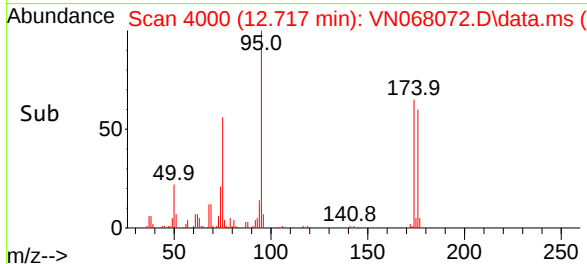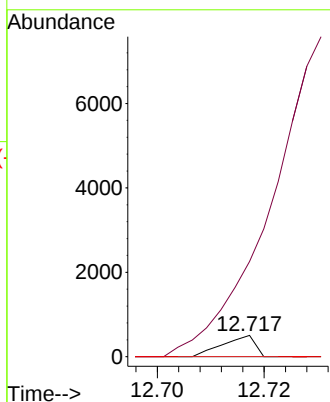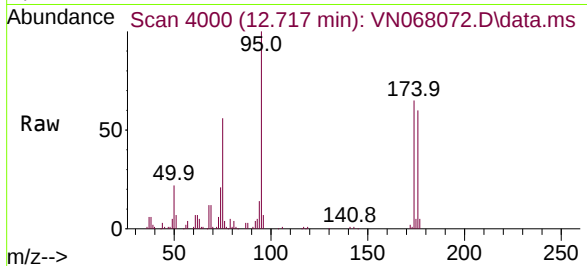

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55


Tgt Ion:152 Resp: 191484
Ion Ratio Lower Upper
152 100
115 62.3 36.1 108.5
150 159.5 0.0 351.8

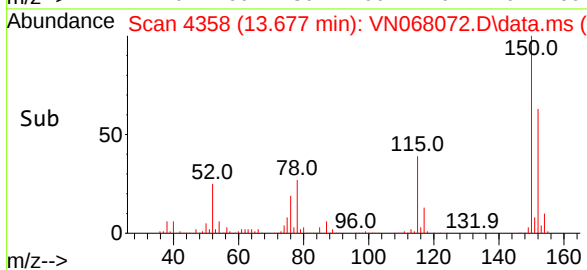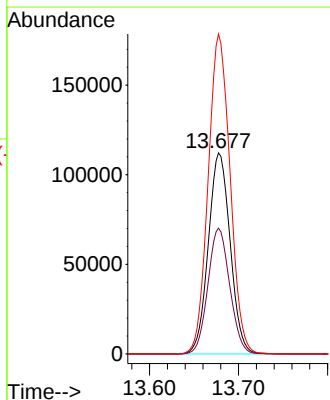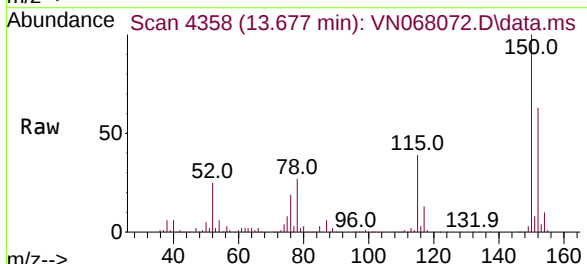






#74
N-amy1 acetate
Concen: 0.21 ug/l
RT: 12.374 min Scan# 3872
Delta R.T. -0.016 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 43 Resp: 1156

Ion	Ratio	Lower	Upper
43	100		
70	0.0	29.4	44.2#
55	0.0	17.0	25.4#
61	0.0	17.6	26.4#

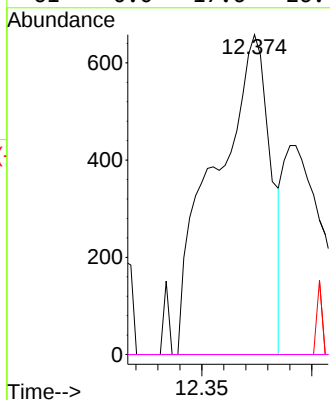




#76
1,2,3-Trichloropropane
Concen: 34.20 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55



Tgt Ion: 75 Resp: 131532

Ion	Ratio	Lower	Upper
75	100		
77	1.1	0.0	0.0#



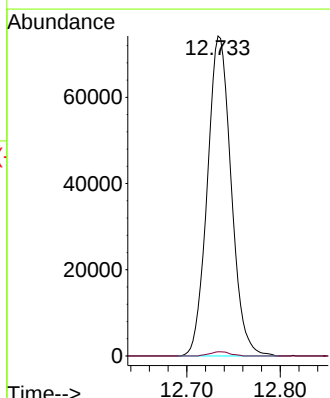



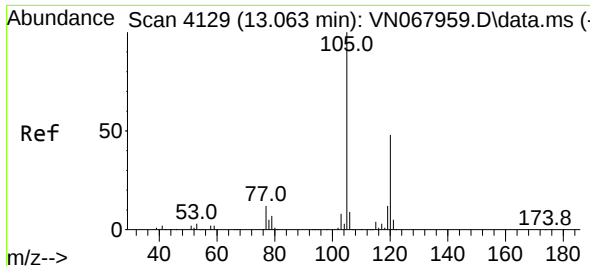

#80
1,3,5-Trimethylbenzene
Concen: 0.86 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.002 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 10874
Ion Ratio Lower Upper
105 100
120 47.6 22.2 66.6

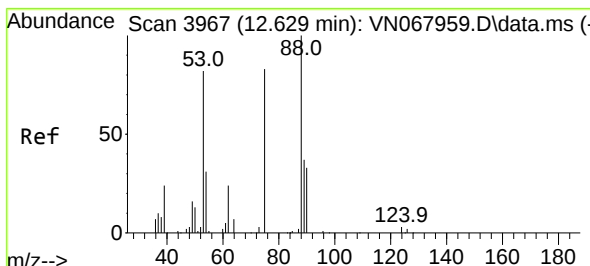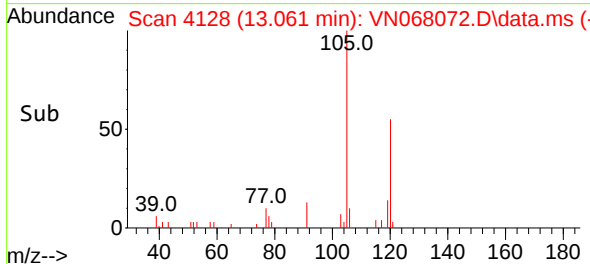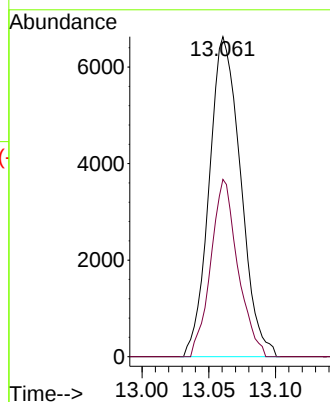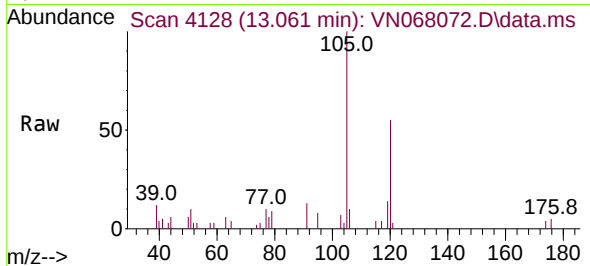

#81
trans-1,4-Dichloro-2-butene
Concen: 91.66 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55


Tgt Ion: 75 Resp: 131532
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

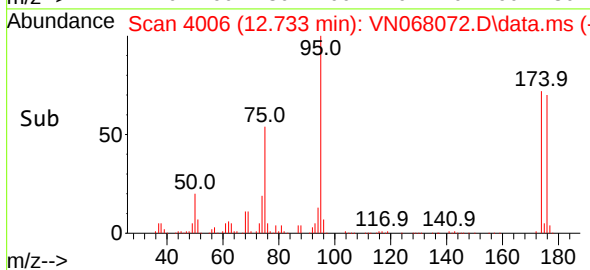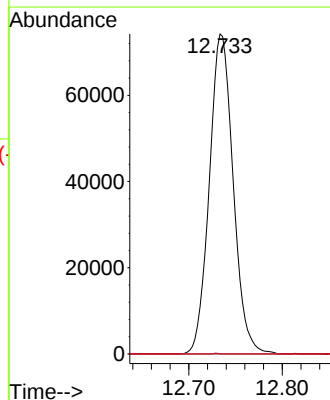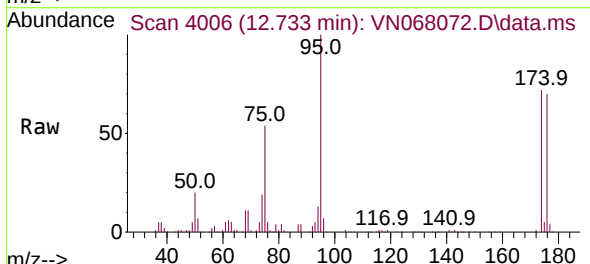






#93
1,2,4-Trichlorobenzene
Concen: 2.58 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:180 Resp: 339
Ion Ratio Lower Upper
180 100
182 47.8 47.5 142.5
145 0.0 17.2 51.6#

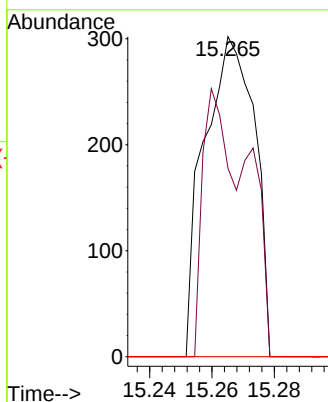


#95
Naphthalene
Concen: 3.21 ug/l
RT: 15.498 min Scan# 5037
Delta R.T. -0.011 min
Lab File: VN068072.D
Acq: 11 Aug 2021 14:55




Tgt Ion:128 Resp: 732
Ion Ratio Lower Upper
128 100
127 11.5 10.6 15.8
129 0.0 8.6 12.8#

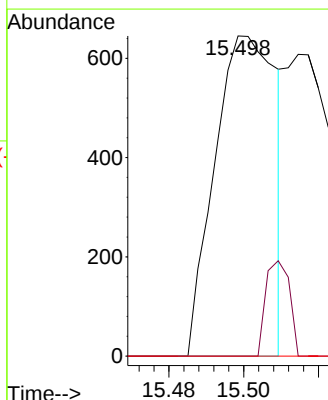



#96
 1,2,3-Trichlorobenzene
 Concen: 2.42 ug/l
 RT: 15.689 min Scan# 5108
 Delta R.T. -0.013 min
 Lab File: VN068072.D
 Acq: 11 Aug 2021 14:55

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:	180	Resp:	150
Ion	Ratio	Lower	Upper
180	100		
182	111.3	47.8	143.3
145	0.0	18.2	54.6#

