

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081122\
 Data File : VN073821.D
 Acq On : 11 Aug 2022 13:35
 Operator : JC\MD
 Sample : PB146912TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB146912TB

Quant Time: Aug 12 06:00:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.022	168	394409	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	629984	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	635254	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	306590	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	225246	46.863	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.720%		
35) Dibromofluoromethane	7.951	113	215823	54.557	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	109.120%		
50) Toluene-d8	10.380	98	732127	47.031	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	94.060%		
62) 4-Bromofluorobenzene	12.674	95	279210	51.033	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	102.060%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.263	50	940	Below Cal		96
5) Bromomethane	2.840	94	1879	0.484 ug/l		92
6) Chloroethane	2.946	64	54	Below Cal	#	42
11) Tert butyl alcohol	5.293	59	1969	1.899 ug/l	#	80
16) Acetone	4.234	43	85171	32.991 ug/l		98
18) Methyl Acetate	4.781	43	3139	0.489 ug/l		91
20) Methylene Chloride	5.010	84	17875	2.172 ug/l		90
25) 2-Butanone	7.269	43	27553	6.872 ug/l		90
26) 2,2-Dichloropropane	7.239	77	1529	0.250 ug/l	#	53
29) Tetrahydrofuran	7.628	42	2446	0.965 ug/l	#	85
31) Cyclohexane	8.010	56	8041	1.124 ug/l	#	47
36) 1,1-Dichloropropene	8.022	75	28426	5.042 ug/l	#	48
37) Ethyl Acetate	7.345	43	74068	9.975 ug/l		99
38) Carbon Tetrachloride	8.016	117	36217	6.325 ug/l	#	17
41) Methacrylonitrile	7.622	41	1259	0.375 ug/l	#	37
42) 1,2-Dichloroethane	8.492	62	2021	0.328 ug/l	#	74
43) Isopropyl Acetate	8.498	43	283984	28.316 ug/l	#	92
45) 1,2-Dichloropropane	9.569	63	4382	0.958 ug/l	#	44
48) Methyl methacrylate	9.486	41	11102	2.529 ug/l	#	38
49) 1,4-Dioxane	9.486	88	54	0.436 ug/l	#	1
51) 4-Methyl-2-Pentanone	10.275	43	24273	3.374 ug/l	#	76
53) t-1,3-Dichloropropene	10.557	75	2204	0.366 ug/l	#	1
54) cis-1,3-Dichloropropene	10.186	75	108865	16.042 ug/l	#	66
57) 1,3-Dichloropropane	11.033	76	14604	1.846 ug/l	#	42
59) 2-Hexanone	11.033	43	197153	36.175 ug/l	#	50
74) N-amyl acetate	12.298	43	2012	0.237 ug/l	#	44
76) 1,2,3-Trichloropropane	12.674	75	141010	23.391 ug/l	#	1
81) trans-1,4-Dichloro-2-b...	12.674	75	141010	59.604 ug/l	#	10
95) Naphthalene	15.433	128	5151	0.296 ug/l	#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081122\
Data File : VN073821.D
Acq On : 11 Aug 2022 13:35
Operator : JC\MD
Sample : PB146912TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB146912TB

Quant Time: Aug 12 06:00:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 05:09:32 2022
Response via : Initial Calibration




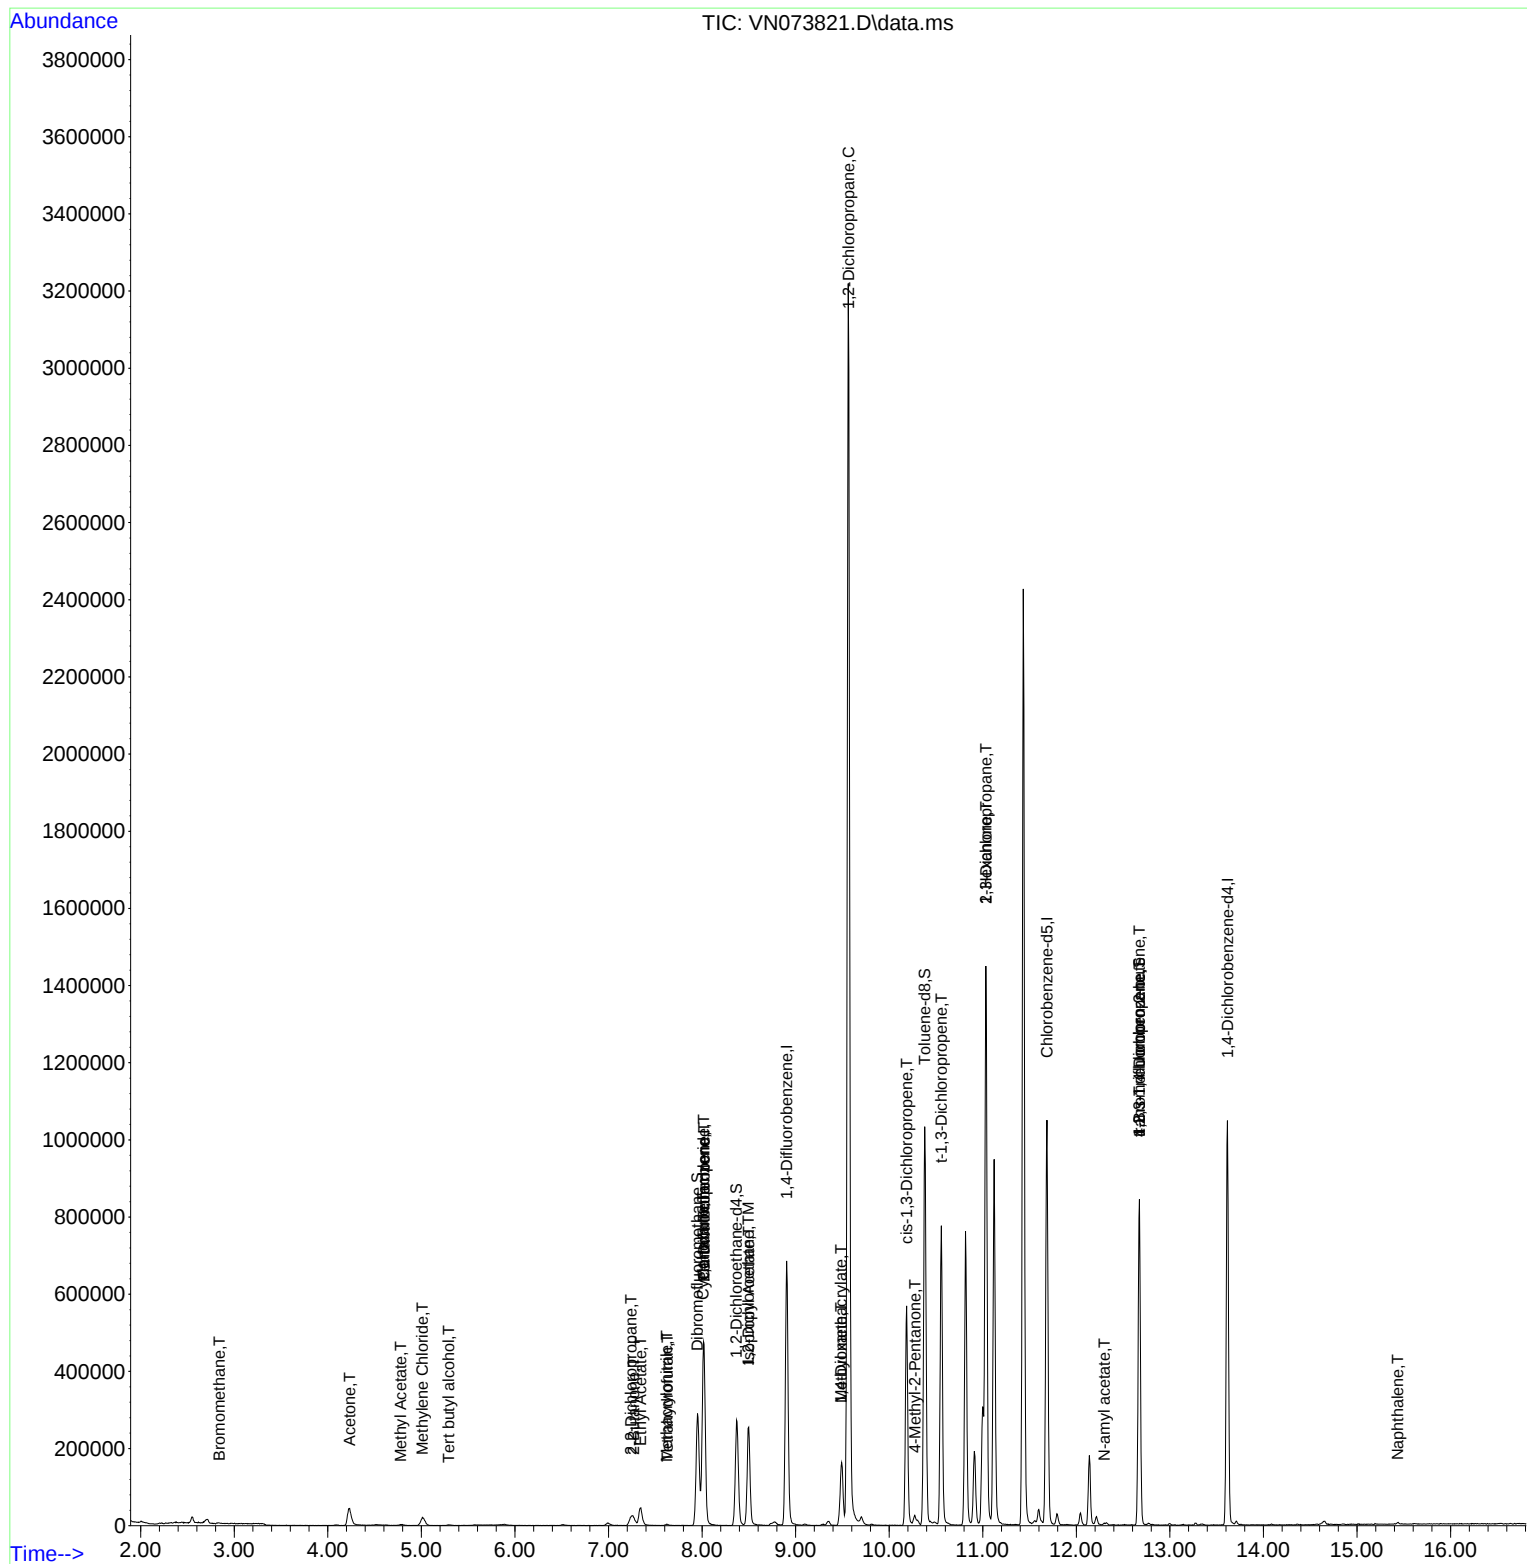




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion:168 Resp: 394409
Ion Ratio Lower Upper
168 100
99 52.4 42.3 63.5

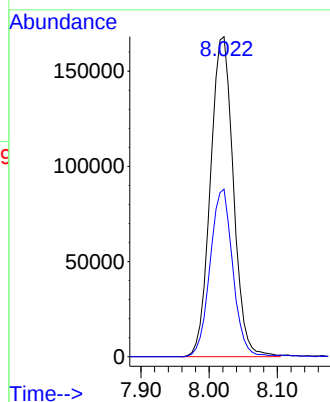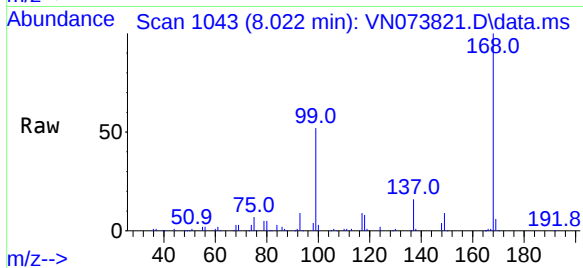

#3
Chloromethane
Concen: Below Cal
RT: 2.263 min Scan# 64
Delta R.T. -0.006 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 50 Resp: 940
Ion Ratio Lower Upper
50 100
52 29.9 25.7 38.5


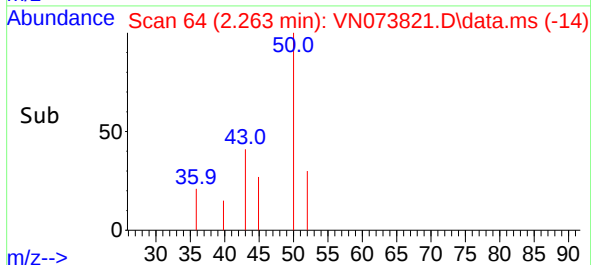

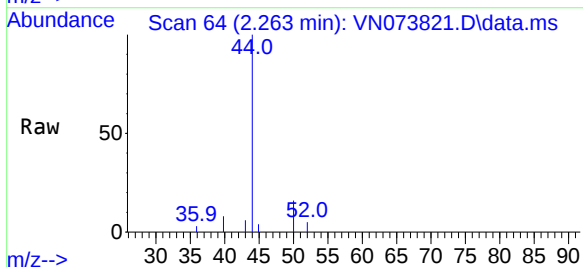




#5
Bromomethane
Concen: 0.484 ug/l
RT: 2.840 min Scan# 11
Delta R.T. 0.053 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 94 Resp: 1879
Ion Ratio Lower Upper
94 100
96 87.3 76.0 114.0

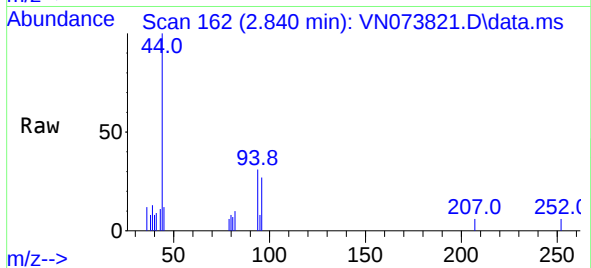

#6
Chloroethane
Concen: Below Cal
RT: 2.946 min Scan# 180
Delta R.T. -0.011 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 64 Resp: 54
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#


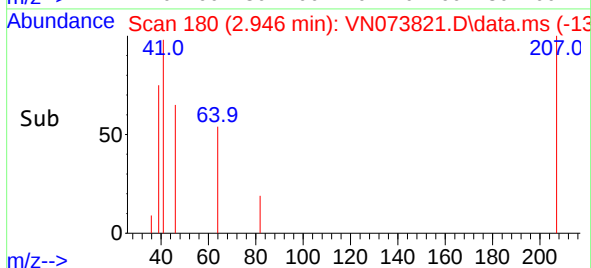
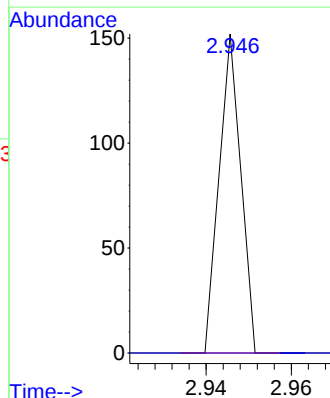





#11
Tert butyl alcohol
Concen: 1.899 ug/l
RT: 5.293 min Scan# 51
Delta R.T. 0.001 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 59 Resp: 1969
Ion Ratio Lower Upper
59 100
57 2.7 8.3 12.5#

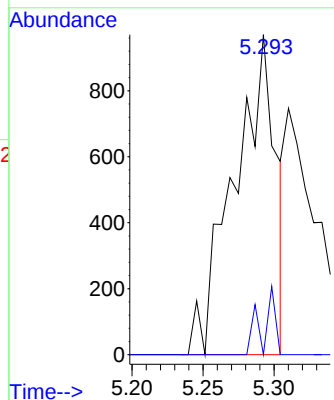

#16
Acetone
Concen: 32.991 ug/l
RT: 4.234 min Scan# 399
Delta R.T. 0.012 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 43 Resp: 85171
Ion Ratio Lower Upper
43 100
58 33.5 26.0 39.0


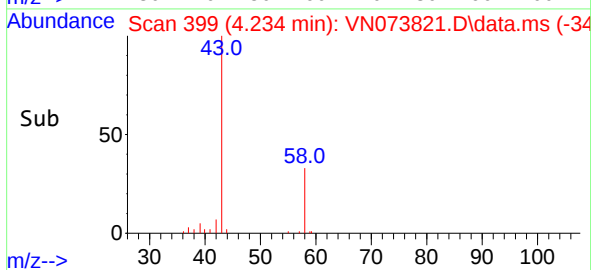
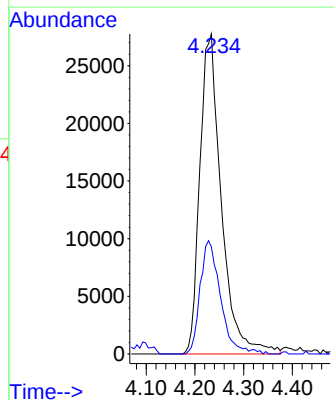





#18
Methyl Acetate
Concen: 0.489 ug/l
RT: 4.781 min Scan# 492
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 43 Resp: 3139
Ion Ratio Lower Upper
43 100
74 22.6 21.6 32.4



#20
Methylene Chloride
Concen: 2.172 ug/l
RT: 5.010 min Scan# 531
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 84 Resp: 17875
Ion Ratio Lower Upper
84 100
49 103.7 88.3 132.5
51 29.8 28.2 42.2
86 51.1 50.6 76.0

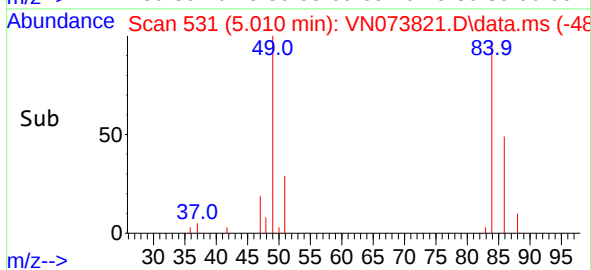



#25

2-Butanone

Concen: 6.872 ug/l

RT: 7.269 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN073821.D

Acq: 11 Aug 2022 13:35

Instrument :

MSVOA_N

ClientSampleId :





PB146912TB

Tgt Ion: 43 Resp: 27553

Ion Ratio Lower Upper

43 100

72 24.0 23.7 35.5

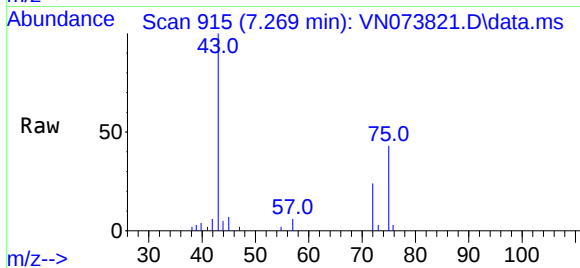

#26

2,2-Dichloropropane

Concen: 0.250 ug/l

RT: 7.239 min Scan# 910

Delta R.T. -0.012 min

Lab File: VN073821.D




Acq: 11 Aug 2022 13:35


Tgt Ion: 77 Resp: 1529

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.2#

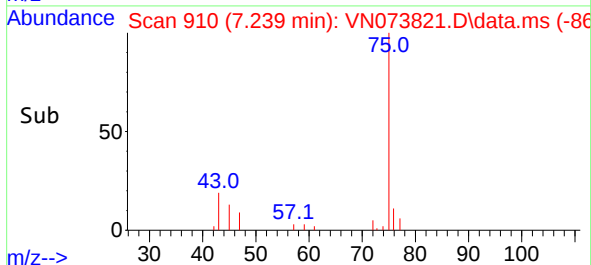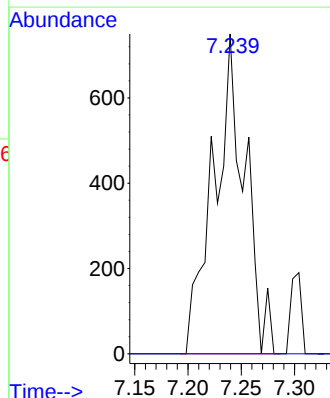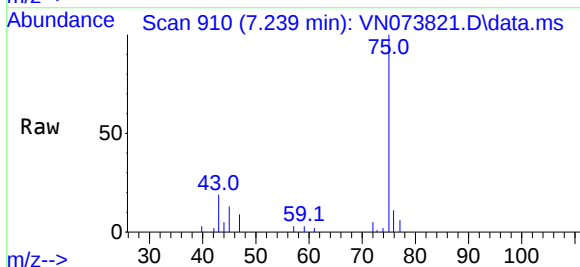



#29

Tetrahydrofuran

Concen: 0.965 ug/l

RT: 7.628 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN073821.D

Acq: 11 Aug 2022 13:35

Instrument :

MSVOA_N

ClientSampleId :

PB146912TB





Tgt Ion: 42 Resp: 2446

Ion Ratio Lower Upper

42 100

72 39.6 39.7 59.5#

71 36.1 36.6 55.0#

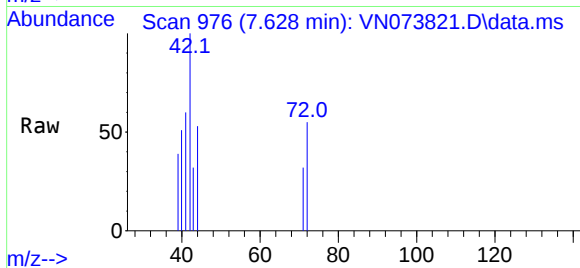

#31

Cyclohexane

Concen: 1.124 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.012 min

Lab File: VN073821.D

Acq: 11 Aug 2022 13:35




Tgt Ion: 56 Resp: 8041


Ion Ratio Lower Upper

56 100

69 122.3 27.8 41.8#

84 113.0 76.9 115.3


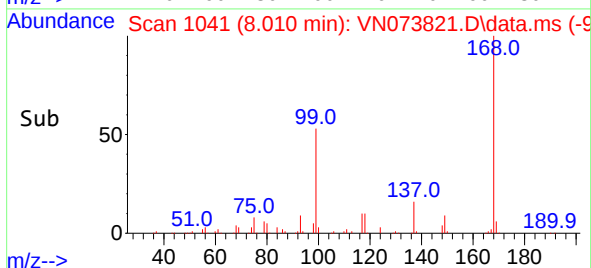
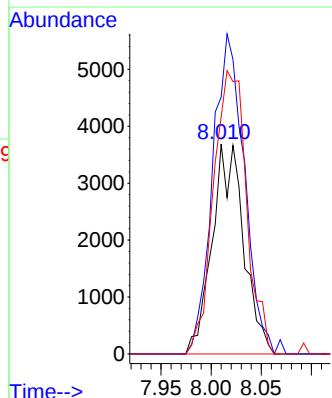
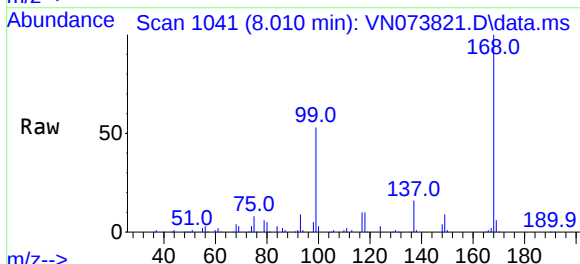


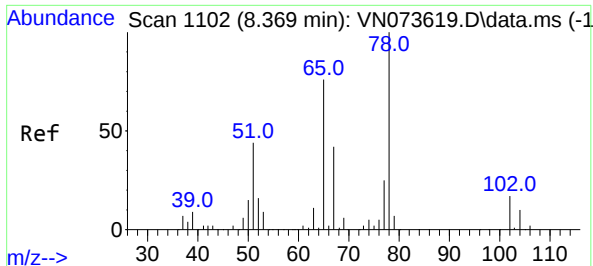

#33
1,2-Dichloroethane-d4
Concen: 46.863 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 65 Resp: 225246
Ion Ratio Lower Upper
65 100
67 53.5 0.0 104.8

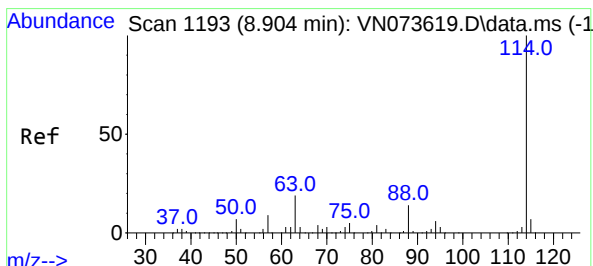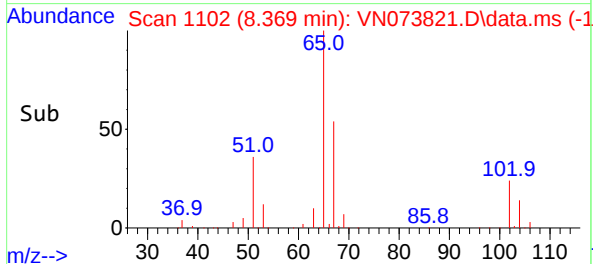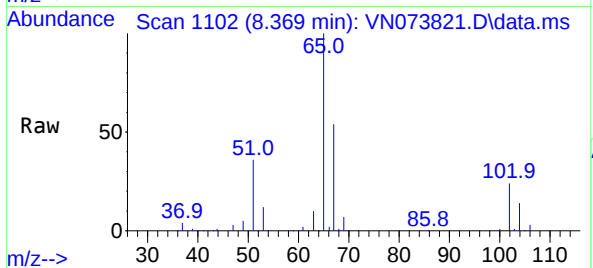

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.904 min Scan# 1193
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 114 Resp: 629984
Ion Ratio Lower Upper
114 100
63 18.4 0.0 40.0
88 14.7 0.0 32.6


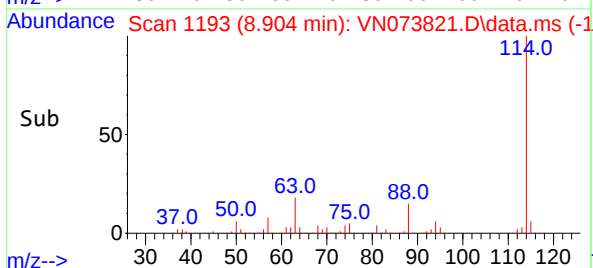

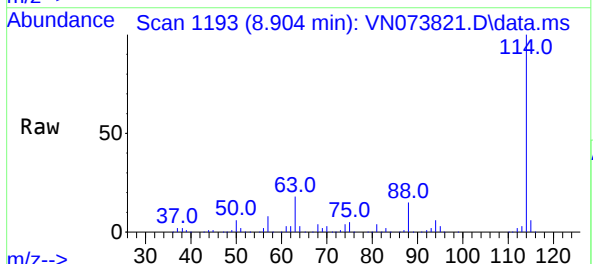


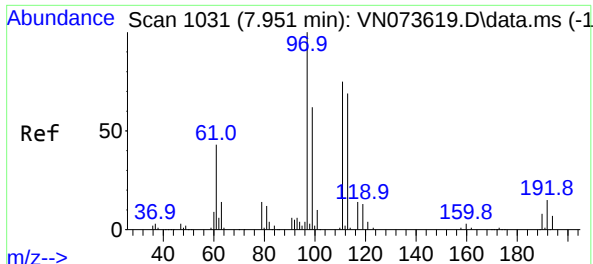

#35
Dibromofluoromethane
Concen: 54.557 ug/l
RT: 7.951 min Scan# 1031
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion:113 Resp: 215823
Ion Ratio Lower Upper
113 100
111 102.9 81.4 122.0
192 20.8 17.0 25.6

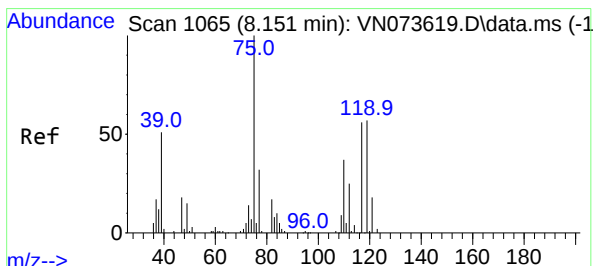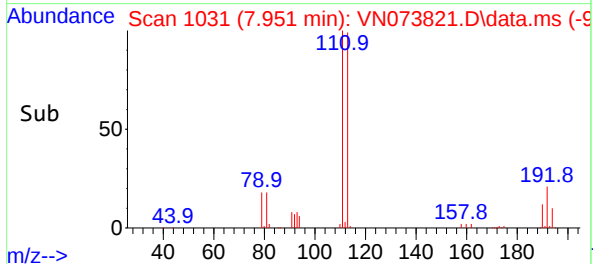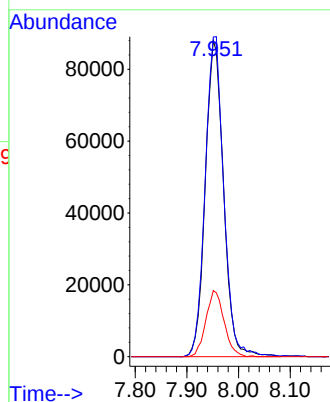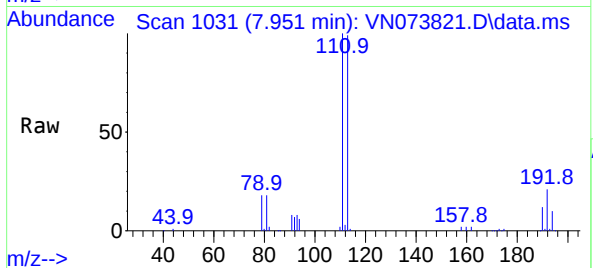

#36
1,1-Dichloropropene
Concen: 5.042 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.129 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 75 Resp: 28426
Ion Ratio Lower Upper
75 100
110 8.4 18.3 54.8#
77 0.0 25.1 37.7#

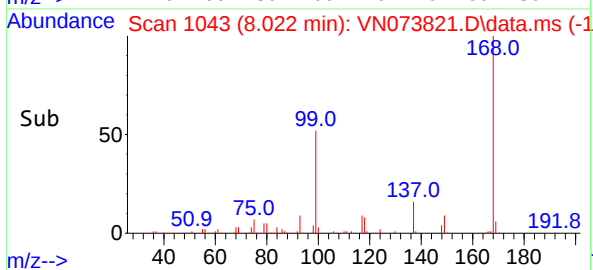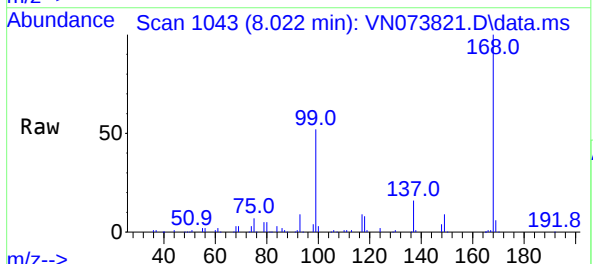







#37
Ethyl Acetate
Concen: 9.975 ug/l
RT: 7.345 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Instrument :
MSVOA_N
ClientSampleId :
PB146912TB

Tgt Ion: 43 Resp: 74068




Ion	Ratio	Lower	Upper
43	100		
61	14.8	11.8	17.6
70	10.7	9.3	13.9

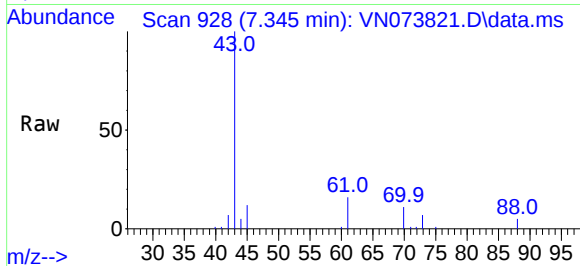


#38
Carbon Tetrachloride
Concen: 6.325 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 117 Resp: 36217


Ion	Ratio	Lower	Upper
117	100		
119	6.0	75.8	113.8#
121	0.0	24.6	37.0#

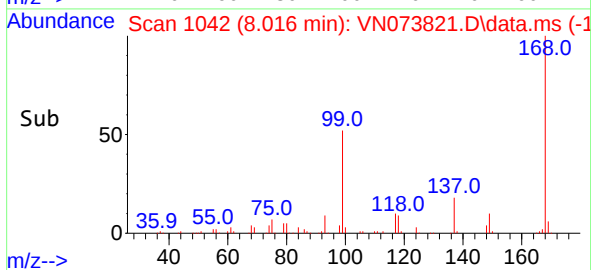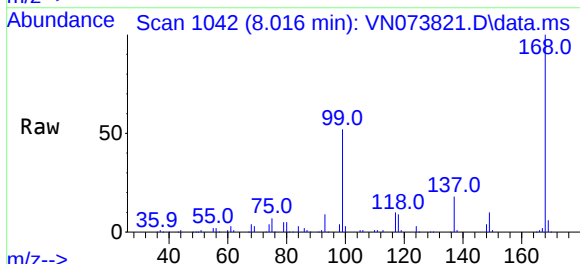






#41
Methacrylonitrile
Concen: 0.375 ug/l
RT: 7.622 min Scan# 91
Delta R.T. 0.059 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Instrument :
MSVOA_N
ClientSampleId :
PB146912TB



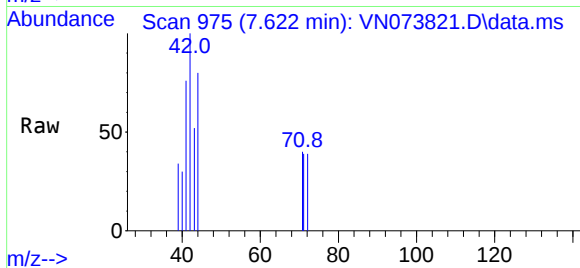



Tgt Ion: 41 Resp: 1259
Ion Ratio Lower Upper
41 100
39 50.0 48.6 73.0
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#



#42
1,2-Dichloroethane
Concen: 0.328 ug/l
RT: 8.492 min Scan# 1123
Delta R.T. 0.029 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 62 Resp: 2021
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4

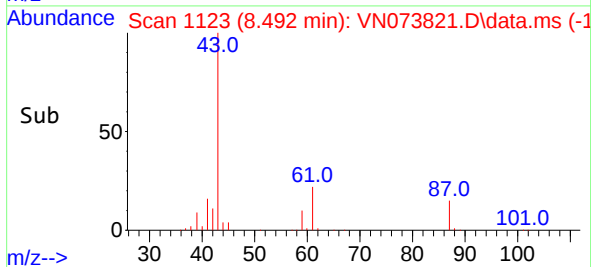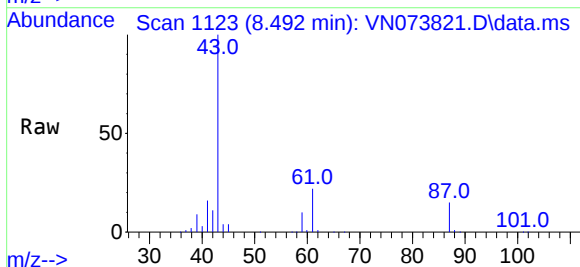

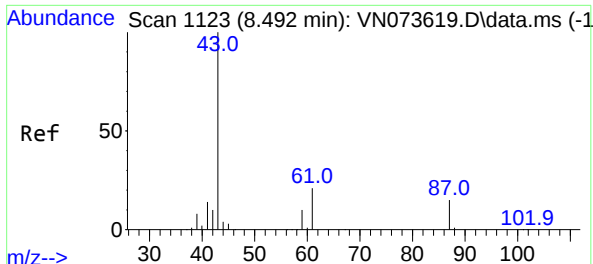

#43

Isopropyl Acetate

Concen: 28.316 ug/l

RT: 8.498 min Scan# 1123

Delta R.T. 0.006 min

Lab File: VN073821.D

Acq: 11 Aug 2022 13:35

Instrument :

MSVOA_N

ClientSampleId :

PB146912TB





Tgt Ion: 43 Resp: 283984

Ion Ratio Lower Upper

43 100

61 21.2 21.9 32.9#

87 15.2 12.0 18.0

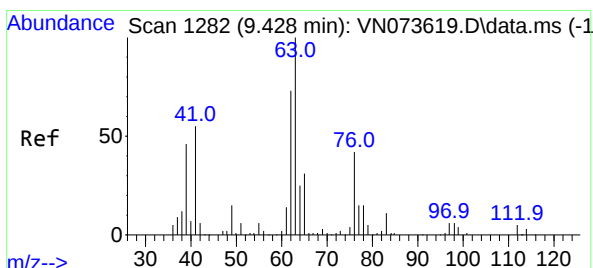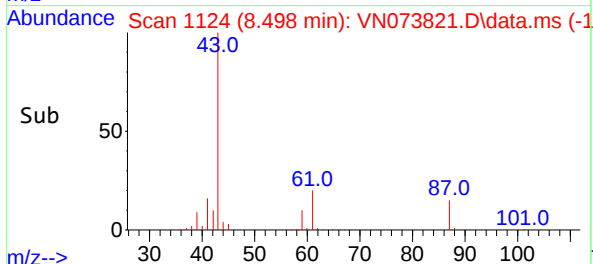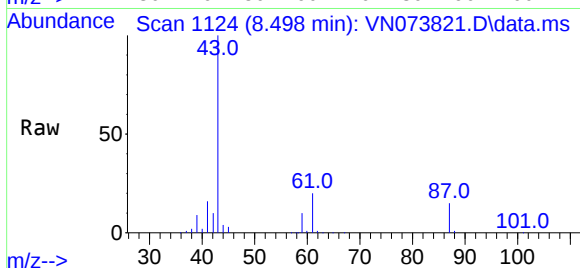

#45

1,2-Dichloropropane

Concen: 0.958 ug/l

RT: 9.569 min Scan# 1306

Delta R.T. 0.141 min

Lab File: VN073821.D




Acq: 11 Aug 2022 13:35


Tgt Ion: 63 Resp: 4382

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#


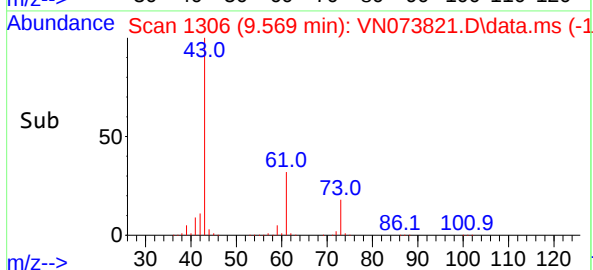

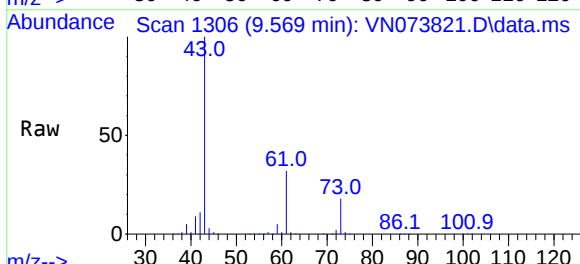


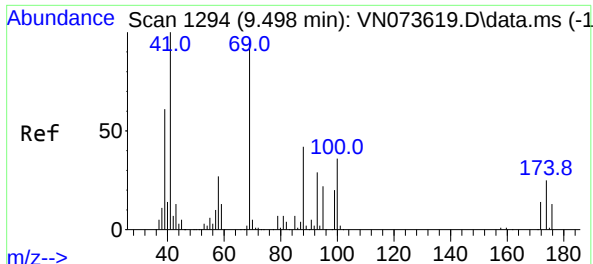

#48
Methyl methacrylate
Concen: 2.529 ug/l
RT: 9.486 min Scan# 1292
Delta R.T. -0.012 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument : MSVOA_N
ClientSampleId : PB146912TB


Tgt Ion: 41 Resp: 11102
Ion Ratio Lower Upper
41 100
69 1.3 74.7 112.1#
39 51.2 45.6 68.4

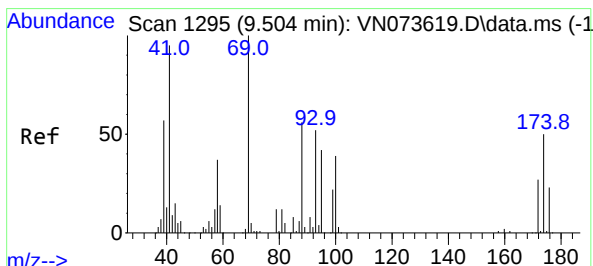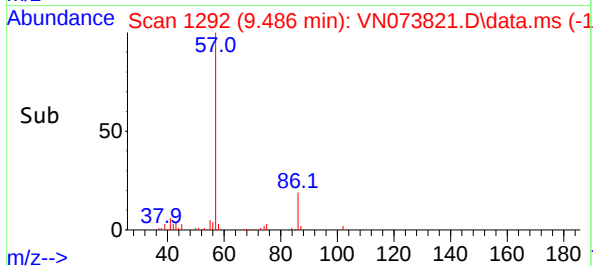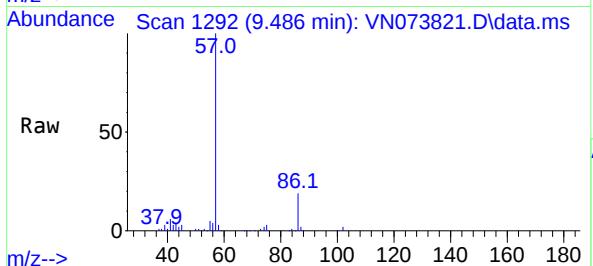

#49
1,4-Dioxane
Concen: 0.436 ug/l
RT: 9.486 min Scan# 1292
Delta R.T. -0.018 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 88 Resp: 54
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 14848.1 54.2 81.4#


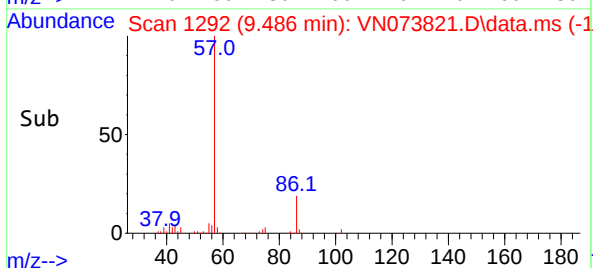
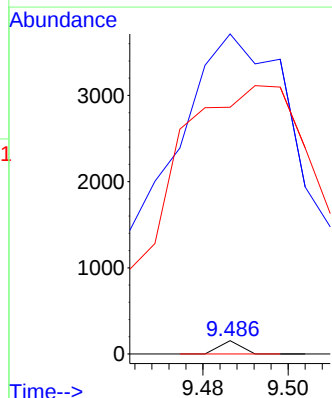
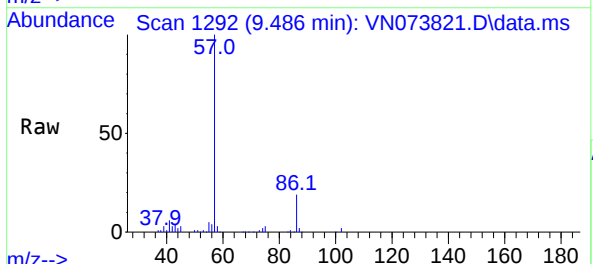




#50
Toluene-d8
Concen: 47.031 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 98 Resp: 732127
Ion Ratio Lower Upper
98 100
100 64.8 52.6 78.8

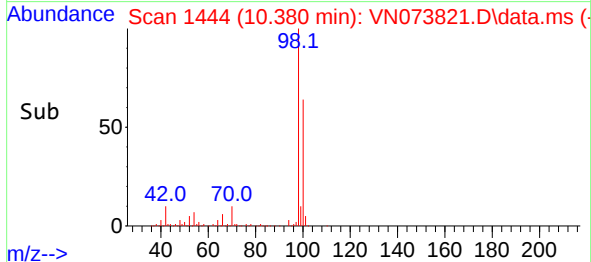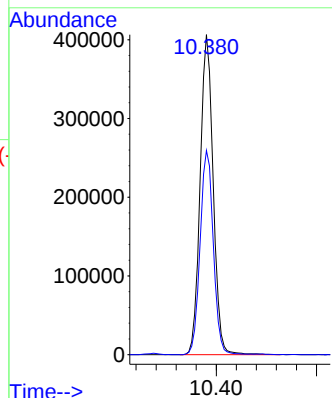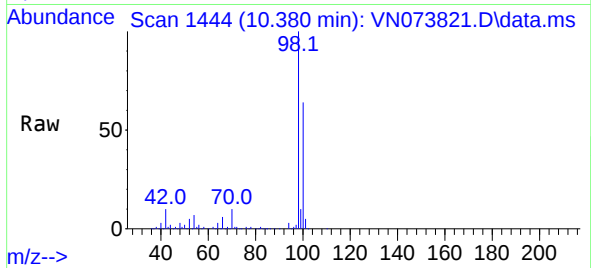

#51
4-Methyl-2-Pentanone
Concen: 3.374 ug/l
RT: 10.275 min Scan# 1426
Delta R.T. -0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 43 Resp: 24273
Ion Ratio Lower Upper
43 100
58 27.3 34.1 51.1#


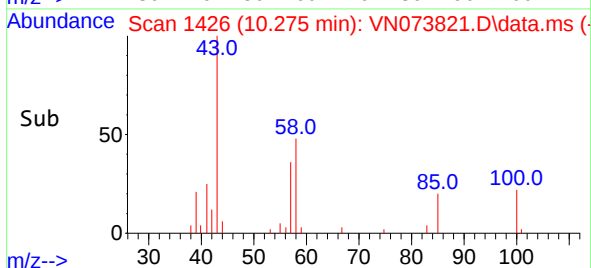
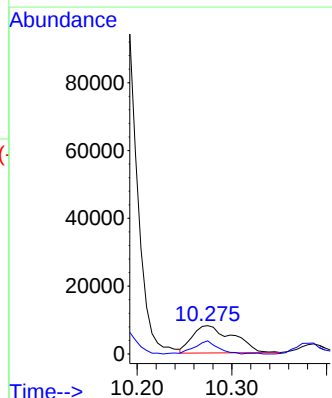





#53
t-1,3-Dichloropropene
Concen: 0.366 ug/l
RT: 10.557 min Scan# 1411
Delta R.T. -0.106 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 75 Resp: 2204
Ion Ratio Lower Upper
75 100
77 106.8 25.6 38.4#

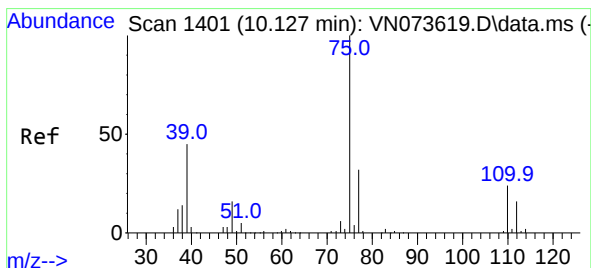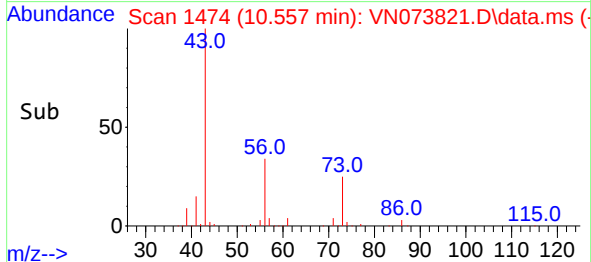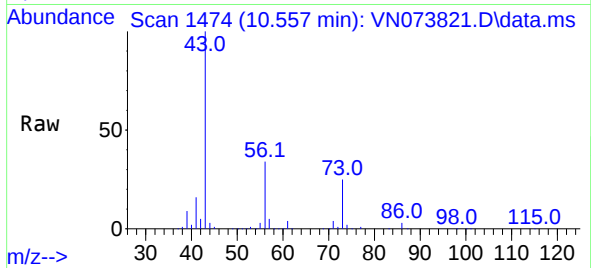

#54
cis-1,3-Dichloropropene
Concen: 16.042 ug/l
RT: 10.186 min Scan# 1411
Delta R.T. 0.059 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 75 Resp: 108865
Ion Ratio Lower Upper
75 100
77 0.9 25.2 37.8#
39 32.0 35.7 53.5#

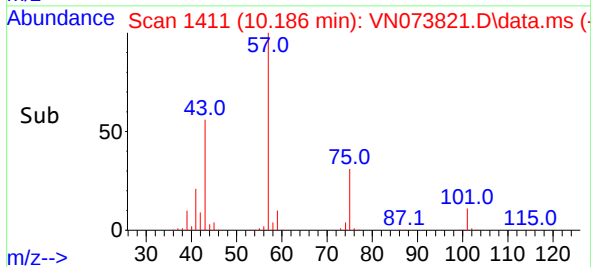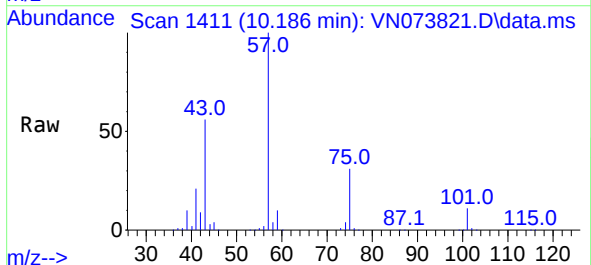

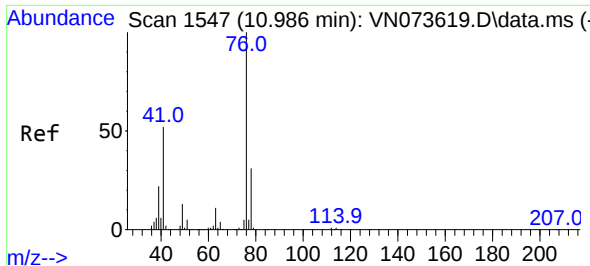

#57

1,3-Dichloropropane

Concen: 1.846 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.047 min

Lab File: VN073821.D

Acq: 11 Aug 2022 13:35

Instrument :

MSVOA_N

ClientSampleId :





PB146912TB

Tgt Ion: 76 Resp: 14604

Ion Ratio Lower Upper

76 100

78 0.0 26.2 39.2#

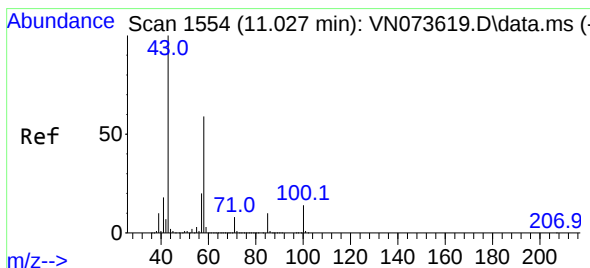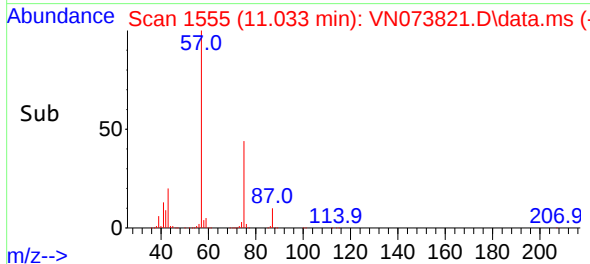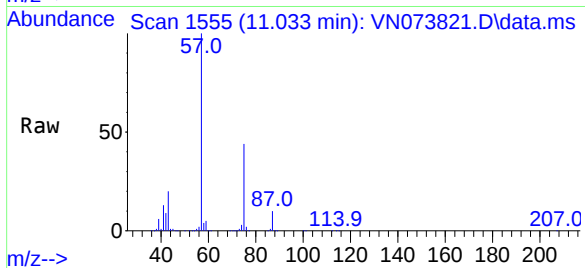

#59

2-Hexanone

Concen: 36.175 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.006 min

Lab File: VN073821.D




Acq: 11 Aug 2022 13:35


Tgt Ion: 43 Resp: 197153

Ion Ratio Lower Upper

43 100

58 21.6 29.7 89.1#


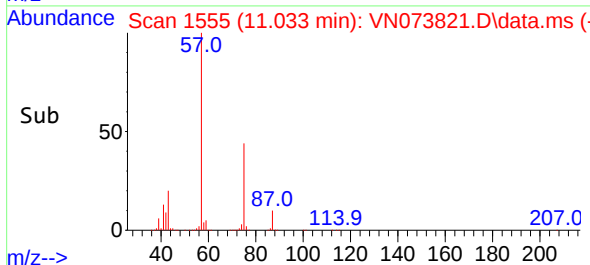
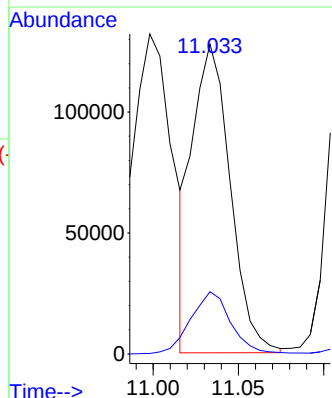
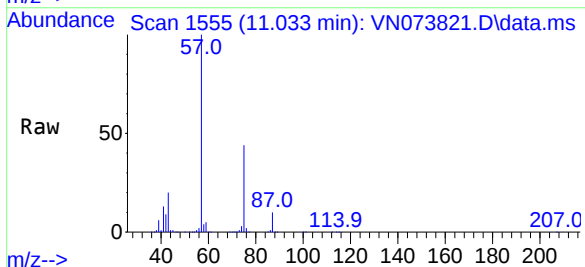


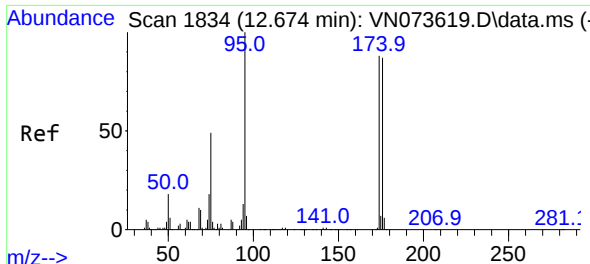

#62
4-Bromofluorobenzene
Concen: 51.033 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 95 Resp: 279210
Ion Ratio Lower Upper
95 100
174 91.9 0.0 167.6
176 88.4 0.0 163.4

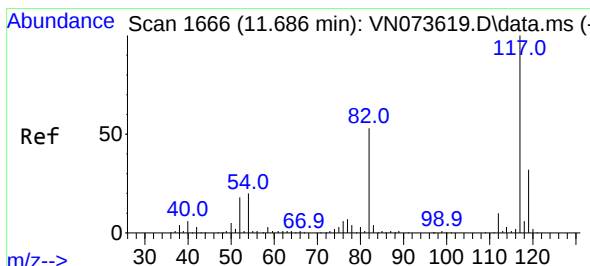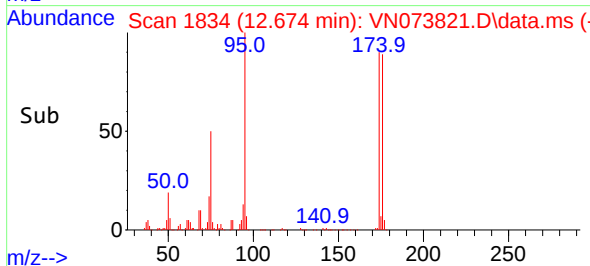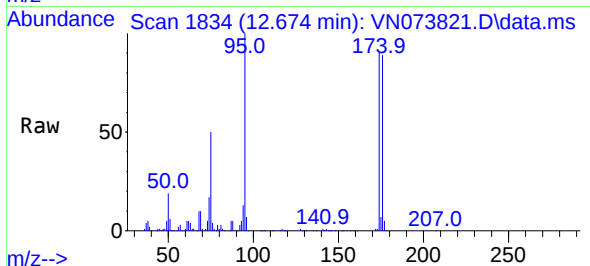

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35


Tgt Ion: 117 Resp: 635254
Ion Ratio Lower Upper
117 100
82 51.9 44.2 66.2
119 32.2 25.4 38.0

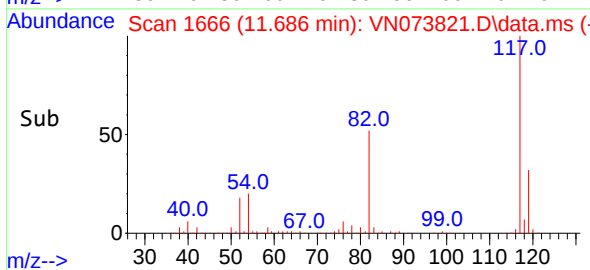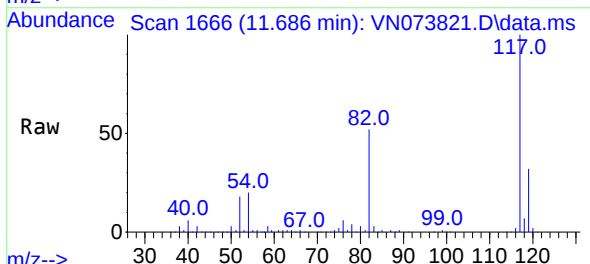






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Instrument :
MSVOA_N
ClientSampleId :
PB146912TB







Tgt Ion:152 Resp: 306590
Ion Ratio Lower Upper
152 100
115 54.5 28.9 86.7
150 155.3 0.0 356.2



#74
N-ethyl acetate
Concen: 0.237 ug/l
RT: 12.298 min Scan# 1770
Delta R.T. -0.029 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Tgt Ion: 43 Resp: 2012
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 10.3 21.1 31.7#
61 0.0 21.1 31.7#


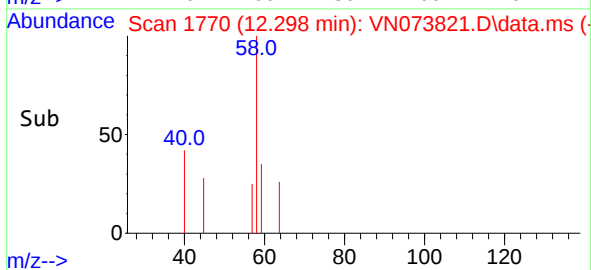






#76
1,2,3-Trichloropropane
Concen: 23.391 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35




Instrument :
MSVOA_N
ClientSampleId :
PB146912TB


Tgt Ion: 75 Resp: 141010
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#

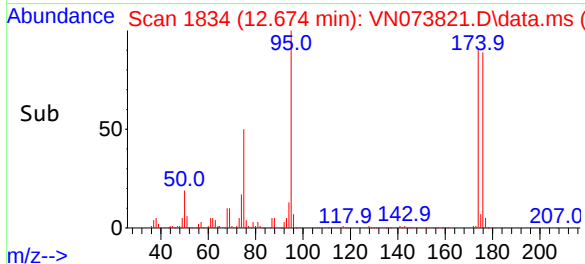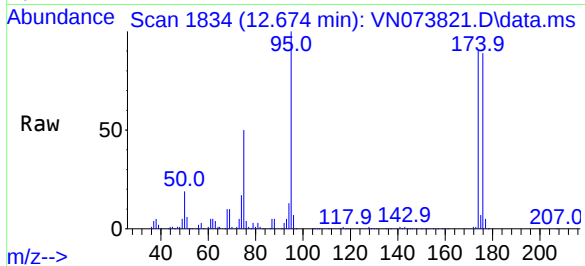

#81
trans-1,4-Dichloro-2-butene
Concen: 59.604 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.106 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35


Tgt Ion: 75 Resp: 141010
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

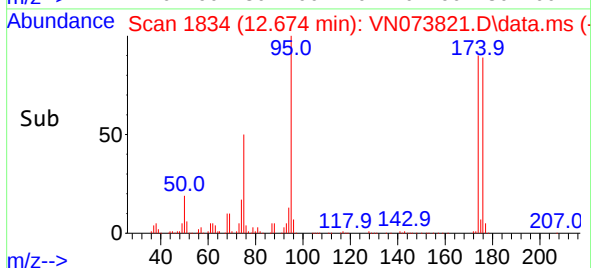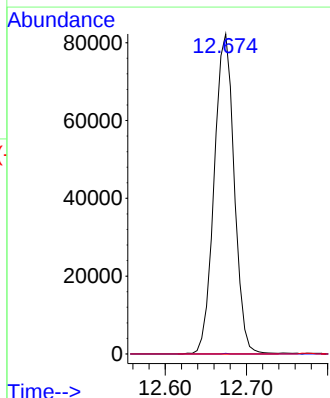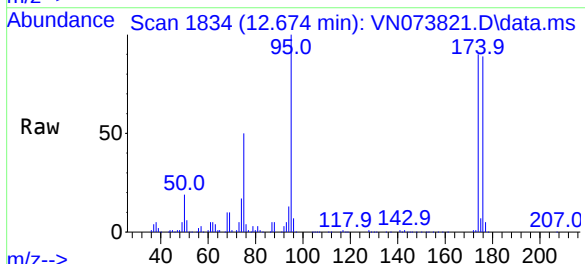

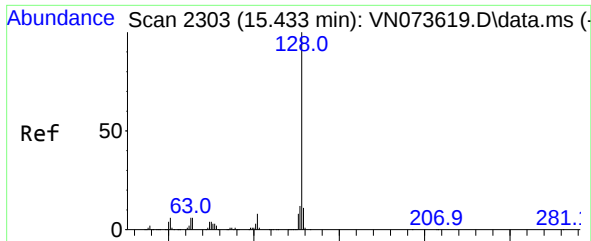

#95
Naphthalene
Concen: 0.296 ug/l
RT: 15.433 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN073821.D
Acq: 11 Aug 2022 13:35

Instrument :
MSVOA_N
ClientSampleId :
PB146912TB

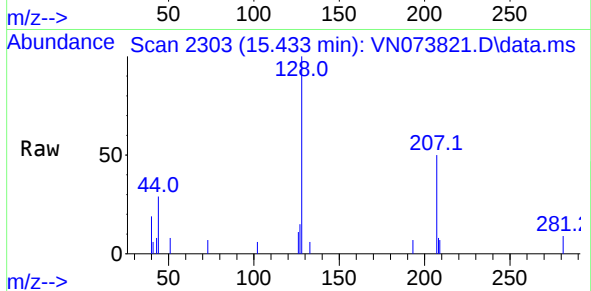

Tgt Ion:	128	Resp:	5151
Ion	Ratio	Lower	Upper
128	100		
127	8.3	10.3	15.5#
129	2.4	8.6	13.0#

