

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081122\
 Data File : VN073837.D
 Acq On : 11 Aug 2022 20:11
 Operator : JC\MD
 Sample : N4136-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-5

Quant Time: Aug 12 06:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.022	168	395155	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	629978	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	627250	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	309143	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	227270	47.195	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 94.380%			
35) Dibromofluoromethane	7.951	113	217503	54.982	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 109.960%			
50) Toluene-d8	10.381	98	740662	47.580	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 95.160%			
62) 4-Bromofluorobenzene	12.674	95	282949	51.680	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 103.360%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.269	50	993	Below Cal	#	81
5) Bromomethane	2.828	94	1701	0.438	ug/l #	80
6) Chloroethane	2.957	64	77	Below Cal	#	42
11) Tert butyl alcohol	5.310	59	3916	3.771	ug/l #	81
13) Acrolein	3.993	56	1021	0.992	ug/l	89
16) Acetone	4.228	43	198158	76.612	ug/l	99
17) Carbon Disulfide	4.457	76	3649	0.367	ug/l #	75
18) Methyl Acetate	4.781	43	10667	1.658	ug/l #	87
20) Methylene Chloride	5.016	84	35708	6.622	ug/l	94
25) 2-Butanone	7.275	43	34997	8.713	ug/l	93
29) Tetrahydrofuran	7.628	42	2617	1.030	ug/l #	72
31) Cyclohexane	8.022	56	7329	1.022	ug/l #	12
36) 1,1-Dichloropropene	8.022	75	27144	4.814	ug/l #	49
37) Ethyl Acetate	7.340	43	69542	9.366	ug/l	99
38) Carbon Tetrachloride	8.016	117	35734	6.240	ug/l #	18
41) Methacrylonitrile	7.622	41	1699	0.506	ug/l #	37
43) Isopropyl Acetate	8.498	43	266128	26.536	ug/l #	91
48) Methyl methacrylate	9.486	41	11719	2.670	ug/l #	41
49) 1,4-Dioxane	9.516	88	60	0.485	ug/l #	25
51) 4-Methyl-2-Pentanone	10.275	43	23680	3.292	ug/l #	80
52) Toluene	10.439	92	3243	0.290	ug/l	83
54) cis-1,3-Dichloropropene	10.186	75	88097	12.982	ug/l #	64
57) 1,3-Dichloropropane	11.033	76	13025	1.646	ug/l #	42
59) 2-Hexanone	11.033	43	167124	30.666	ug/l #	51
69) o-Xylene	12.222	106	1730	0.207	ug/l	94
74) N-amyl acetate	12.292	43	17741	2.075	ug/l #	45
76) 1,2,3-Trichloropropane	12.674	75	141642	23.288	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.674	75	141642	59.377	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.310	105	11187	0.611	ug/l	94
95) Naphthalene	15.439	128	10247	0.583	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.615	180	1197	0.210	ug/l #	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081122\
Data File : VN073837.D
Acq On : 11 Aug 2022 20:11
Operator : JC\MD
Sample : N4136-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-5

Quant Time: Aug 12 06:10:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 05:09:32 2022
Response via : Initial Calibration




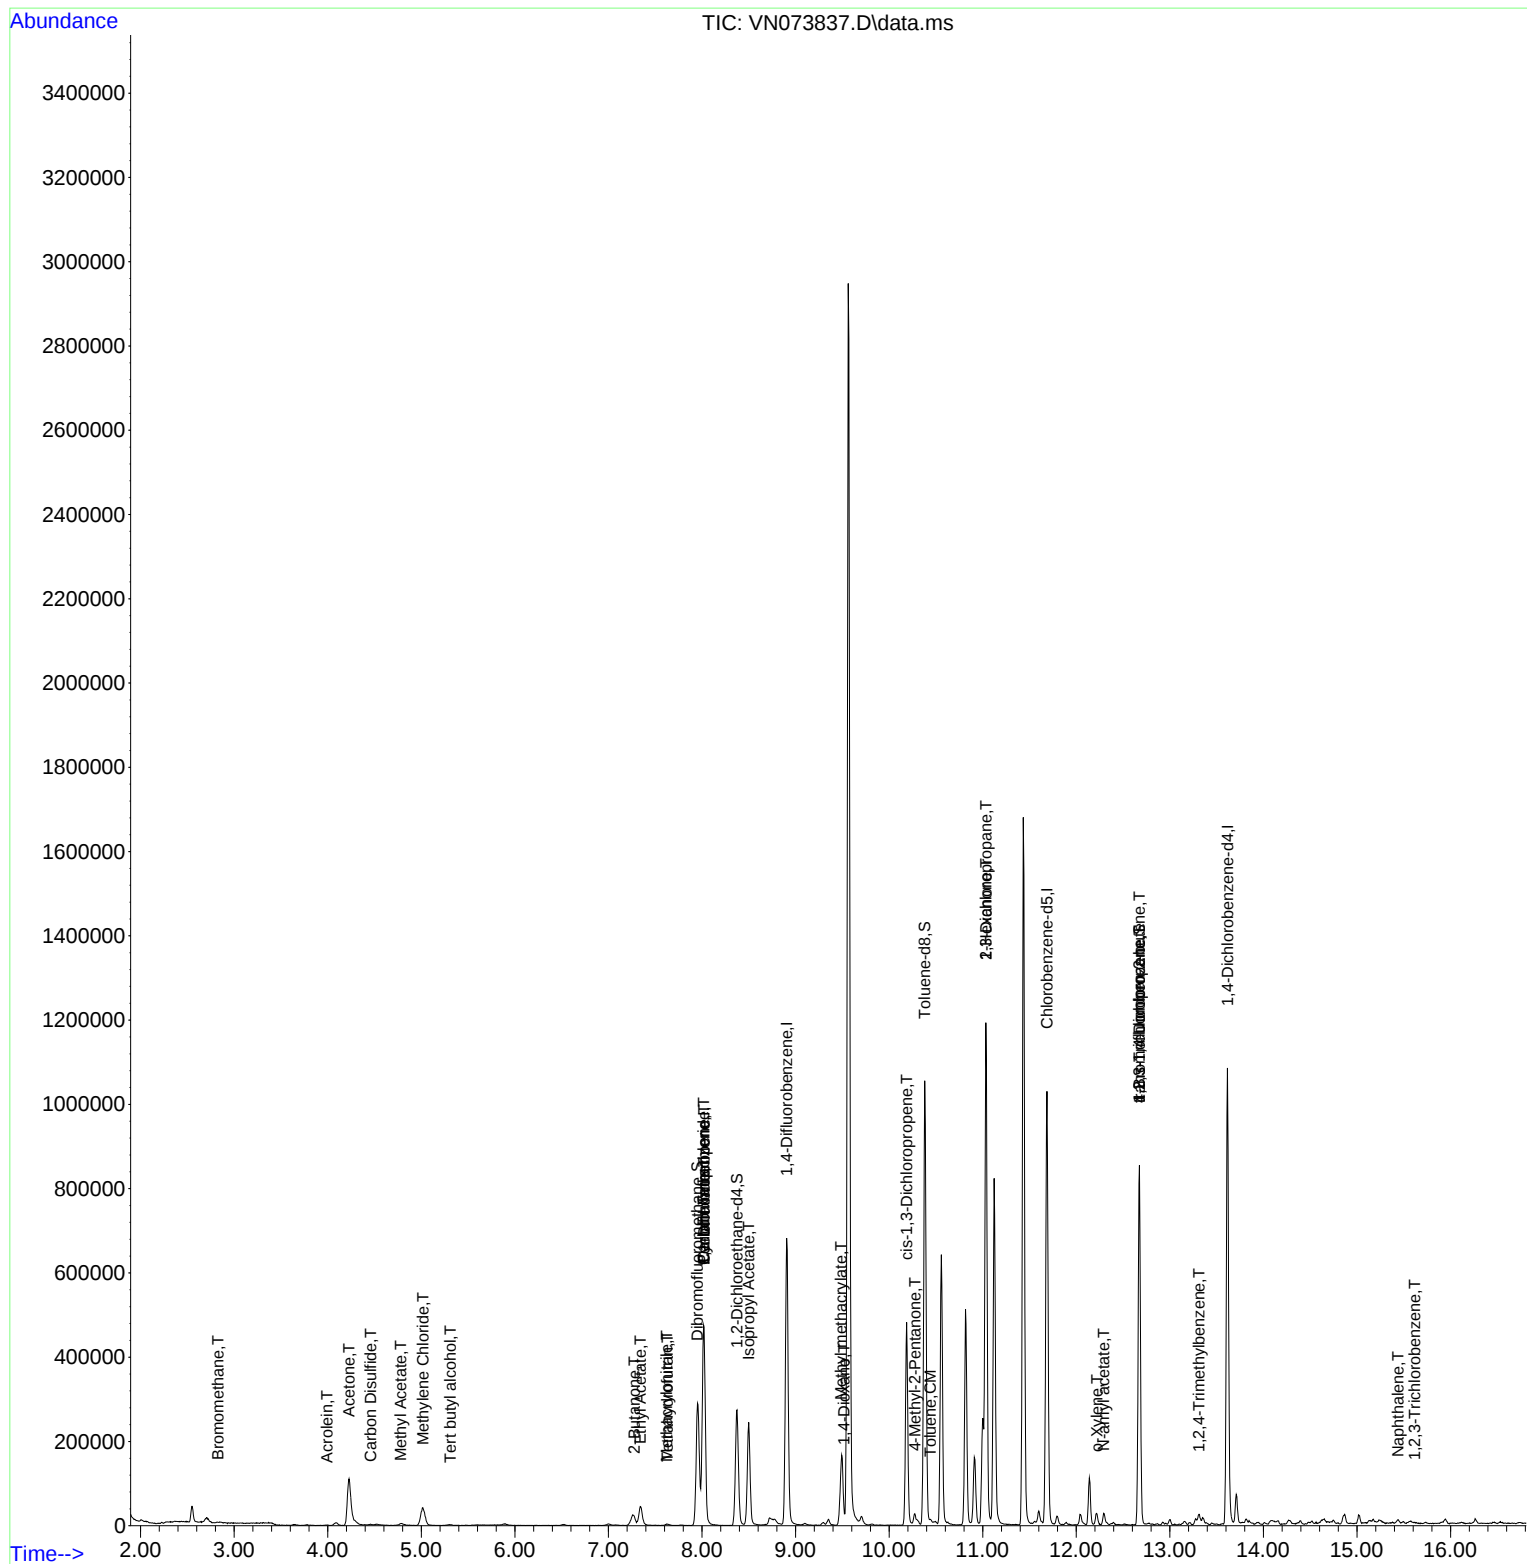




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. 0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion:168 Resp: 395155
Ion Ratio Lower Upper
168 100
99 51.4 42.3 63.5

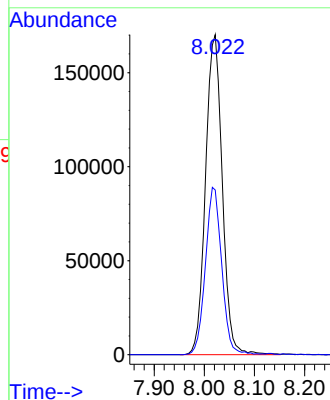

#3
Chloromethane
Concen: Below Cal
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 50 Resp: 993
Ion Ratio Lower Upper
50 100
52 21.4 25.7 38.5#


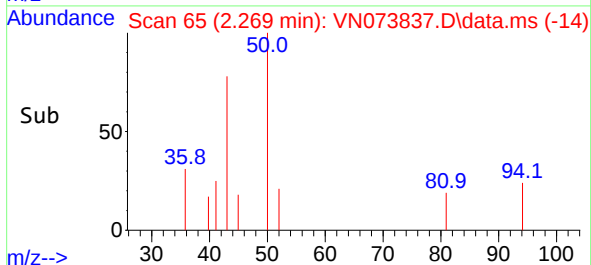
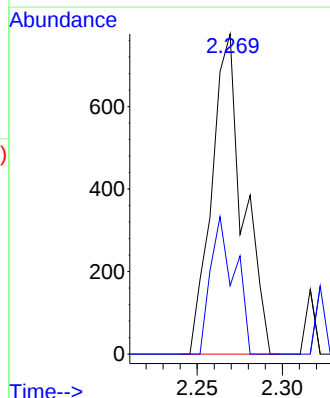
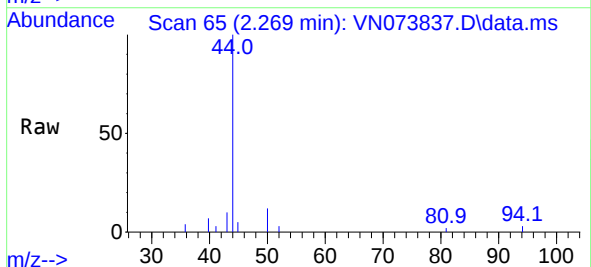




#5
Bromomethane
Concen: 0.438 ug/l
RT: 2.828 min Scan# 1
Delta R.T. 0.041 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 94 Resp: 1701
Ion Ratio Lower Upper
94 100
96 75.5 76.0 114.0#

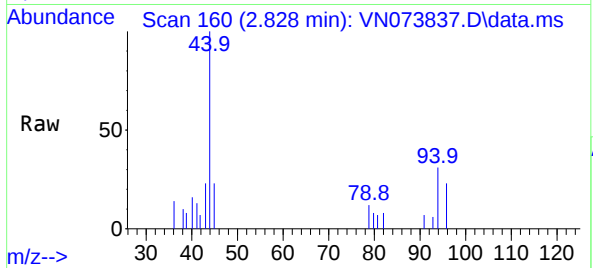

#6
Chloroethane
Concen: Below Cal
RT: 2.957 min Scan# 182
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 64 Resp: 77
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

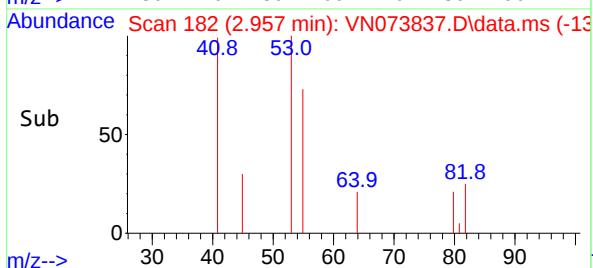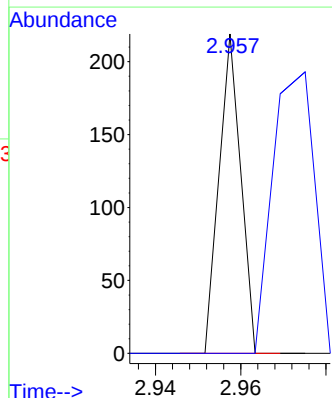



#11

Tert butyl alcohol

Concen: 3.771 ug/l

RT: 5.310 min Scan# 5

Delta R.T. 0.018 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11

Instrument :

MSVOA_N

ClientSampleId :





WC-5

Tgt Ion: 59 Resp: 3916

Ion Ratio Lower Upper

59 100

57 3.2 8.3 12.5#

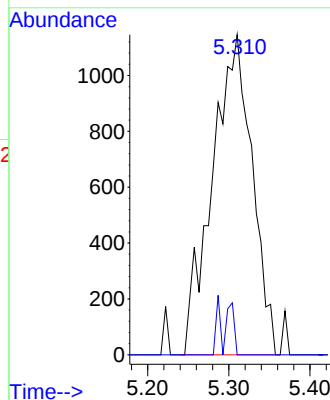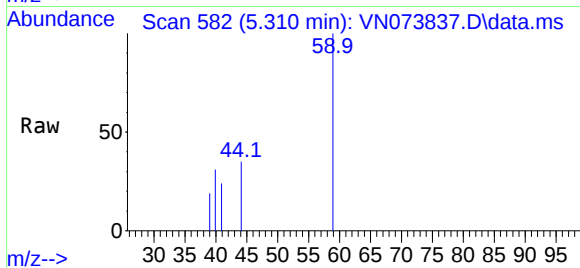

#13

Acrolein

Concen: 0.992 ug/l

RT: 3.993 min Scan# 358

Delta R.T. 0.012 min

Lab File: VN073837.D




Acq: 11 Aug 2022 20:11


Tgt Ion: 56 Resp: 1021

Ion Ratio Lower Upper

56 100

55 77.5 54.8 82.2



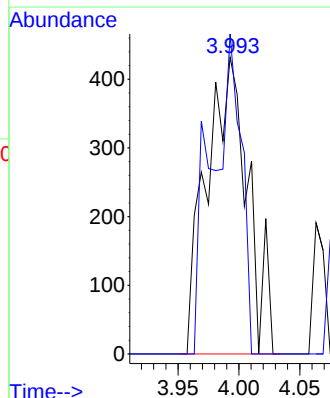
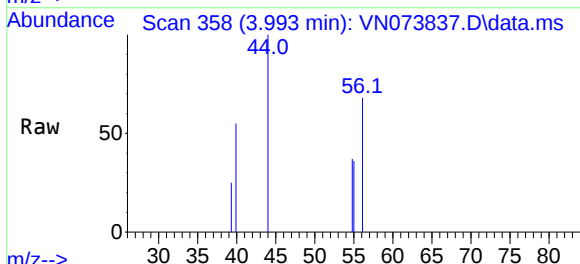




#16
Acetone
Concen: 76.612 ug/l
RT: 4.228 min Scan# 397
Delta R.T. 0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 43 Resp: 198158
Ion Ratio Lower Upper
43 100
58 33.0 26.0 39.0



#17
Carbon Disulfide
Concen: 0.367 ug/l
RT: 4.457 min Scan# 437
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 76 Resp: 3649
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


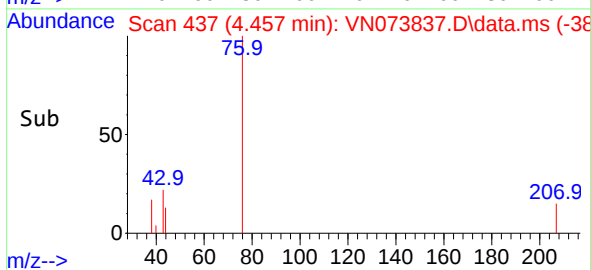






#18
Methyl Acetate
Concen: 1.658 ug/l
RT: 4.781 min Scan# 492
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 43 Resp: 10667
Ion Ratio Lower Upper
43 100
74 20.5 21.6 32.4#



#20
Methylene Chloride
Concen: 6.622 ug/l
RT: 5.016 min Scan# 532
Delta R.T. 0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 84 Resp: 35708
Ion Ratio Lower Upper
84 100
49 115.8 88.3 132.5
51 29.2 28.2 42.2
86 67.6 50.6 76.0

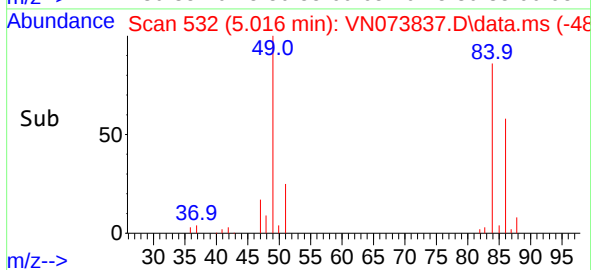



#25

2-Butanone

Concen: 8.713 ug/l

RT: 7.275 min Scan# 913

Delta R.T. 0.018 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11

Instrument :

MSVOA_N

ClientSampleId :





WC-5

Tgt Ion: 43 Resp: 34997

Ion Ratio Lower Upper

43 100

72 25.6 23.7 35.5

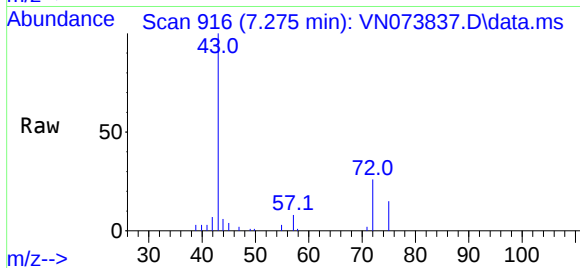

#29

Tetrahydrofuran

Concen: 1.030 ug/l

RT: 7.628 min Scan# 976

Delta R.T. 0.018 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11




Tgt Ion: 42 Resp: 2617


Ion Ratio Lower Upper

42 100

72 39.4 39.7 59.5#

71 17.7 36.6 55.0#


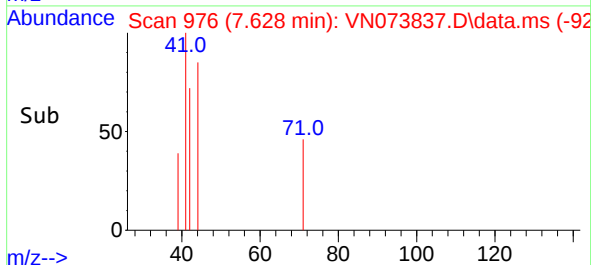
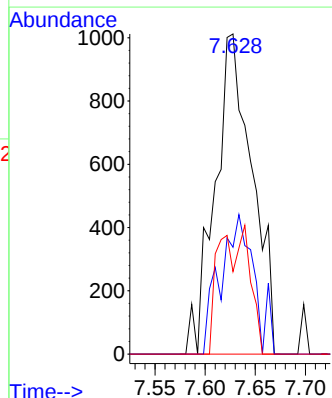
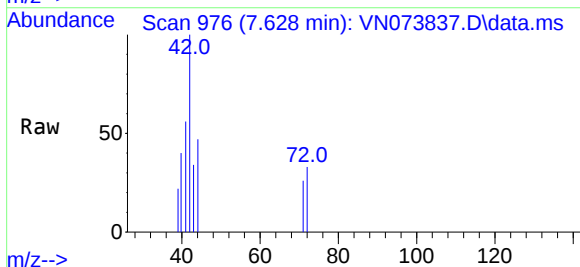




#31
Cyclohexane
Concen: 1.022 ug/l
RT: 8.022 min Scan# 1103
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 56 Resp: 7329
Ion Ratio Lower Upper
56 100
69 157.7 27.8 41.8#
84 138.7 76.9 115.3#

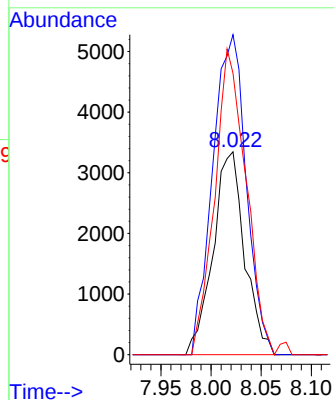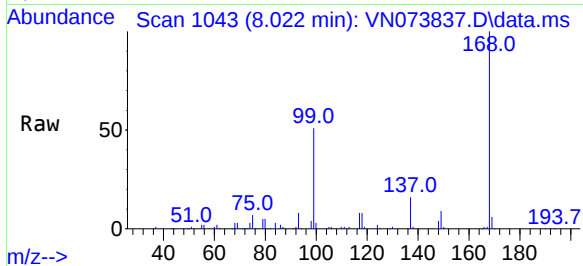

#33
1,2-Dichloroethane-d4
Concen: 47.195 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 65 Resp: 227270
Ion Ratio Lower Upper
65 100
67 53.0 0.0 104.8

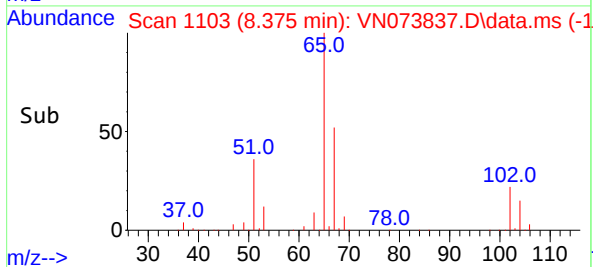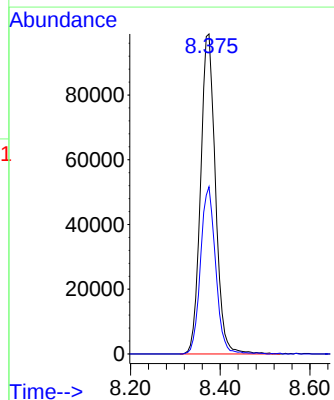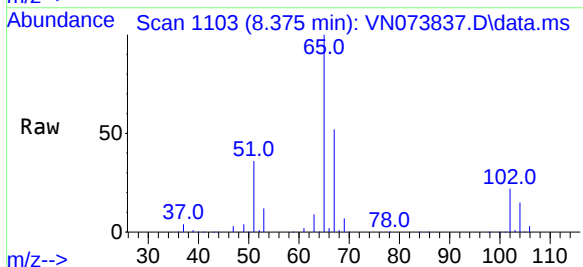



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11

Instrument :

MSVOA_N

ClientSampleId :

WC-5





Tgt Ion:114 Resp: 629978

Ion Ratio Lower Upper

114 100

63 19.1 0.0 40.0

88 14.6 0.0 32.6

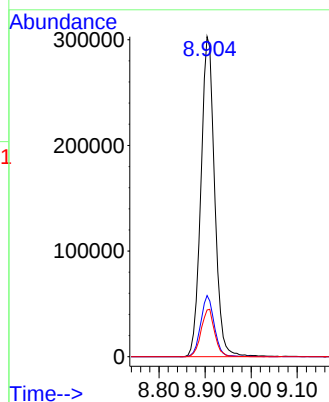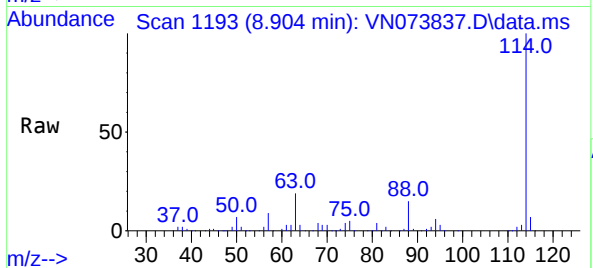

#35

Dibromofluoromethane

Concen: 54.982 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11




Tgt Ion:113 Resp: 217503


Ion Ratio Lower Upper

113 100

111 101.7 81.4 122.0

192 21.5 17.0 25.6


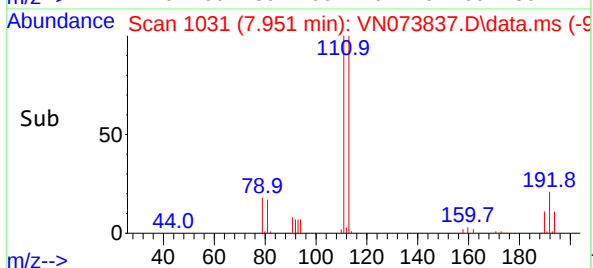
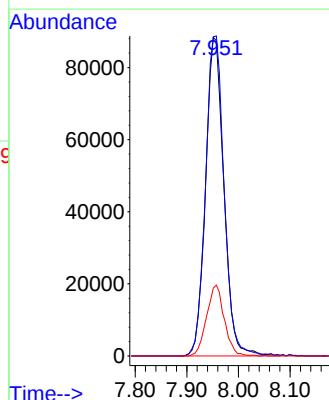





#36
1,1-Dichloropropene
Concen: 4.814 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.129 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 75 Resp: 27144
Ion Ratio Lower Upper
75 100
110 8.8 18.3 54.8#
77 0.0 25.1 37.7#

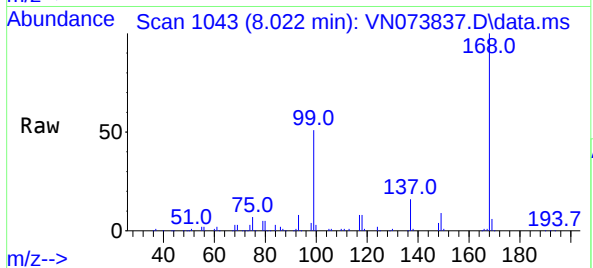

#37
Ethyl Acetate
Concen: 9.366 ug/l
RT: 7.340 min Scan# 927
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 43 Resp: 69542
Ion Ratio Lower Upper
43 100
61 15.5 11.8 17.6
70 11.5 9.3 13.9


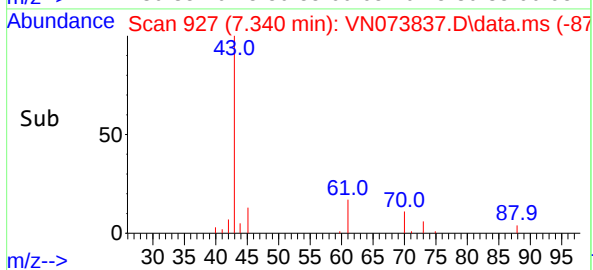






#38
Carbon Tetrachloride
Concen: 6.240 ug/l
RT: 8.016 min Scan# 1
Delta R.T. -0.118 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion:117 Resp: 35734
Ion Ratio Lower Upper
117 100
119 7.1 75.8 113.8#
121 0.0 24.6 37.0#

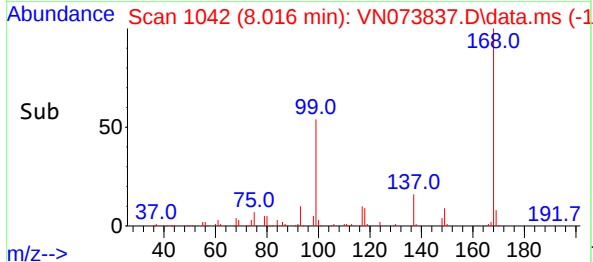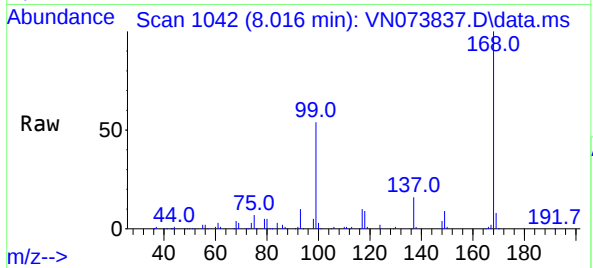

#41
Methacrylonitrile
Concen: 0.506 ug/l
RT: 7.622 min Scan# 975
Delta R.T. 0.059 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 41 Resp: 1699
Ion Ratio Lower Upper
41 100
39 49.7 48.6 73.0
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

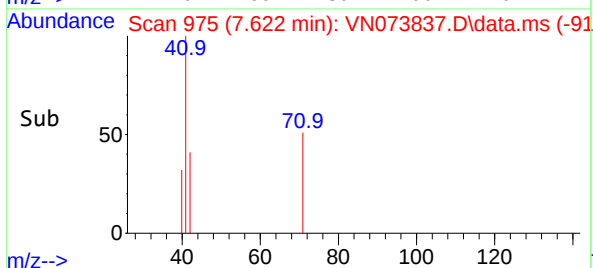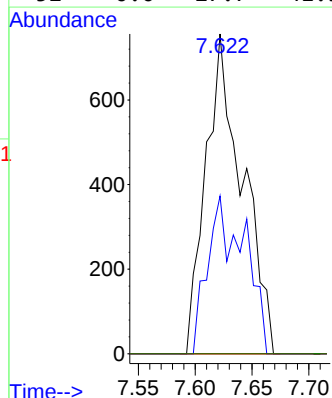



#43

Isopropyl Acetate

Concen: 26.536 ug/l

RT: 8.498 min Scan# 1123

Delta R.T. 0.006 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11

Instrument :

MSVOA_N

ClientSampleId :

WC-5





Tgt Ion: 43 Resp: 266128

Ion Ratio Lower Upper

43 100

61 20.1 21.9 32.9#

87 14.9 12.0 18.0

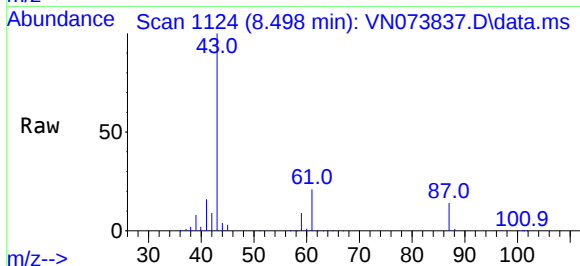

#48

Methyl methacrylate

Concen: 2.670 ug/l

RT: 9.486 min Scan# 1292

Delta R.T. -0.012 min

Lab File: VN073837.D

Acq: 11 Aug 2022 20:11




Tgt Ion: 41 Resp: 11719


Ion Ratio Lower Upper

41 100

69 2.4 74.7 112.1#

39 56.3 45.6 68.4


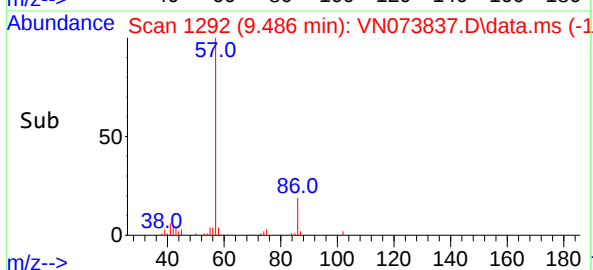

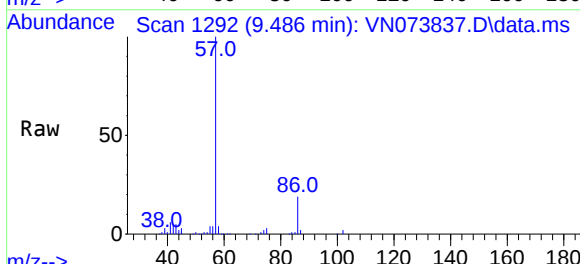




#49
1,4-Dioxane
Concen: 0.485 ug/l
RT: 9.516 min Scan# 1295
Delta R.T. 0.012 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 88 Resp: 60
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 0.0 54.2 81.4#

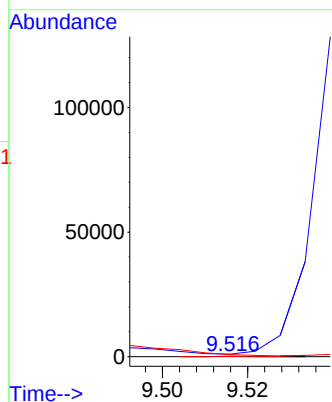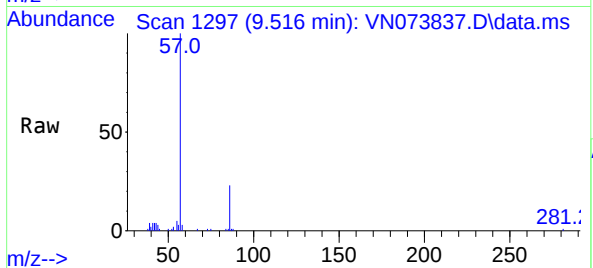

#50
Toluene-d8
Concen: 47.580 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 98 Resp: 740662
Ion Ratio Lower Upper
98 100
100 63.8 52.6 78.8


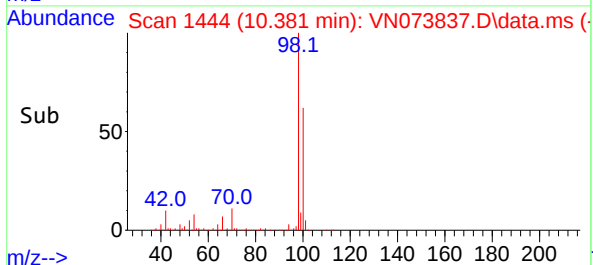

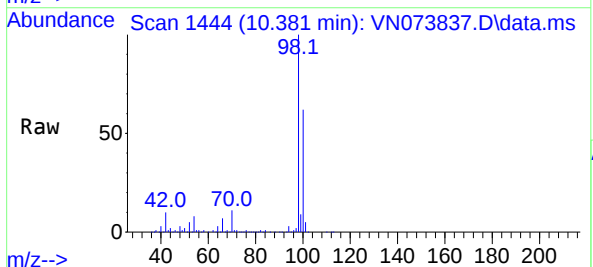




#51
4-Methyl-2-Pentanone
Concen: 3.292 ug/l
RT: 10.275 min Scan# 1426
Delta R.T. -0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 43 Resp: 23680
Ion Ratio Lower Upper
43 100
58 29.8 34.1 51.1#

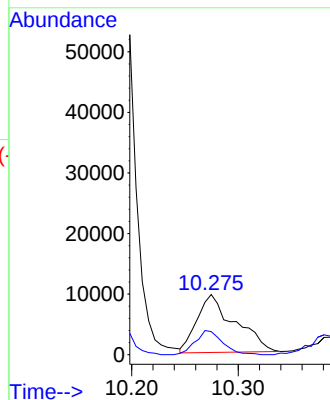

#52
Toluene
Concen: 0.290 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. -0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 92 Resp: 3243
Ion Ratio Lower Upper
92 100
91 196.2 138.6 207.8


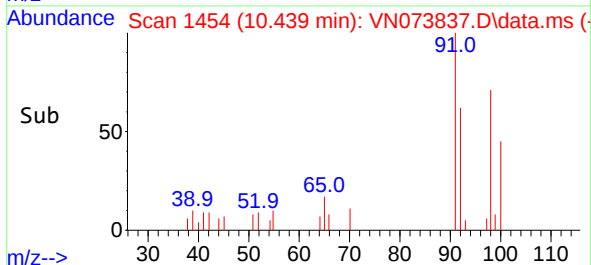
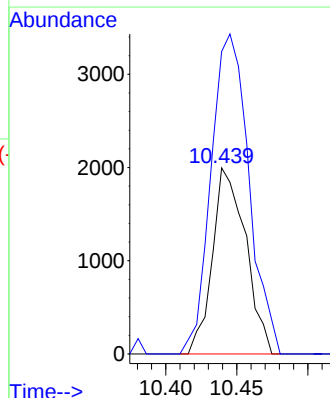
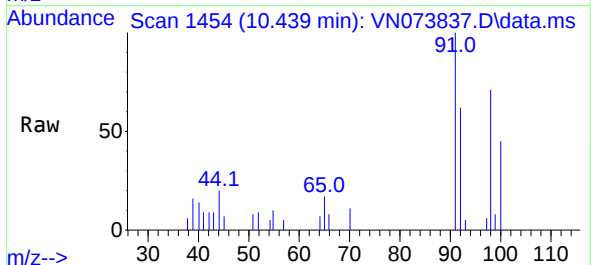




#54
 cis-1,3-Dichloropropene
 Concen: 12.982 ug/l
 RT: 10.186 min Scan# 1411
 Delta R.T. 0.059 min
 Lab File: VN073837.D
 Acq: 11 Aug 2022 20:11




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-5


Tgt Ion: 75 Resp: 88097
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.2 37.8#
 39 30.7 35.7 53.5#

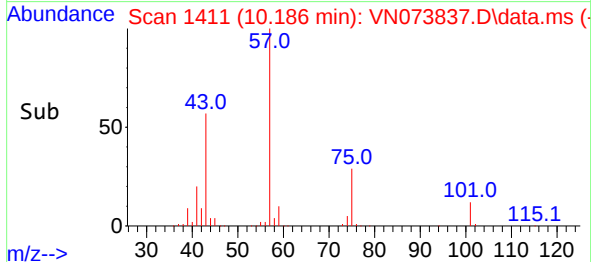

#57
 1,3-Dichloropropane
 Concen: 1.646 ug/l
 RT: 11.033 min Scan# 1555
 Delta R.T. 0.047 min
 Lab File: VN073837.D
 Acq: 11 Aug 2022 20:11

Tgt Ion: 76 Resp: 13025
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.2#



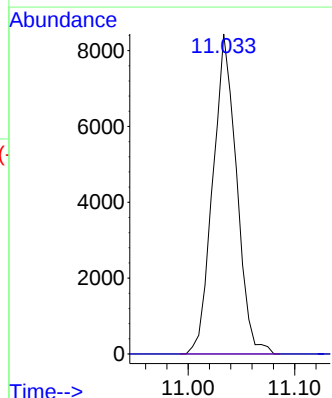



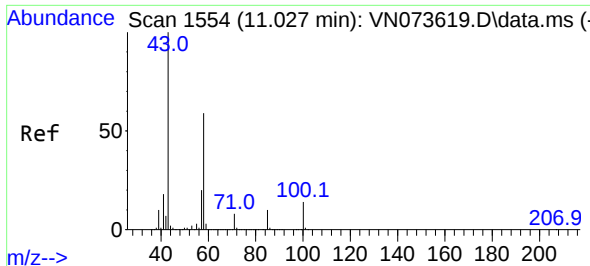

#59
2-Hexanone
Concen: 30.666 ug/l
RT: 11.033 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 43 Resp: 167124
Ion Ratio Lower Upper
43 100
58 22.7 29.7 89.1#

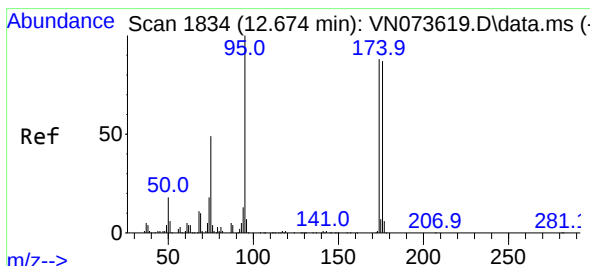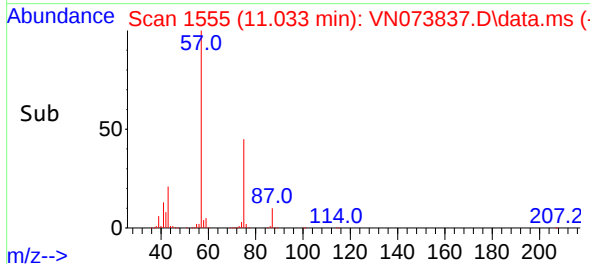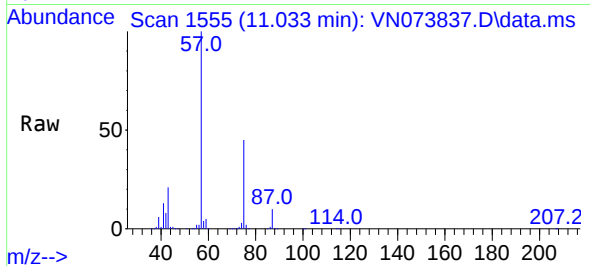

#62
4-Bromofluorobenzene
Concen: 51.680 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 95 Resp: 282949
Ion Ratio Lower Upper
95 100
174 91.8 0.0 167.6
176 87.4 0.0 163.4


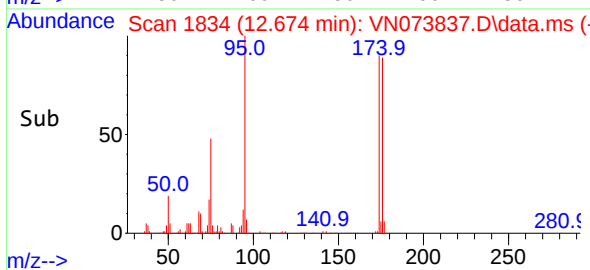

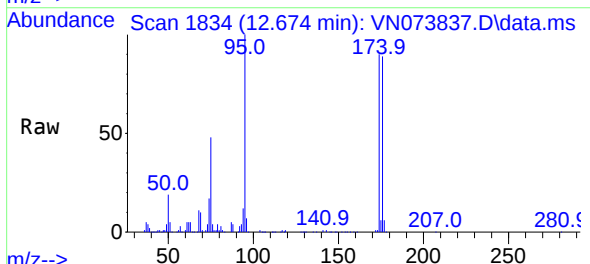




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion:117 Resp: 627250
Ion Ratio Lower Upper
117 100
82 53.3 44.2 66.2
119 33.4 25.4 38.0

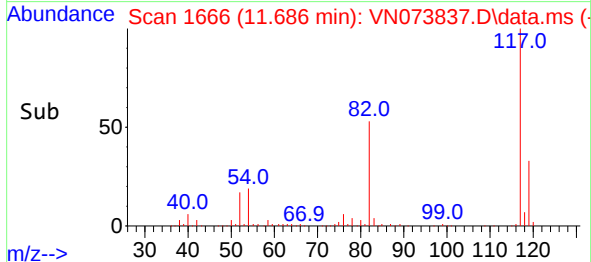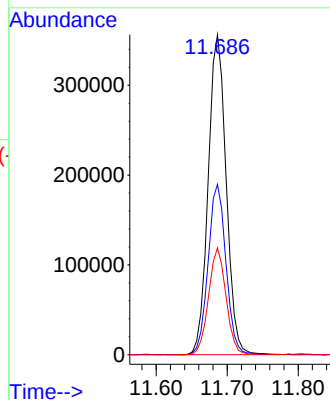

#69
o-Xylene
Concen: 0.207 ug/l
RT: 12.222 min Scan# 1757
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11


Tgt Ion:106 Resp: 1730
Ion Ratio Lower Upper
106 100
91 202.6 106.0 318.0

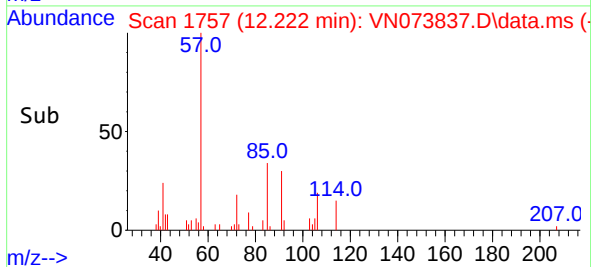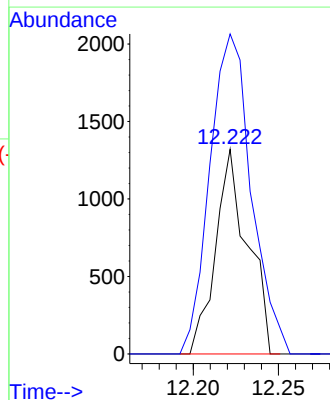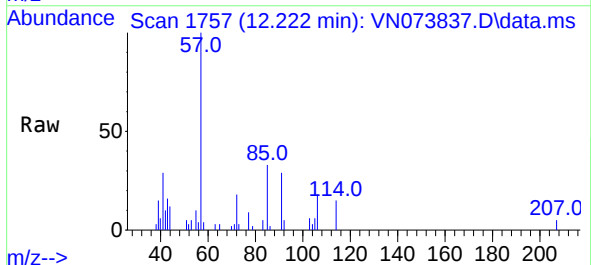



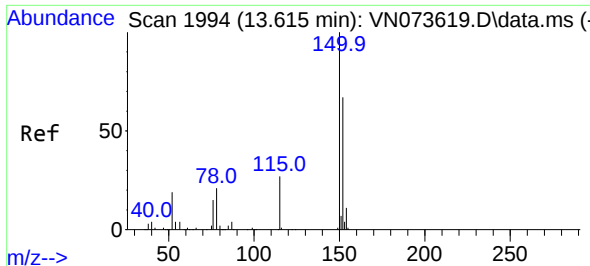


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Instrument :
MSVOA_N
ClientSampleId :
WC-5



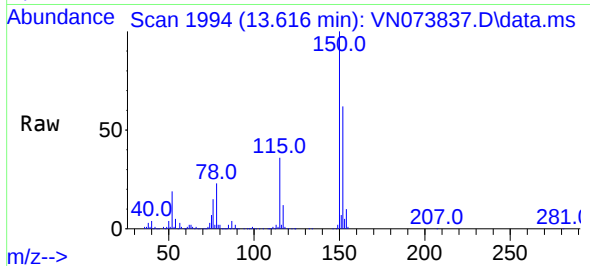



Tgt Ion:152 Resp: 309143
Ion Ratio Lower Upper
152 100
115 55.6 28.9 86.7
150 156.3 0.0 356.2

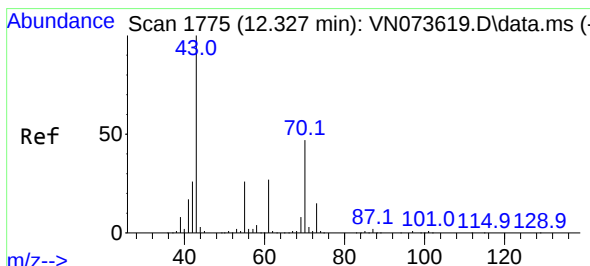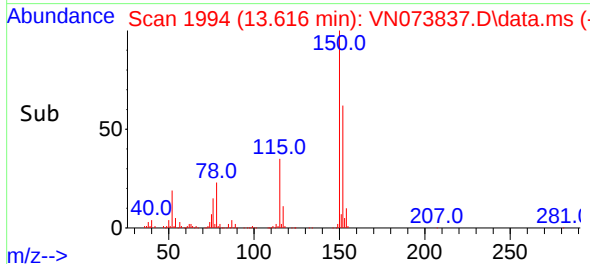

#74
N-ethyl acetate
Concen: 2.075 ug/l
RT: 12.292 min Scan# 1769
Delta R.T. -0.035 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 43 Resp: 17741
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 12.1 21.1 31.7#
61 0.0 21.1 31.7#


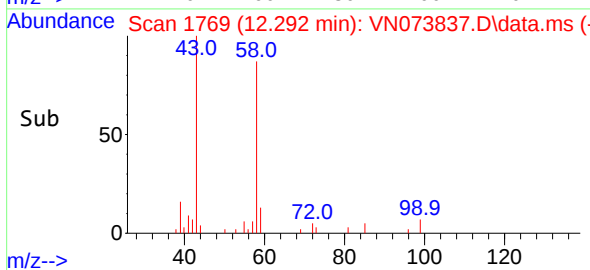

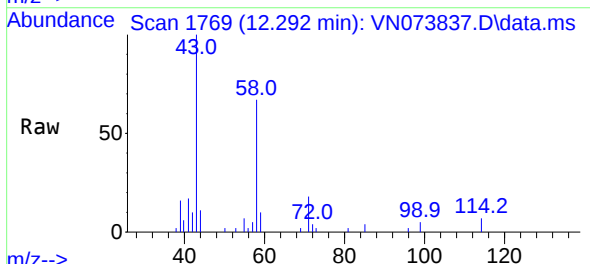




#76
1,2,3-Trichloropropane
Concen: 23.288 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion: 75 Resp: 141642
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#



#81
trans-1,4-Dichloro-2-butene
Concen: 59.377 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.106 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11

Tgt Ion: 75 Resp: 141642
Ion Ratio Lower Upper
75 100
53 0.2 78.0 117.0#
89 0.0 37.2 55.8#



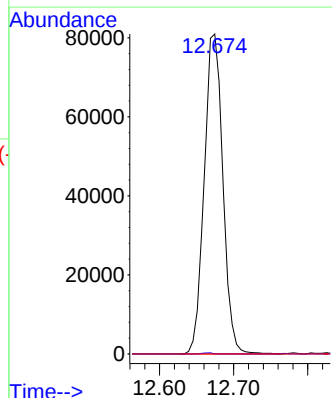





#84
1,2,4-Trimethylbenzene
Concen: 0.611 ug/l
RT: 13.310 min Scan# 1942
Delta R.T. 0.000 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11




Instrument :
MSVOA_N
ClientSampleId :
WC-5


Tgt Ion:105 Resp: 11187
Ion Ratio Lower Upper
105 100
120 42.3 23.3 69.8

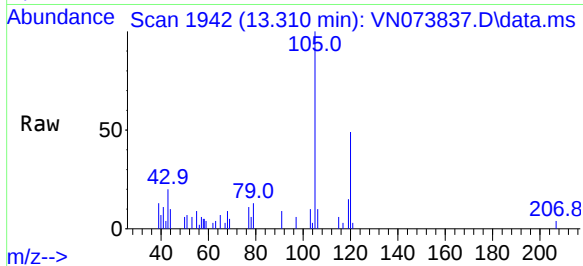

#95
Naphthalene
Concen: 0.583 ug/l
RT: 15.439 min Scan# 2304
Delta R.T. 0.006 min
Lab File: VN073837.D
Acq: 11 Aug 2022 20:11


Tgt Ion:128 Resp: 10247
Ion Ratio Lower Upper
128 100
127 14.3 10.3 15.5
129 8.6 8.6 13.0#

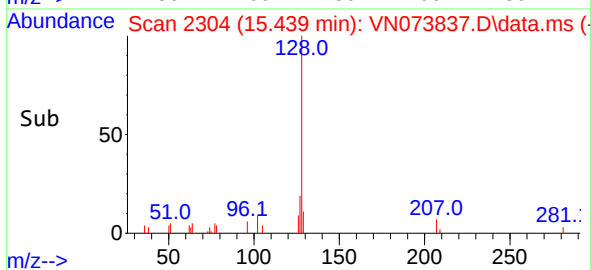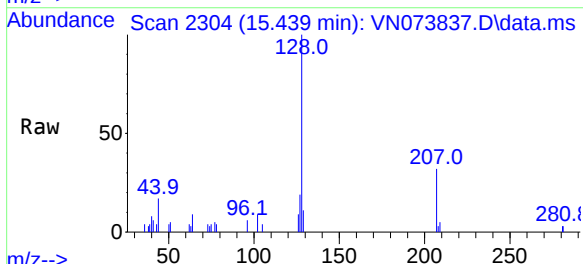



#96
 1,2,3-Trichlorobenzene
 Concen: 0.210 ug/l
 RT: 15.615 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: VN073837.D
 Acq: 11 Aug 2022 20:11

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-5

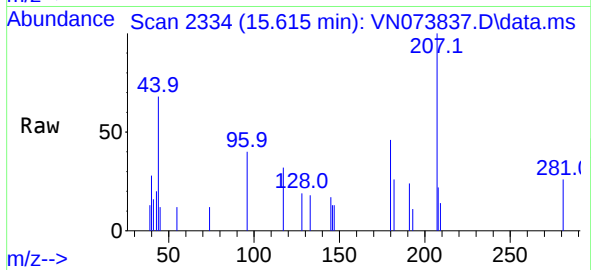

Tgt Ion:	180	Resp:	1197
Ion	Ratio	Lower	Upper
180	100		
182	0.0	47.8	143.3#
145	48.8	15.5	46.5#

