
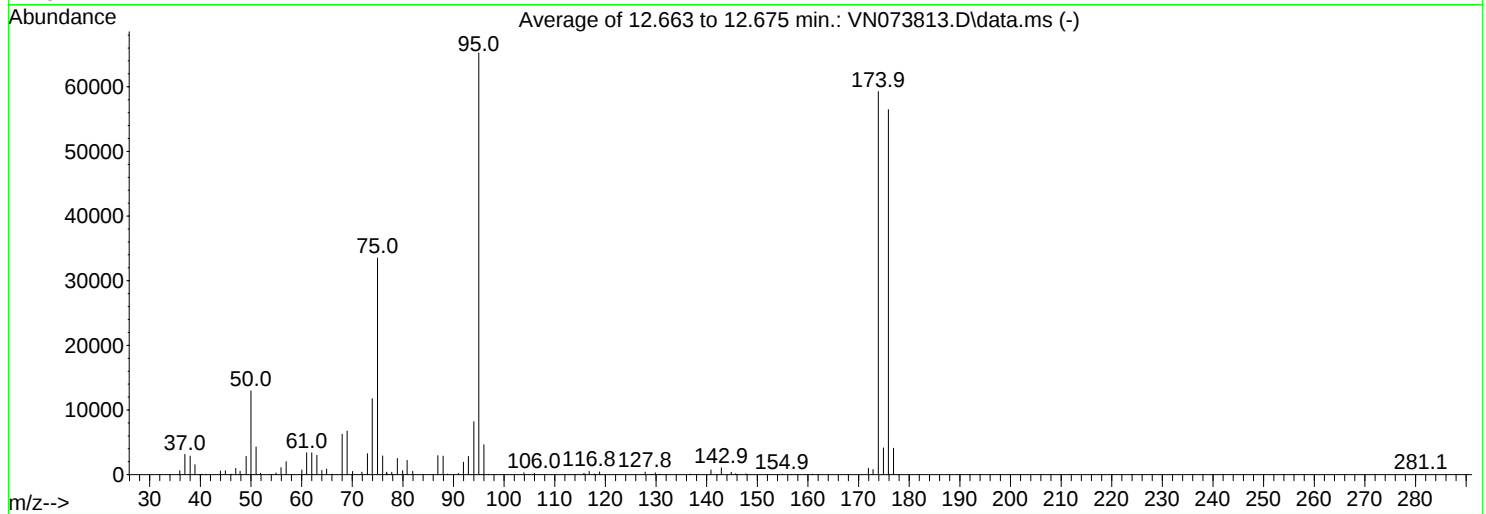


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081122\
 Data File : VN073813.D
 Acq On : 11 Aug 2022 09:28
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Title : SW846 8260
 Last Update : Wed Aug 10 05:09:32 2022

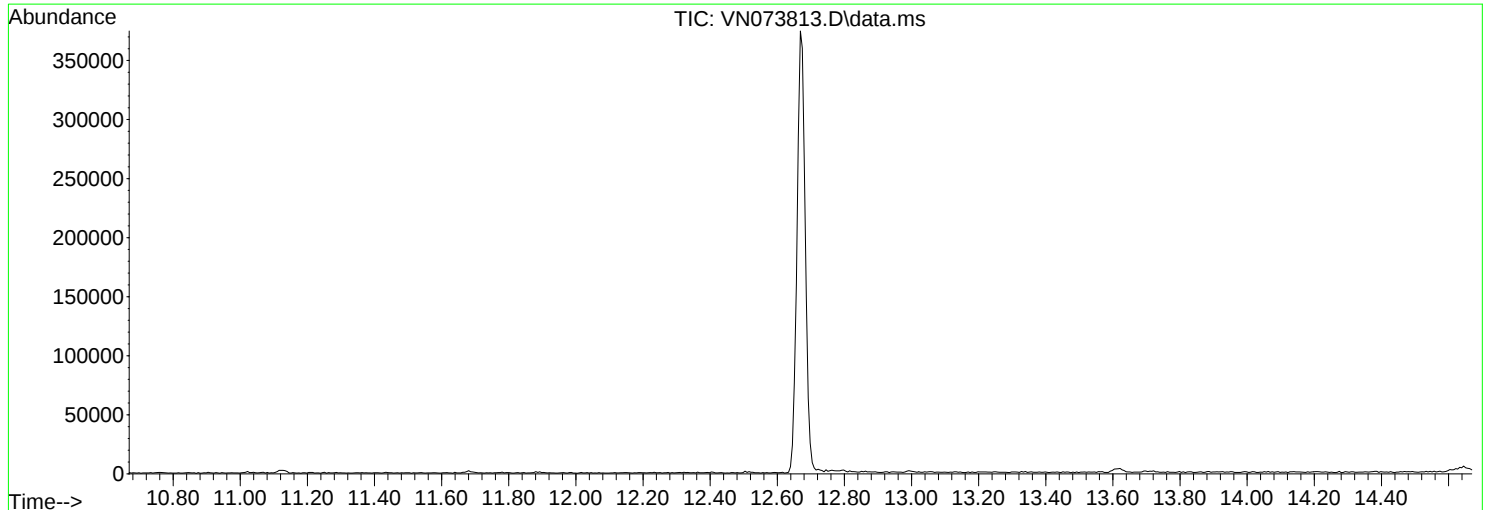

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	12963	PASS
75	95	30	60	51.4	33528	PASS
95	95	100	100	100.0	65256	PASS
96	95	5	9	7.1	4638	PASS
173	174	0.00	2	1.4	807	PASS
174	95	50	100	90.8	59251	PASS
175	174	5	9	7.0	4139	PASS
176	174	95	101	95.3	56453	PASS
177	176	5	9	7.2	4076	PASS