


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081123\
Data File : VN078852.D
Acq On : 11 Aug 2023 08:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 09 05:05:47 2023

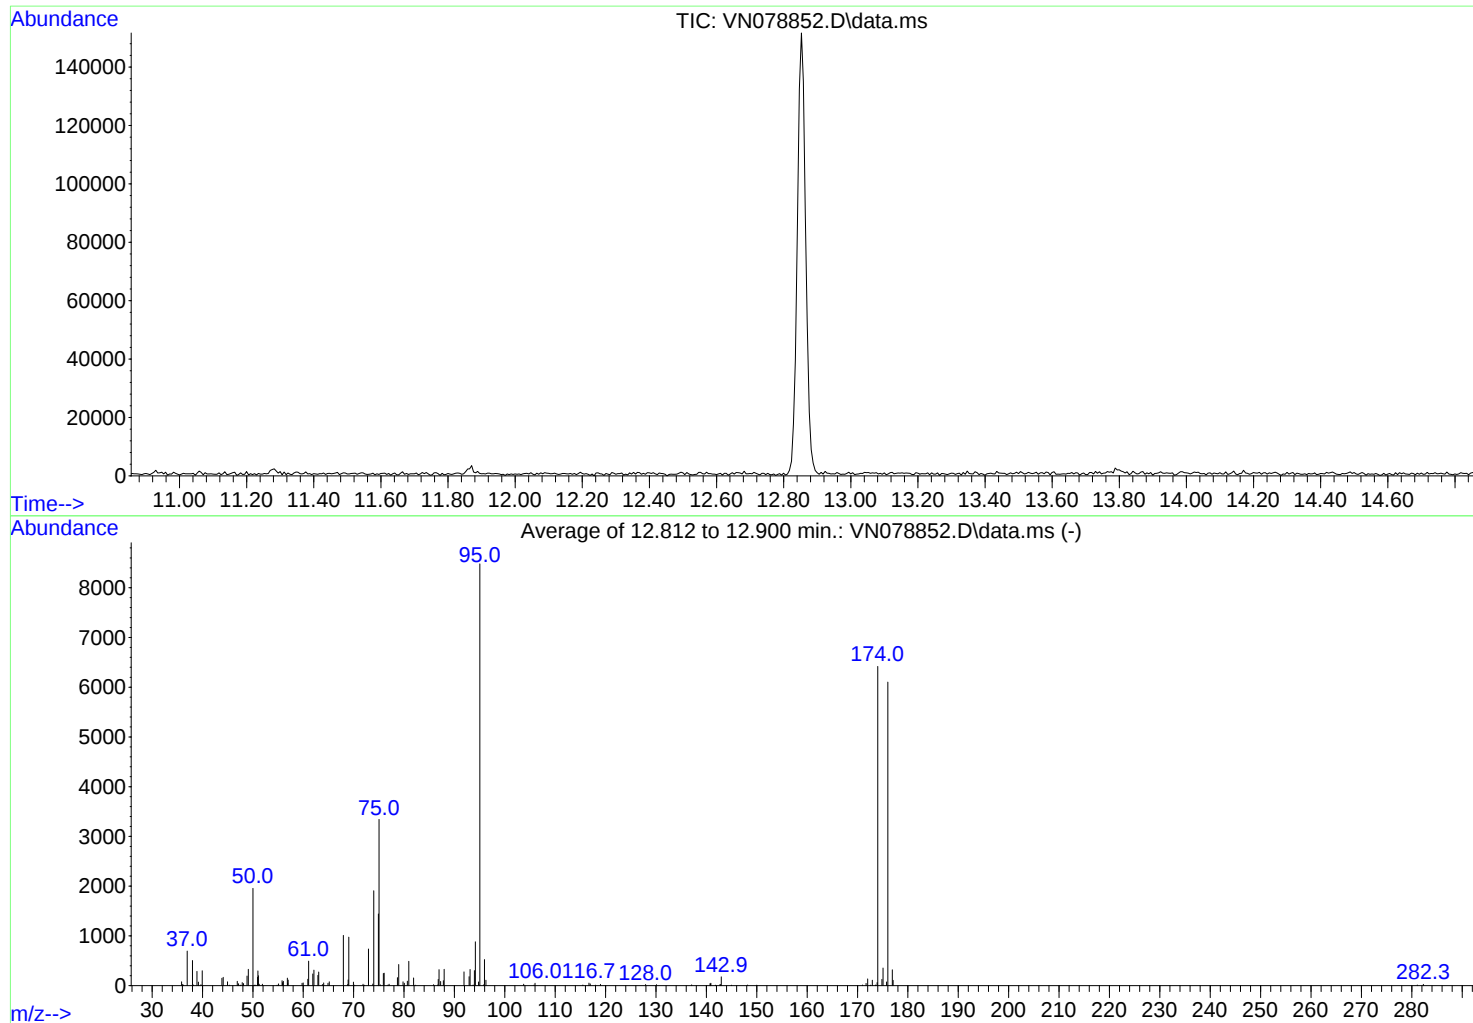

AutoFind: Averaged scan 1846 to 1861; Bkg corrected with scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	1957	PASS
75	95	30	60	39.4	3341	PASS
95	95	100	100	100.0	8480	PASS
96	95	5	9	6.2	523	PASS
173	174	0.00	2	1.7	111	PASS
174	95	50	100	75.7	6419	PASS
175	174	5	9	5.5	354	PASS
176	174	95	101	95.0	6101	PASS
177	176	5	9	5.2	318	PASS