

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081219\
 Data File : VN057225.D
 Acq On : 12 Aug 2019 19:16
 Operator : JC/SP
 Sample : K4229-24
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 2S-C4-(0)

Quant Time: Aug 13 01:47:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:49:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	1327585	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.01	114	1846797	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.91	117	1563675	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.88	152	390532	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.44	65	622839	45.62	ug/l	0.00
Spiked Amount			Recovery	=	91.24%	
35) Dibromofluoromethane	6.99	113	570489	49.23	ug/l	0.00
Spiked Amount			Recovery	=	98.46%	
50) Toluene-d8	9.56	98	2160669	48.73	ug/l	0.00
Spiked Amount			Recovery	=	97.46%	
62) 4-Bromofluorobenzene	11.92	95	559731	39.18	ug/l	0.00
Spiked Amount			Recovery	=	78.36%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.23	59	523	0.269	ug/l #	73
16) Acetone	3.48	43	29948	7.263	ug/l #	82
18) Methyl Acetate	3.90	43	24341	1.342	ug/l	99
20) Methylene Chloride	4.10	84	19985	1.469	ug/l	88
25) 2-Butanone	6.22	43	1509	0.240	ug/l	99
31) Cyclohexane	7.05	56	19545	0.987	ug/l #	1
36) 1,1-Dichloropropene	7.06	75	80159	5.272	ug/l #	48
38) Carbon Tetrachloride	7.05	117	112909	7.125	ug/l #	17
43) Isopropyl Acetate	7.57	43	128837	6.023	ug/l #	87
45) 1,2-Dichloropropane	8.70	63	2688	0.216	ug/l #	43
48) Methyl methacrylate	8.63	41	7399	0.734	ug/l #	10
51) 4-Methyl-2-Pentanone	9.45	43	9514	0.764	ug/l	99
54) cis-1,3-Dichloropropene	9.36	75	63017	3.400	ug/l #	64
57) 1,3-Dichloropropane	10.25	76	10105	0.522	ug/l #	42
59) 2-Hexanone	10.25	43	120621	14.316	ug/l #	51
71) Bromoform	11.92	173	2364	0.274	ug/l #	1
73) Isopropylbenzene	11.77	105	392	Below Cal	#	48
74) N-amyl acetate	11.54	43	2539	0.257	ug/l #	40
76) 1,2,3-Trichloropropane	11.92	75	265210	33.835	ug/l #	100
79) 2-Chlorotoluene	12.19	91	63	Below Cal	#	39
81) trans-1,4-Dichloro-2-buten	11.92	75	265210	99.851	ug/l #	14
83) tert-Butylbenzene	12.60	119	30	Below Cal	#	28
90) Hexachloroethane	13.63	117	32	Below Cal	#	1
95) Naphthalene	14.67	128	460	2.848	ug/l #	77
96) 1,2,3-Trichlorobenzene	14.84	180	121	5.739	ug/l #	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN081219\
Data File : VN057225.D
Acq On : 12 Aug 2019 19:16
Operator : JC/SP
Sample : K4229-24
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
2S-C4-(0)

Quant Time: Aug 13 01:47:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:49:25 2019
Response via : Initial Calibration

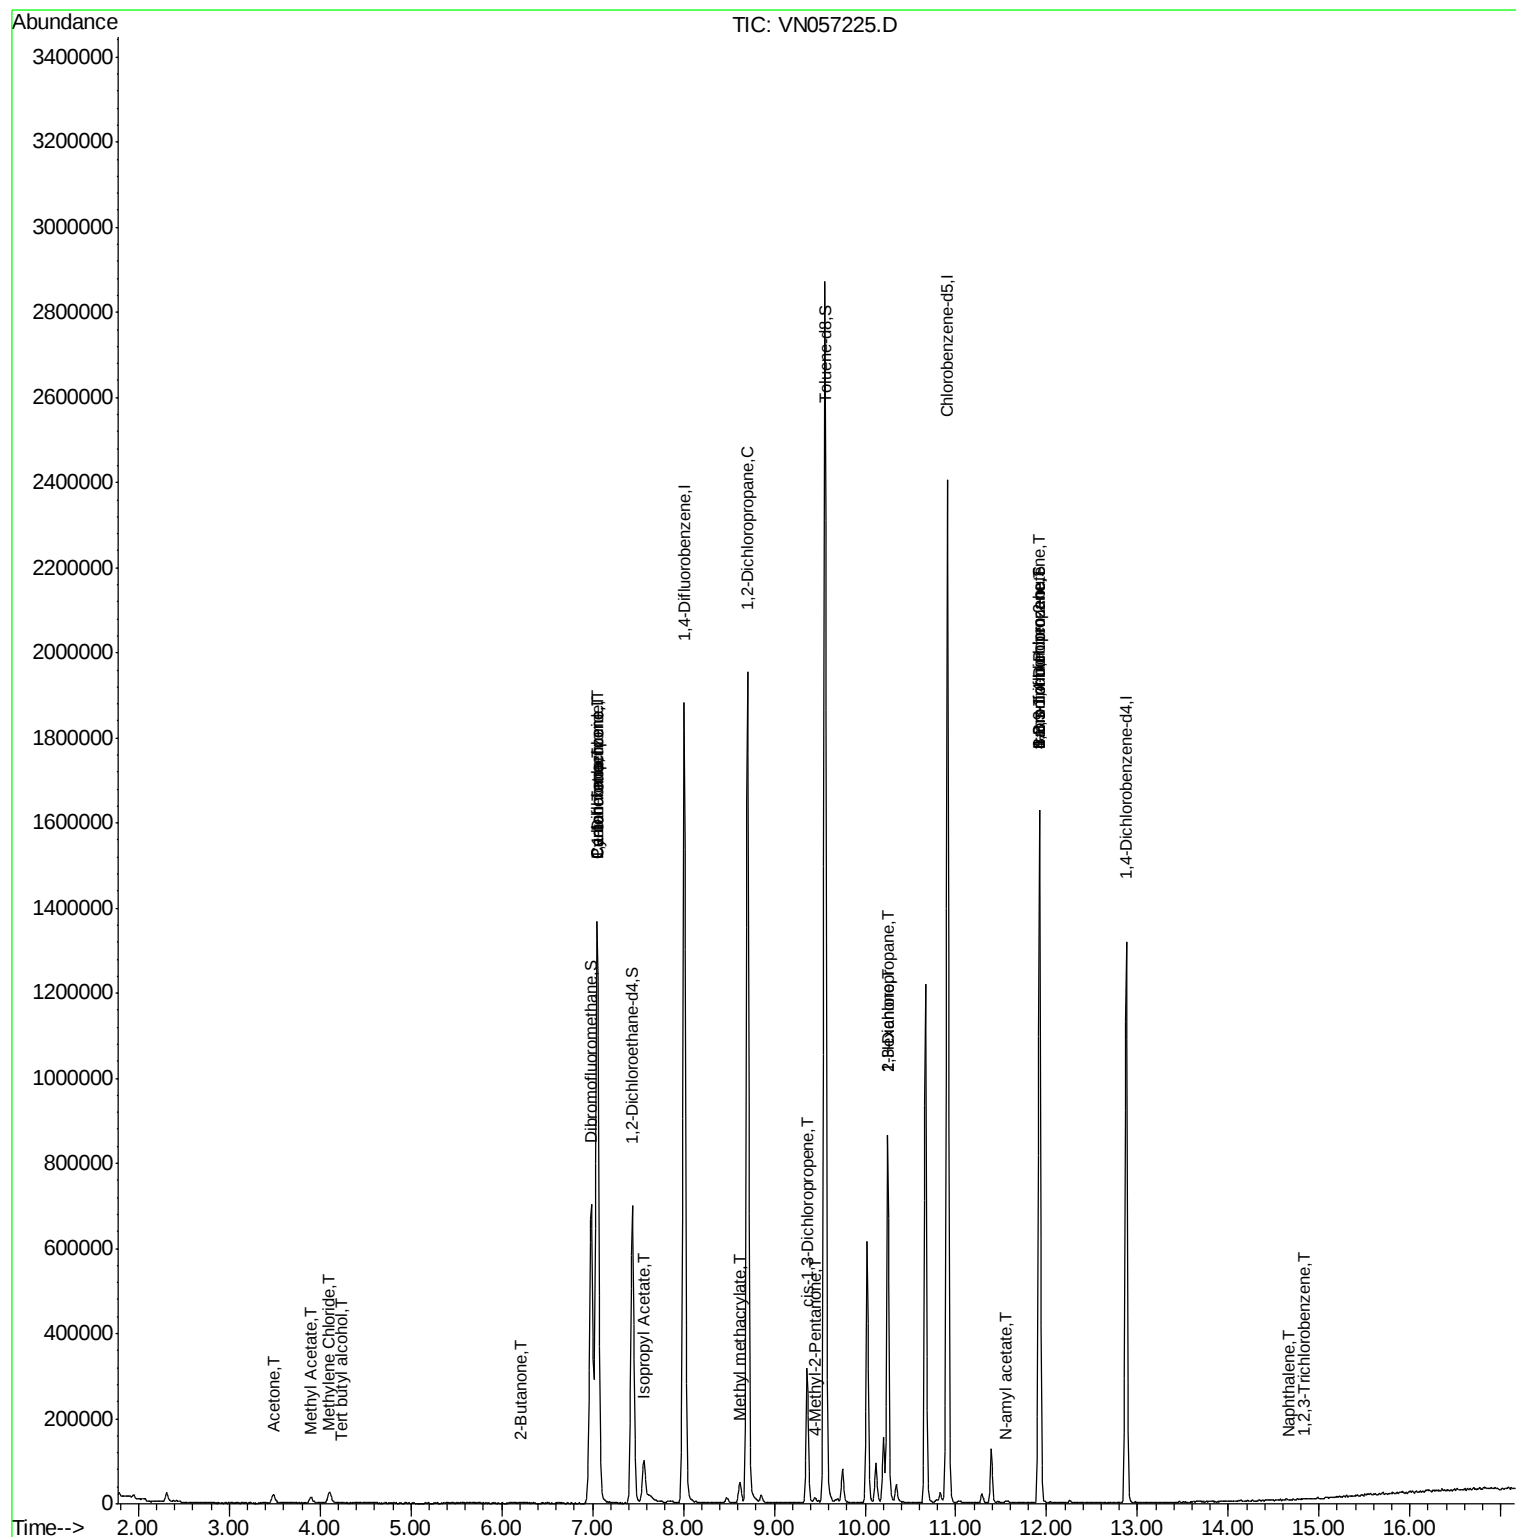



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 1642

Delta R.T. 0.00 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :


2S-C4-(0)

Tgt Ion:168 Resp: 1327585

Ion Ratio Lower Upper

168 100

99 47.2 38.6 57.8



Abundance Ion 167.90 (167.60 to 168.60): VN057115.D (-1620) (-)

Ion 98.90 (98.60 to 99.60): VN057115.D (-1620) (-)

7.05

600000

500000

400000



300000

200000

100000

0

Time-->



#11

Tert butyl alcohol

Concen: 0.269 ug/l

RT: 4.23 min Scan# 764

Delta R.T. -0.00 min

Lab File: VN057225.D


Acq: 12 Aug 2019 19:16

Tgt Ion: 59 Resp: 523

Ion Ratio Lower Upper

59 100

57 0.0 7.9 11.9#



Abundance Ion 59.00 (58.70 to 59.70): VN057115.D (-739) (-)

Ion 57.00 (56.70 to 57.70): VN057115.D (-739) (-)

4.23

500

400


300


200

100

0

Time-->



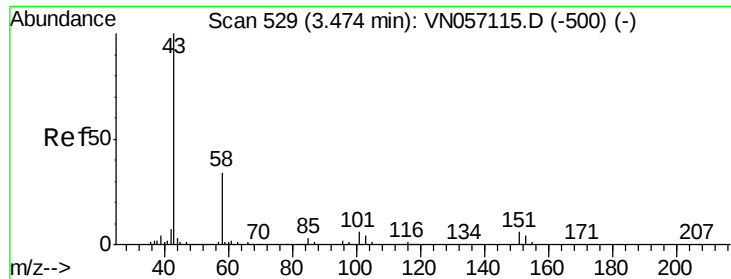

#16

Acetone

Concen: 7.263 ug/l

RT: 3.48 min Scan# 532

Delta R.T. 0.01 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :





2S-C4-(0)

Tgt Ion: 43 Resp: 29948

Ion Ratio Lower Upper

43 100

58 23.8 27.4 41.2#

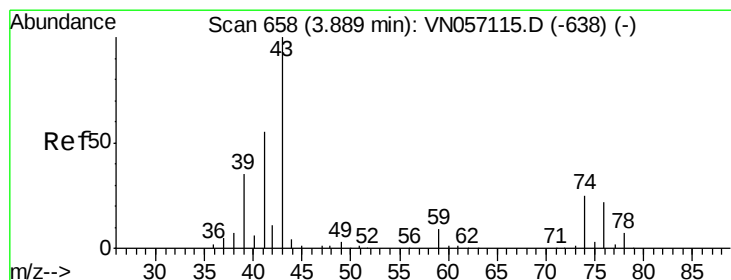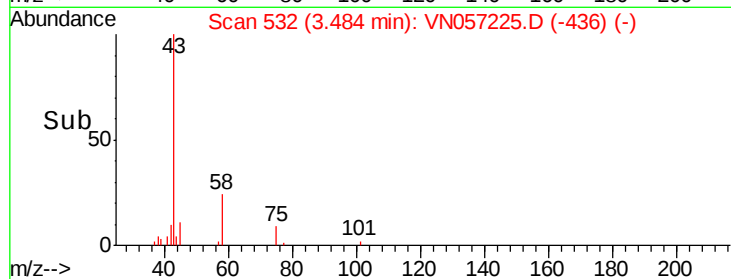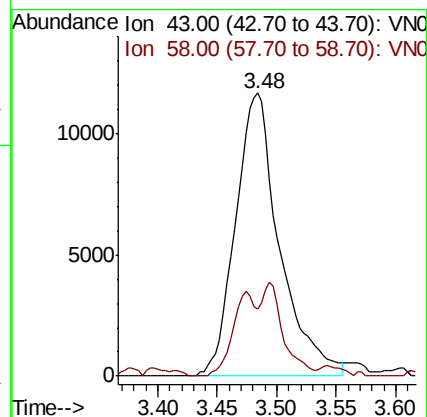

#18

Methyl Acetate

Concen: 1.342 ug/l

RT: 3.90 min Scan# 660

Delta R.T. 0.01 min

Lab File: VN057225.D




Acq: 12 Aug 2019 19:16


Tgt Ion: 43 Resp: 24341

Ion Ratio Lower Upper

43 100

74 24.6 20.2 30.4


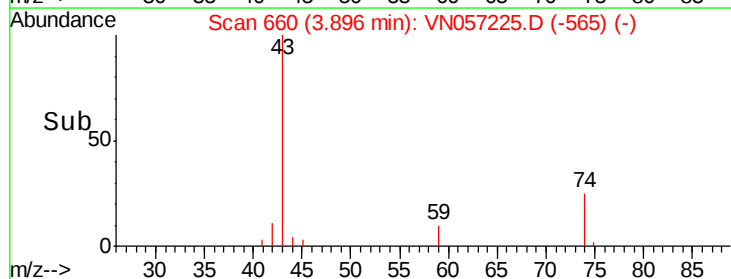
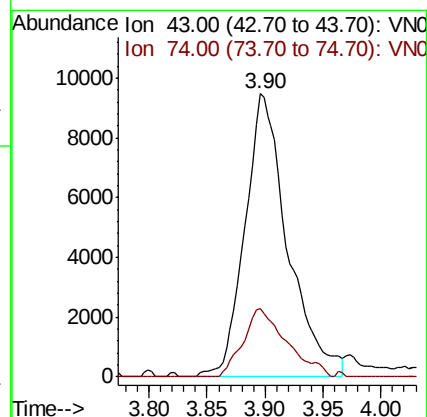
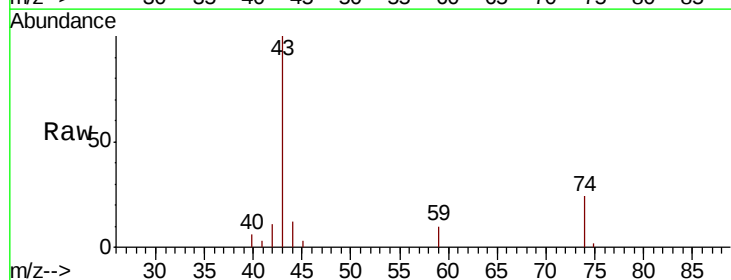




#20
Methylene Chloride
Concen: 1.469 ug/l
RT: 4.10 min Scan# 725
Delta R.T. 0.01 min
Lab File: VN057225.D
Acq: 12 Aug 2019 19:16




Instrument :
MSVOA_N
ClientSampled :
2S-C4-(0)


Tgt Ion: 84 Resp: 19985
Ion Ratio Lower Upper
84 100
49 91.7 89.5 134.3
51 28.9 27.2 40.8
86 62.9 50.6 75.8

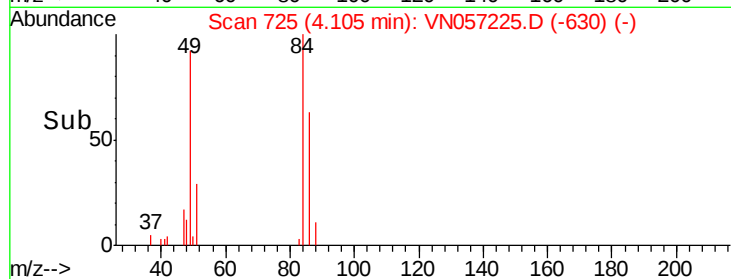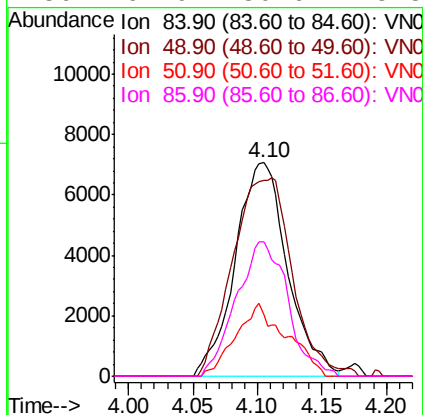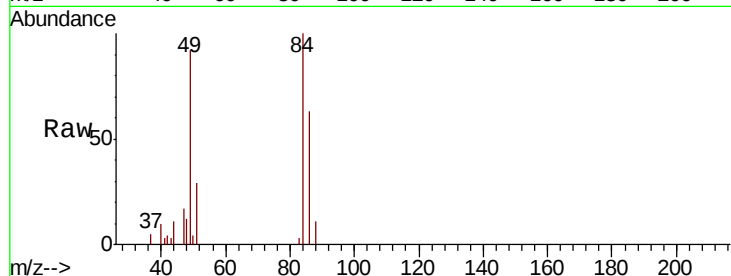

#25
2-Butanone
Concen: 0.240 ug/l
RT: 6.22 min Scan# 1382
Delta R.T. 0.02 min
Lab File: VN057225.D
Acq: 12 Aug 2019 19:16

Tgt Ion: 43 Resp: 1509
Ion Ratio Lower Upper
43 100
72 27.0 22.2 33.4

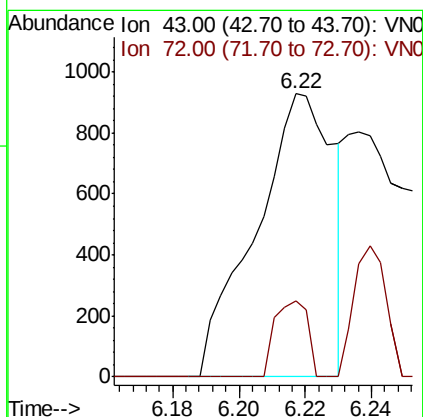


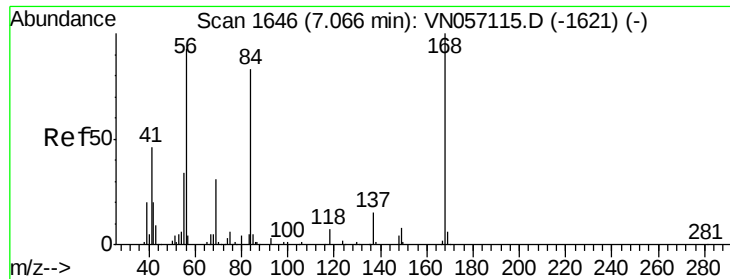




#31
Cyclohexane
Concen: 0.987 ug/l
RT: 7.05 min Scan# 1642
Delta R.T. -0.01 min
Lab File: VN057225.D
Acq: 12 Aug 2019 19:16

Instrument :
MSVOA_N
ClientSampleId :
2S-C4-(0)

Tgt Ion: 56 Resp: 19545
Ion Ratio Lower Upper
56 100
69 214.8 26.9 40.3#
84 163.9 71.9 107.9#




Abundance Ion 56.00 (55.70 to 56.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 84.00 (83.70 to 84.70): VNC

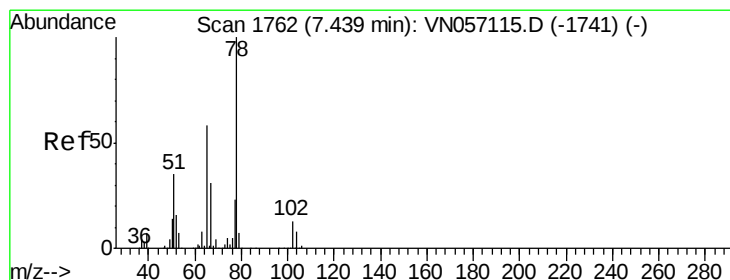
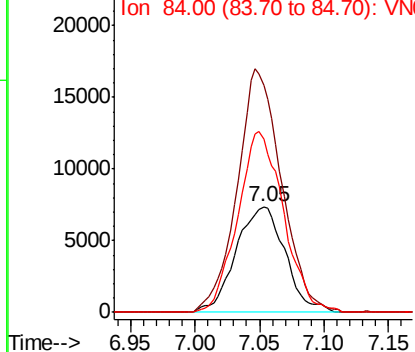



#33
1,2-Dichloroethane-d4
Concen: 45.618 ug/l
RT: 7.44 min Scan# 1762
Delta R.T. -0.00 min
Lab File: VN057225.D
Acq: 12 Aug 2019 19:16

Tgt Ion: 65 Resp: 622839
Ion Ratio Lower Upper
65 100
67 54.1 0.0 108.2

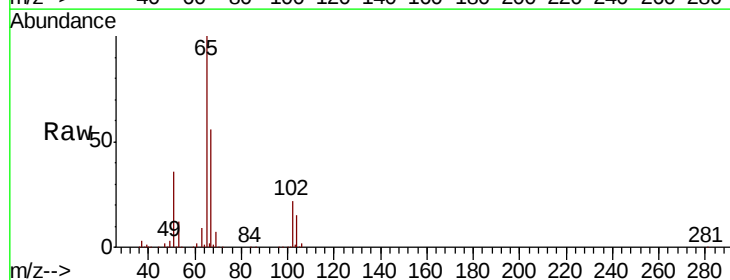

Abundance Ion 64.90 (64.60 to 65.60): VNC
Ion 66.90 (66.60 to 67.60): VNC




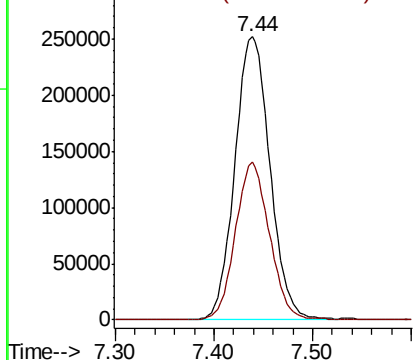




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.01 min Scan# 1939
 Delta R.T. -0.00 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16




Instrument :
 MSVOA_N
 ClientSampleId :
 2S-C4-(0)


Tgt Ion:114 Resp: 1846797
 Ion Ratio Lower Upper
 114 100
 63 19.3 0.0 36.2
 88 15.9 0.0 30.0

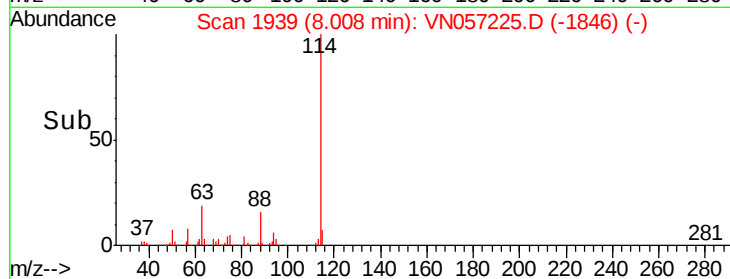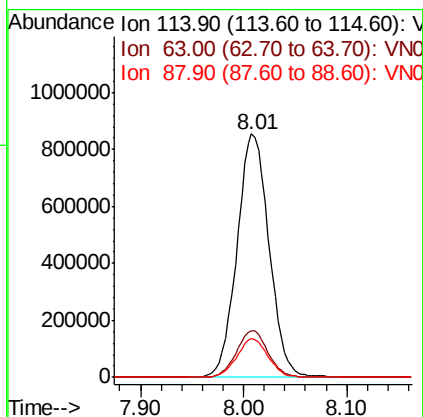

#35
 Dibromofluoromethane
 Concen: 49.227 ug/l
 RT: 6.99 min Scan# 1621
 Delta R.T. -0.00 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16

Tgt Ion:113 Resp: 570489
 Ion Ratio Lower Upper
 113 100
 111 101.2 81.3 121.9
 192 23.7 19.0 28.4



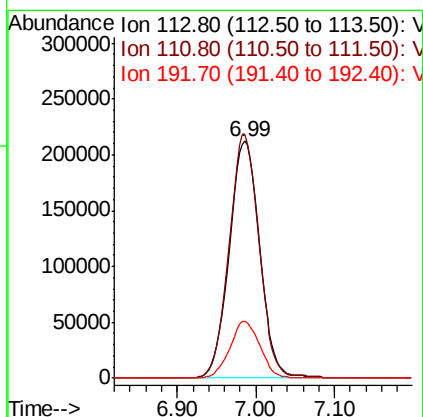





#36
 1,1-Dichloropropene
 Concen: 5.272 ug/l
 RT: 7.06 min Scan# 1643
 Delta R.T. -0.14 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16




Instrument :
 MSVOA_N
 ClientSampleId :
 2S-C4-(0)


Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.9	18.7	56.1#
77	0.0	25.0	37.4#

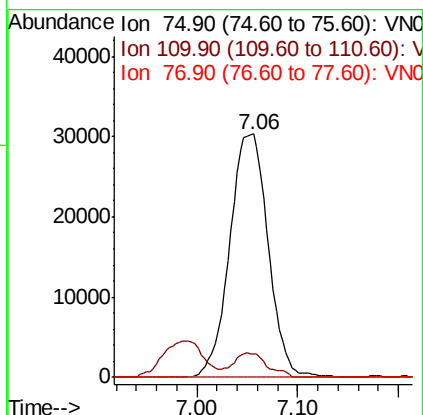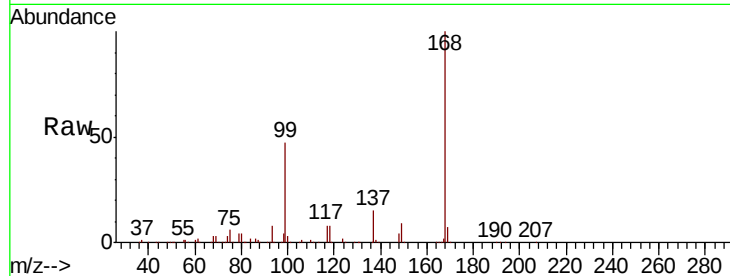

#38
 Carbon Tetrachloride
 Concen: 7.125 ug/l
 RT: 7.05 min Scan# 1640
 Delta R.T. -0.14 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.1	75.8	113.6#
121	0.0	24.4	36.6#

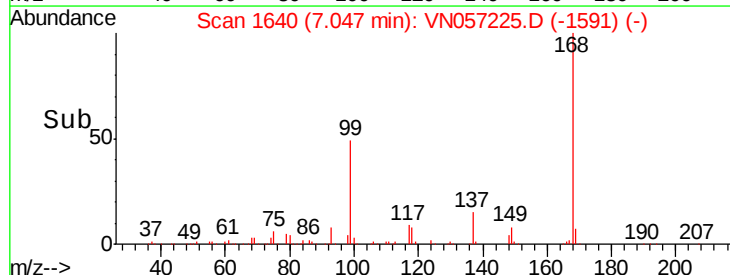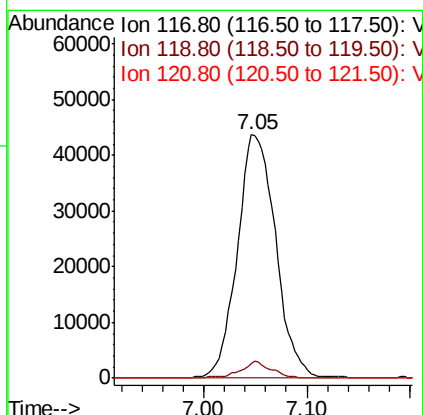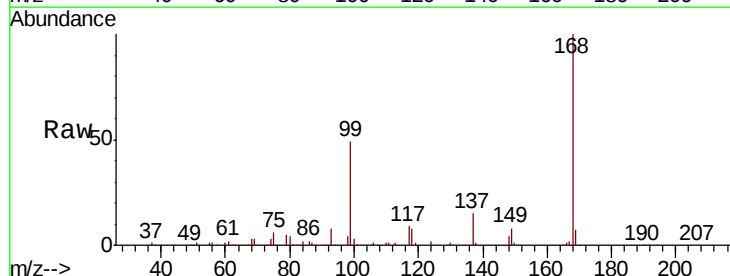



#43

Isopropyl Acetate

Concen: 6.023 ug/l

RT: 7.57 min Scan# 1802

Delta R.T. 0.01 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :

2S-C4-(0)


Tgt Ion: 43 Resp: 128837

Ion Ratio Lower Upper

43 100

61 20.5 24.2 36.2#




87 13.6 11.8 17.8

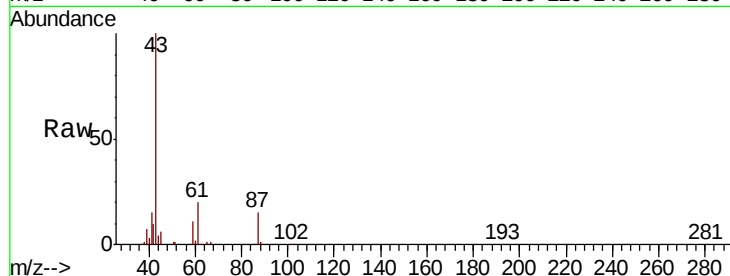

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

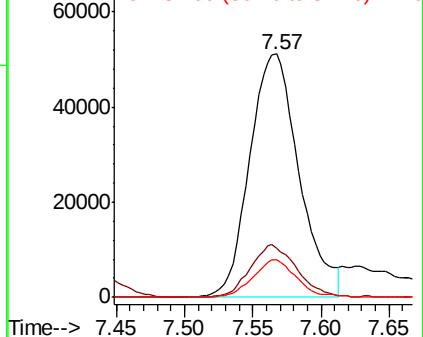

#45

1,2-Dichloropropane

Concen: 0.216 ug/l

RT: 8.70 min Scan# 2155

Delta R.T. 0.14 min

Lab File: VN057225.D


Acq: 12 Aug 2019 19:16

Tgt Ion: 63 Resp: 2688

Ion Ratio Lower Upper



63 100


65 0.0 25.2 37.8#



Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0




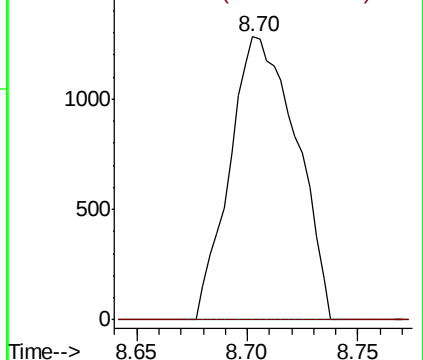


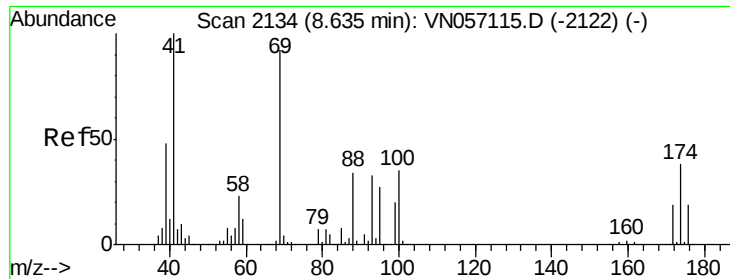

#48
Methyl methacrylate
Concen: 0.734 ug/l
RT: 8.63 min Scan# 2131
Delta R.T. -0.01 min
Lab File: VN057225.D
Acq: 12 Aug 2019 19:16




Instrument :
MSVOA_N
ClientSampleId :
2S-C4-(0)


Tgt Ion: 41 Resp: 7399
Ion Ratio Lower Upper
41 100
69 0.0 77.5 116.3#
39 0.0 39.8 59.6#

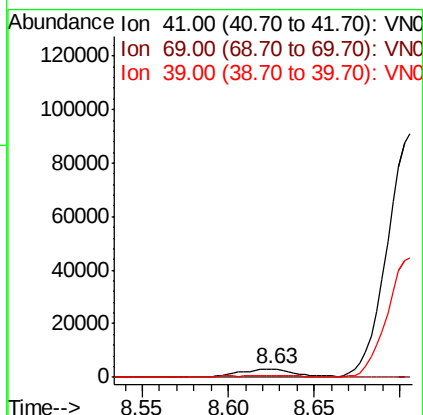

#50
Toluene-d8
Concen: 48.733 ug/l
RT: 9.56 min Scan# 2421
Delta R.T. -0.00 min
Lab File: VN057225.D
Acq: 12 Aug 2019 19:16

Tgt Ion: 98 Resp: 2160669
Ion Ratio Lower Upper
98 100
100 64.8 51.2 76.8


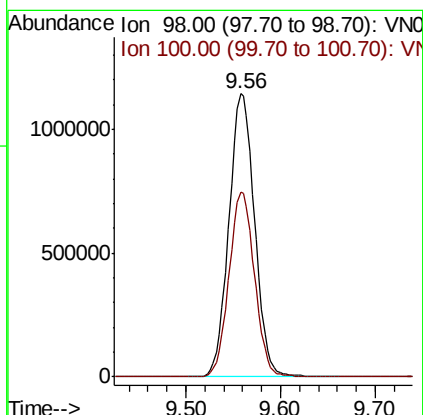






#51
 4-Methyl-2-Pentanone
 Concen: 0.764 ug/l
 RT: 9.45 min Scan# 2387
 Delta R.T. 0.00 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16




Instrument :
 MSVOA_N
 ClientSampleId :
 2S-C4-(0)


Tgt Ion: 43 Resp: 9514
 Ion Ratio Lower Upper
 43 100
 58 40.6 33.2 49.8

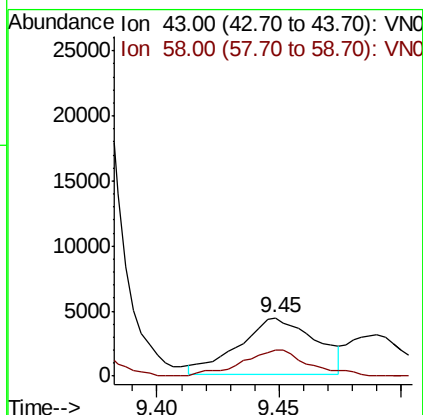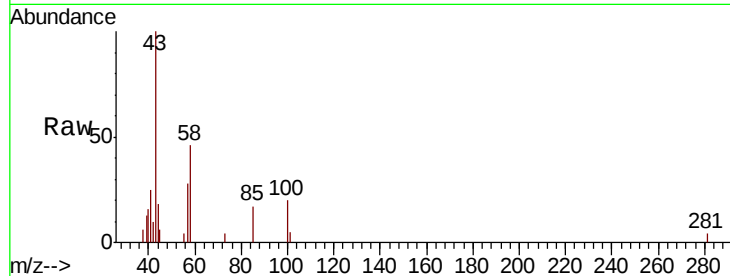

#54
 cis-1,3-Dichloropropene
 Concen: 3.400 ug/l
 RT: 9.36 min Scan# 2361
 Delta R.T. 0.07 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16

Tgt Ion: 75 Resp: 63017
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.1 37.7#
 39 28.6 32.5 48.7#



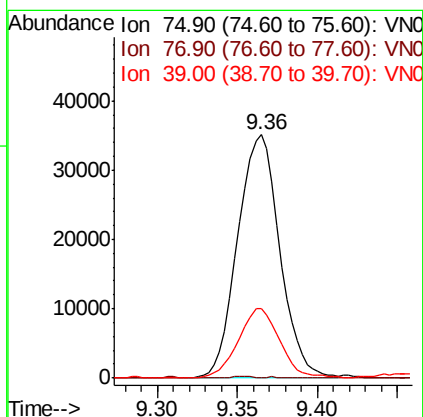





#57
 1,3-Dichloropropane
 Concen: 0.522 ug/l
 RT: 10.25 min Scan# 2636
 Delta R.T. 0.06 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16




Instrument :
 MSVOA_N
 ClientSampleId :
 2S-C4-(0)


Tgt Ion: 76 Resp: 10105
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.9 38.9#

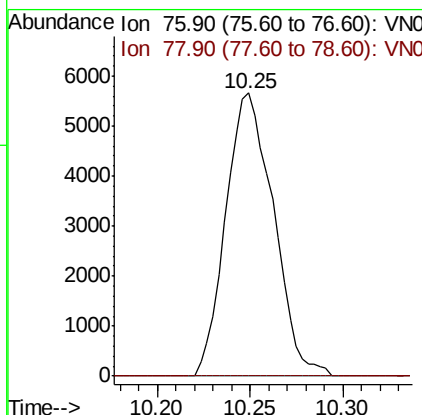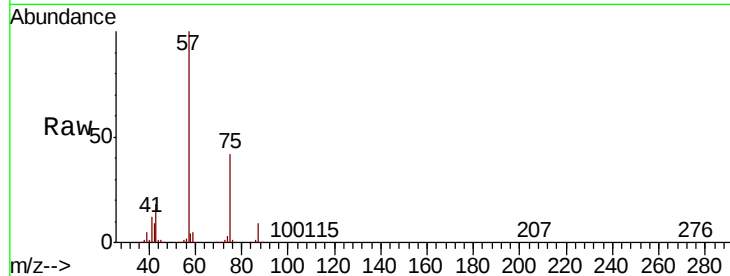

#59
 2-Hexanone
 Concen: 14.316 ug/l
 RT: 10.25 min Scan# 2636
 Delta R.T. 0.01 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16

Tgt Ion: 43 Resp: 120621
 Ion Ratio Lower Upper
 43 100
 58 21.7 29.2 87.6#

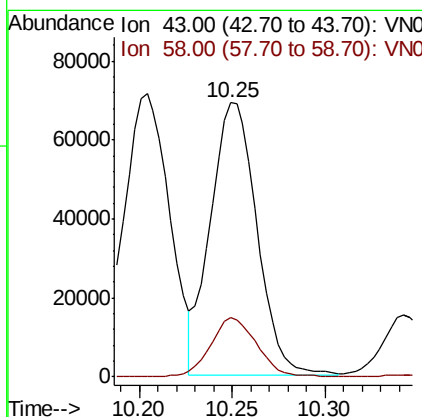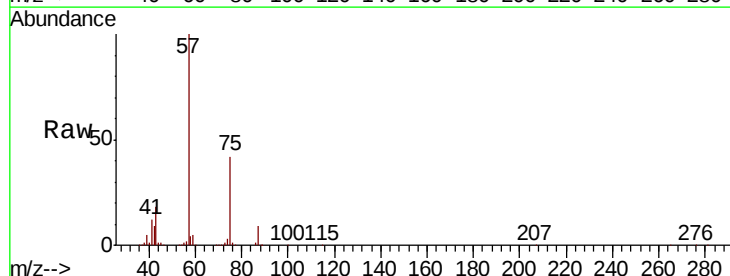



#62

4-Bromofluorobenzene

Concen: 39.181 ug/l

RT: 11.92 min Scan# 3156

Delta R.T. 0.00 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :

2S-C4-(0)


Tgt Ion: 95 Resp: 559731

Ion Ratio Lower Upper

95 100

174 96.3 0.0 185.0




176 94.5 0.0 181.2

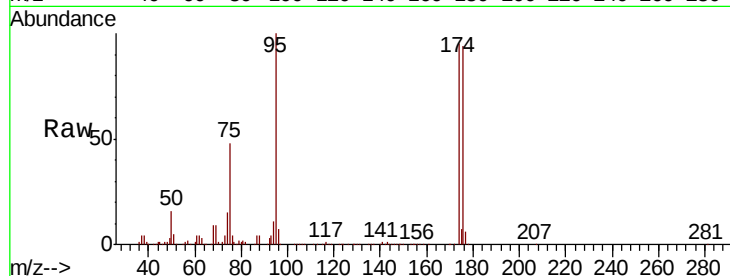

Abundance Ion 94.90 (94.60 to 95.60): VN057115.D (-3140) (-)

Ion 173.80 (173.50 to 174.50): VN057115.D (-3140) (-)

Ion 175.80 (175.50 to 176.50): VN057115.D (-3140) (-)

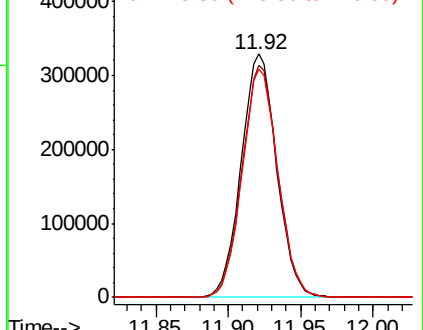

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.91 min Scan# 2841

Delta R.T. 0.00 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16


Tgt Ion: 117 Resp: 1563675

Ion Ratio Lower Upper

117 100

82 51.5 40.8 61.2



119 32.3 25.7 38.5




Abundance Ion 116.90 (116.60 to 117.60): VN057115.D (-2824) (-)

Ion 82.00 (81.70 to 82.70): VN057115.D (-2824) (-)

Ion 118.90 (118.60 to 119.60): VN057115.D (-2824) (-)

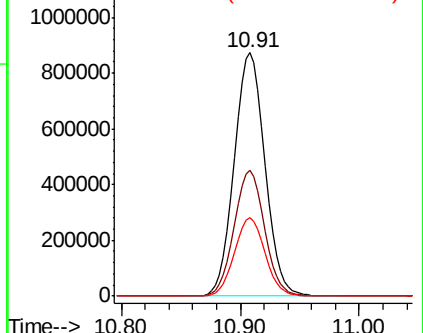

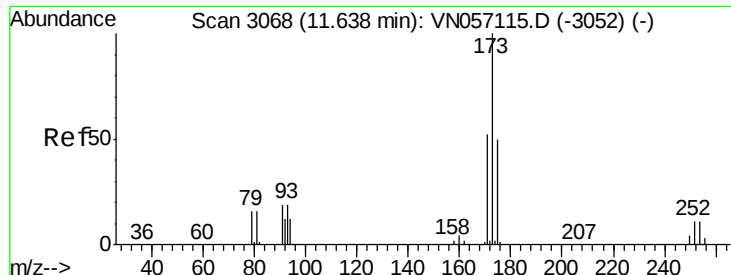

#71

Bromoform

Concen: 0.274 ug/l

RT: 11.92 min Scan# 3155

Delta R.T. 0.28 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :

2S-C4-(0)


Tgt Ion:173 Resp: 2364

Ion Ratio Lower Upper

173 100

175 1061.5 24.6 73.8#




254 0.0 0.1 0.1#

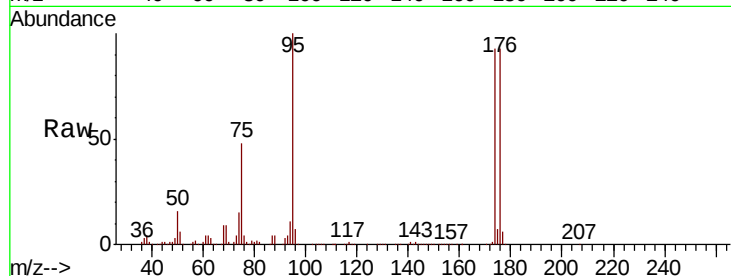

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

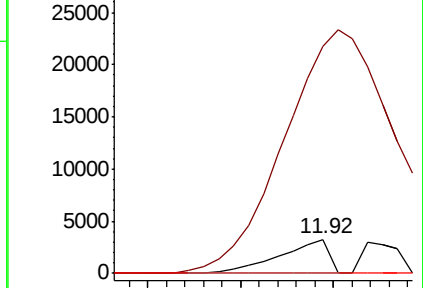

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.88 min Scan# 3453

Delta R.T. 0.00 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16


Tgt Ion:152 Resp: 390532

Ion Ratio Lower Upper

152 100

115 55.2 27.5 82.5



150 156.9 0.0 341.6




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

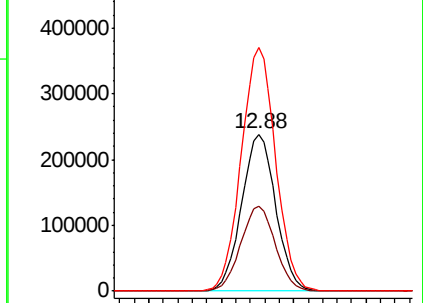



#73

Isopropylbenzene

Concen: Below Cal

RT: 11.77 min Scan# 3108

Delta R.T. 0.00 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampled :


2S-C4-(0)

Tgt Ion: 105 Resp: 392

Ion Ratio Lower Upper

105 100

120 0.0 13.7 41.0#

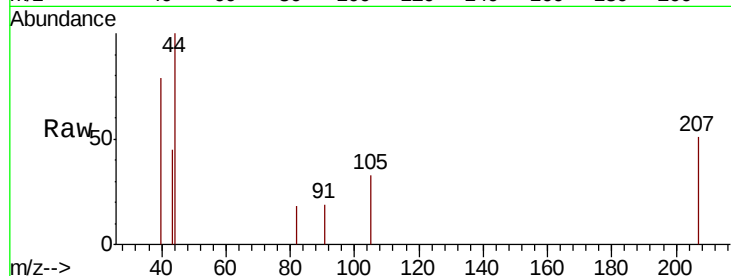

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

11.77

300

250

200



150

100

50

0

Time--> 11.74 11.76 11.78 11.80



#74

N-ethyl acetate

Concen: 0.257 ug/l

RT: 11.54 min Scan# 3039

Delta R.T. -0.04 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Tgt Ion: 43 Resp: 2539


Ion Ratio Lower Upper

43 100

70 0.0 36.8 55.2#

55 0.0 20.6 31.0#

61 0.0 21.0 31.4#



Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

2000


1500


1000

500

0

Time--> 11.50 11.55





#76

1,2,3-Trichloropropane

Concen: 33.835 ug/l

RT: 11.92 min Scan# 3156

Delta R.T. -0.15 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampled :


2S-C4-(0)

Tgt Ion: 75 Resp: 265210

Ion Ratio Lower Upper




75 100

77 1.3 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

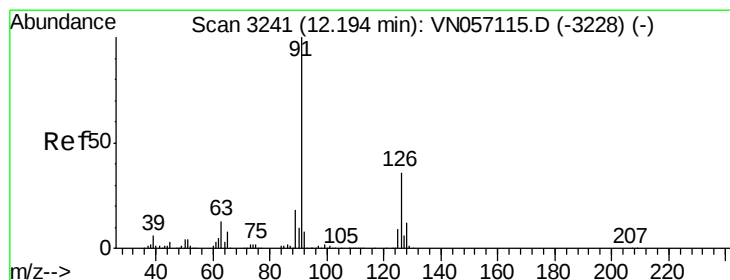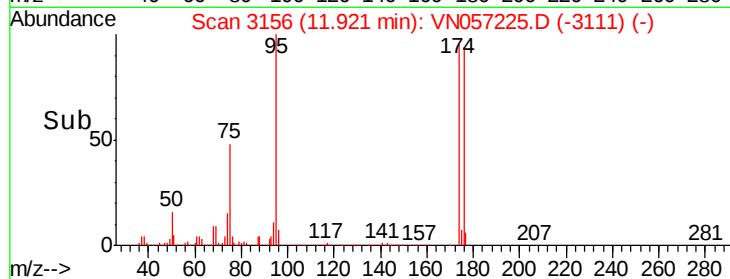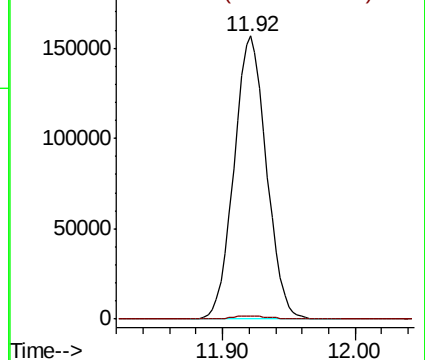

#79

2-Chlorotoluene

Concen: Below Cal

RT: 12.19 min Scan# 3239

Delta R.T. -0.01 min

Lab File: VN057225.D


Acq: 12 Aug 2019 19:16

Tgt Ion: 91 Resp: 63

Ion Ratio Lower Upper



91 100


126 0.0 18.1 54.3#



Abundance Ion 91.00 (90.70 to 91.70): VN0

Ion 125.90 (125.60 to 126.60): V

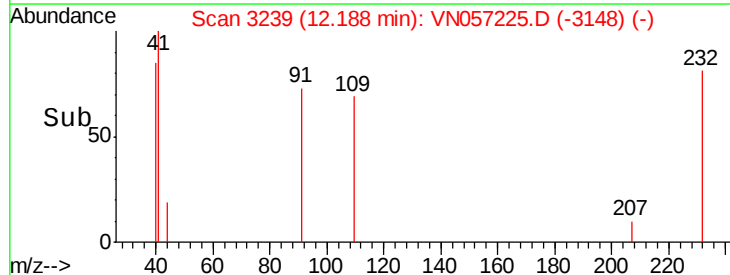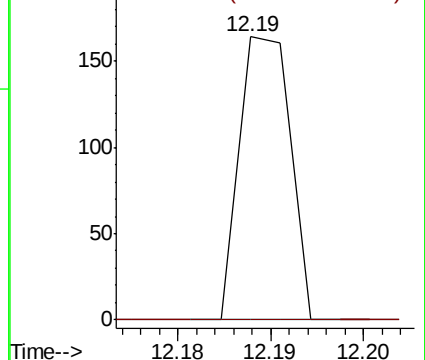



#81

trans-1,4-Dichloro-2-butene

Concen: 99.851 ug/l

RT: 11.92 min Scan# 3156

Delta R.T. 0.10 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :

2S-C4-(0)


Tgt Ion: 75 Resp: 265210

Ion Ratio Lower Upper

75 100

53 0.0 70.6 106.0#




89 0.0 36.4 54.6#



Abundance Ion 74.90 (74.60 to 75.60): VN057115.D (-3114) (-)

Ion 53.00 (52.70 to 53.70): VN057115.D (-3114) (-)

Ion 88.90 (88.60 to 89.60): VN057115.D (-3114) (-)

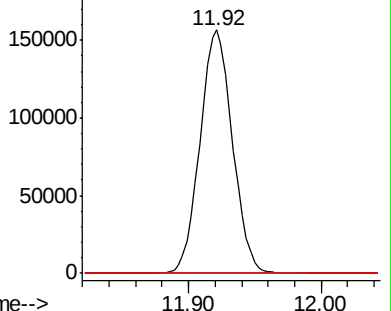

#83

tert-Butylbenzene

Concen: Below Cal

RT: 12.60 min Scan# 3366

Delta R.T. 0.07 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16


Tgt Ion: 119 Resp: 30

Ion Ratio Lower Upper

119 100

91 0.0 31.4 94.2#



134 0.0 13.2 39.6#




Abundance Ion 119.00 (118.70 to 119.70): VN057115.D (-3327) (-)

Ion 91.00 (90.70 to 91.70): VN057115.D (-3327) (-)

Ion 134.00 (133.70 to 134.70): VN057115.D (-3327) (-)

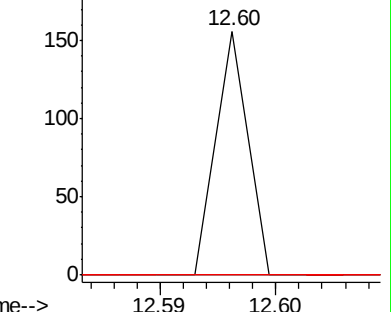

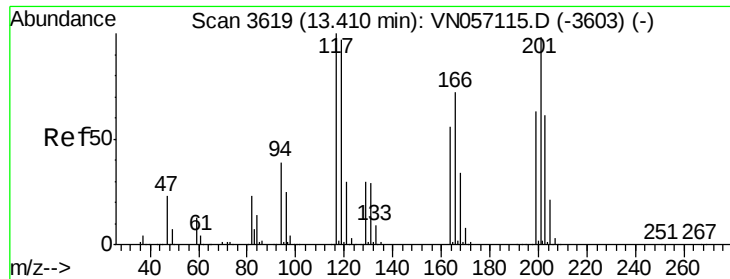

#90

Hexachloroethane

Concen: Below Cal

RT: 13.63 min Scan# 3688

Delta R.T. 0.22 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16

Instrument :

MSVOA_N

ClientSampleId :


2S-C4-(0)

Tgt Ion:117 Resp: 32

Ion Ratio Lower Upper




117 100

201 0.0 49.3 147.8#

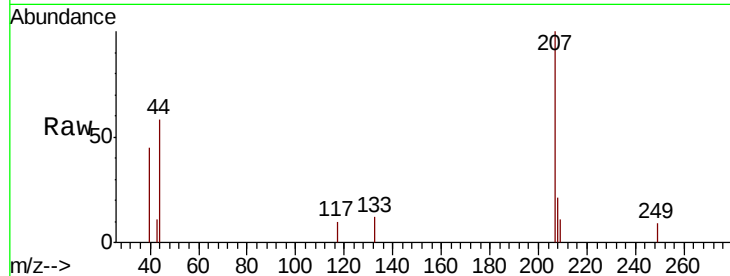

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

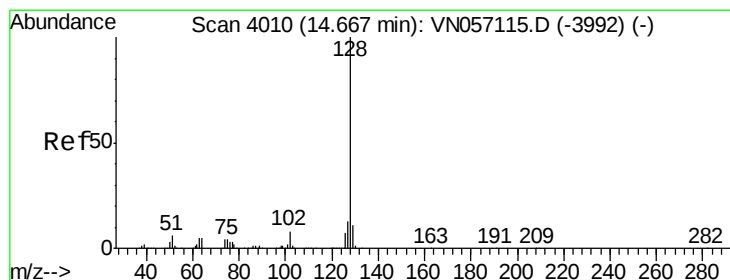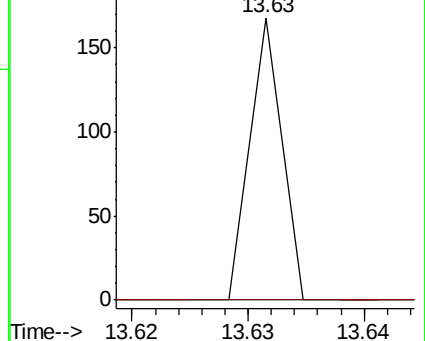

#95

Naphthalene

Concen: 2.848 ug/l

RT: 14.67 min Scan# 4012

Delta R.T. 0.01 min

Lab File: VN057225.D

Acq: 12 Aug 2019 19:16


Tgt Ion:128 Resp: 460

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#



129 6.7 8.8 13.2#




Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

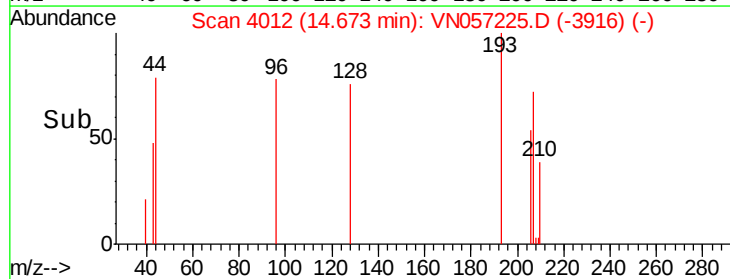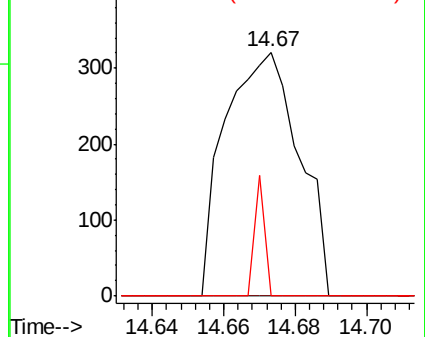

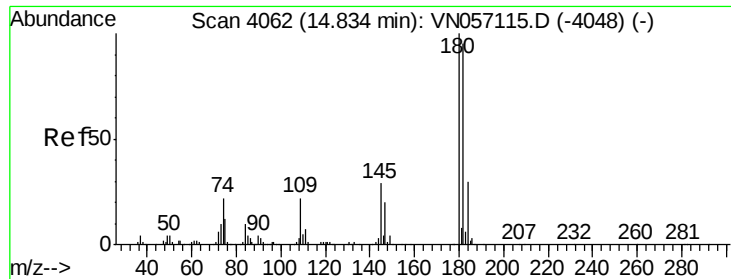

#96
 1,2,3-Trichlorobenzene
 Concen: 5.739 ug/l
 RT: 14.84 min Scan# 4064
 Delta R.T. 0.01 min
 Lab File: VN057225.D
 Acq: 12 Aug 2019 19:16

Instrument :
 MSVOA_N
 ClientSampleId :
 2S-C4-(0)

Tgt Ion	Ratio	Lower	Upper
180	100		
182	173.6	48.3	144.8#
145	0.0	14.9	44.5#

