

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081219\
 Data File : VN057232.D
 Acq On : 12 Aug 2019 22:07
 Operator : JC/SP
 Sample : K4229-31
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 2S-A3-(0)

Quant Time: Aug 13 03:31:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:49:25 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	1292024	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.01	114	1816879	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.91	117	1522931	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.88	152	410013	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.44	65	602519	45.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.68%	
35) Dibromofluoromethane	6.99	113	548246	48.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.18%	
50) Toluene-d8	9.56	98	2097204	48.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.16%	
62) 4-Bromofluorobenzene	11.92	95	571035	40.63	ug/l	0.00
Spiked Amount 50.000			Recovery	=	81.26%	
Target Compounds						
16) Acetone	3.48	43	24018	5.985	ug/l	98
18) Methyl Acetate	3.90	43	29571	1.840	ug/l	98
43) Isopropyl Acetate	7.56	43	169444	8.052	ug/l #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN081219\
Data File : VN057232.D
Acq On : 12 Aug 2019 22:07
Operator : JC/SP
Sample : K4229-31
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
2S-A3-(0)

Quant Time: Aug 13 03:31:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N080719W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:49:25 2019
Response via : Initial Calibration

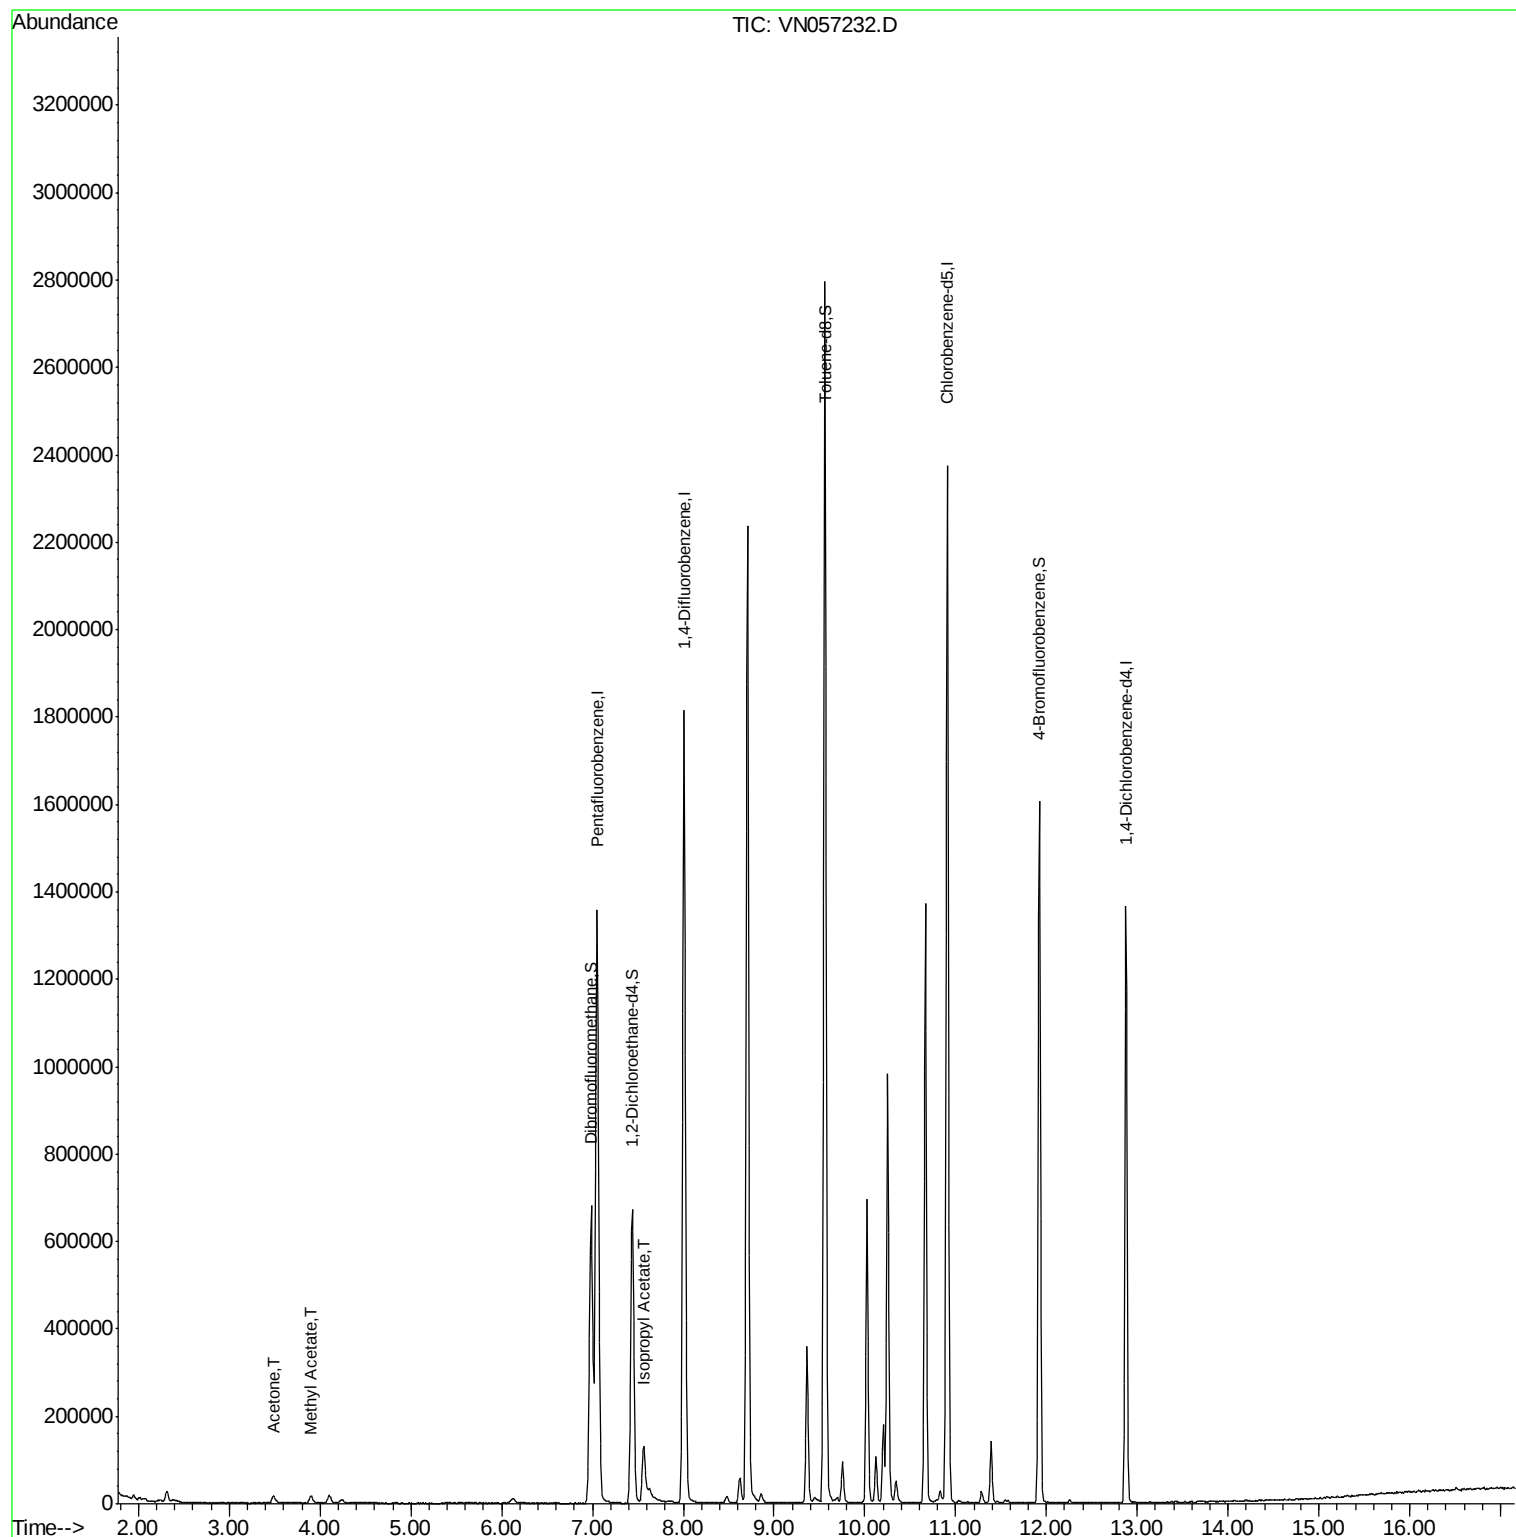

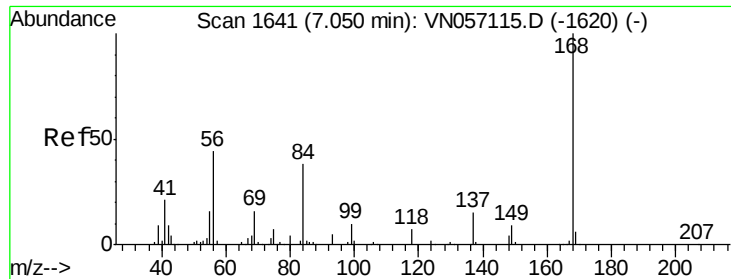

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 1642

Delta R.T. 0.00 min

Lab File: VN057232.D

Acq: 12 Aug 2019 22:07

Instrument :

MSVOA_N

ClientSampled :


2S-A3-(0)

Tot Ion:168 Resp: 1292024

Ion Ratio Lower Upper

168 100

99 47.9 38.6 57.8

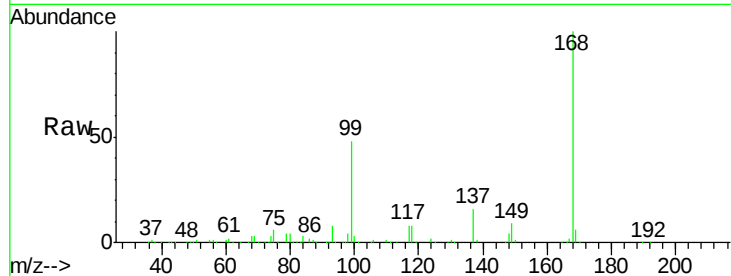

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.05

600000

500000

400000



300000

200000

100000

0

Time--> 6.90 7.00 7.10 7.20

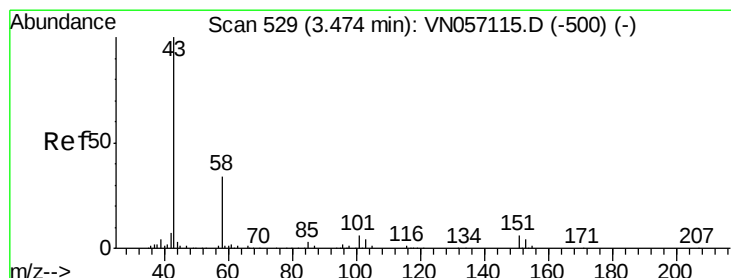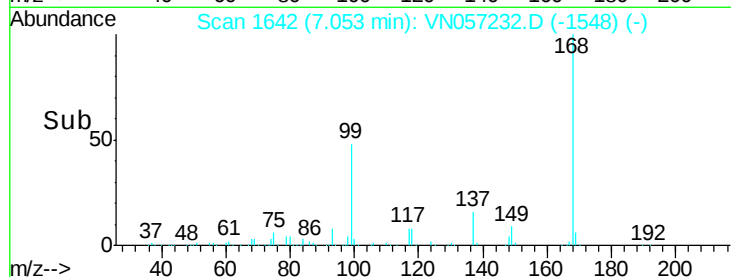

#16

Acetone

Concen: 5.985 ug/l

RT: 3.48 min Scan# 532

Delta R.T. 0.01 min

Lab File: VN057232.D


Acq: 12 Aug 2019 22:07

Tgt Ion: 43 Resp: 24018

Ion Ratio Lower Upper

43 100

58 33.2 27.4 41.2

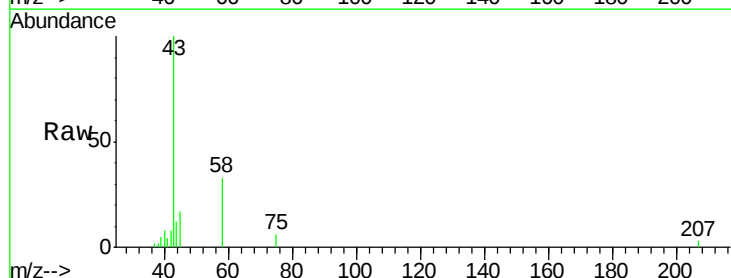

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.48

10000

8000


6000


4000

2000

0

Time--> 3.40 3.45 3.50 3.55 3.60




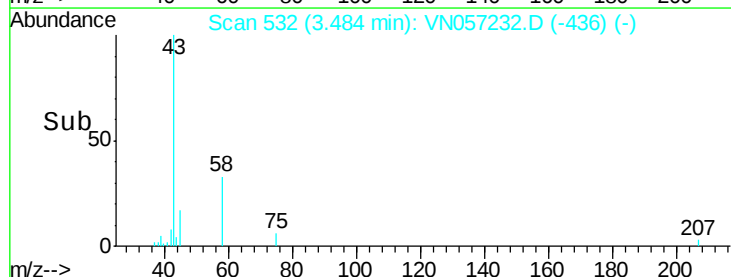




#18
Methvl Acetate
Concen: 1.840 ug/l
RT: 3.90 min Scan# 660
Delta R.T. 0.01 min
Lab File: VN057232.D
Acq: 12 Aug 2019 22:07




Instrument :
MSVOA_N
ClientSampleId :
2S-A3-(0)


Tot Ion: 43 Resp: 29571
Ion Ratio Lower Upper
43 100
74 24.2 20.2 30.4

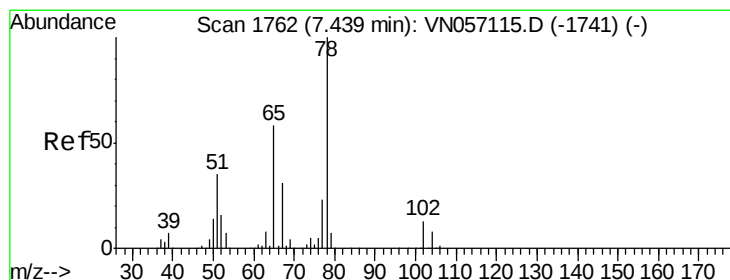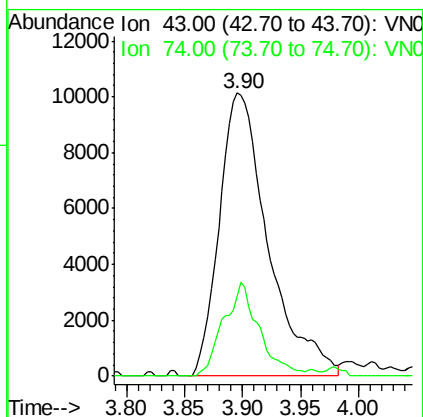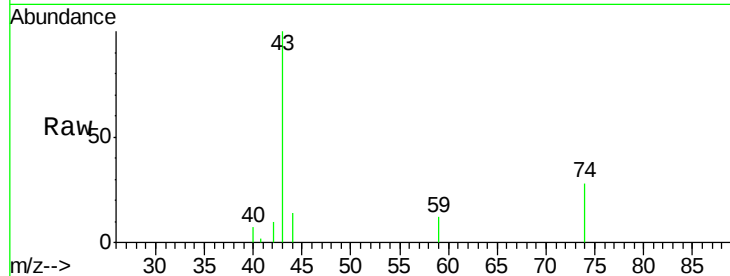

#33
1,2-Dichloroethane-d4
Concen: 45.345 ug/l
RT: 7.44 min Scan# 1762
Delta R.T. -0.00 min
Lab File: VN057232.D
Acq: 12 Aug 2019 22:07

Tgt Ion: 65 Resp: 602519
Ion Ratio Lower Upper
65 100
67 53.2 0.0 108.2



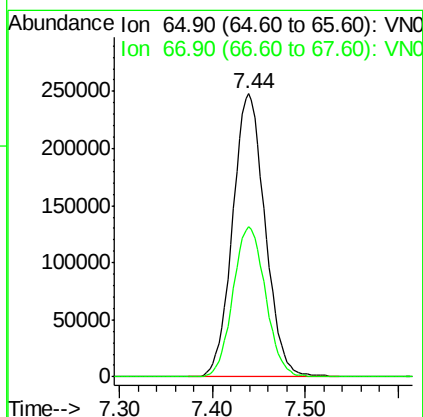





#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.01 min Scan# 1939
 Delta R.T. -0.00 min
 Lab File: VN057232.D
 Acq: 12 Aug 2019 22:07




Instrument :
 MSVOA_N
 ClientSampleId :
 2S-A3-(0)


Tot Ion:114 Resp: 1816879
 Ion Ratio Lower Upper
 114 100
 63 19.0 0.0 36.2
 88 15.2 0.0 30.0

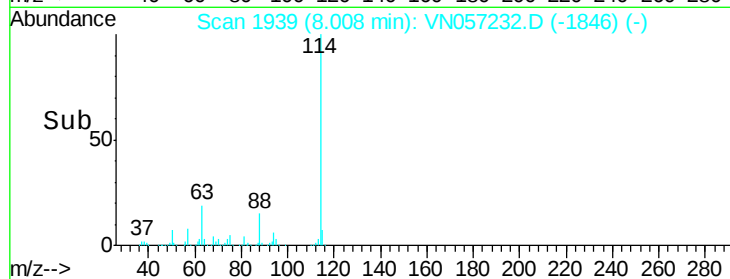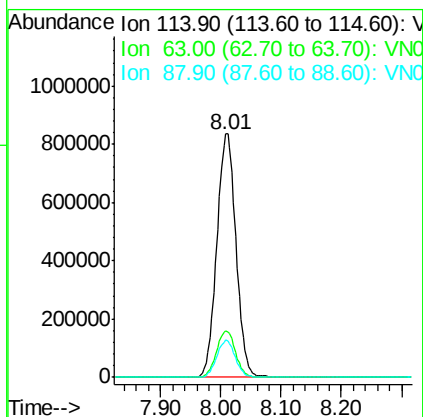

#35
 Dibromofluoromethane
 Concen: 48.087 ug/l
 RT: 6.99 min Scan# 1621
 Delta R.T. -0.00 min
 Lab File: VN057232.D
 Acq: 12 Aug 2019 22:07

Tgt Ion:113 Resp: 548246
 Ion Ratio Lower Upper
 113 100
 111 101.1 81.3 121.9
 192 23.7 19.0 28.4

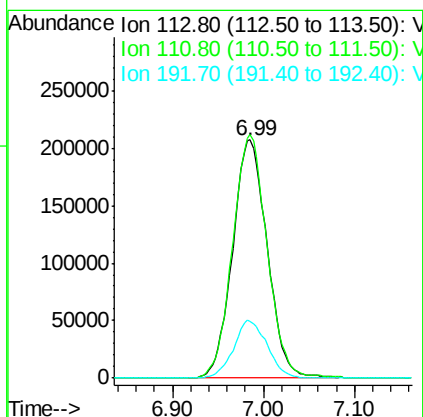



#43

Isopropyl Acetate

Concen: 8.052 ug/l

RT: 7.56 min Scan# 1801

Delta R.T. 0.00 min

Lab File: VN057232.D

Acq: 12 Aug 2019 22:07

Instrument :





MSVOA_N

ClientSampleId :

2S-A3-(0)

Tot Ion: 43 Resp: 169444

Ion	Ratio	Lower	Upper
43	100		
61	17.7	24.2	36.2#
87	12.7	11.8	17.8

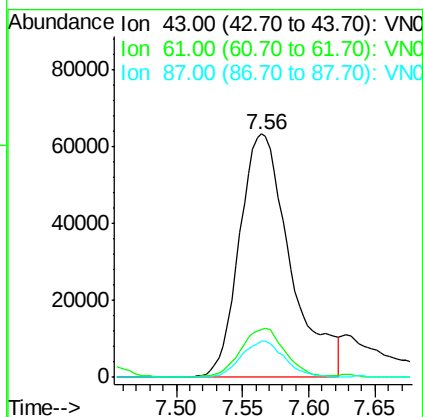

#50

Toluene-d8

Concen: 48.080 ug/l

RT: 9.56 min Scan# 2422




Delta R.T. 0.00 min


Lab File: VN057232.D

Acq: 12 Aug 2019 22:07

Tgt Ion: 98 Resp: 2097204

Ion	Ratio	Lower	Upper
98	100		
100	65.1	51.2	76.8

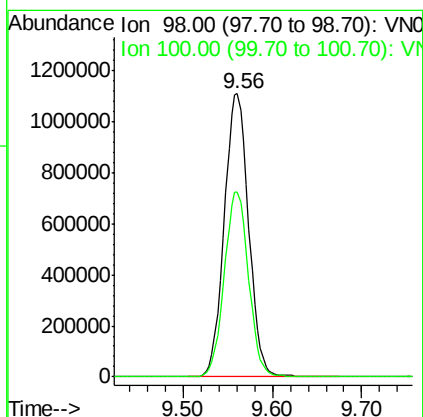

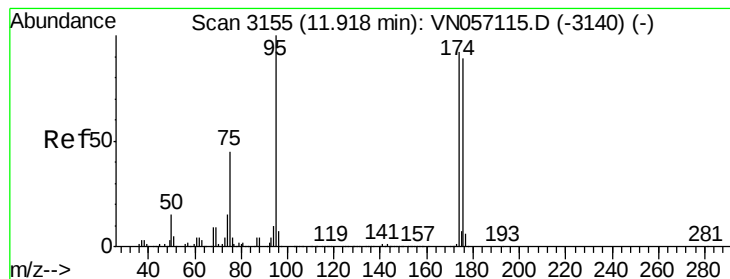

#62

4-Bromofluorobenzene

Concen: 40.630 ug/l

RT: 11.92 min Scan# 3156

Delta R.T. 0.00 min

Lab File: VN057232.D

Acq: 12 Aug 2019 22:07

Instrument :

MSVOA_N

ClientSampleId :

2S-A3-(0)


Tot Ion: 95 Resp: 571035

Ion Ratio Lower Upper

95 100

174 94.3 0.0 185.0

176 92.4 0.0 181.2




Abundance Ion 94.90 (94.60 to 95.60): VN057115.D (-3140) (-)

Ion 173.80 (173.50 to 174.50): VN057115.D (-3140) (-)

Ion 175.80 (175.50 to 176.50): VN057115.D (-3140) (-)

Time-->




Abundance Ion 94.90 (94.60 to 95.60): VN057232.D (-3062) (-)

Ion 173.80 (173.50 to 174.50): VN057232.D (-3062) (-)

Ion 175.80 (175.50 to 176.50): VN057232.D (-3062) (-)

Time-->

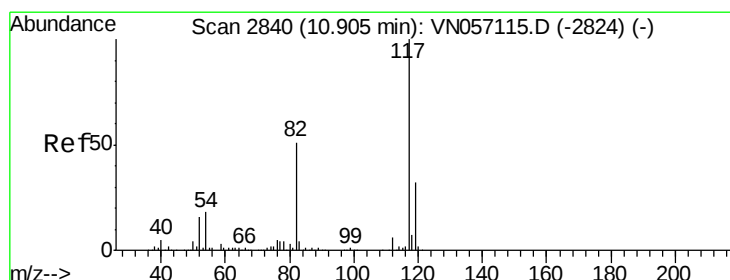

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.91 min Scan# 2841

Delta R.T. 0.00 min

Lab File: VN057232.D

Acq: 12 Aug 2019 22:07


Tgt Ion: 117 Resp: 1522931

Ion Ratio Lower Upper

117 100

82 51.6 40.8 61.2

119 31.5 25.7 38.5




Abundance Ion 116.90 (116.60 to 117.60): VN057115.D (-2824) (-)

Ion 82.00 (81.70 to 82.70): VN057115.D (-2824) (-)

Ion 118.90 (118.60 to 119.60): VN057115.D (-2824) (-)

Time-->




Abundance Ion 116.90 (116.60 to 117.60): VN057232.D (-2747) (-)

Ion 82.00 (81.70 to 82.70): VN057232.D (-2747) (-)

Ion 118.90 (118.60 to 119.60): VN057232.D (-2747) (-)

Time-->

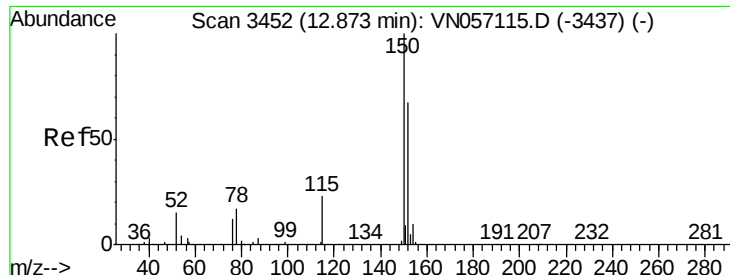

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.88 min Scan# 3453

Delta R.T. 0.00 min

Lab File: VN057232.D

Acq: 12 Aug 2019 22:07

Instrument :

MSVOA_N

ClientSampleId :

2S-A3-(0)


Tot Ion:152 Resp: 410013

Ion Ratio Lower Upper

152 100

115 53.4 27.5 82.5

150 153.5 0.0 341.6



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

