


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081219\
Data File : VN057210.D
Acq On : 12 Aug 2019 12:35
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N081019W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sun Aug 11 03:53:25 2019

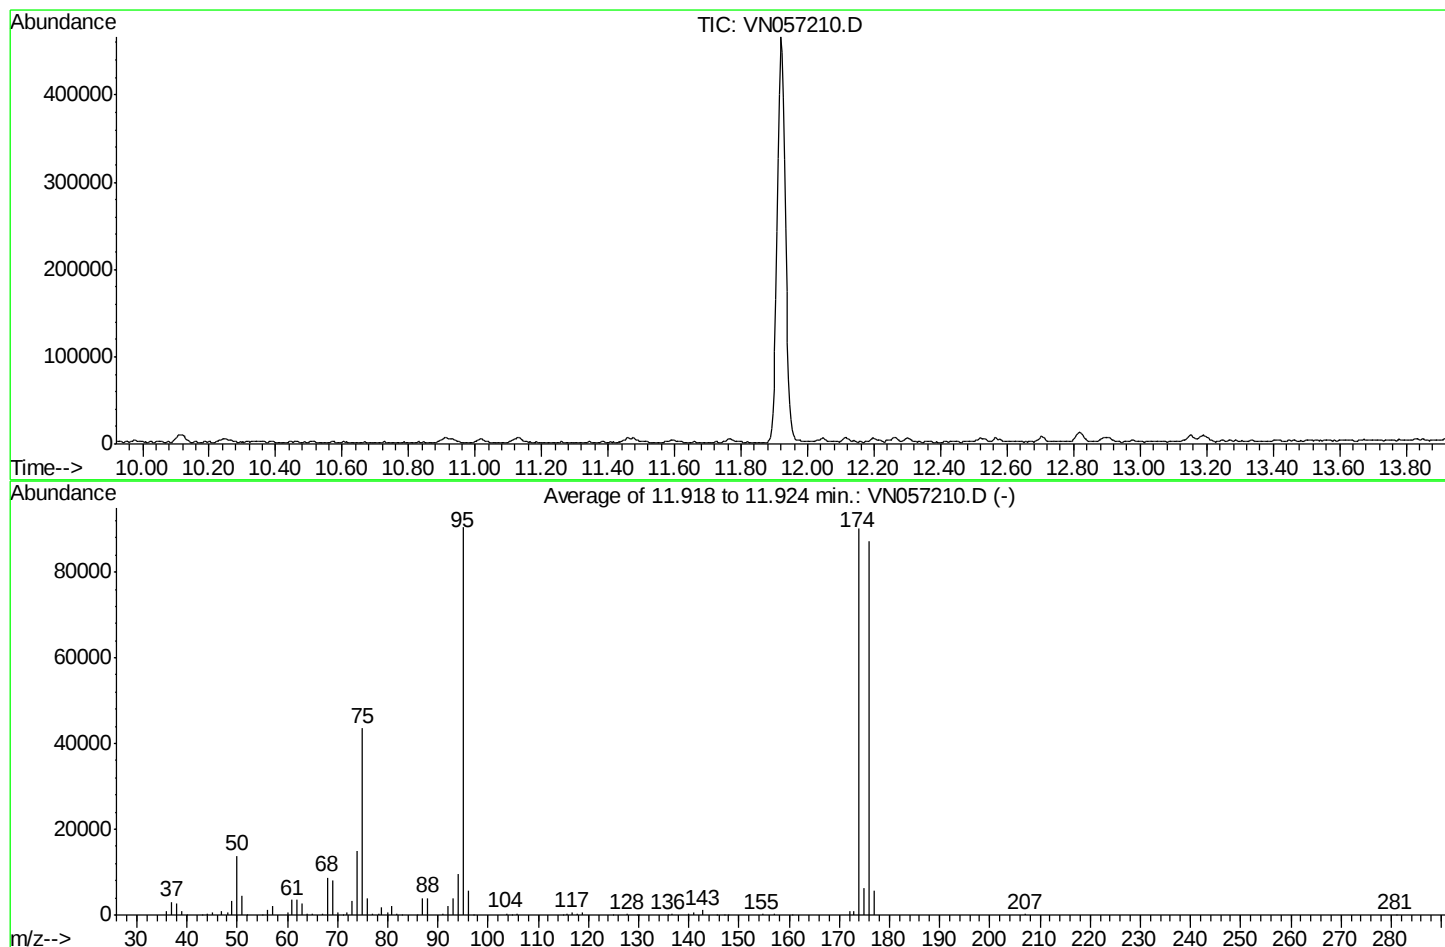

AutoFind: Scans 3155, 3156, 3157; Background Corrected with Scan 3142

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	13846	PASS
75	95	30	60	48.1	43528	PASS
95	95	100	100	100.0	90432	PASS
96	95	5	9	6.3	5708	PASS
173	174	0.00	2	1.0	938	PASS
174	95	50	100	99.6	90090	PASS
175	174	5	9	7.1	6372	PASS
176	174	95	101	96.7	87104	PASS
177	176	5	9	6.4	5555	PASS