


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081220\
 Data File : VN062873.D
 Acq On : 12 Aug 2020 22:16
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
 Title : SW846 8260
 Last Update : Wed Aug 05 13:26:42 2020

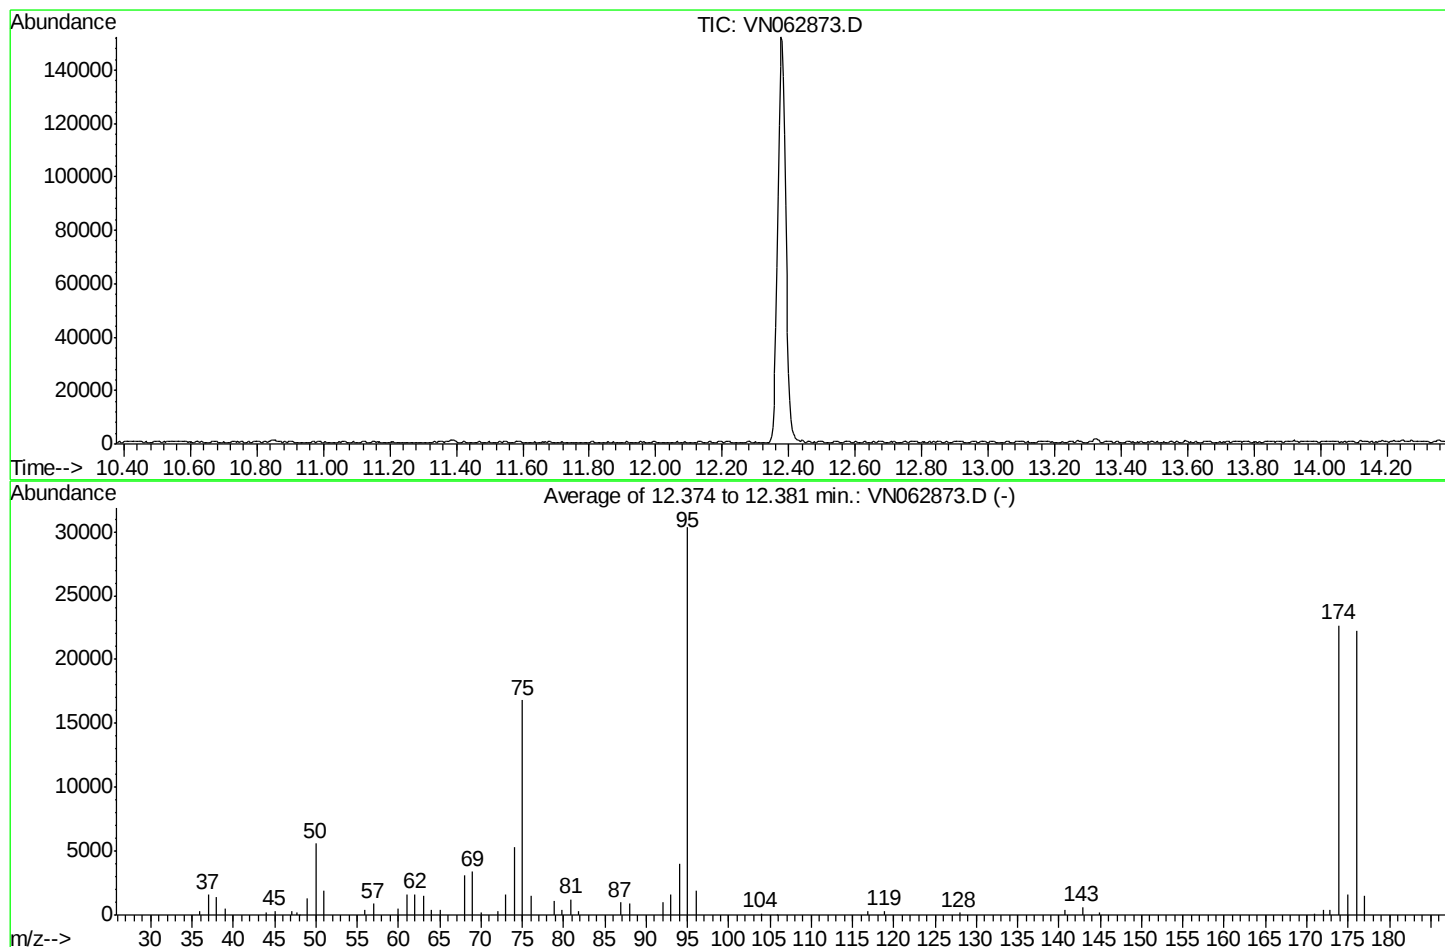

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5610	PASS
75	95	30	60	55.5	16827	PASS
95	95	100	100	100.0	30344	PASS
96	95	5	9	6.3	1925	PASS
173	174	0.00	2	1.8	414	PASS
174	95	50	100	74.6	22648	PASS
175	174	5	9	7.2	1636	PASS
176	174	95	101	98.4	22277	PASS
177	176	5	9	6.5	1457	PASS