
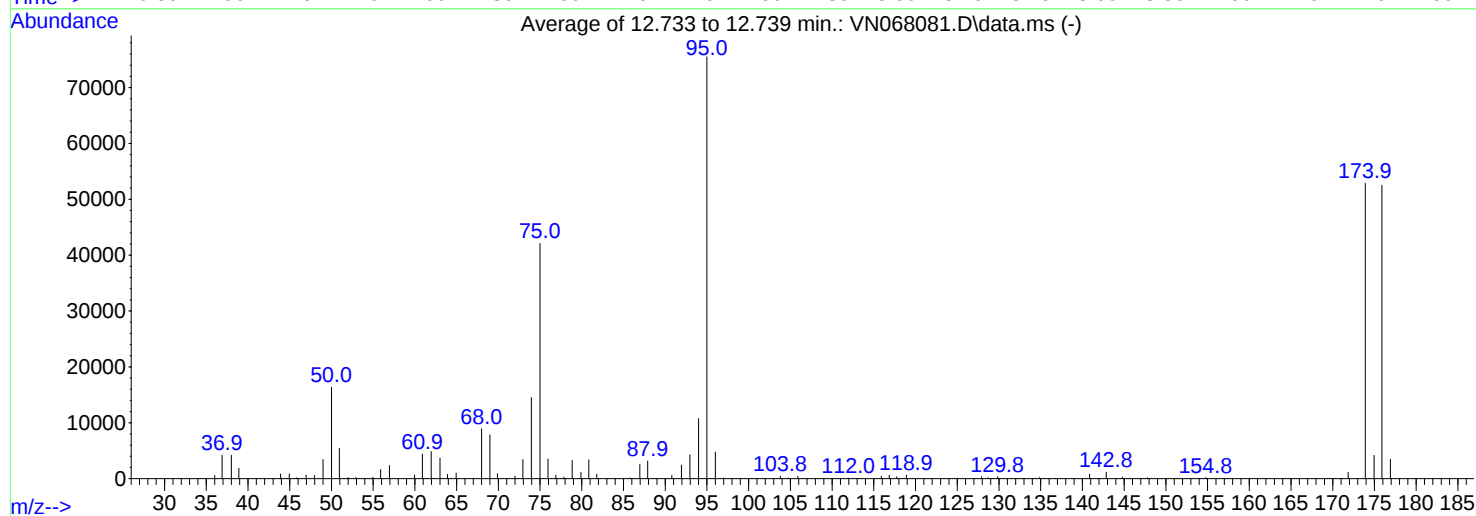


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081221\
 Data File : VN068081.D
 Acq On : 12 Aug 2021 9:35
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Title : SW846 8260
 Last Update : Thu Jul 29 15:02:35 2021

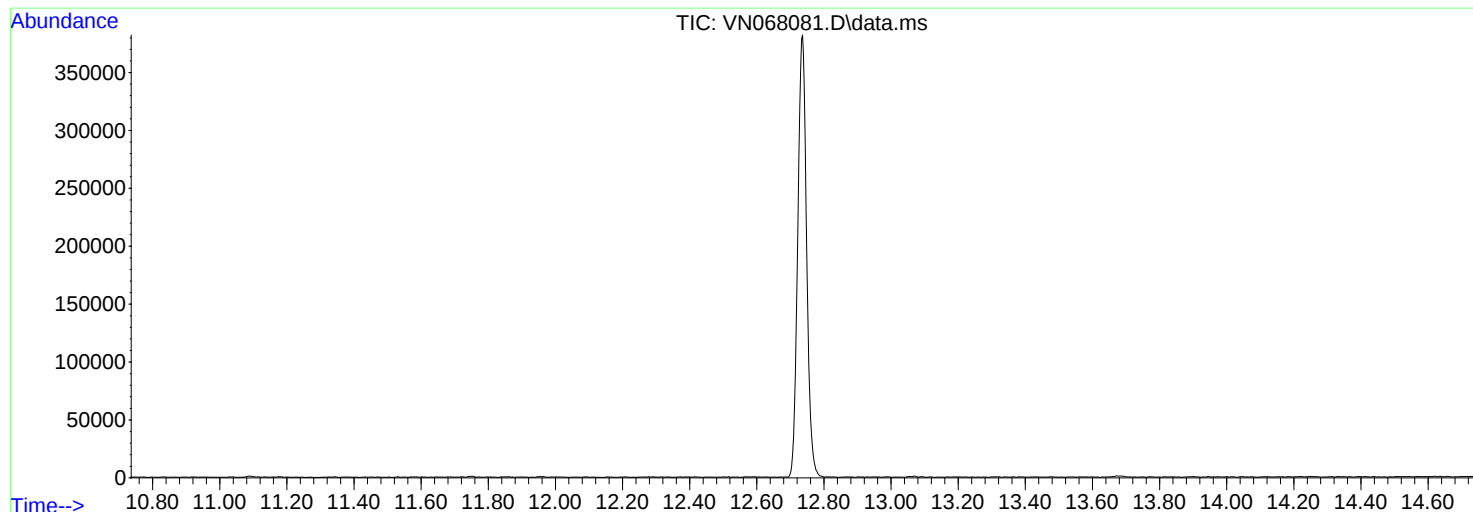

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	16364	PASS
75	95	30	60	55.8	42112	PASS
95	95	100	100	100.0	75496	PASS
96	95	5	9	6.3	4758	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.0	52875	PASS
175	174	5	9	7.9	4162	PASS
176	174	95	101	99.3	52523	PASS
177	176	5	9	6.6	3483	PASS