

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081222\
 Data File : VN073849.D
 Acq On : 12 Aug 2022 14:10
 Operator : JC\MD
 Sample : N4194-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Aug 13 05:02:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.022	168	404324	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	634337	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	590427	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	287020	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	243279	49.373	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.740%
35) Dibromofluoromethane	7.957	113	227701	57.165	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	114.320%
50) Toluene-d8	10.380	98	720074	45.939	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.880%
62) 4-Bromofluorobenzene	12.674	95	260167	47.431	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.860%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081222\
Data File : VN073849.D
Acq On : 12 Aug 2022 14:10
Operator : JC\MD
Sample : N4194-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Aug 13 05:02:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 05:09:32 2022
Response via : Initial Calibration




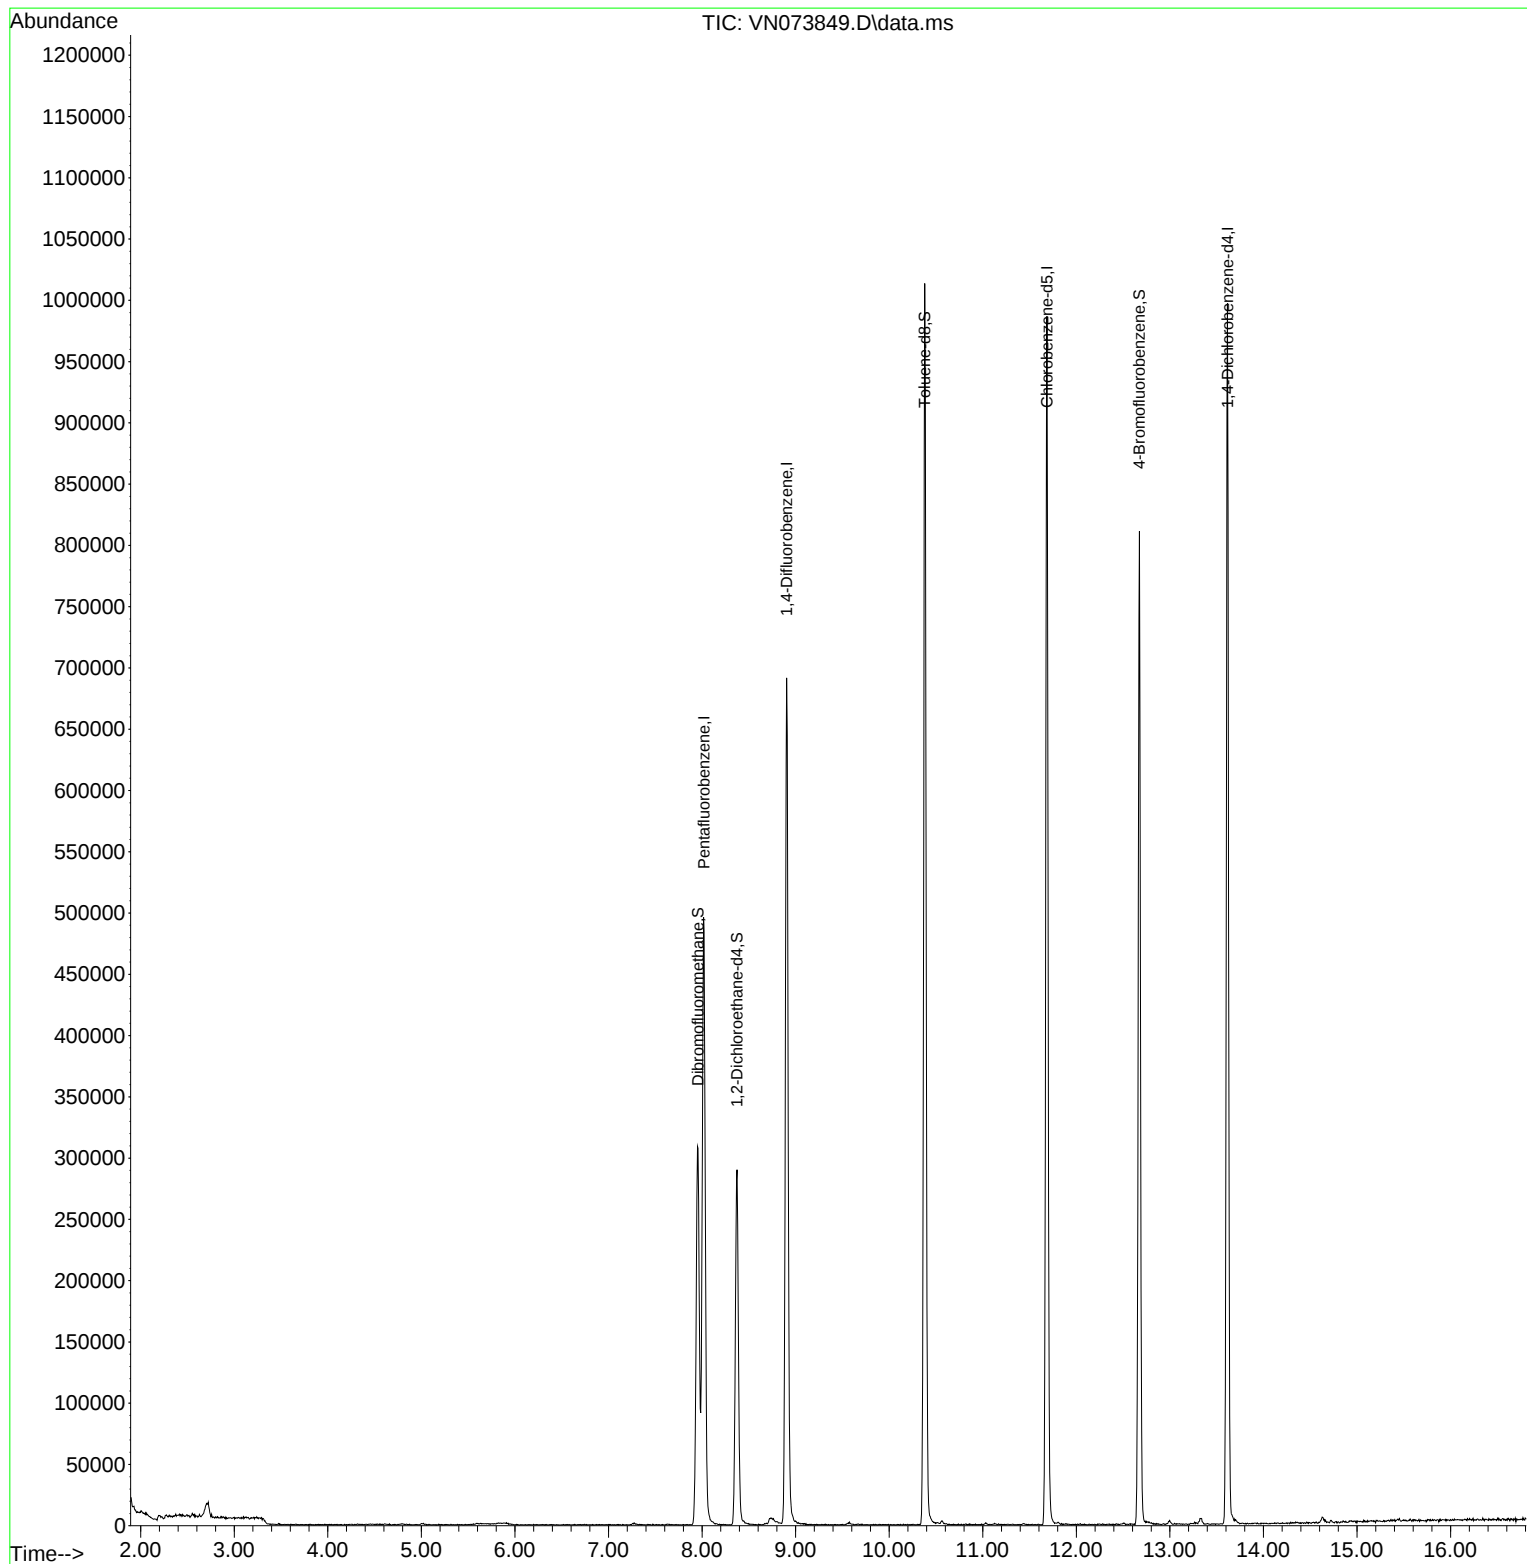


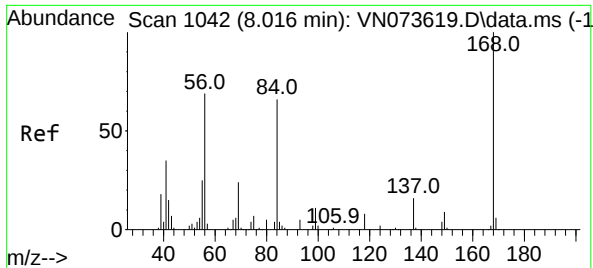

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073849.D
Acq: 12 Aug 2022 14:10




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 404324
Ion Ratio Lower Upper
168 100
99 49.5 42.3 63.5

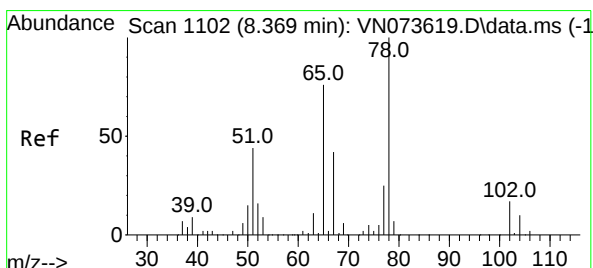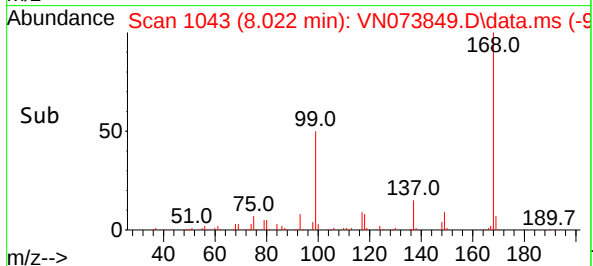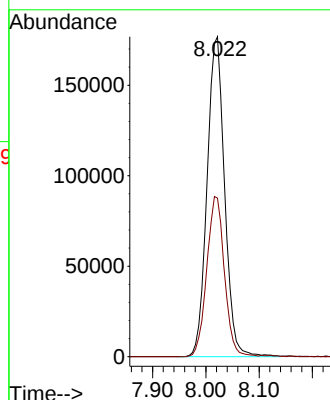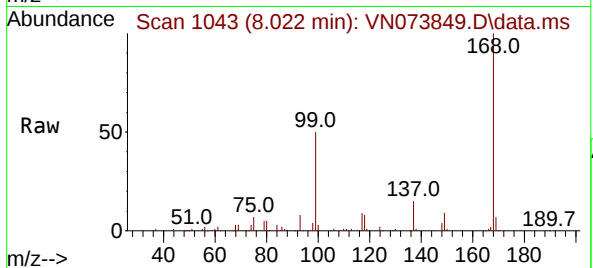

#33
1,2-Dichloroethane-d4
Concen: 49.373 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073849.D
Acq: 12 Aug 2022 14:10

Tgt Ion: 65 Resp: 243279
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.8

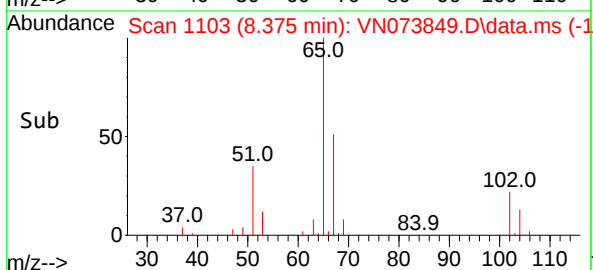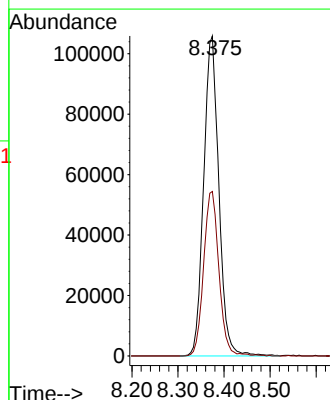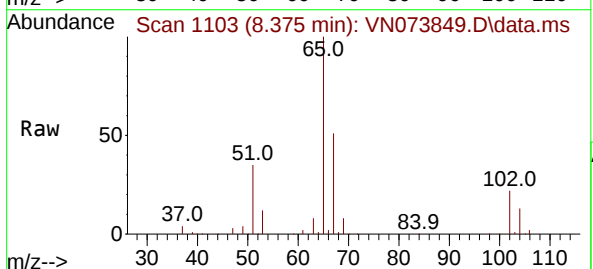

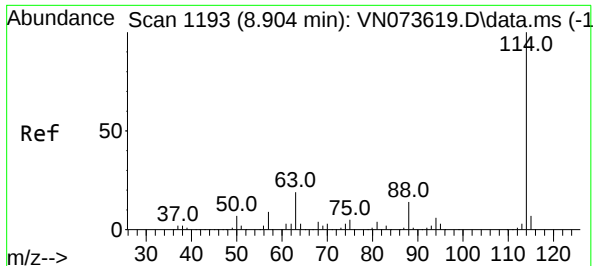

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN073849.D

Acq: 12 Aug 2022 14:10

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6





Tgt Ion:114 Resp: 634337

Ion Ratio Lower Upper

114 100

63 19.1 0.0 40.0

88 14.9 0.0 32.6

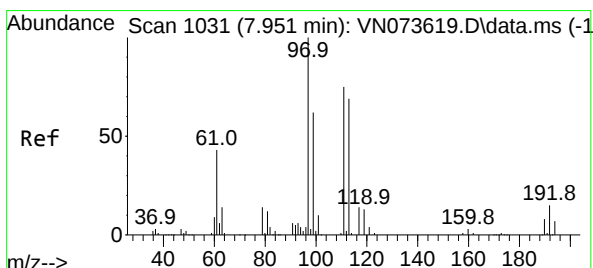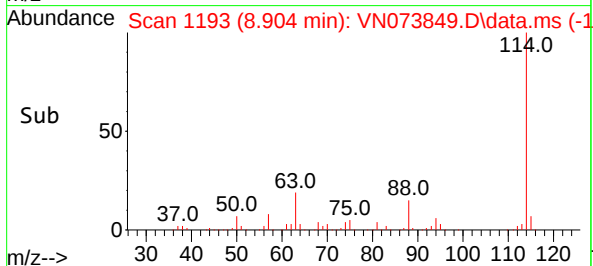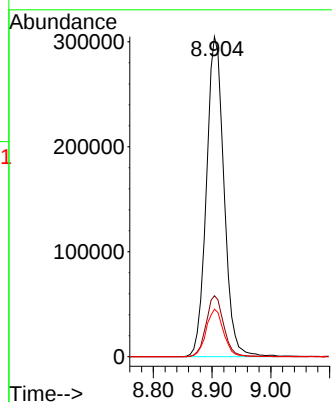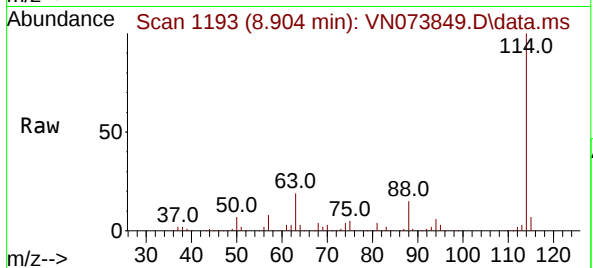

#35

Dibromofluoromethane

Concen: 57.165 ug/l

RT: 7.957 min Scan# 1032

Delta R.T. 0.006 min

Lab File: VN073849.D

Acq: 12 Aug 2022 14:10




Tgt Ion:113 Resp: 227701


Ion Ratio Lower Upper

113 100

111 102.4 81.4 122.0

192 21.9 17.0 25.6


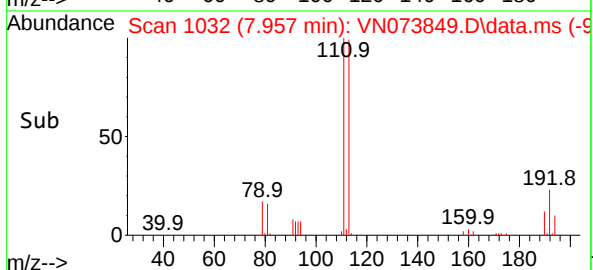
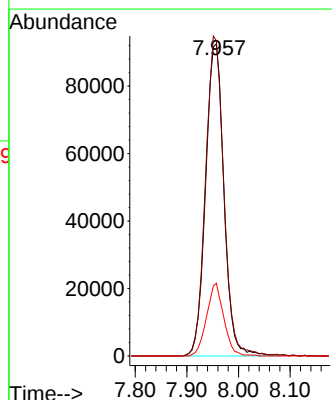
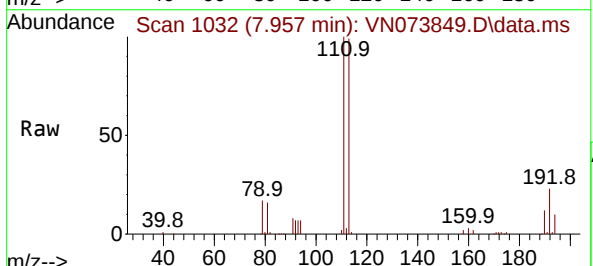


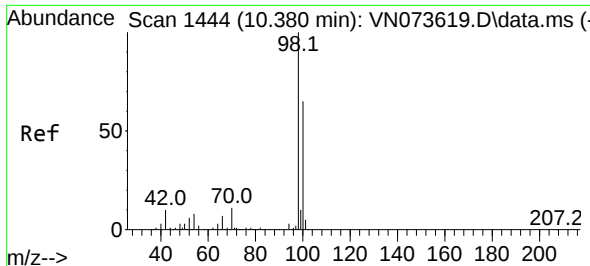

#50
Toluene-d8
Concen: 45.939 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073849.D
Acq: 12 Aug 2022 14:10




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 720074
Ion Ratio Lower Upper
98 100
100 63.9 52.6 78.8

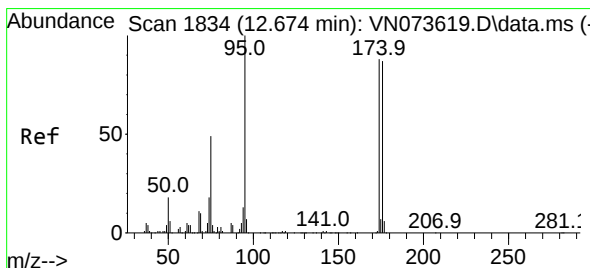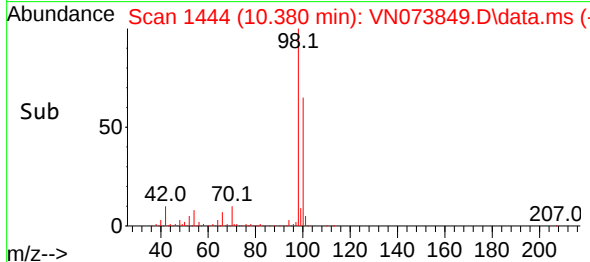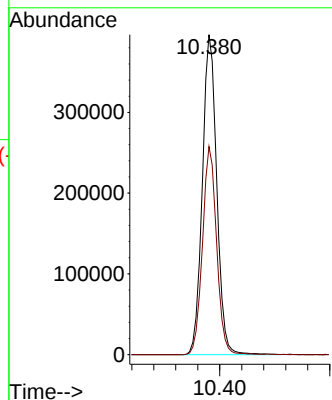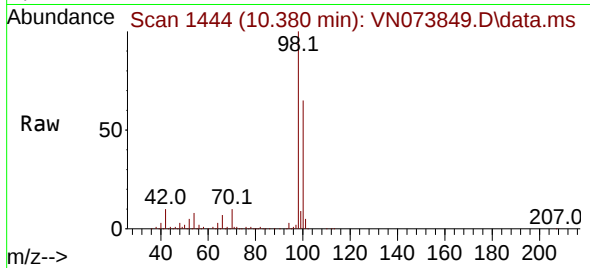

#62
4-Bromofluorobenzene
Concen: 47.431 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073849.D
Acq: 12 Aug 2022 14:10

Tgt Ion: 95 Resp: 260167
Ion Ratio Lower Upper
95 100
174 95.0 0.0 167.6
176 89.7 0.0 163.4

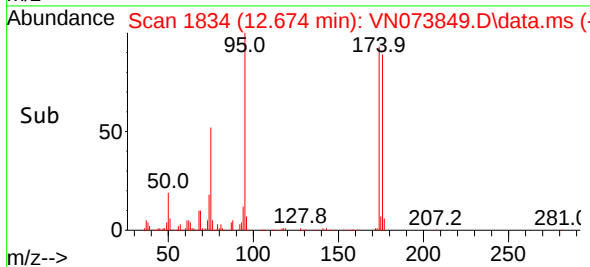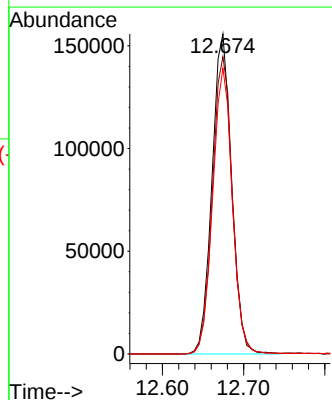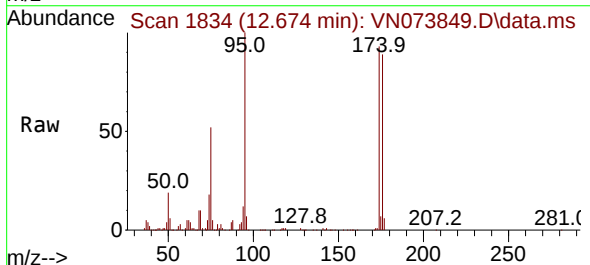

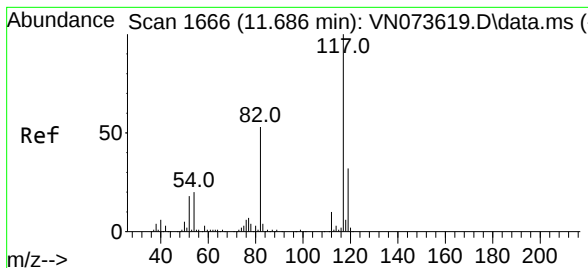

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.686 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN073849.D

Acq: 12 Aug 2022 14:10

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6





Tgt Ion:117 Resp: 590427

Ion Ratio Lower Upper

117 100

82 52.7 44.2 66.2

119 32.2 25.4 38.0

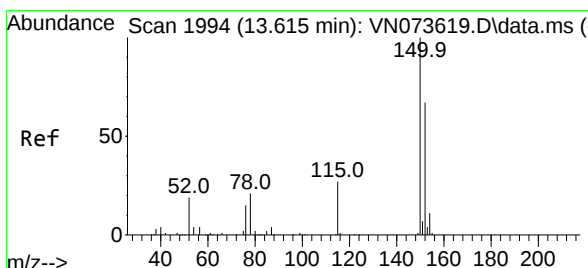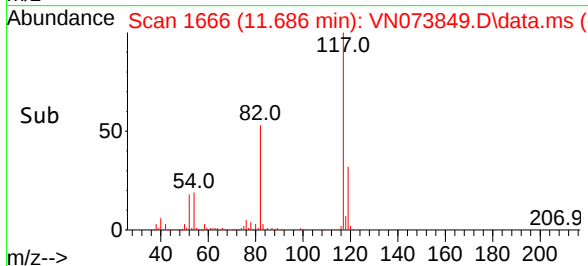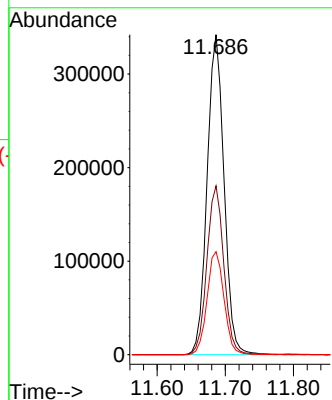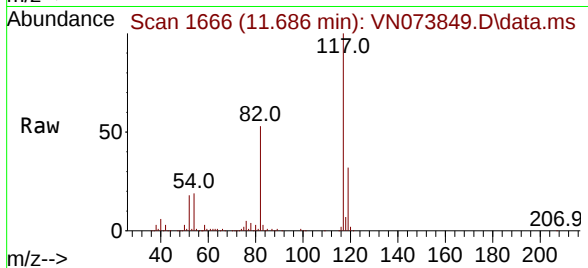

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.616 min Scan# 1994

Delta R.T. 0.000 min

Lab File: VN073849.D

Acq: 12 Aug 2022 14:10

Tgt Ion:152 Resp: 287020

Ion Ratio Lower Upper

152 100

115 55.3 28.9 86.7

150 157.6 0.0 356.2

