
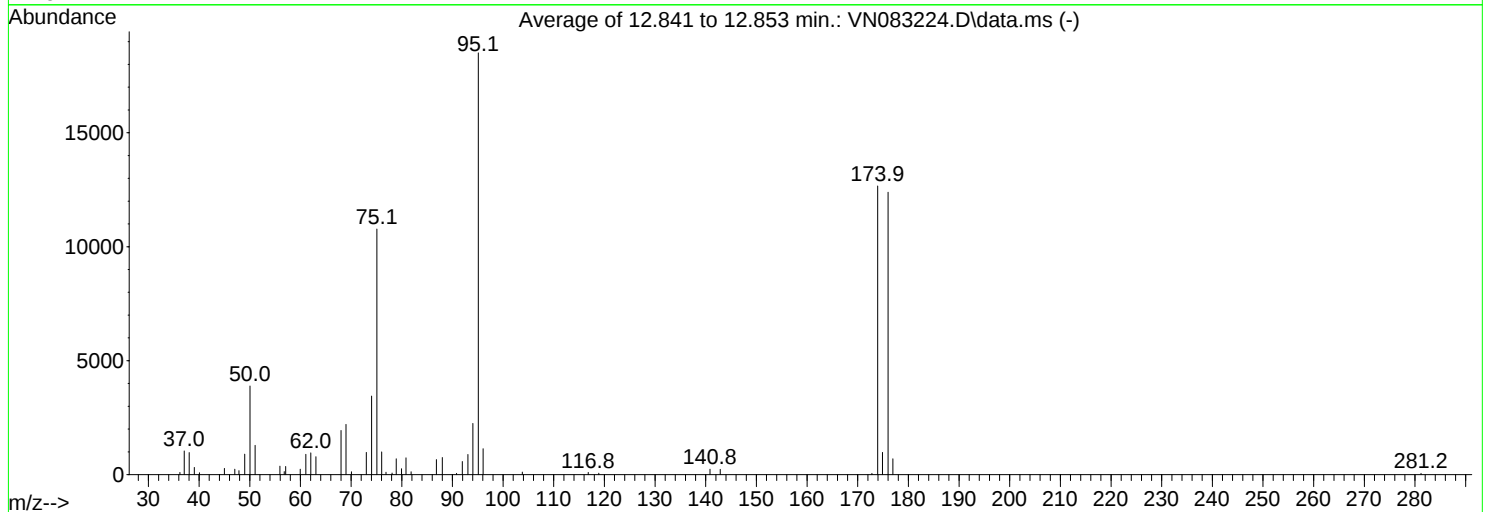


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081224\
Data File : VN083224.D
Acq On : 12 Aug 2024 08:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

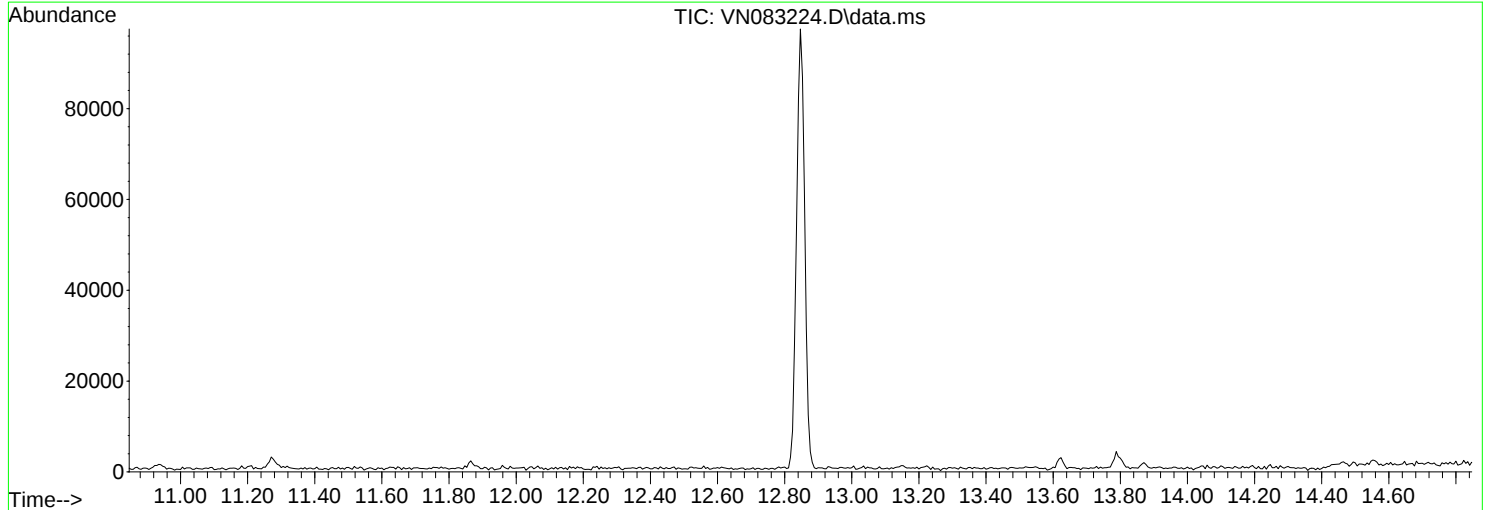

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	3887	PASS
75	95	30	60	58.2	10779	PASS
95	95	100	100	100.0	18507	PASS
96	95	5	9	6.1	1134	PASS
173	174	0.00	2	0.4	54	PASS
174	95	50	100	68.4	12665	PASS
175	174	5	9	7.7	977	PASS
176	174	95	101	97.9	12393	PASS
177	176	5	9	5.6	697	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.20	97	51.05	1282	73.00	973	88.00	75
37.05	1040	55.95	371	74.05	3448	90.80	5
38.05	972	56.80	136	75.10	10779	91.95	57
39.05	315	57.10	361	76.05	998	93.05	88
40.05	85	59.95	236	76.90	103	94.05	2244
44.00	7	61.05	889	78.10	68	95.10	18507
45.00	274	62.05	956	78.90	695	96.05	1134
47.05	238	63.05	788	79.95	257	103.80	111
47.85	177	68.00	1938	80.85	740	116.80	98
49.00	901	69.00	2208	81.85	130	118.90	63
50.05	3887	70.05	125	86.85	660	140.85	236

Average of 12.841 to 12.853 min.: VN083224.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.85	234						
172.80	54						
173.95	12665						
174.90	977						
176.00	12393						
176.95	697						
281.20	58						

Instrument :

MSVOA_N

ClientSampleId :

BFB