


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081318\
Data File : VN050557.D
Acq On : 13 Aug 2018 9:26
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Title : SW846 8260
Last Update : Tue Aug 07 05:22:15 2018

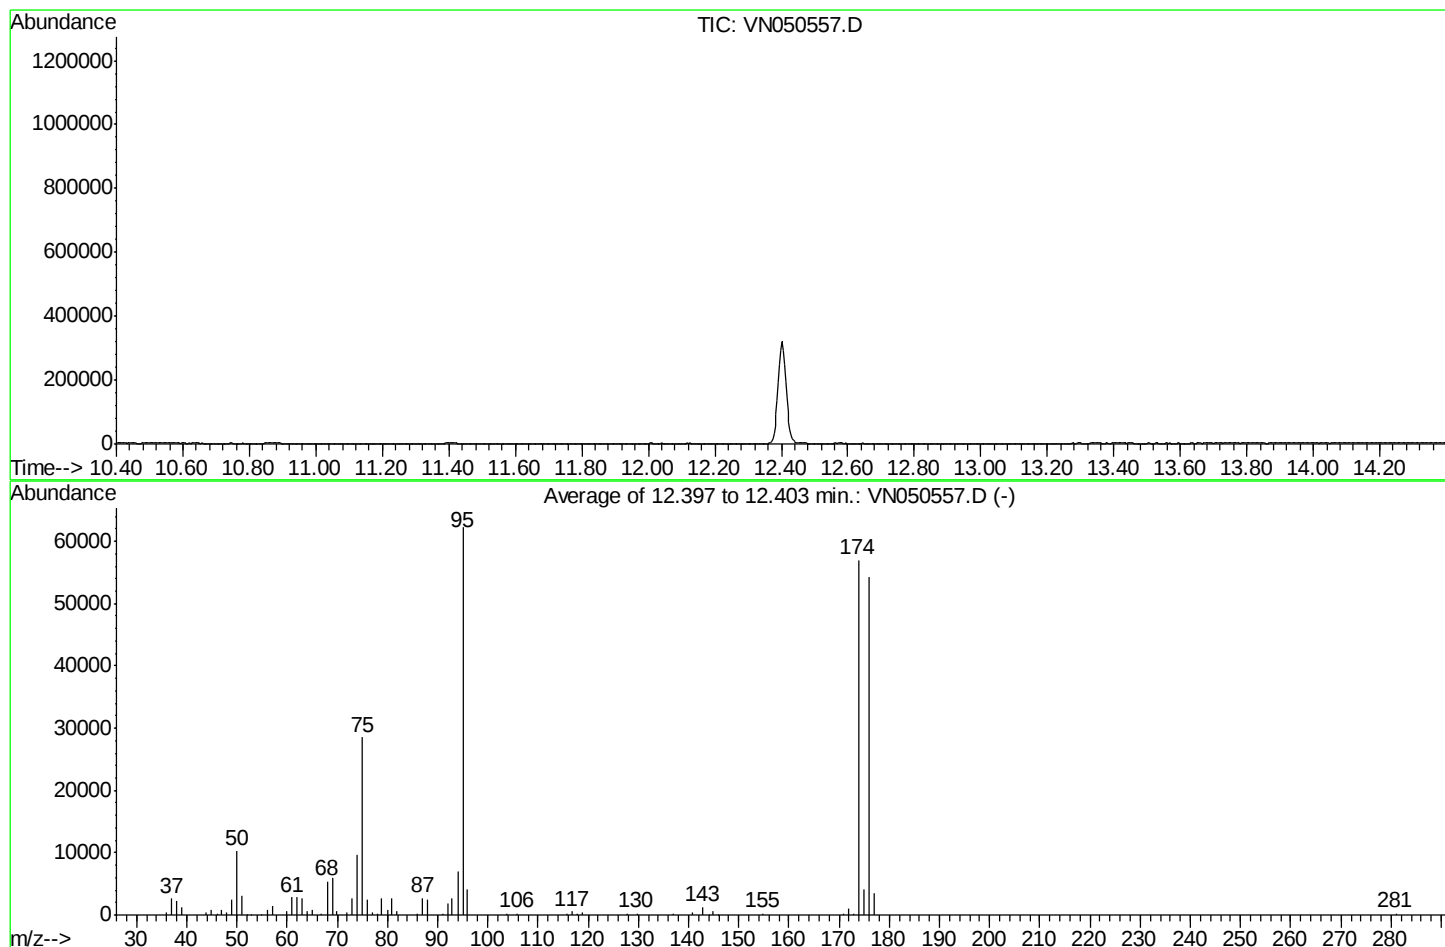

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	10281	PASS
75	95	30	60	45.8	28482	PASS
95	95	100	100	100.0	62237	PASS
96	95	5	9	6.5	4071	PASS
173	174	0.00	2	0.5	274	PASS
174	95	50	100	91.6	57013	PASS
175	174	5	9	7.4	4211	PASS
176	174	95	101	95.3	54306	PASS
177	176	5	9	6.4	3482	PASS