

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081319\
 Data File : VN057263.D
 Acq On : 13 Aug 2019 22:15
 Operator : JC/SP
 Sample : K4266-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 R1-R2-A3-(0)

Quant Time: Aug 14 07:39:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081319W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 14 06:25:03 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	1524546	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	2121192	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1771893	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	450154	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.02	65	692052	45.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.00%	
35) Dibromofluoromethane	7.58	113	623210	46.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.02%	
50) Toluene-d8	10.09	98	2467182	49.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.88%	
62) 4-Bromofluorobenzene	12.40	95	649668	38.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	76.70%	
Target Compounds						
16) Acetone	3.81	43	29799	5.652	ug/l	99
20) Methylene Chloride	4.55	84	47780	3.102	ug/l	97
43) Isopropyl Acetate	8.16	43	198173	8.073	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN081319\
Data File : VN057263.D
Acq On : 13 Aug 2019 22:15
Operator : JC/SP
Sample : K4266-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
R1-R2-A3-(0)

Quant Time: Aug 14 07:39:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081319W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 14 06:25:03 2019
Response via : Initial Calibration

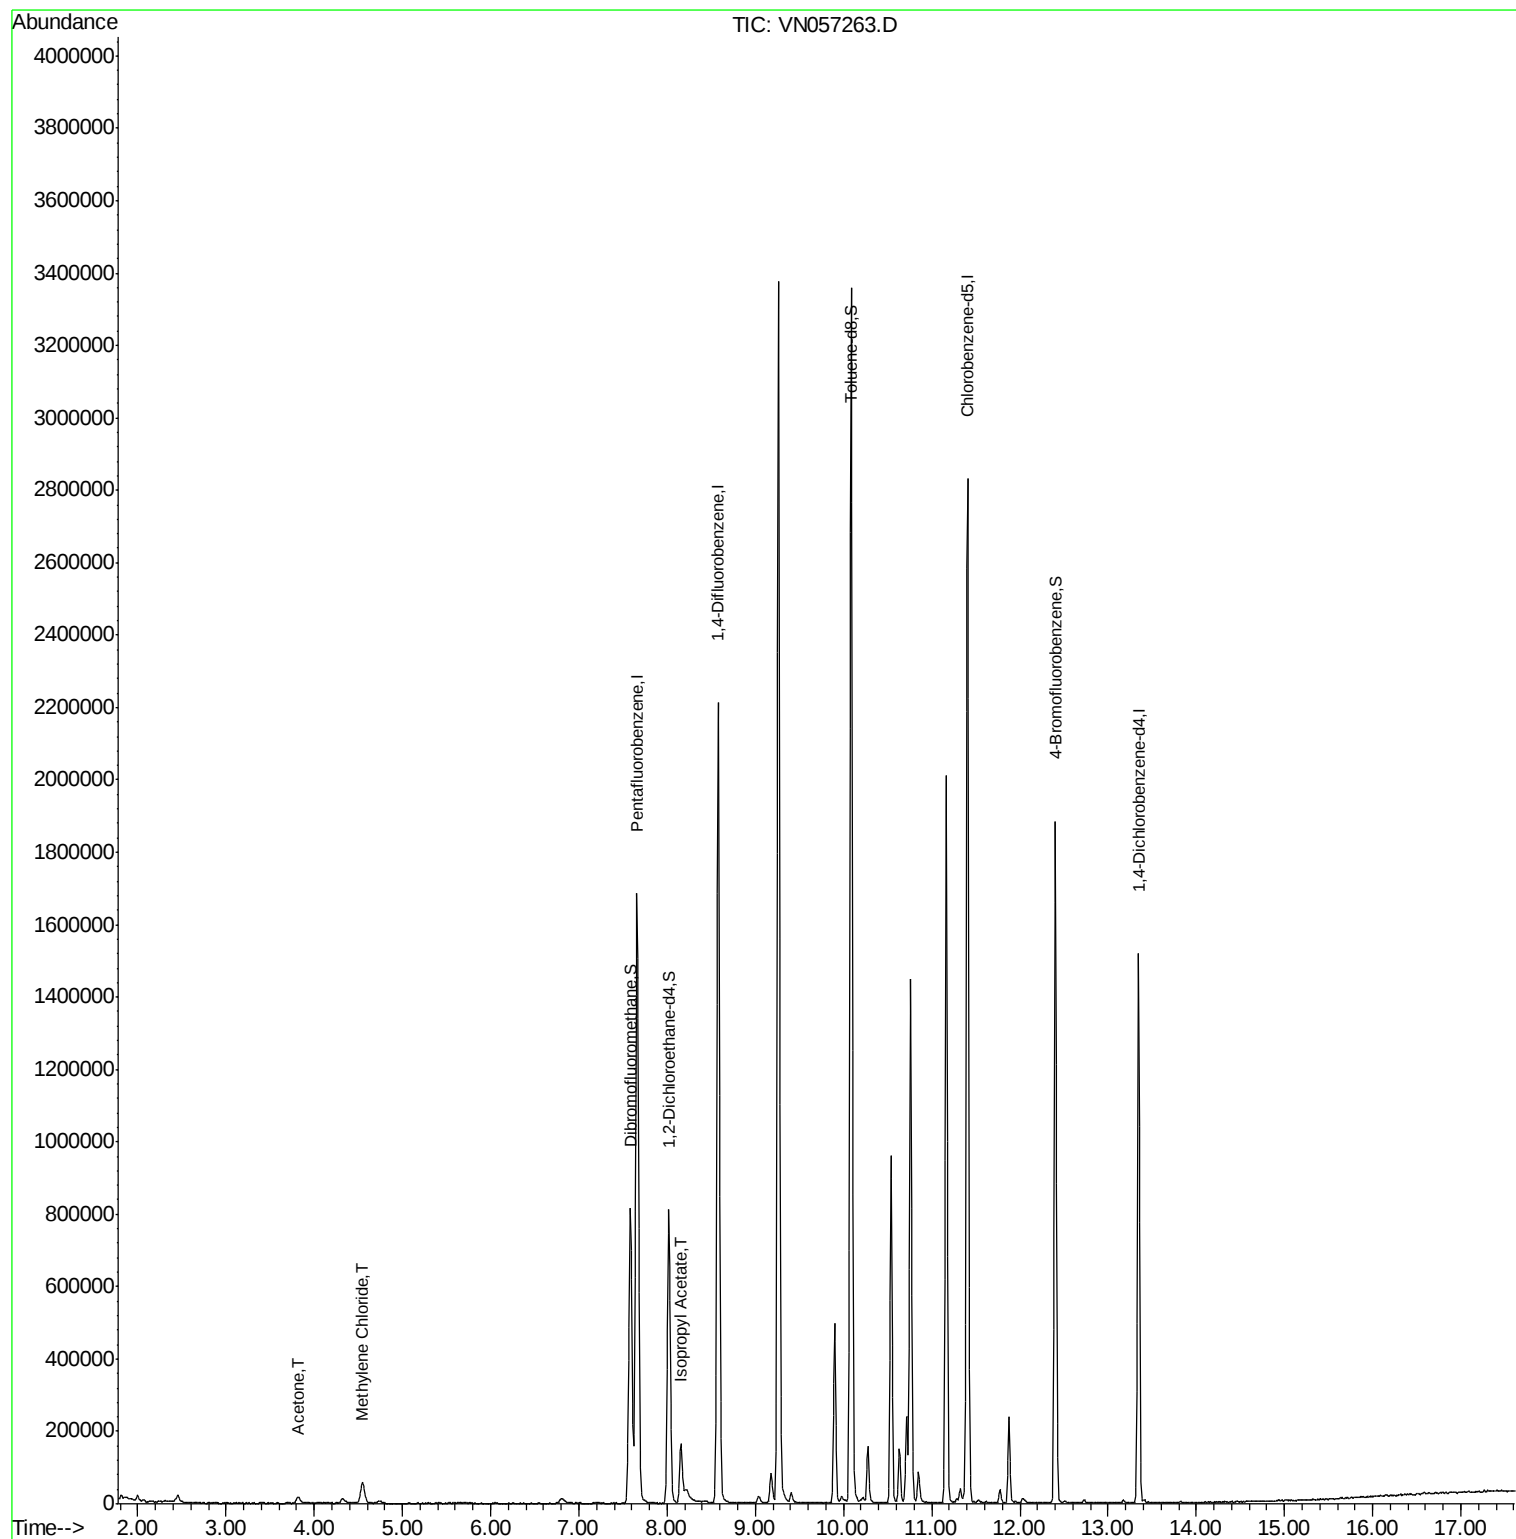

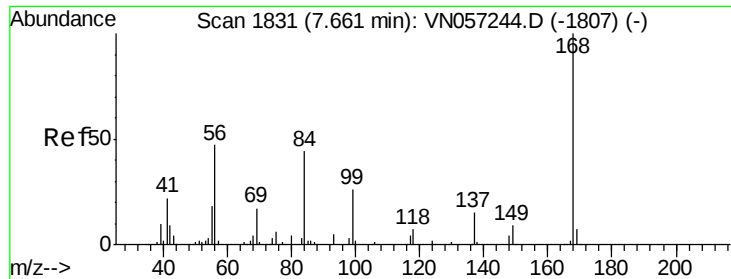

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15

Instrument :

MSVOA_N

ClientSampleId :


R1-R2-A3-(0)

Tot Ion:168 Resp: 1524546

Ion Ratio Lower Upper

168 100

99 48.8 38.6 58.0

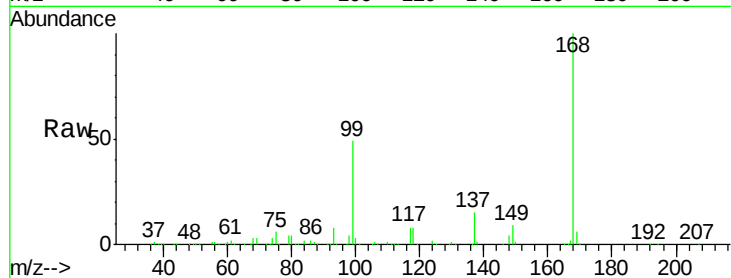

Abundance Ion 167.90 (167.60 to 168.60): VN057244.D (-1807) (-)

Ion 98.90 (98.60 to 99.60): VN057244.D (-1807) (-)

7.66



600000

400000

200000

0

Time--> 7.50 7.60 7.70 7.80

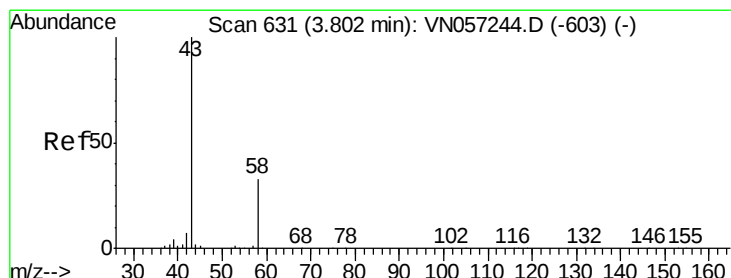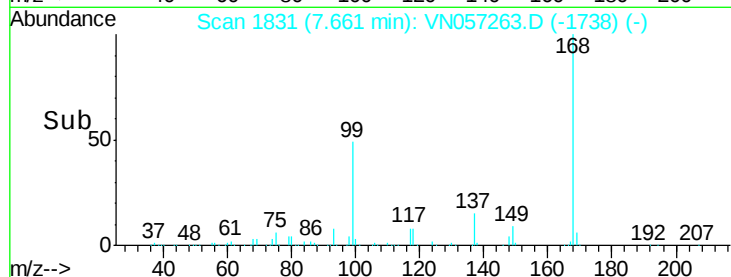

#16

Acetone

Concen: 5.652 ug/l

RT: 3.81 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN057263.D


Acq: 13 Aug 2019 22:15

Tgt Ion: 43 Resp: 29799

Ion Ratio Lower Upper

43 100

58 32.7 26.7 40.1

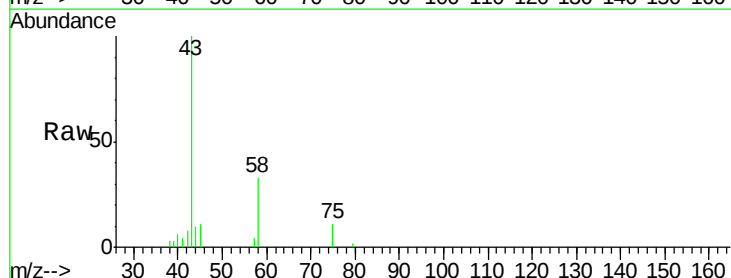

Abundance Ion 43.00 (42.70 to 43.70): VN057244.D (-603) (-)

Ion 58.00 (57.70 to 58.70): VN057244.D (-603) (-)

3.81

10000

8000


6000


4000

2000

0

Time--> 3.70 3.75 3.80 3.85 3.90




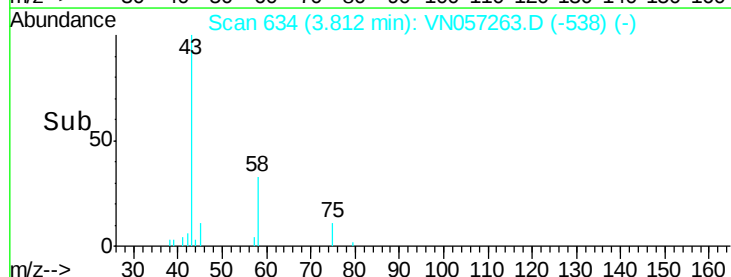


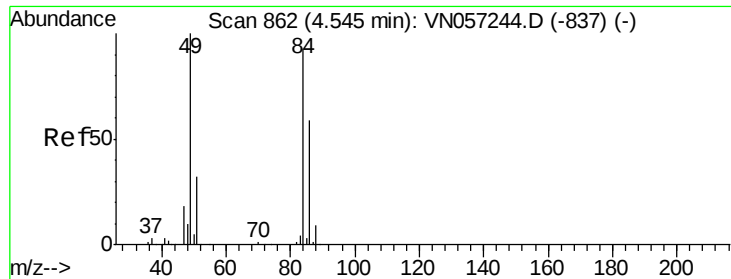

#20
Methylene Chloride
Concen: 3.102 ug/l
RT: 4.55 min Scan# 863
Delta R.T. 0.00 min
Lab File: VN057263.D
Acq: 13 Aug 2019 22:15




Instrument :
MSVOA_N
ClientSampleId :
R1-R2-A3-(0)


Tot Ion: 84 Resp: 47780
Ion Ratio Lower Upper
84 100
49 104.3 85.9 128.9
51 34.1 27.1 40.7
86 61.4 51.0 76.6

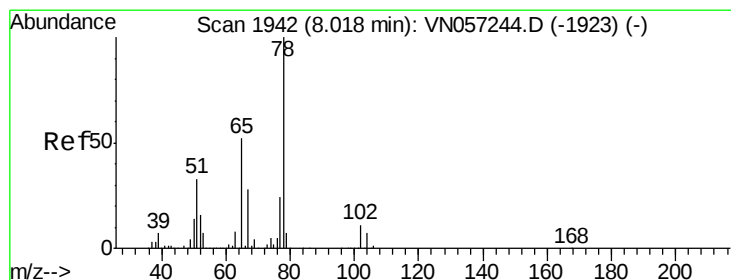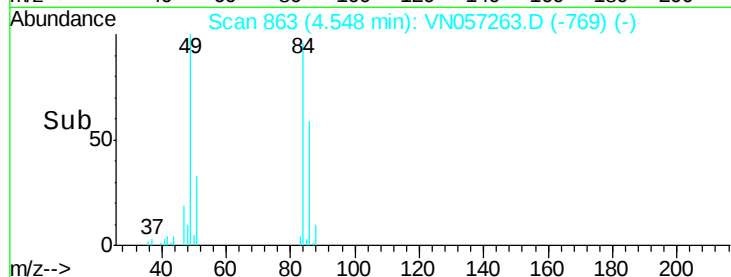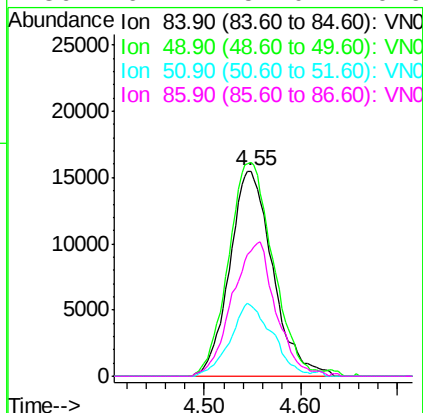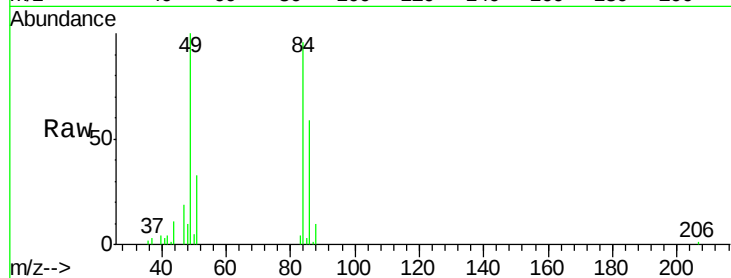

#33
1,2-Dichloroethane-d4
Concen: 44.999 ug/l
RT: 8.02 min Scan# 1943
Delta R.T. 0.00 min
Lab File: VN057263.D
Acq: 13 Aug 2019 22:15

Tgt Ion: 65 Resp: 692052
Ion Ratio Lower Upper
65 100
67 54.5 0.0 107.0

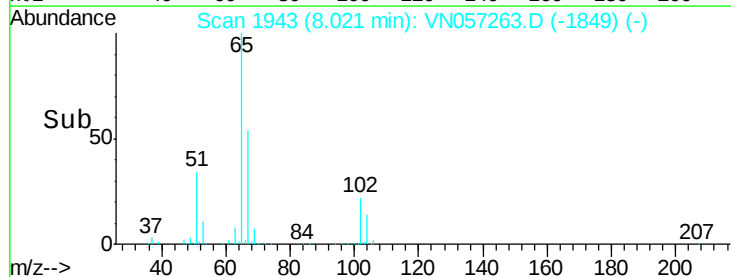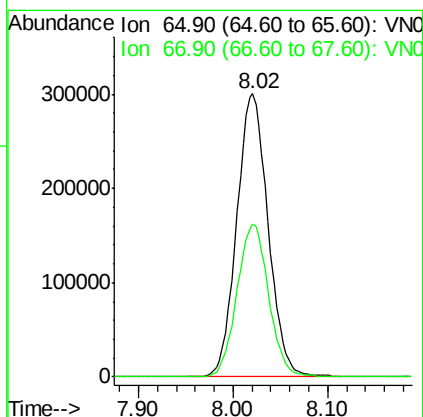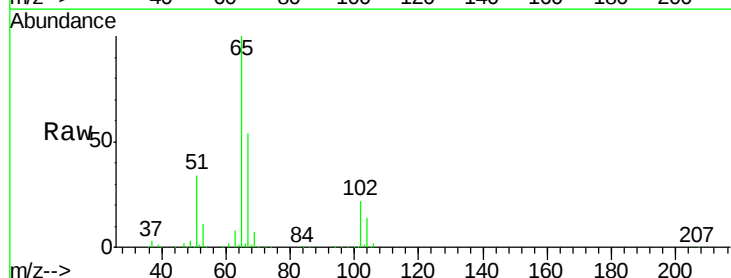

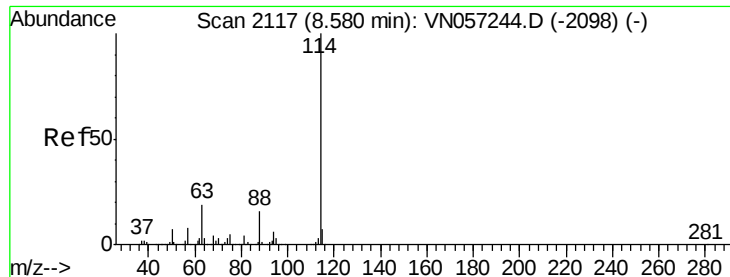

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.58 min Scan# 2117

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15

Instrument :

MSVOA_N

ClientSampleId :

R1-R2-A3-(0)


Tot Ion:114 Resp: 2121192

Ion Ratio Lower Upper

114 100

63 18.8 0.0 37.0




88 15.5 0.0 31.0

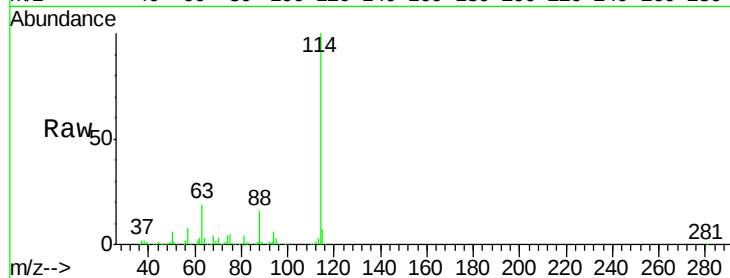

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

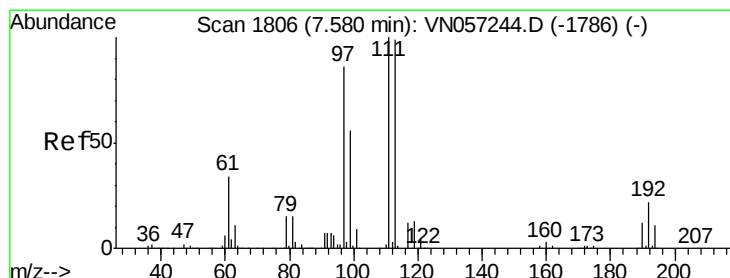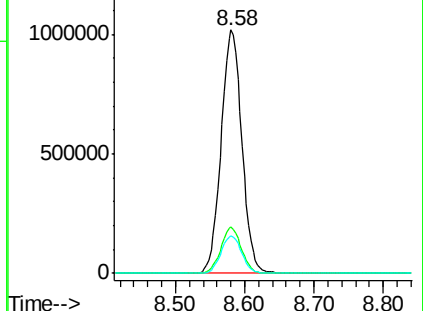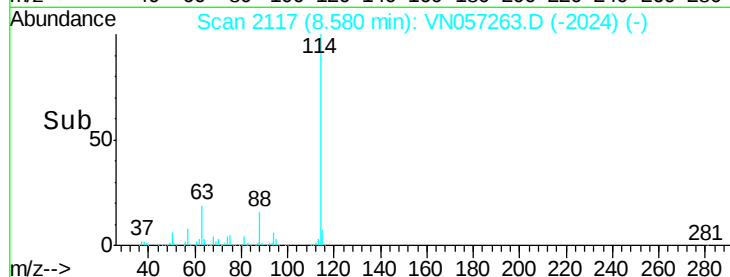

#35

Dibromofluoromethane

Concen: 46.013 ug/l

RT: 7.58 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15


Tgt Ion:113 Resp: 623210

Ion Ratio Lower Upper

113 100

111 104.3 81.4 122.2



192 24.0 18.8 28.2

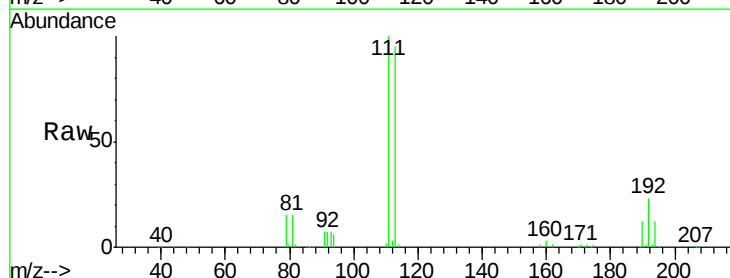


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

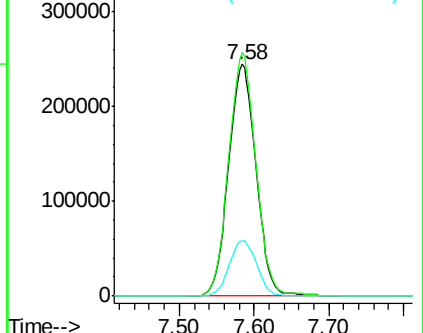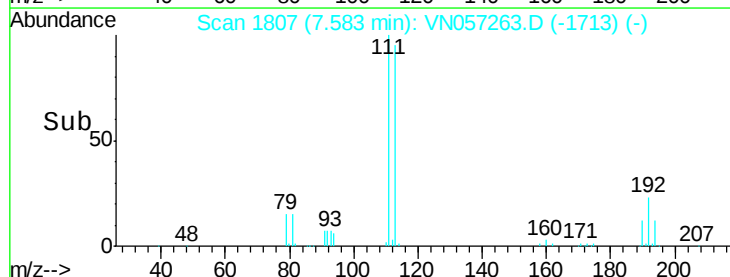

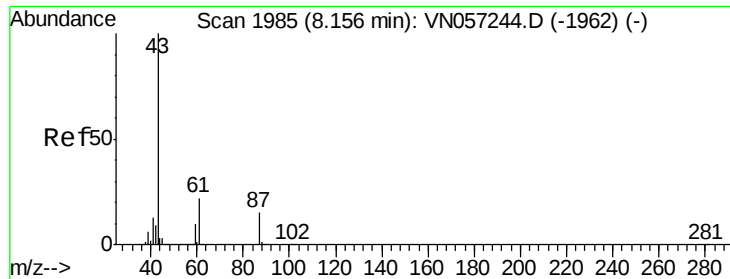

#43

Isopropyl Acetate

Concen: 8.073 ug/l

RT: 8.16 min Scan# 1985

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15

Instrument :

MSVOA_N

ClientSampleId :

R1-R2-A3-(0)


Tot Ion: 43 Resp: 198173

Ion Ratio Lower Upper

43 100

61 20.7 23.5 35.3#




87 14.1 12.1 18.1

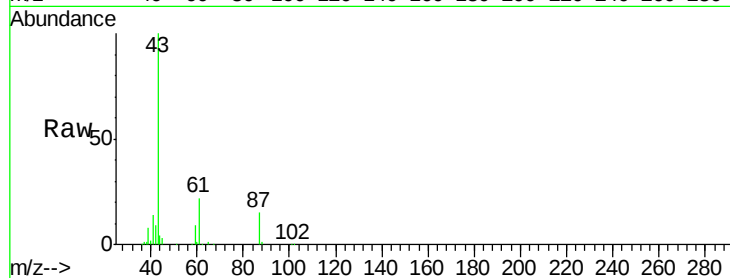

Abundance Ion 43.00 (42.70 to 43.70): VN057244.D (-1962) (-)

Ion 61.00 (60.70 to 61.70): VN057244.D (-1962) (-)

Ion 87.00 (86.70 to 87.70): VN057244.D (-1962) (-)

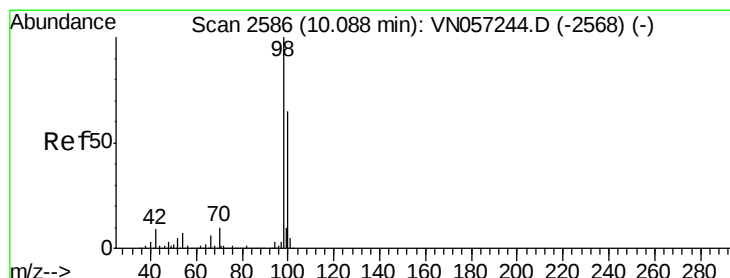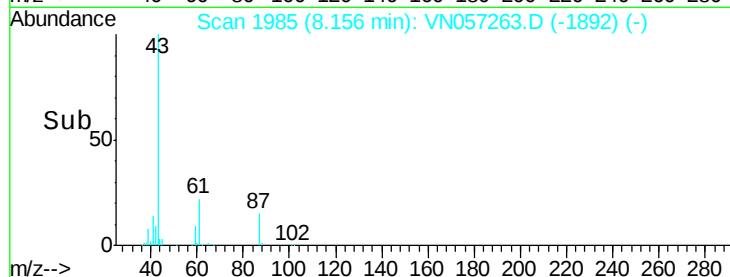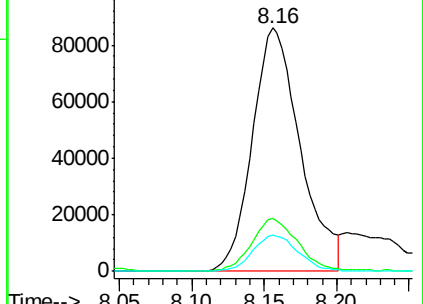

#50

Toluene-d8

Concen: 49.942 ug/l

RT: 10.09 min Scan# 2586

Delta R.T. 0.00 min

Lab File: VN057263.D


Acq: 13 Aug 2019 22:15

Tgt Ion: 98 Resp: 2467182

Ion Ratio Lower Upper



98 100


100 64.5 51.8 77.6

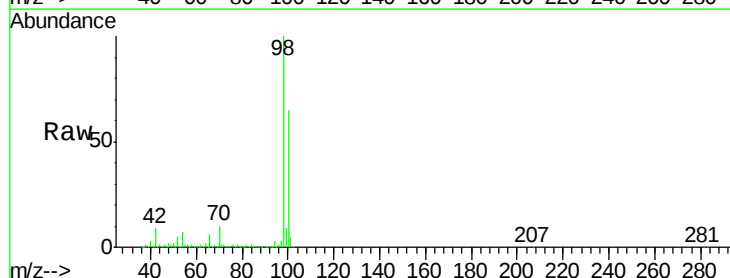

Abundance Ion 98.00 (97.70 to 98.70): VN057244.D (-2568) (-)

Ion 100.00 (99.70 to 100.70): VN057244.D (-2568) (-)

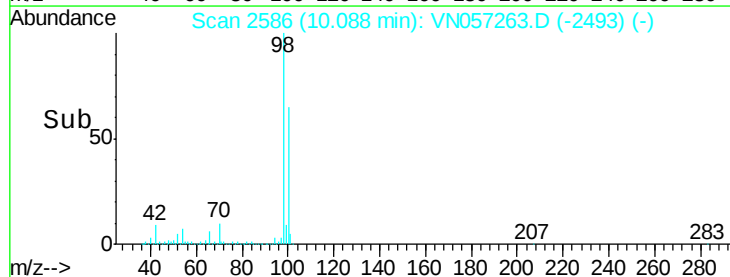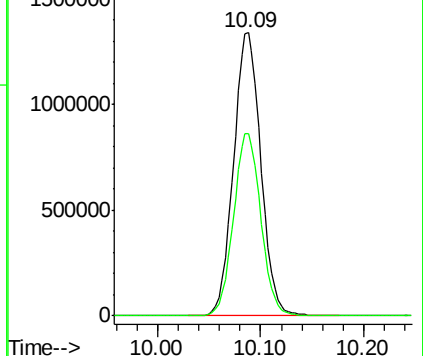

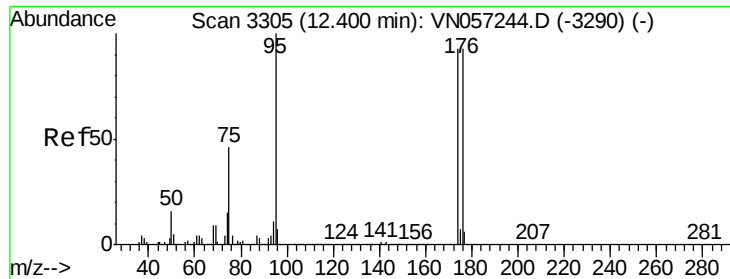

#62

4-Bromofluorobenzene

Concen: 38.347 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15

Instrument :

MSVOA_N

ClientSampleId :

R1-R2-A3-(0)


Tot Ion: 95 Resp: 649668

Ion Ratio Lower Upper

95 100

174 95.4 0.0 187.6




176 92.8 0.0 185.8

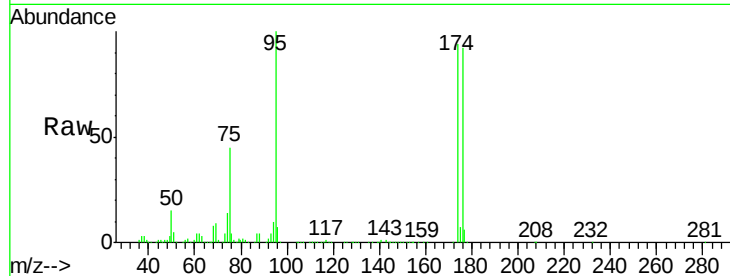

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): VN0

Ion 175.80 (175.50 to 176.50): VN0

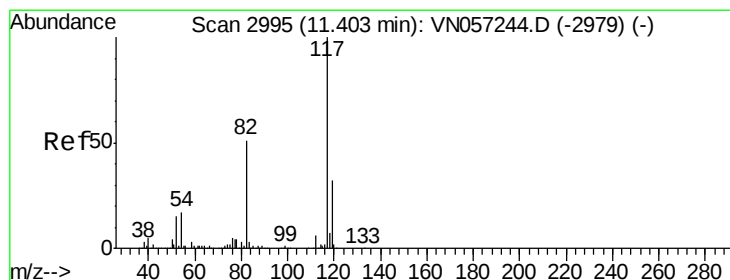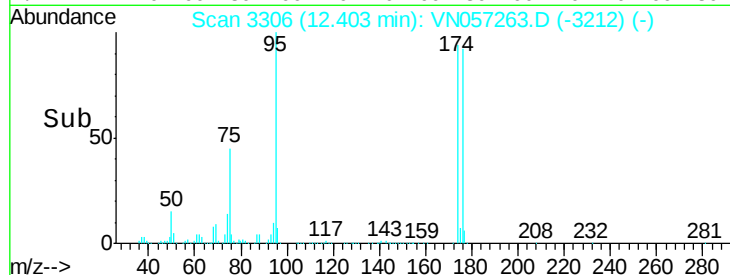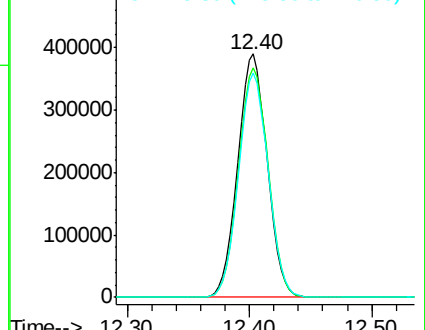

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15


Tgt Ion: 117 Resp: 1771893

Ion Ratio Lower Upper

117 100

82 50.2 40.9 61.3



119 32.2 25.4 38.2

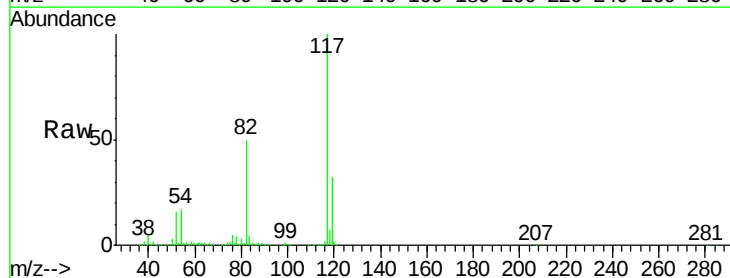


Abundance Ion 116.90 (116.60 to 117.60): VN0

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): VN0

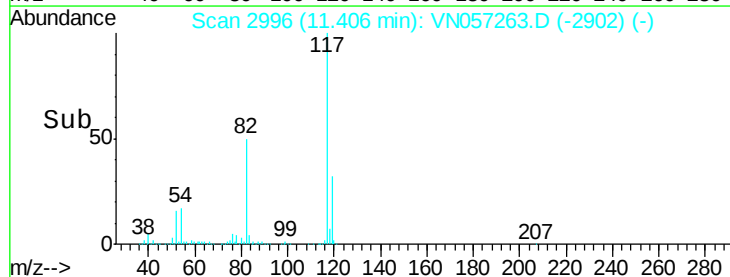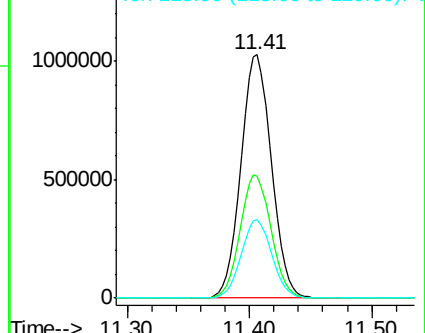

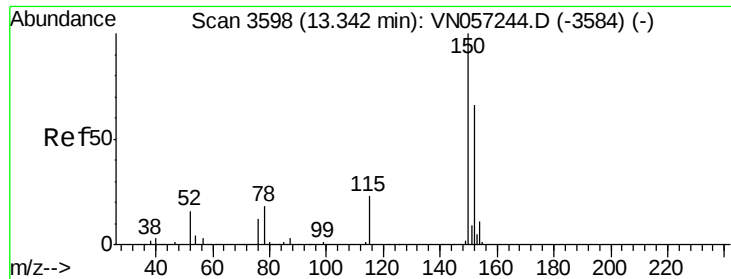

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. 0.00 min

Lab File: VN057263.D

Acq: 13 Aug 2019 22:15

Instrument :

MSVOA_N

ClientSampleId :

R1-R2-A3-(0)


Tot Ion:152 Resp: 450154

Ion Ratio Lower Upper

152 100

115 55.5 27.6 82.8

150 156.8 0.0 348.4

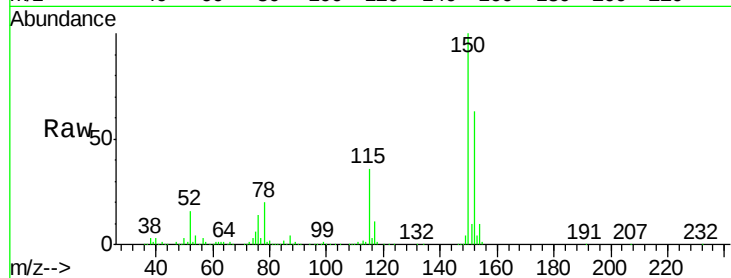

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

