


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081319\
Data File : VN057239.D
Acq On : 13 Aug 2019 9:26
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081319W.M
Title : SW846 8260
Last Update : Wed Aug 14 06:25:03 2019

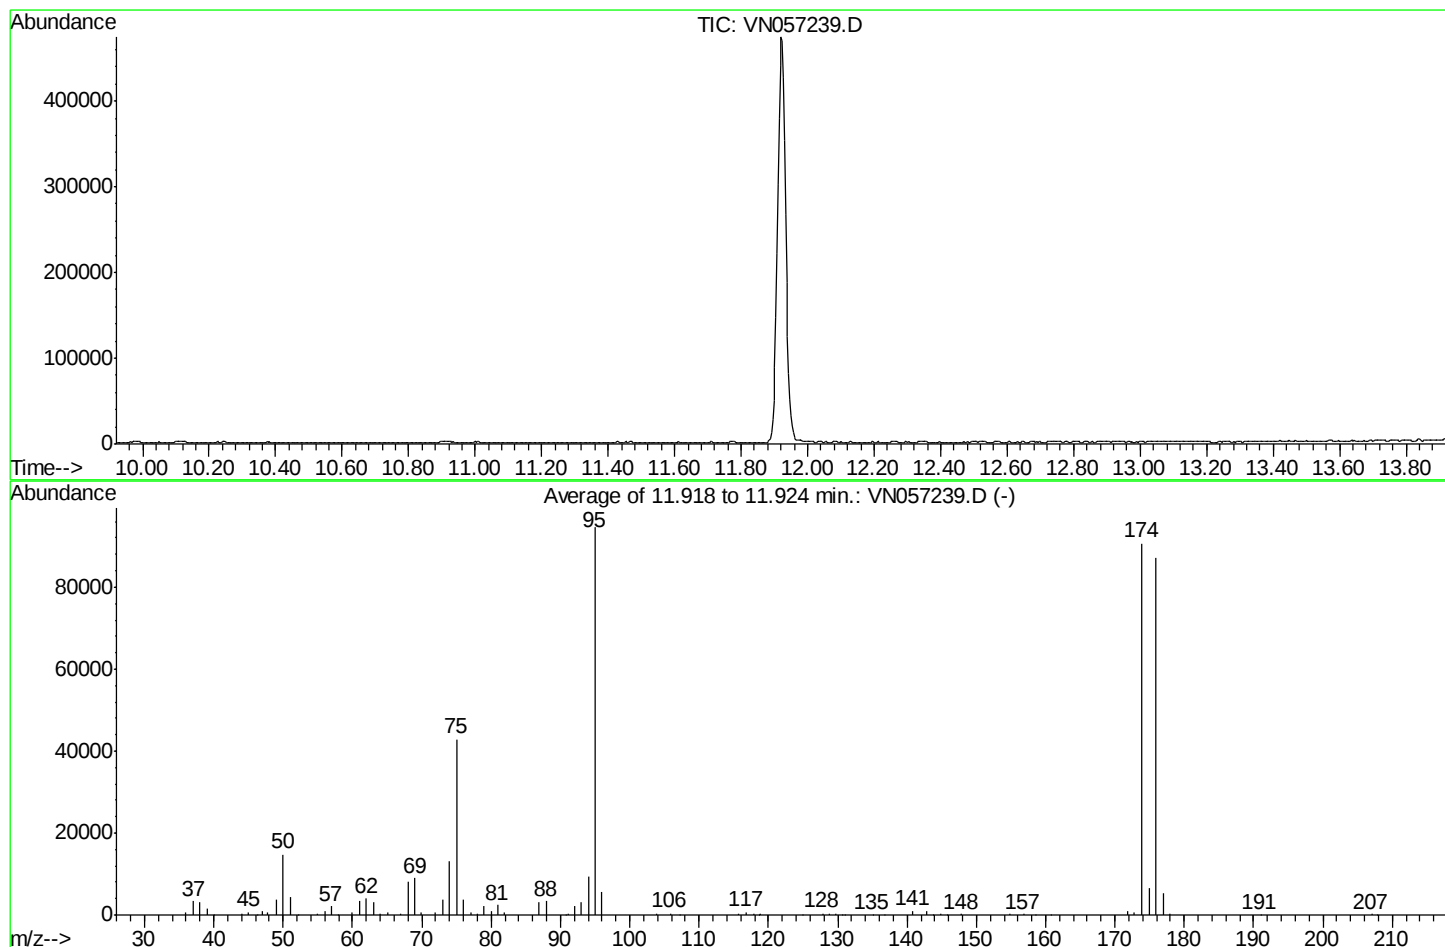

AutoFind: Scans 3155, 3156, 3157; Background Corrected with Scan 3141

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	14797	PASS
75	95	30	60	45.3	42864	PASS
95	95	100	100	100.0	94597	PASS
96	95	5	9	6.1	5728	PASS
173	174	0.00	2	0.7	598	PASS
174	95	50	100	95.9	90688	PASS
175	174	5	9	7.3	6650	PASS
176	174	95	101	96.2	87213	PASS
177	176	5	9	6.2	5389	PASS