


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081319\
 Data File : VN057248.D
 Acq On : 13 Aug 2019 15:41
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081319W.M
 Title : SW846 8260
 Last Update : Wed Aug 14 06:25:03 2019

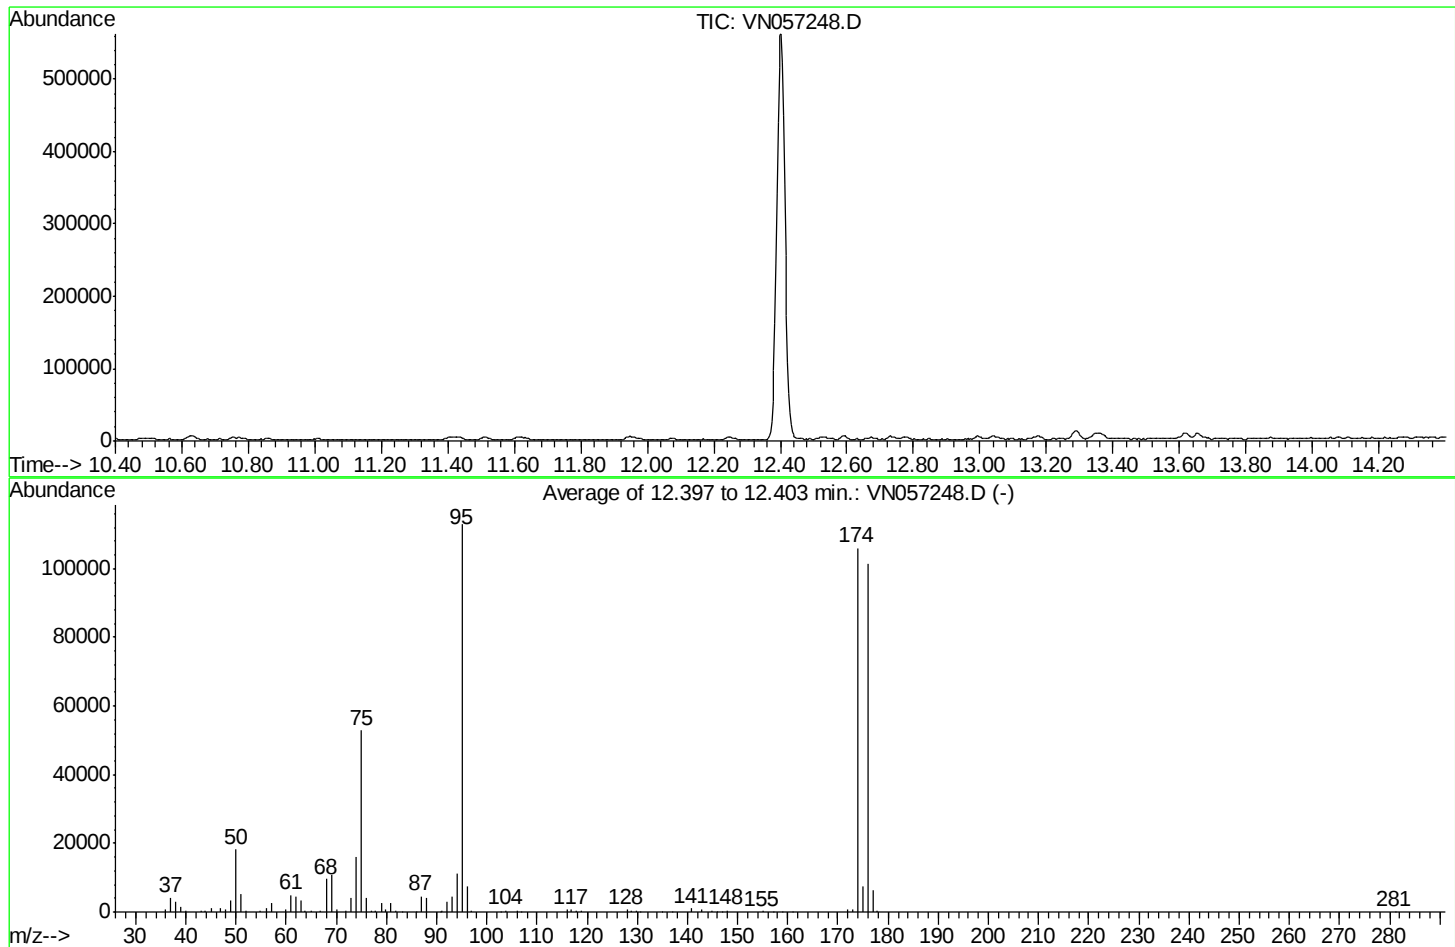

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	18178	PASS
75	95	30	60	46.8	52840	PASS
95	95	100	100	100.0	112938	PASS
96	95	5	9	6.5	7348	PASS
173	174	0.00	2	0.8	862	PASS
174	95	50	100	93.8	105920	PASS
175	174	5	9	7.2	7606	PASS
176	174	95	101	95.9	101549	PASS
177	176	5	9	6.3	6434	PASS