

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
 Data File : VN073871.D
 Acq On : 13 Aug 2022 16:25
 Operator : JC\MD
 Sample : N4156-04DL 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FMC-0074DL

Quant Time: Aug 14 02:35:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	612468	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	872482	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	807936	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	412144	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	306029	41.001	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	82.000%
35) Dibromofluoromethane	7.951	113	295174	53.877	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.760%
50) Toluene-d8	10.380	98	996506	46.222	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.440%
62) 4-Bromofluorobenzene	12.674	95	382277	50.482	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.960%
Target Compounds						
					Qvalue	
3) Chloromethane	2.269	50	1333	Below Cal		93
5) Bromomethane	2.810	94	3086	0.512 ug/l	#	66
6) Chloroethane	2.987	64	66	Below Cal	#	42
10) Methyl Iodide	4.340	142	1753	0.291 ug/l	#	70
13) Acrolein	3.981	56	663	0.415 ug/l		89
16) Acetone	4.228	43	24916	6.215 ug/l		100
18) Methyl Acetate	4.787	43	6968	0.699 ug/l		95
20) Methylene Chloride	5.016	84	4555	Below Cal		91
25) 2-Butanone	7.269	43	12151	1.952 ug/l		99
29) Tetrahydrofuran	7.628	42	1102	0.280 ug/l	#	84
31) Cyclohexane	8.016	56	9395	0.845 ug/l	#	1
36) 1,1-Dichloropropene	8.016	75	36178	4.633 ug/l	#	50
37) Ethyl Acetate	7.339	43	4093	0.398 ug/l	#	78
38) Carbon Tetrachloride	8.016	117	52267	6.591 ug/l	#	16
43) Isopropyl Acetate	8.498	43	11935	0.859 ug/l	#	90
48) Methyl methacrylate	9.475	41	3847	0.633 ug/l	#	41
49) 1,4-Dioxane	9.510	88	86	0.502 ug/l	#	25
51) 4-Methyl-2-Pentanone	10.269	43	5880	0.590 ug/l		87
52) Toluene	10.445	92	49902	3.222 ug/l		100
58) 2-Chloroethyl Vinyl ether	9.986	63	212	9.985 ug/l	#	44
59) 2-Hexanone	11.033	43	8936	1.184 ug/l		68
68) m/p-Xylenes	11.892	106	3684	0.334 ug/l		94
76) 1,2,3-Trichloropropane	12.674	75	191439	23.657 ug/l	#	1
81) trans-1,4-Dichloro-2-b...	12.674	75	191439	60.195 ug/l	#	10
84) 1,2,4-Trimethylbenzene	13.310	105	9239	0.378 ug/l		100
92) 1,2-Dibromo-3-Chloropr...	14.551	75	559	0.239 ug/l		72
93) 1,2,4-Trichlorobenzene	15.198	180	3541	0.491 ug/l		97
95) Naphthalene	15.433	128	18762	0.801 ug/l		100
96) 1,2,3-Trichlorobenzene	15.627	180	4208	0.554 ug/l		97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
Data File : VN073871.D
Acq On : 13 Aug 2022 16:25
Operator : JC\MD
Sample : N4156-04DL 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL

Quant Time: Aug 14 02:35:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 05:09:32 2022
Response via : Initial Calibration




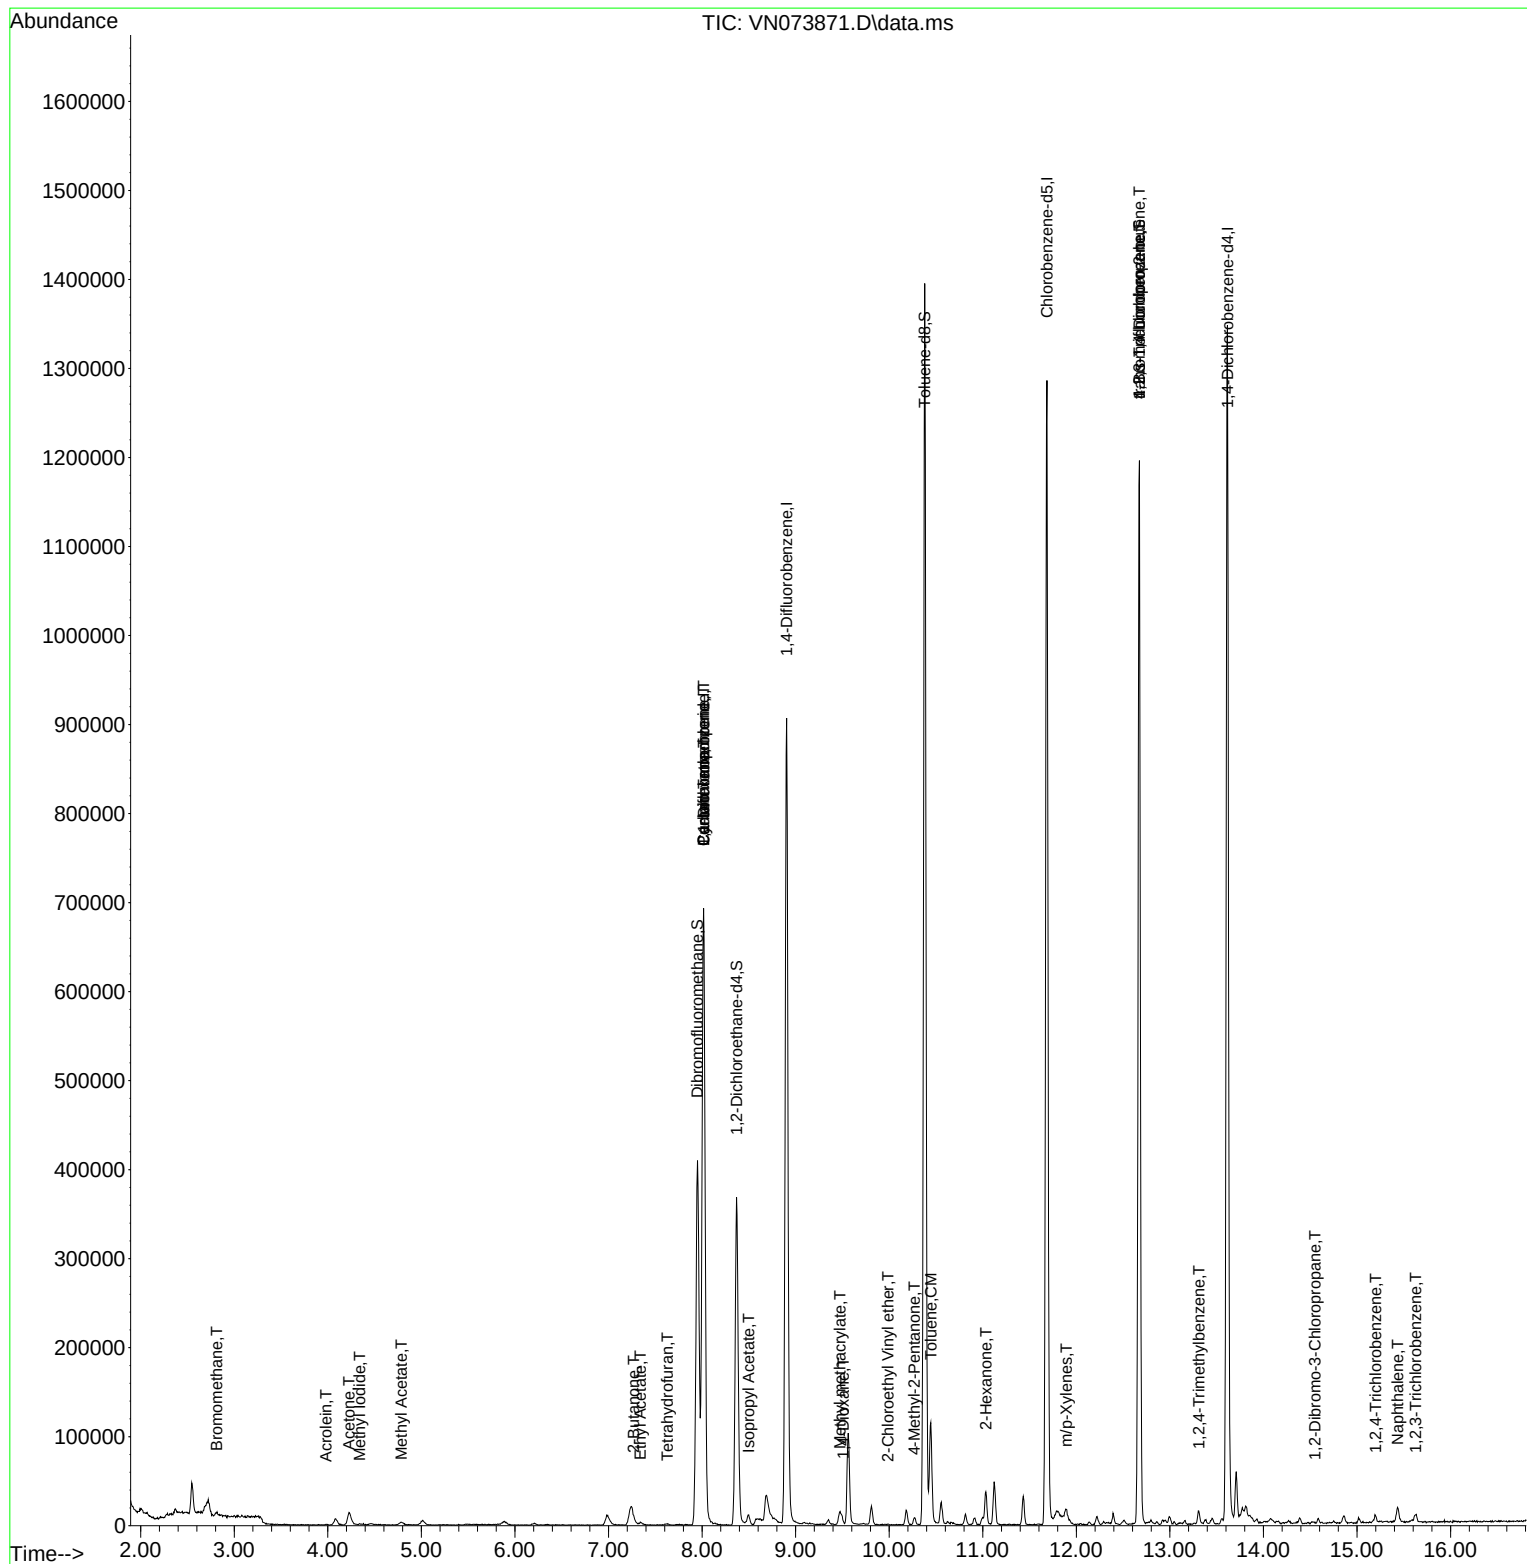




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion:168 Resp: 612468
Ion Ratio Lower Upper
168 100
99 48.8 42.3 63.5

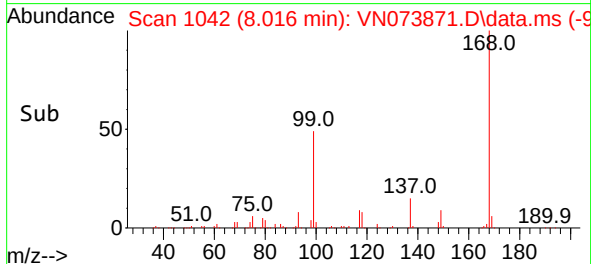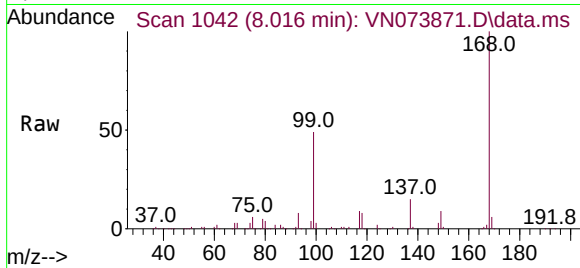

#3
Chloromethane
Concen: Below Cal
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 50 Resp: 1333
Ion Ratio Lower Upper
50 100
52 35.9 25.7 38.5


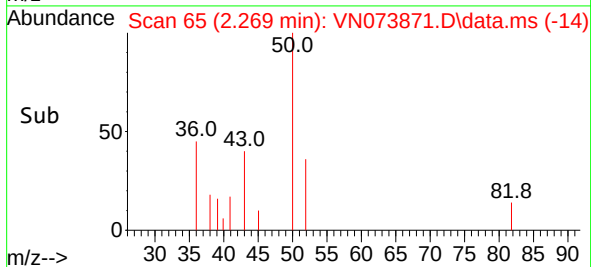

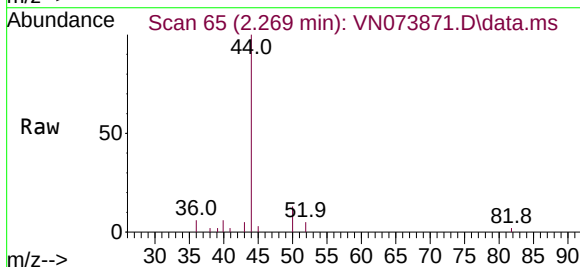




#5
Bromomethane
Concen: 0.512 ug/l
RT: 2.810 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion: 94 Resp: 3086
Ion Ratio Lower Upper
94 100
96 62.1 76.0 114.0#

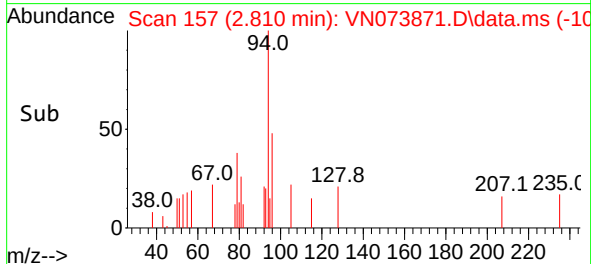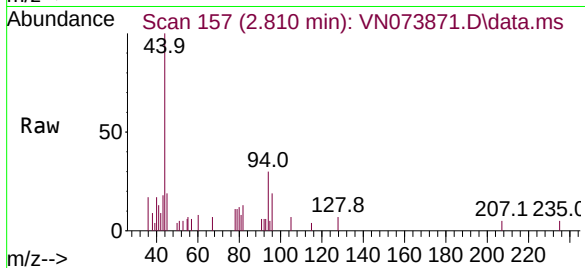

#6
Chloroethane
Concen: Below Cal
RT: 2.987 min Scan# 187
Delta R.T. 0.030 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 64 Resp: 66
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#


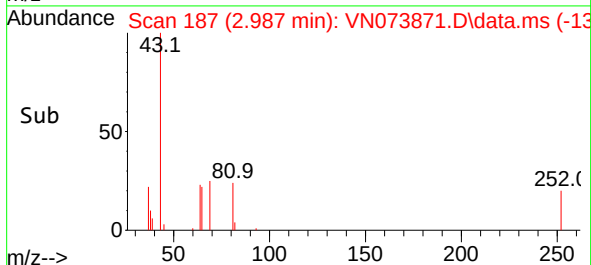

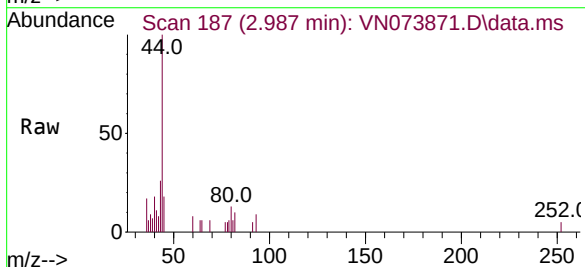




#10
Methyl Iodide
Concen: 0.291 ug/l
RT: 4.340 min Scan# 419
Delta R.T. -0.012 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion:142 Resp: 1753
Ion Ratio Lower Upper
142 100
127 19.7 31.3 46.9#
141 3.7 11.2 16.8#

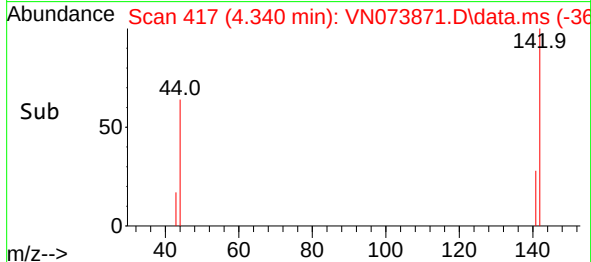

#13
Acrolein
Concen: 0.415 ug/l
RT: 3.981 min Scan# 356
Delta R.T. -0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 56 Resp: 663
Ion Ratio Lower Upper
56 100
55 59.6 54.8 82.2

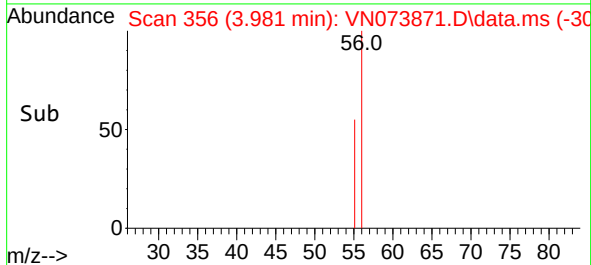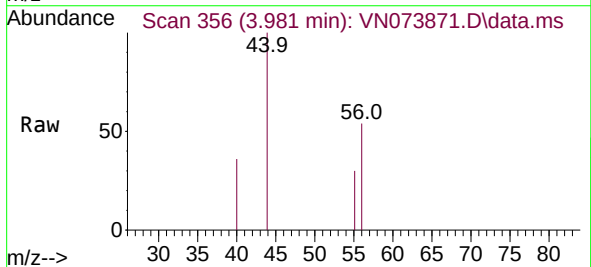



#16

Acetone

Concen: 6.215 ug/l

RT: 4.228 min Scan# 397

Delta R.T. 0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :





FMC-0074DL

Tgt Ion: 43 Resp: 24916

Ion Ratio Lower Upper

43 100

58 32.7 26.0 39.0

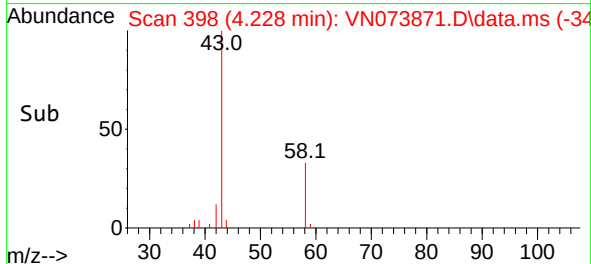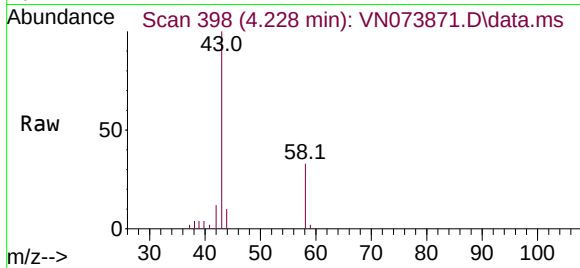

#18

Methyl Acetate

Concen: 0.699 ug/l

RT: 4.787 min Scan# 493

Delta R.T. 0.006 min

Lab File: VN073871.D




Acq: 13 Aug 2022 16:25


Tgt Ion: 43 Resp: 6968

Ion Ratio Lower Upper

43 100

74 29.7 21.6 32.4

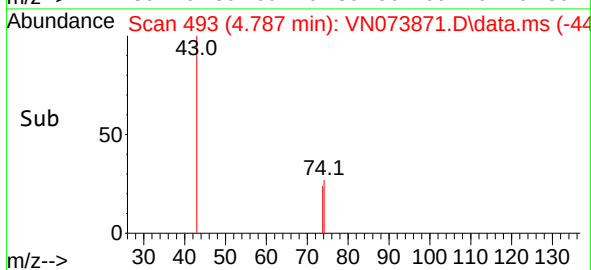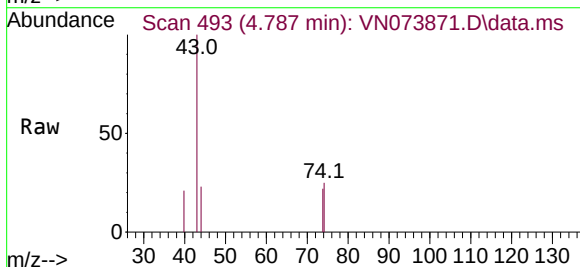



#20

Methylene Chloride

Concen: Below Cal

RT: 5.016 min Scan# 51

Delta R.T. 0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

FMC-0074DL

Tgt Ion: 84 Resp: 4555





Ion Ratio Lower Upper

84 100

49 96.6 88.3 132.5

51 37.2 28.2 42.2

86 59.5 50.6 76.0

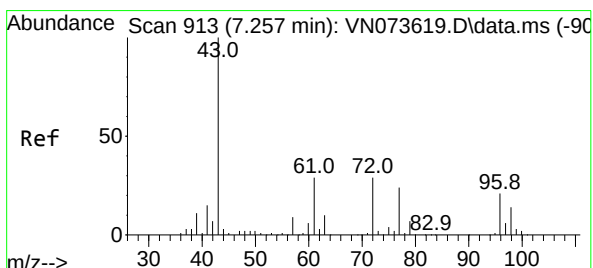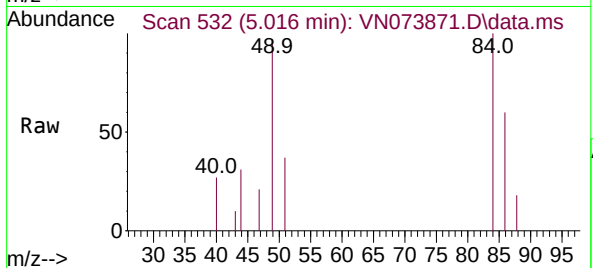

#25

2-Butanone

Concen: 1.952 ug/l

RT: 7.269 min Scan# 915

Delta R.T. 0.012 min

Lab File: VN073871.D




Acq: 13 Aug 2022 16:25


Tgt Ion: 43 Resp: 12151

Ion Ratio Lower Upper

43 100

72 30.2 23.7 35.5

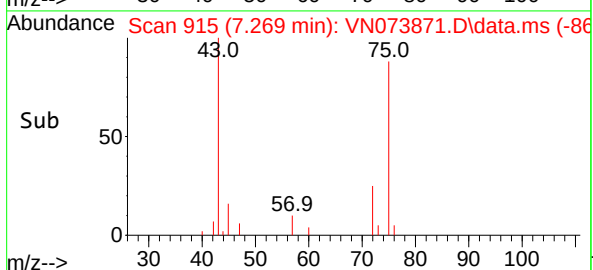



#29

Tetrahydrofuran

Concen: 0.280 ug/l

RT: 7.628 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

FMC-0074DL





Tgt Ion: 42 Resp: 1102

Ion Ratio Lower Upper

42 100

72 29.9 39.7 59.5#

71 43.8 36.6 55.0

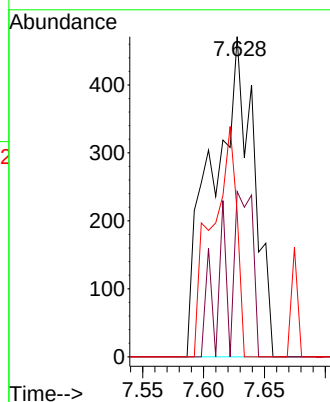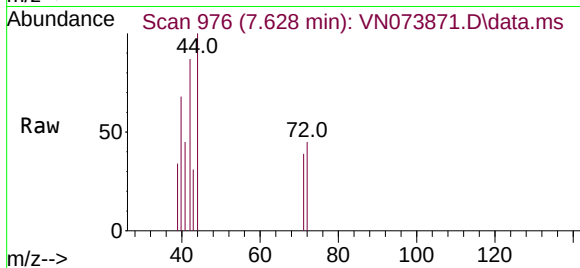

#31

Cyclohexane

Concen: 0.845 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25




Tgt Ion: 56 Resp: 9395


Ion Ratio Lower Upper

56 100

69 198.3 27.8 41.8#

84 145.8 76.9 115.3#

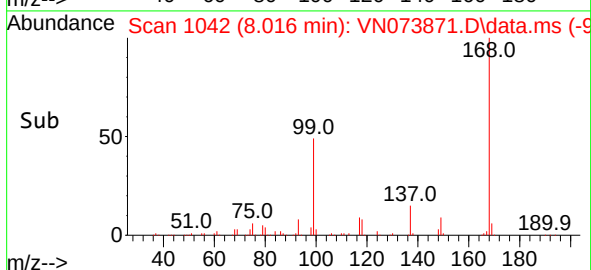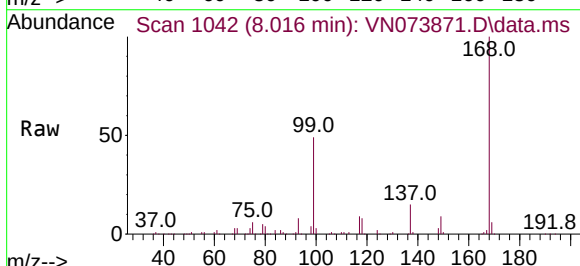



#33

1,2-Dichloroethane-d4

Concen: 41.001 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :





FMC-0074DL

Tgt Ion: 65 Resp: 306029

Ion Ratio Lower Upper

65 100

67 51.9 0.0 104.8

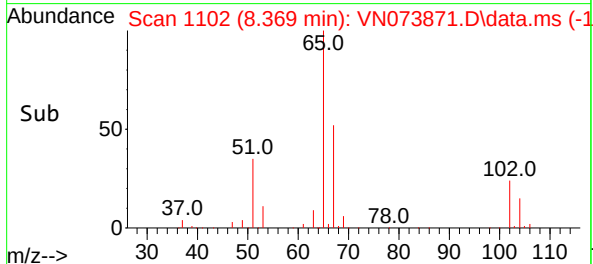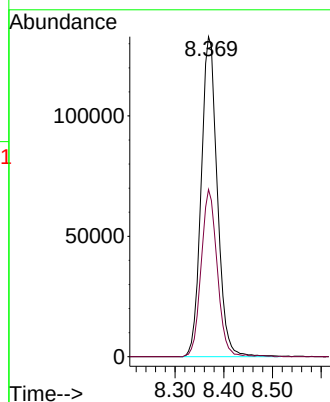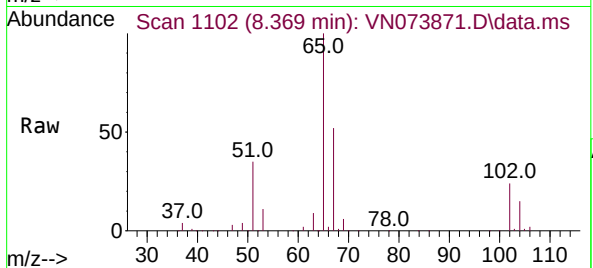

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25




Tgt Ion: 114 Resp: 872482


Ion Ratio Lower Upper

114 100

63 17.0 0.0 40.0

88 14.4 0.0 32.6

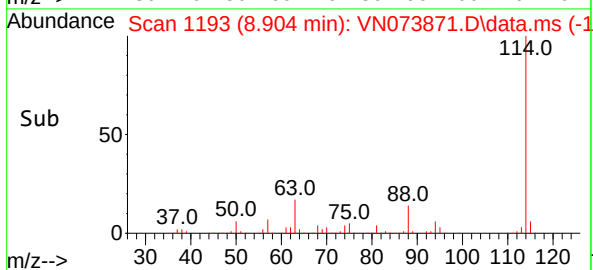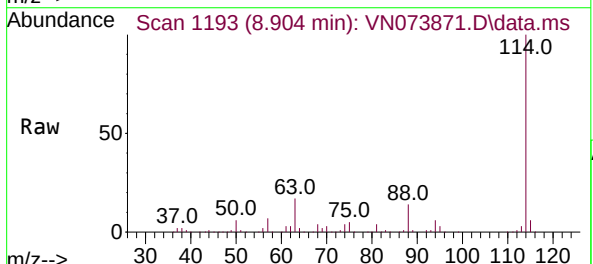



#35

Dibromofluoromethane

Concen: 53.877 ug/l

RT: 7.951 min Scan# 1042

Delta R.T. -0.000 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

FMC-0074DL





Tgt Ion:113 Resp: 295174

Ion Ratio Lower Upper

113 100

111 102.1 81.4 122.0

192 24.3 17.0 25.6

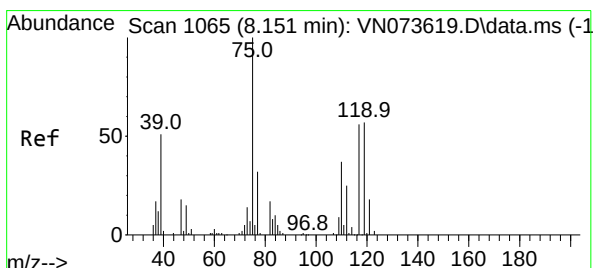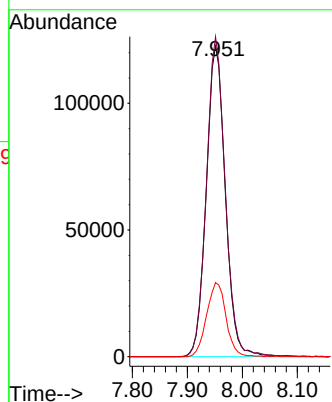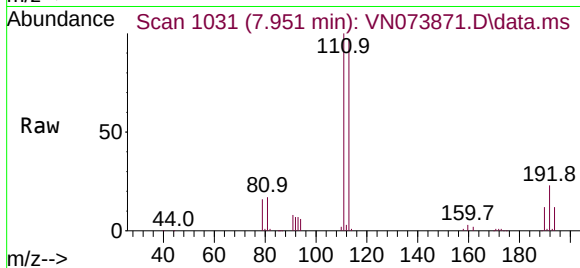

#36

1,1-Dichloropropene

Concen: 4.633 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25




Tgt Ion: 75 Resp: 36178


Ion Ratio Lower Upper

75 100

110 10.1 18.3 54.8#

77 0.0 25.1 37.7#


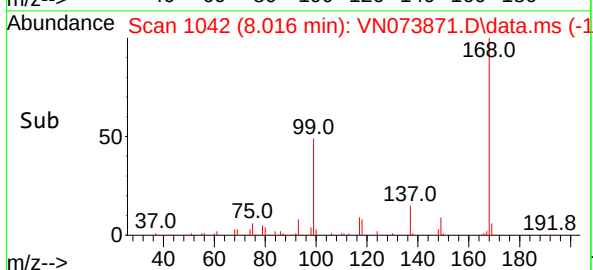
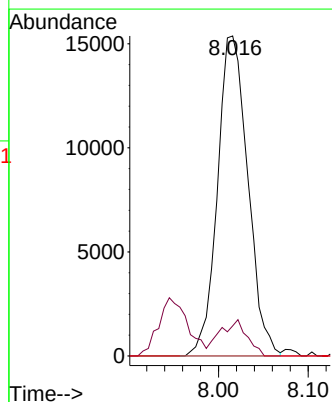
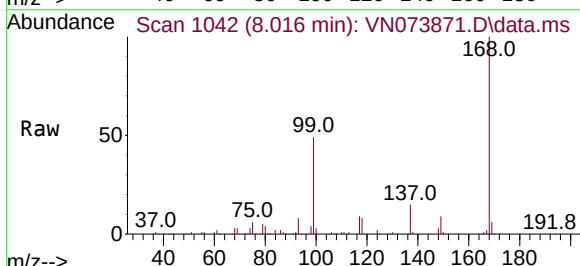




#37
Ethyl Acetate
Concen: 0.398 ug/l
RT: 7.339 min Scan# 91
Delta R.T. -0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion: 43 Resp: 4093
Ion Ratio Lower Upper
43 100
61 3.0 11.8 17.6#
70 6.2 9.3 13.9#

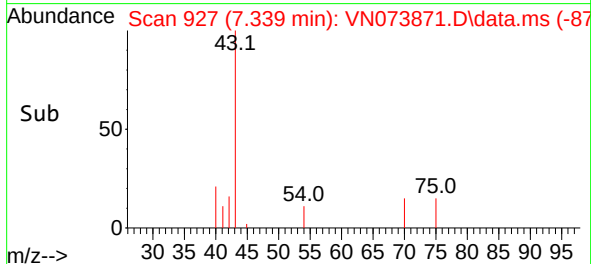

#38
Carbon Tetrachloride
Concen: 6.591 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 117 Resp: 52267
Ion Ratio Lower Upper
117 100
119 4.4 75.8 113.8#
121 0.0 24.6 37.0#

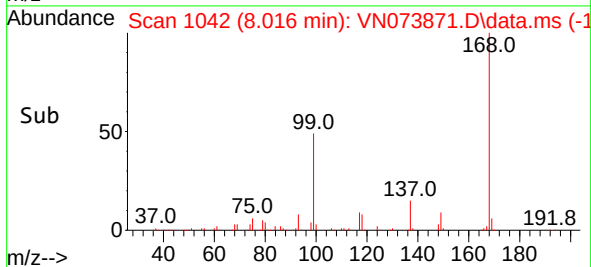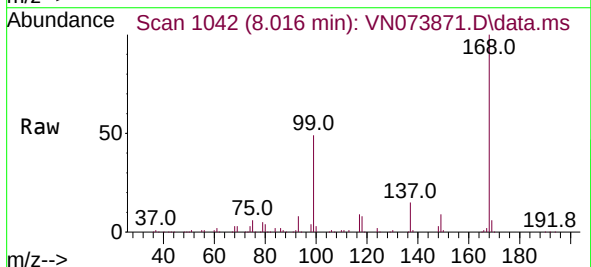



#43

Isopropyl Acetate

Concen: 0.859 ug/l

RT: 8.498 min Scan# 1124

Delta R.T. 0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25





Instrument :

MSVOA_N

ClientSampleId :

FMC-0074DL

Tgt Ion: 43	Resp: 11935
Ion Ratio	Lower Upper
43	100
61	19.7 21.9 32.9#
87	16.0 12.0 18.0

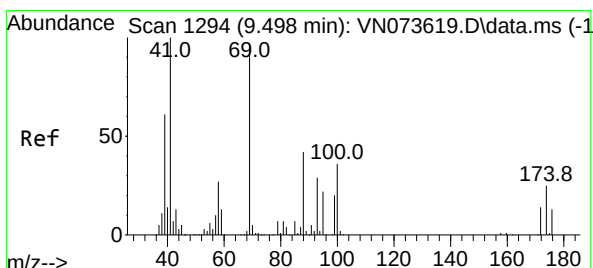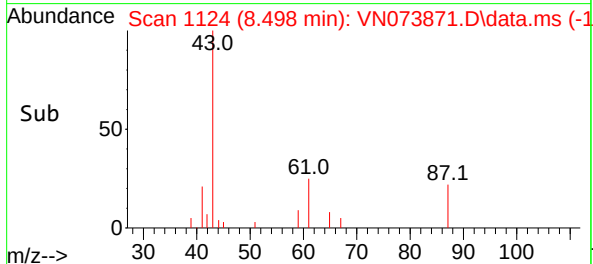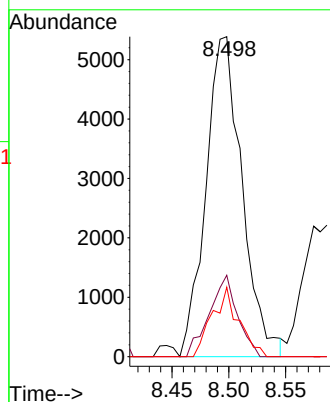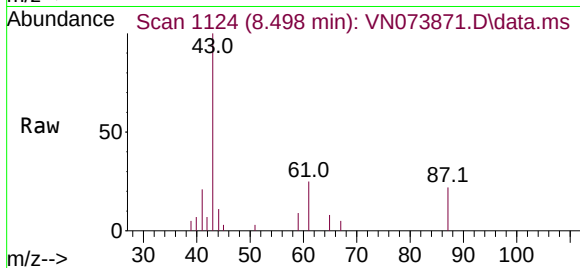

#48

Methyl methacrylate

Concen: 0.633 ug/l




RT: 9.475 min Scan# 1290


Delta R.T. -0.024 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Tgt Ion: 41	Resp: 3847
Ion Ratio	Lower Upper
41	100
69	4.7 74.7 112.1#
39	54.5 45.6 68.4

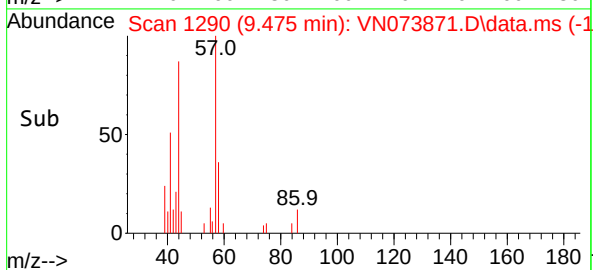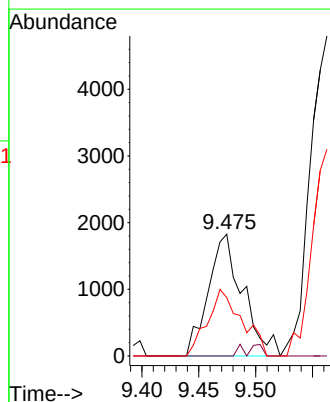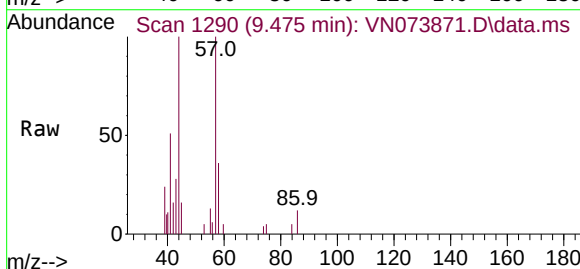



#49

1,4-Dioxane

Concen: 0.502 ug/l

RT: 9.510 min Scan# 1295

Delta R.T. 0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

FMC-0074DL





Tgt Ion: 88 Resp: 86

Ion Ratio Lower Upper

88 100

43 0.0 20.2 30.4#

58 0.0 54.2 81.4#

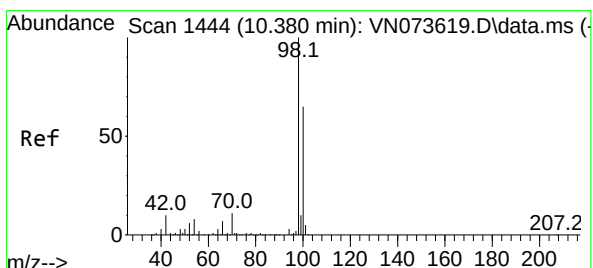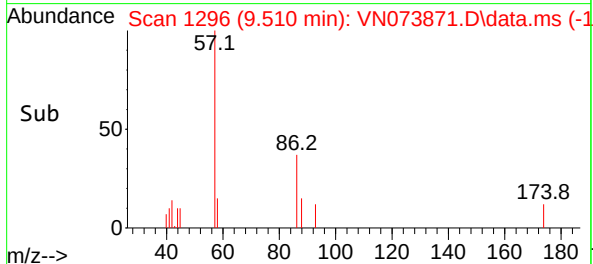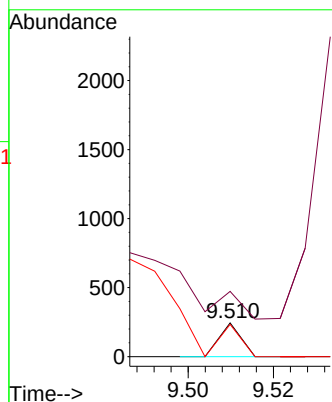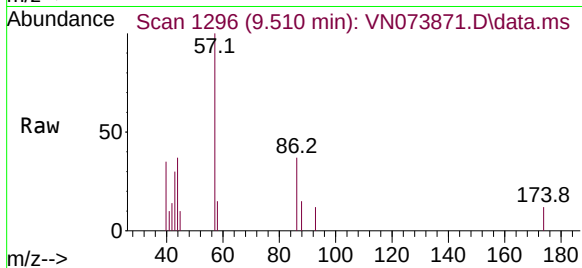

#50

Toluene-d8

Concen: 46.222 ug/l

RT: 10.380 min Scan# 1444

Delta R.T. -0.000 min

Lab File: VN073871.D




Acq: 13 Aug 2022 16:25


Tgt Ion: 98 Resp: 996506

Ion Ratio Lower Upper

98 100

100 64.7 52.6 78.8


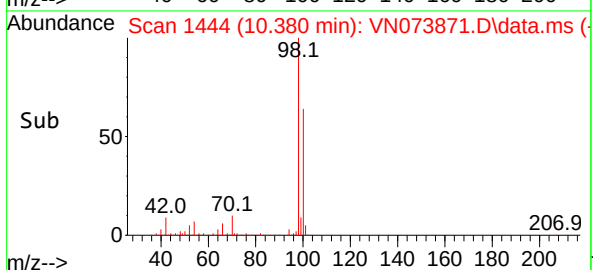

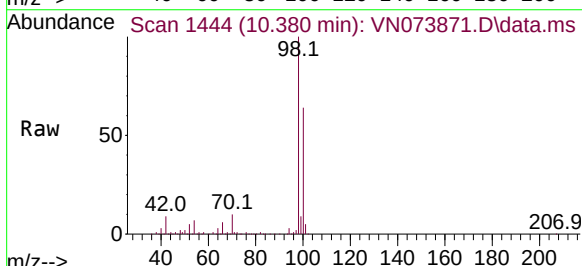




#51
4-Methyl-2-Pentanone
Concen: 0.590 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.006 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion: 43 Resp: 5880
Ion Ratio Lower Upper
43 100
58 34.5 34.1 51.1

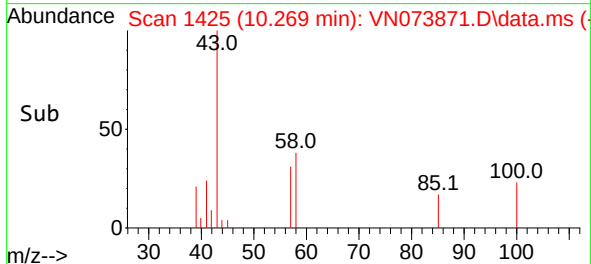

#52
Toluene
Concen: 3.222 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. -0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 92 Resp: 49902
Ion Ratio Lower Upper
92 100
91 173.7 138.6 207.8

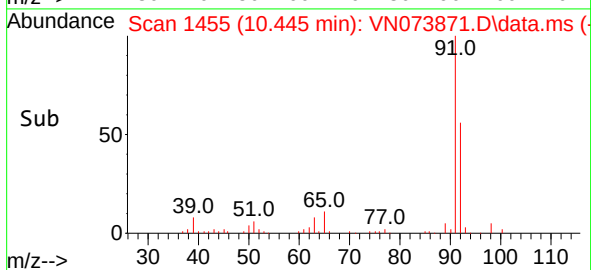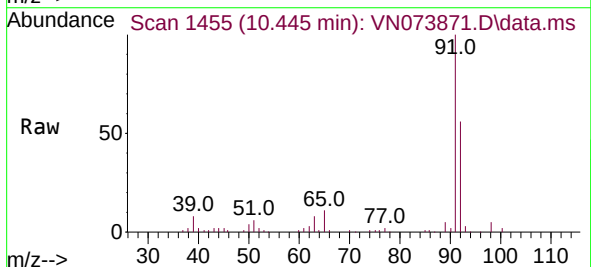



#58

2-Chloroethyl Vinyl ether

Concen: 9.985 ug/l

RT: 9.986 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :





FMC-0074DL

Tgt Ion: 63 Resp: 212

Ion Ratio Lower Upper

63 100

106 0.0 24.6 36.8#

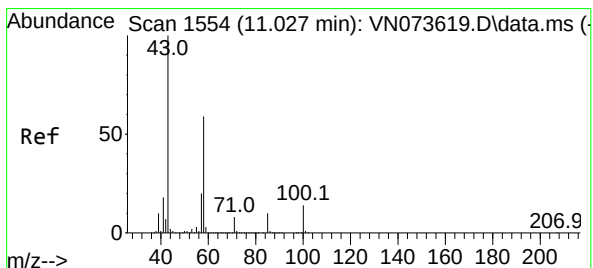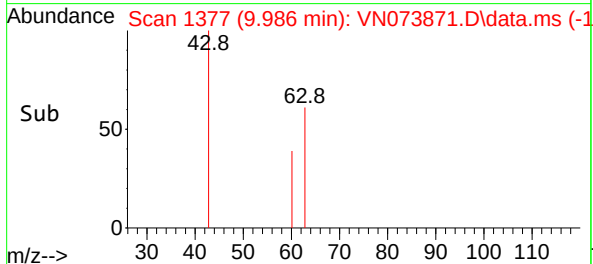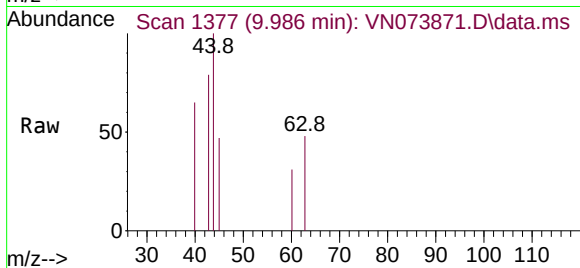

#59

2-Hexanone

Concen: 1.184 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.006 min

Lab File: VN073871.D




Acq: 13 Aug 2022 16:25


Tgt Ion: 43 Resp: 8936

Ion Ratio Lower Upper

43 100

58 35.5 29.7 89.1


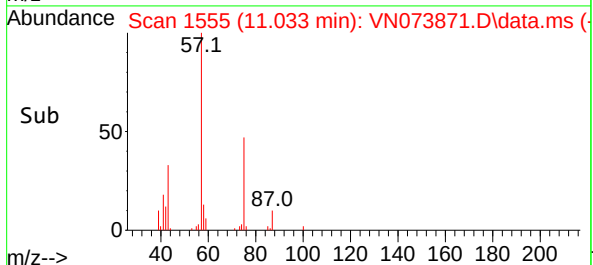
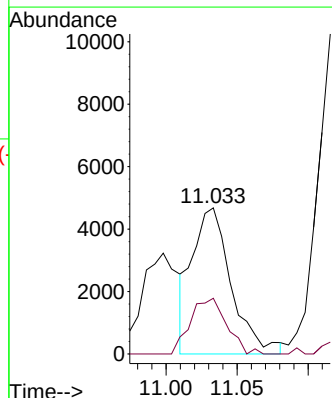
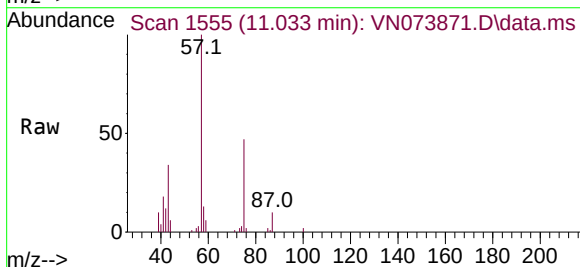


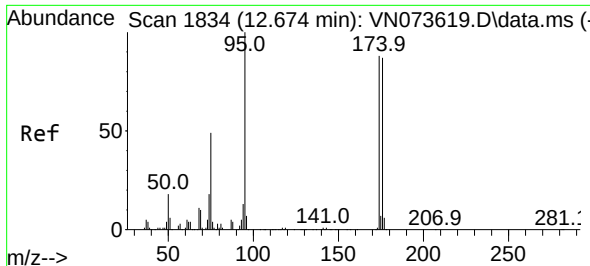

#62
4-Bromofluorobenzene
Concen: 50.482 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion: 95 Resp: 382277
Ion Ratio Lower Upper
95 100
174 98.9 0.0 167.6
176 96.2 0.0 163.4

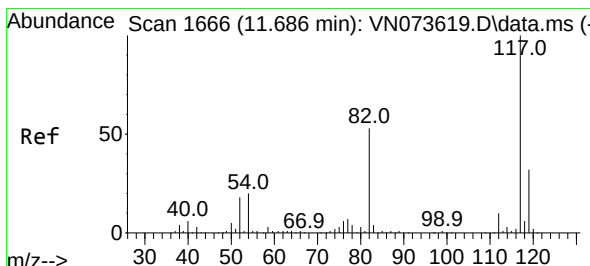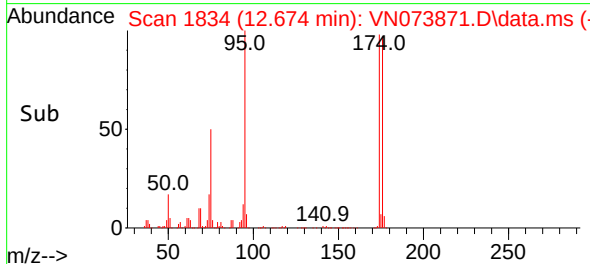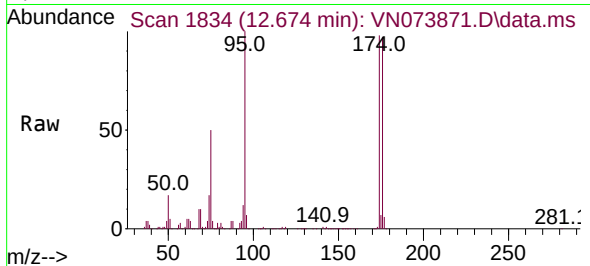

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. -0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 117 Resp: 807936
Ion Ratio Lower Upper
117 100
82 49.4 44.2 66.2
119 33.0 25.4 38.0


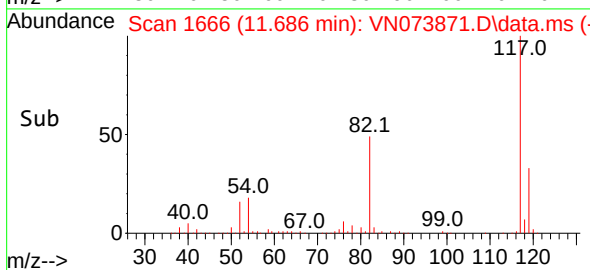

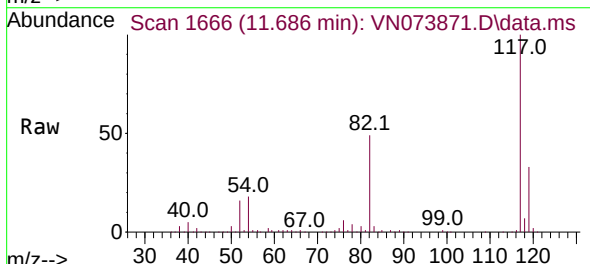




#68
m/p-Xylenes
Concen: 0.334 ug/l
RT: 11.892 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion:106 Resp: 3684
Ion Ratio Lower Upper
106 100
91 208.1 158.9 238.3

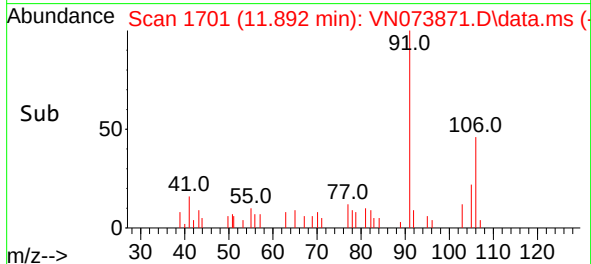

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. -0.000 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion:152 Resp: 412144
Ion Ratio Lower Upper
152 100
115 53.5 28.9 86.7
150 155.8 0.0 356.2


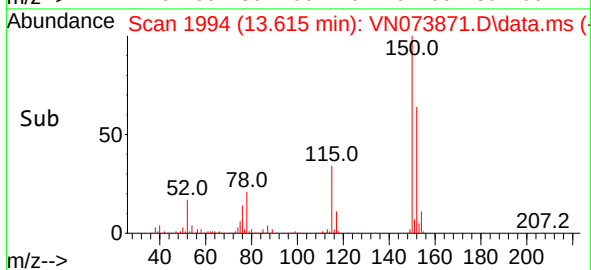

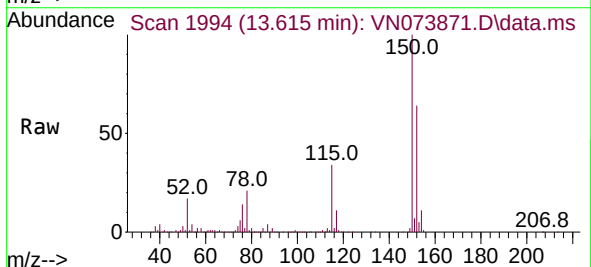




#76
1,2,3-Trichloropropane
Concen: 23.657 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
FMC-0074DL


Tgt Ion: 75 Resp: 191439
Ion Ratio Lower Upper
75 100
77 1.0 98.5 295.5#

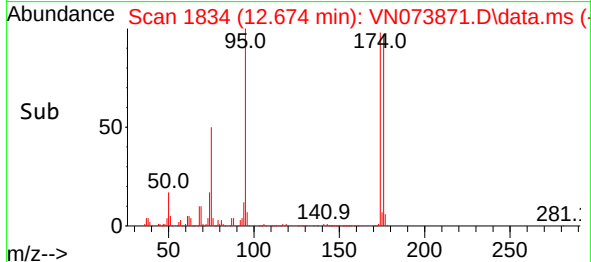

#81
trans-1,4-Dichloro-2-butene
Concen: 60.195 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.106 min
Lab File: VN073871.D
Acq: 13 Aug 2022 16:25

Tgt Ion: 75 Resp: 191439
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.1 37.2 55.8#

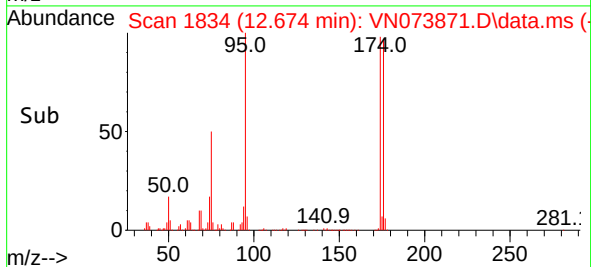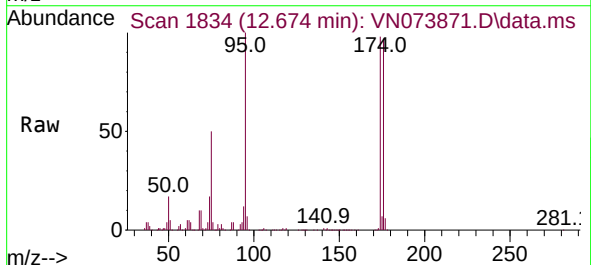



#84

1,2,4-Trimethylbenzene

Concen: 0.378 ug/l

RT: 13.310 min Scan# 1942

Delta R.T. -0.000 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :





FMC-0074DL

Tgt Ion:105 Resp: 9239

Ion Ratio Lower Upper

105 100

120 46.3 23.3 69.8

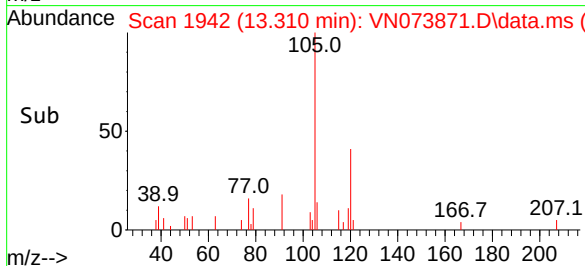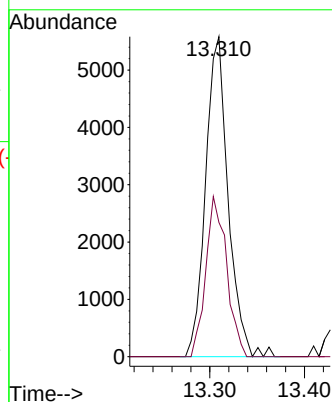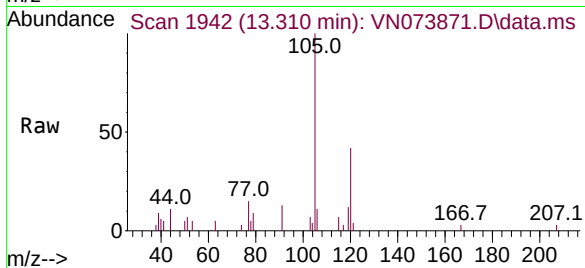

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.239 ug/l

RT: 14.551 min Scan# 2153

Delta R.T. 0.006 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25




Tgt Ion: 75 Resp: 559


Ion Ratio Lower Upper

75 100

155 89.4 44.9 134.5

157 63.5 59.0 176.8

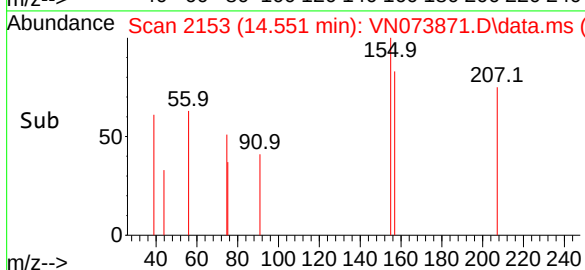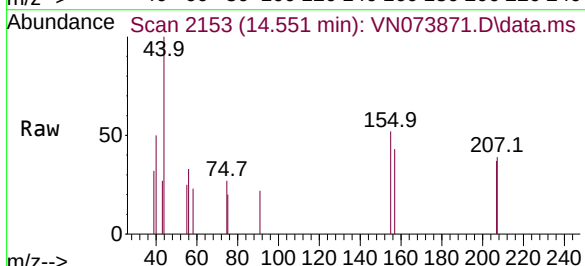



#93

1,2,4-Trichlorobenzene

Concen: 0.491 ug/l

RT: 15.198 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

FMC-0074DL





Tgt Ion:180 Resp: 3541

Ion Ratio Lower Upper

180 100

182 97.5 47.5 142.5

145 32.2 14.5 43.5

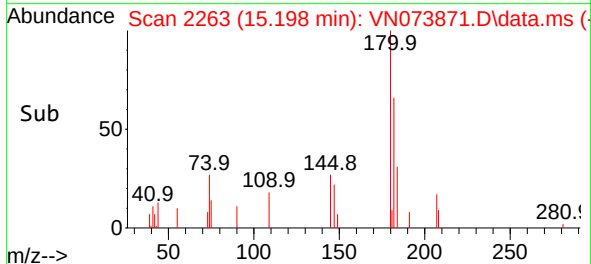

#95

Naphthalene

Concen: 0.801 ug/l

RT: 15.433 min Scan# 2303

Delta R.T. -0.000 min

Lab File: VN073871.D

Acq: 13 Aug 2022 16:25




Tgt Ion:128 Resp: 18762


Ion Ratio Lower Upper

128 100

127 13.0 10.3 15.5


129 10.7 8.6 13.0

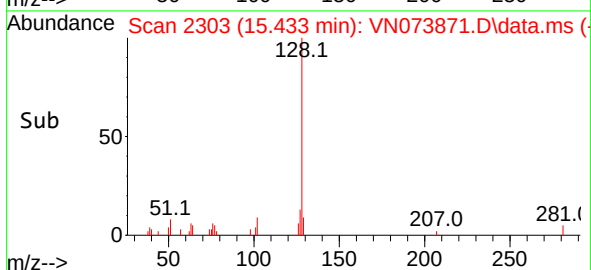



#96
 1,2,3-Trichlorobenzene
 Concen: 0.554 ug/l
 RT: 15.627 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN073871.D
 Acq: 13 Aug 2022 16:25

Instrument :
 MSVOA_N
 ClientSampleId :
 FMC-0074DL

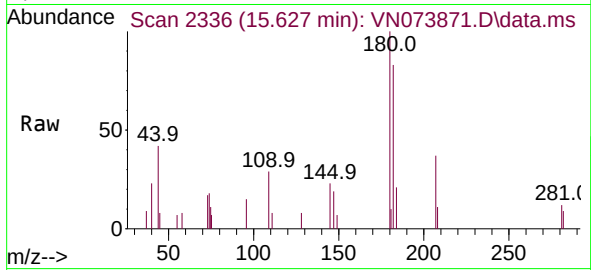

Tgt Ion:	180	Resp:	4208
Ion	Ratio	Lower	Upper
180	100		
182	98.3	47.8	143.3
145	29.4	15.5	46.5

