

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
 Data File : VN073877.D
 Acq On : 13 Aug 2022 18:53
 Operator : JC\MD
 Sample : PB146976ZHE#03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#03

Quant Time: Aug 14 02:38:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.022	168	672097	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	969583	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	929143	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	518476	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	306435	37.413	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	74.820%		
35) Dibromofluoromethane	7.951	113	303095	49.783	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.560%		
50) Toluene-d8	10.380	98	1020576	42.598	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	85.200%#		
62) 4-Bromofluorobenzene	12.674	95	440374	52.230	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.460%		
Target Compounds						Qvalue
3) Chloromethane	2.263	50	1422	Below Cal		94
6) Chloroethane	2.951	64	142	Below Cal	#	78
11) Tert butyl alcohol	5.287	59	846	0.479	ug/l #	72
16) Acetone	4.222	43	68140	15.489	ug/l	96
18) Methyl Acetate	4.787	43	17136	1.566	ug/l	95
20) Methylene Chloride	5.016	84	32933	2.535	ug/l	97
25) 2-Butanone	7.269	43	15119	2.213	ug/l	96
26) 2,2-Dichloropropane	7.233	77	2830	0.272	ug/l #	53
29) Tetrahydrofuran	7.622	42	4159	0.963	ug/l #	74
31) Cyclohexane	8.016	56	10423	0.855	ug/l #	8
36) 1,1-Dichloropropene	8.016	75	40825	4.705	ug/l #	49
37) Ethyl Acetate	7.339	43	84743	7.416	ug/l	97
38) Carbon Tetrachloride	8.016	117	57456	6.519	ug/l #	16
42) 1,2-Dichloroethane	8.498	62	2955	0.311	ug/l #	74
43) Isopropyl Acetate	8.498	43	521970	33.816	ug/l #	82
48) Methyl methacrylate	9.486	41	12326	1.824	ug/l #	41
49) 1,4-Dioxane	9.504	88	443	2.326	ug/l #	1
51) 4-Methyl-2-Pentanone	10.274	43	17043	1.539	ug/l	96
52) Toluene	10.445	92	101337	5.888	ug/l	98
53) t-1,3-Dichloropropene	10.557	75	3269	0.353	ug/l #	37
54) cis-1,3-Dichloropropene	10.186	75	147243	14.098	ug/l #	60
57) 1,3-Dichloropropane	11.033	76	20257	1.664	ug/l #	42
59) 2-Hexanone	11.033	43	224641	26.782	ug/l #	51
67) Ethyl Benzene	11.786	91	9483	0.285	ug/l #	86
68) m/p-Xylenes	11.886	106	17073	1.344	ug/l	93
69) o-Xylene	12.221	106	7770	0.628	ug/l	99
74) N-amyl acetate	12.292	43	40338	2.813	ug/l #	43
76) 1,2,3-Trichloropropane	12.674	75	215617	20.820	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.674	75	215617	53.894	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.304	105	9279	0.302	ug/l	90
89) n-Butylbenzene	13.810	91	8923	0.364	ug/l #	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
Data File : VN073877.D
Acq On : 13 Aug 2022 18:53
Operator : JC\MD
Sample : PB146976ZHE#03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03

Quant Time: Aug 14 02:38:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 05:09:32 2022
Response via : Initial Calibration




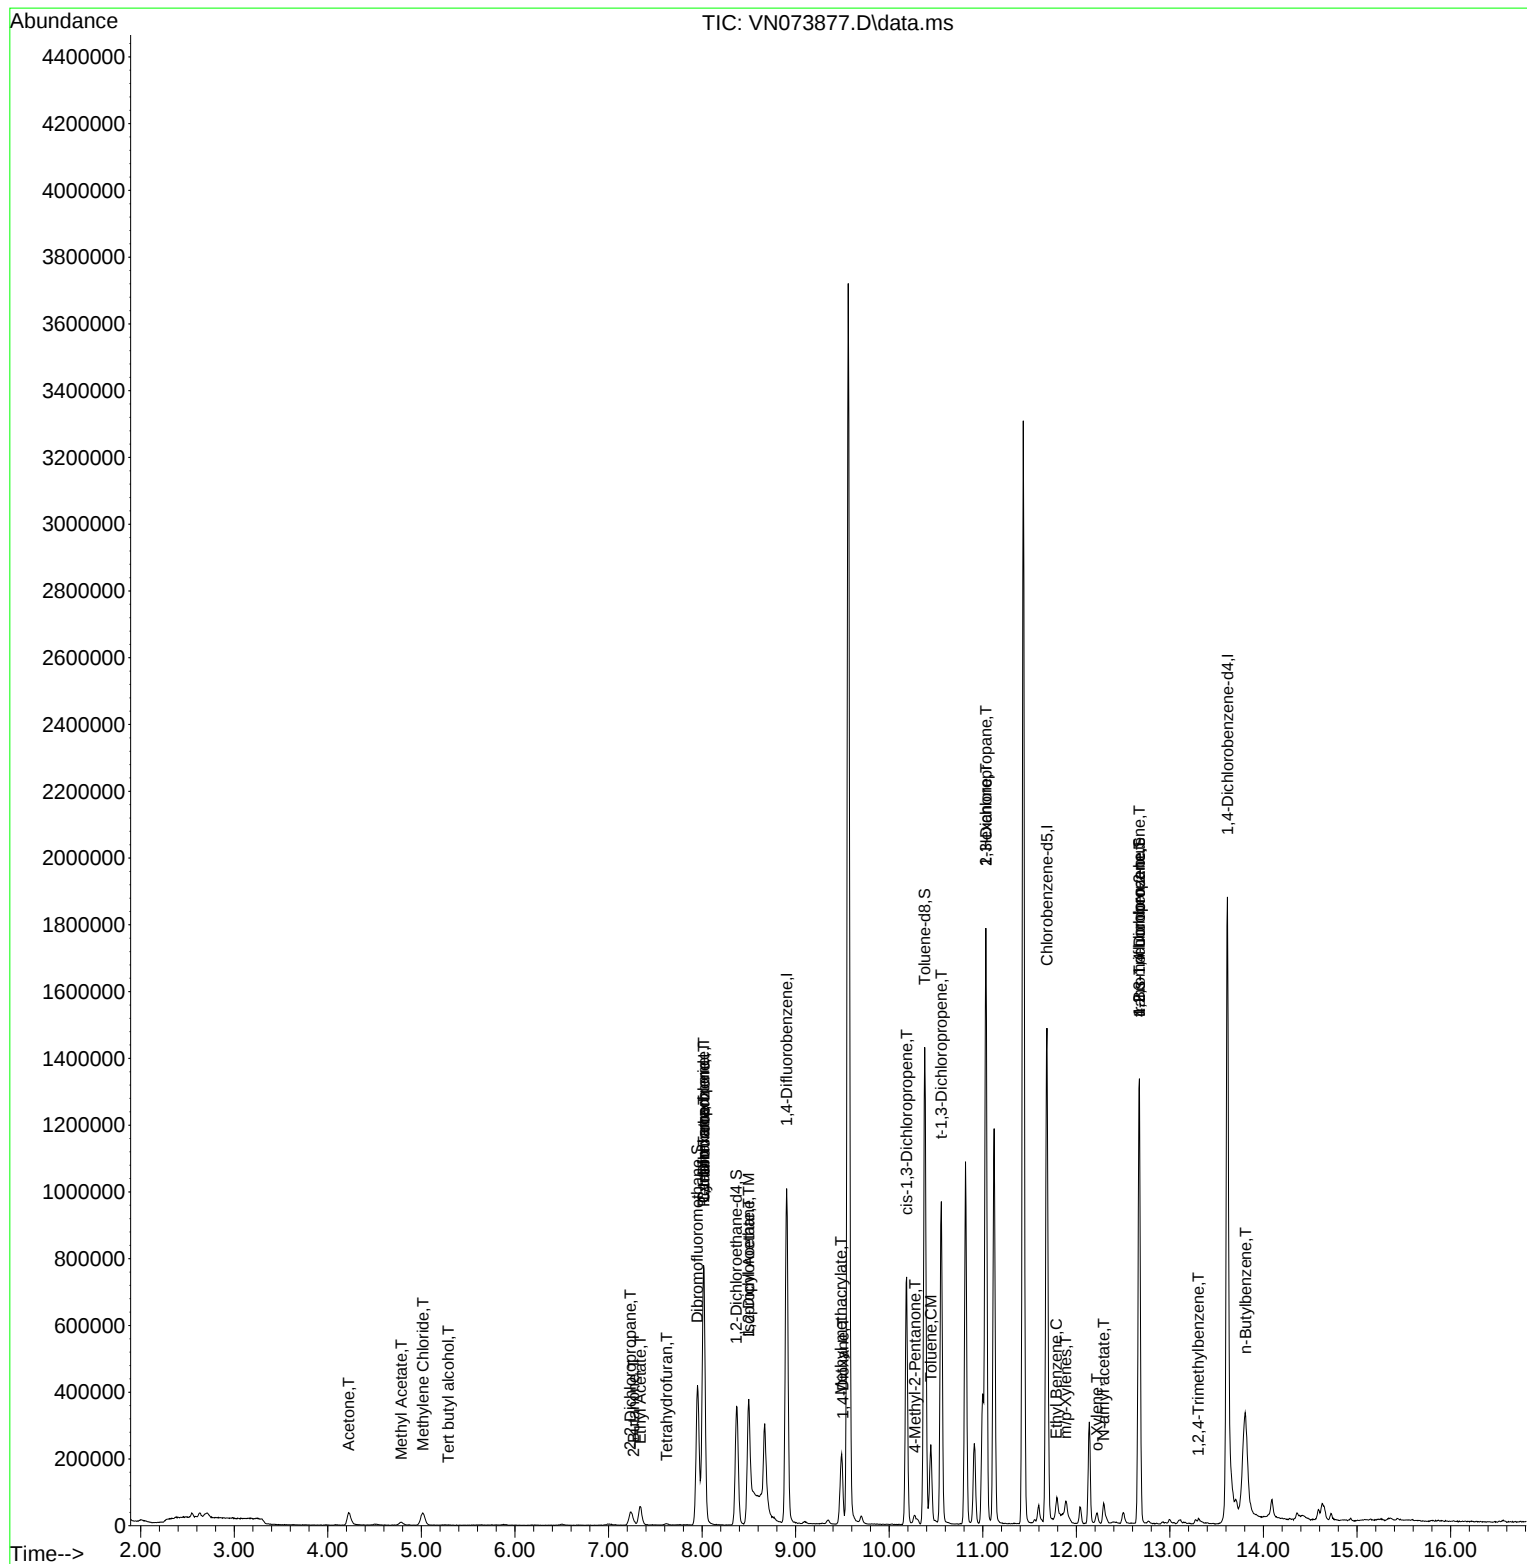




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion:168 Resp: 672097
Ion Ratio Lower Upper
168 100
99 46.4 42.3 63.5

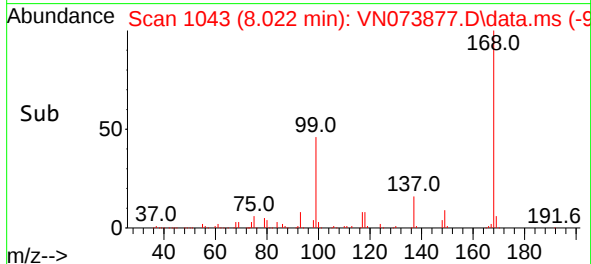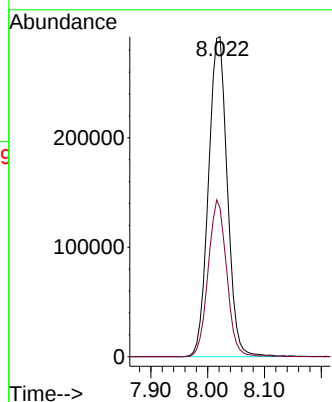

#3
Chloromethane
Concen: Below Cal
RT: 2.263 min Scan# 64
Delta R.T. -0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 50 Resp: 1422
Ion Ratio Lower Upper
50 100
52 28.8 25.7 38.5


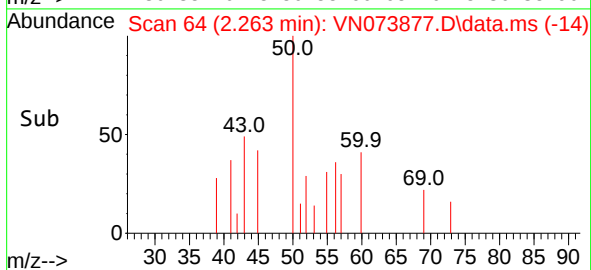
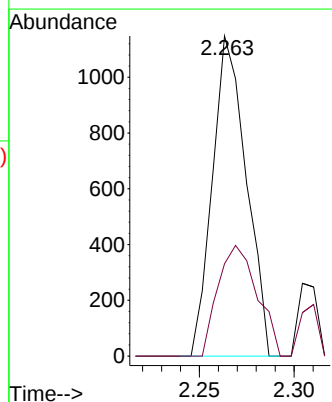
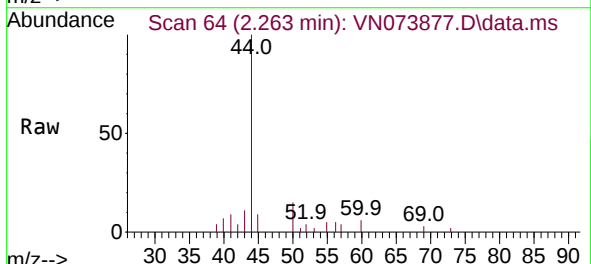




#6
Chloroethane
Concen: Below Cal
RT: 2.951 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 64 Resp: 142
Ion Ratio Lower Upper
64 100
66 20.5 26.2 39.4#

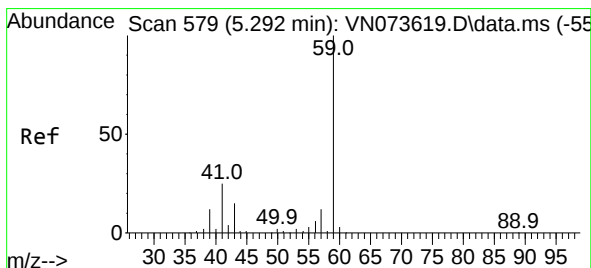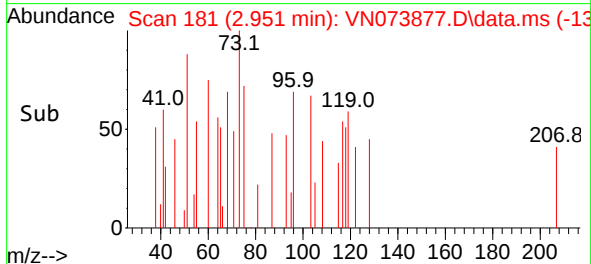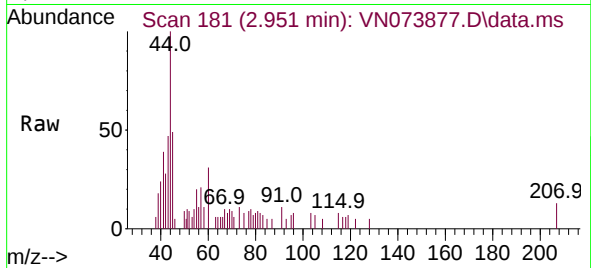

#11
Tert butyl alcohol
Concen: 0.479 ug/l
RT: 5.287 min Scan# 578
Delta R.T. -0.005 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 59 Resp: 846
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


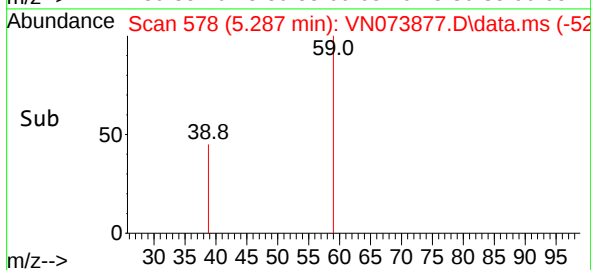

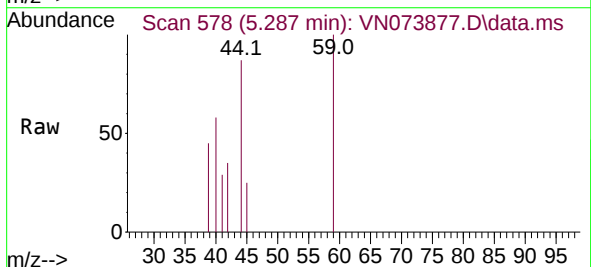




#16
Acetone
Concen: 15.489 ug/l
RT: 4.222 min Scan# 397
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03

Tgt Ion: 43 Resp: 68140
Ion Ratio Lower Upper
43 100
58 34.6 26.0 39.0

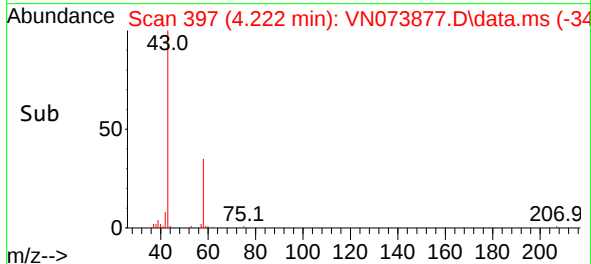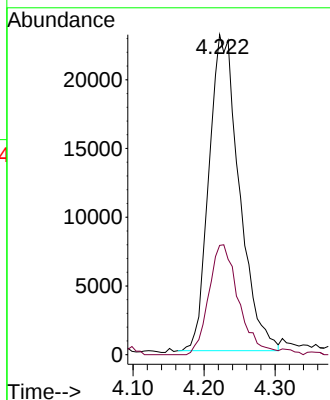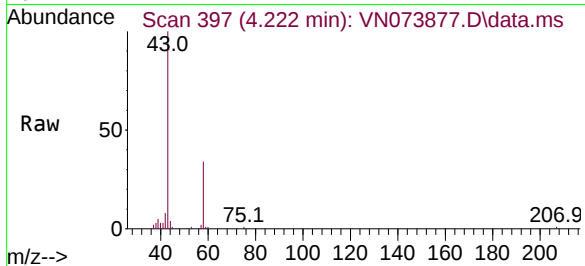

#18
Methyl Acetate
Concen: 1.566 ug/l
RT: 4.787 min Scan# 493
Delta R.T. 0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53


Tgt Ion: 43 Resp: 17136
Ion Ratio Lower Upper
43 100
74 29.4 21.6 32.4

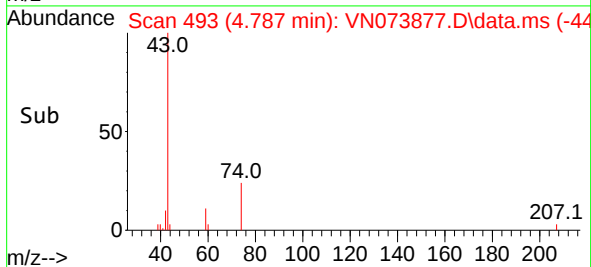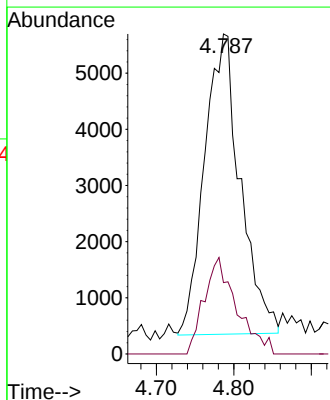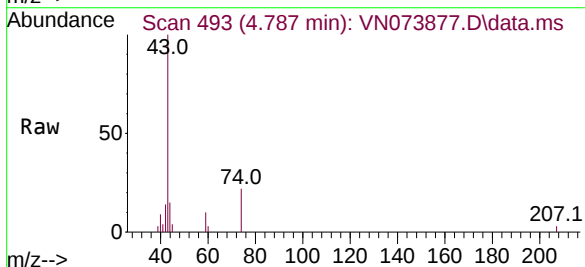






#20
Methylene Chloride
Concen: 2.535 ug/l
RT: 5.016 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03



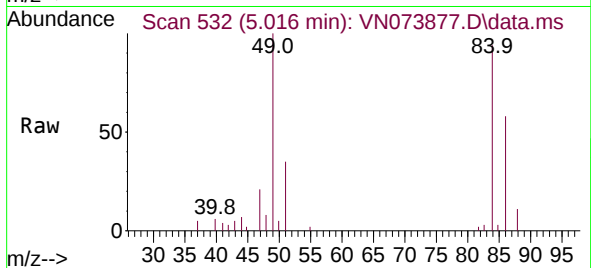



Tgt Ion:	84	Resp:	32933
Ion	Ratio	Lower	Upper
84	100		
49	106.5	88.3	132.5
51	37.7	28.2	42.2
86	61.6	50.6	76.0

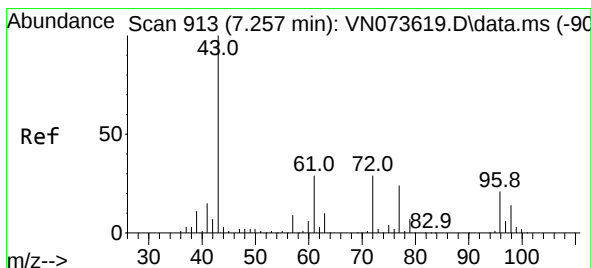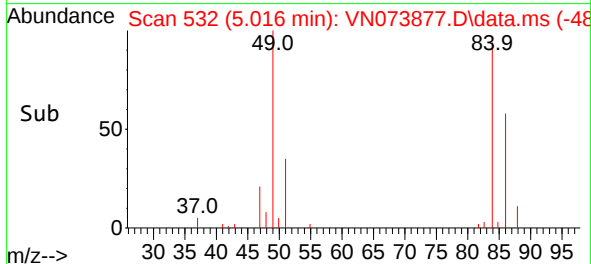

#25
2-Butanone
Concen: 2.213 ug/l
RT: 7.269 min Scan# 915
Delta R.T. 0.012 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion:	43	Resp:	15119
Ion	Ratio	Lower	Upper
43	100		
72	32.0	23.7	35.5


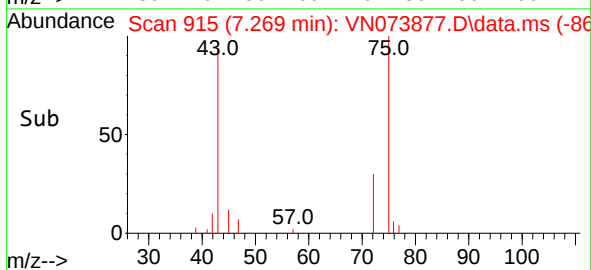

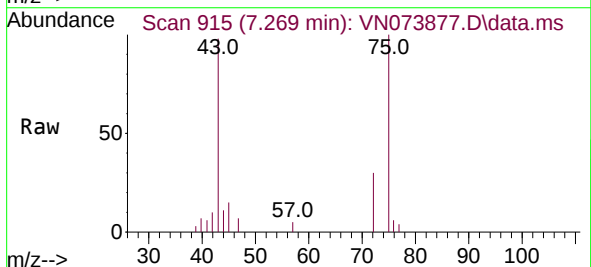




#26
2,2-Dichloropropane
Concen: 0.272 ug/l
RT: 7.233 min Scan# 909
Delta R.T. -0.018 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 77 Resp: 2830
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2#

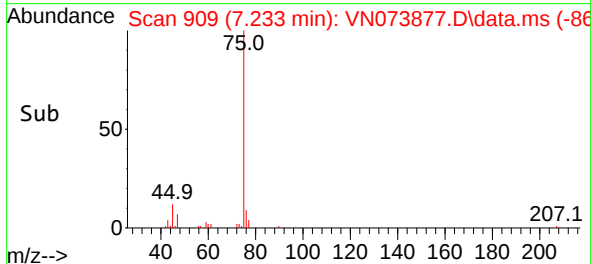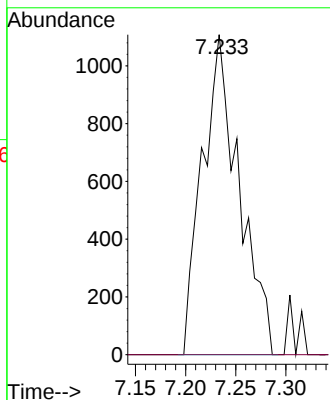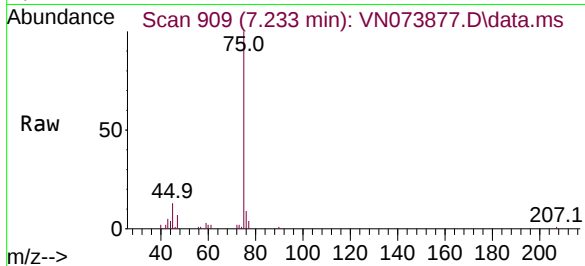

#29
Tetrahydrofuran
Concen: 0.963 ug/l
RT: 7.622 min Scan# 975
Delta R.T. 0.012 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 42 Resp: 4159
Ion Ratio Lower Upper
42 100
72 31.1 39.7 59.5#
71 29.7 36.6 55.0#


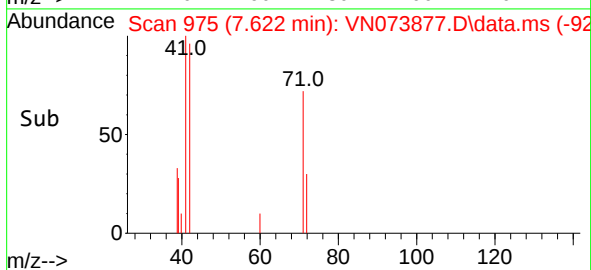
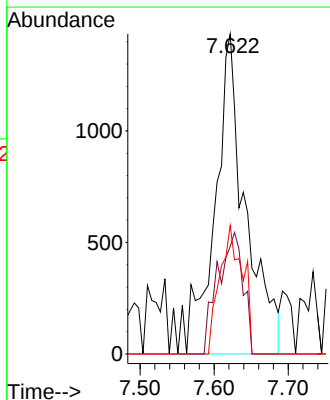
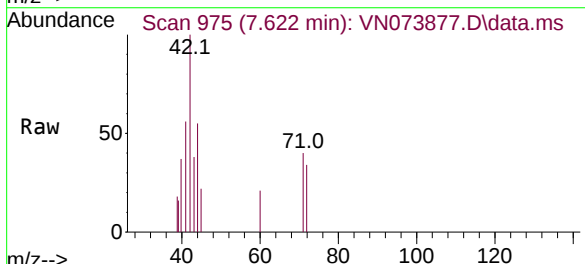


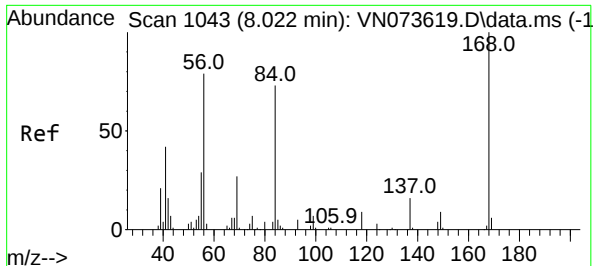

#31
Cyclohexane
Concen: 0.855 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 56 Resp: 10423
Ion Ratio Lower Upper
56 100
69 169.1 27.8 41.8#
84 136.5 76.9 115.3#

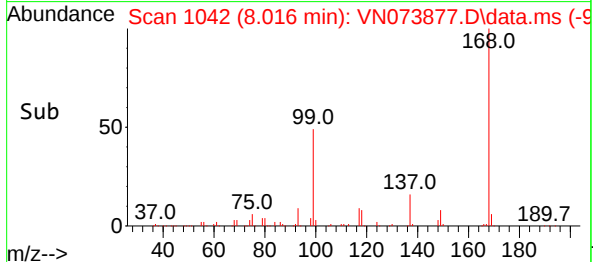

#33
1,2-Dichloroethane-d4
Concen: 37.413 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 65 Resp: 306435
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.8

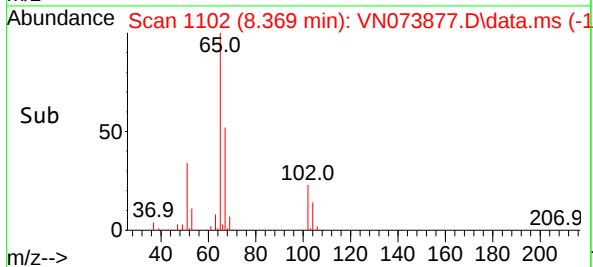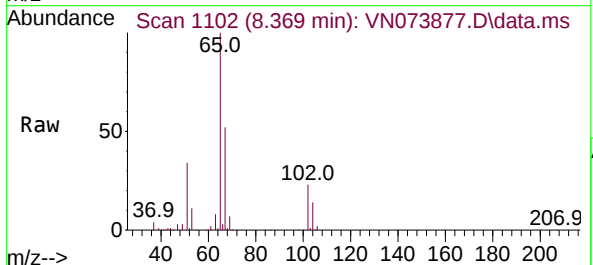

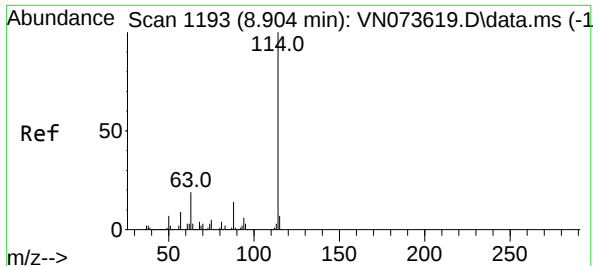

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN073877.D

Acq: 13 Aug 2022 18:53

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#03





Tgt Ion:114 Resp: 969583

Ion Ratio Lower Upper

114 100

63 17.3 0.0 40.0

88 14.6 0.0 32.6

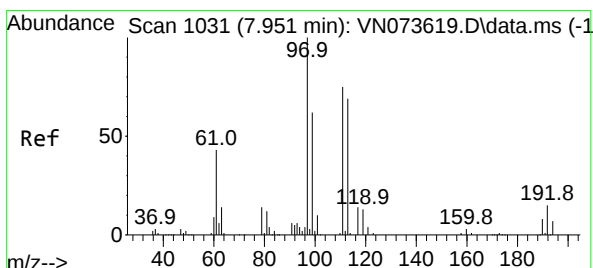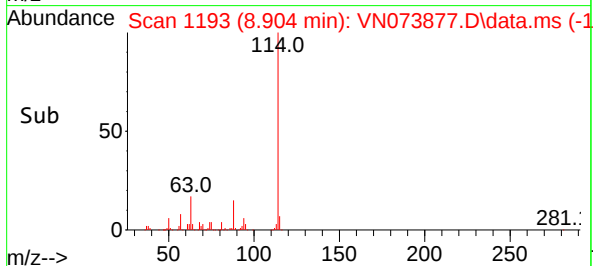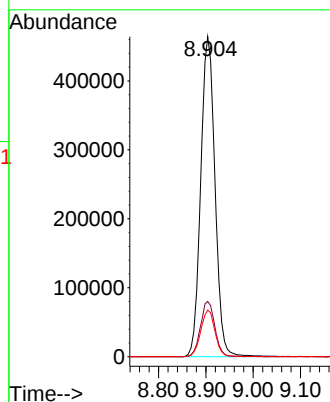

#35

Dibromofluoromethane

Concen: 49.783 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. -0.000 min

Lab File: VN073877.D

Acq: 13 Aug 2022 18:53




Tgt Ion:113 Resp: 303095


Ion Ratio Lower Upper

113 100

111 102.9 81.4 122.0

192 24.1 17.0 25.6


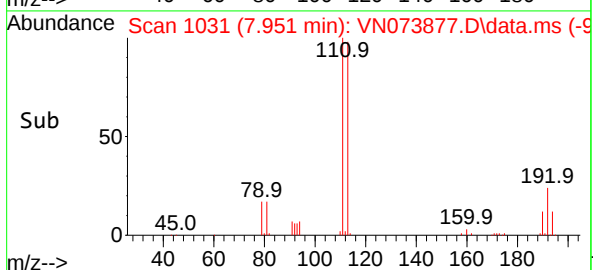
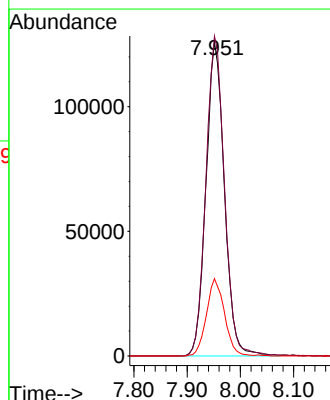
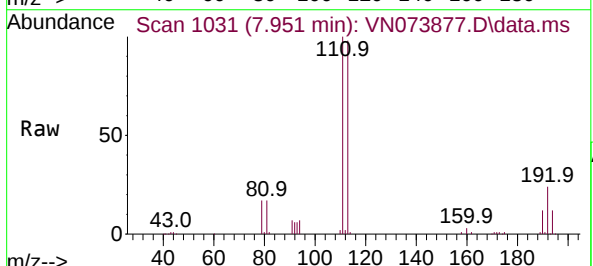


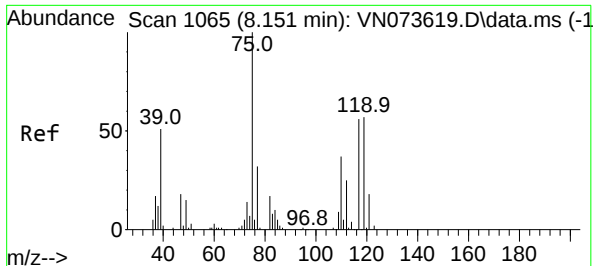

#36
1,1-Dichloropropene
Concen: 4.705 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.135 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 75 Resp: 40825
Ion Ratio Lower Upper
75 100
110 9.5 18.3 54.8#
77 0.0 25.1 37.7#

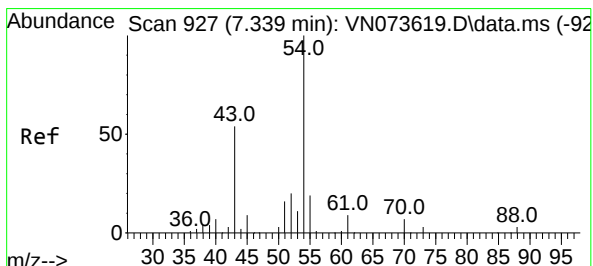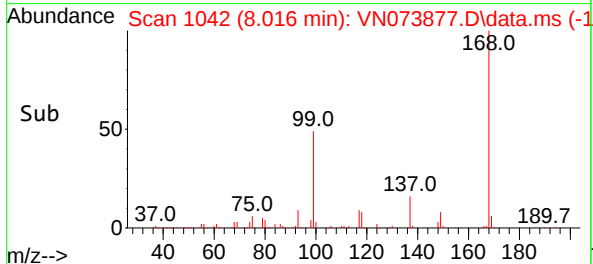

#37
Ethyl Acetate
Concen: 7.416 ug/l
RT: 7.339 min Scan# 927
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53


Tgt Ion: 43 Resp: 84743
Ion Ratio Lower Upper
43 100
61 15.0 11.8 17.6
70 13.4 9.3 13.9

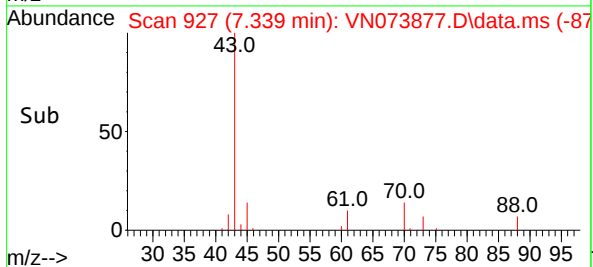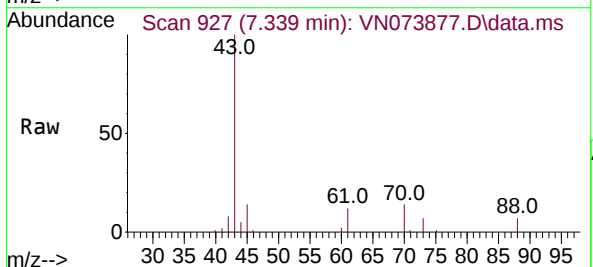






#38
Carbon Tetrachloride
Concen: 6.519 ug/l
RT: 8.016 min Scan# 110
Delta R.T. -0.118 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03







Tgt Ion:117 Resp: 57456
Ion Ratio Lower Upper
117 100
119 4.6 75.8 113.8#
121 0.0 24.6 37.0#

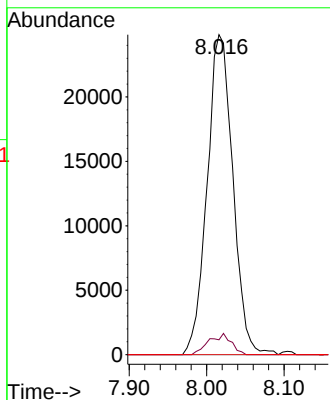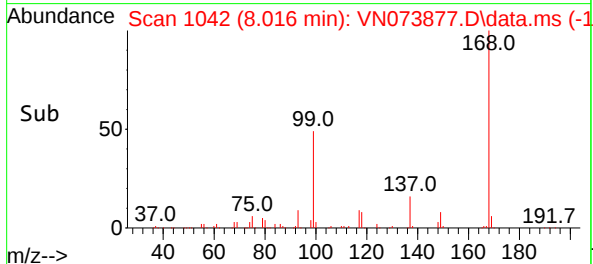

#42
1,2-Dichloroethane
Concen: 0.311 ug/l
RT: 8.498 min Scan# 1124
Delta R.T. 0.035 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 62 Resp: 2955
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4

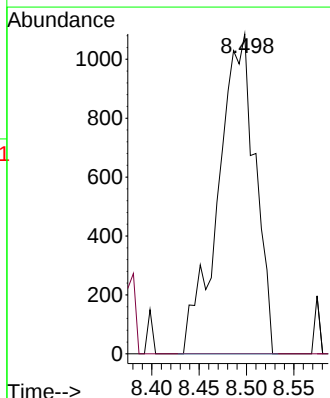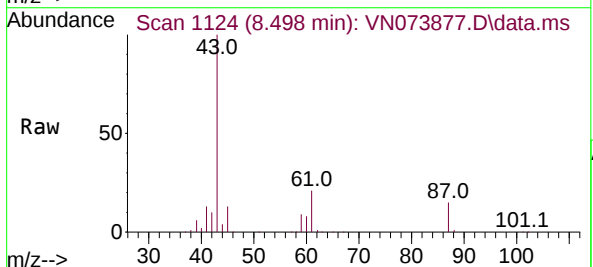

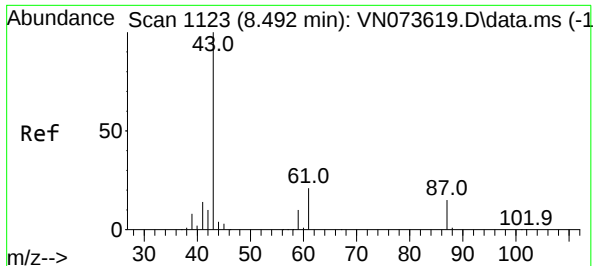

#43

Isopropyl Acetate

Concen: 33.816 ug/l

RT: 8.498 min Scan# 1123

Delta R.T. 0.006 min

Lab File: VN073877.D

Acq: 13 Aug 2022 18:53

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#03





Tgt Ion: 43 Resp: 521970

Ion Ratio Lower Upper

43 100

61 15.8 21.9 32.9#

87 11.4 12.0 18.0#

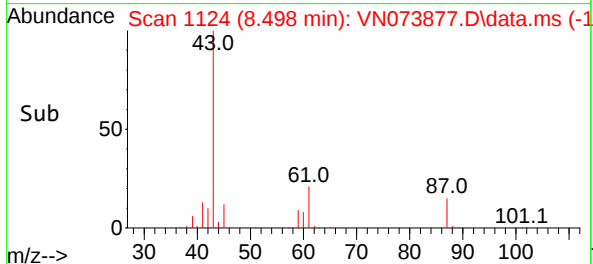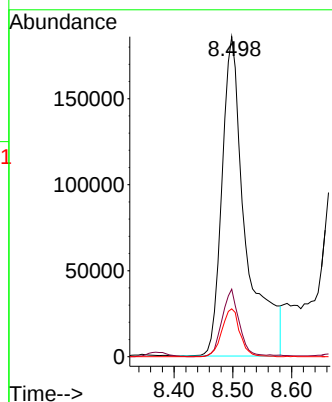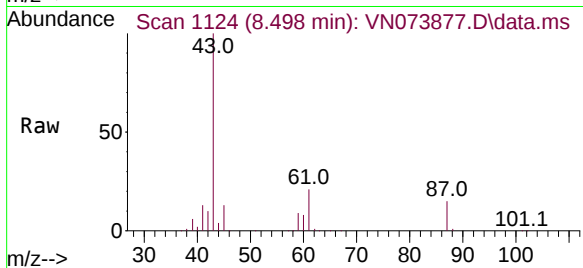

#48

Methyl methacrylate

Concen: 1.824 ug/l

RT: 9.486 min Scan# 1292

Delta R.T. -0.012 min

Lab File: VN073877.D

Acq: 13 Aug 2022 18:53




Tgt Ion: 41 Resp: 12326


Ion Ratio Lower Upper

41 100

69 2.8 74.7 112.1#

39 56.7 45.6 68.4

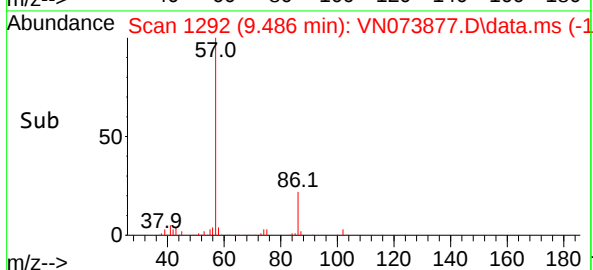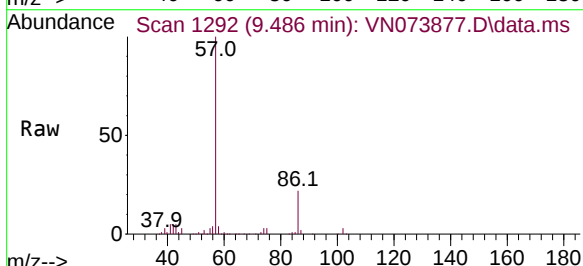



#49

1,4-Dioxane

Concen: 2.326 ug/l

RT: 9.504 min Scan# 1295

Delta R.T. -0.000 min

Lab File: VN073877.D

Acq: 13 Aug 2022 18:53

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#03





Tgt Ion: 88 Resp: 443

Ion Ratio Lower Upper

88 100

43 0.0 20.2 30.4#

58 2200.2 54.2 81.4#

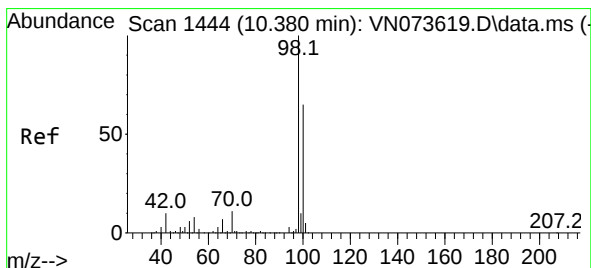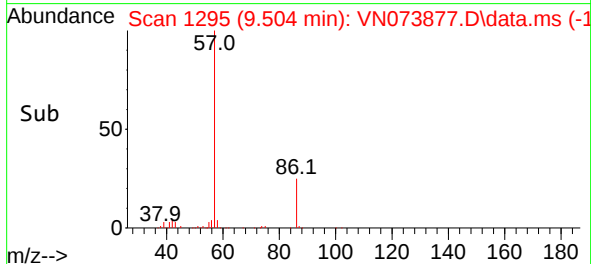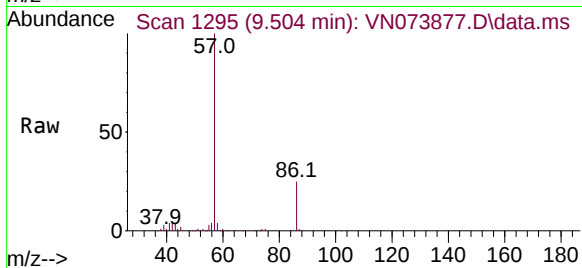

#50

Toluene-d8

Concen: 42.598 ug/l

RT: 10.380 min Scan# 1444

Delta R.T. -0.000 min

Lab File: VN073877.D




Acq: 13 Aug 2022 18:53


Tgt Ion: 98 Resp: 1020576

Ion Ratio Lower Upper

98 100

100 65.5 52.6 78.8


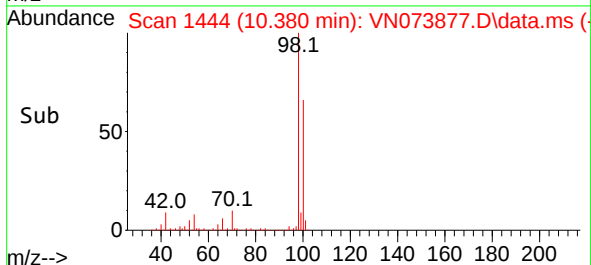
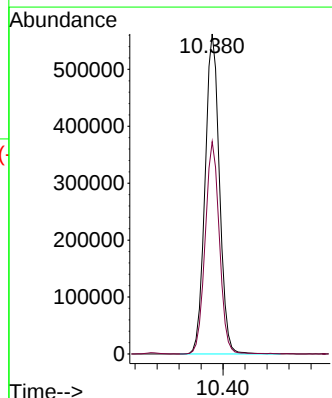
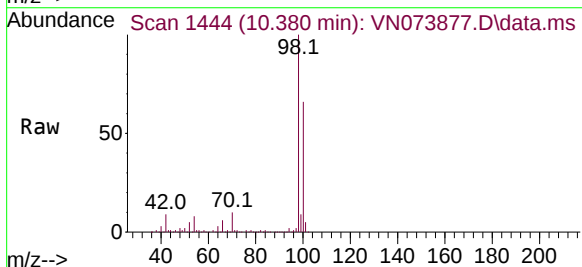


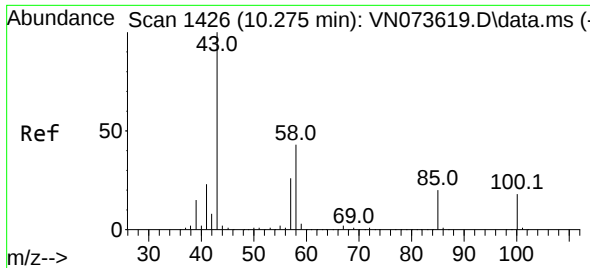

#51
4-Methyl-2-Pentanone
Concen: 1.539 ug/l
RT: 10.274 min Scan# 1426
Delta R.T. -0.001 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 43 Resp: 17043
Ion Ratio Lower Upper
43 100
58 45.4 34.1 51.1

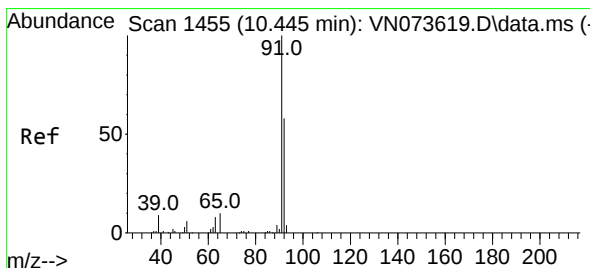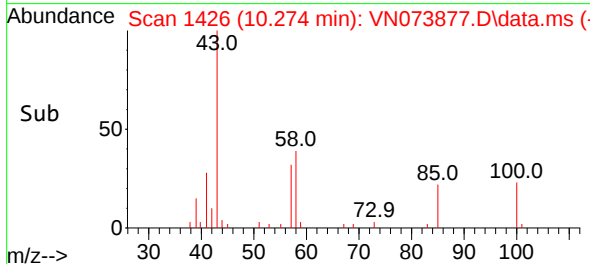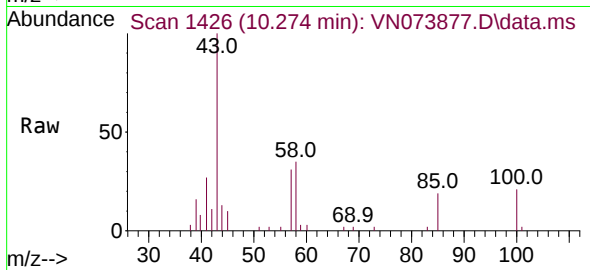

#52
Toluene
Concen: 5.888 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 92 Resp: 101337
Ion Ratio Lower Upper
92 100
91 176.6 138.6 207.8


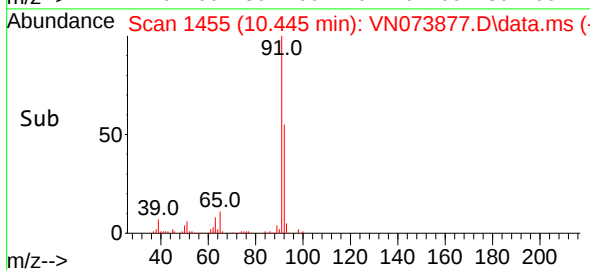

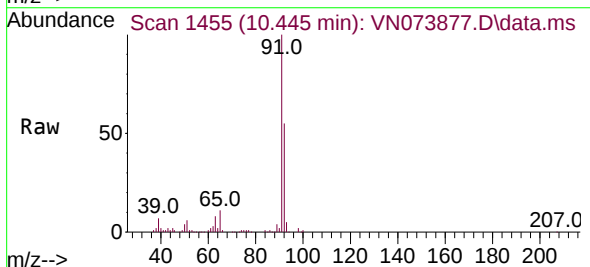


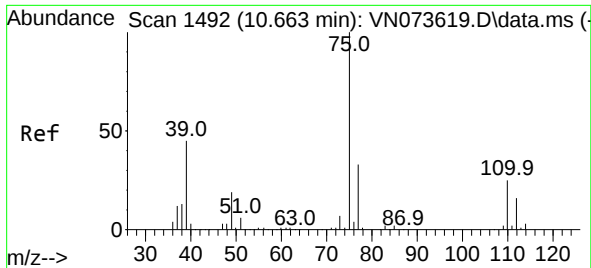

#53
 t-1,3-Dichloropropene
 Concen: 0.353 ug/l
 RT: 10.557 min Scan# 1410
 Delta R.T. -0.106 min
 Lab File: VN073877.D
 Acq: 13 Aug 2022 18:53




Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#03


Tgt Ion: 75 Resp: 3269
 Ion Ratio Lower Upper
 75 100
 77 67.0 25.6 38.4#

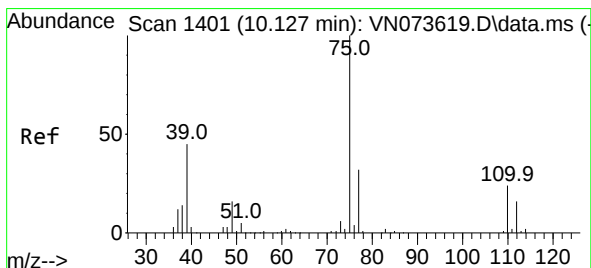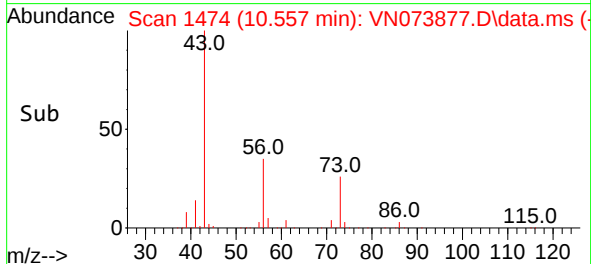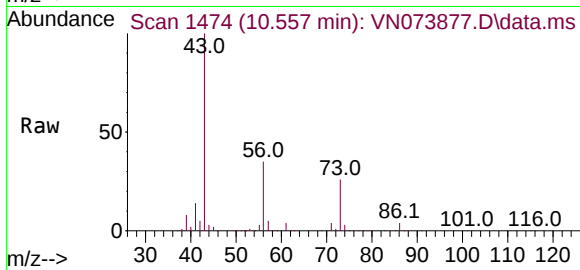

#54
 cis-1,3-Dichloropropene
 Concen: 14.098 ug/l
 RT: 10.186 min Scan# 1411
 Delta R.T. 0.059 min
 Lab File: VN073877.D
 Acq: 13 Aug 2022 18:53

Tgt Ion: 75 Resp: 147243
 Ion Ratio Lower Upper
 75 100
 77 0.7 25.2 37.8#
 39 25.9 35.7 53.5#

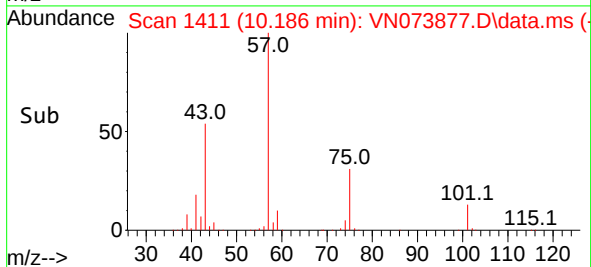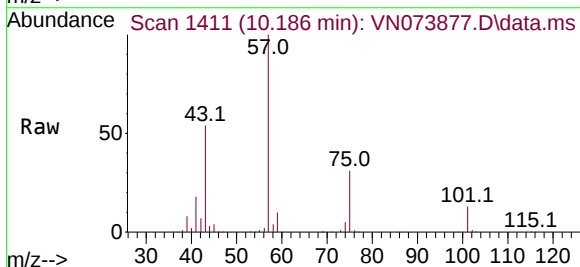

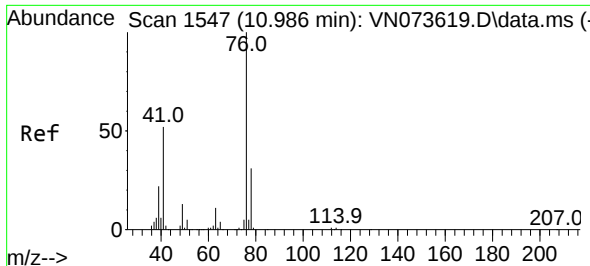

#57

1,3-Dichloropropane

Concen: 1.664 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.047 min

Lab File: VN073877.D

Acq: 13 Aug 2022 18:53

Instrument :

MSVOA_N

ClientSampleId :





PB146976ZHE#03

Tgt Ion: 76 Resp: 20257

Ion Ratio Lower Upper

76 100

78 0.0 26.2 39.2#

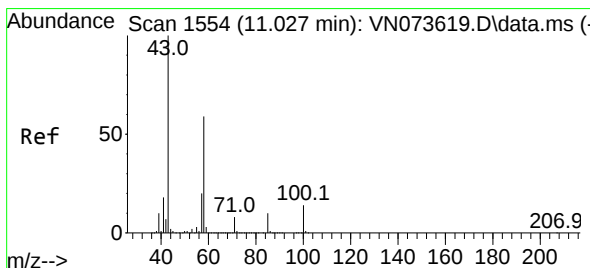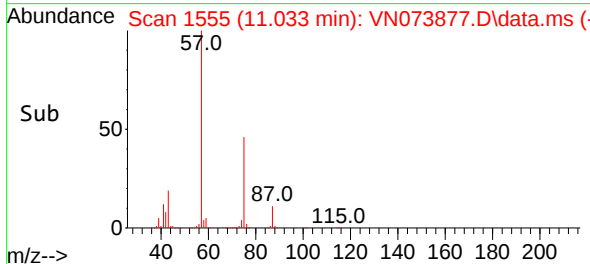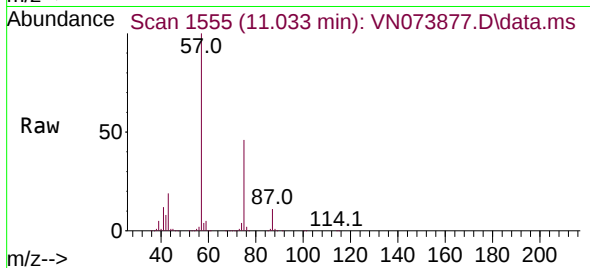

#59

2-Hexanone

Concen: 26.782 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.006 min

Lab File: VN073877.D




Acq: 13 Aug 2022 18:53


Tgt Ion: 43 Resp: 224641

Ion Ratio Lower Upper

43 100

58 22.4 29.7 89.1#


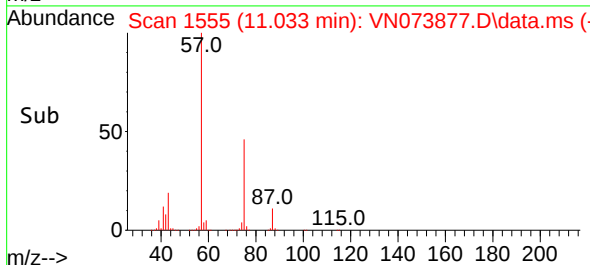

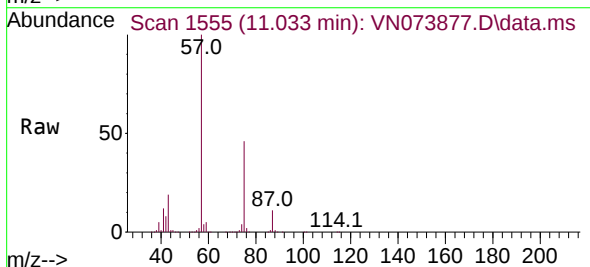


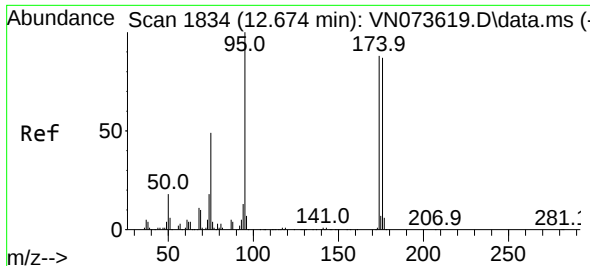

#62
4-Bromofluorobenzene
Concen: 52.230 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 95 Resp: 440374
Ion Ratio Lower Upper
95 100
174 95.6 0.0 167.6
176 93.5 0.0 163.4

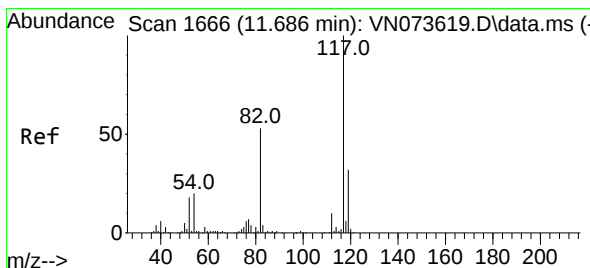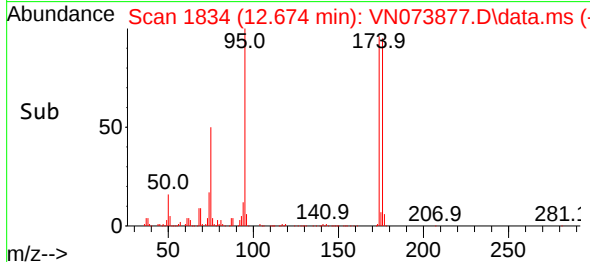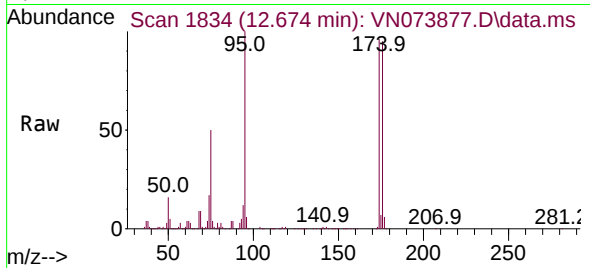

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 117 Resp: 929143
Ion Ratio Lower Upper
117 100
82 51.9 44.2 66.2
119 32.9 25.4 38.0


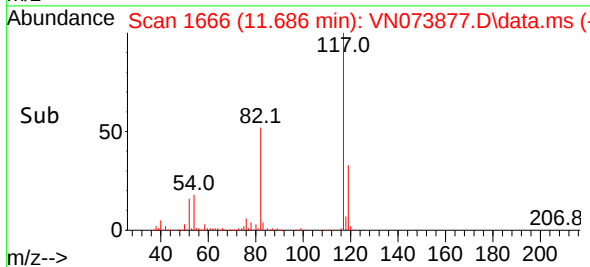

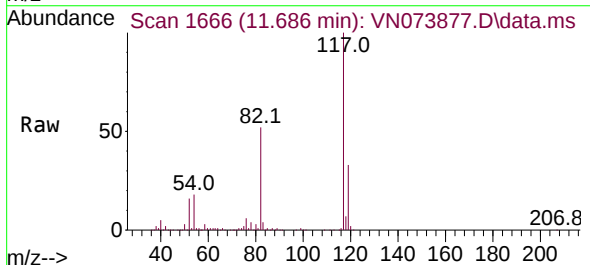


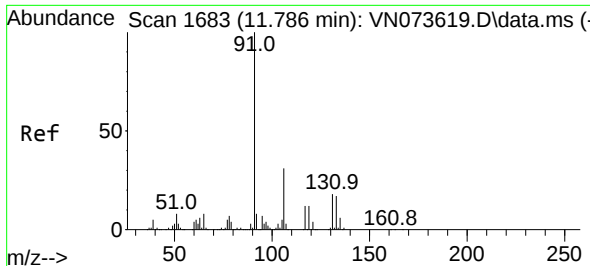

#67
Ethyl Benzene
Concen: 0.285 ug/l
RT: 11.786 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 91 Resp: 9483
Ion Ratio Lower Upper
91 100
106 38.7 24.9 37.3#

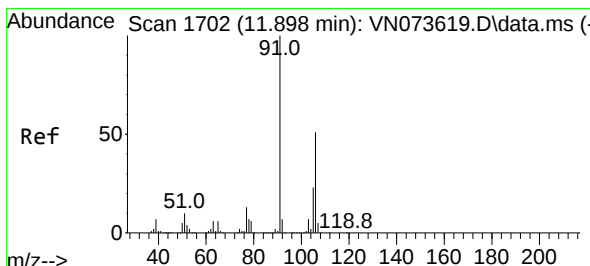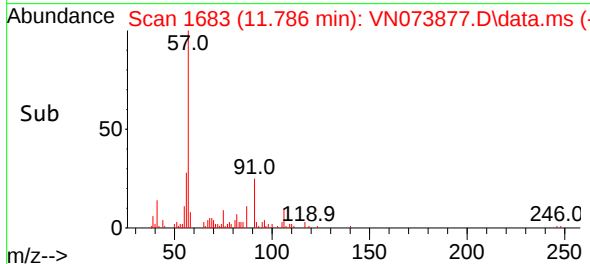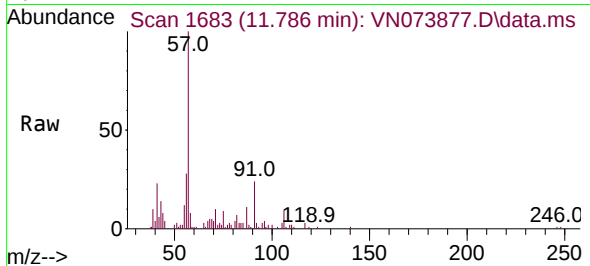

#68
m/p-Xylenes
Concen: 1.344 ug/l
RT: 11.886 min Scan# 1700
Delta R.T. -0.012 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion:106 Resp: 17073
Ion Ratio Lower Upper
106 100
91 209.7 158.9 238.3


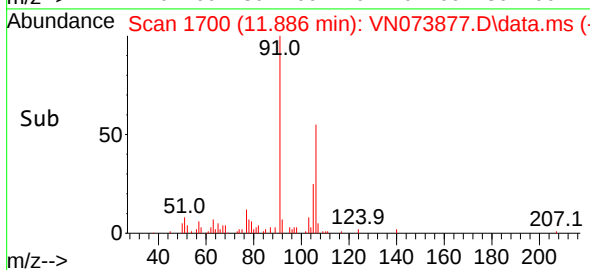

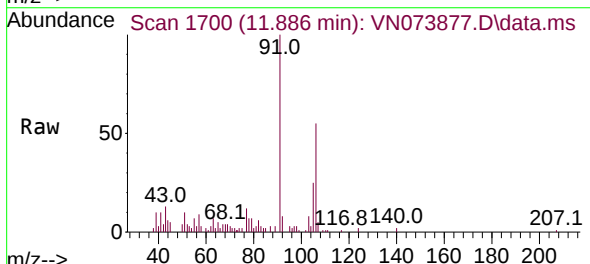


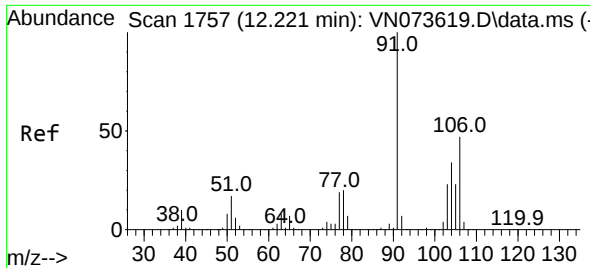

#69
o-Xylene
Concen: 0.628 ug/l
RT: 12.221 min Scan# 1757
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion:106 Resp: 7770
Ion Ratio Lower Upper
106 100
91 209.7 106.0 318.0

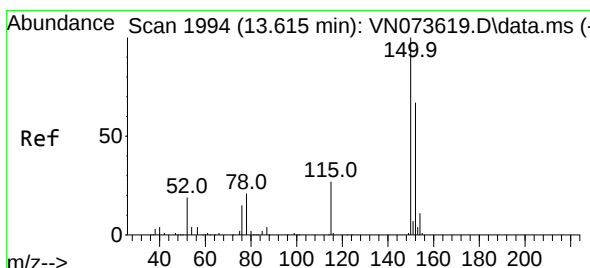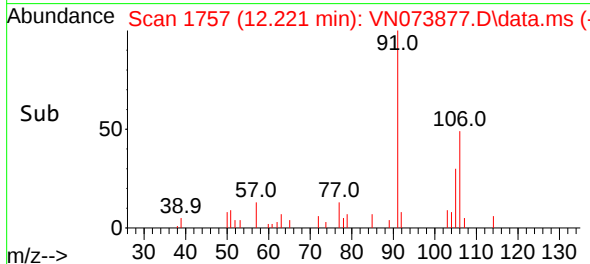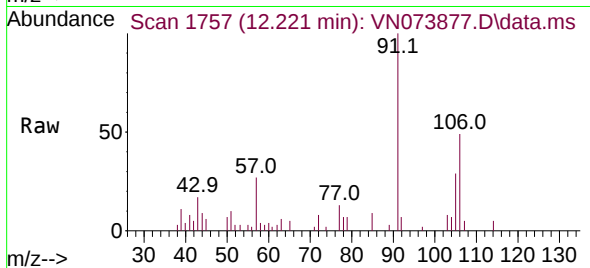

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. -0.000 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion:152 Resp: 518476
Ion Ratio Lower Upper
152 100
115 54.2 28.9 86.7
150 155.0 0.0 356.2


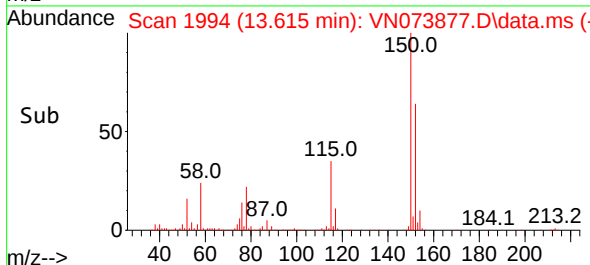

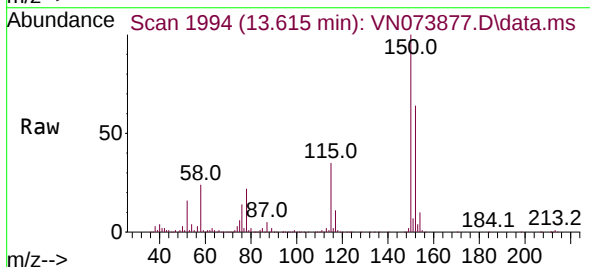


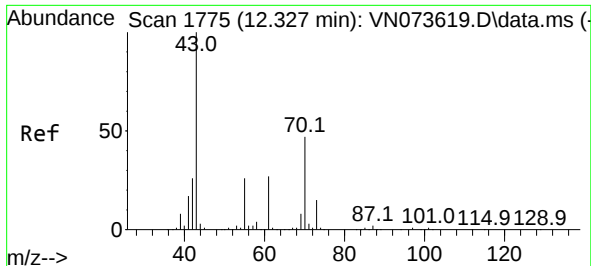

#74
N-amy1 acetate
Concen: 2.813 ug/l
RT: 12.292 min Scan# 11
Delta R.T. -0.035 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion:	43	Resp:	40338
Ion	Ratio	Lower	Upper
43	100		
70	0.0	39.0	58.4#
55	8.0	21.1	31.7#
61	0.0	21.1	31.7#

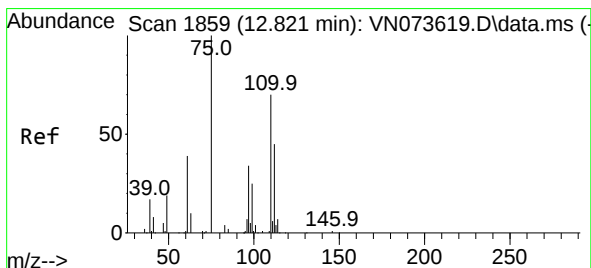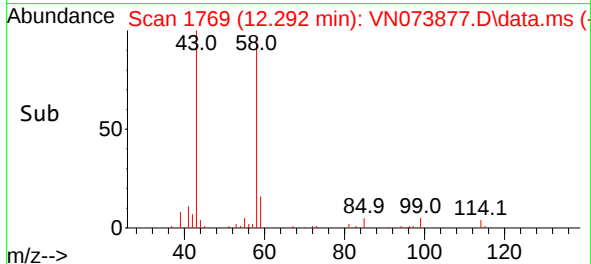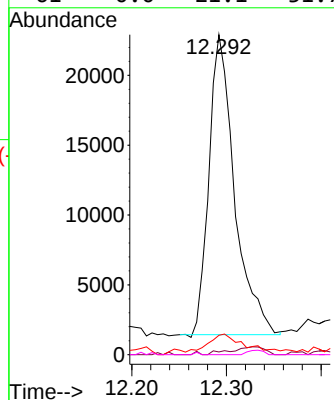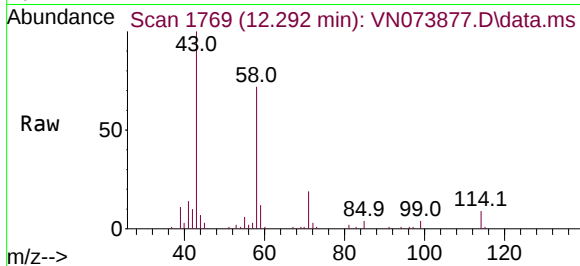

#76
1,2,3-Trichloropropane
Concen: 20.820 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion:	75	Resp:	215617
Ion	Ratio	Lower	Upper
75	100		
77	1.3	98.5	295.5#


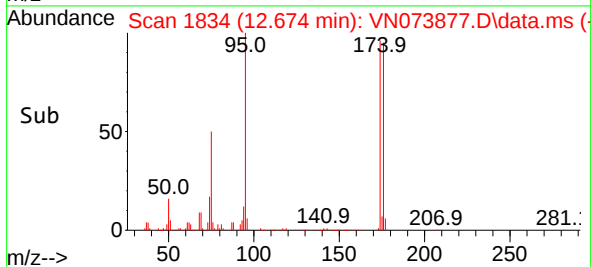
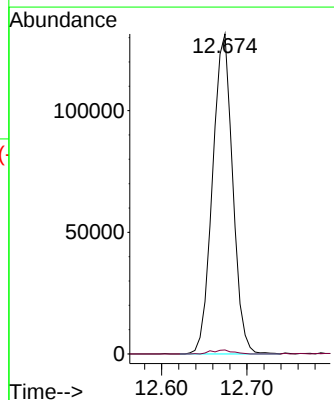
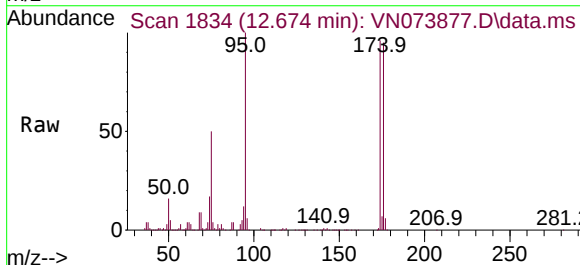


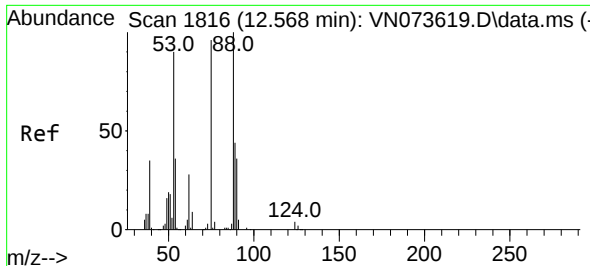

#81
trans-1,4-Dichloro-2-butene
Concen: 53.894 ug/l
RT: 12.674 min Scan# 1816
Delta R.T. 0.106 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#03


Tgt Ion: 75 Resp: 215617
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

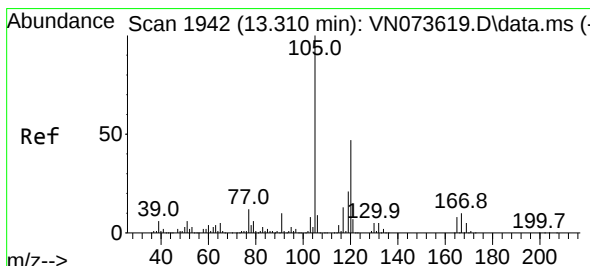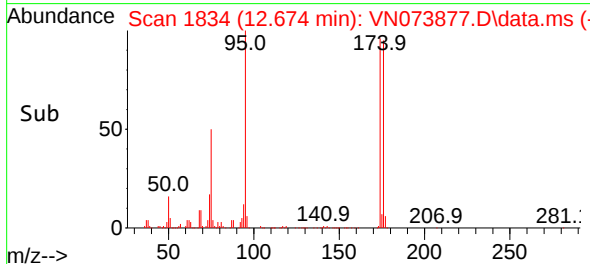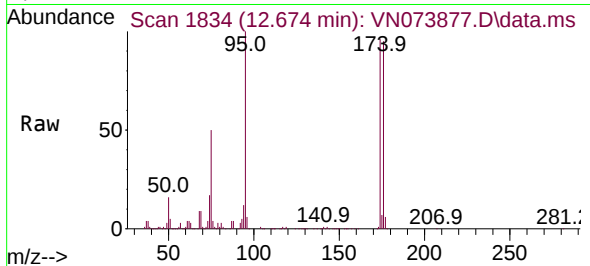

#84
1,2,4-Trimethylbenzene
Concen: 0.302 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. -0.006 min
Lab File: VN073877.D
Acq: 13 Aug 2022 18:53

Tgt Ion: 105 Resp: 9279
Ion Ratio Lower Upper
105 100
120 39.7 23.3 69.8

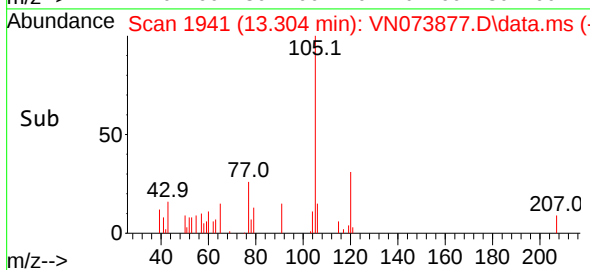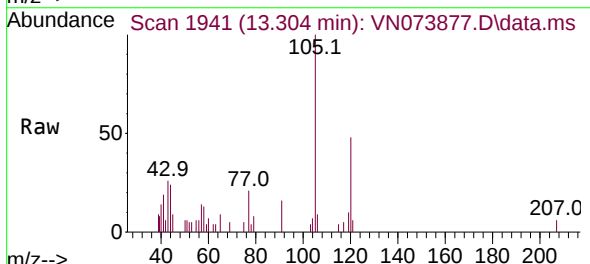

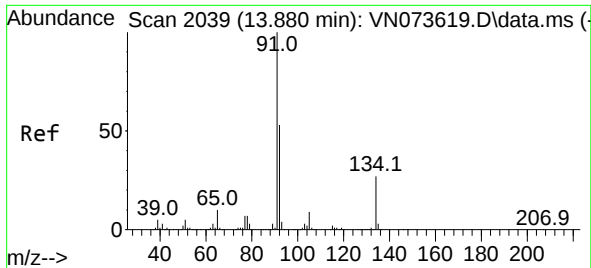

#89

n-Butylbenzene

Concen: 0.364 ug/l

RT: 13.810 min Scan# 20

Delta R.T. -0.071 min

Lab File: VN073877.D


Acq: 13 Aug 2022 18:53

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#03

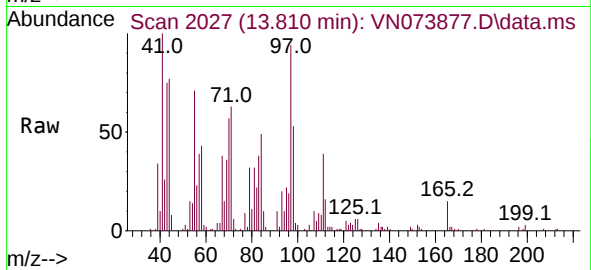

Tgt Ion: 91 Resp: 8923

Ion Ratio Lower Upper

91 100

92 14.4 26.9 80.7#

134 1.0 13.6 40.8#

