

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
 Data File : VN073879.D
 Acq On : 13 Aug 2022 19:42
 Operator : JC\MD
 Sample : PB146976ZHE#05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1


Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#05

Quant Time: Aug 14 02:38:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	658812	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	945027	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	911687	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	493495	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	296028	36.871	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	73.740%#		
35) Dibromofluoromethane	7.951	113	294664	49.655	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.320%		
50) Toluene-d8	10.380	98	994788	42.600	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	85.200%#		
62) 4-Bromofluorobenzene	12.674	95	419162	51.070	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	102.140%		
Target Compounds					Qvalue	
3) Chloromethane	2.269	50	1104	Below Cal		89
6) Chloroethane	2.934	64	54	Below Cal	#	1
11) Tert butyl alcohol	5.269	59	2588	1.495	ug/l #	72
16) Acetone	4.222	43	96691	22.422	ug/l	94
18) Methyl Acetate	4.793	43	14341	1.337	ug/l	94
20) Methylene Chloride	5.016	84	25564	1.528	ug/l	96
25) 2-Butanone	7.263	43	21681	3.237	ug/l	97
29) Tetrahydrofuran	7.616	42	4842	1.144	ug/l	89
31) Cyclohexane	8.016	56	10020	0.838	ug/l #	1
36) 1,1-Dichloropropene	8.022	75	40018	4.732	ug/l #	50
37) Ethyl Acetate	7.334	43	77969	7.000	ug/l	97
38) Carbon Tetrachloride	8.016	117	55748	6.490	ug/l #	16
41) Methacrylonitrile	7.622	41	2962	0.588	ug/l #	36
42) 1,2-Dichloroethane	8.486	62	2424	0.262	ug/l #	74
43) Isopropyl Acetate	8.498	43	475601	31.613	ug/l #	83
45) 1,2-Dichloropropane	9.569	63	4385	0.639	ug/l #	44
48) Methyl methacrylate	9.492	41	10548	1.602	ug/l #	40
49) 1,4-Dioxane	9.516	88	361	1.945	ug/l #	25
51) 4-Methyl-2-Pentanone	10.269	43	30789	2.853	ug/l #	76
52) Toluene	10.445	92	46830	2.792	ug/l	99
53) t-1,3-Dichloropropene	10.557	75	2662	0.295	ug/l #	1
54) cis-1,3-Dichloropropene	10.186	75	139122	13.666	ug/l #	60
57) 1,3-Dichloropropane	11.033	76	18725	1.578	ug/l #	42
59) 2-Hexanone	11.033	43	211775	25.904	ug/l #	49
68) m/p-Xylenes	11.886	106	8467	0.680	ug/l	95
69) o-Xylene	12.222	106	3717	0.306	ug/l	86
71) Bromoform	12.669	173	2386	0.416	ug/l #	28
74) N-amyl acetate	12.292	43	19122	1.401	ug/l #	45
76) 1,2,3-Trichloropropane	12.669	75	207724	21.115	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.669	75	207724	54.549	ug/l #	10





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion:168 Resp: 658812
Ion Ratio Lower Upper
168 100
99 47.5 42.3 63.5

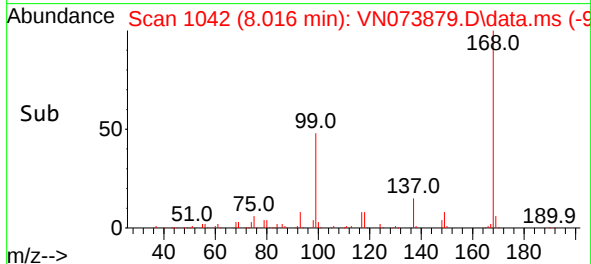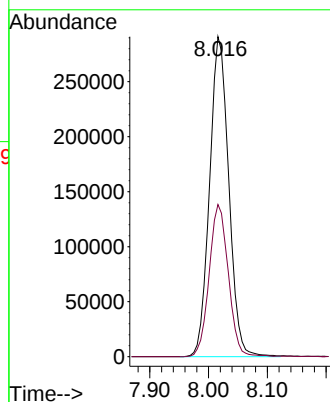

#3
Chloromethane
Concen: Below Cal
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 50 Resp: 1104
Ion Ratio Lower Upper
50 100
52 26.1 25.7 38.5


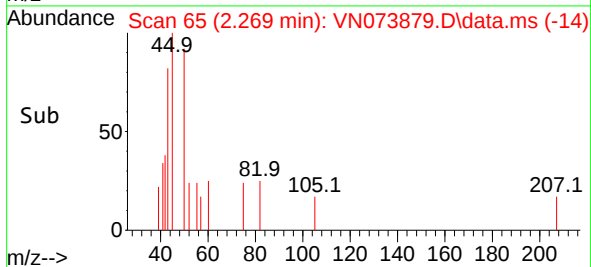
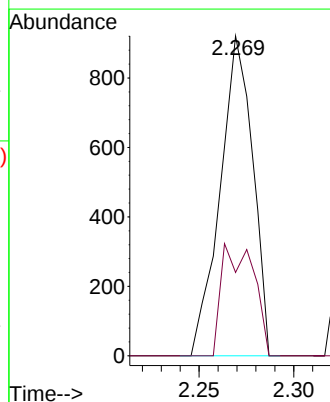
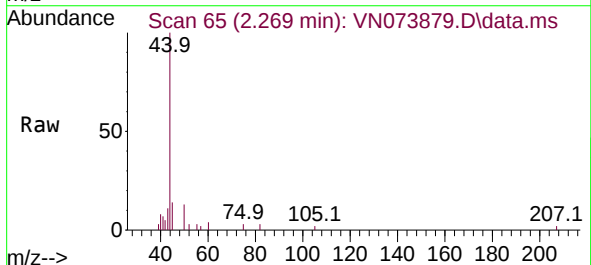


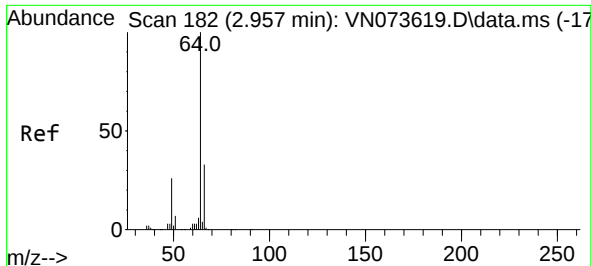

#6
Chloroethane
Concen: Below Cal
RT: 2.934 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 64 Resp: 54
Ion Ratio Lower Upper
64 100
66 106.6 26.2 39.4#

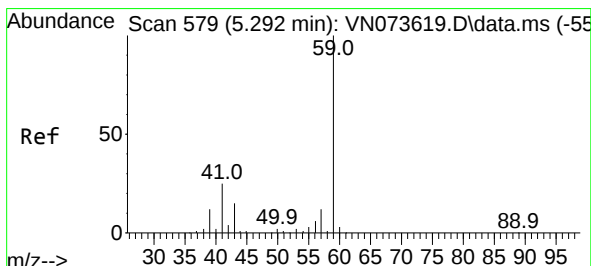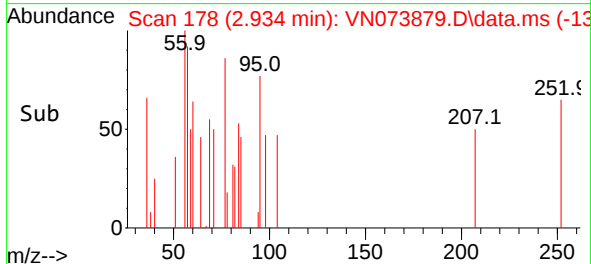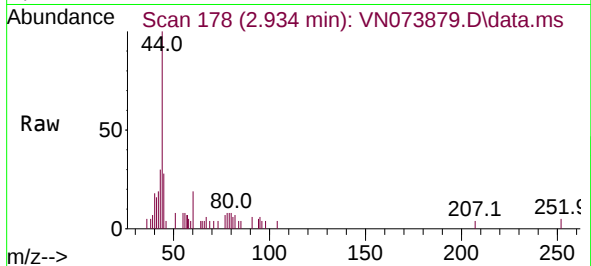

#11
Tert butyl alcohol
Concen: 1.495 ug/l
RT: 5.269 min Scan# 575
Delta R.T. -0.023 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 59 Resp: 2588
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

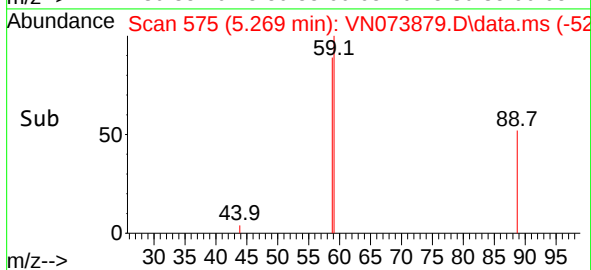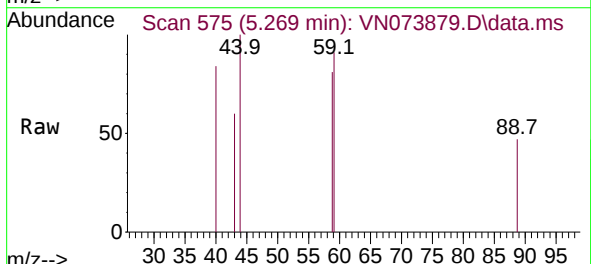



#16

Acetone

Concen: 22.422 ug/l

RT: 4.222 min Scan# 397

Delta R.T. 0.000 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42

Instrument :

MSVOA_N

ClientSampleId :





PB146976ZHE#05

Tgt Ion: 43 Resp: 96691

Ion Ratio Lower Upper

43 100

58 35.7 26.0 39.0

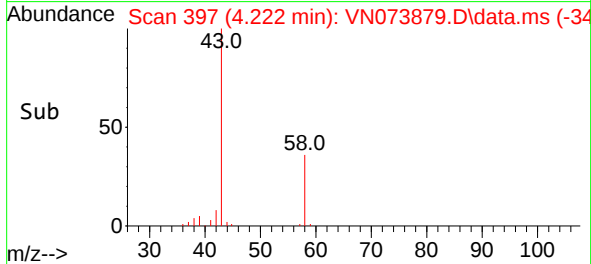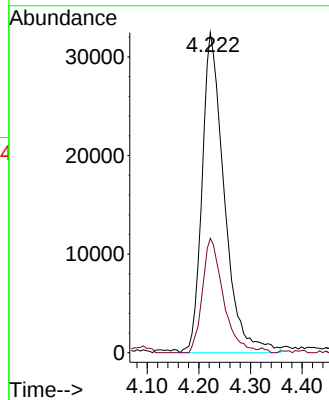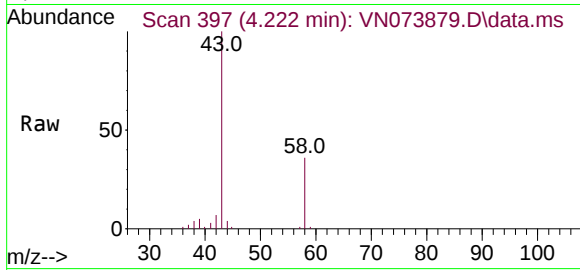

#18

Methyl Acetate

Concen: 1.337 ug/l

RT: 4.793 min Scan# 494

Delta R.T. 0.012 min

Lab File: VN073879.D




Acq: 13 Aug 2022 19:42


Tgt Ion: 43 Resp: 14341

Ion Ratio Lower Upper

43 100

74 30.1 21.6 32.4


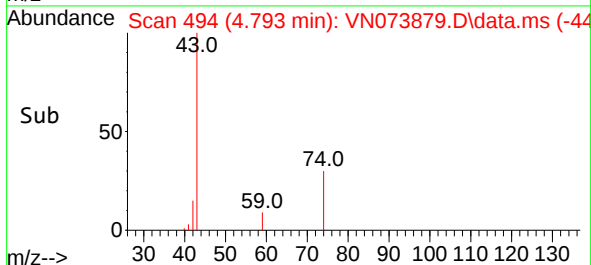
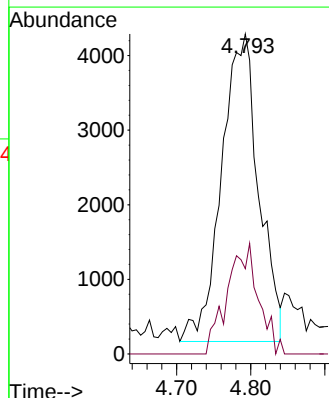
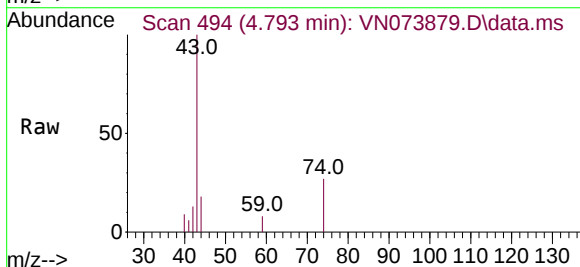


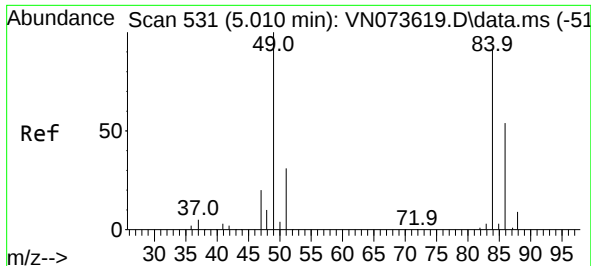

#20
Methylene Chloride
Concen: 1.528 ug/l
RT: 5.016 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 84	Resp: 25564
Ion Ratio	Lower Upper
84 100	
49 108.5	88.3 132.5
51 35.8	28.2 42.2
86 69.6	50.6 76.0

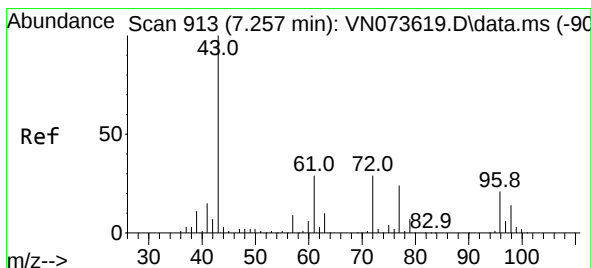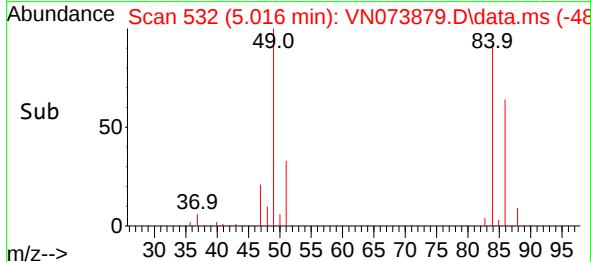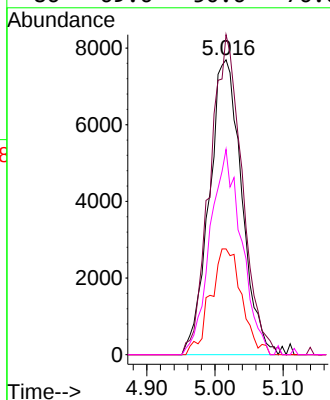

#25
2-Butanone
Concen: 3.237 ug/l
RT: 7.263 min Scan# 914
Delta R.T. 0.006 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 43	Resp: 21681
Ion Ratio	Lower Upper
43 100	
72 27.9	23.7 35.5

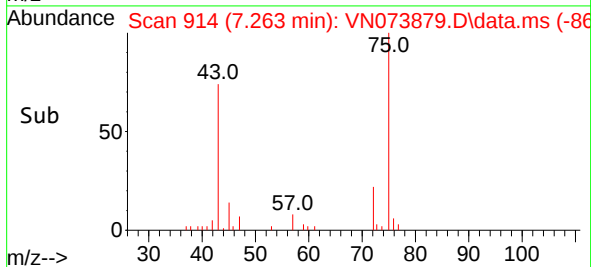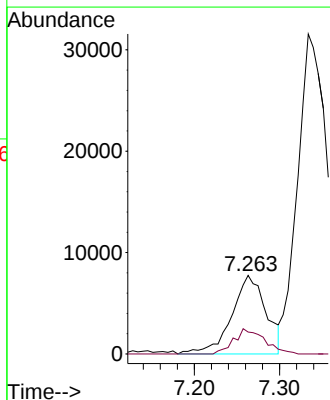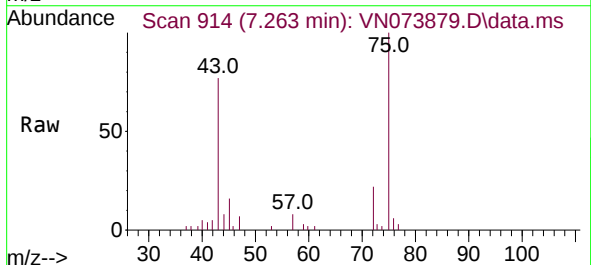

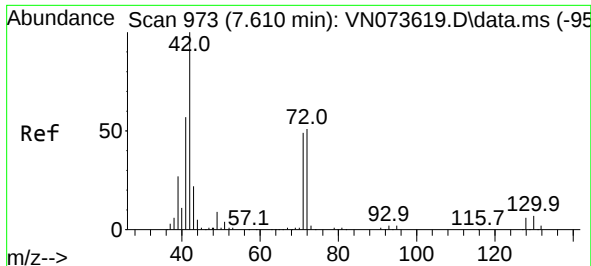

#29

Tetrahydrofuran

Concen: 1.144 ug/l

RT: 7.616 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#05





Tgt Ion: 42 Resp: 4842

Ion Ratio Lower Upper

42 100

72 41.0 39.7 59.5

71 39.6 36.6 55.0

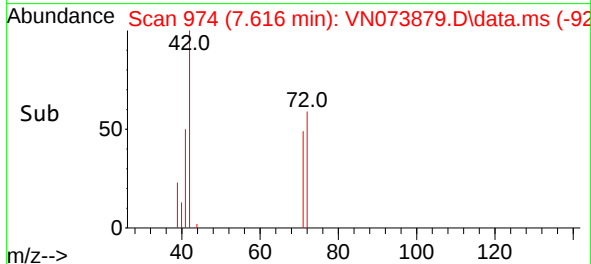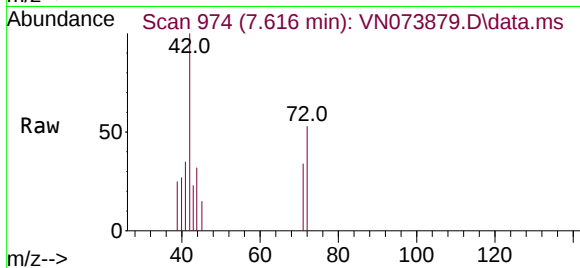

#31

Cyclohexane

Concen: 0.838 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.006 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42




Tgt Ion: 56 Resp: 10020


Ion Ratio Lower Upper

56 100

69 184.4 27.8 41.8#

84 141.5 76.9 115.3#

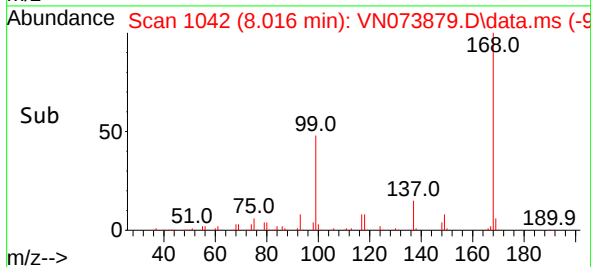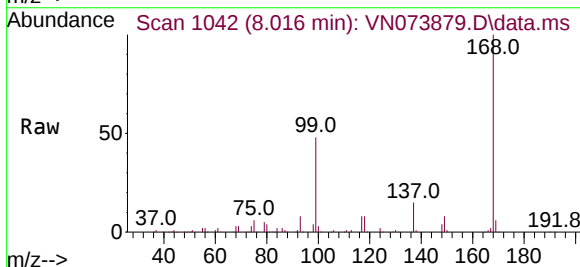

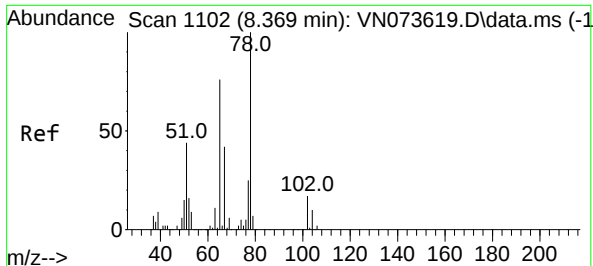

#33

1,2-Dichloroethane-d4

Concen: 36.871 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. 0.000 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42

Instrument :

MSVOA_N

ClientSampleId :





PB146976ZHE#05

Tgt Ion: 65 Resp: 296028

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.8

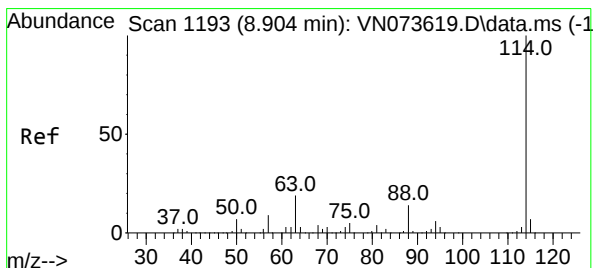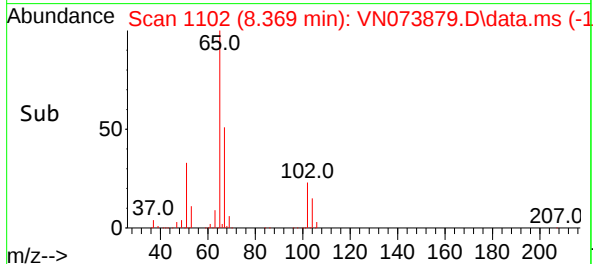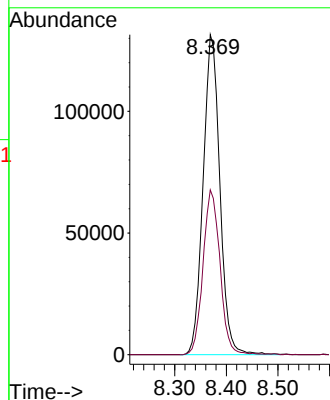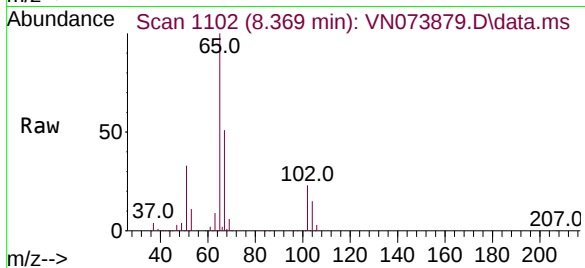

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42




Tgt Ion: 114 Resp: 945027


Ion Ratio Lower Upper

114 100

63 17.2 0.0 40.0

88 15.0 0.0 32.6

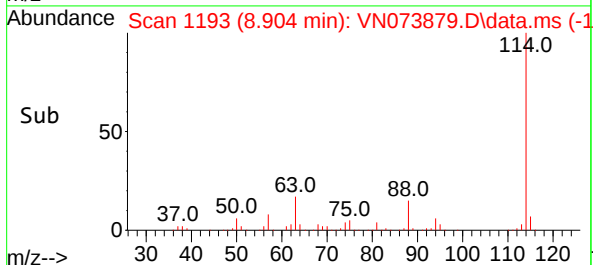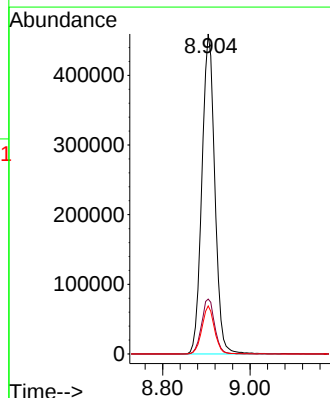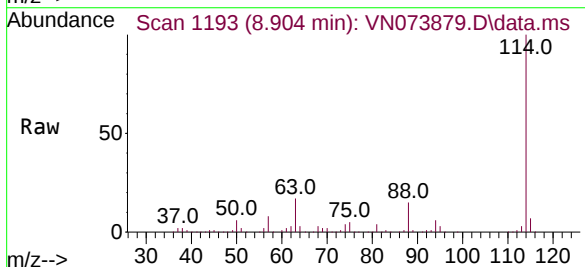

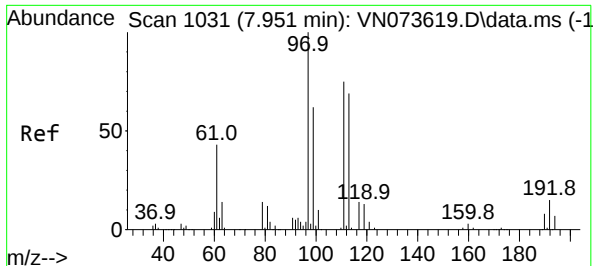

#35

Dibromofluoromethane

Concen: 49.655 ug/l

RT: 7.951 min Scan# 1043

Delta R.T. 0.000 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#05





Tgt Ion:113 Resp: 294664

Ion Ratio Lower Upper

113 100

111 102.9 81.4 122.0

192 24.4 17.0 25.6

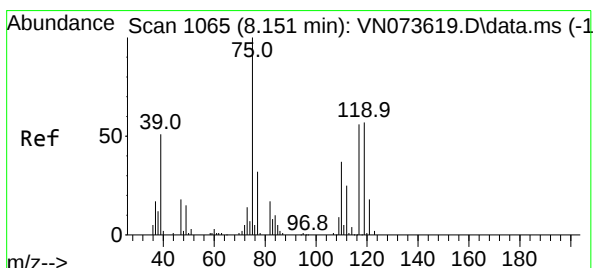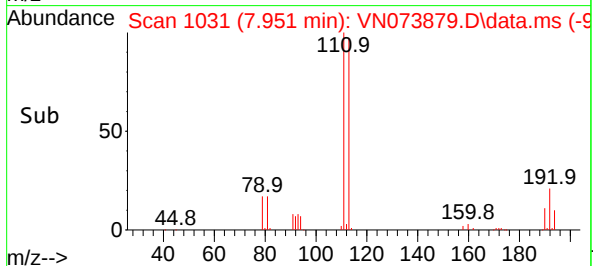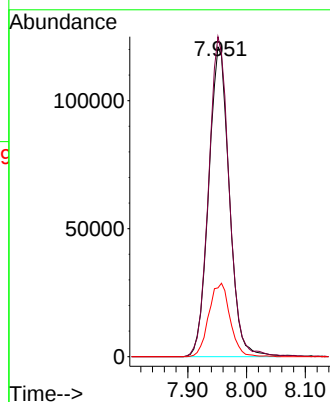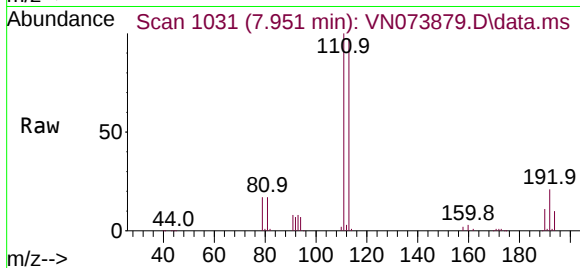

#36

1,1-Dichloropropene

Concen: 4.732 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. -0.129 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42




Tgt Ion: 75 Resp: 40018


Ion Ratio Lower Upper

75 100

110 9.9 18.3 54.8#

77 0.0 25.1 37.7#


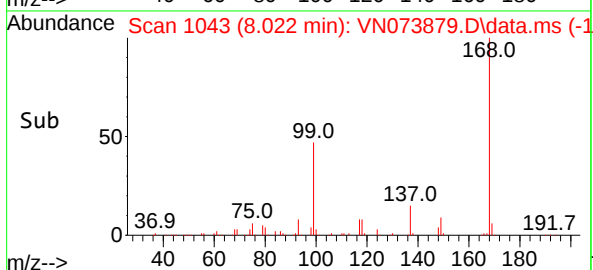
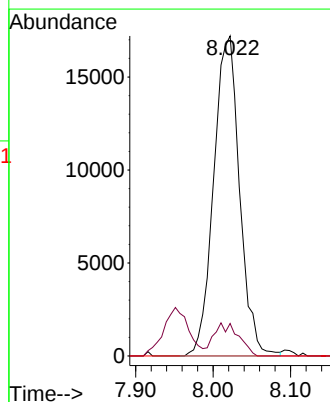
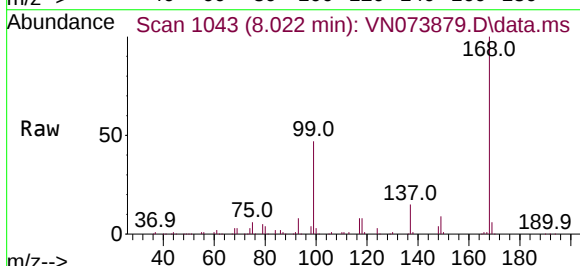


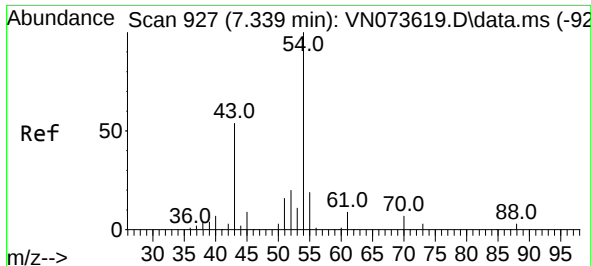

#37
Ethyl Acetate
Concen: 7.000 ug/l
RT: 7.334 min Scan# 91
Delta R.T. -0.006 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 43	Resp: 77969
Ion Ratio	Lower Upper
43 100	
61 15.9	11.8 17.6
70 12.5	9.3 13.9

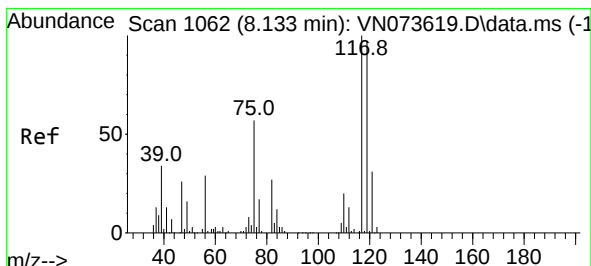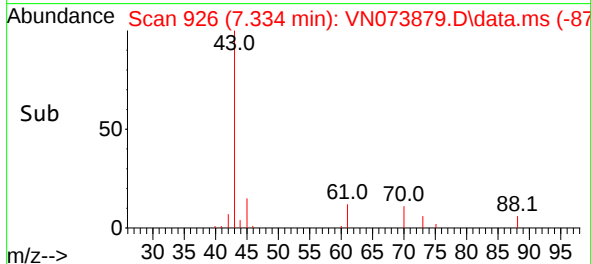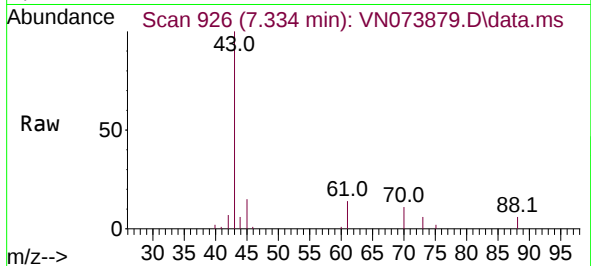

#38
Carbon Tetrachloride
Concen: 6.490 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 117	Resp: 55748
Ion Ratio	Lower Upper
117 100	
119 5.1	75.8 113.8#
121 0.0	24.6 37.0#


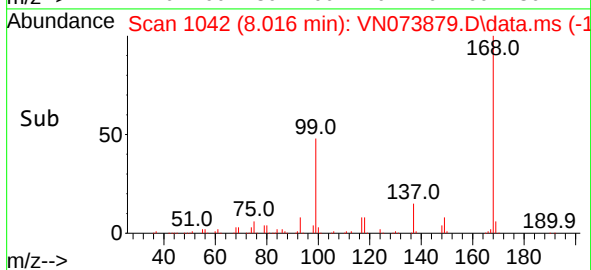

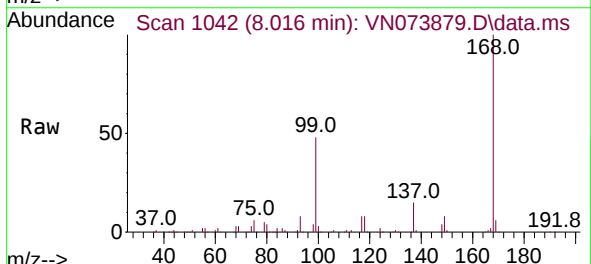


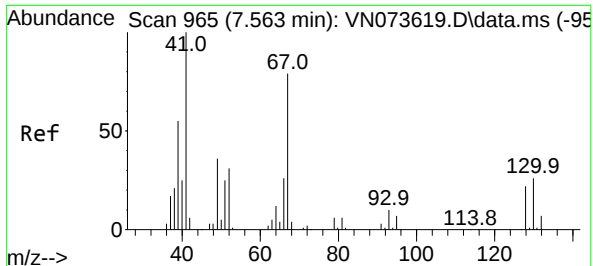

#41
Methacrylonitrile
Concen: 0.588 ug/l
RT: 7.622 min Scan# 91
Delta R.T. 0.059 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 41 Resp: 2962
Ion Ratio Lower Upper
41 100
39 47.5 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

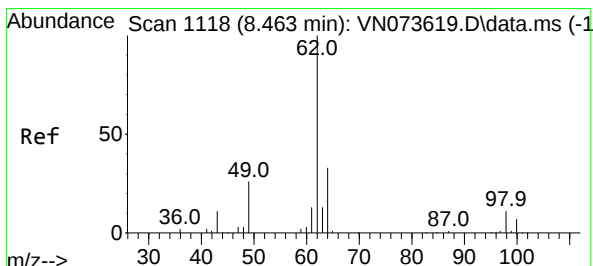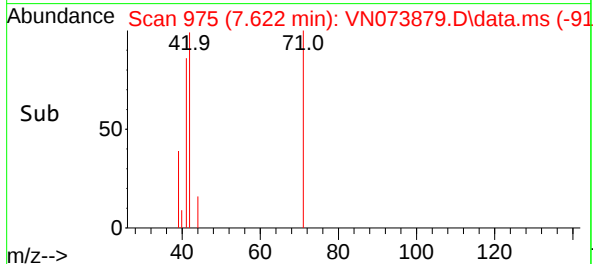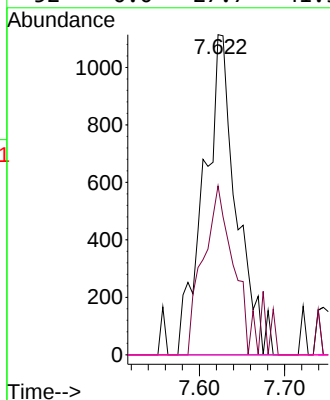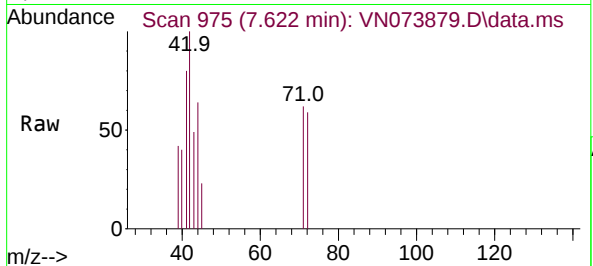

#42
1,2-Dichloroethane
Concen: 0.262 ug/l
RT: 8.486 min Scan# 1122
Delta R.T. 0.024 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 62 Resp: 2424
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4

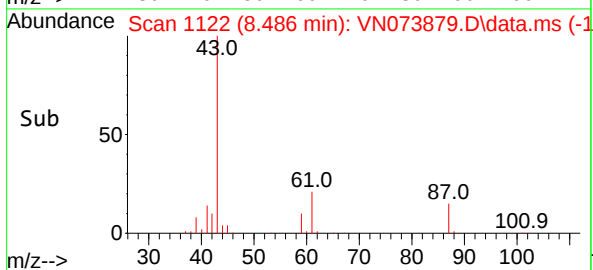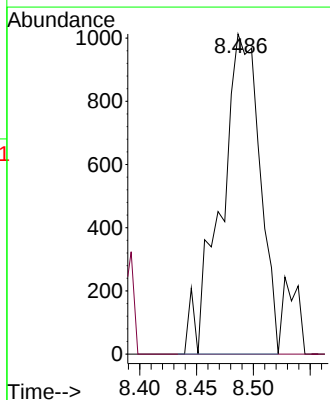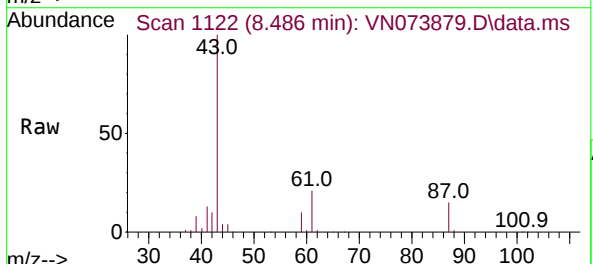

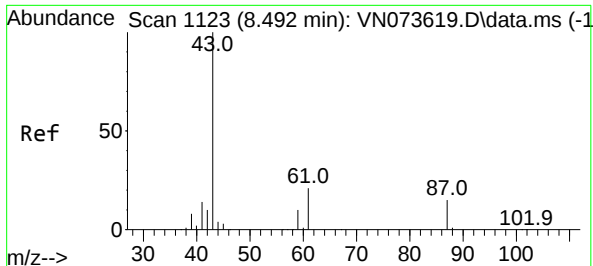

#43

Isopropyl Acetate

Concen: 31.613 ug/l

RT: 8.498 min Scan# 1123

Delta R.T. 0.006 min

Lab File: VN073879.D

Acq: 13 Aug 2022 19:42

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#05





Tgt Ion: 43 Resp: 475601

Ion Ratio Lower Upper

43 100

61 15.8 21.9 32.9#

87 11.9 12.0 18.0#

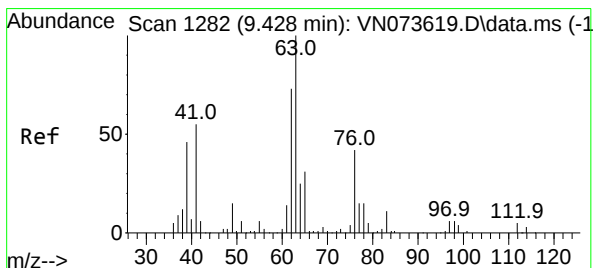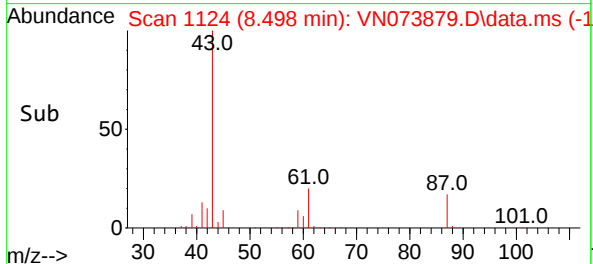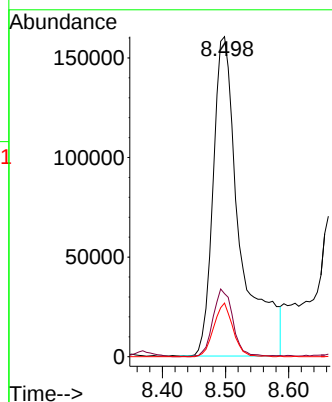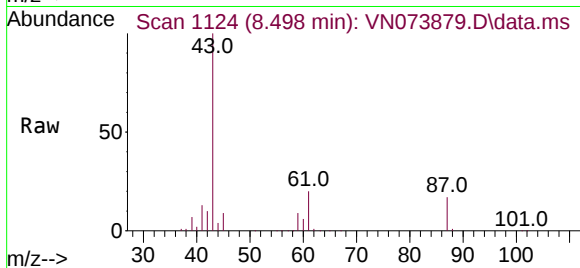

#45

1,2-Dichloropropane

Concen: 0.639 ug/l

RT: 9.569 min Scan# 1306

Delta R.T. 0.141 min

Lab File: VN073879.D




Acq: 13 Aug 2022 19:42


Tgt Ion: 63 Resp: 4385

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#


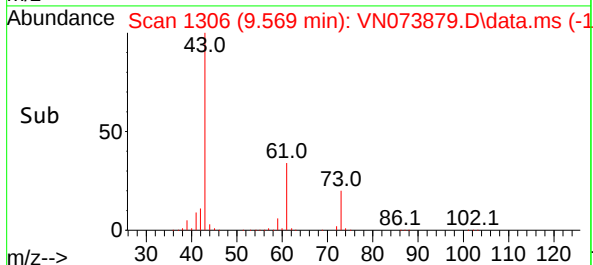

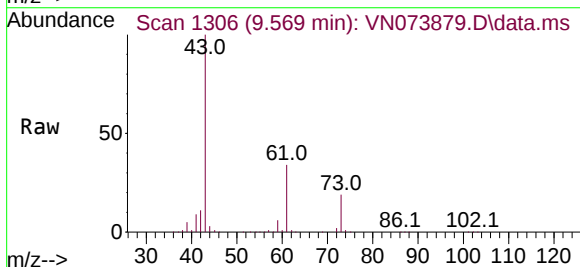


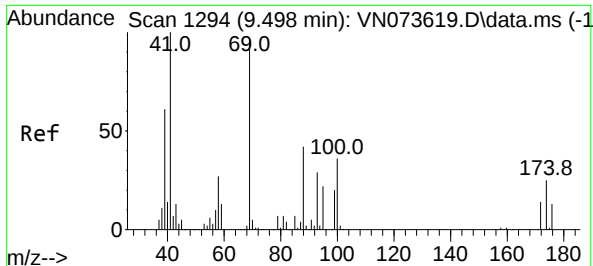

#48
Methyl methacrylate
Concen: 1.602 ug/l
RT: 9.492 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 41 Resp: 10548
Ion Ratio Lower Upper
41 100
69 2.1 74.7 112.1#
39 58.2 45.6 68.4

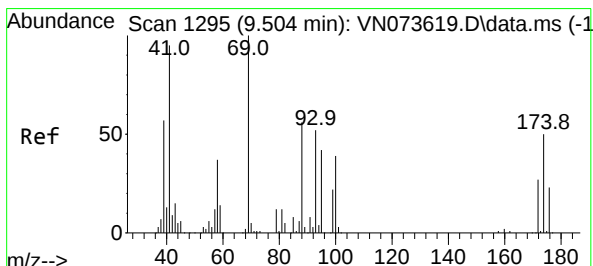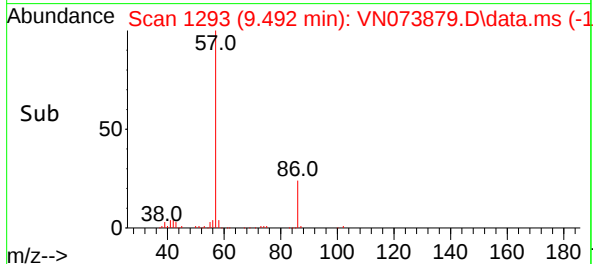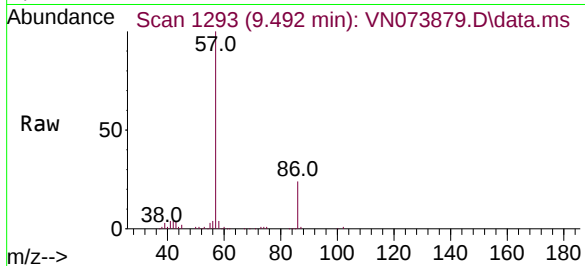

#49
1,4-Dioxane
Concen: 1.945 ug/l
RT: 9.516 min Scan# 1297
Delta R.T. 0.012 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 88 Resp: 361
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 0.0 54.2 81.4#


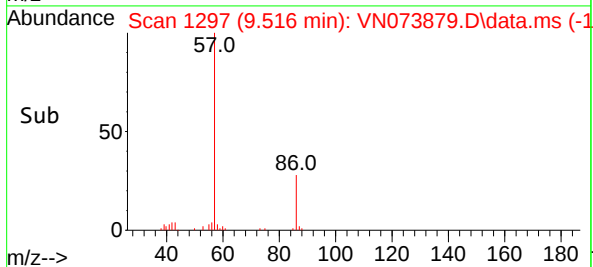

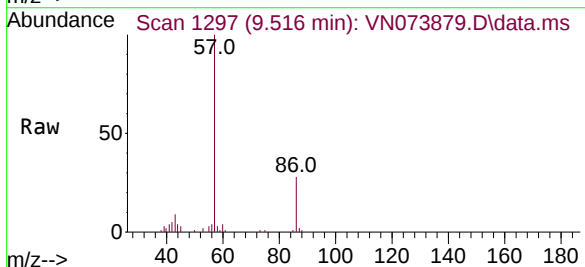


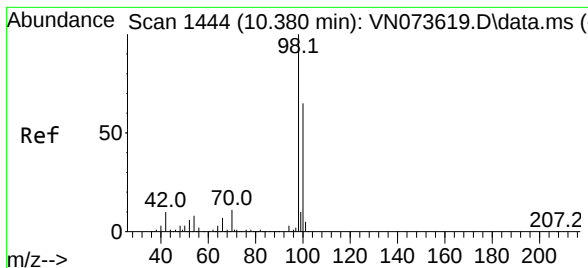

#50
Toluene-d8
Concen: 42.600 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 98 Resp: 994788
Ion Ratio Lower Upper
98 100
100 65.5 52.6 78.8

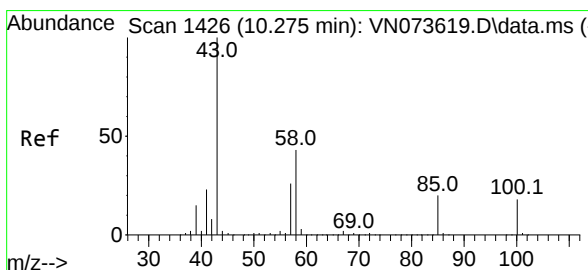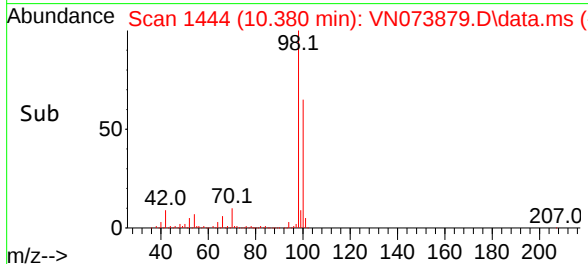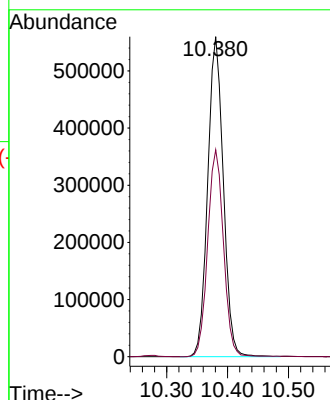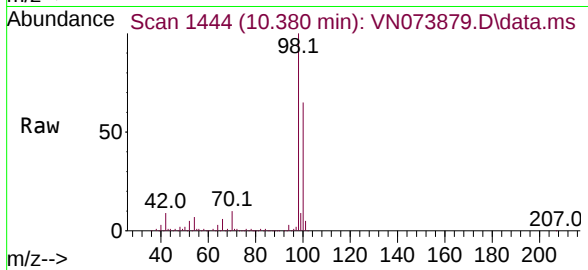

#51
4-Methyl-2-Pentanone
Concen: 2.853 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.006 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 43 Resp: 30789
Ion Ratio Lower Upper
43 100
58 27.2 34.1 51.1#


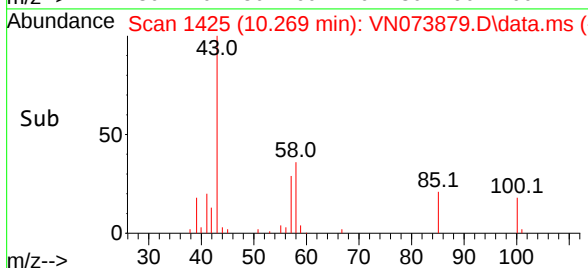
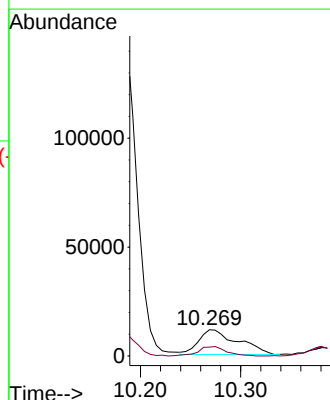
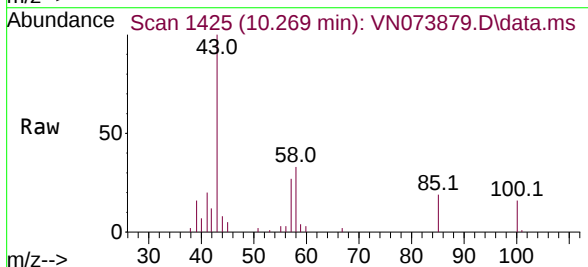


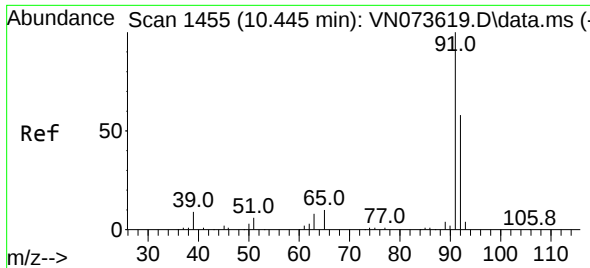

#52
Toluene
Concen: 2.792 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 92 Resp: 46830
Ion Ratio Lower Upper
92 100
91 171.1 138.6 207.8

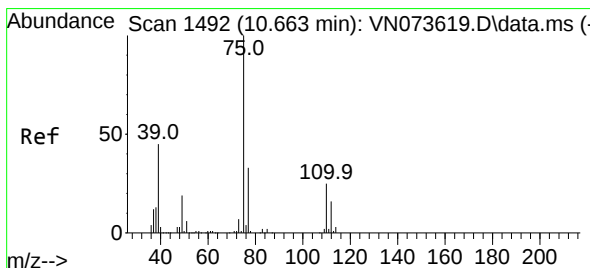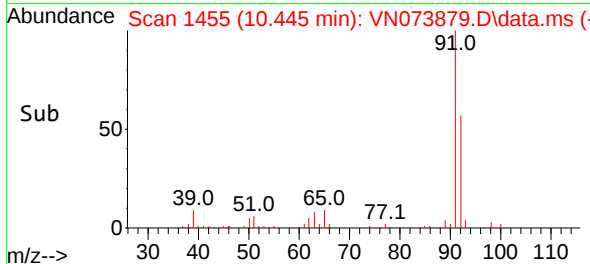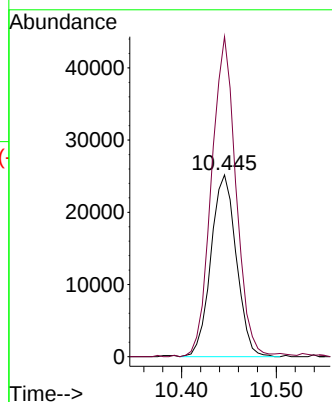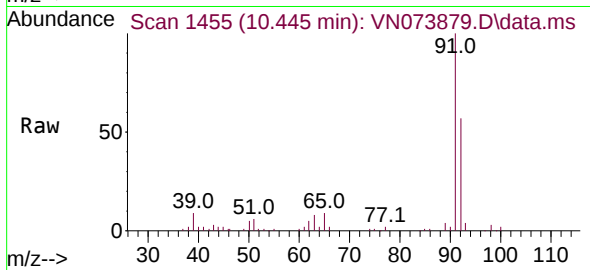

#53
t-1,3-Dichloropropene
Concen: 0.295 ug/l
RT: 10.557 min Scan# 1474
Delta R.T. -0.106 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 75 Resp: 2662
Ion Ratio Lower Upper
75 100
77 88.8 25.6 38.4#


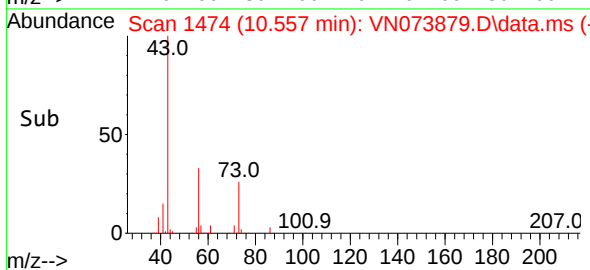
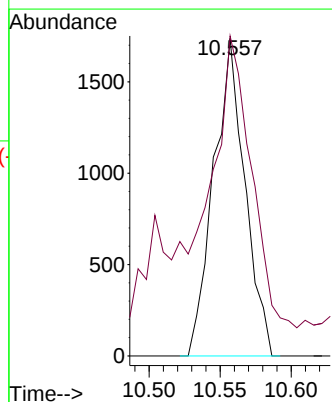
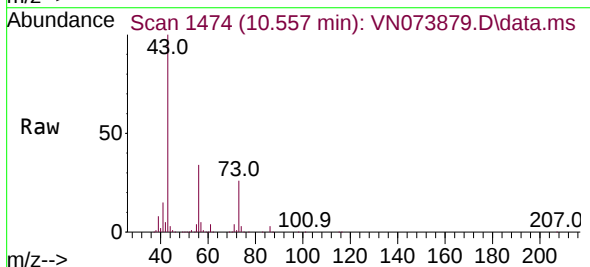


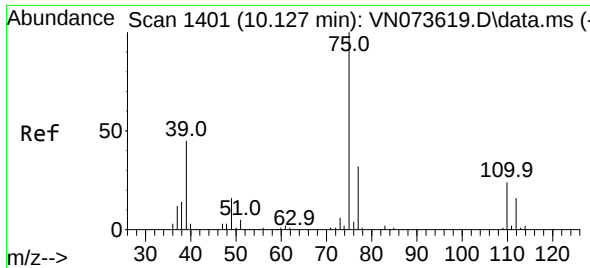

#54
 cis-1,3-Dichloropropene
 Concen: 13.666 ug/l
 RT: 10.186 min Scan# 14
 Delta R.T. 0.059 min
 Lab File: VN073879.D
 Acq: 13 Aug 2022 19:42




Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#05


Tgt Ion: 75 Resp: 139122
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.2 37.8#
 39 25.7 35.7 53.5#

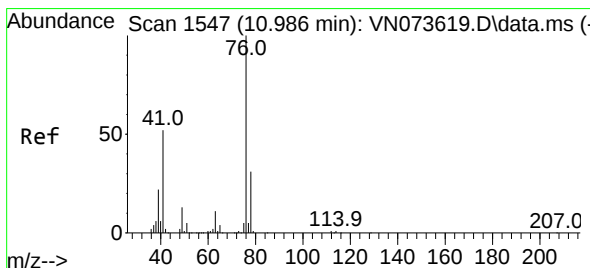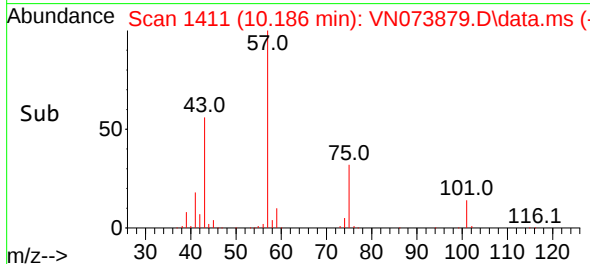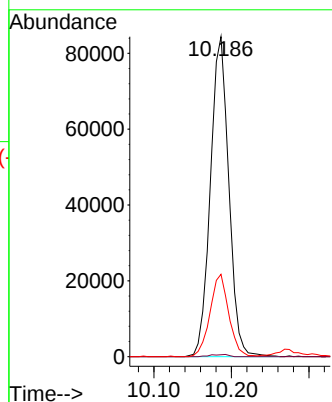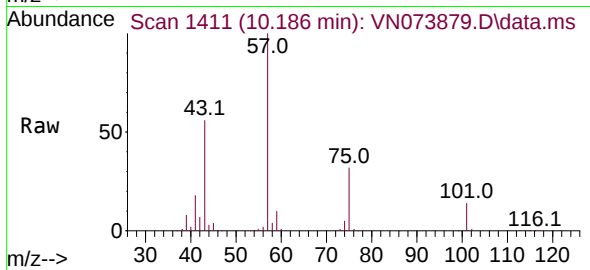

#57
 1,3-Dichloropropane
 Concen: 1.578 ug/l
 RT: 11.033 min Scan# 1555
 Delta R.T. 0.047 min
 Lab File: VN073879.D
 Acq: 13 Aug 2022 19:42

Tgt Ion: 76 Resp: 18725
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.2#


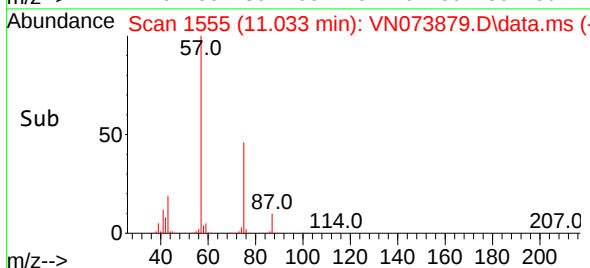

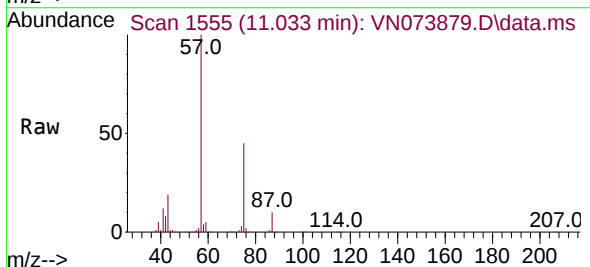


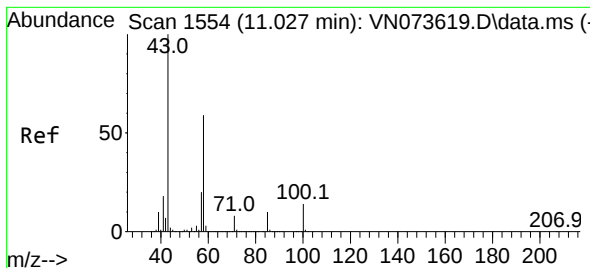

#59
2-Hexanone
Concen: 25.904 ug/l
RT: 11.033 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion: 43 Resp: 211775
Ion Ratio Lower Upper
43 100
58 20.8 29.7 89.1#

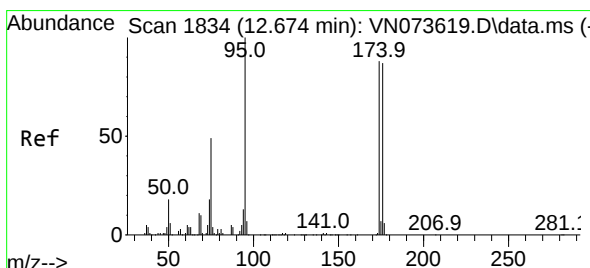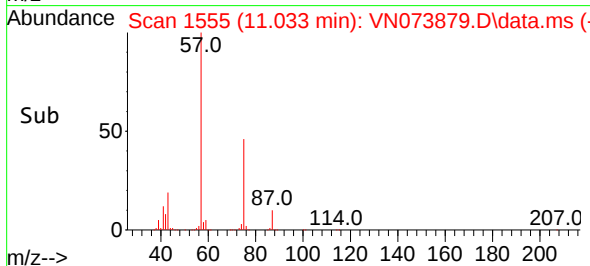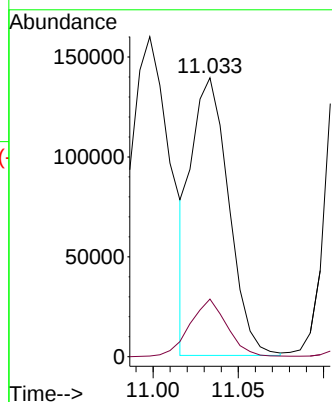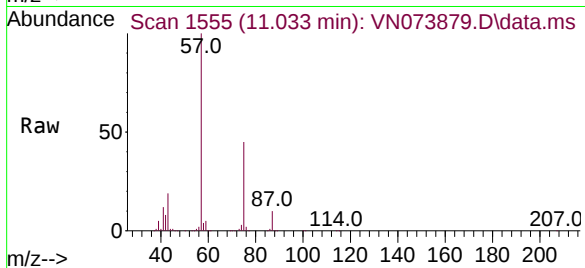

#62
4-Bromofluorobenzene
Concen: 51.070 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 95 Resp: 419162
Ion Ratio Lower Upper
95 100
174 97.6 0.0 167.6
176 92.5 0.0 163.4


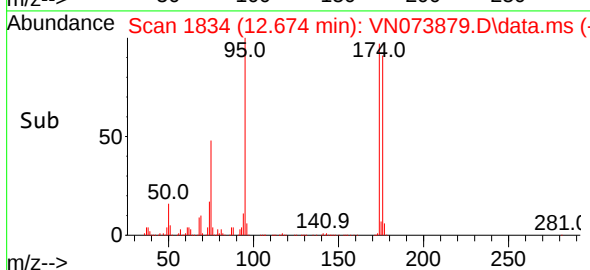

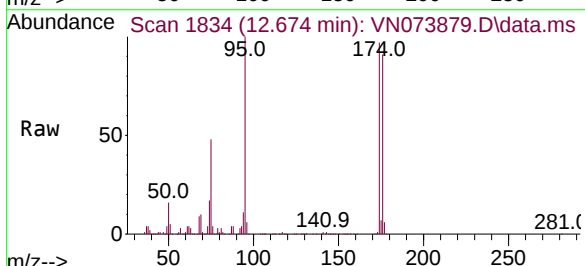


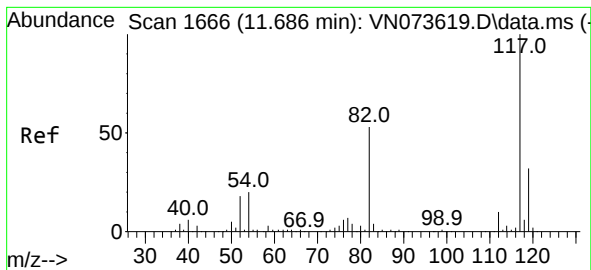

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion:117 Resp: 911687
Ion Ratio Lower Upper
117 100
82 49.0 44.2 66.2
119 32.3 25.4 38.0

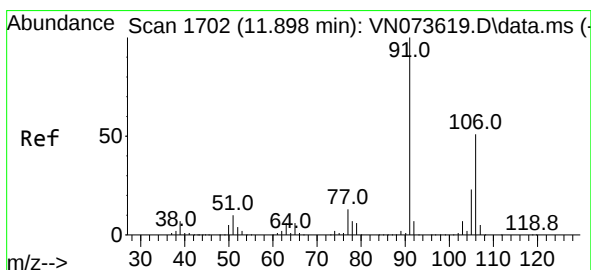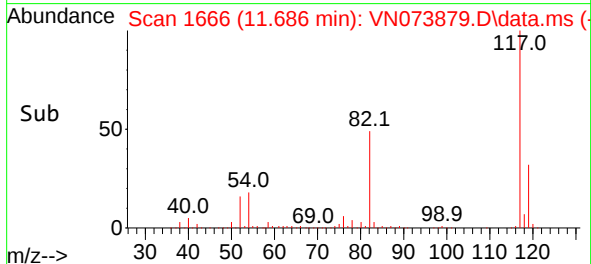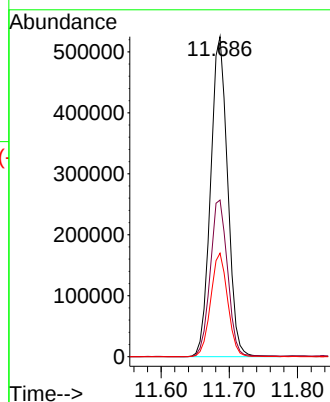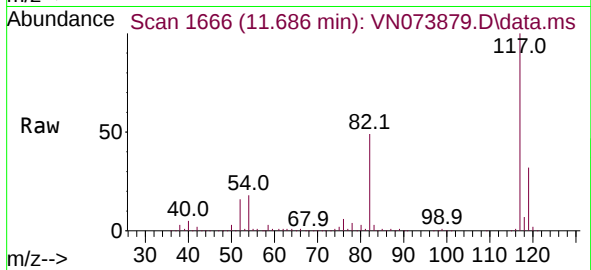

#68
m/p-Xylenes
Concen: 0.680 ug/l
RT: 11.886 min Scan# 1700
Delta R.T. -0.012 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion:106 Resp: 8467
Ion Ratio Lower Upper
106 100
91 190.7 158.9 238.3


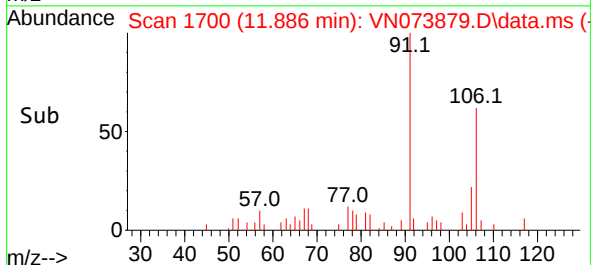
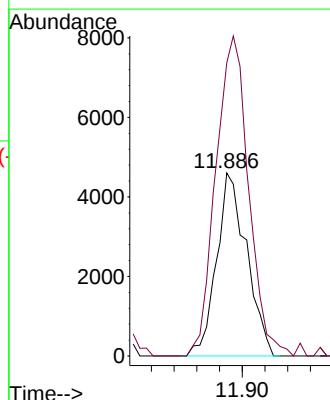
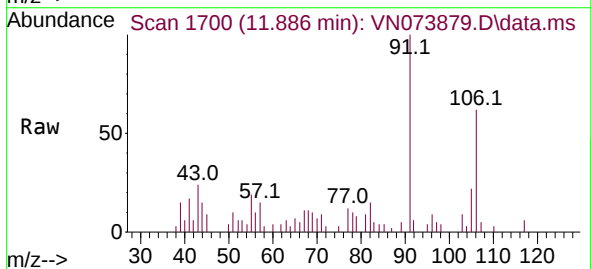




#69
o-Xylene
Concen: 0.306 ug/l
RT: 12.222 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion:106 Resp: 3717
Ion Ratio Lower Upper
106 100
91 190.1 106.0 318.0

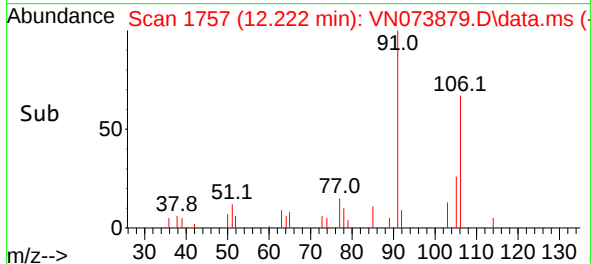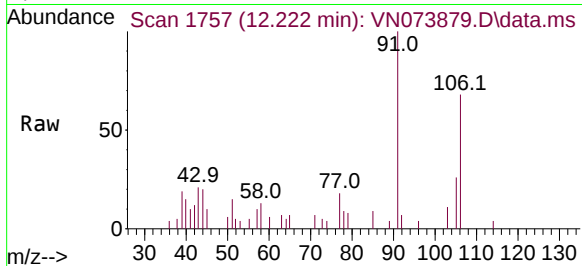

#71
Bromoform
Concen: 0.416 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.271 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion:173 Resp: 2386
Ion Ratio Lower Upper
173 100
175 0.0 24.6 73.6#
254 0.0 0.1 0.1#


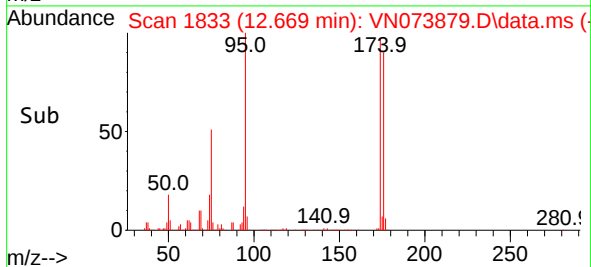

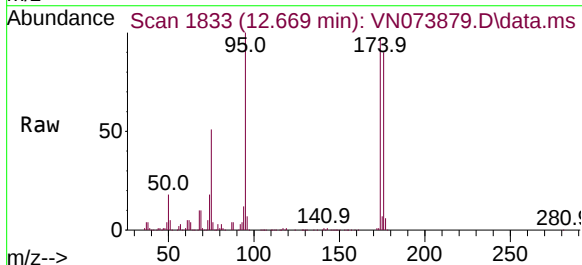


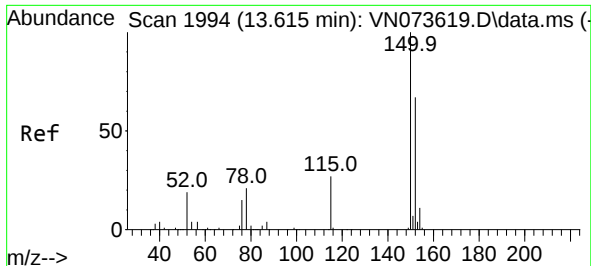

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05


Tgt Ion:152 Resp: 493495
Ion Ratio Lower Upper
152 100
115 53.1 28.9 86.7
150 155.4 0.0 356.2

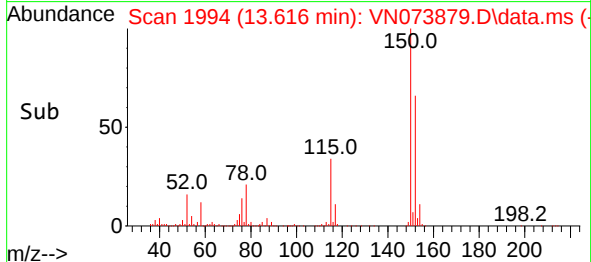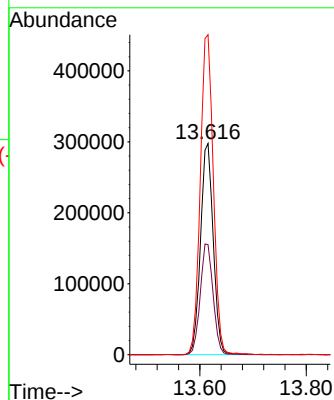

#74
N-ethyl acetate
Concen: 1.401 ug/l
RT: 12.292 min Scan# 1769
Delta R.T. -0.035 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 43 Resp: 19122
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 11.6 21.1 31.7#
61 0.0 21.1 31.7#


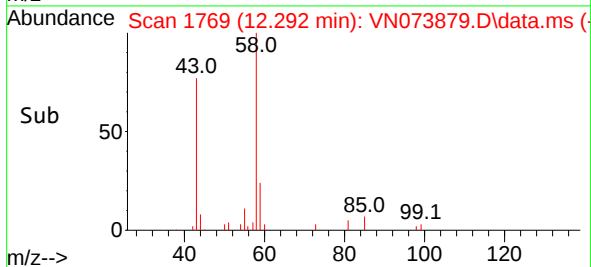
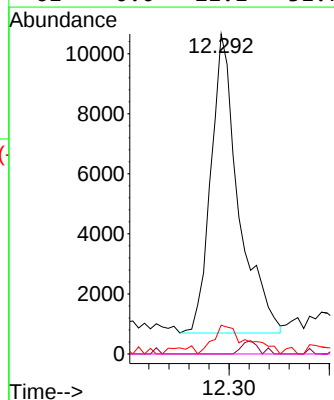
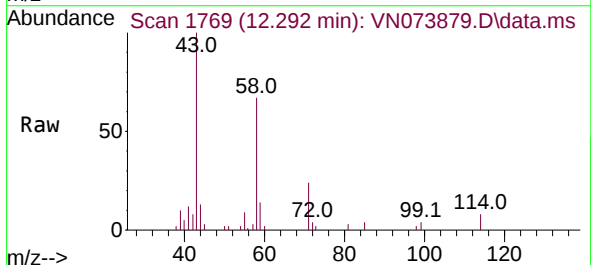


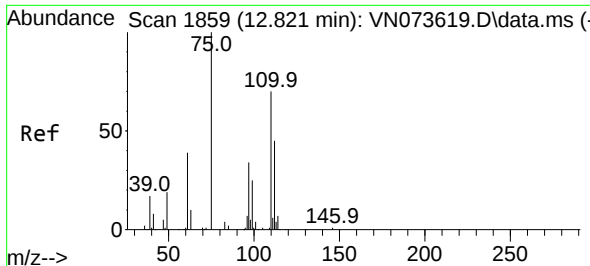

#76
1,2,3-Trichloropropane
Concen: 21.115 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.152 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#05

Tgt Ion: 75 Resp: 207724
Ion Ratio Lower Upper
75 100
77 1.0 98.5 295.5#

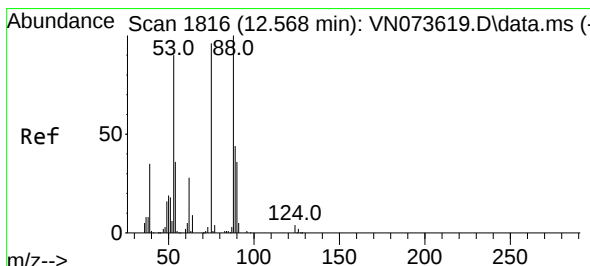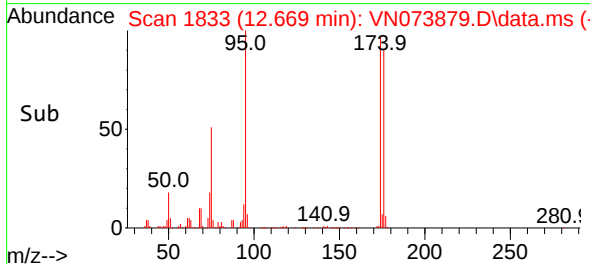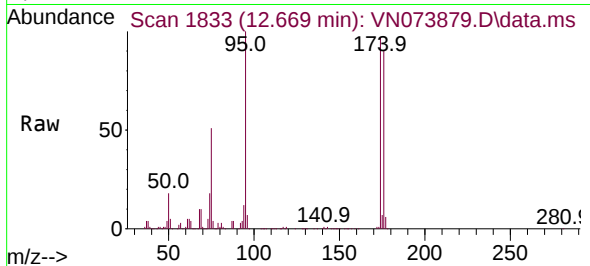

#81
trans-1,4-Dichloro-2-butene
Concen: 54.549 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.100 min
Lab File: VN073879.D
Acq: 13 Aug 2022 19:42

Tgt Ion: 75 Resp: 207724
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

