

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
 Data File : VN073883.D
 Acq On : 13 Aug 2022 21:20
 Operator : JC\MD
 Sample : PB146976ZHE#09
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#09

Quant Time: Aug 14 02:40:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 05:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	625585	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	902393	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.687	117	865298	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	459074	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	281325	36.901	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	73.800%#		
35) Dibromofluoromethane	7.951	113	280553	49.511	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.020%		
50) Toluene-d8	10.381	98	947521	42.493	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	84.980%#		
62) 4-Bromofluorobenzene	12.669	95	386281	49.384	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.760%		
Target Compounds						Qvalue
3) Chloromethane	2.264	50	928	Below Cal		94
6) Chloroethane	3.005	64	55	Below Cal	#	42
11) Tert butyl alcohol	5.293	59	879	0.535	ug/l #	72
16) Acetone	4.222	43	89699	21.906	ug/l	100
18) Methyl Acetate	4.781	43	11001	1.080	ug/l	97
20) Methylene Chloride	5.022	84	24820	1.614	ug/l	87
25) 2-Butanone	7.257	43	19508	3.068	ug/l	96
26) 2,2-Dichloropropane	7.240	77	2572	0.265	ug/l #	53
29) Tetrahydrofuran	7.616	42	4095	1.019	ug/l #	89
31) Cyclohexane	8.016	56	10067	0.887	ug/l #	1
36) 1,1-Dichloropropene	8.016	75	37585	4.654	ug/l #	50
37) Ethyl Acetate	7.340	43	73367	6.898	ug/l	96
38) Carbon Tetrachloride	8.016	117	52732	6.429	ug/l #	18
41) Methacrylonitrile	7.616	41	2242	0.466	ug/l #	40
42) 1,2-Dichloroethane	8.493	62	2075	0.235	ug/l #	74
43) Isopropyl Acetate	8.498	43	394059	27.430	ug/l #	87
48) Methyl methacrylate	9.493	41	10570	1.681	ug/l #	38
49) 1,4-Dioxane	9.493	88	113	0.637	ug/l #	1
51) 4-Methyl-2-Pentanone	10.269	43	27377	2.657	ug/l #	80
52) Toluene	10.445	92	18416	1.150	ug/l	95
53) t-1,3-Dichloropropene	10.551	75	2857	0.331	ug/l #	53
54) cis-1,3-Dichloropropene	10.181	75	131161	13.493	ug/l #	60
57) 1,3-Dichloropropane	11.034	76	17625	1.555	ug/l #	42
59) 2-Hexanone	11.034	43	200947	25.741	ug/l #	49
68) m/p-Xylenes	11.887	106	3224	0.273	ug/l	98
71) Bromoform	12.669	173	1902	0.350	ug/l #	28
74) N-amyl acetate	12.292	43	9542	0.752	ug/l #	43
76) 1,2,3-Trichloropropane	12.669	75	193516	21.150	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.669	75	193516	54.628	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081322\
Data File : VN073883.D
Acq On : 13 Aug 2022 21:20
Operator : JC\MD
Sample : PB146976ZHE#09
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09

Quant Time: Aug 14 02:40:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 05:09:32 2022
Response via : Initial Calibration




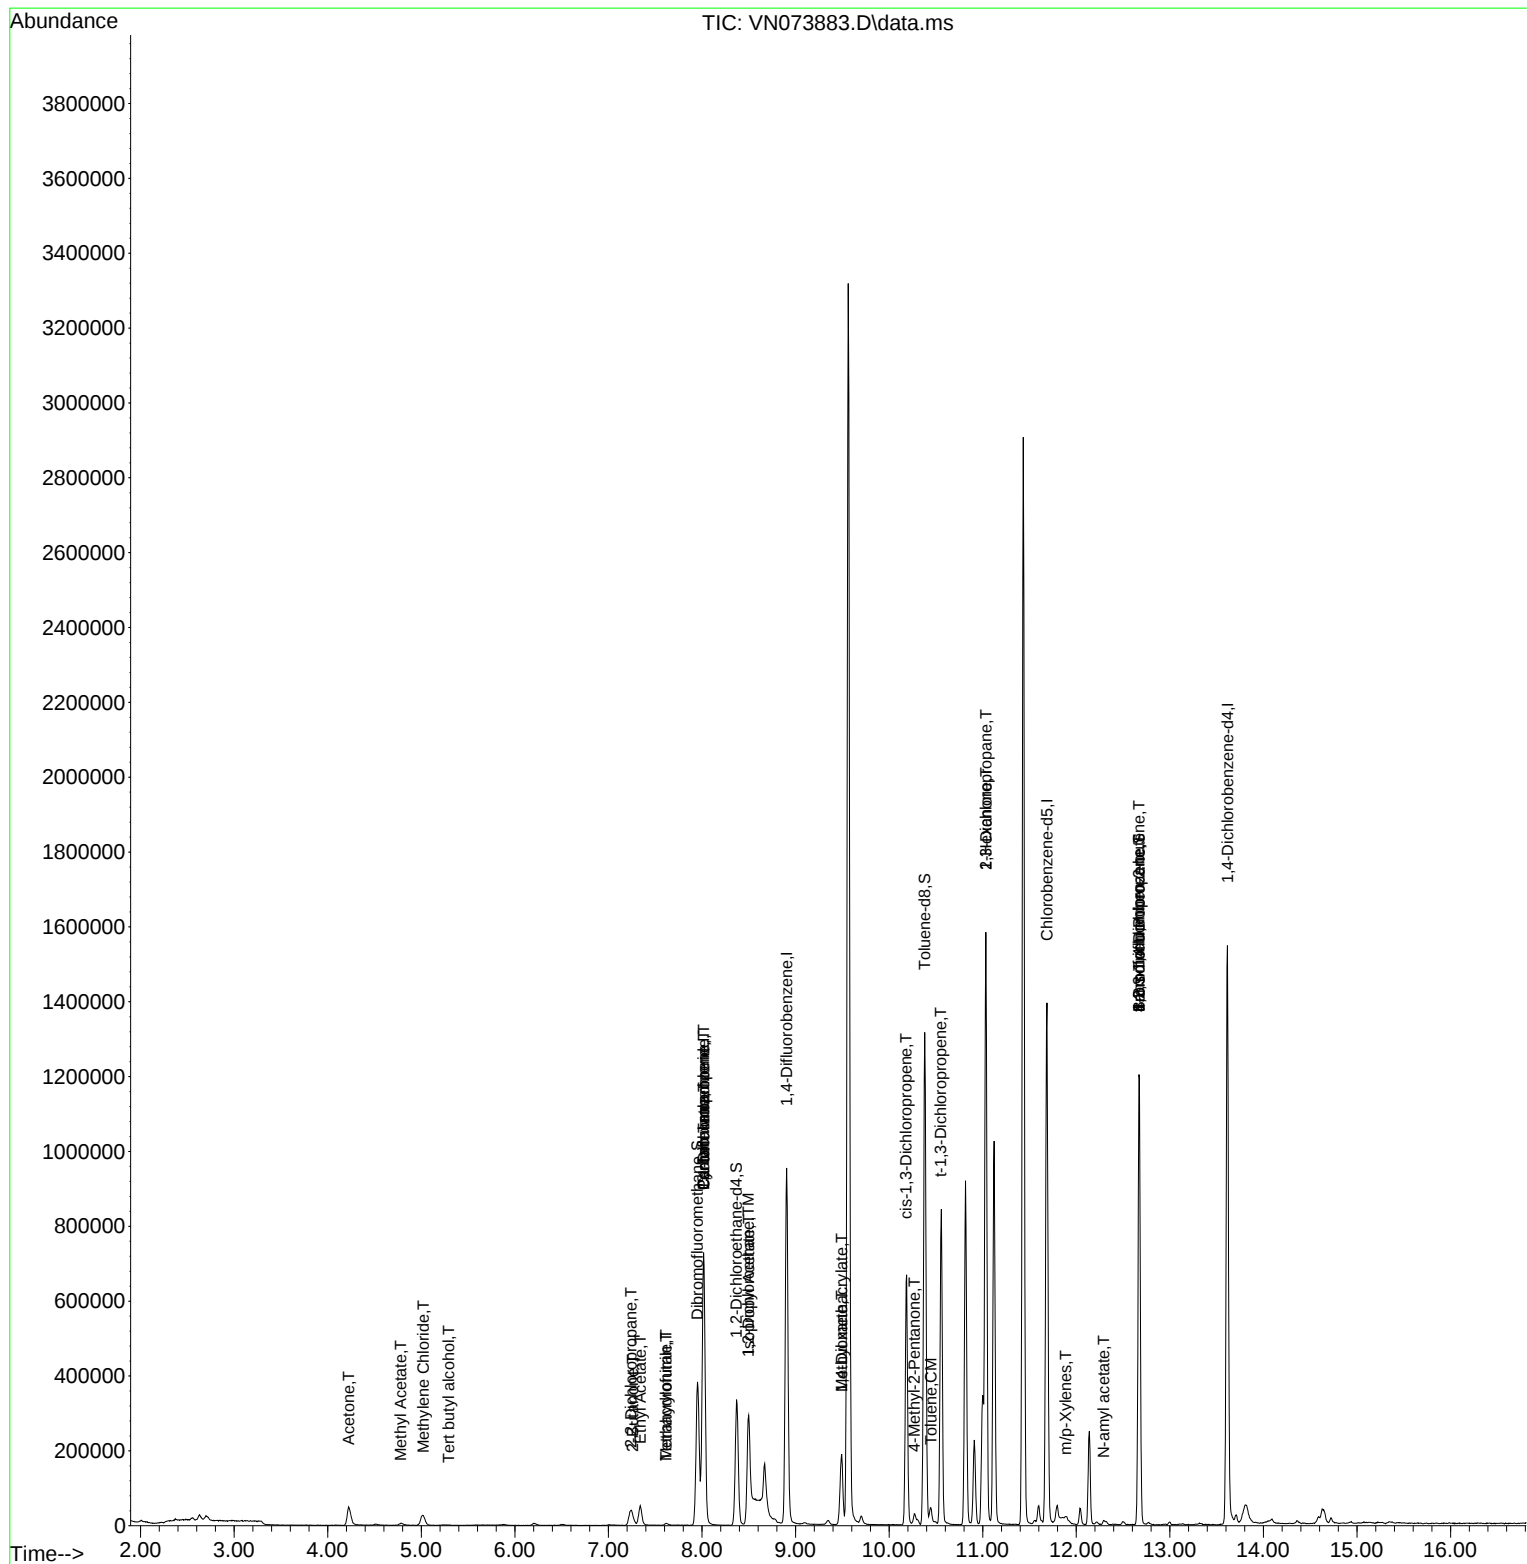




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion:168 Resp: 625585
Ion Ratio Lower Upper
168 100
99 46.0 42.3 63.5

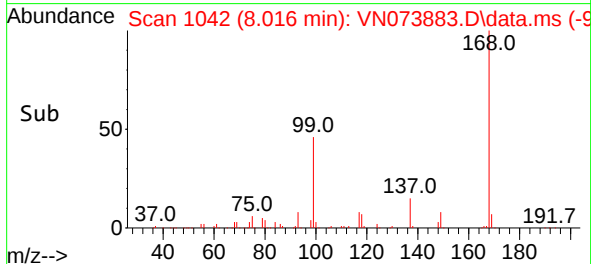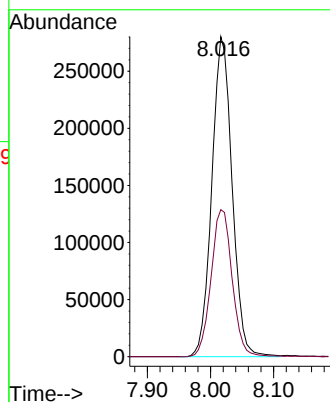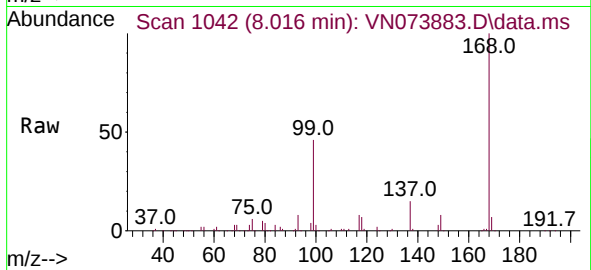

#3
Chloromethane
Concen: Below Cal
RT: 2.264 min Scan# 64
Delta R.T. -0.005 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 50 Resp: 928
Ion Ratio Lower Upper
50 100
52 29.0 25.7 38.5


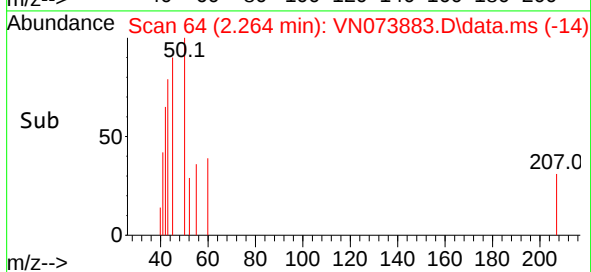
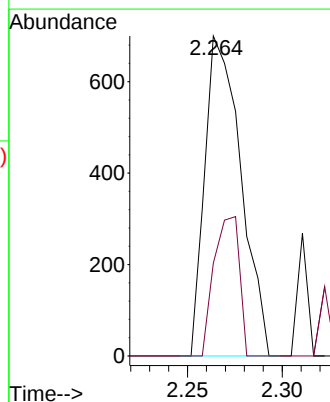
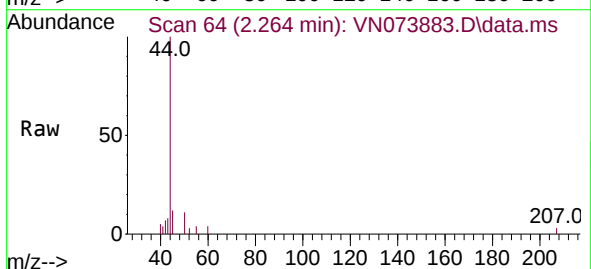


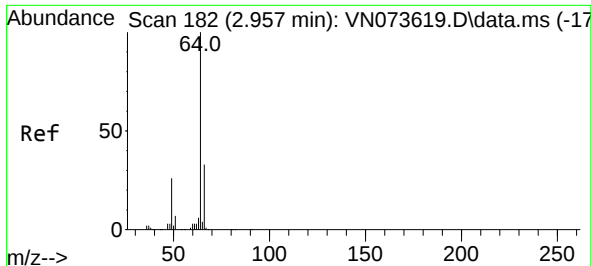

#6
Chloroethane
Concen: Below Cal
RT: 3.005 min Scan# 11
Delta R.T. 0.048 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 64 Resp: 55
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

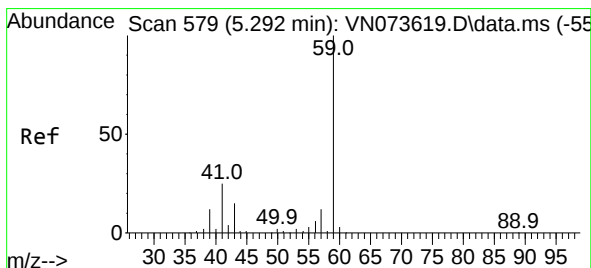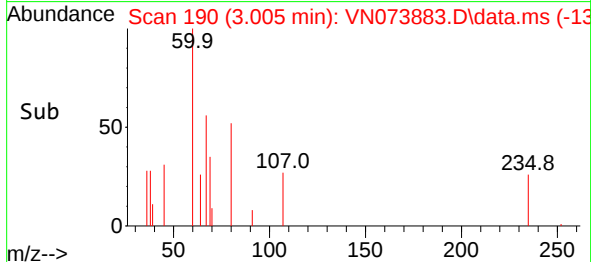

#11
Tert butyl alcohol
Concen: 0.535 ug/l
RT: 5.293 min Scan# 579
Delta R.T. 0.001 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 59 Resp: 879
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

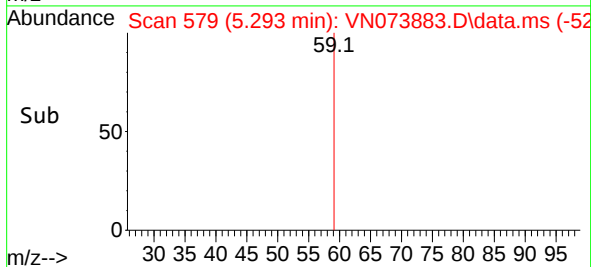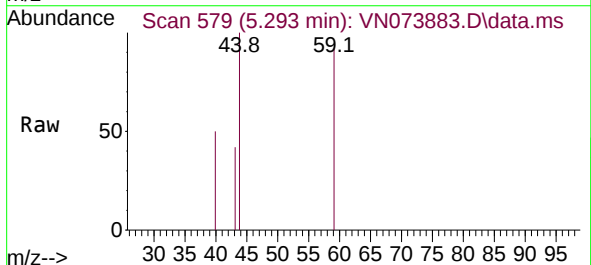

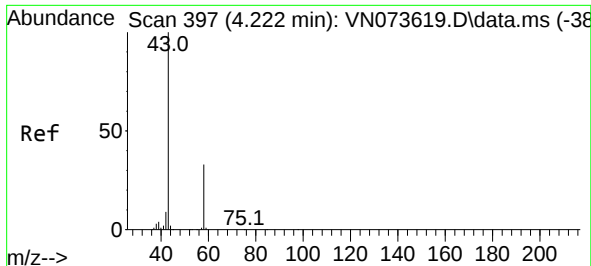

#16

Acetone

Concen: 21.906 ug/l

RT: 4.222 min Scan# 397

Delta R.T. 0.000 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20

Instrument :

MSVOA_N

ClientSampleId :





PB146976ZHE#09

Tgt Ion: 43 Resp: 89699

Ion Ratio Lower Upper

43 100

58 32.7 26.0 39.0

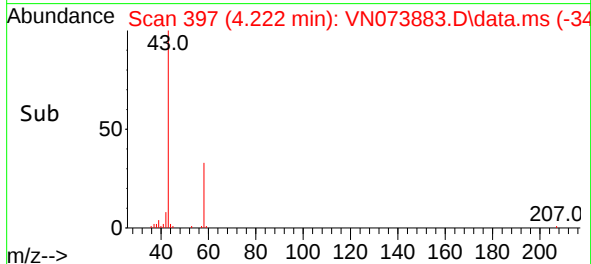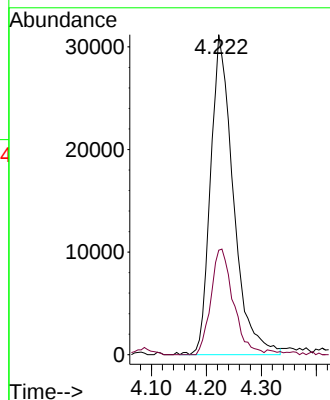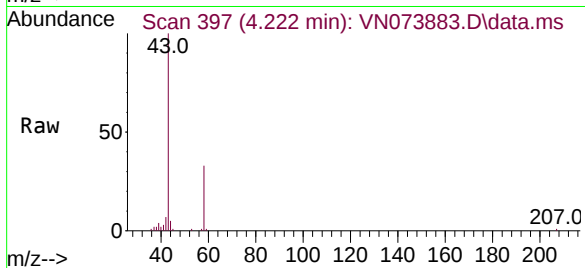

#18

Methyl Acetate

Concen: 1.080 ug/l

RT: 4.781 min Scan# 492

Delta R.T. 0.000 min

Lab File: VN073883.D




Acq: 13 Aug 2022 21:20


Tgt Ion: 43 Resp: 11001

Ion Ratio Lower Upper

43 100

74 25.2 21.6 32.4


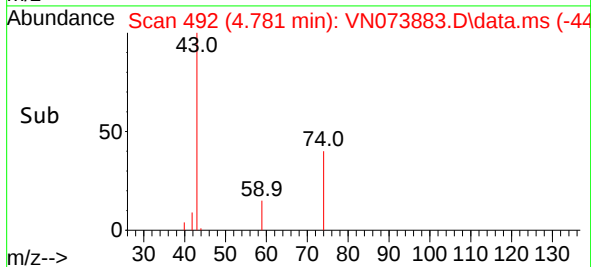
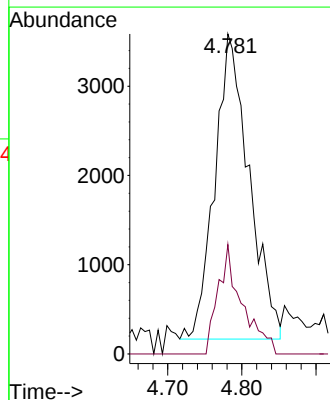
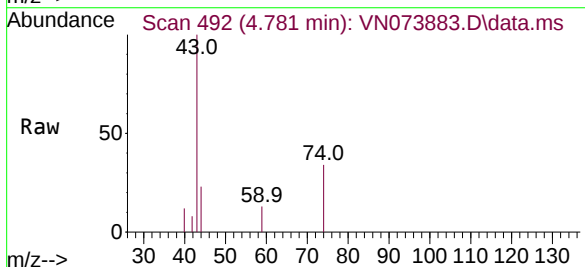


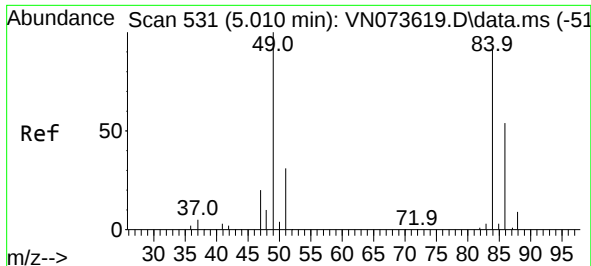

#20
Methylene Chloride
Concen: 1.614 ug/l
RT: 5.022 min Scan# 511
Delta R.T. 0.012 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion:	84	Resp:	24820
Ion	Ratio	Lower	Upper
84	100		
49	88.6	88.3	132.5
51	28.7	28.2	42.2
86	64.9	50.6	76.0

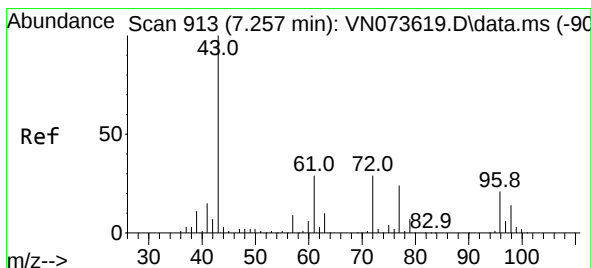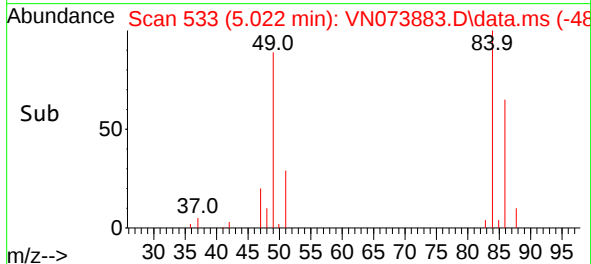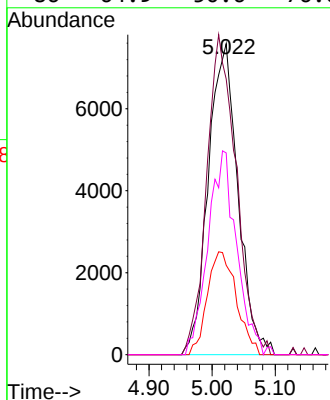

#25
2-Butanone
Concen: 3.068 ug/l
RT: 7.257 min Scan# 913
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion:	43	Resp:	19508
Ion	Ratio	Lower	Upper
43	100		
72	27.5	23.7	35.5


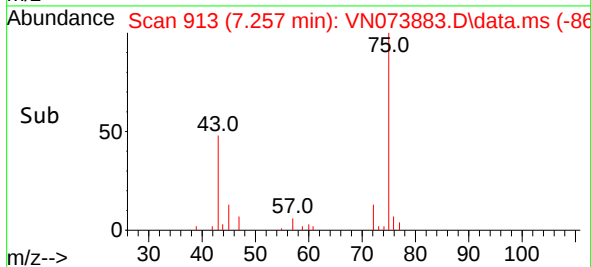
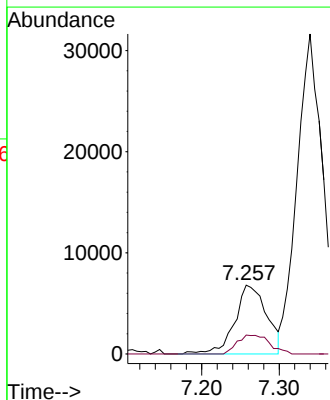
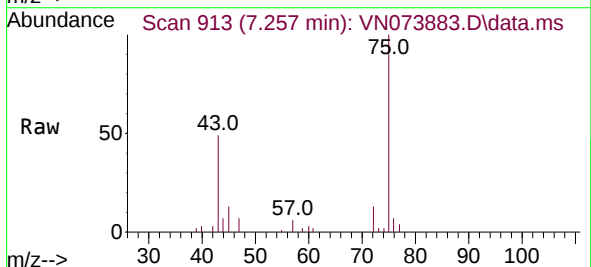


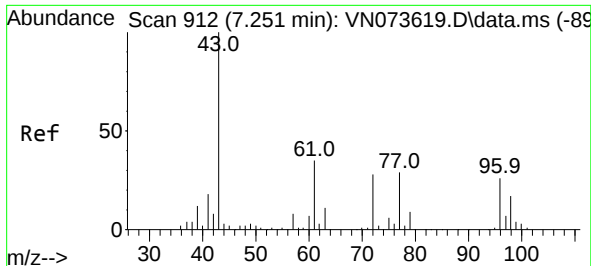

#26
2,2-Dichloropropane
Concen: 0.265 ug/l
RT: 7.240 min Scan# 912
Delta R.T. -0.011 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 77 Resp: 2572
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2#

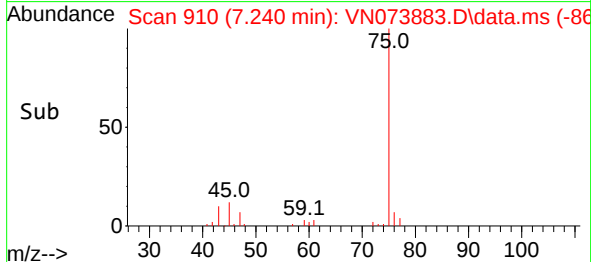

#29
Tetrahydrofuran
Concen: 1.019 ug/l
RT: 7.616 min Scan# 974
Delta R.T. 0.006 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 42 Resp: 4095
Ion Ratio Lower Upper
42 100
72 38.4 39.7 59.5#
71 43.0 36.6 55.0


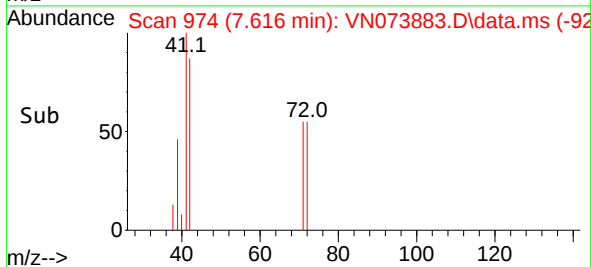

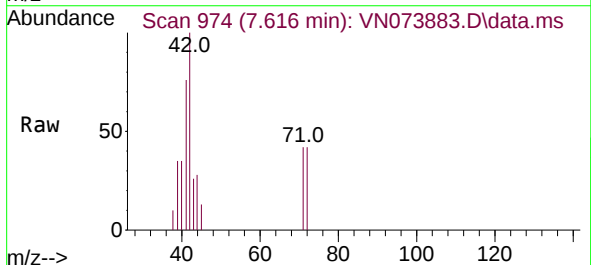


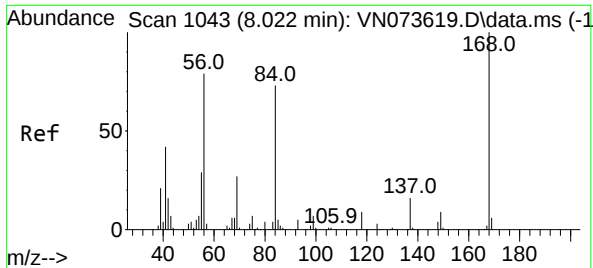

#31
Cyclohexane
Concen: 0.887 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 56 Resp: 10067
Ion Ratio Lower Upper
56 100
69 167.1 27.8 41.8#
84 183.2 76.9 115.3#

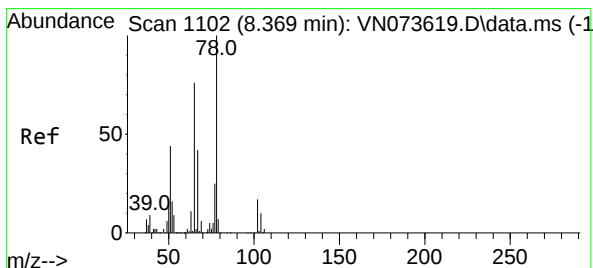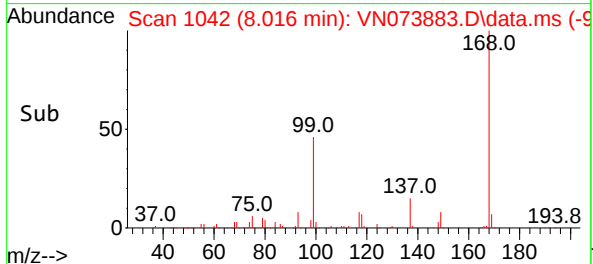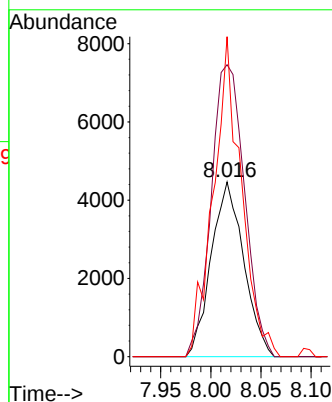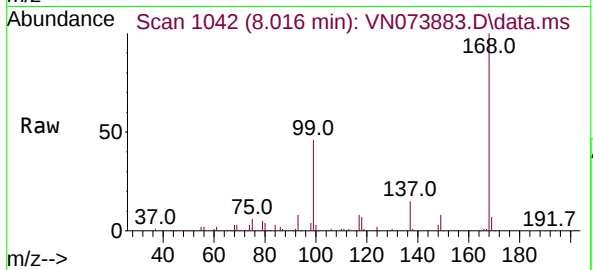

#33
1,2-Dichloroethane-d4
Concen: 36.901 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 65 Resp: 281325
Ion Ratio Lower Upper
65 100
67 51.7 0.0 104.8

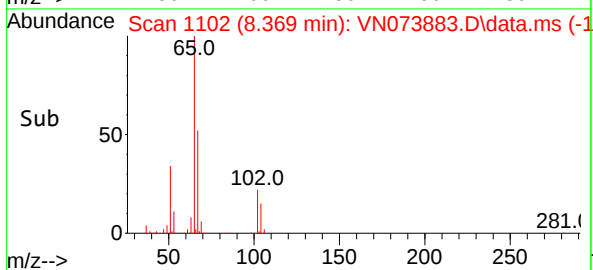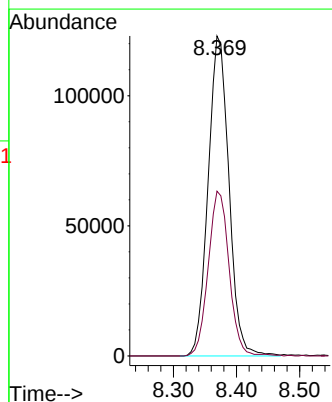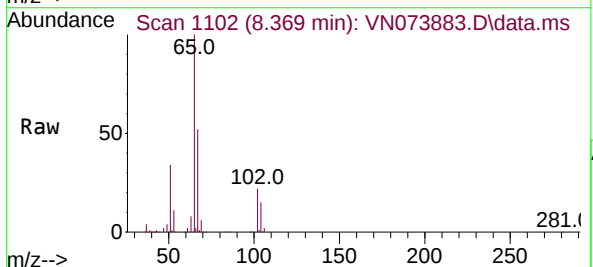

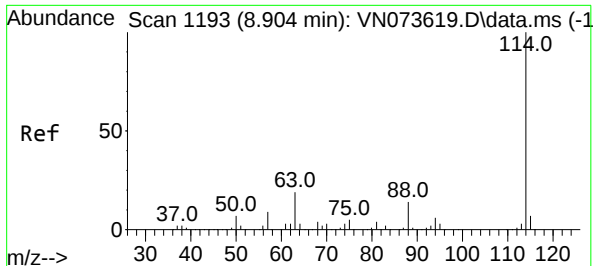

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#09





Tgt Ion:114 Resp: 902393

Ion Ratio Lower Upper

114 100

63 17.2 0.0 40.0

88 14.5 0.0 32.6

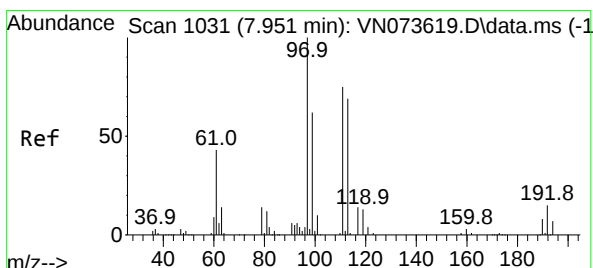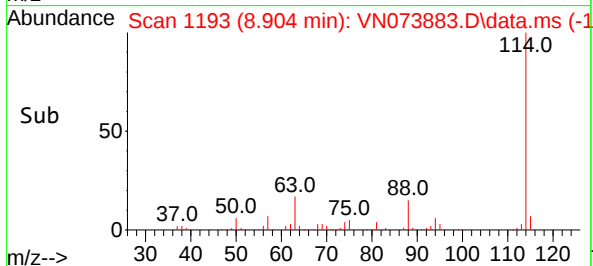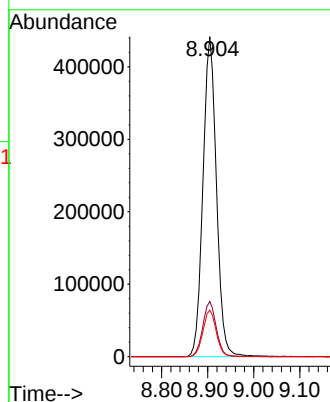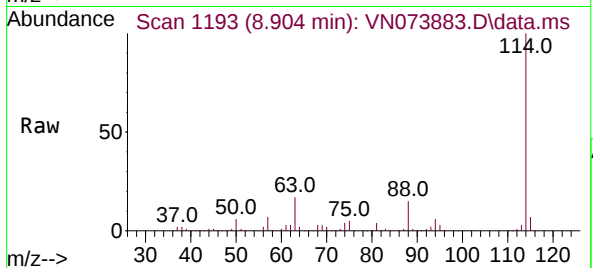

#35

Dibromofluoromethane

Concen: 49.511 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20




Tgt Ion:113 Resp: 280553


Ion Ratio Lower Upper

113 100

111 102.7 81.4 122.0

192 24.4 17.0 25.6

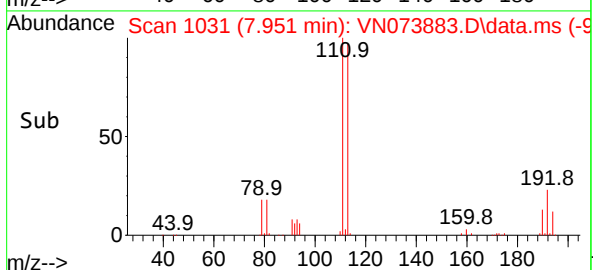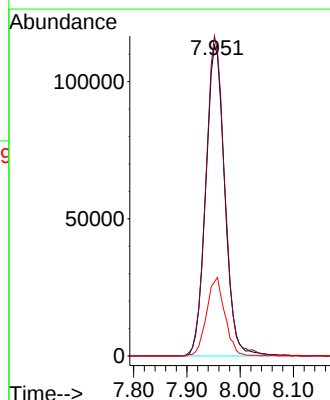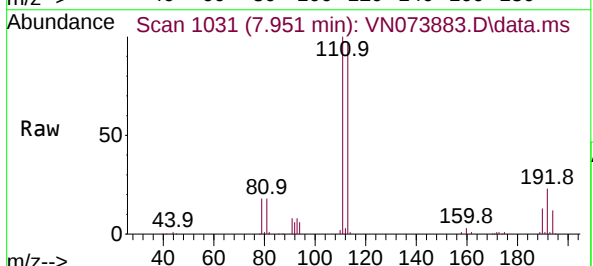

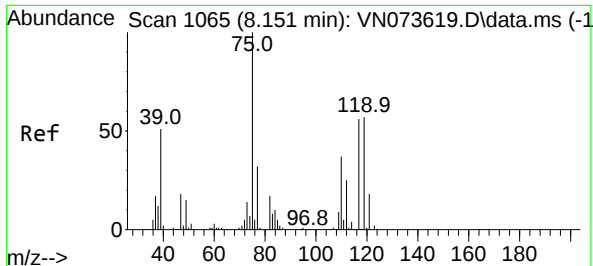

#36

1,1-Dichloropropene

Concen: 4.654 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20

Instrument :

MSVOA_N

ClientSampleId :

PB146976ZHE#09





Tgt Ion: 75 Resp: 37585

Ion Ratio Lower Upper

75 100

110 10.4 18.3 54.8#

77 0.0 25.1 37.7#

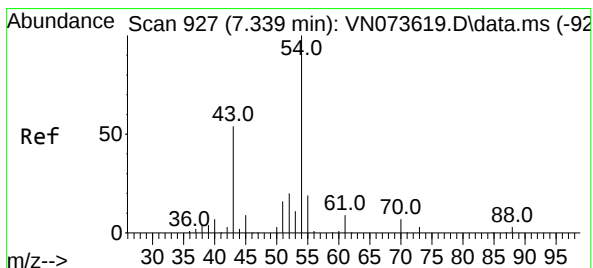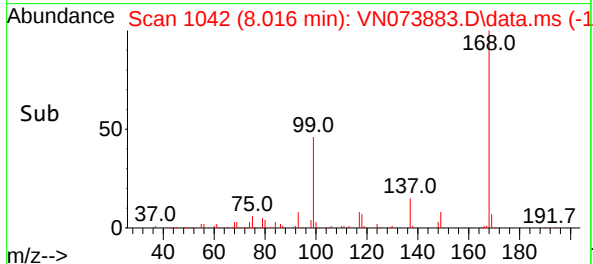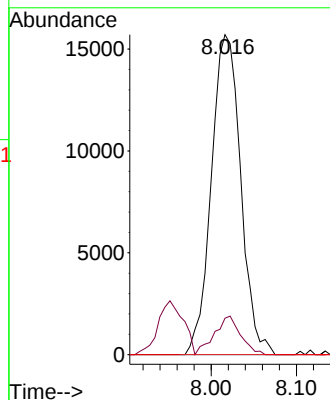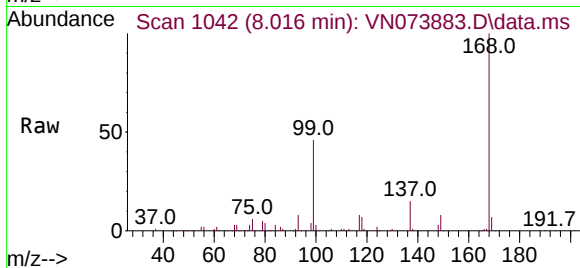

#37

Ethyl Acetate

Concen: 6.898 ug/l

RT: 7.340 min Scan# 927

Delta R.T. 0.000 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20




Tgt Ion: 43 Resp: 73367


Ion Ratio Lower Upper

43 100

61 16.1 11.8 17.6


70 13.0 9.3 13.9

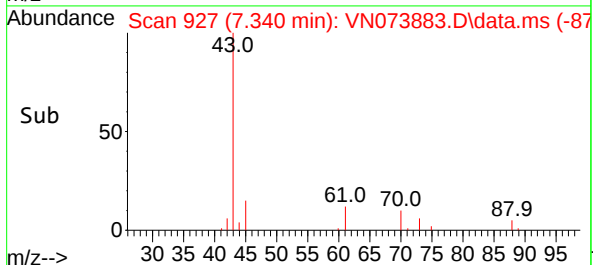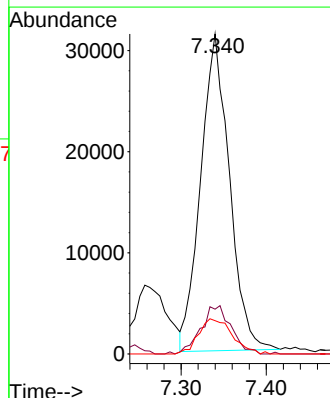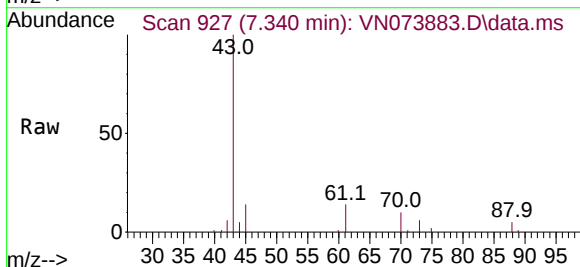



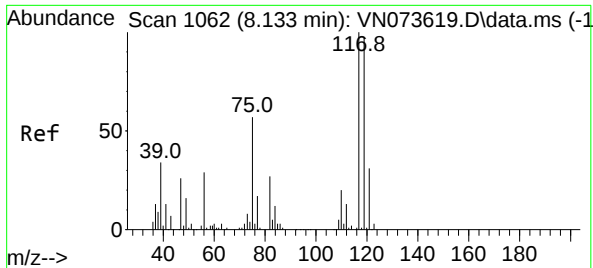


#38
Carbon Tetrachloride
Concen: 6.429 ug/l
RT: 8.016 min Scan# 117
Delta R.T. -0.117 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09



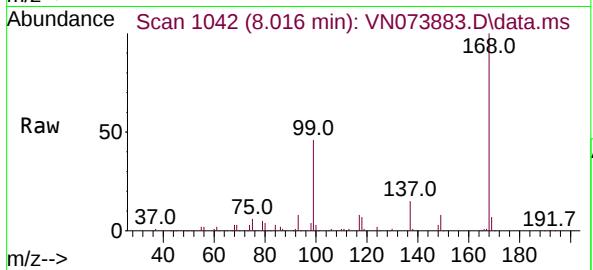



Tgt Ion:117 Resp: 52732
Ion Ratio Lower Upper
117 100
119 6.5 75.8 113.8#
121 0.0 24.6 37.0#

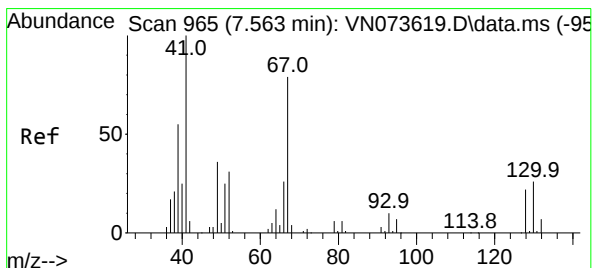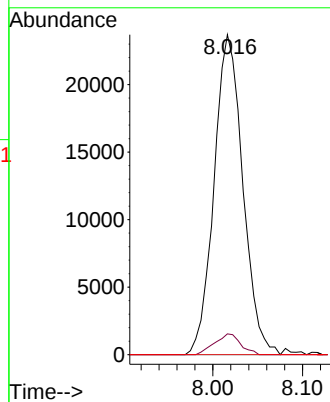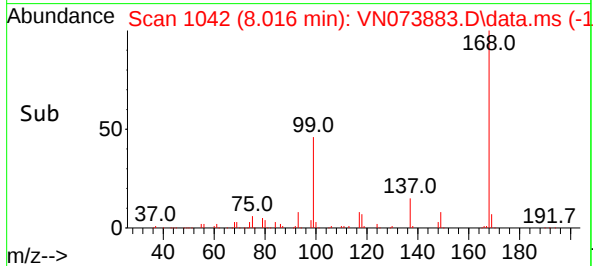

#41
Methacrylonitrile
Concen: 0.466 ug/l
RT: 7.616 min Scan# 974
Delta R.T. 0.053 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 41 Resp: 2242
Ion Ratio Lower Upper
41 100
39 57.0 48.6 73.0
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

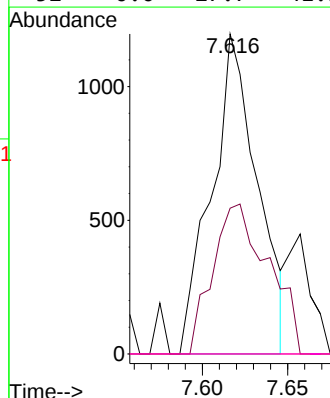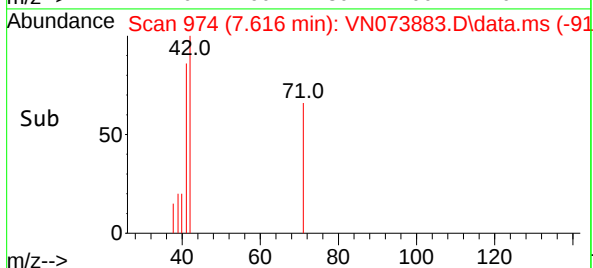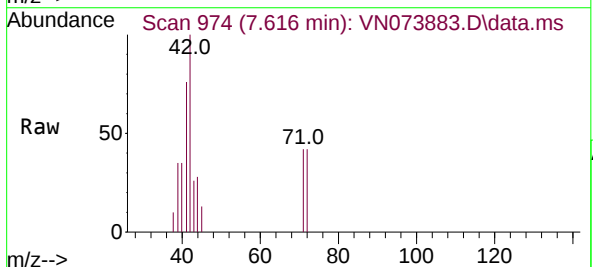

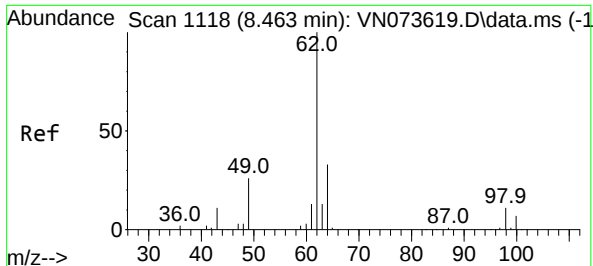

#42

1,2-Dichloroethane

Concen: 0.235 ug/l

RT: 8.493 min Scan# 1118

Delta R.T. 0.030 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20

Instrument :

MSVOA_N

ClientSampleId :





PB146976ZHE#09

Tgt Ion: 62 Resp: 2075

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.4

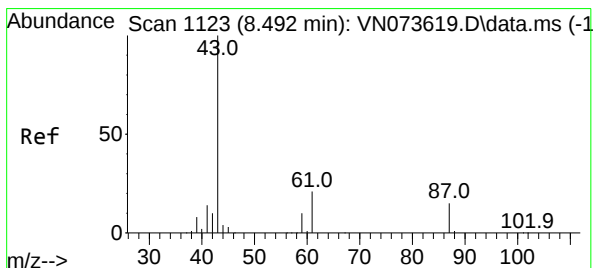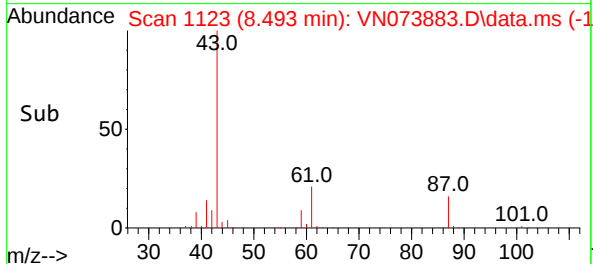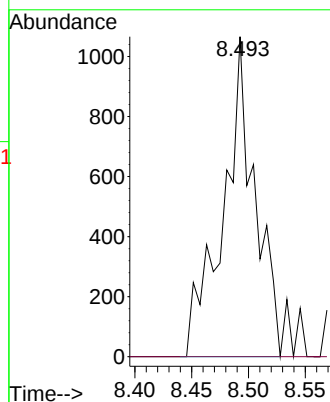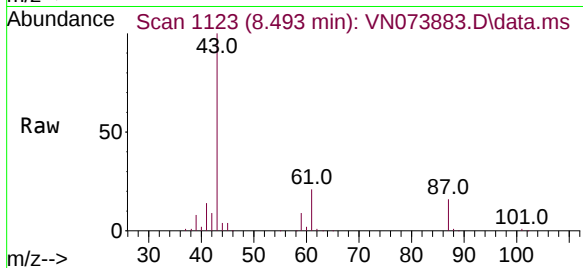

#43

Isopropyl Acetate

Concen: 27.430 ug/l

RT: 8.498 min Scan# 1124

Delta R.T. 0.006 min

Lab File: VN073883.D

Acq: 13 Aug 2022 21:20




Tgt Ion: 43 Resp: 394059


Ion Ratio Lower Upper

43 100

61 17.8 21.9 32.9#

87 13.5 12.0 18.0


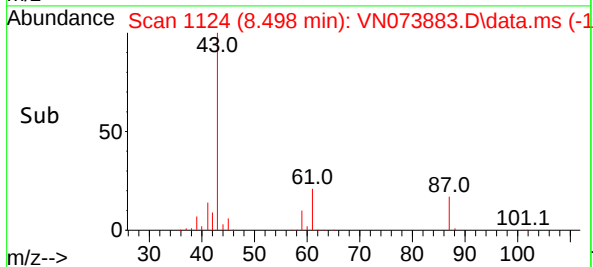
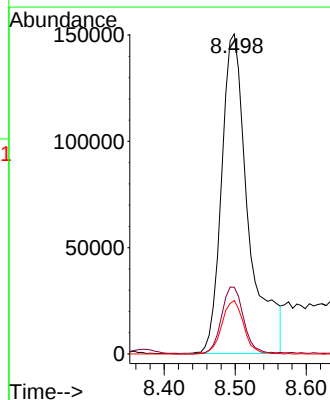
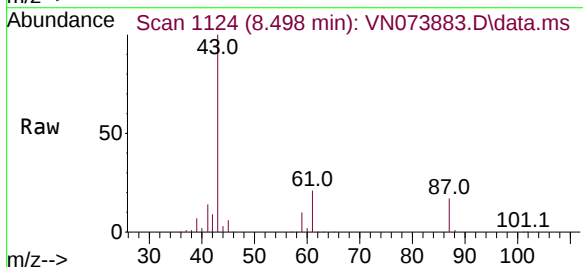


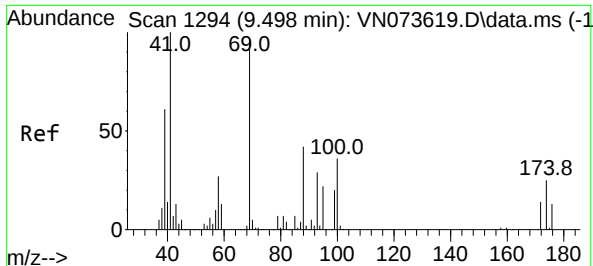

#48
Methyl methacrylate
Concen: 1.681 ug/l
RT: 9.493 min Scan# 1293
Delta R.T. -0.006 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 41 Resp: 10570
Ion Ratio Lower Upper
41 100
69 0.0 74.7 112.1#
39 59.8 45.6 68.4

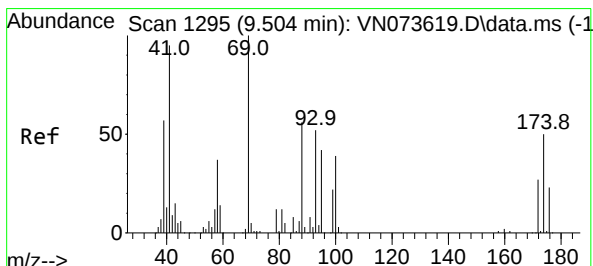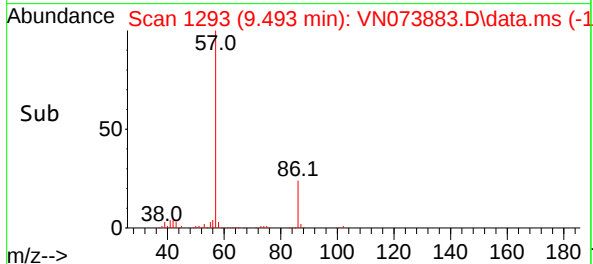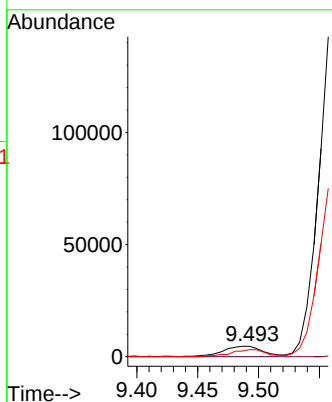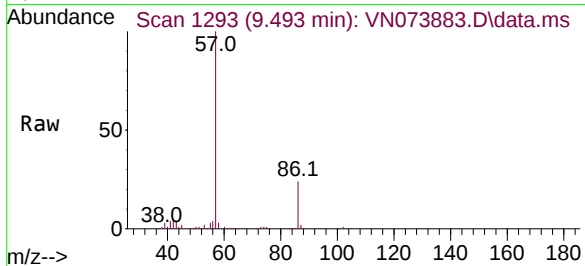

#49
1,4-Dioxane
Concen: 0.637 ug/l
RT: 9.493 min Scan# 1293
Delta R.T. -0.011 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 88 Resp: 113
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 7469.9 54.2 81.4#


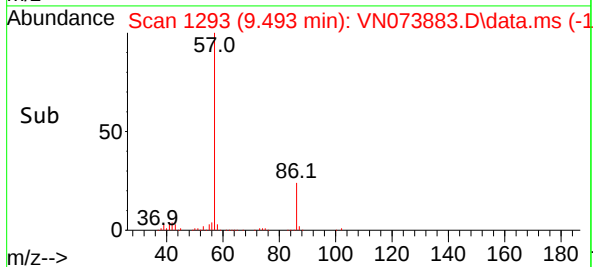

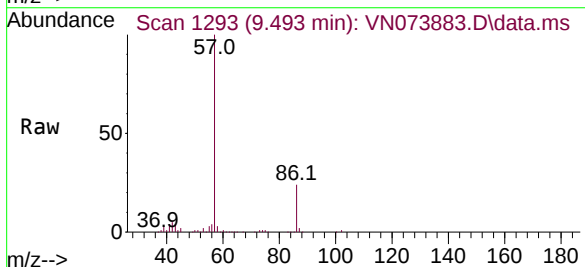


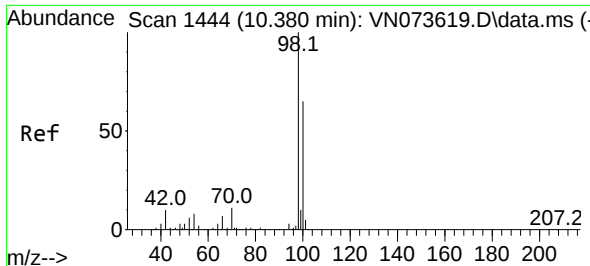

#50
Toluene-d8
Concen: 42.493 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 98 Resp: 947521
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8

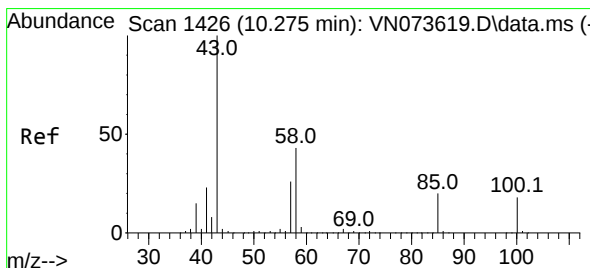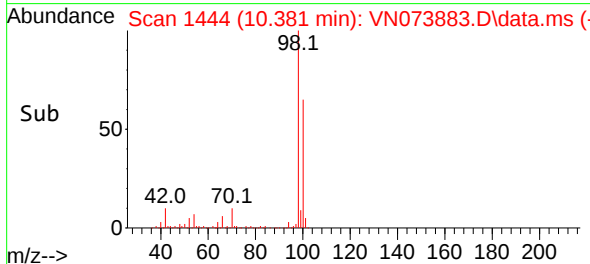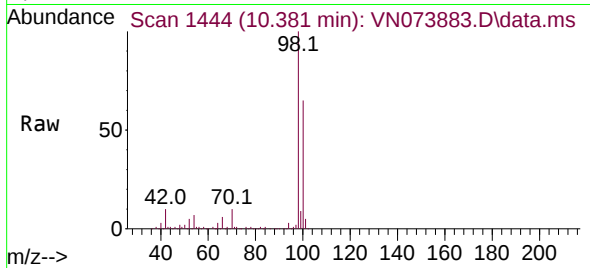

#51
4-Methyl-2-Pentanone
Concen: 2.657 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.006 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 43 Resp: 27377
Ion Ratio Lower Upper
43 100
58 29.6 34.1 51.1#


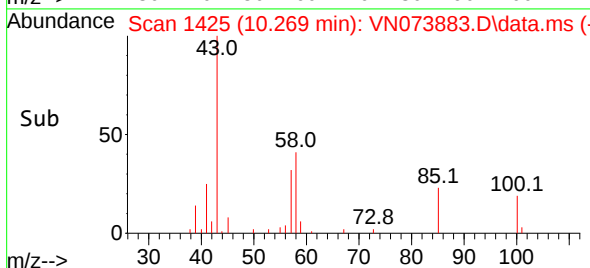

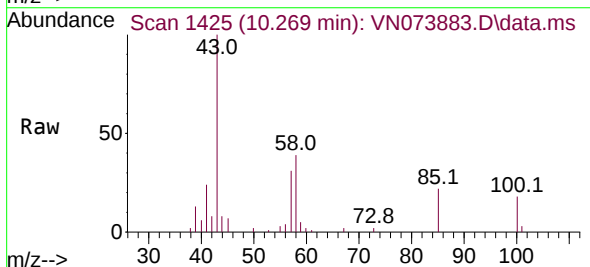


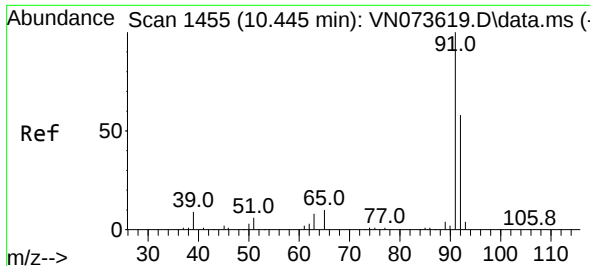

#52
Toluene
Concen: 1.150 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 92 Resp: 18416
Ion Ratio Lower Upper
92 100
91 179.8 138.6 207.8

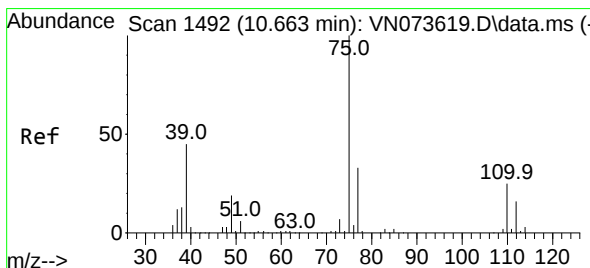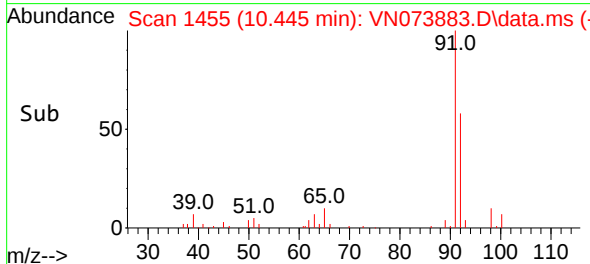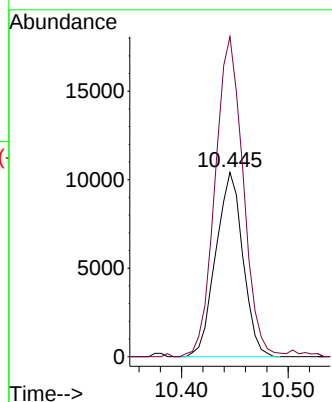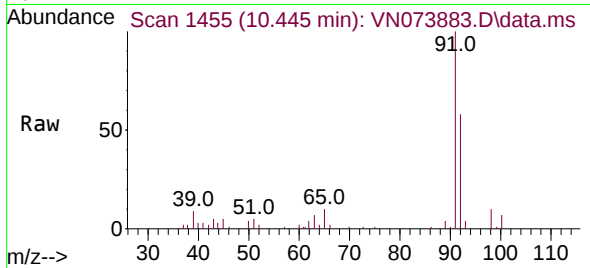

#53
t-1,3-Dichloropropene
Concen: 0.331 ug/l
RT: 10.551 min Scan# 1473
Delta R.T. -0.111 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 75 Resp: 2857
Ion Ratio Lower Upper
75 100
77 58.1 25.6 38.4#


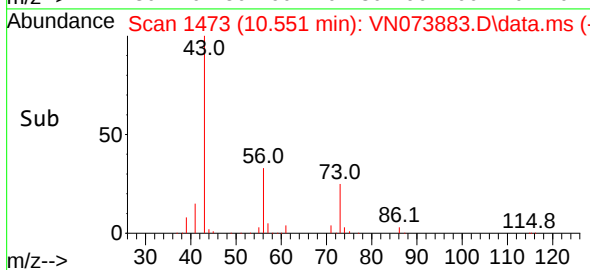
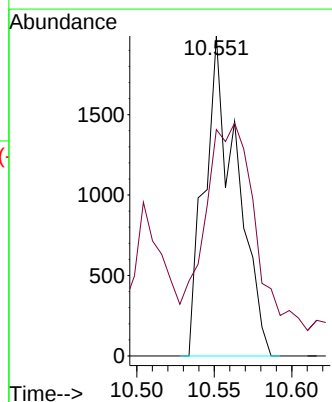
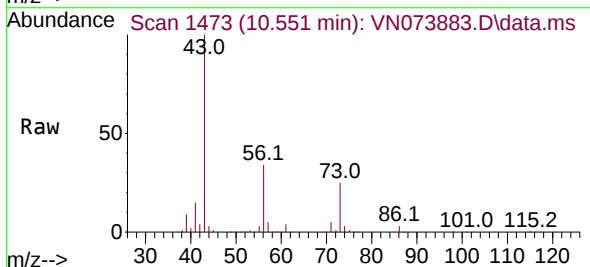


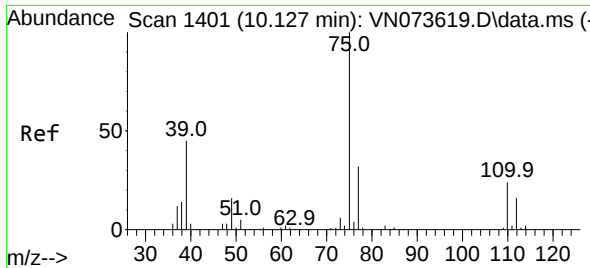

#54
 cis-1,3-Dichloropropene
 Concen: 13.493 ug/l
 RT: 10.181 min Scan# 1401
 Delta R.T. 0.053 min
 Lab File: VN073883.D
 Acq: 13 Aug 2022 21:20




Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#09


Tgt Ion: 75 Resp: 131161
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.2 37.8#
 39 26.2 35.7 53.5#

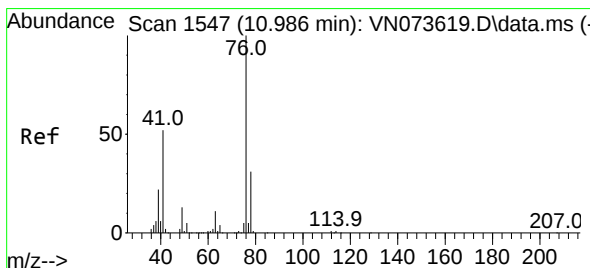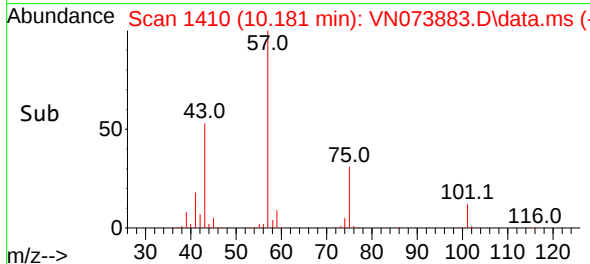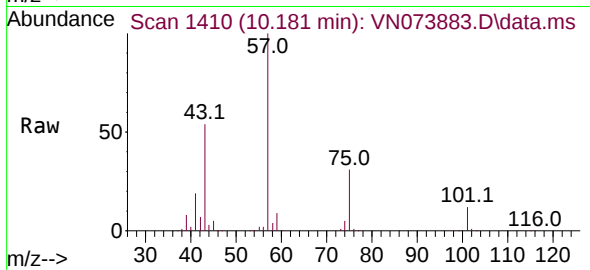

#57
 1,3-Dichloropropane
 Concen: 1.555 ug/l
 RT: 11.034 min Scan# 1555
 Delta R.T. 0.047 min
 Lab File: VN073883.D
 Acq: 13 Aug 2022 21:20

Tgt Ion: 76 Resp: 17625
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.2#


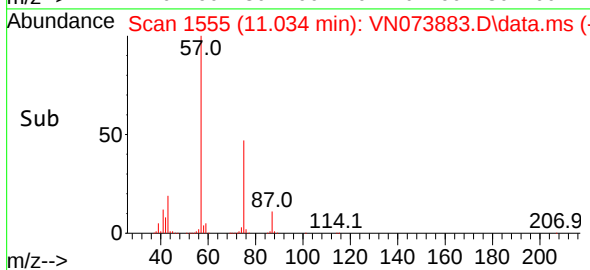

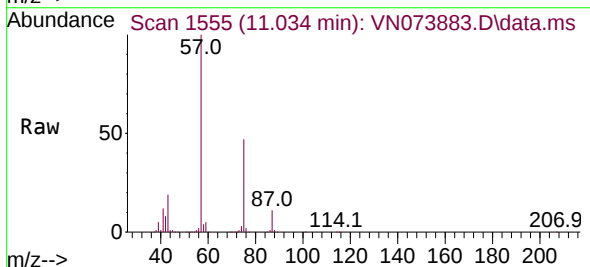


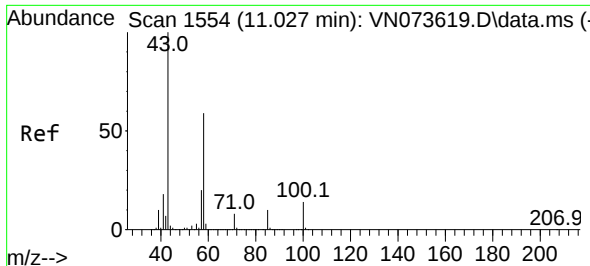

#59
2-Hexanone
Concen: 25.741 ug/l
RT: 11.034 min Scan# 11
Delta R.T. 0.007 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 43 Resp: 200947
Ion Ratio Lower Upper
43 100
58 21.4 29.7 89.1#

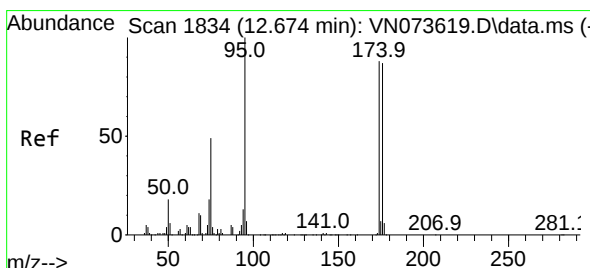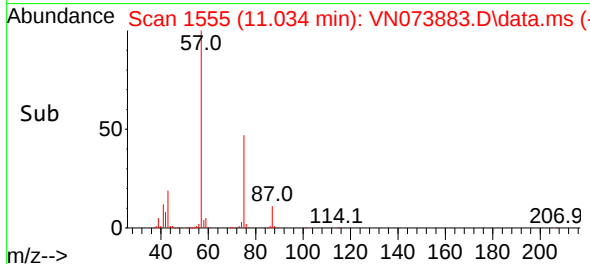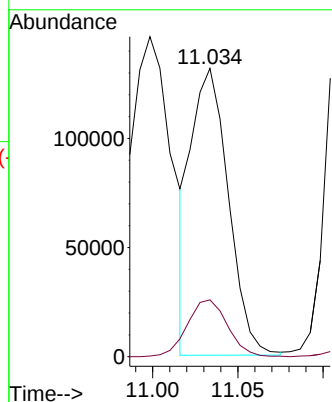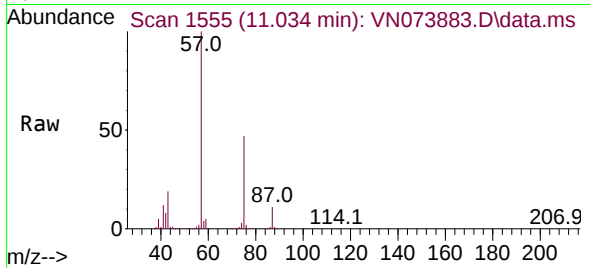

#62
4-Bromofluorobenzene
Concen: 49.384 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.005 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 95 Resp: 386281
Ion Ratio Lower Upper
95 100
174 99.8 0.0 167.6
176 95.1 0.0 163.4


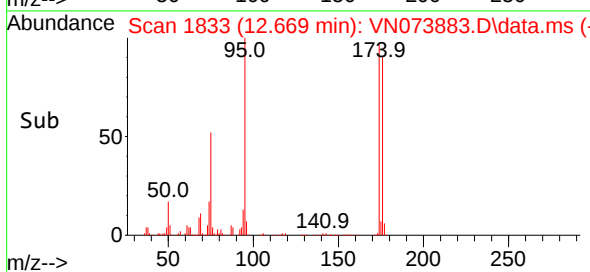
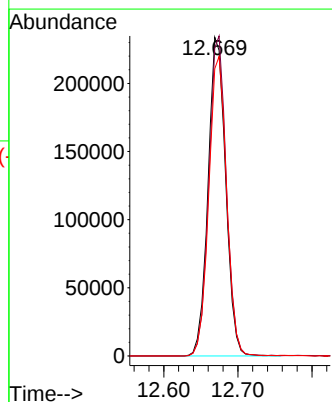
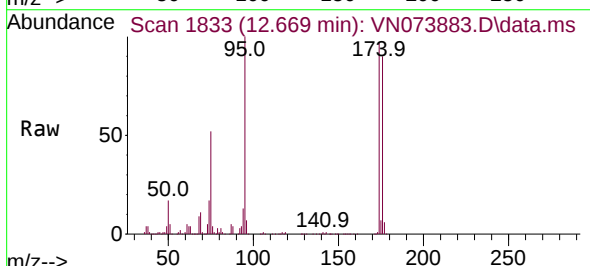




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.687 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion:117 Resp: 865298
Ion Ratio Lower Upper
117 100
82 49.6 44.2 66.2
119 32.5 25.4 38.0

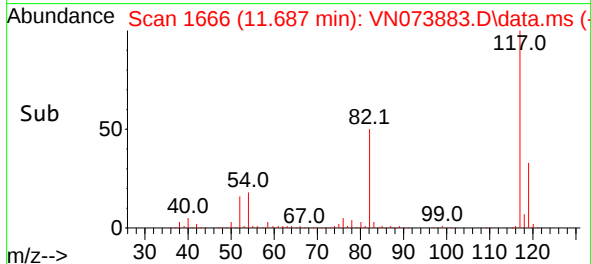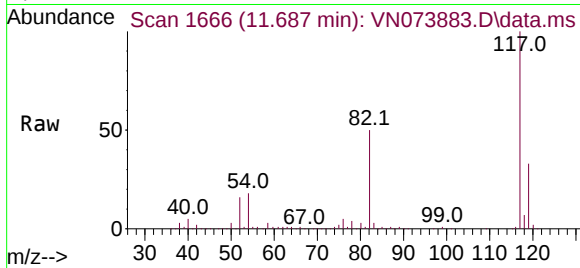

#68
m/p-Xylenes
Concen: 0.273 ug/l
RT: 11.887 min Scan# 1700
Delta R.T. -0.011 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion:106 Resp: 3224
Ion Ratio Lower Upper
106 100
91 200.9 158.9 238.3


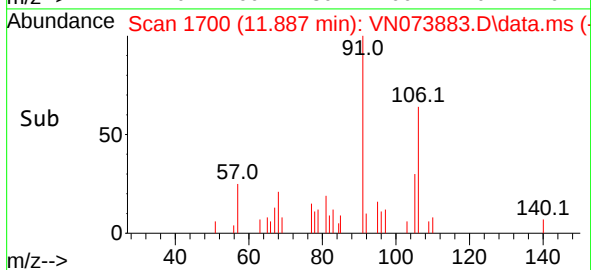

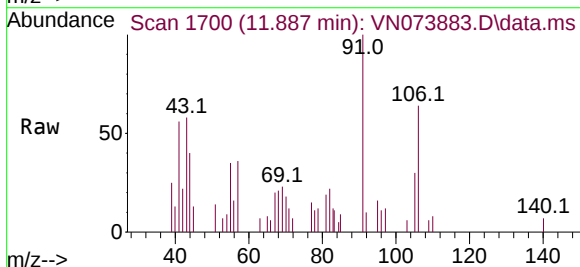


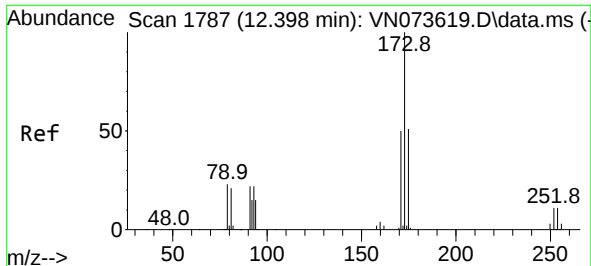

#71
Bromoform
Concen: 0.350 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.271 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion:173 Resp: 1902
Ion Ratio Lower Upper
173 100
175 0.0 24.6 73.6#
254 0.0 0.1 0.1#

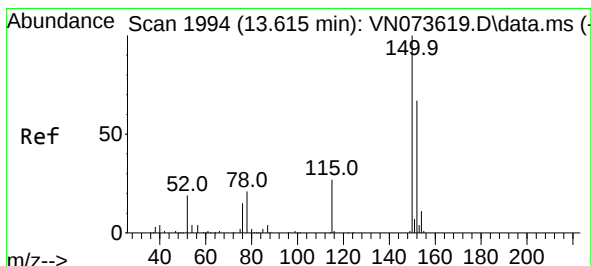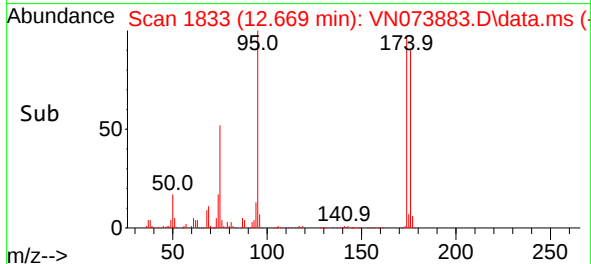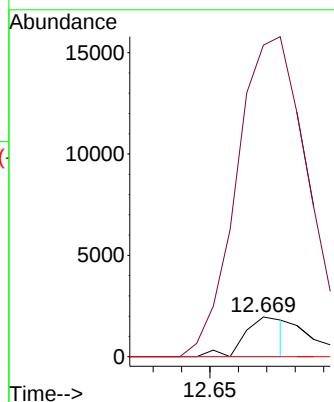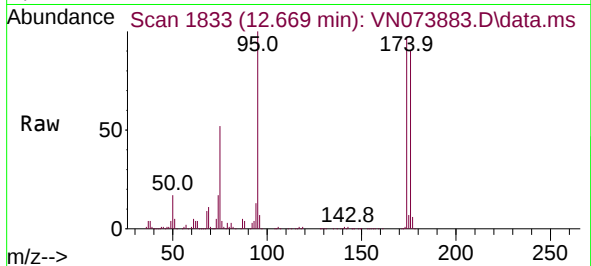

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion:152 Resp: 459074
Ion Ratio Lower Upper
152 100
115 52.7 28.9 86.7
150 155.5 0.0 356.2


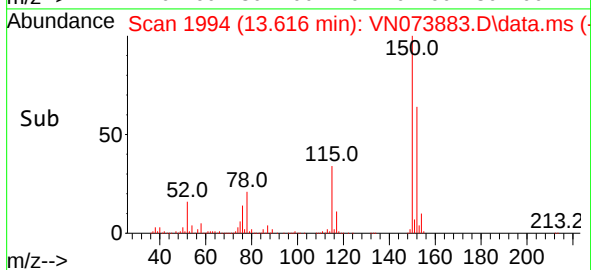
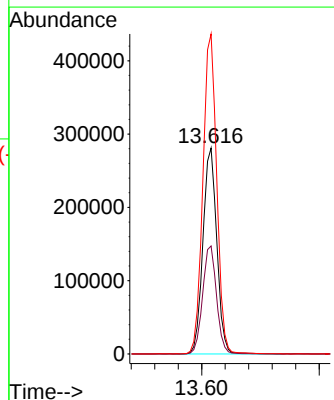
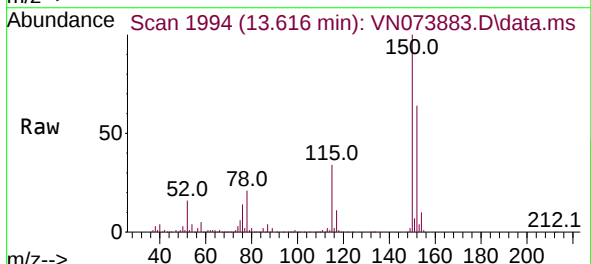


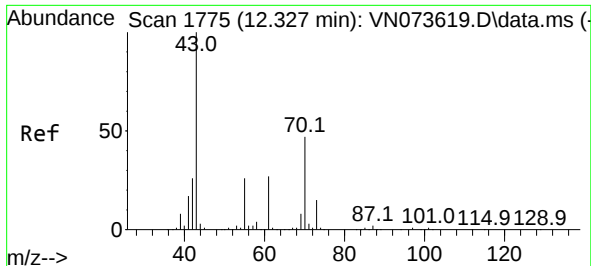

#74
N-amy1 acetate
Concen: 0.752 ug/l
RT: 12.292 min Scan# 1
Delta R.T. -0.035 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20




Instrument :
MSVOA_N
ClientSampleId :
PB146976ZHE#09


Tgt Ion: 43	Resp: 9542
Ion Ratio	Lower Upper
43	100
70	0.0 39.0 58.4#
55	7.3 21.1 31.7#
61	0.0 21.1 31.7#

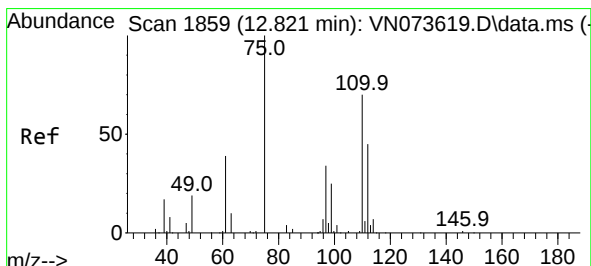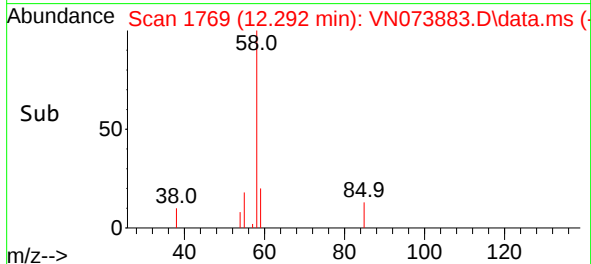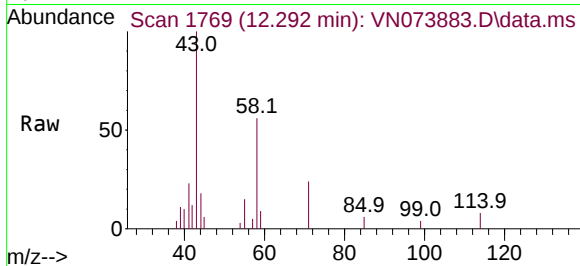

#76
1,2,3-Trichloropropane
Concen: 21.150 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.152 min
Lab File: VN073883.D
Acq: 13 Aug 2022 21:20

Tgt Ion: 75	Resp: 193516
Ion Ratio	Lower Upper
75	100
77	1.3 98.5 295.5#

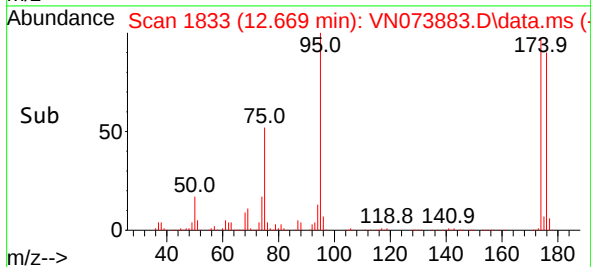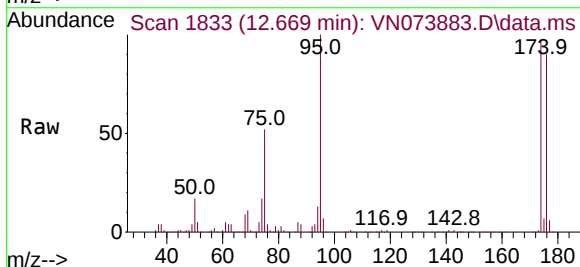

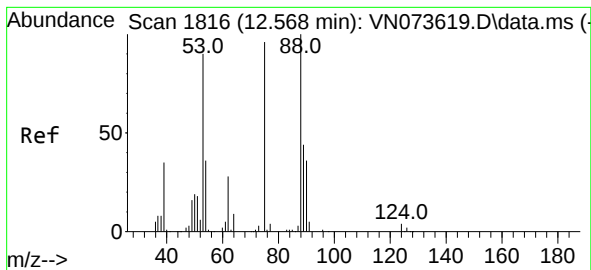

#81
 trans-1,4-Dichloro-2-butene
 Concen: 54.628 ug/l
 RT: 12.669 min Scan# 11
 Delta R.T. 0.100 min
 Lab File: VN073883.D
 Acq: 13 Aug 2022 21:20

Instrument :
 MSVOA_N
 ClientSampleId :
 PB146976ZHE#09

Tgt Ion: 75 Resp: 193516
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.0 117.0#
 89 0.0 37.2 55.8#

