

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081325\
 Data File : VN087531.D
 Acq On : 13 Aug 2025 13:45
 Operator : JC\MD
 Sample : Q2816-05DL 5X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 14 03:59:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 17 02:56:13 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.212	168	242235	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.088	114	538435	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	477328	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	224016	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	257078	62.546	ug/l	0.00
Spiked Amount 50.000	Range 74	- 125	Recovery	=	125.100%#	
35) Dibromofluoromethane	8.153	113	182278	49.077	ug/l	0.00
Spiked Amount 50.000	Range 75	- 124	Recovery	=	98.160%	
50) Toluene-d8	10.547	98	678568	51.218	ug/l	0.00
Spiked Amount 50.000	Range 86	- 113	Recovery	=	102.440%	
62) 4-Bromofluorobenzene	12.829	95	242040	49.449	ug/l	0.00
Spiked Amount 50.000	Range 77	- 121	Recovery	=	98.900%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.977	94	478	0.287	ug/l #	75
10) Methyl Iodide	4.589	142	498	5.807	ug/l #	78
11) Tert butyl alcohol	5.524	59	396	0.507	ug/l #	72
13) Acrolein	4.183	56	644	1.028	ug/l #	1
15) Acrylonitrile	5.730	53	612	0.289	ug/l #	52
16) Acetone	4.442	43	9349	4.851	ug/l #	89
17) Carbon Disulfide	4.700	76	3713	0.453	ug/l #	71
20) Methylene Chloride	5.248	84	459	Below Cal	#	76
21) trans-1,2-Dichloroethene	5.777	96	4652	1.492	ug/l #	84
25) 2-Butanone	7.483	43	1843	0.619	ug/l #	1
27) cis-1,2-Dichloroethene	7.477	96	47912	13.345	ug/l	95
29) Tetrahydrofuran	7.824	42	849	0.439	ug/l #	45
31) Cyclohexane	8.212	56	9017	1.784	ug/l #	27
36) 1,1-Dichloropropene	8.206	75	24925	5.079	ug/l #	44
38) Carbon Tetrachloride	8.206	117	28463	5.266	ug/l #	15
44) Trichloroethene	9.335	130	85704	22.870	ug/l	87
51) 4-Methyl-2-Pentanone	10.430	43	1754	0.252	ug/l #	37
55) 1,1,2-Trichloroethane	11.071	97	1039	0.266	ug/l #	72
59) 2-Hexanone	11.053	43	1175	0.255	ug/l	83
60) Dibromochloromethane	11.082	129	97179	21.834	ug/l #	10
64) Tetrachloroethene	11.082	164	96136	31.293	ug/l	96
76) 1,2,3-Trichloropropane	12.829	75	142222	28.312	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.829	75	142222	77.466	ug/l #	8
87) 1,3-Dichlorobenzene	13.718	146	1436	0.200	ug/l #	79
88) 1,4-Dichlorobenzene	13.794	146	2097	0.274	ug/l #	1
89) n-Butylbenzene	14.029	91	3468	0.300	ug/l #	88
93) 1,2,4-Trichlorobenzene	15.365	180	1586	0.397	ug/l #	74
94) Hexachlorobutadiene	15.476	225	759	0.511	ug/l	95
95) Naphthalene	15.623	128	4997	0.353	ug/l #	73
96) 1,2,3-Trichlorobenzene	15.806	180	1482	0.370	ug/l	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081325\
Data File : VN087531.D
Acq On : 13 Aug 2025 13:45
Operator : JC\MD
Sample : Q2816-05DL 5X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 14 03:59:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 17 02:56:13 2025
Response via : Initial Calibration




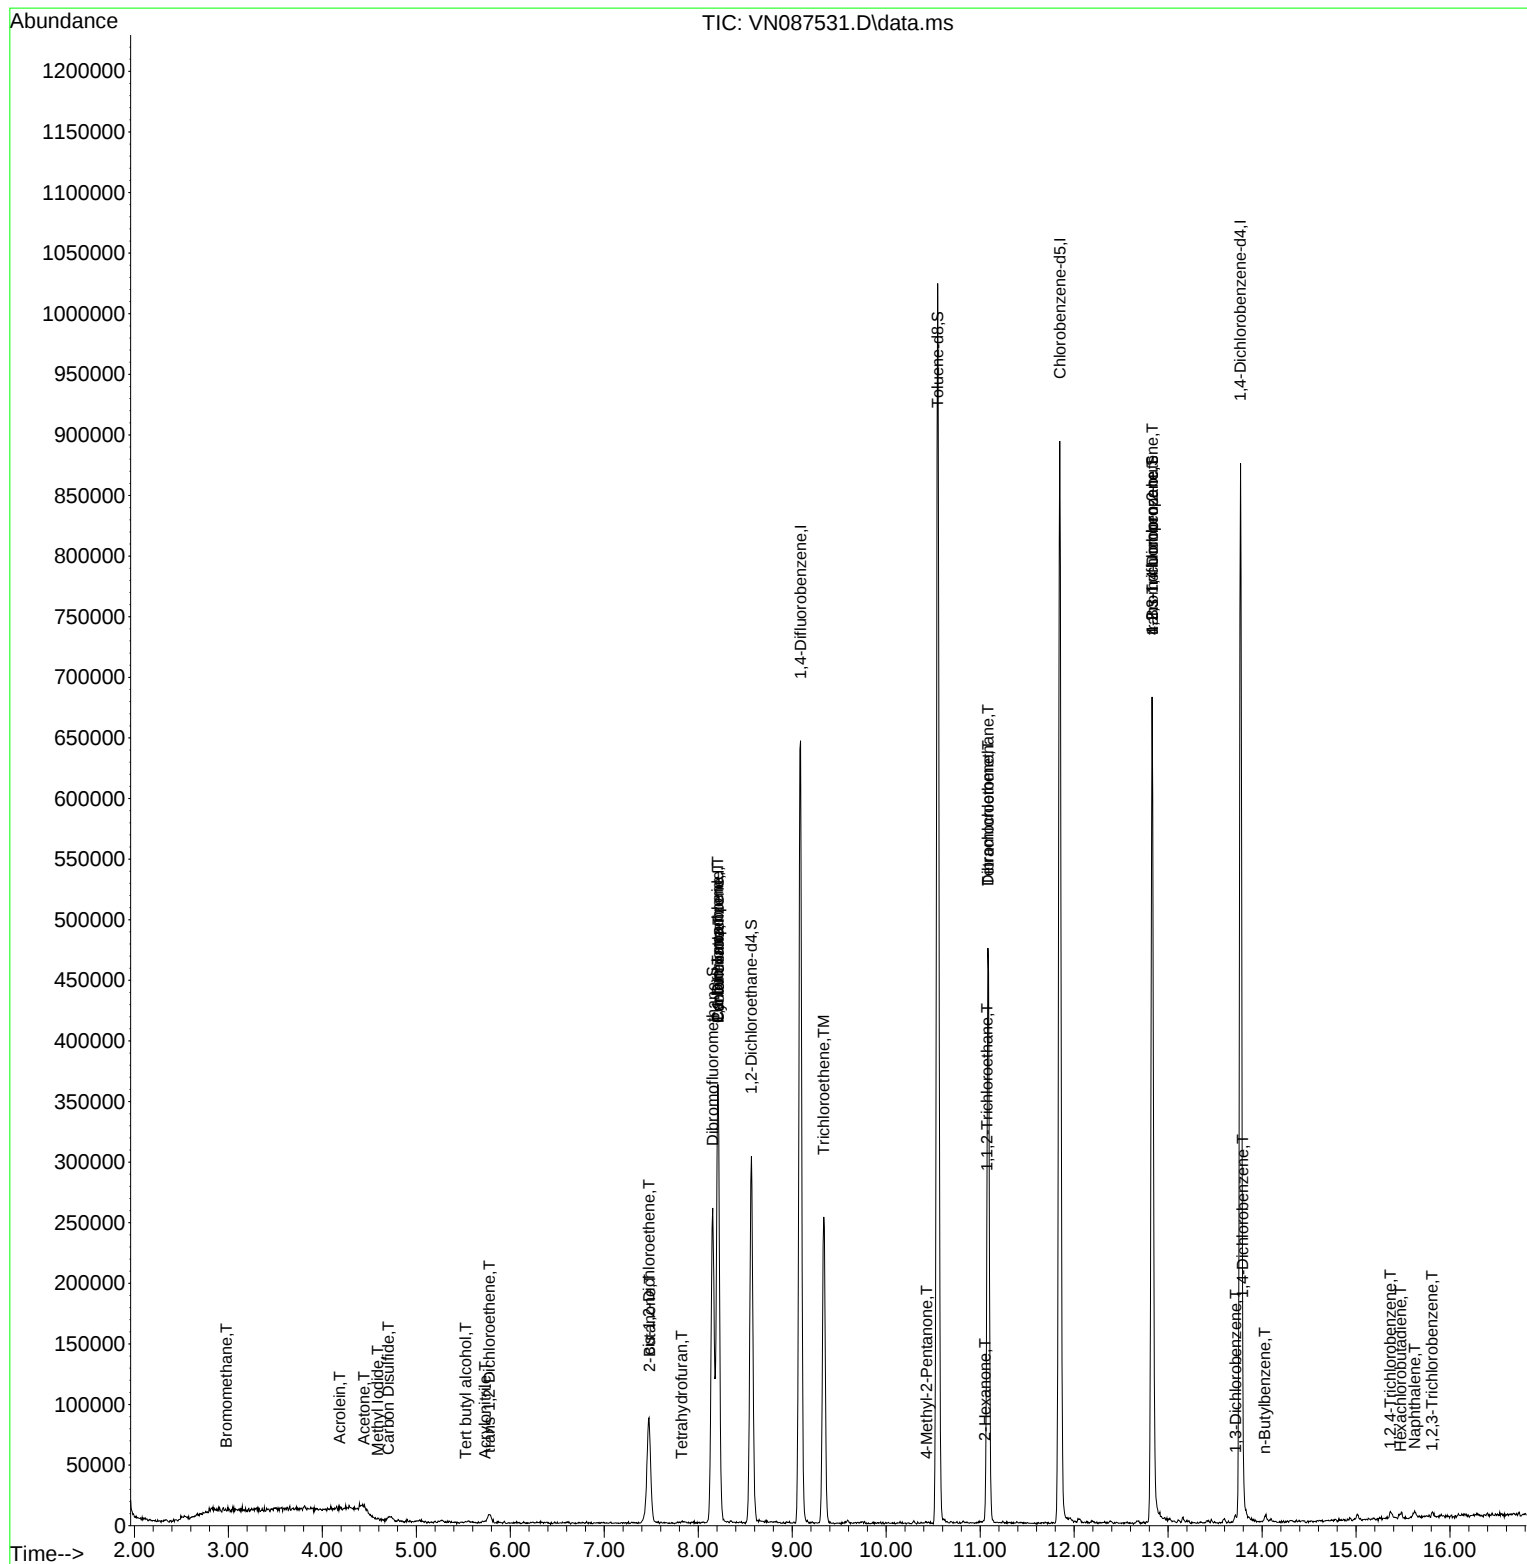


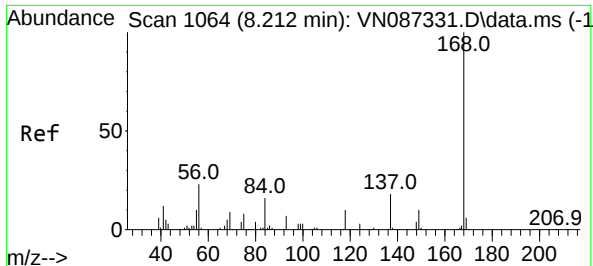

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. 0.000 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 242235
Ion Ratio Lower Upper
168 100
99 69.6 47.9 71.9

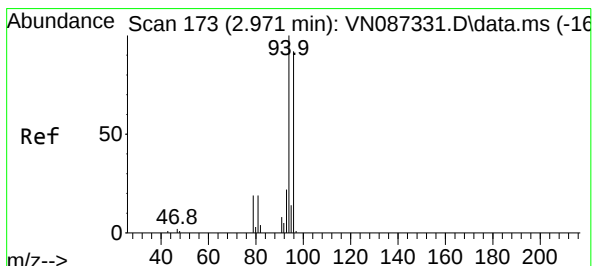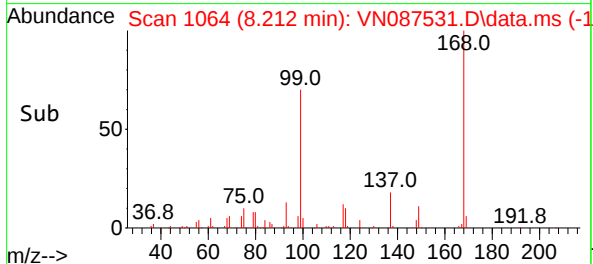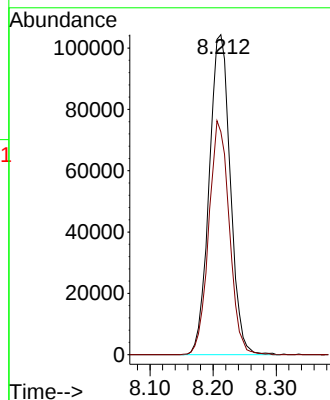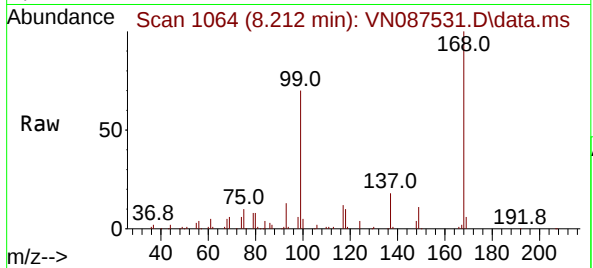

#5
Bromomethane
Concen: 0.287 ug/l
RT: 2.977 min Scan# 174
Delta R.T. 0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45


Tgt Ion: 94 Resp: 478
Ion Ratio Lower Upper
94 100
96 68.2 73.4 110.2#

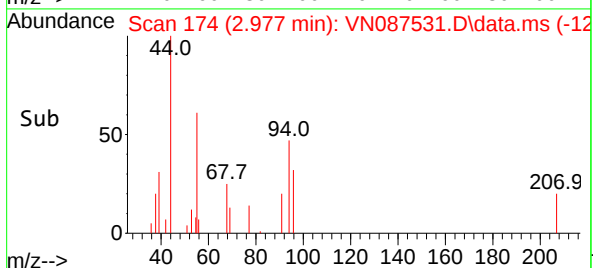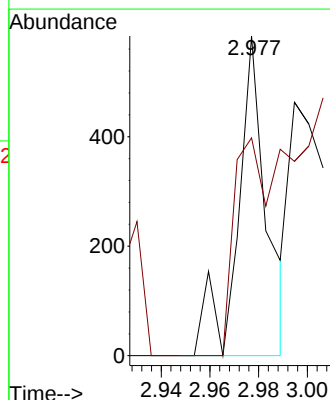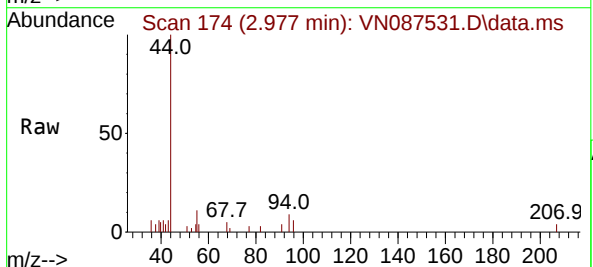






#10
Methyl Iodide
Concen: 5.807 ug/l
RT: 4.589 min Scan# 446
Delta R.T. 0.012 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:142 Resp: 498
Ion Ratio Lower Upper
142 100
127 56.5 35.7 53.5#
141 0.0 10.4 15.6#

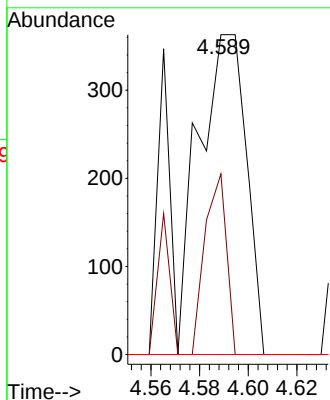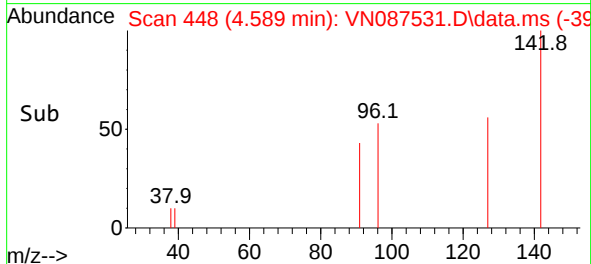

#11
Tert butyl alcohol
Concen: 0.507 ug/l
RT: 5.524 min Scan# 607
Delta R.T. 0.000 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45


Tgt Ion: 59 Resp: 396
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

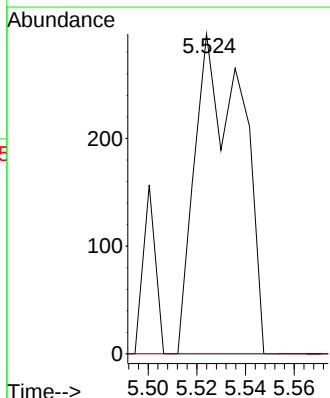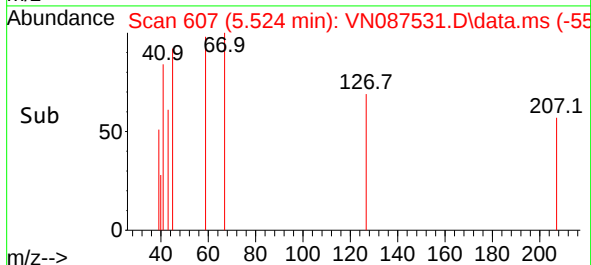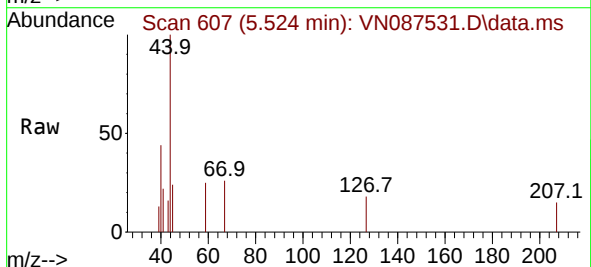






#13
Acrolein
Concen: 1.028 ug/l
RT: 4.183 min Scan# 31
Delta R.T. 0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 644
Ion Ratio Lower Upper
56 100
55 260.1 56.2 84.4#

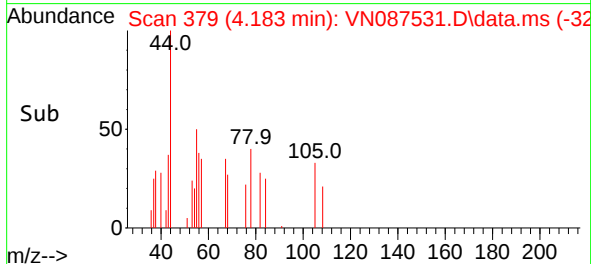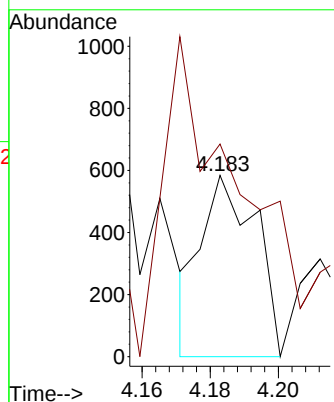

#15
Acrylonitrile
Concen: 0.289 ug/l
RT: 5.730 min Scan# 642
Delta R.T. 0.018 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Tgt Ion: 53 Resp: 612
Ion Ratio Lower Upper
53 100
52 44.1 65.5 98.3#
51 0.0 28.7 43.1#


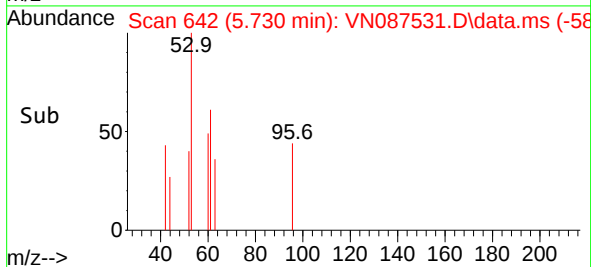
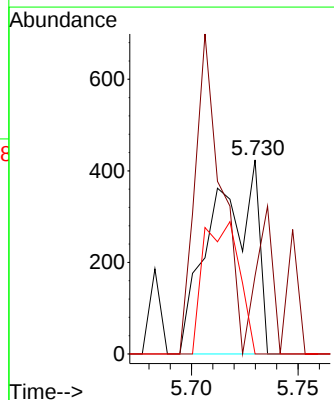
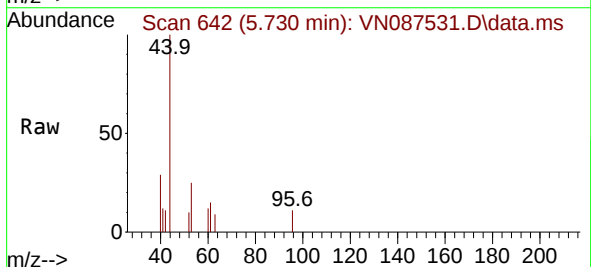




#16
Acetone
Concen: 4.851 ug/l
RT: 4.442 min Scan# 41
Delta R.T. 0.018 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 9349
Ion Ratio Lower Upper
43 100
58 22.0 22.3 33.5#

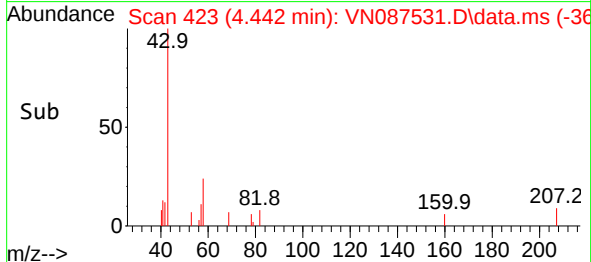

#17
Carbon Disulfide
Concen: 0.453 ug/l
RT: 4.700 min Scan# 467
Delta R.T. 0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45


Tgt Ion: 76 Resp: 3713
Ion Ratio Lower Upper
76 100
78 0.0 8.6 13.0#

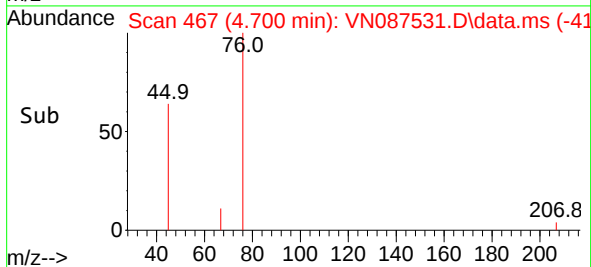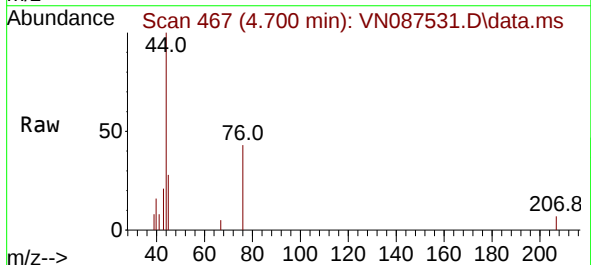






#20
Methylene Chloride
Concen: Below Cal
RT: 5.248 min Scan# 51
Delta R.T. -0.011 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	84	Resp:	459
Ion	Ratio	Lower	Upper
84	100		
49	161.6	107.5	161.3#
51	0.0	30.2	45.2#
86	58.4	49.3	73.9

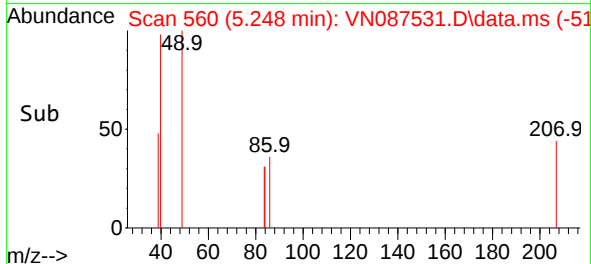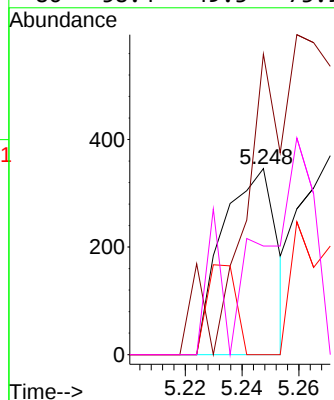

#21
trans-1,2-Dichloroethene
Concen: 1.492 ug/l
RT: 5.777 min Scan# 650
Delta R.T. 0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Tgt Ion:	96	Resp:	4652
Ion	Ratio	Lower	Upper
96	100		
61	141.7	122.0	183.0
98	88.3	50.0	75.0#


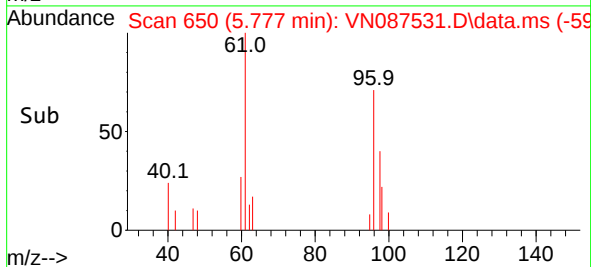
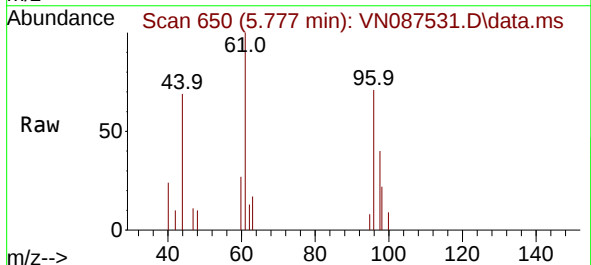
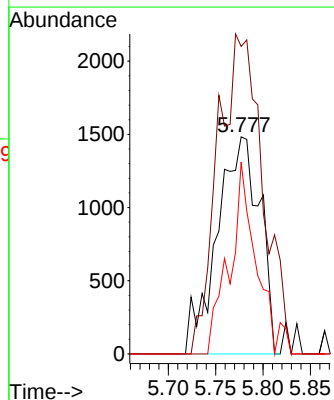




#25
2-Butanone
Concen: 0.619 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.012 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1843
Ion Ratio Lower Upper
43 100
72 76.5 19.6 29.4#

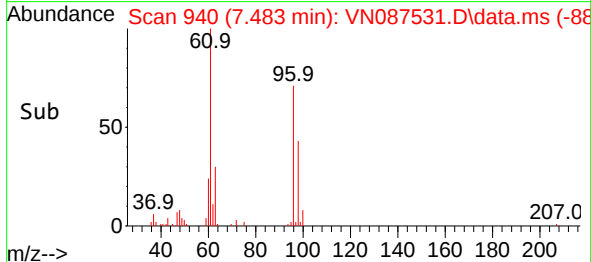

#27
cis-1,2-Dichloroethene
Concen: 13.345 ug/l
RT: 7.477 min Scan# 939
Delta R.T. 0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Tgt Ion: 96 Resp: 47912
Ion Ratio Lower Upper
96 100
61 140.6 0.0 297.8
98 65.4 0.0 132.4

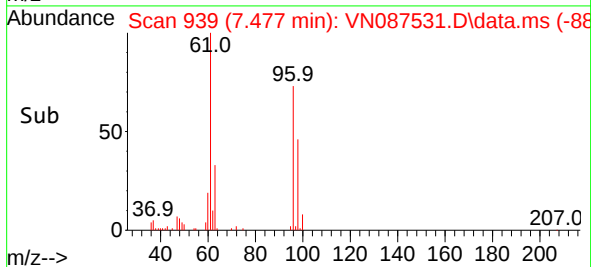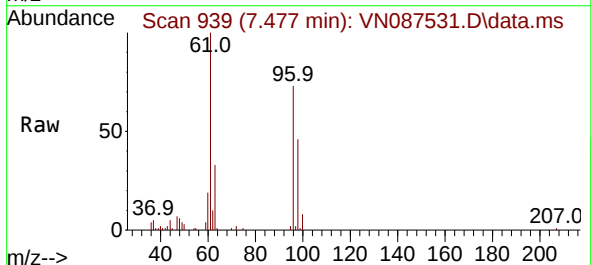



#29

Tetrahydrofuran

Concen: 0.439 ug/l

RT: 7.824 min Scan# 91

Delta R.T. -0.006 min


Lab File: VN087531.D

Acq: 13 Aug 2025 13:45




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	849
Ion Ratio	100	Lower	Upper
42	100		
72	0.0	33.4	50.0#
71	12.1	31.2	46.8#

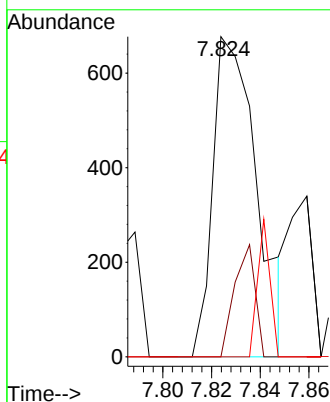

#31

Cyclohexane

Concen: 1.784 ug/l




RT: 8.212 min Scan# 1064


Delta R.T. -0.029 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Tgt Ion:	56	Resp:	9017
Ion Ratio	100	Lower	Upper
56	100		
69	155.4	22.7	34.1#
84	96.5	65.8	98.6

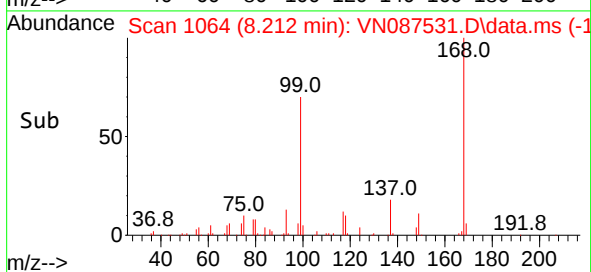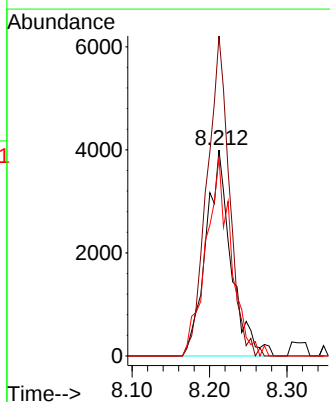

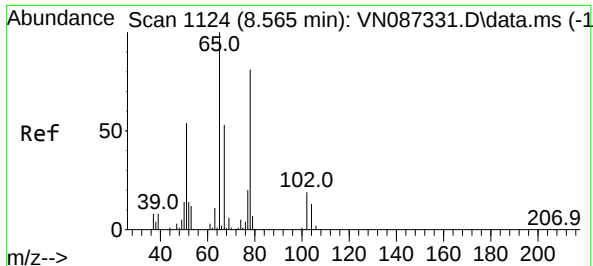

#33

1,2-Dichloroethane-d4

Concen: 62.546 ug/l

RT: 8.565 min Scan# 1124

Delta R.T. 0.000 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 257078

Ion Ratio Lower Upper

65 100

67 49.4 0.0 104.0

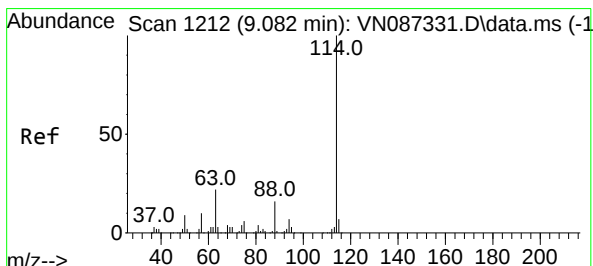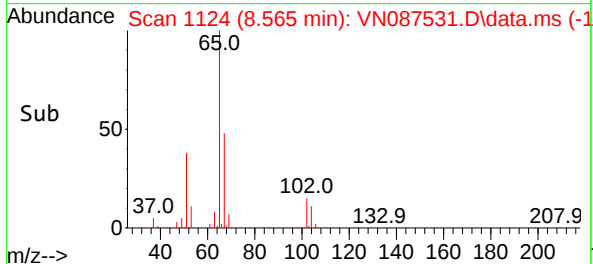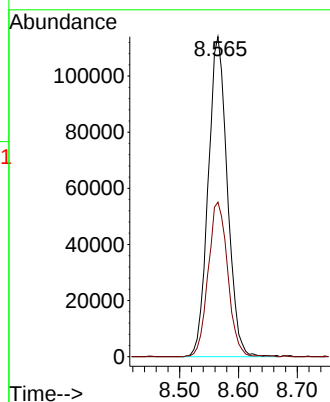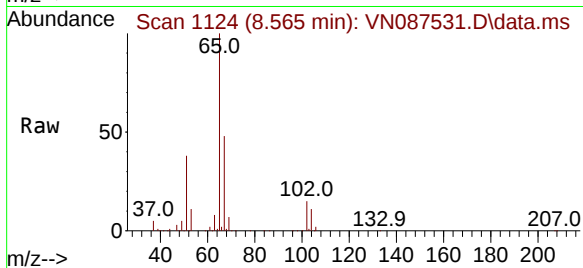

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.088 min Scan# 1213

Delta R.T. 0.006 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45




Tgt Ion: 114 Resp: 538435


Ion Ratio Lower Upper

114 100

63 22.1 0.0 44.6

88 15.9 0.0 32.8

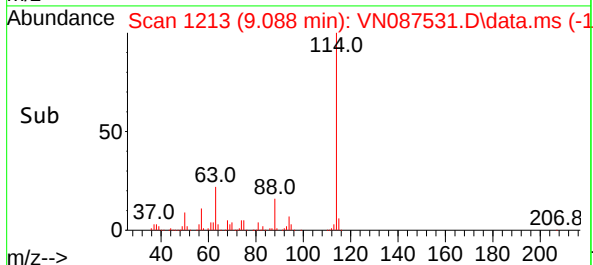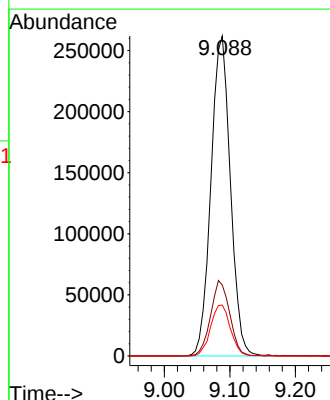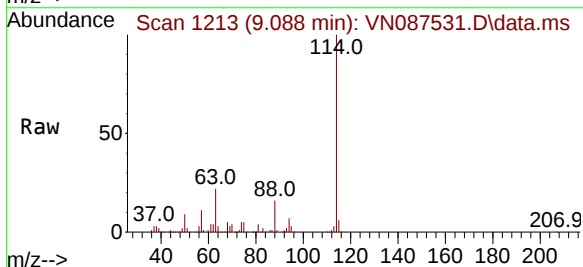

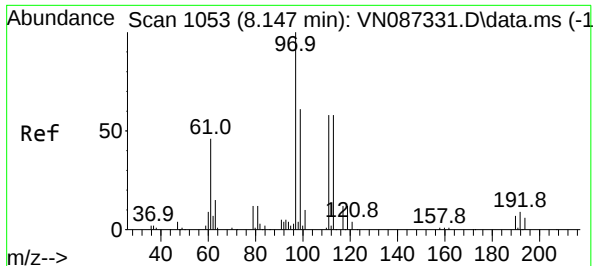

#35

Dibromofluoromethane

Concen: 49.077 ug/l

RT: 8.153 min Scan# 1054

Delta R.T. 0.006 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:113 Resp: 182278

Ion Ratio Lower Upper

113 100

111 103.4 82.5 123.7

192 16.5 13.7 20.5

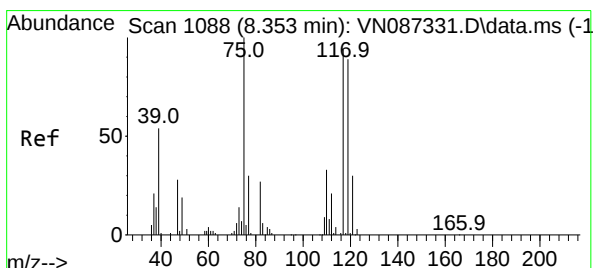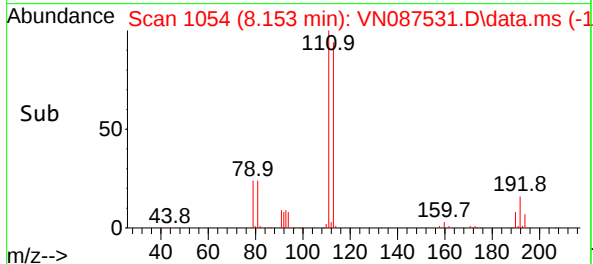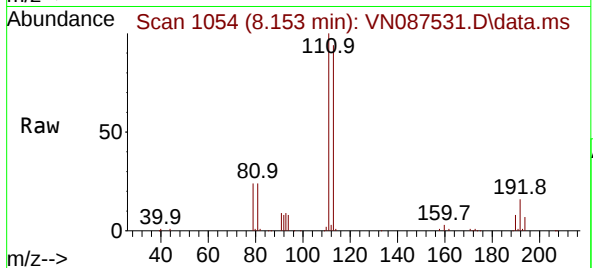

#36

1,1-Dichloropropene

Concen: 5.079 ug/l

RT: 8.206 min Scan# 1063

Delta R.T. -0.147 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45




Tgt Ion: 75 Resp: 24925


Ion Ratio Lower Upper

75 100

110 1.6 16.7 50.1#


77 0.0 25.2 37.8#

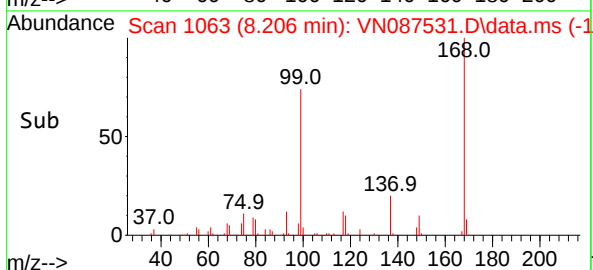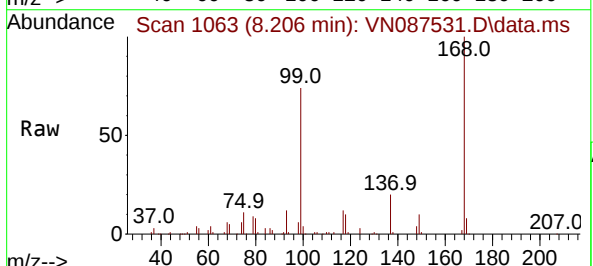



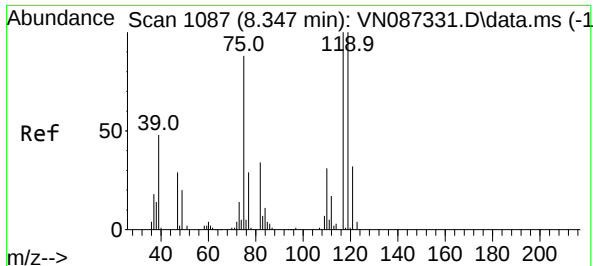


#38
Carbon Tetrachloride
Concen: 5.266 ug/l
RT: 8.206 min Scan# 1087
Delta R.T. -0.141 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Instrument :
MSVOA_N
ClientSampleId :



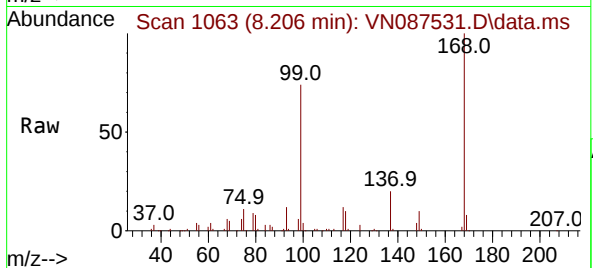



Tgt Ion:117 Resp: 28463
Ion Ratio Lower Upper
117 100
119 5.9 80.2 120.2#
121 0.0 25.4 38.2#

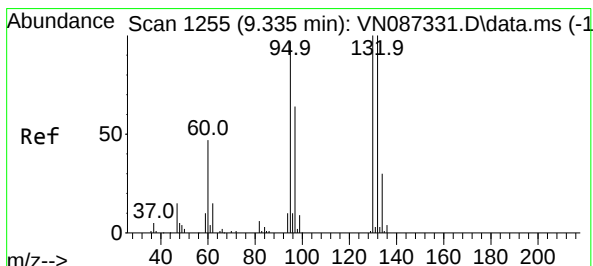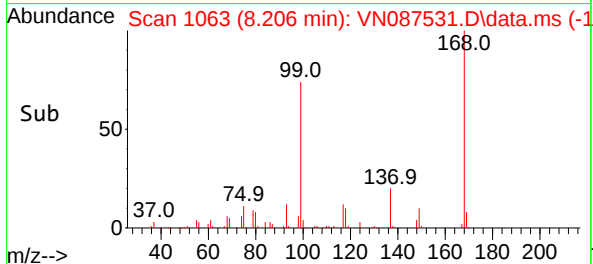

#44
Trichloroethene
Concen: 22.870 ug/l
RT: 9.335 min Scan# 1255
Delta R.T. 0.000 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Tgt Ion:130 Resp: 85704
Ion Ratio Lower Upper
130 100
95 110.3 0.0 195.2


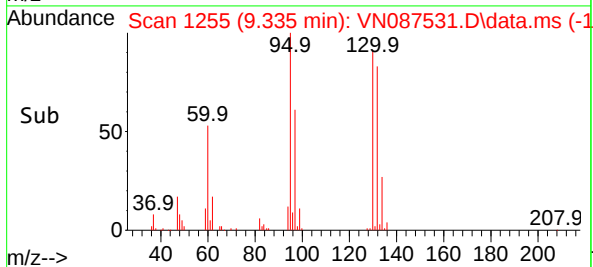

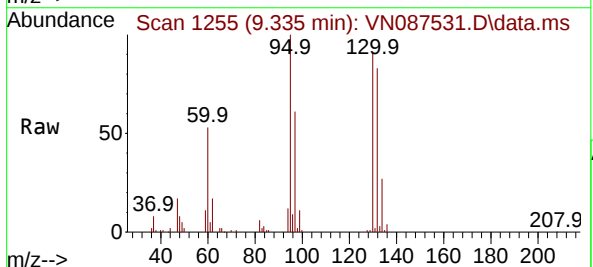




#50
Toluene-d8
Concen: 51.218 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. 0.000 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 678568
Ion Ratio Lower Upper
98 100
100 64.4 52.1 78.1

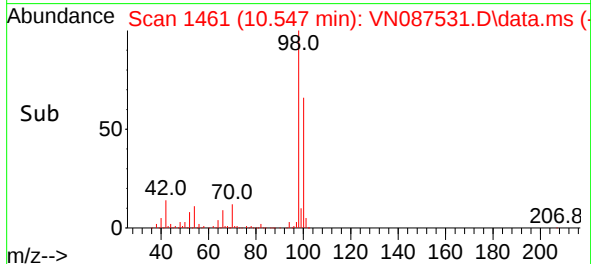

#51
4-Methyl-2-Pentanone
Concen: 0.252 ug/l
RT: 10.430 min Scan# 1441
Delta R.T. 0.001 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45


Tgt Ion: 43 Resp: 1754
Ion Ratio Lower Upper
43 100
58 0.0 30.8 46.2#

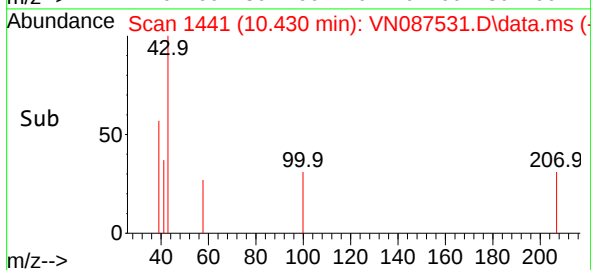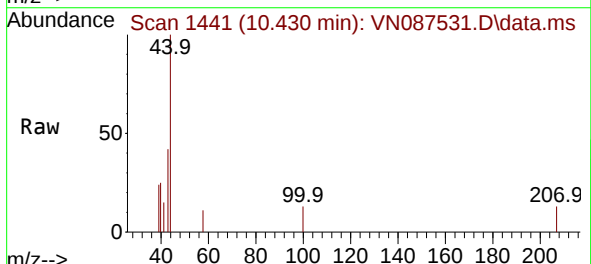






#55
1,1,2-Trichloroethane
Concen: 0.266 ug/l
RT: 11.071 min Scan# 1550
Delta R.T. 0.071 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	97	Resp:	1039
Ion	Ratio	Lower	Upper
97	100		
83	110.5	72.6	109.0#
85	43.1	46.7	70.1#
99	33.1	54.1	81.1#

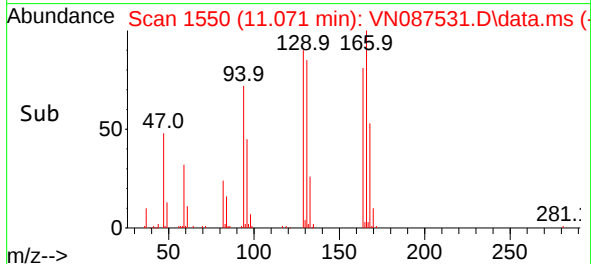

#59
2-Hexanone
Concen: 0.255 ug/l
RT: 11.053 min Scan# 1547
Delta R.T. -0.129 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Tgt Ion:	43	Resp:	1175
Ion	Ratio	Lower	Upper
43	100		
58	65.2	26.7	80.0




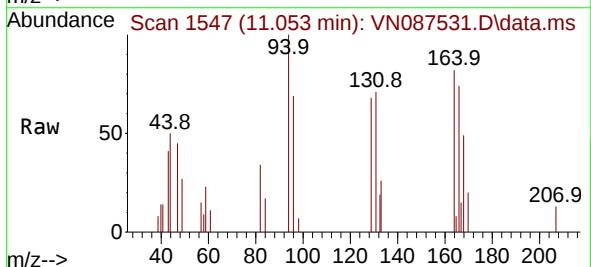


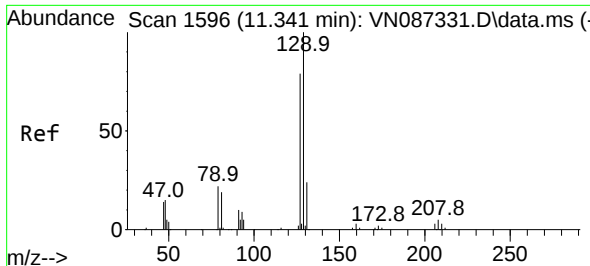

#60
Dibromochloromethane
Concen: 21.834 ug/l
RT: 11.082 min Scan# 11
Delta R.T. -0.259 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 97179
Ion Ratio Lower Upper
129 100
127 0.1 39.1 117.5#

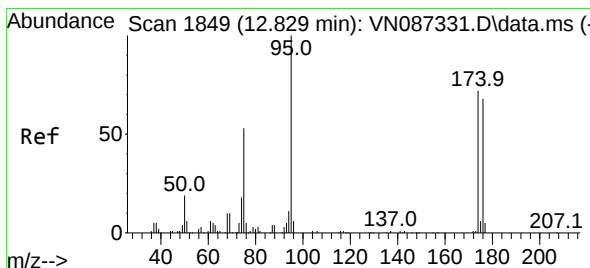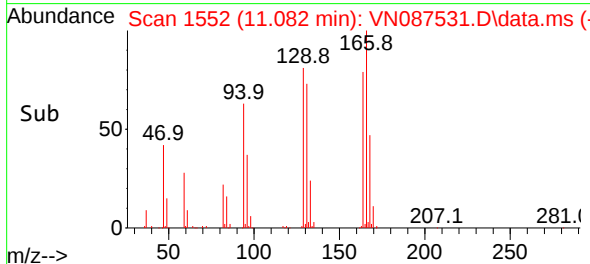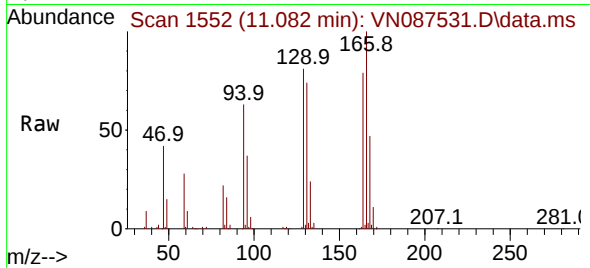

#62
4-Bromofluorobenzene
Concen: 49.449 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.000 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

Tgt Ion: 95 Resp: 242040
Ion Ratio Lower Upper
95 100
174 67.5 0.0 149.4
176 63.1 0.0 141.2

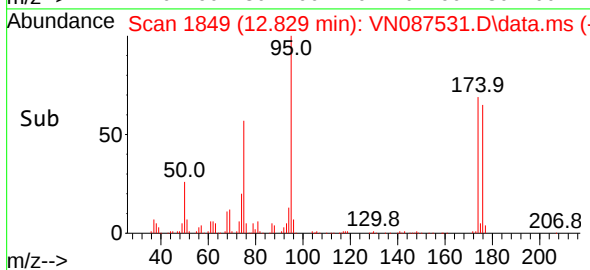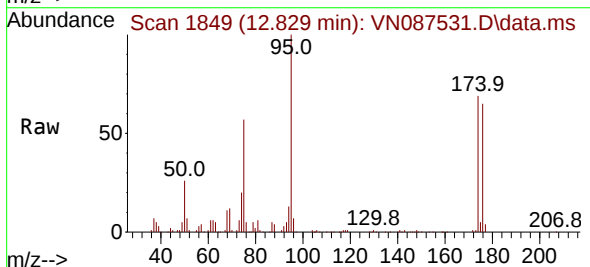



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.847 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:117 Resp: 477328

Ion Ratio Lower Upper

117 100

82 61.3 47.4 71.2

119 32.5 23.8 35.8

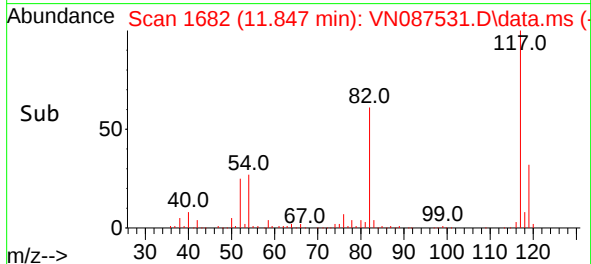

#64

Tetrachloroethene

Concen: 31.293 ug/l

RT: 11.082 min Scan# 1552

Delta R.T. -0.006 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Tgt Ion:164 Resp: 96136




Ion Ratio Lower Upper


164 100

166 127.2 105.5 158.3

129 103.0 77.4 116.2


131 93.8 77.3 115.9

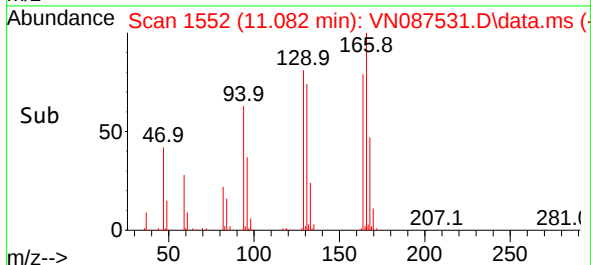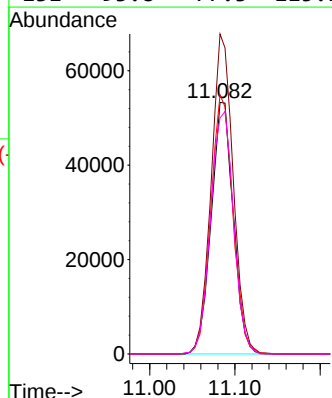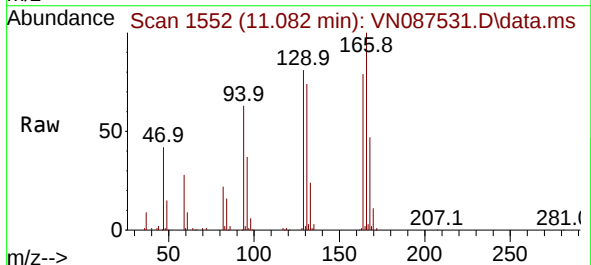



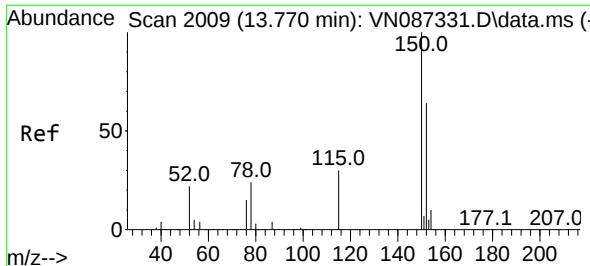


#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.770 min Scan# 2009
 Delta R.T. 0.000 min
 Lab File: VN087531.D
 Acq: 13 Aug 2025 13:45

Instrument :
 MSVOA_N
 ClientSampleId :



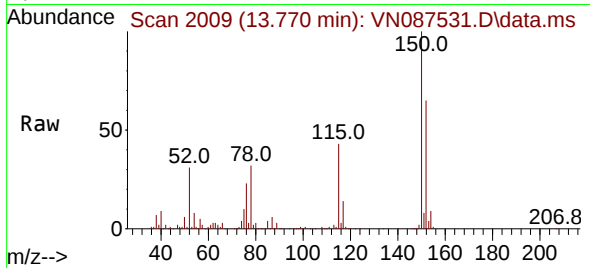



Tgt Ion:152 Resp: 224016
 Ion Ratio Lower Upper
 152 100
 115 64.9 31.1 93.5
 150 157.2 0.0 349.0

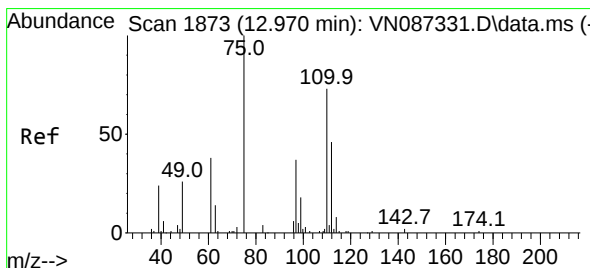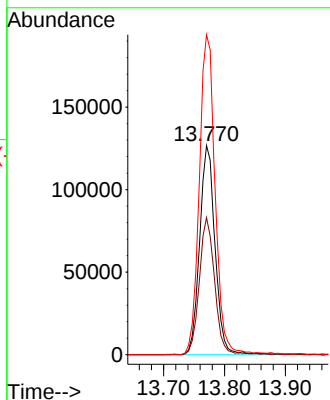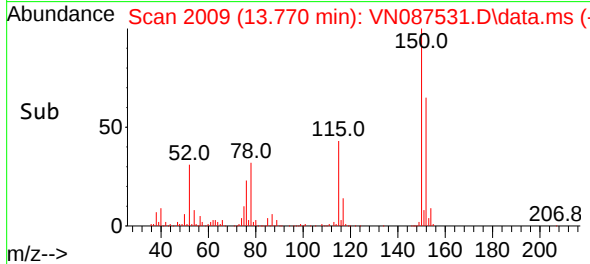

#76
 1,2,3-Trichloropropane
 Concen: 28.312 ug/l
 RT: 12.829 min Scan# 1849
 Delta R.T. -0.141 min
 Lab File: VN087531.D
 Acq: 13 Aug 2025 13:45

Tgt Ion: 75 Resp: 142222
 Ion Ratio Lower Upper
 75 100
 77 0.9 94.5 283.6#


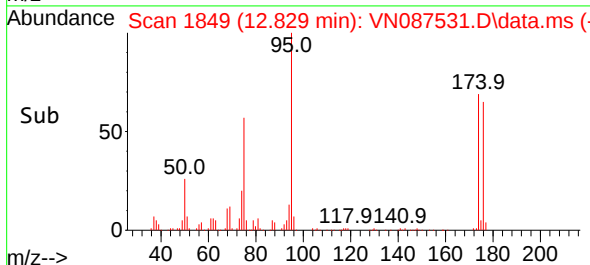
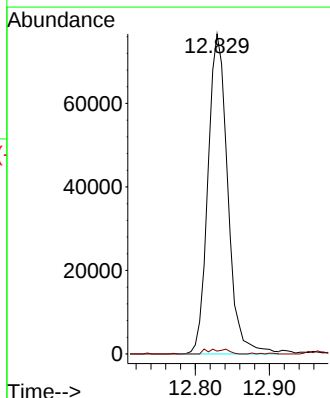
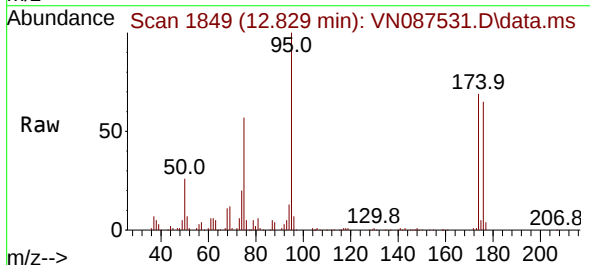




#81
 trans-1,4-Dichloro-2-butene
 Concen: 77.466 ug/l
 RT: 12.829 min Scan# 1849
 Delta R.T. 0.112 min
 Lab File: VN087531.D
 Acq: 13 Aug 2025 13:45




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 142222
 Ion Ratio Lower Upper
 75 100
 53 0.0 83.5 125.3#
 89 0.0 38.4 57.6#

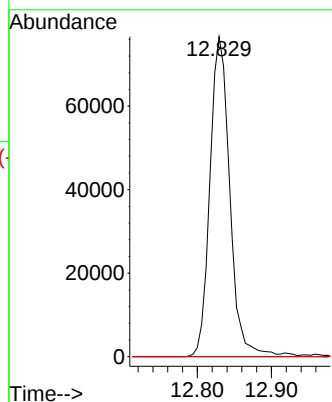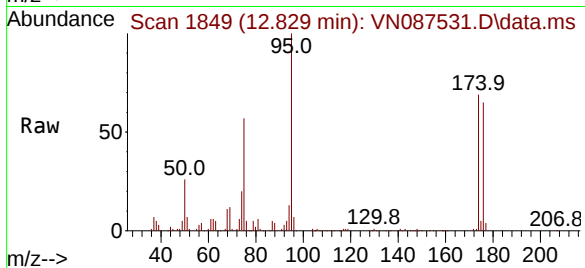

#87
 1,3-Dichlorobenzene
 Concen: 0.200 ug/l
 RT: 13.718 min Scan# 2000
 Delta R.T. 0.006 min
 Lab File: VN087531.D
 Acq: 13 Aug 2025 13:45

Tgt Ion: 146 Resp: 1436
 Ion Ratio Lower Upper
 146 100
 111 16.8 21.4 64.3#
 148 56.8 31.6 95.0


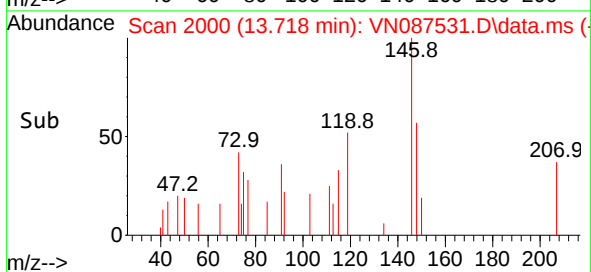
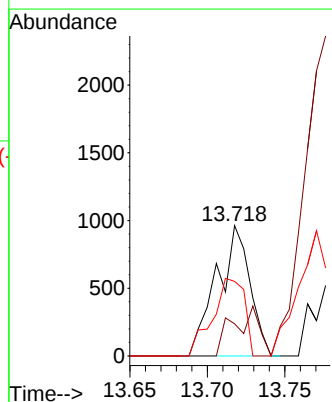
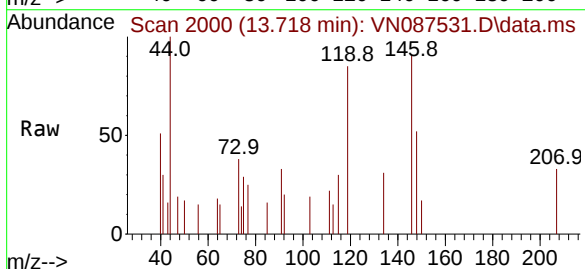




#88
1,4-Dichlorobenzene
Concen: 0.274 ug/l
RT: 13.794 min Scan# 2012
Delta R.T. 0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
146	100		
111	192.9	19.6	58.7#
148	116.8	31.4	94.0#

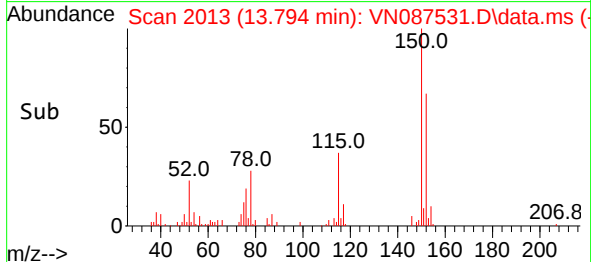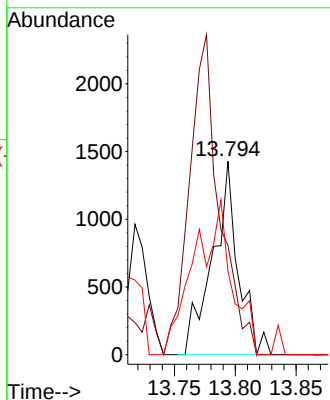

#89
n-Butylbenzene
Concen: 0.300 ug/l
RT: 14.029 min Scan# 2053
Delta R.T. -0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45


Tgt Ion	Ratio	Lower	Upper
91	100		
92	54.6	26.2	78.6
134	9.0	12.4	37.2#

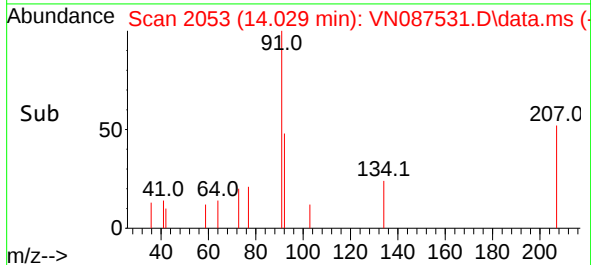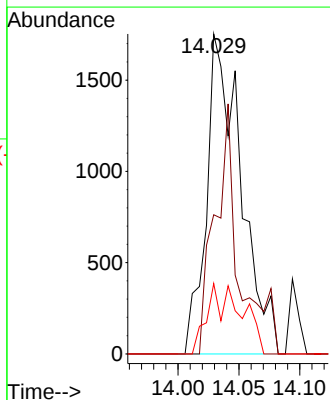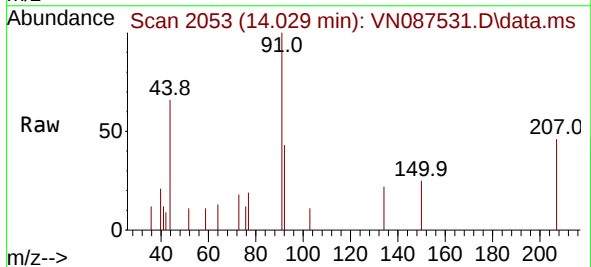






#93
1,2,4-Trichlorobenzene
Concen: 0.397 ug/l
RT: 15.365 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45


Instrument :
MSVOA_N
ClientSampleId :

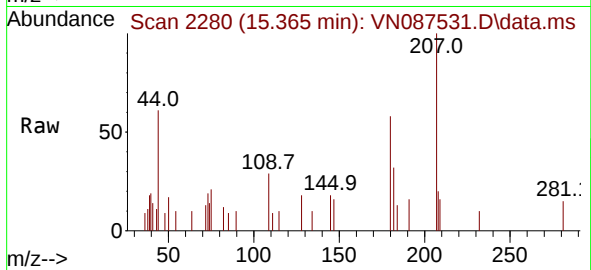



Tgt Ion:180 Resp: 1586
Ion Ratio Lower Upper
180 100
182 118.5 47.3 141.8
145 48.3 15.4 46.4#

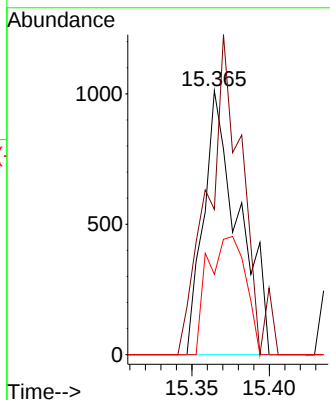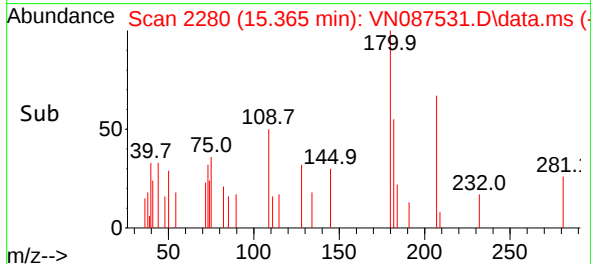


#94
Hexachlorobutadiene
Concen: 0.511 ug/l
RT: 15.476 min Scan# 2299
Delta R.T. 0.000 min
Lab File: VN087531.D
Acq: 13 Aug 2025 13:45

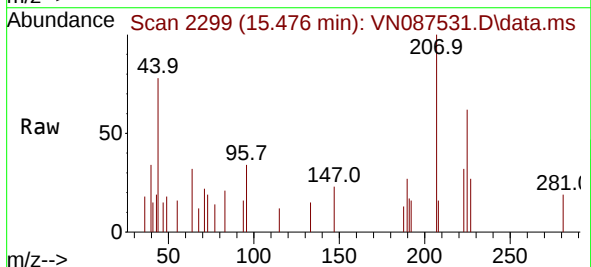

Tgt Ion:225 Resp: 759
Ion Ratio Lower Upper
225 100
223 71.5 32.1 96.3
227 62.6 31.3 93.9

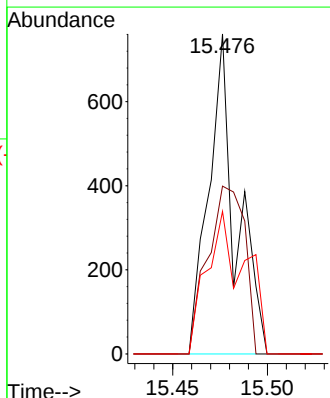



#95

Naphthalene

Concen: 0.353 ug/l

RT: 15.623 min Scan# 21

Delta R.T. 0.006 min


Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Instrument :

MSVOA_N

ClientSampleId :

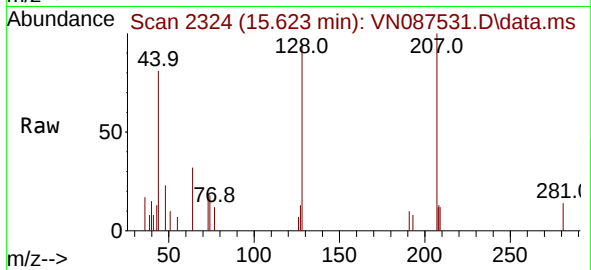




Tgt Ion:128 Resp: 4997

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 3.5 8.4 12.6#

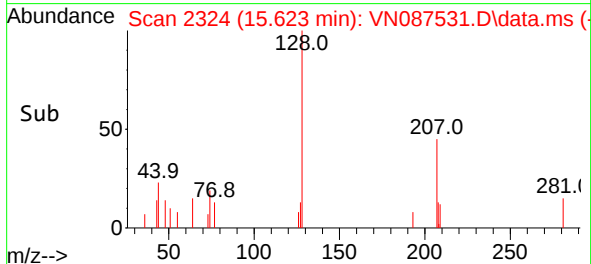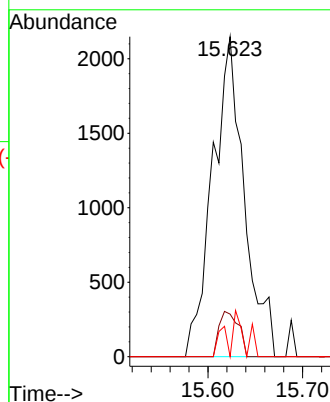

#96

1,2,3-Trichlorobenzene

Concen: 0.370 ug/l

RT: 15.806 min Scan# 2355

Delta R.T. -0.006 min

Lab File: VN087531.D

Acq: 13 Aug 2025 13:45

Tgt Ion:180 Resp: 1482

Ion Ratio Lower Upper

180 100

182 77.9 47.1 141.4

145 23.8 16.9 50.6

