

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081418\
 Data File : VN050598.D
 Acq On : 14 Aug 2018 13:32
 Operator : MD\SY
 Sample : J4426-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGEBLANK-WATERREF-4

Quant Time: Aug 15 08:54:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	663975	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1034453	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	905386	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	323368	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	438530	52.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.80%	
35) Dibromofluoromethane	7.59	113	412311	49.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.84%	
50) Toluene-d8	10.09	98	1469325	47.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.54%	
62) 4-Bromofluorobenzene	12.40	95	397535	38.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	77.42%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081418\
Data File : VN050598.D
Acq On : 14 Aug 2018 13:32
Operator : MD\SY
Sample : J4426-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGEBLANK-WATERREF-4

Quant Time: Aug 15 08:54:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration

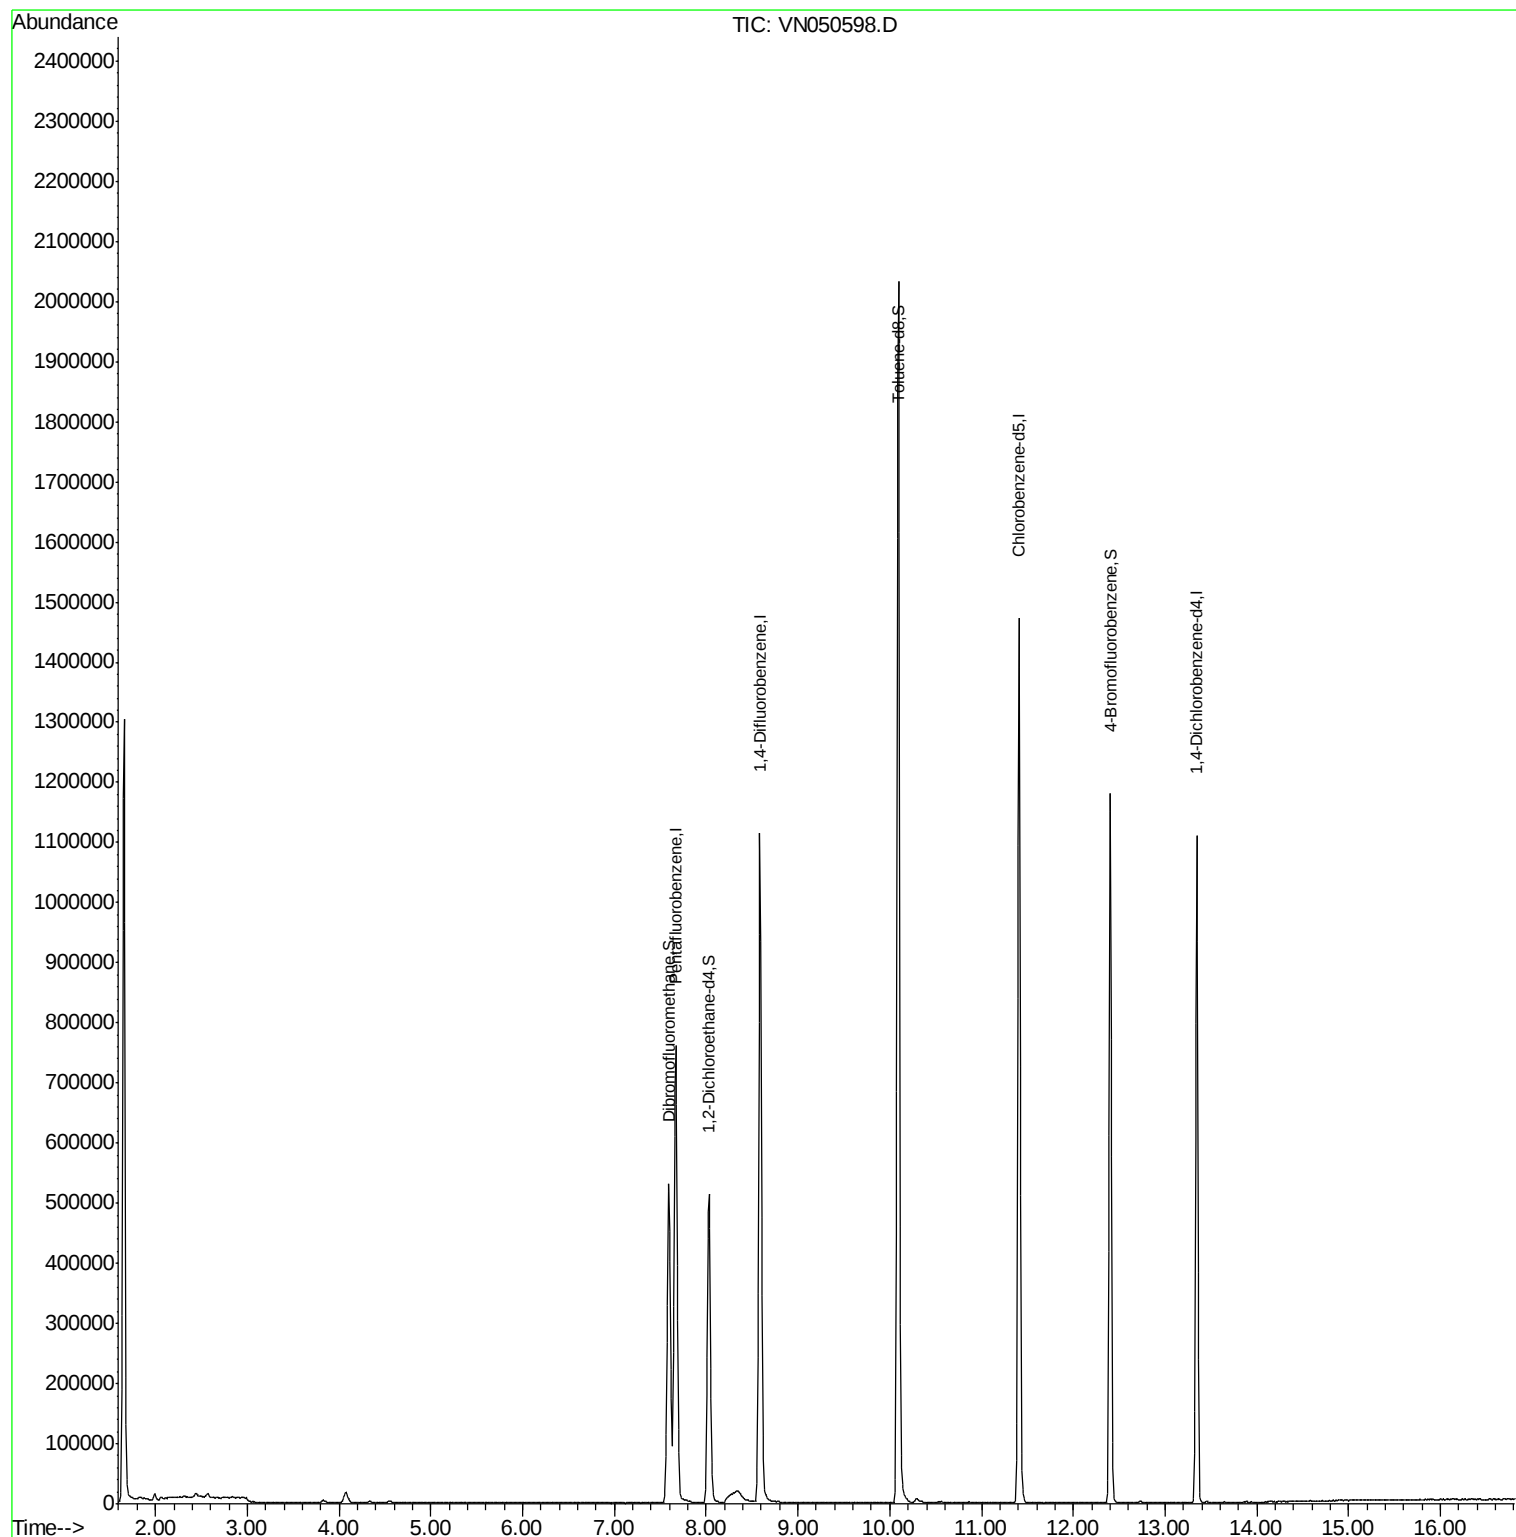

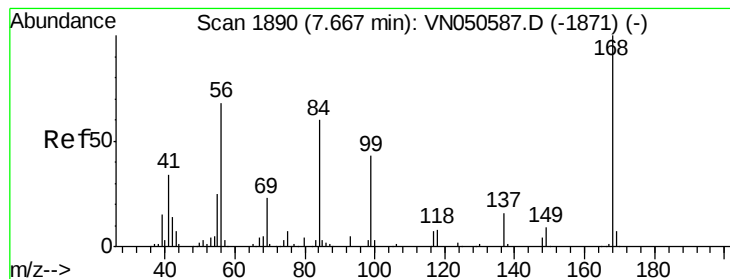

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. 0.00 min

Lab File: VN050598.D

Acq: 14 Aug 2018 13:32

Instrument :

MSVOA_N

ClientSampleId :


STORAGEBLANK-WATERREF-4

Tgt Ion:168 Resp: 663975

Ion Ratio Lower Upper

168 100

99 51.8 40.8 61.2

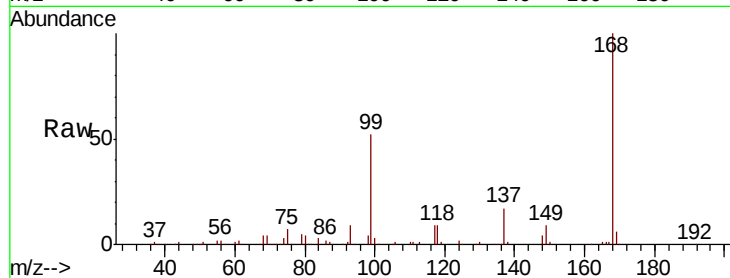

Abundance Ion 167.90 (167.60 to 168.60): VN050587.D (-1871) (-)

Ion 98.90 (98.60 to 99.60): VN050587.D (-1871) (-)

7.67

250000

200000



150000

100000

50000

0

Time-->

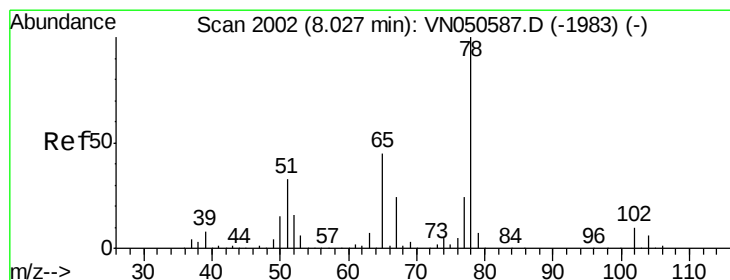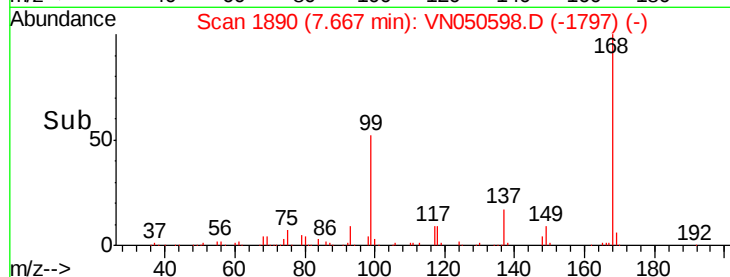

#33

1,2-Dichloroethane-d4

Concen: 52.397 ug/l

RT: 8.03 min Scan# 2003

Delta R.T. 0.00 min

Lab File: VN050598.D


Acq: 14 Aug 2018 13:32

Tgt Ion: 65 Resp: 438530

Ion Ratio Lower Upper

65 100

67 54.6 0.0 109.8

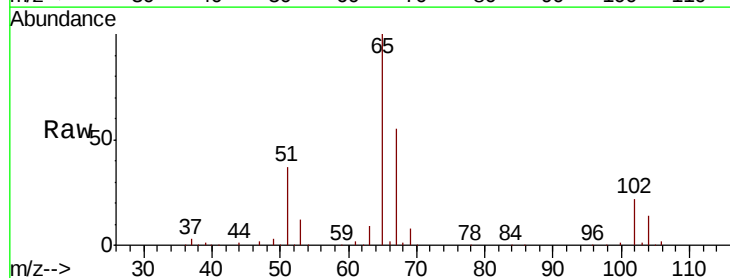

Abundance Ion 64.90 (64.60 to 65.60): VN050587.D (-1983) (-)

Ion 66.90 (66.60 to 67.60): VN050587.D (-1983) (-)

8.03

200000


150000


100000

50000

0

Time-->

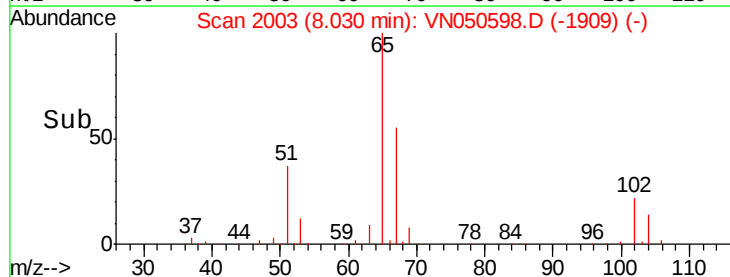


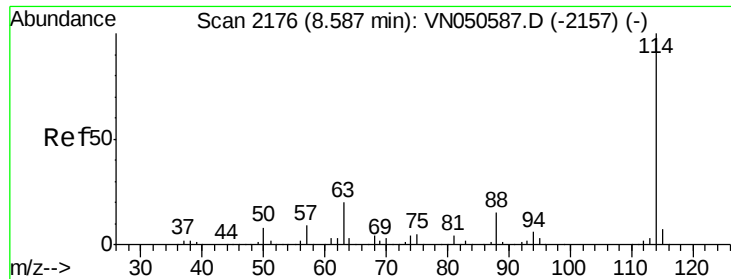




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN050598.D
 Acq: 14 Aug 2018 13:32

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGEBLANK-WATERREF-4

Tgt Ion:114 Resp: 1034453
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 40.0
 88 15.1 0.0 30.8

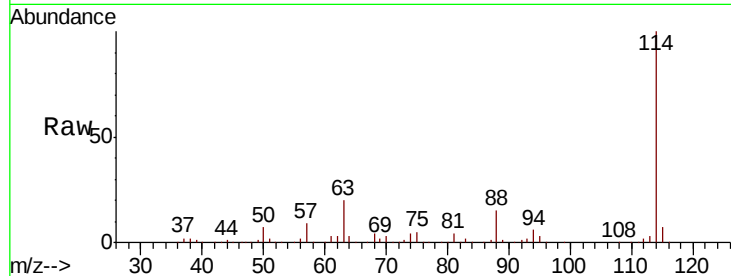


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

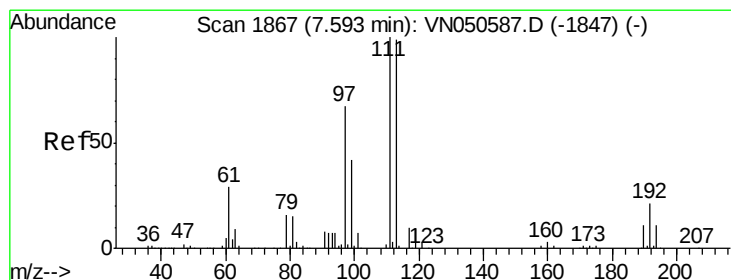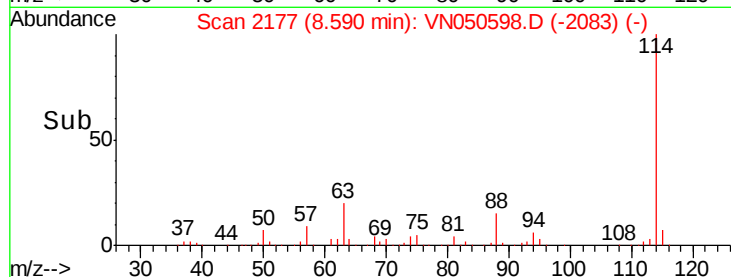
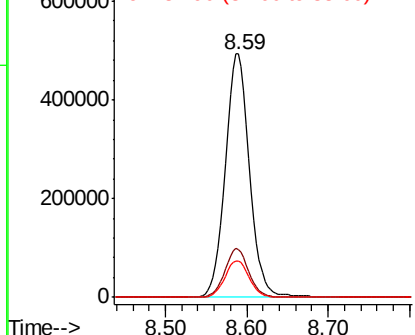



#35
 Dibromofluoromethane
 Concen: 49.924 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050598.D
 Acq: 14 Aug 2018 13:32

Tgt Ion:113 Resp: 412311
 Ion Ratio Lower Upper
 113 100
 111 103.1 81.0 121.6
 192 22.1 17.6 26.4

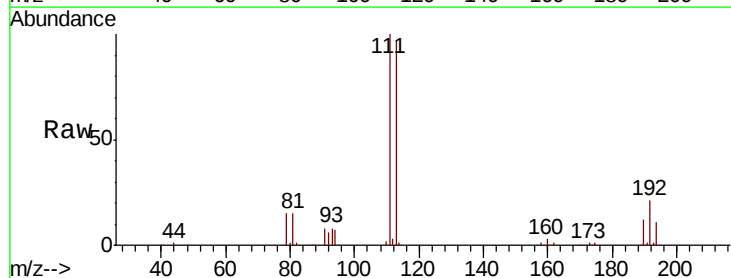

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



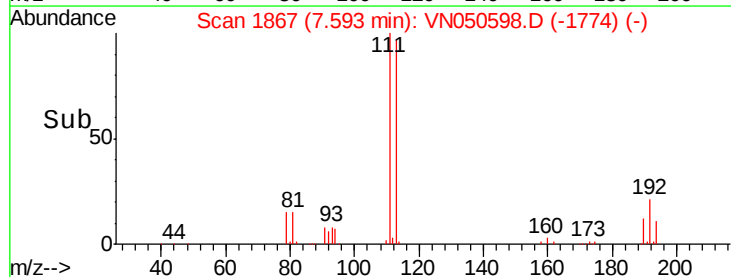
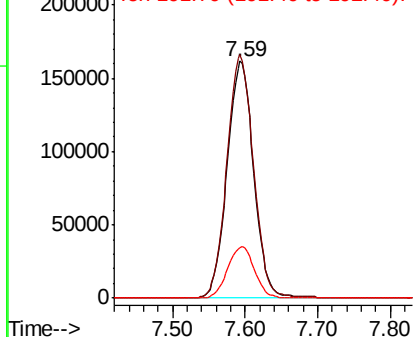


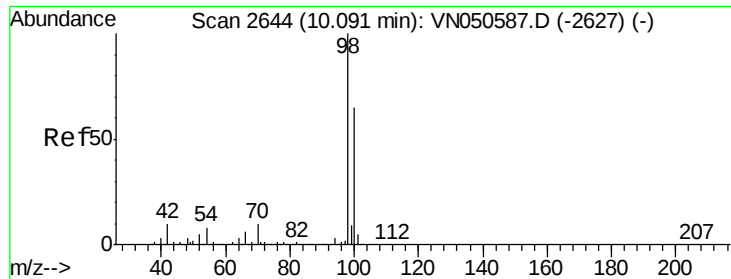

#50
Toluene-d8
Concen: 47.273 ug/l
RT: 10.09 min Scan# 2645
Delta R.T. 0.00 min
Lab File: VN050598.D
Acq: 14 Aug 2018 13:32




Instrument :
MSVOA_N
ClientSampleId :
STORAGEBLANK-WATERREF-4


Tgt Ion: 98 Resp: 1469325
Ion Ratio Lower Upper
98 100
100 63.7 51.8 77.8

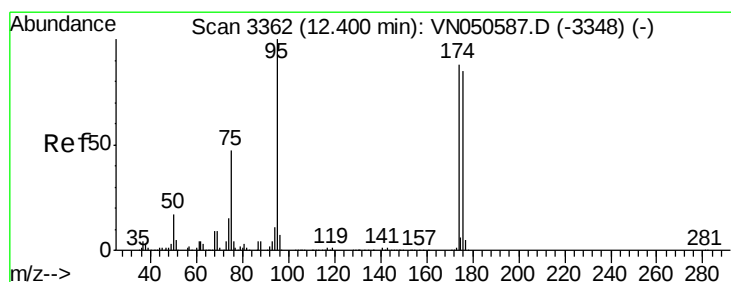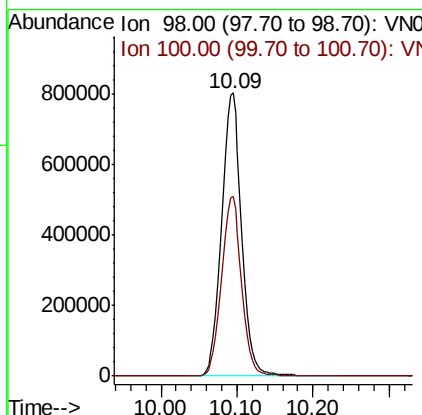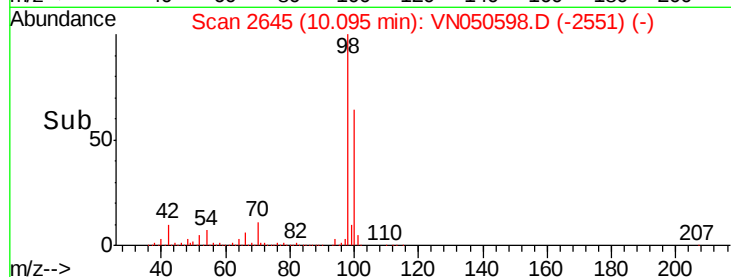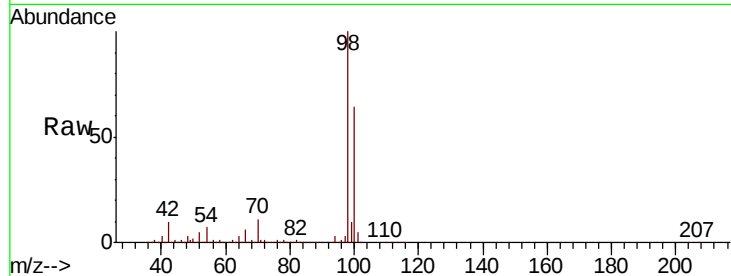

#62
4-Bromofluorobenzene
Concen: 38.715 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. 0.00 min
Lab File: VN050598.D
Acq: 14 Aug 2018 13:32

Tgt Ion: 95 Resp: 397535
Ion Ratio Lower Upper
95 100
174 91.7 0.0 177.8
176 87.6 0.0 175.0

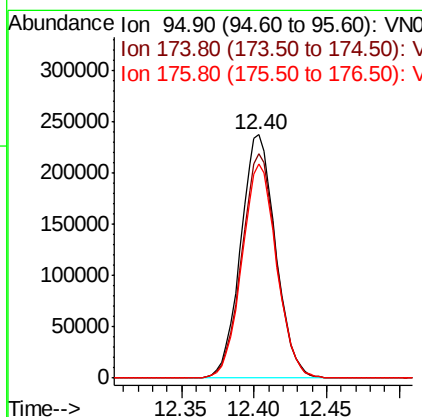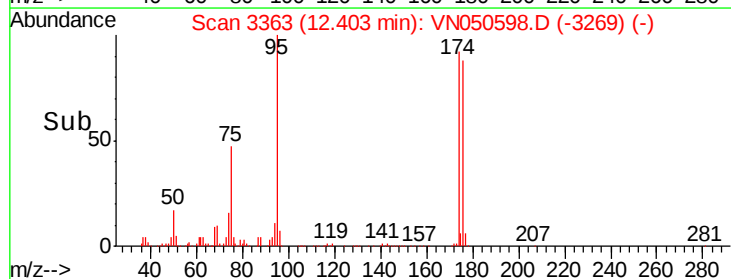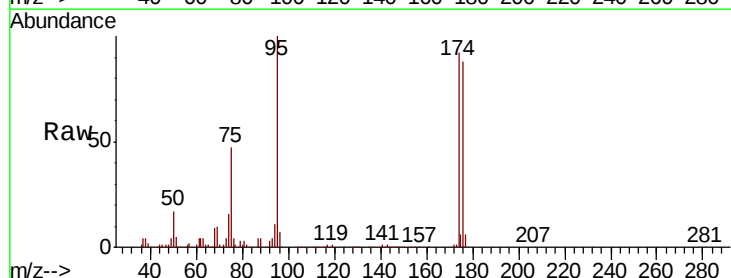


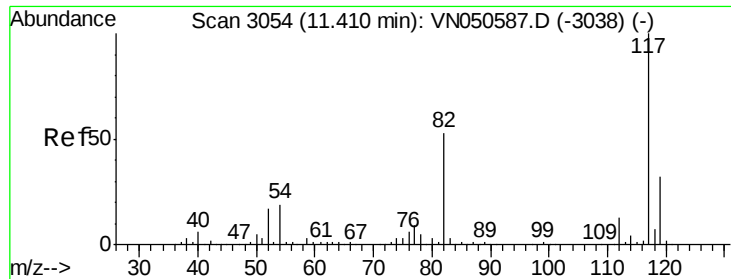




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050598.D
Acq: 14 Aug 2018 13:32

Instrument :
MSVOA_N
ClientSampleId :
STORAGEBLANK-WATERREF-4

Tgt Ion:117 Resp: 905386
Ion Ratio Lower Upper
117 100
82 53.1 42.4 63.6
119 31.8 25.8 38.8

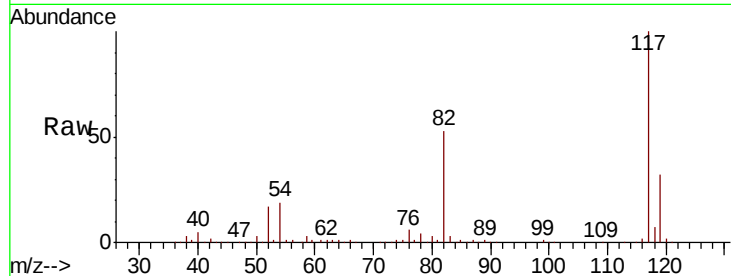


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V

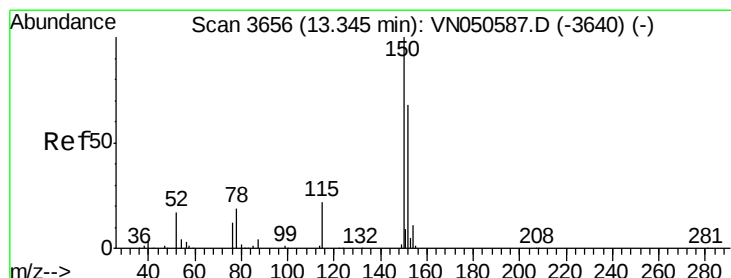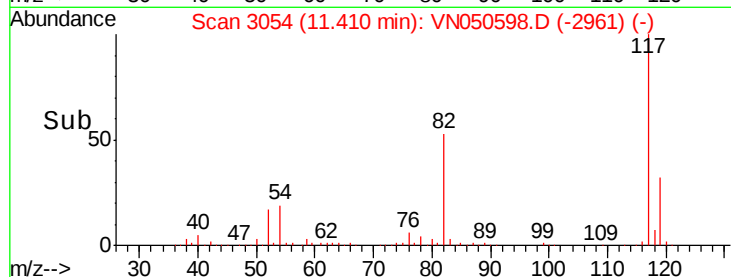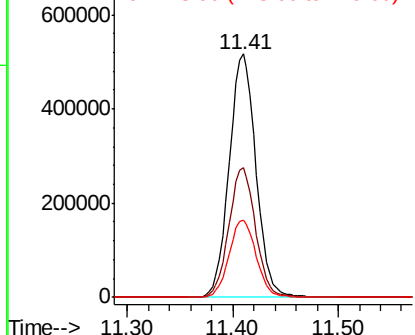

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3656
Delta R.T. 0.00 min
Lab File: VN050598.D
Acq: 14 Aug 2018 13:32

Tgt Ion:152 Resp: 323368
Ion Ratio Lower Upper
152 100
115 56.2 28.1 84.2
150 157.3 0.0 347.8

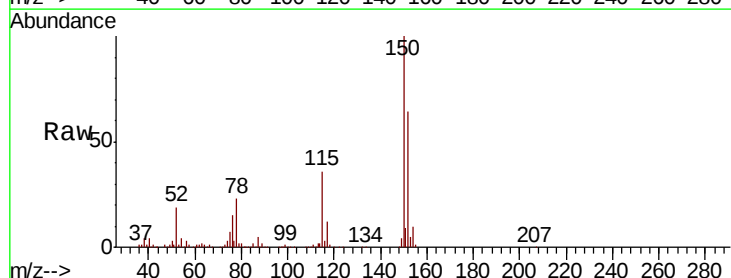

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

