

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081418\
 Data File : VN050606.D
 Acq On : 14 Aug 2018 16:50
 Operator : MD\SY
 Sample : J4427-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RB47197

Quant Time: Aug 14 17:13:34 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	647133	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1063528	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	889053	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	335355	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	441994	54.18	ug/l	0.00
Spiked Amount			Recovery	=	108.36%	
35) Dibromofluoromethane	7.59	113	410158	48.31	ug/l	0.00
Spiked Amount			Recovery	=	96.62%	
50) Toluene-d8	10.09	98	1455963	45.56	ug/l	0.00
Spiked Amount			Recovery	=	91.12%	
62) 4-Bromofluorobenzene	12.40	95	401482	38.03	ug/l	0.00
Spiked Amount			Recovery	=	76.06%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	2807	Below Cal		93
5) Bromomethane	2.57	94	3172	Below Cal		90
6) Chloroethane	2.71	64	339	Below Cal	#	43
8) Diethyl Ether	3.42	74	966	0.228	ug/l	88
10) Methyl Iodide	3.96	142	1413	7.171	ug/l #	67
16) Acetone	3.82	43	15794	6.342	ug/l	97
17) Carbon Disulfide	4.05	76	7027	0.318	ug/l	99
18) Methyl Acetate	4.33	43	10983	0.941	ug/l	98
20) Methylene Chloride	4.56	84	15062	0.688	ug/l	88
25) 2-Butanone	6.86	43	3777	1.129	ug/l #	77
30) Chloroform	7.38	83	14194	0.967	ug/l	93
31) Cyclohexane	7.67	56	11595	0.596	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	44540	3.762	ug/l #	48
38) Carbon Tetrachloride	7.67	117	56946	4.637	ug/l #	17
43) Isopropyl Acetate	8.17	43	193019	15.827	ug/l	97
47) Bromodichloromethane	9.41	83	3499	0.289	ug/l	88
48) Methyl methacrylate	9.18	41	6228	1.015	ug/l #	20
56) Ethyl methacrylate	10.23	69	429	1.945	ug/l #	23
59) 2-Hexanone	10.77	43	5488	1.031	ug/l #	61
70) Styrene	11.96	104	30	0.942	ug/l #	26
71) Bromoform	12.40	173	1654	0.301	ug/l #	28
75) 1,1,2,2-Tetrachloroethane	12.41	83	99	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	189540	34.667	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	189540	125.654	ug/l #	13
90) Hexachloroethane	13.99	117	830	0.205	ug/l #	4
93) 1,2,4-Trichlorobenzene	14.90	180	66	2.684	ug/l #	12
95) Naphthalene	15.13	128	4423	4.177	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081418\
Data File : VN050606.D
Acq On : 14 Aug 2018 16:50
Operator : MD\SY
Sample : J4427-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RB47197

Quant Time: Aug 14 17:13:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration

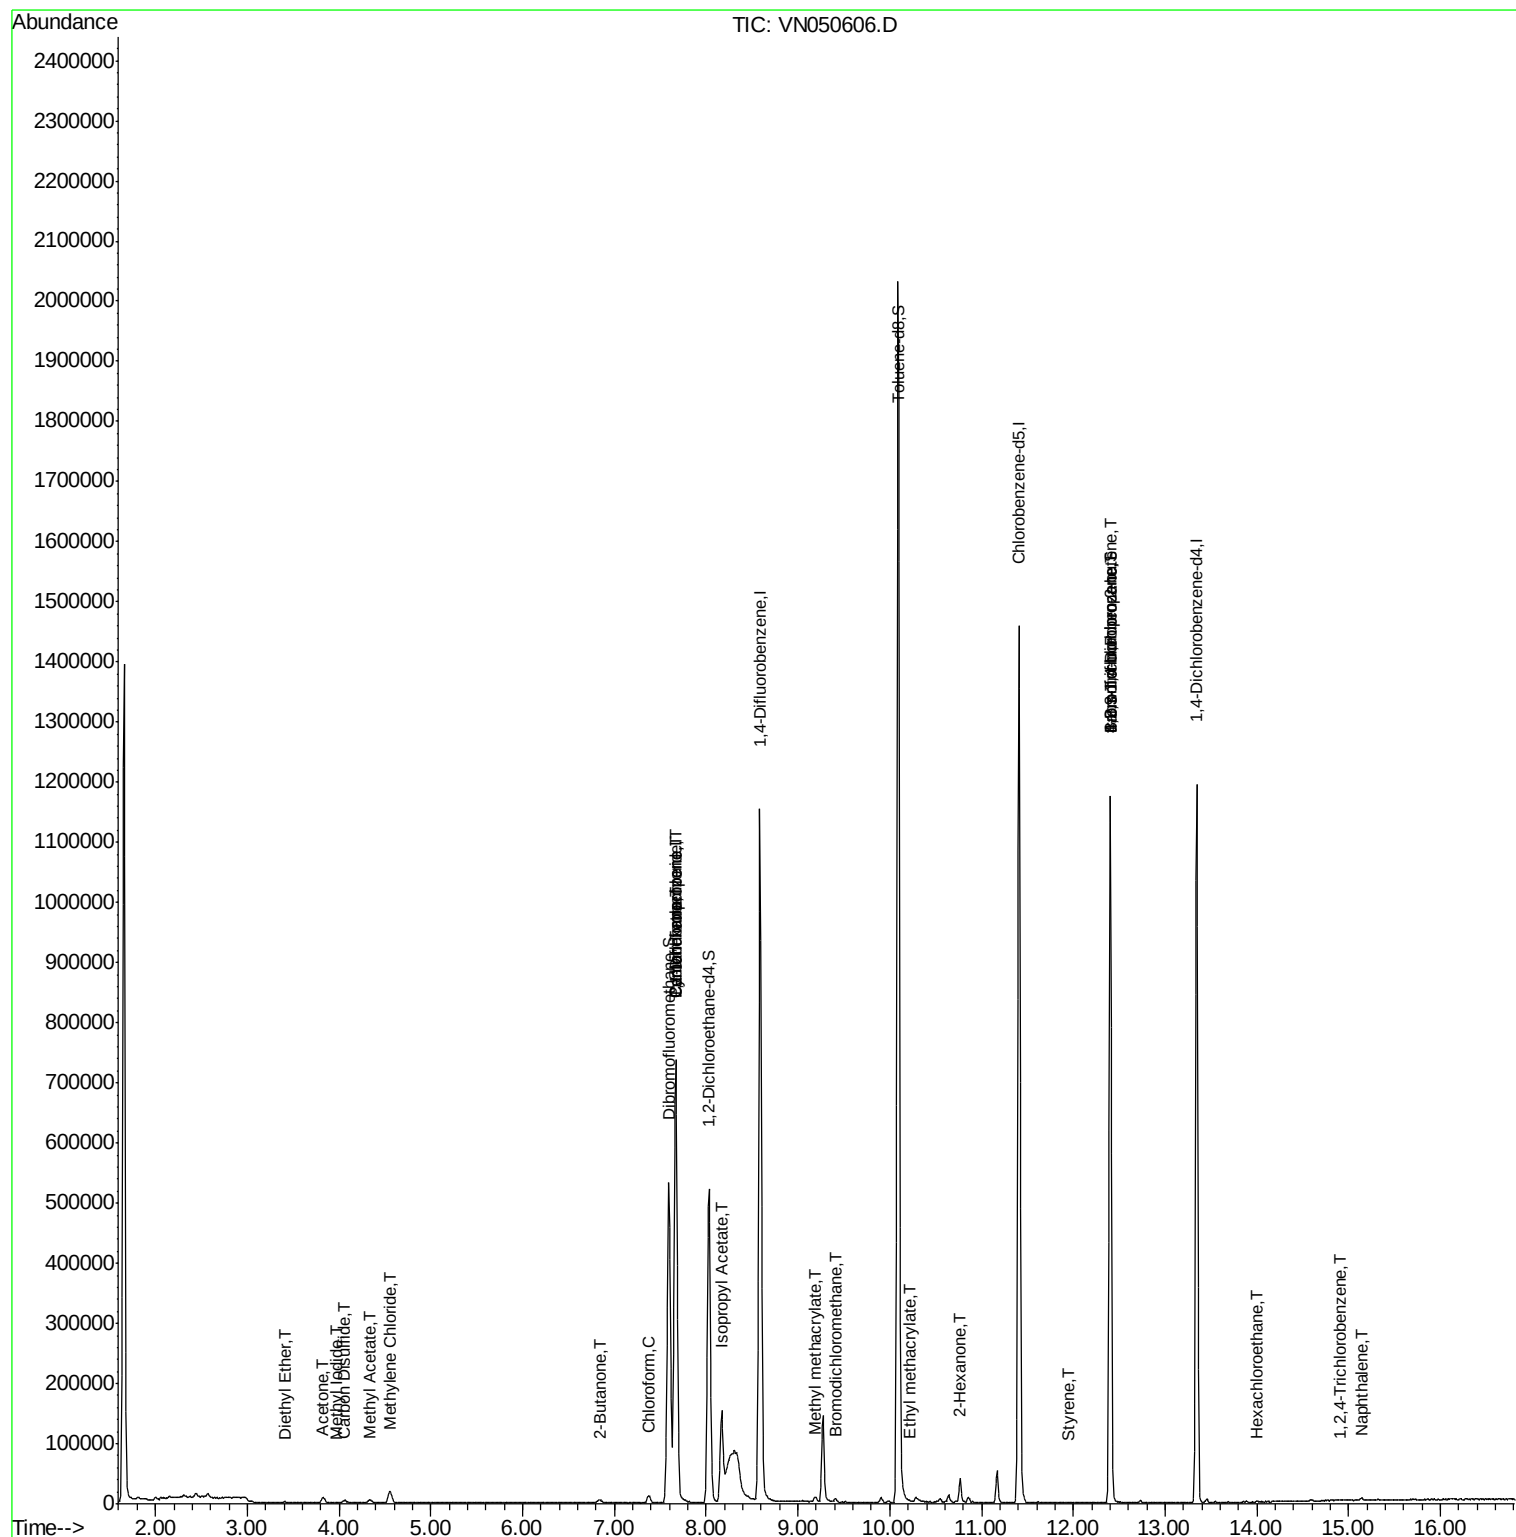

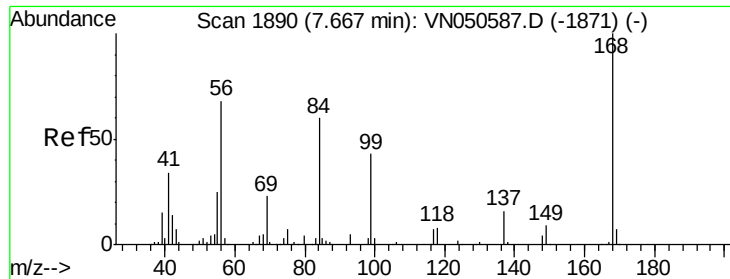

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampled :


RB47197

Tgt Ion:168 Resp: 647133

Ion Ratio Lower Upper

168 100

99 50.6 40.8 61.2

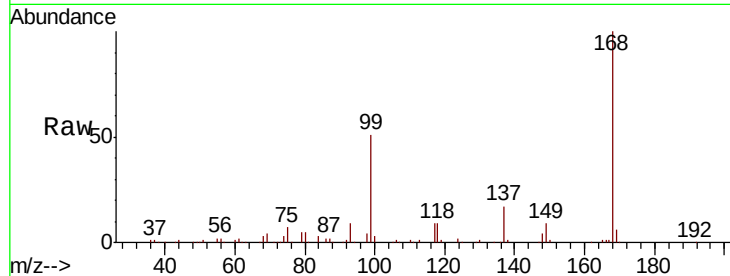

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.67

250000

200000



150000

100000

50000

0

Time-->

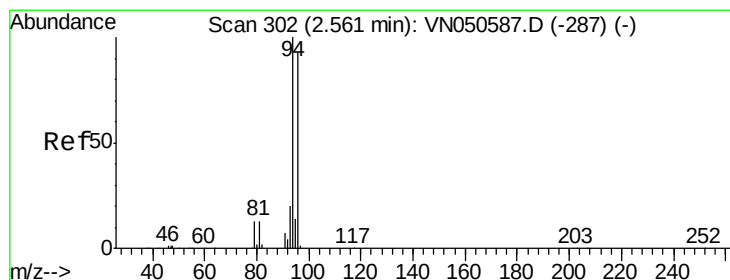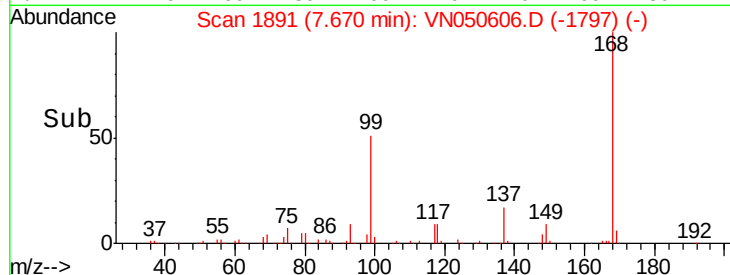

#5

Bromomethane

Concen: Below Cal

RT: 2.57 min Scan# 305

Delta R.T. 0.01 min

Lab File: VN050606.D


Acq: 14 Aug 2018 16:50

Tgt Ion: 94 Resp: 3172

Ion Ratio Lower Upper

94 100

96 102.5 74.0 111.0



Abundance Ion 93.90 (93.60 to 94.60): VN

Ion 95.90 (95.60 to 96.60): VN

2000


1500


1000

500

0

Time-->





#6

Chloroethane

Concen: Below Cal

RT: 2.71 min Scan# 347

Delta R.T. 0.01 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampleId :





RB47197

Tgt Ion: 64 Resp: 339

Ion Ratio Lower Upper

64 100

66 0.0 25.7 38.5#

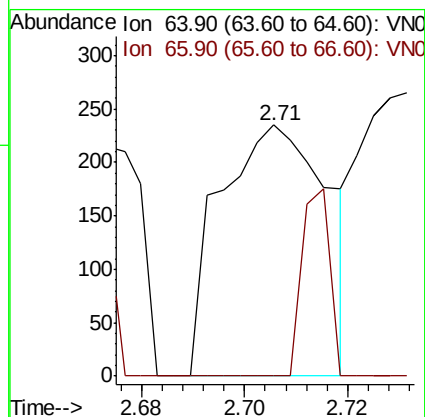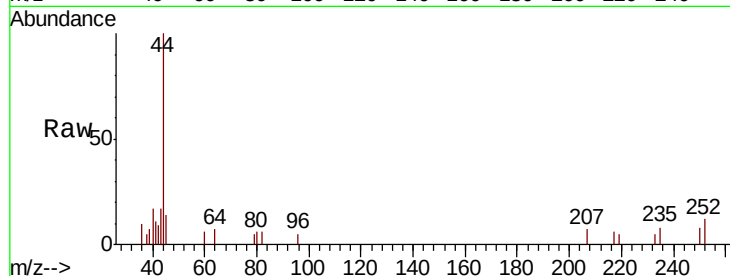

#8

Diethyl Ether

Concen: 0.228 ug/l

RT: 3.42 min Scan# 568

Delta R.T. 0.00 min

Lab File: VN050606.D




Acq: 14 Aug 2018 16:50


Tgt Ion: 74 Resp: 966

Ion Ratio Lower Upper

74 100

45 107.9 48.0 144.2



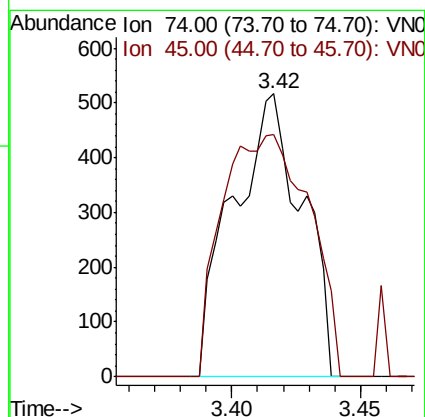





#10
Methyl Iodide
Concen: 7.171 ug/l
RT: 3.96 min Scan# 738
Delta R.T. 0.01 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50




Instrument :
MSVOA_N
ClientSampleId :
RB47197


Tgt Ion:142 Resp: 1413
Ion Ratio Lower Upper
142 100
127 19.5 32.6 49.0#
141 2.2 11.5 17.3#

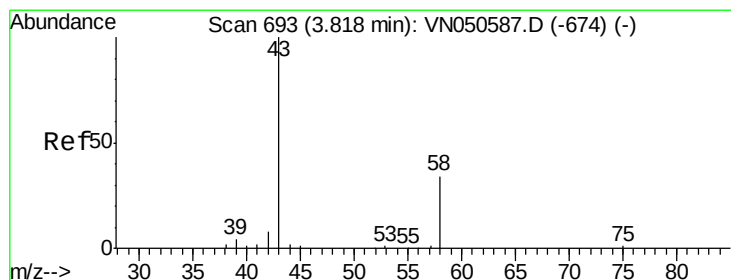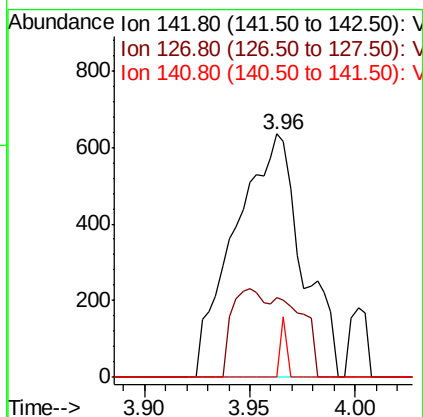

#16
Acetone
Concen: 6.342 ug/l
RT: 3.82 min Scan# 694
Delta R.T. 0.00 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50

Tgt Ion: 43 Resp: 15794
Ion Ratio Lower Upper
43 100
58 32.1 27.1 40.7

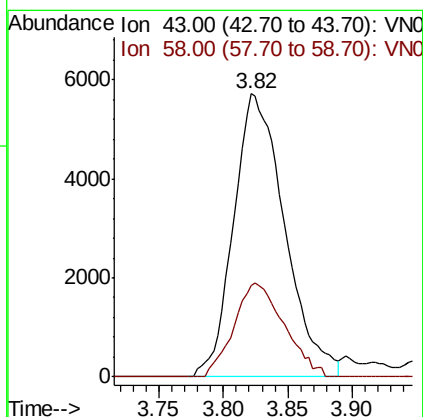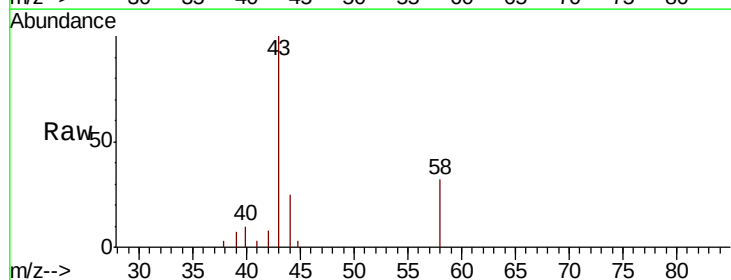



#17

Carbon Disulfide

Concen: 0.318 ug/l

RT: 4.05 min Scan# 765

Delta R.T. -0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampleId :





RB47197

Tgt Ion: 76 Resp: 7027

Ion Ratio Lower Upper

76 100

78 9.3 7.3 10.9

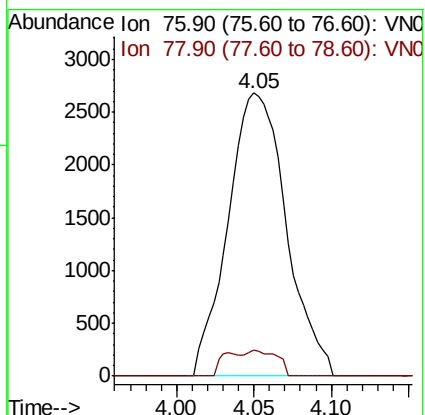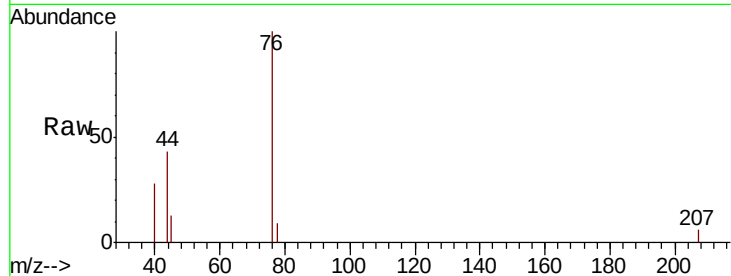

#18

Methyl Acetate

Concen: 0.941 ug/l

RT: 4.33 min Scan# 853

Delta R.T. 0.01 min

Lab File: VN050606.D




Acq: 14 Aug 2018 16:50


Tgt Ion: 43 Resp: 10983

Ion Ratio Lower Upper

43 100

74 23.7 19.7 29.5



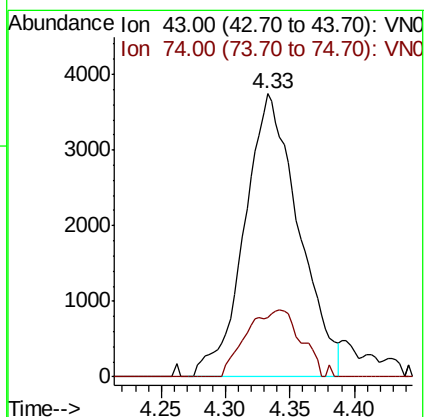





#20
Methylene Chloride
Concen: 0.688 ug/l
RT: 4.56 min Scan# 923
Delta R.T. 0.01 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50




Instrument :
MSVOA_N
ClientSampleId :
RB47197


Tgt Ion:	84	Resp:	15062
Ion	Ratio	Lower	Upper
84	100		
49	96.4	92.6	138.8
51	33.9	28.6	43.0
86	60.2	52.2	78.2

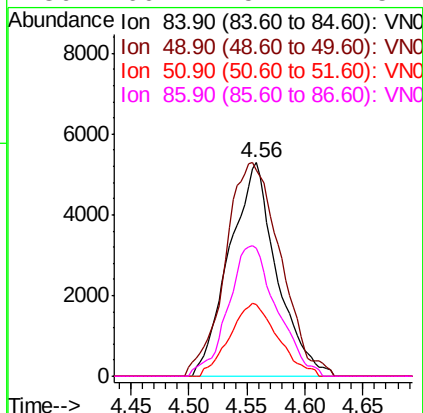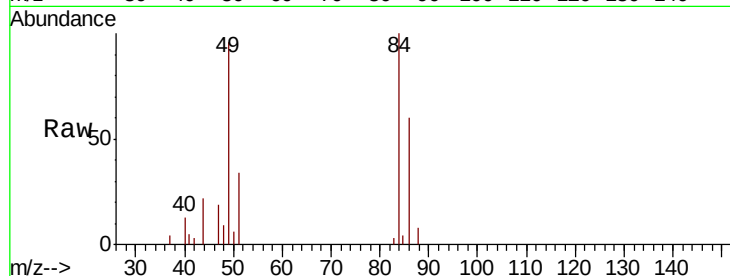

#25
2-Butanone
Concen: 1.129 ug/l
RT: 6.86 min Scan# 1638
Delta R.T. 0.02 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50

Tgt Ion:	43	Resp:	3777
Ion	Ratio	Lower	Upper
43	100		
72	15.5	21.8	32.6#


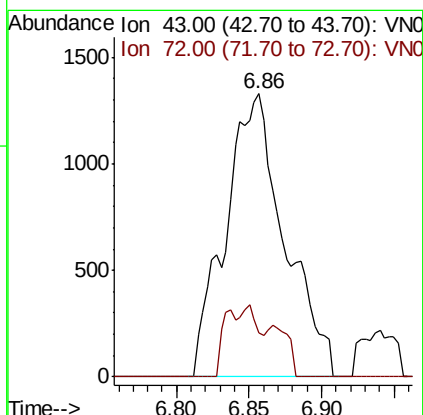






#30
Chloroform
Concen: 0.967 ug/l
RT: 7.38 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50




Instrument :
MSVOA_N
ClientSampleId :
RB47197


Tgt Ion: 83 Resp: 14194
Ion Ratio Lower Upper
83 100
85 60.1 52.5 78.7

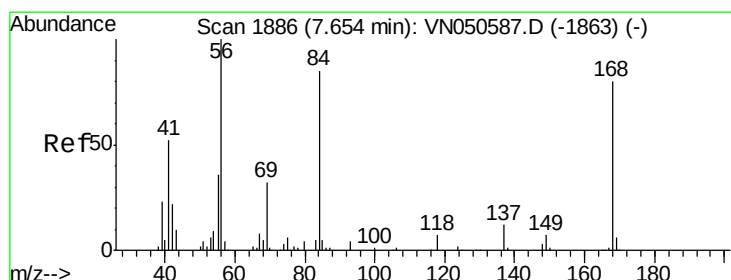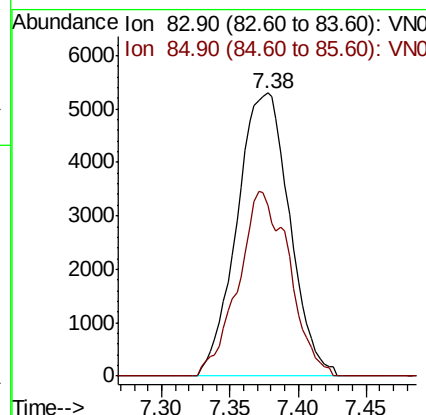

#31
Cyclohexane
Concen: 0.596 ug/l
RT: 7.67 min Scan# 1890
Delta R.T. 0.01 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50

Tgt Ion: 56 Resp: 11595
Ion Ratio Lower Upper
56 100
69 194.0 25.8 38.6#
84 127.7 67.8 101.6#


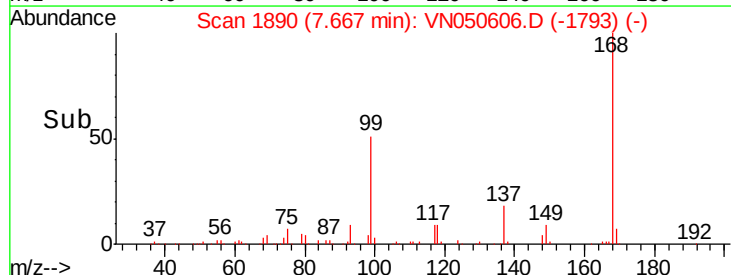
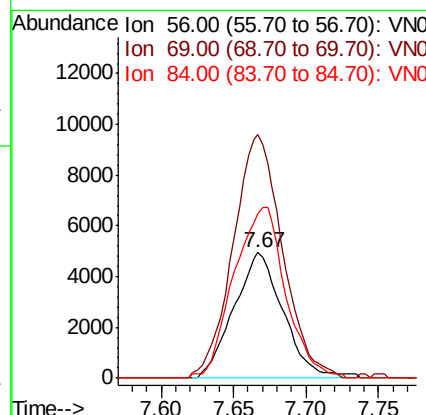





#33
 1,2-Dichloroethane-d4
 Concen: 54.185 ug/l
 RT: 8.03 min Scan# 2003
 Delta R.T. 0.00 min
 Lab File: VN050606.D
 Acq: 14 Aug 2018 16:50




Instrument :
 MSVOA_N
 ClientSampleId :
 RB47197


Tgt Ion: 65 Resp: 441994
 Ion Ratio Lower Upper
 65 100
 67 54.3 0.0 109.8

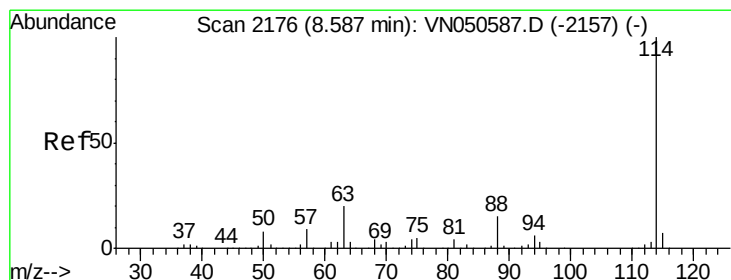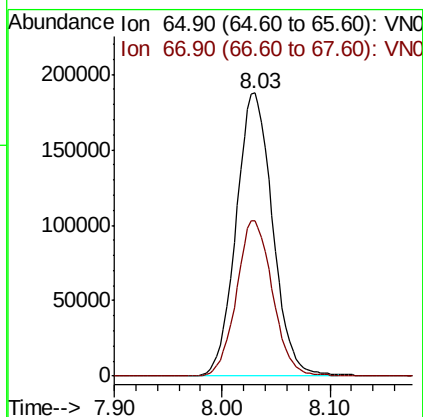

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. -0.00 min
 Lab File: VN050606.D
 Acq: 14 Aug 2018 16:50

Tgt Ion: 114 Resp: 1063528
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 40.0
 88 15.8 0.0 30.8



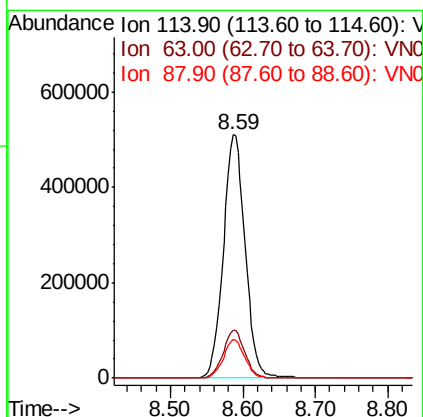
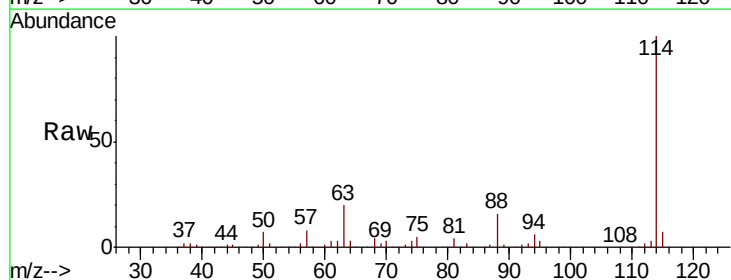




#35
 Dibromofluoromethane
 Concen: 48.306 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: VN050606.D
 Acq: 14 Aug 2018 16:50




Instrument :
 MSVOA_N
 ClientSampleId :
 RB47197


Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.0	81.0	121.6
192	22.3	17.6	26.4

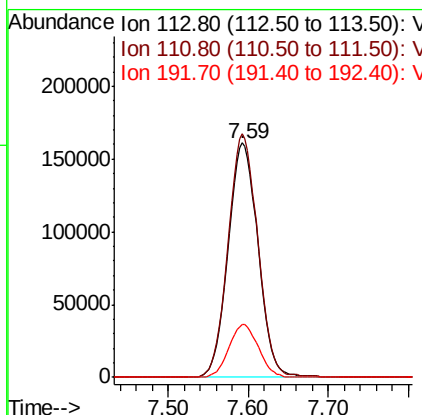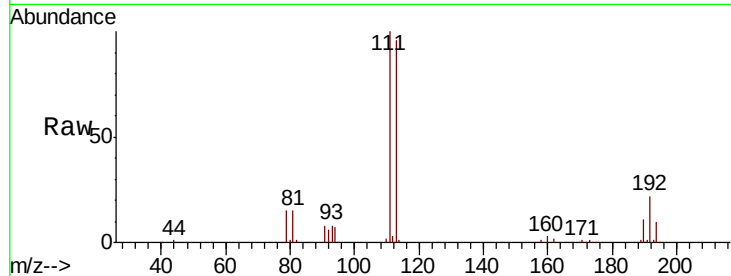

#36
 1,1-Dichloropropene
 Concen: 3.762 ug/l
 RT: 7.67 min Scan# 1891
 Delta R.T. -0.12 min
 Lab File: VN050606.D
 Acq: 14 Aug 2018 16:50

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.5	18.3	54.9#
77	0.0	25.0	37.4#

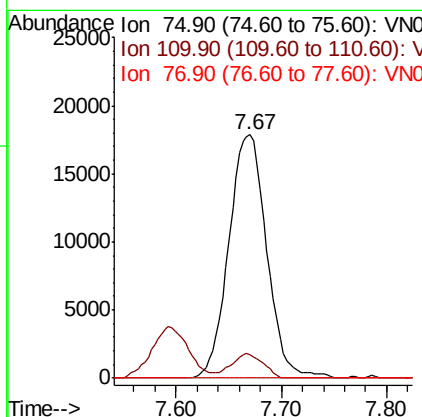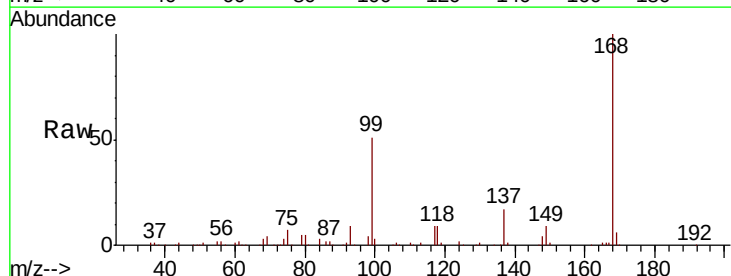



#38

Carbon Tetrachloride

Concen: 4.637 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. -0.11 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampleId :

RB47197


Tgt Ion: 117 Resp: 56946

Ion Ratio Lower Upper

117 100

119 6.4 76.6 115.0#




121 0.0 25.0 37.6#

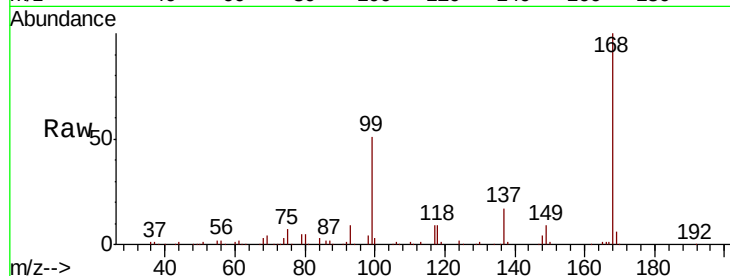

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

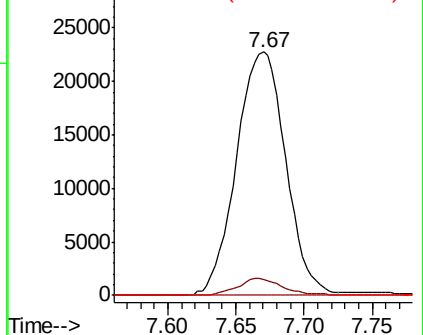

#43

Isopropyl Acetate

Concen: 15.827 ug/l

RT: 8.17 min Scan# 2046

Delta R.T. 0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50


Tgt Ion: 43 Resp: 193019

Ion Ratio Lower Upper

43 100

61 19.1 16.2 24.2



87 12.2 10.9 16.3




Abundance Ion 43.00 (42.70 to 43.70): V

Ion 61.00 (60.70 to 61.70): V

Ion 87.00 (86.70 to 87.70): V

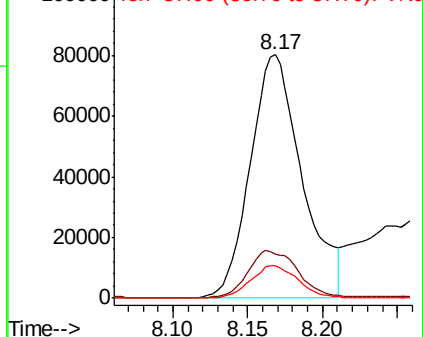



#47

Bromodichloromethane

Concen: 0.289 ug/l

RT: 9.41 min Scan# 2431

Delta R.T. 0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampled :

RB47197


Tgt Ion: 83 Resp: 3499

Ion Ratio Lower Upper

83 100

85 53.9 51.8 77.6




127 7.6 7.2 10.8

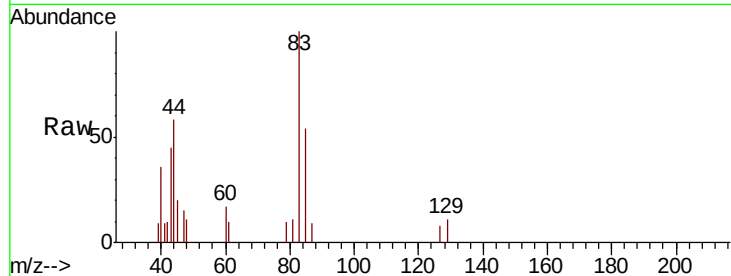

Abundance Ion 82.90 (82.60 to 83.60): VN050587.D (-2413) (-)

Ion 84.90 (84.60 to 85.60): VN050587.D (-2413) (-)

Ion 126.80 (126.50 to 127.50): VN050587.D (-2413) (-)

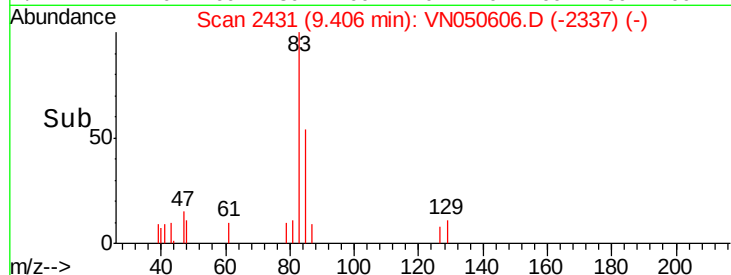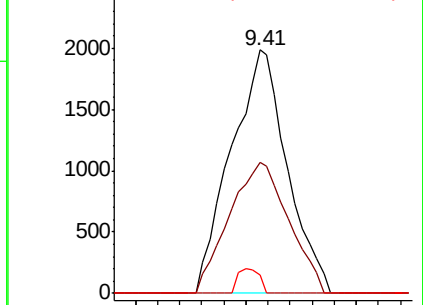

#48

Methyl methacrylate

Concen: 1.015 ug/l

RT: 9.18 min Scan# 2360

Delta R.T. -0.02 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50


Tgt Ion: 41 Resp: 6228

Ion Ratio Lower Upper

41 100

69 0.0 73.4 110.0#



39 17.0 43.0 64.6#




Abundance Ion 41.00 (40.70 to 41.70): VN050587.D (-2355) (-)

Ion 69.00 (68.70 to 69.70): VN050587.D (-2355) (-)

Ion 39.00 (38.70 to 39.70): VN050587.D (-2355) (-)




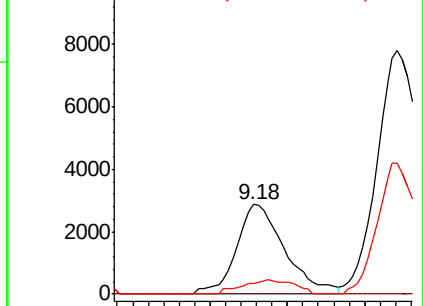




#50
Toluene-d8
Concen: 45.562 ug/l
RT: 10.09 min Scan# 2644
Delta R.T. -0.00 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50




Instrument :
MSVOA_N
ClientSampled :
RB47197


Tgt Ion: 98 Resp: 1455963
Ion Ratio Lower Upper
98 100
100 63.1 51.8 77.8

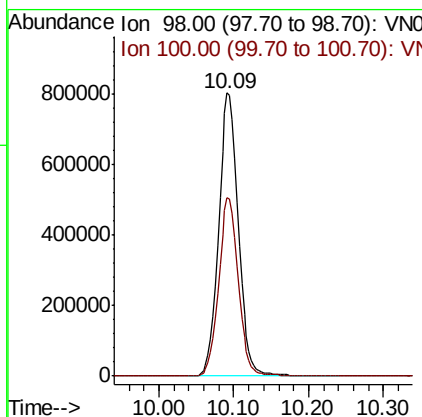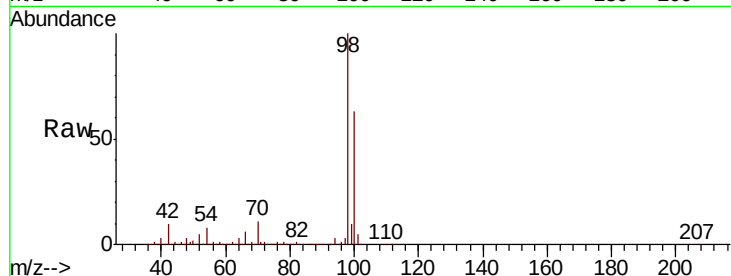

#56
Ethyl methacrylate
Concen: 1.945 ug/l
RT: 10.23 min Scan# 2688
Delta R.T. -0.20 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50

Tgt Ion: 69 Resp: 429
Ion Ratio Lower Upper
69 100
41 0.0 49.7 74.5#
39 68.3 24.2 36.2#

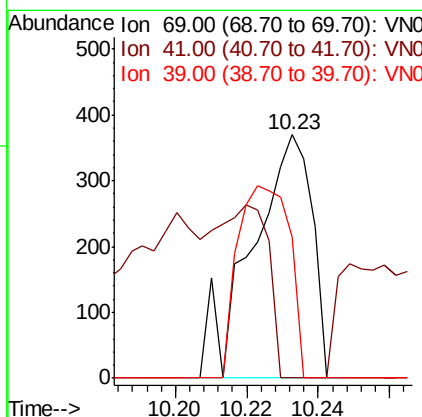



#59

2-Hexanone

Concen: 1.031 ug/l

RT: 10.77 min Scan# 2854

Delta R.T. 0.01 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampleId :





RB47197

Tgt Ion: 43 Resp: 5488

Ion Ratio Lower Upper

43 100

58 27.2 28.0 84.0#

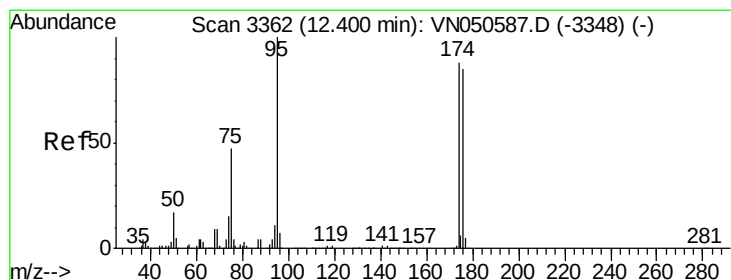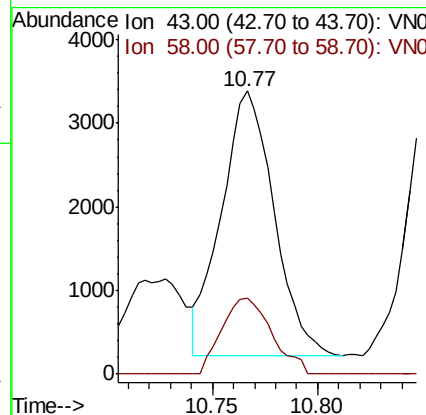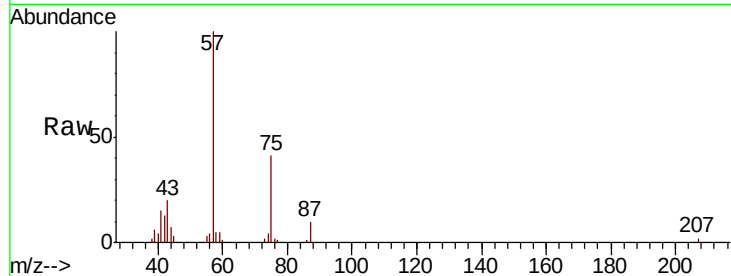

#62

4-Bromofluorobenzene

Concen: 38.030 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50




Tgt Ion: 95 Resp: 401482


Ion Ratio Lower Upper

95 100

174 91.2 0.0 177.8

176 87.8 0.0 175.0



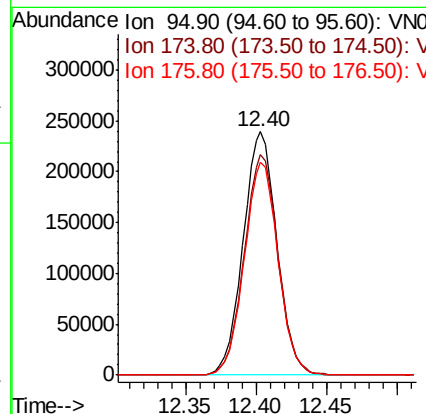





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. -0.00 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50




Instrument :
MSVOA_N
ClientSampleId :
RB47197


Tgt Ion:117 Resp: 889053
Ion Ratio Lower Upper
117 100
82 54.0 42.4 63.6
119 32.4 25.8 38.8

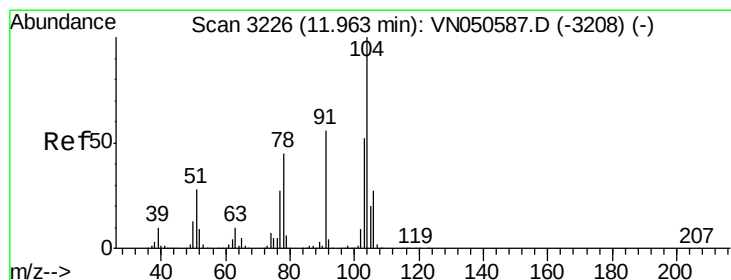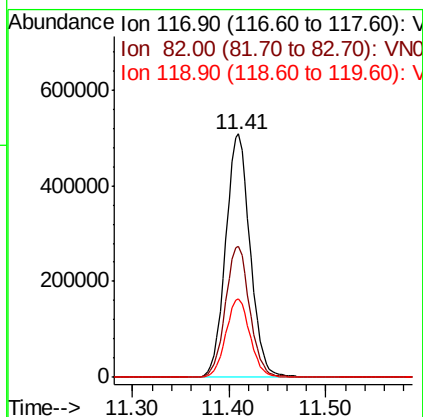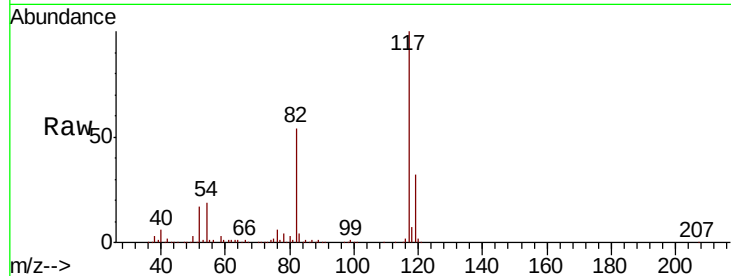

#70
Styrene
Concen: 0.942 ug/l
RT: 11.96 min Scan# 3226
Delta R.T. 0.00 min
Lab File: VN050606.D
Acq: 14 Aug 2018 16:50

Tgt Ion:104 Resp: 30
Ion Ratio Lower Upper
104 100
78 0.0 39.1 58.7#
103 0.0 44.9 67.3#

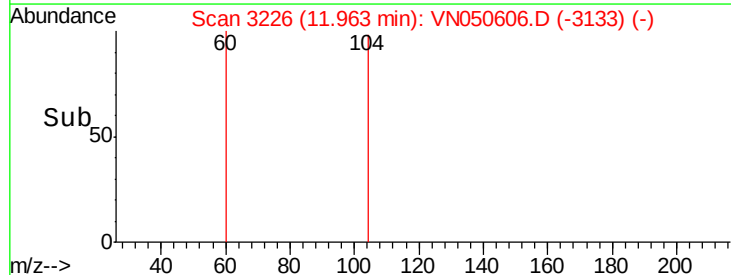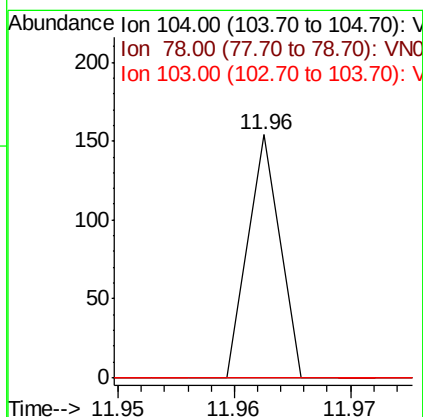



#71

Bromoform

Concen: 0.301 ug/l

RT: 12.40 min Scan# 3361

Delta R.T. 0.27 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampleId :

RB47197


Tgt Ion:173 Resp: 1654

Ion Ratio Lower Upper

173 100

175 0.0 24.4 73.2#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

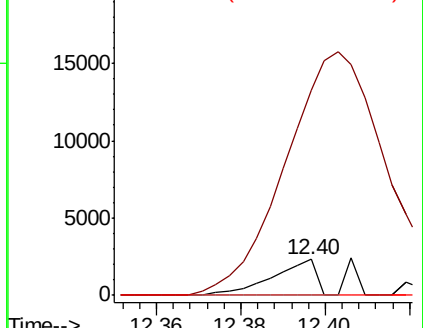

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. -0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50


Tgt Ion:152 Resp: 335355

Ion Ratio Lower Upper

152 100

115 56.6 28.1 84.2



150 157.2 0.0 347.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

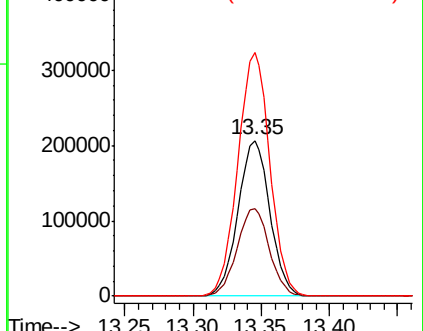

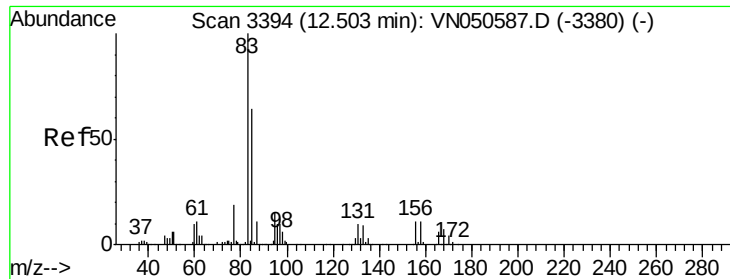

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.41 min Scan# 3364

Delta R.T. -0.10 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampleId :

RB47197


Tgt Ion: 83 Resp: 99

Ion Ratio Lower Upper

83 100

131 354.5 5.3 15.9#




85 0.0 32.1 96.5#

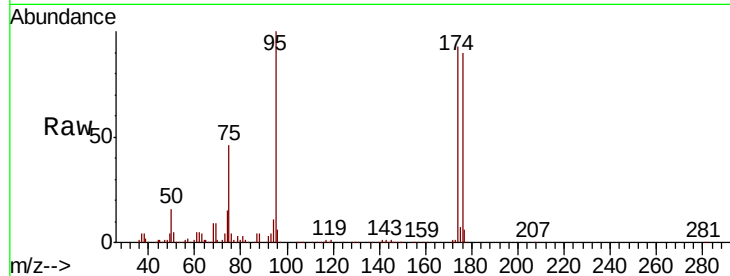

Abundance Ion 82.90 (82.60 to 83.60): VN0

Ion 130.80 (130.50 to 131.50): VN0

Ion 84.90 (84.60 to 85.60): VN0

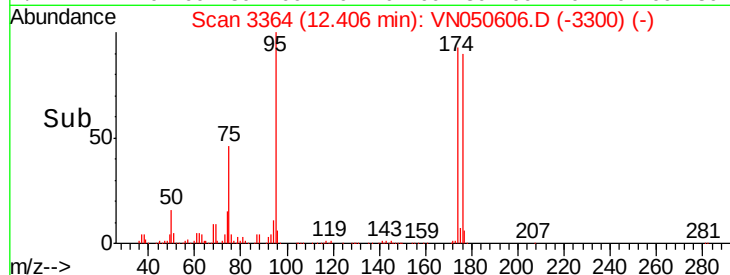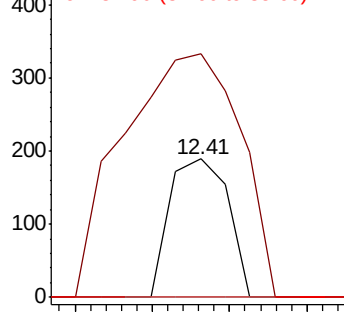

#76

1,2,3-Trichloropropane

Concen: 34.667 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050606.D


Acq: 14 Aug 2018 16:50

Tgt Ion: 75 Resp: 189540

Ion Ratio Lower Upper



75 100


77 1.4 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

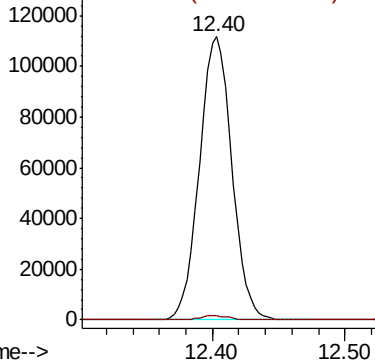



#81

trans-1,4-Dichloro-2-butene

Concen: 125.654 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.10 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Instrument :

MSVOA_N

ClientSampled :

RB47197


Tgt Ion: 75 Resp: 189540

Ion Ratio Lower Upper

75 100

53 0.2 72.2 108.2#




89 0.0 36.3 54.5#

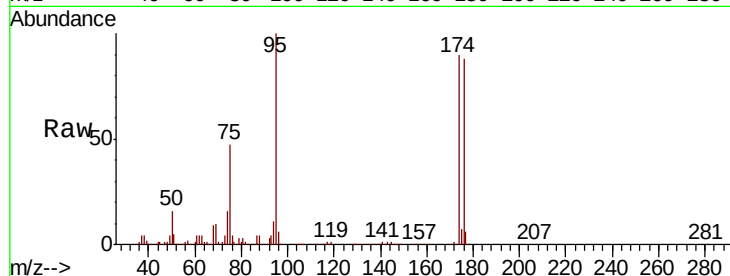

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

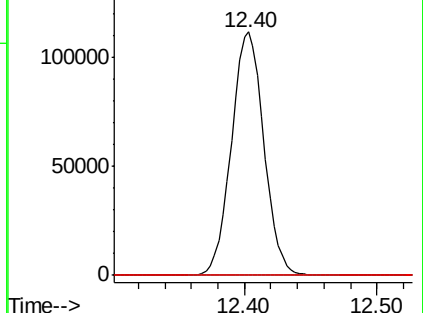

#90

Hexachloroethane

Concen: 0.205 ug/l

RT: 13.99 min Scan# 3858

Delta R.T. 0.12 min

Lab File: VN050606.D


Acq: 14 Aug 2018 16:50

Tgt Ion: 117 Resp: 830

Ion Ratio Lower Upper



117 100


201 0.0 45.5 136.5#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

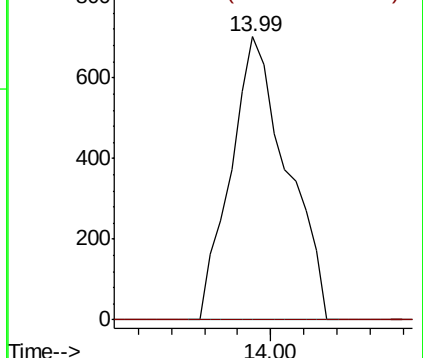



#93

1,2,4-Trichlorobenzene

Concen: 2.684 ug/l

RT: 14.90 min Scan# 4140

Delta R.T. -0.01 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50


Instrument :

MSVOA_N

ClientSampleId :

RB47197

Tgt Ion:	180	Resp:	66
Ion	Ratio	Lower	Upper
180	100		
182	0.0	47.9	143.7#
145	0.0	14.4	43.4#



Abundance Ion 179.80 (179.50 to 180.50): V


Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V


14.90

14.89

14.91



Time-->



#95

Naphthalene

Concen: 4.177 ug/l


RT: 15.13 min Scan# 4212

Delta R.T. 0.00 min

Lab File: VN050606.D

Acq: 14 Aug 2018 16:50

Tgt Ion:	128	Resp:	4423
Ion	Ratio	Lower	Upper
128	100		
127	6.9	10.3	15.5#
129	9.7	8.5	12.7



Abundance Ion 128.00 (127.70 to 128.70): V


Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

15.13

15.10

15.15



Time-->