

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081418\
 Data File : VN050611.D
 Acq On : 14 Aug 2018 18:53
 Operator : MD\SY
 Sample : J4469-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 958-IW-15(19)

Quant Time: Aug 15 07:09:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	714105	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1101270	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	940280	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	337662	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	455830	50.64	ug/l	0.00
Spiked Amount			Recovery	=	101.28%	
35) Dibromofluoromethane	7.59	113	432646	49.21	ug/l	0.00
Spiked Amount			Recovery	=	98.42%	
50) Toluene-d8	10.09	98	1520125	45.94	ug/l	0.00
Spiked Amount			Recovery	=	91.88%	
62) 4-Bromofluorobenzene	12.40	95	407827	37.31	ug/l	0.00
Spiked Amount			Recovery	=	74.62%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	3121	Below Cal		94
5) Bromomethane	2.57	94	2838	Below Cal		94
6) Chloroethane	2.69	64	164	Below Cal	#	43
10) Methyl Iodide	3.95	142	1036	7.097	ug/l #	88
16) Acetone	3.82	43	13940	4.780	ug/l	92
20) Methylene Chloride	4.56	84	896	Below Cal	#	78
21) trans-1,2-Dichloroethene	5.05	96	12943	1.541	ug/l	96
25) 2-Butanone	6.84	43	1293	0.350	ug/l #	8
27) cis-1,2-Dichloroethene	6.83	96	316586	33.845	ug/l	92
29) Tetrahydrofuran	7.22	42	923	0.479	ug/l #	47
31) Cyclohexane	7.67	56	13252	0.630	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	48100	3.924	ug/l #	49
38) Carbon Tetrachloride	7.67	117	62793	4.938	ug/l #	17
39) Methylcyclohexane	8.84	83	3588	0.283	ug/l #	1
43) Isopropyl Acetate	8.26	43	38531	3.051	ug/l #	60
44) Trichloroethene	8.84	130	285462	28.575	ug/l	98
48) Methyl methacrylate	9.44	41	1989	0.313	ug/l #	22
55) 1,1,2-Trichloroethane	10.63	97	5589	0.672	ug/l #	1
60) Dibromochloromethane	10.63	129	667087	72.660	ug/l #	10
64) Tetrachloroethene	10.63	164	782501	89.611	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.40	83	223	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	196842	35.790	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	196842	129.603	ug/l #	13
95) Naphthalene	15.14	128	716	3.912	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081418\
Data File : VN050611.D
Acq On : 14 Aug 2018 18:53
Operator : MD\SY
Sample : J4469-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
958-IW-15(19)

Quant Time: Aug 15 07:09:45 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration

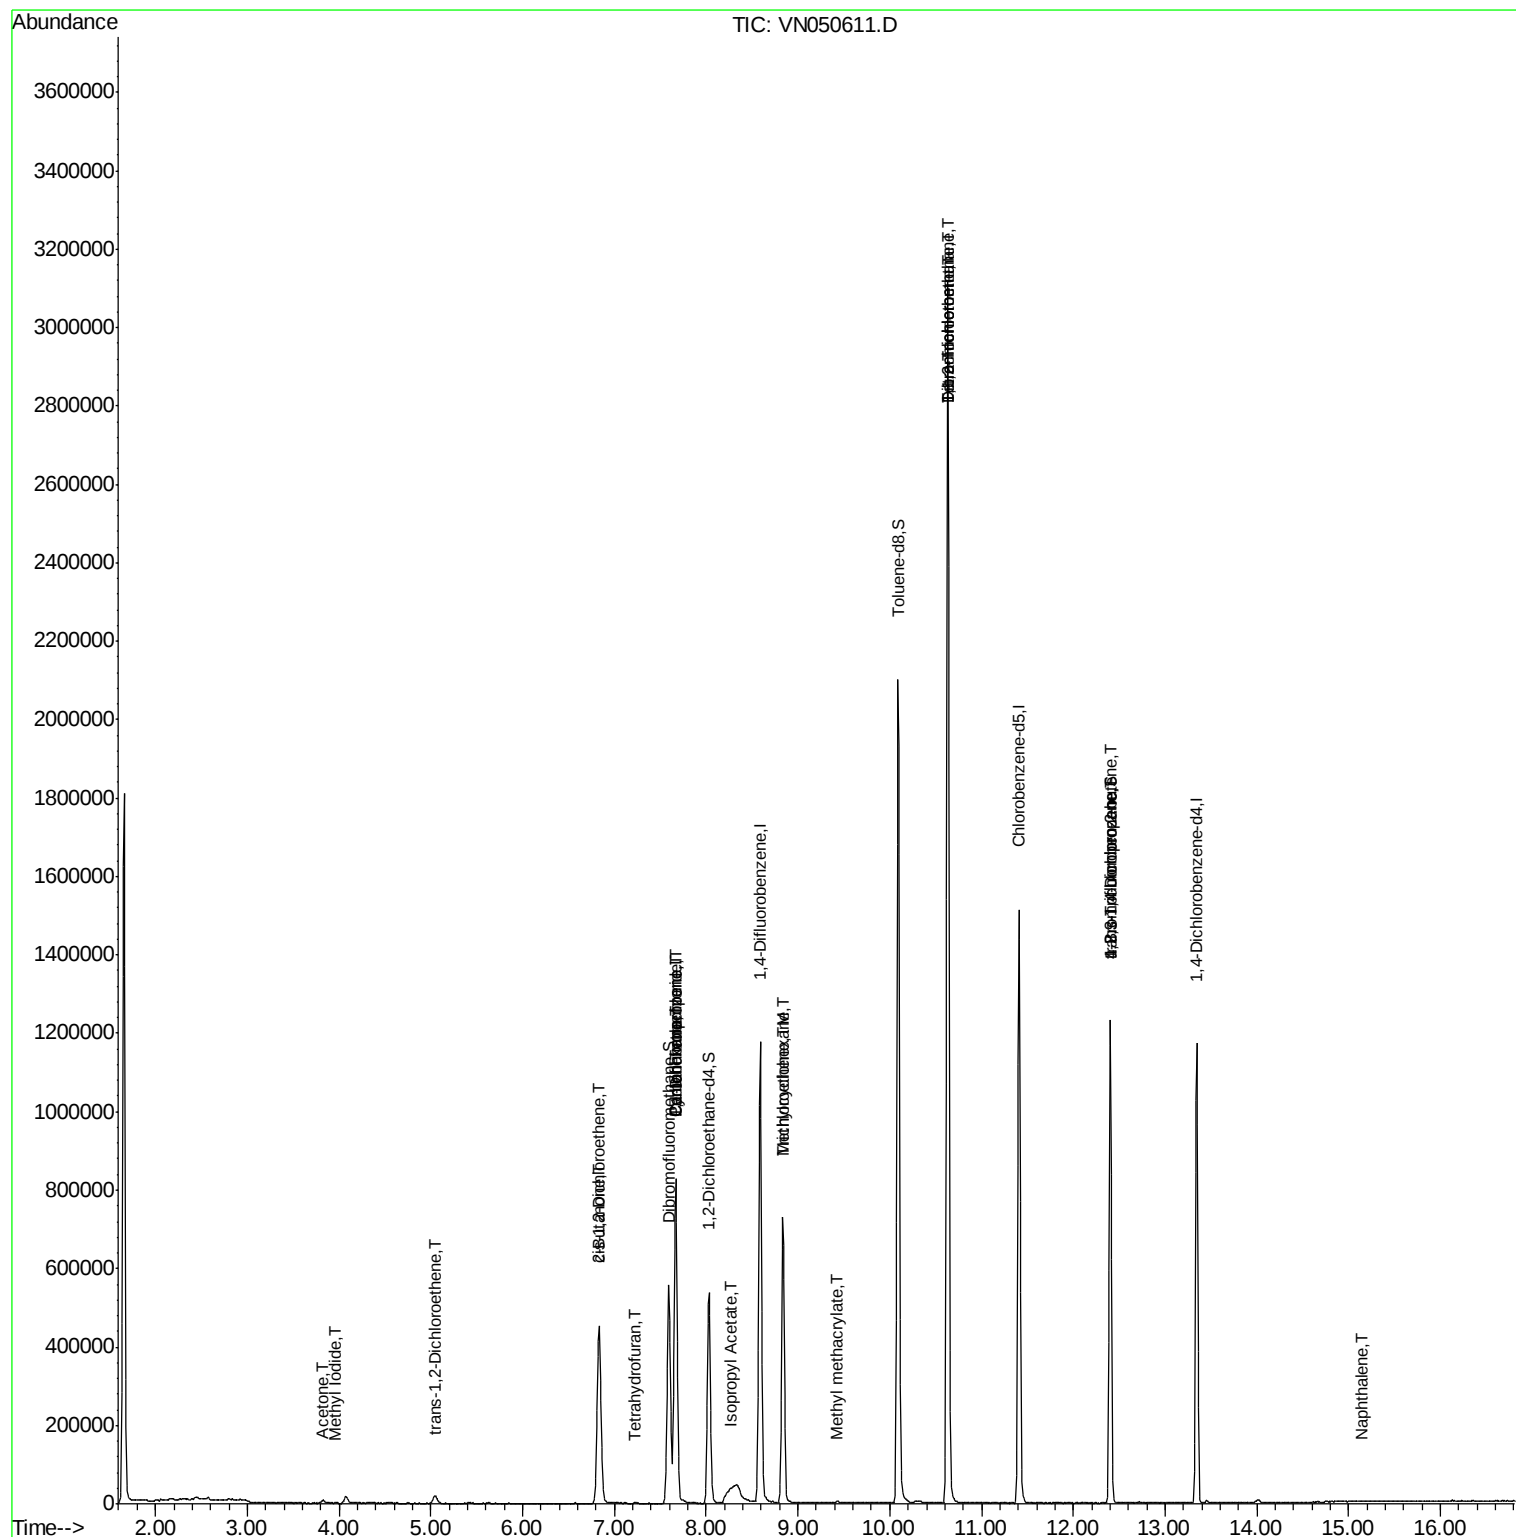

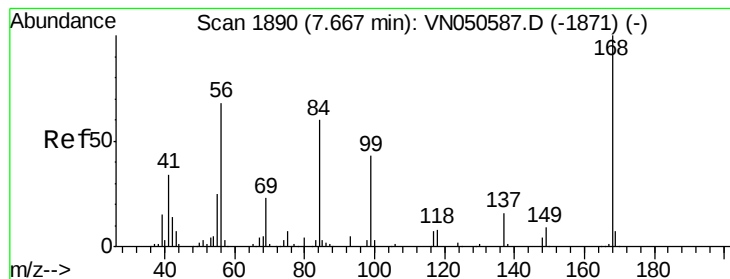

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :


958-IW-15(19)

Tgt Ion:168 Resp: 714105

Ion Ratio Lower Upper

168 100

99 50.4 40.8 61.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.67



300000

200000

100000

0

Time--> 7.50 7.60 7.70 7.80

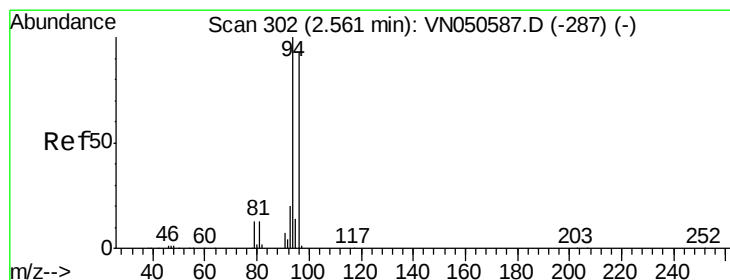

#5

Bromomethane

Concen: Below Cal

RT: 2.57 min Scan# 305

Delta R.T. 0.01 min

Lab File: VN050611.D


Acq: 14 Aug 2018 18:53

Tgt Ion: 94 Resp: 2838

Ion Ratio Lower Upper

94 100

96 98.3 74.0 111.0



Abundance Ion 93.90 (93.60 to 94.60): VN

Ion 95.90 (95.60 to 96.60): VN

2000


1500


1000

500

0

Time--> 2.50 2.55 2.60





#6

Chloroethane

Concen: Below Cal

RT: 2.69 min Scan# 343

Delta R.T. -0.01 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :


958-IW-15(19)

Tgt Ion: 64 Resp: 164

Ion Ratio Lower Upper




64 100

66 0.0 25.7 38.5#

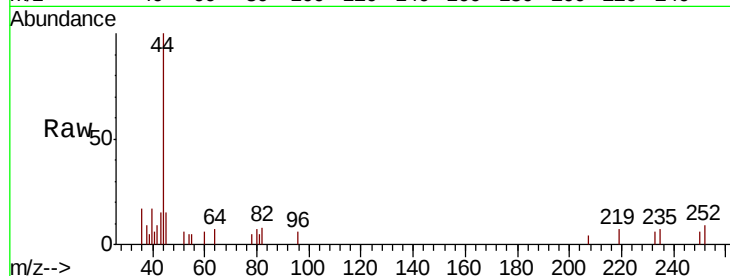

Abundance Ion 63.90 (63.60 to 64.60): VN050587.D (-329) (-)

Ion 65.90 (65.60 to 66.60): VN050587.D (-329) (-)

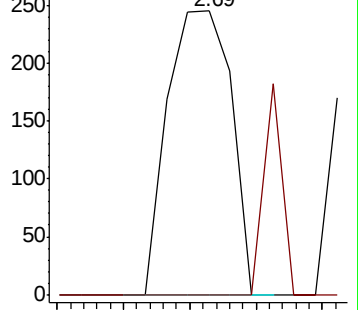

#10

Methyl Iodide

Concen: 7.097 ug/l

RT: 3.95 min Scan# 733

Delta R.T. -0.01 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53


Tgt Ion: 142 Resp: 1036

Ion Ratio Lower Upper

142 100

127 38.3 32.6 49.0



141 0.0 11.5 17.3#




Abundance Ion 141.80 (141.50 to 142.50): VN050587.D (-713) (-)

Ion 126.80 (126.50 to 127.50): VN050587.D (-713) (-)

Ion 140.80 (140.50 to 141.50): VN050587.D (-713) (-)

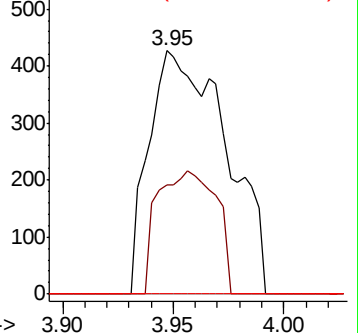



#16

Acetone

Concen: 4.780 ug/l

RT: 3.82 min Scan# 694

Delta R.T. 0.00 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampled :


958-IW-15(19)

Tgt Ion: 43 Resp: 13940

Ion Ratio Lower Upper




43 100

58 29.0 27.1 40.7



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

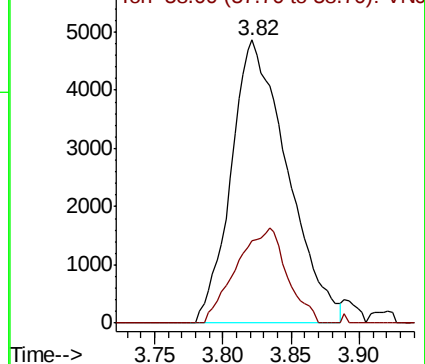

#20

Methylene Chloride

Concen: Below Cal

RT: 4.56 min Scan# 923

Delta R.T. 0.01 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Tgt Ion: 84 Resp: 896


Ion Ratio Lower Upper

84 100

49 95.9 92.6 138.8

51 28.7 28.6 43.0

86 39.4 52.2 78.2#






Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO

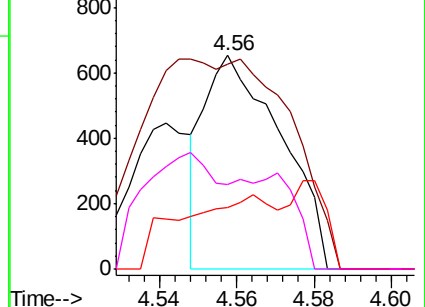



#21

trans-1,2-Dichloroethene

Concen: 1.541 ug/l

RT: 5.05 min Scan# 1076

Delta R.T. 0.01 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

958-IW-15(19)


Tgt Ion: 96 Resp: 12943

Ion Ratio Lower Upper

96 100

61 143.2 111.2 166.8




98 59.8 51.6 77.4

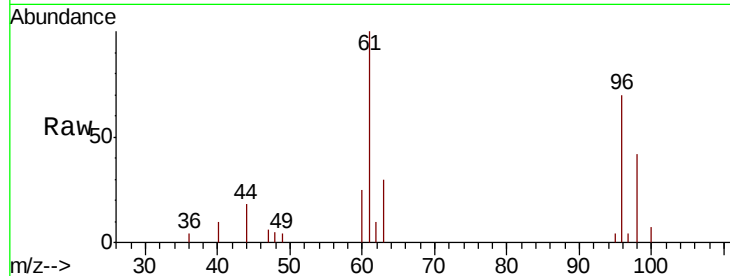

Abundance Ion 95.90 (95.60 to 96.60): VN050611.D (-1540) (-)

Ion 60.90 (60.60 to 61.60): VN050611.D (-1540) (-)

Ion 97.90 (97.60 to 98.60): VN050611.D (-1540) (-)

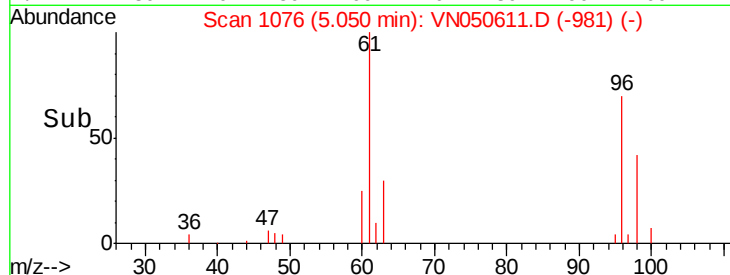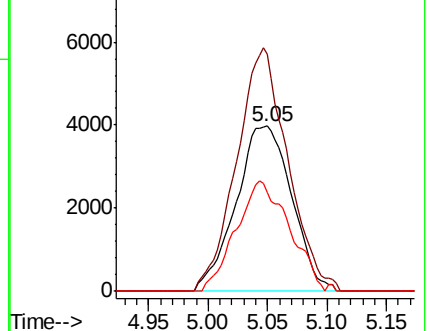

#25

2-Butanone

Concen: 0.350 ug/l

RT: 6.84 min Scan# 1632

Delta R.T. -0.00 min

Lab File: VN050611.D


Acq: 14 Aug 2018 18:53

Tgt Ion: 43 Resp: 1293

Ion Ratio Lower Upper



43 100


72 74.9 21.8 32.6#

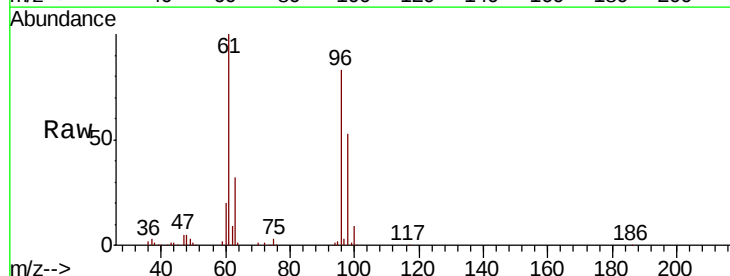

Abundance Ion 43.00 (42.70 to 43.70): VN050611.D (-1540) (-)

Ion 72.00 (71.70 to 72.70): VN050611.D (-1540) (-)




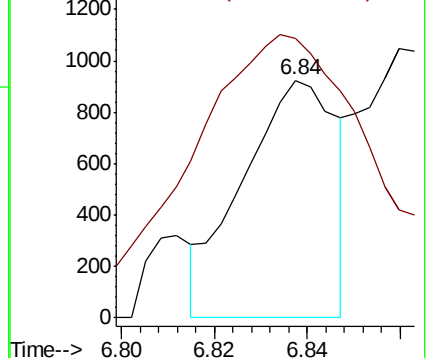




#27
 cis-1,2-Dichloroethene
 Concen: 33.845 ug/l
 RT: 6.83 min Scan# 1631
 Delta R.T. 0.00 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53




Instrument :
 MSVOA_N
 ClientSampleId :
 958-IW-15(19)


Tgt Ion: 96 Resp: 316586
 Ion Ratio Lower Upper
 96 100
 61 124.7 0.0 278.2
 98 64.4 0.0 128.8

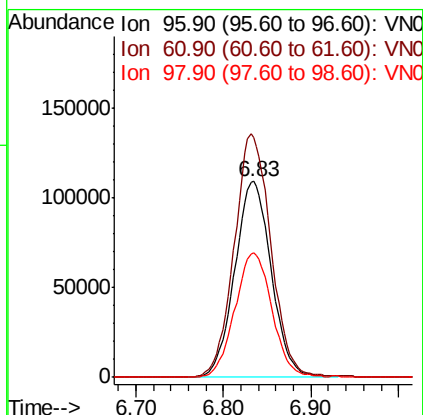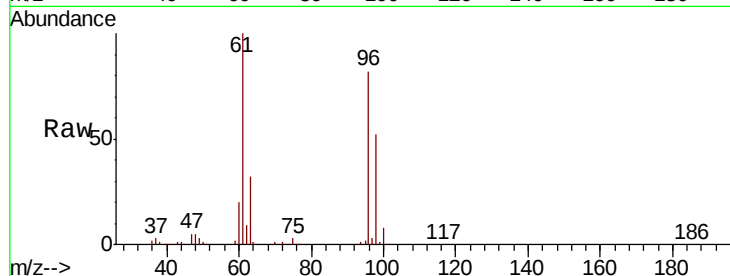

#29
 Tetrahydrofuran
 Concen: 0.479 ug/l
 RT: 7.22 min Scan# 1751
 Delta R.T. 0.01 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53

Tgt Ion: 42 Resp: 923
 Ion Ratio Lower Upper
 42 100
 72 7.3 35.8 53.6#
 71 11.8 33.4 50.0#

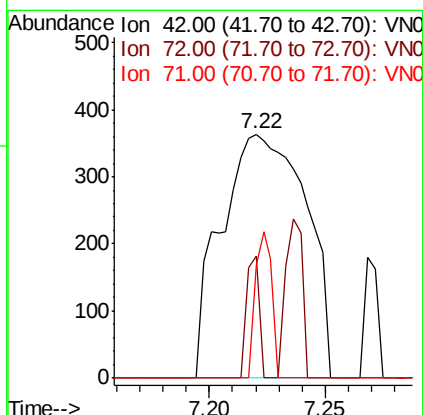

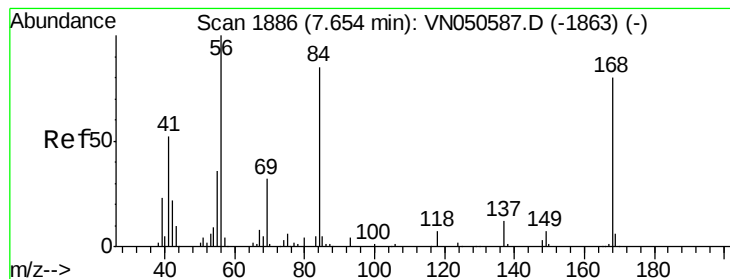

#31

Cyclohexane

Concen: 0.630 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. 0.01 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

958-IW-15(19)


Tgt Ion: 56 Resp: 13252

Ion Ratio Lower Upper

56 100

69 191.5 25.8 38.6#




84 154.1 67.8 101.6#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

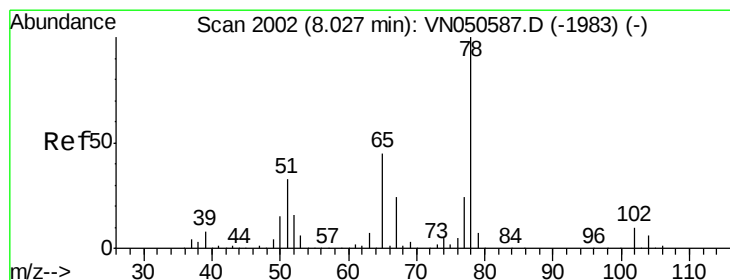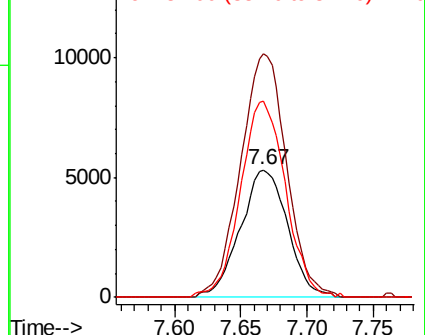

#33

1,2-Dichloroethane-d4

Concen: 50.640 ug/l

RT: 8.03 min Scan# 2003

Delta R.T. 0.00 min

Lab File: VN050611.D


Acq: 14 Aug 2018 18:53

Tgt Ion: 65 Resp: 455830

Ion Ratio Lower Upper



65 100


67 53.7 0.0 109.8



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0




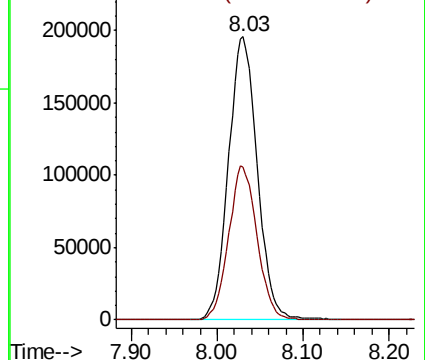


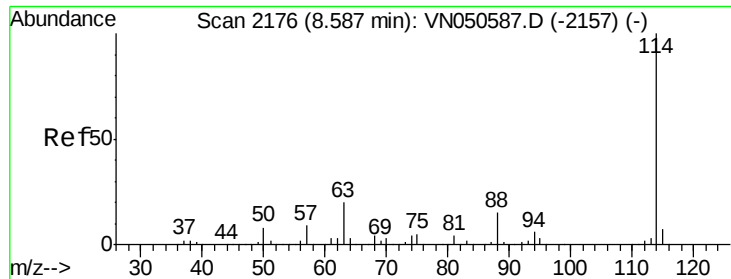

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53




Instrument :
 MSVOA_N
 ClientSampleId :
 958-IW-15(19)


Tgt Ion:114 Resp: 1101270
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 40.0
 88 15.6 0.0 30.8

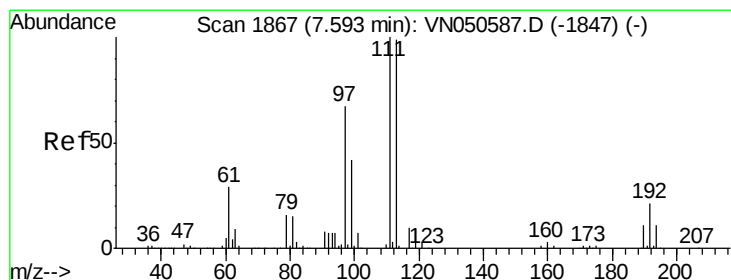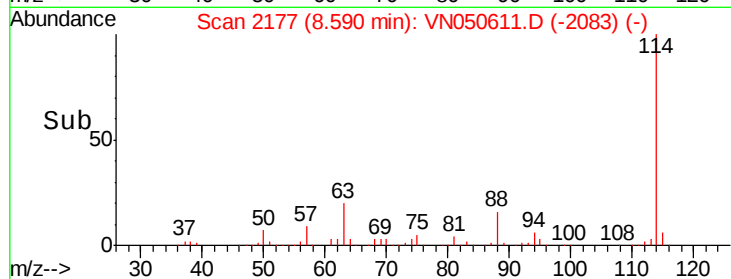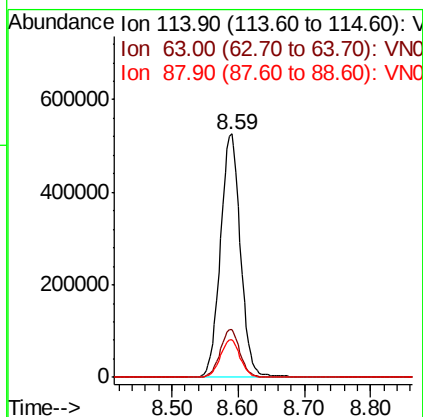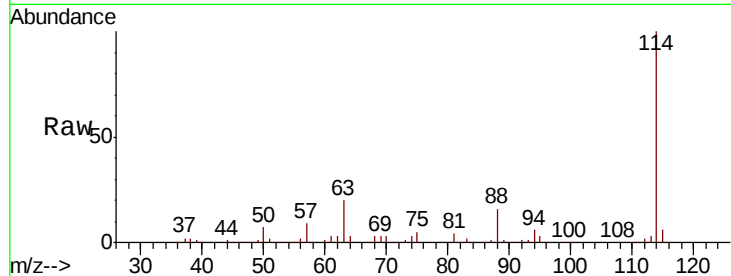

#35
 Dibromofluoromethane
 Concen: 49.208 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53

Tgt Ion:113 Resp: 432646
 Ion Ratio Lower Upper
 113 100
 111 101.9 81.0 121.6
 192 22.0 17.6 26.4


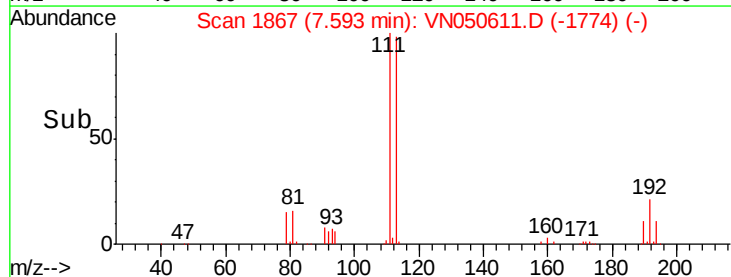
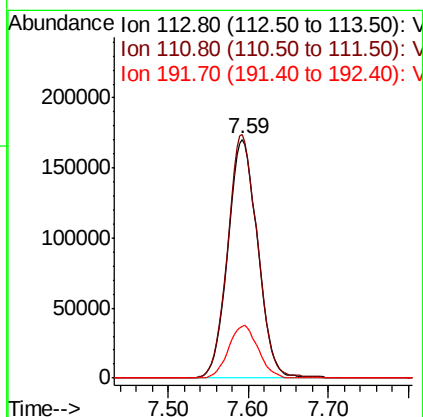
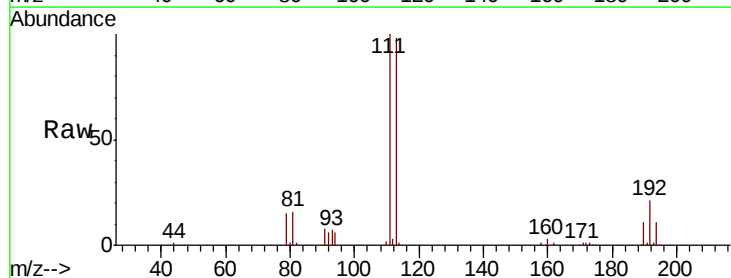


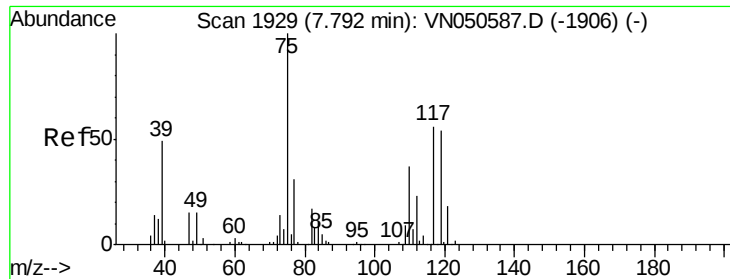

#36
 1,1-Dichloropropene
 Concen: 3.924 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.13 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53




Instrument :
 MSVOA_N
 ClientSampleId :
 958-IW-15(19)


Tgt Ion: 75 Resp: 48100
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.3 54.9#
 77 0.0 25.0 37.4#

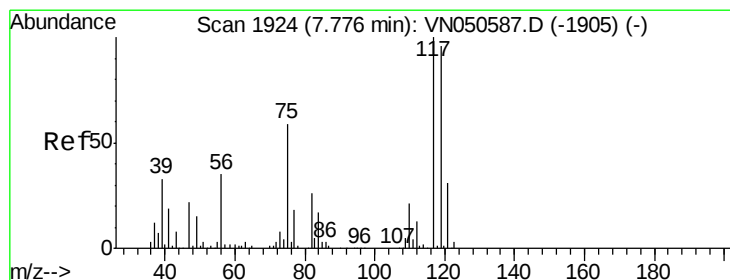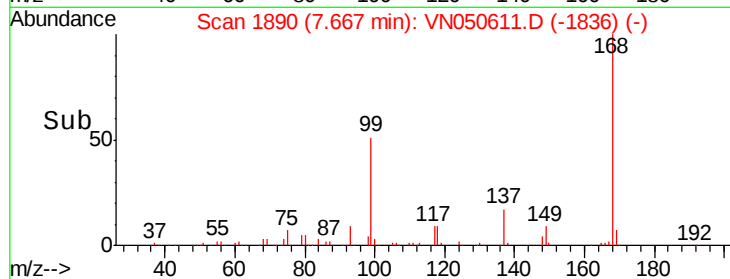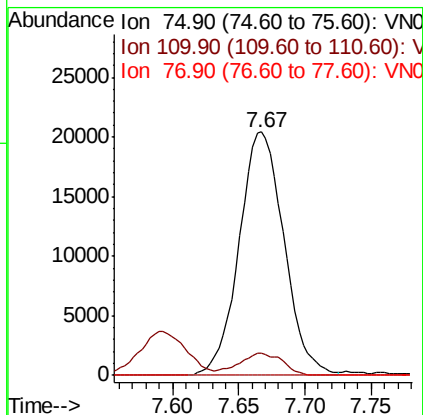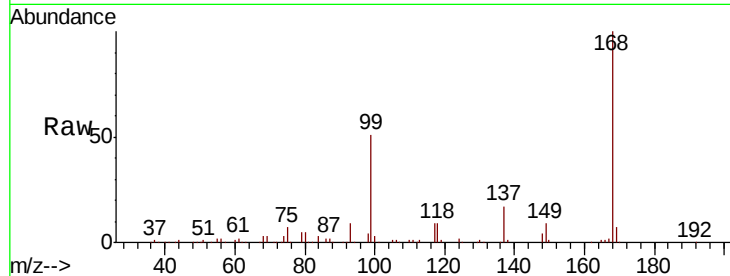

#38
 Carbon Tetrachloride
 Concen: 4.938 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.11 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53

Tgt Ion: 117 Resp: 62793
 Ion Ratio Lower Upper
 117 100
 119 7.0 76.6 115.0#
 121 0.0 25.0 37.6#

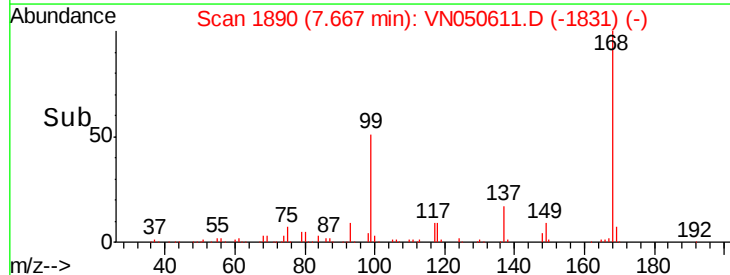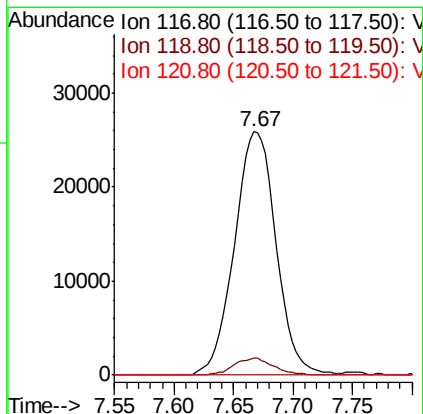


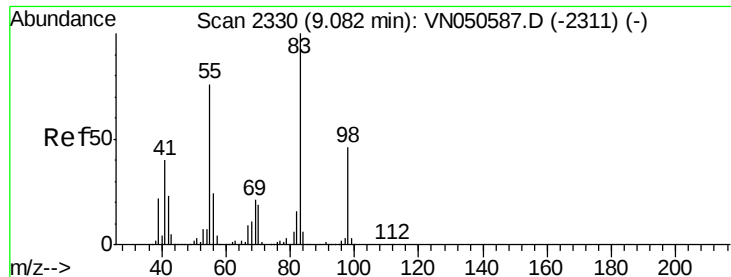




#39
Methylcyclohexane
Concen: 0.283 ug/l
RT: 8.84 min Scan# 2254
Delta R.T. -0.24 min
Lab File: VN050611.D
Acq: 14 Aug 2018 18:53

Instrument :
MSVOA_N
ClientSampleId :
958-IW-15(19)

Tgt Ion: 83 Resp: 3588
Ion Ratio Lower Upper
83 100
55 0.0 60.6 91.0#
98 211.8 37.0 55.4#

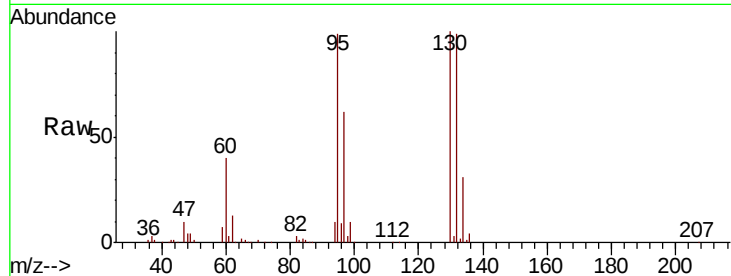


Abundance Ion 83.00 (82.70 to 83.70): VNO
Ion 55.00 (54.70 to 55.70): VNO
Ion 98.00 (97.70 to 98.70): VNO

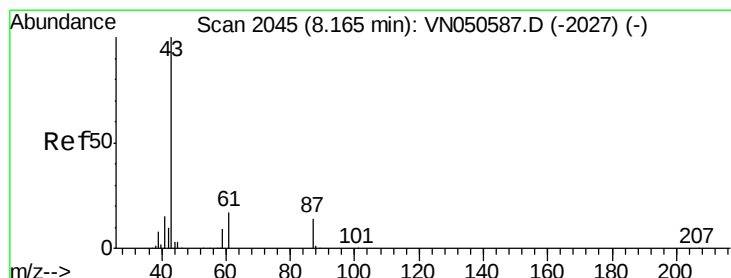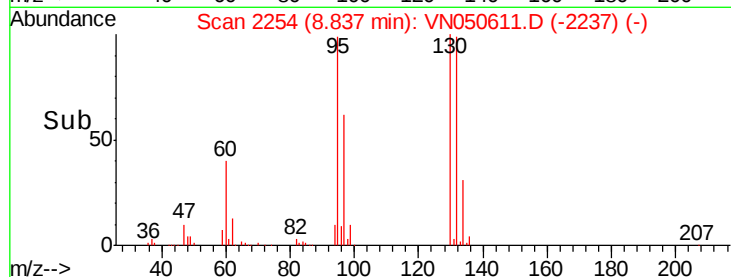
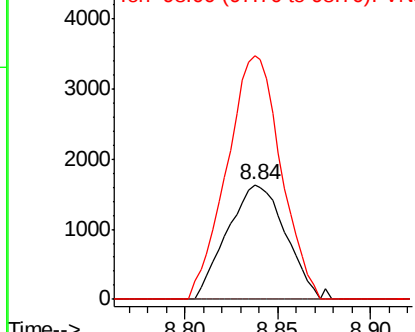



#43
Isopropyl Acetate
Concen: 3.051 ug/l
RT: 8.26 min Scan# 2073
Delta R.T. 0.09 min
Lab File: VN050611.D
Acq: 14 Aug 2018 18:53

Tgt Ion: 43 Resp: 38531
Ion Ratio Lower Upper
43 100
61 0.0 16.2 24.2#
87 0.0 10.9 16.3#

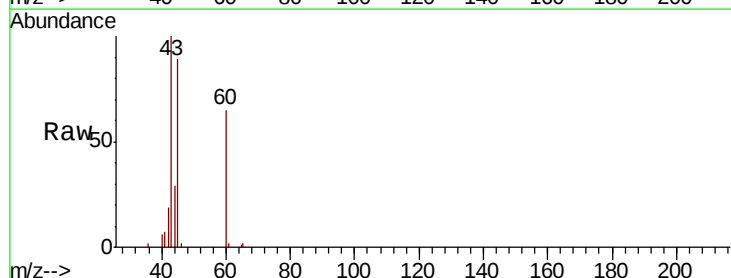

Abundance Ion 43.00 (42.70 to 43.70): VNO
Ion 61.00 (60.70 to 61.70): VNO
Ion 87.00 (86.70 to 87.70): VNO



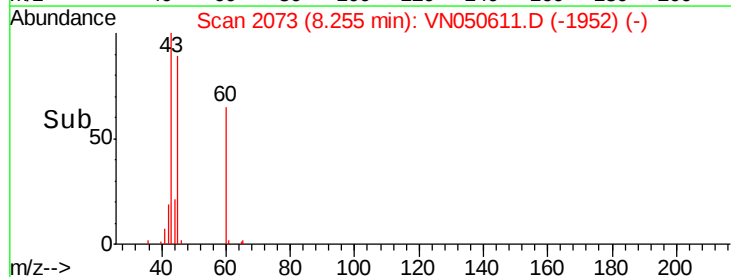
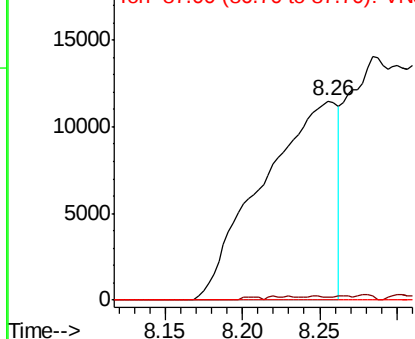


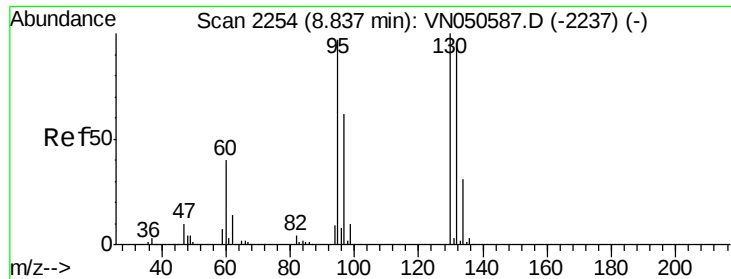

#44
 Trichloroethene
 Concen: 28.575 ug/l
 RT: 8.84 min Scan# 2254
 Delta R.T. 0.00 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53




Instrument :
 MSVOA_N
 ClientSampleId :
 958-IW-15(19)


Tgt Ion: 130 Resp: 285462
 Ion Ratio Lower Upper
 130 100
 95 98.8 0.0 193.8

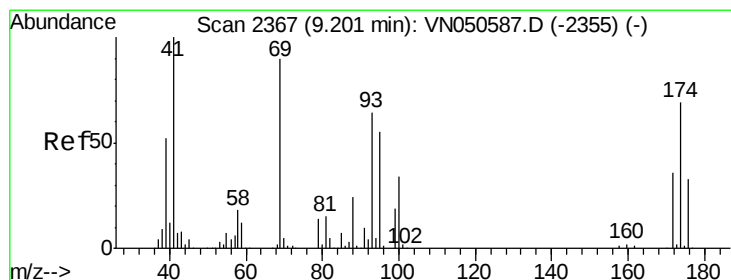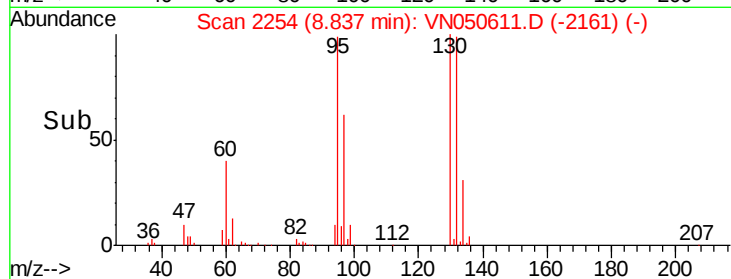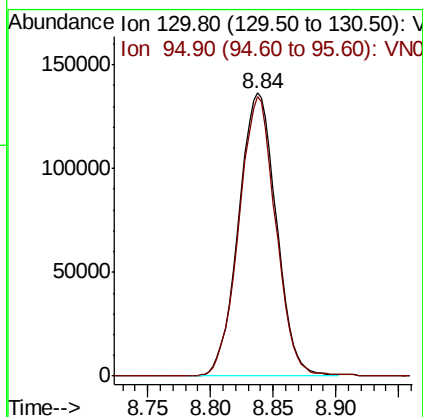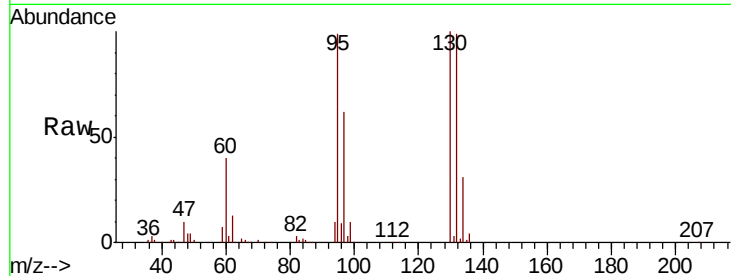

#48
 Methyl methacrylate
 Concen: 0.313 ug/l
 RT: 9.44 min Scan# 2440
 Delta R.T. 0.23 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53

Tgt Ion: 41 Resp: 1989
 Ion Ratio Lower Upper
 41 100
 69 0.0 73.4 110.0#
 39 20.8 43.0 64.6#

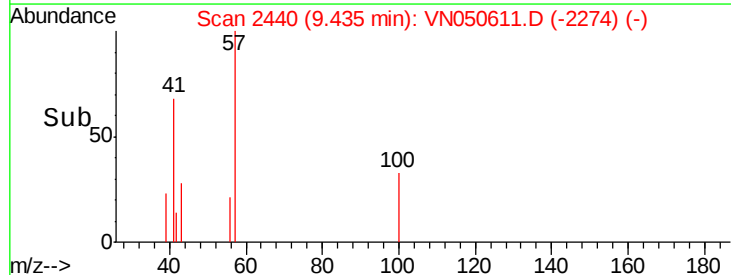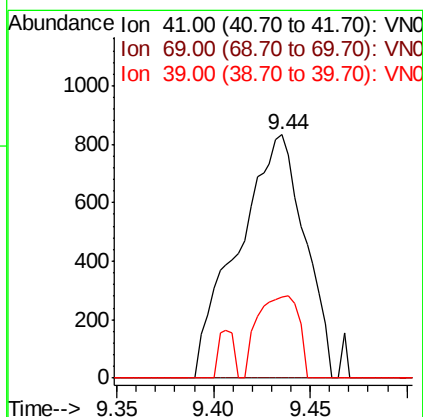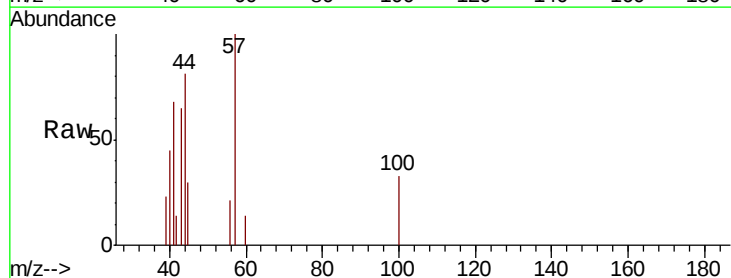

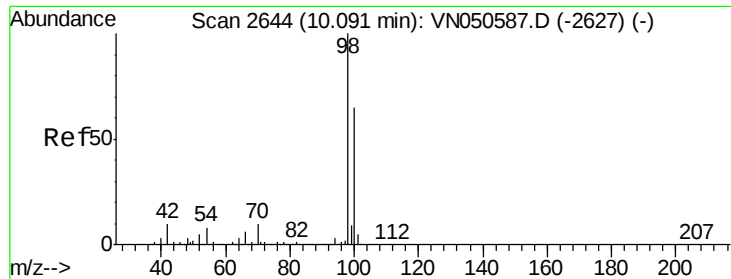

#50

Toluene-d8

Concen: 45.940 ug/l

RT: 10.09 min Scan# 2644

Delta R.T. 0.00 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :


958-IW-15(19)

Tgt Ion: 98 Resp: 1520125

Ion Ratio Lower Upper

98 100

100 63.4 51.8 77.8

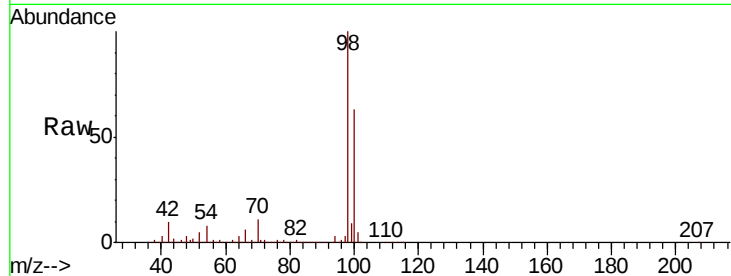

Abundance Ion 98.00 (97.70 to 98.70): VN050587.D (-2627) (-)

Ion 100.00 (99.70 to 100.70): VN050587.D (-2627) (-)

10.09

800000

600000



400000

200000

0

10.00 10.10 10.20

Time-->

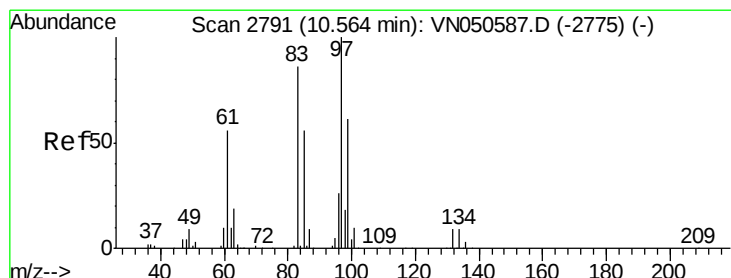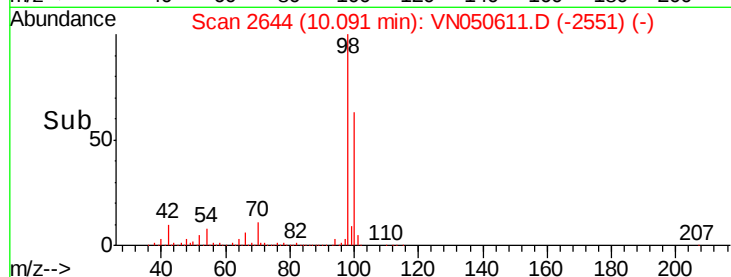

#55

1,1,2-Trichloroethane

Concen: 0.672 ug/l

RT: 10.63 min Scan# 2811

Delta R.T. 0.06 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Tgt Ion: 97 Resp: 5589


Ion Ratio Lower Upper

97 100

83 284.3 68.5 102.7#

85 46.0 44.6 66.8

99 19.3 49.1 73.7#

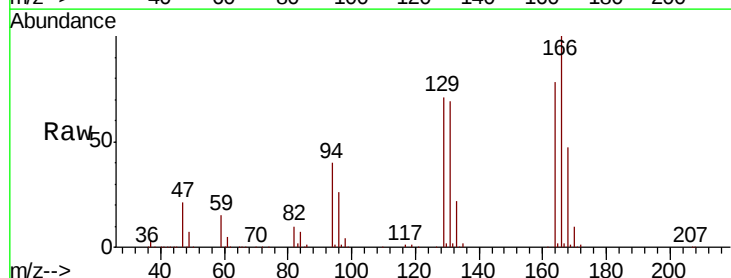

Abundance Ion 96.90 (96.60 to 97.60): VN050587.D (-2775) (-)

Ion 82.90 (82.60 to 83.60): VN050587.D (-2775) (-)

Ion 84.90 (84.60 to 85.60): VN050587.D (-2775) (-)

Ion 98.90 (98.60 to 99.60): VN050587.D (-2775) (-)


10000


5000

0

10.60 10.65

Time-->




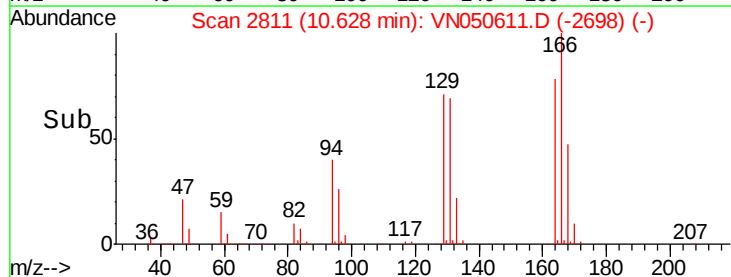


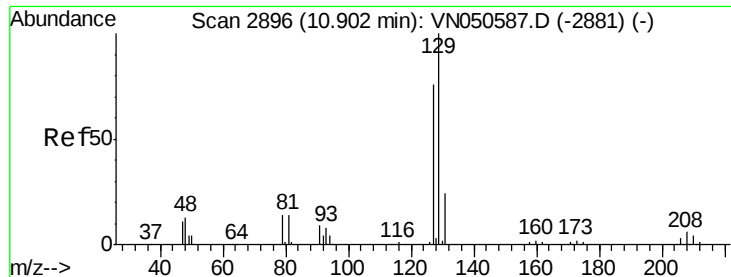

#60
 Dibromochloromethane
 Concen: 72.660 ug/l
 RT: 10.63 min Scan# 2812
 Delta R.T. -0.27 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53




Instrument :
 MSVOA_N
 ClientSampleId :
 958-IW-15(19)


Tgt Ion: 129 Resp: 667087
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.9 116.7#

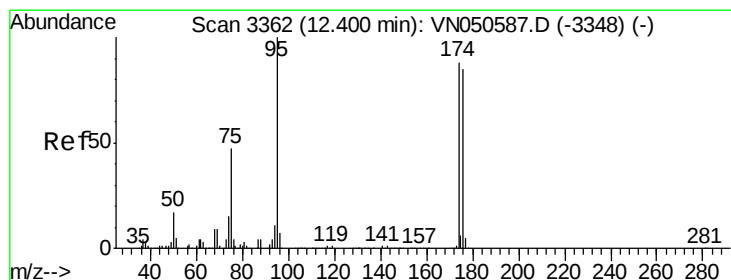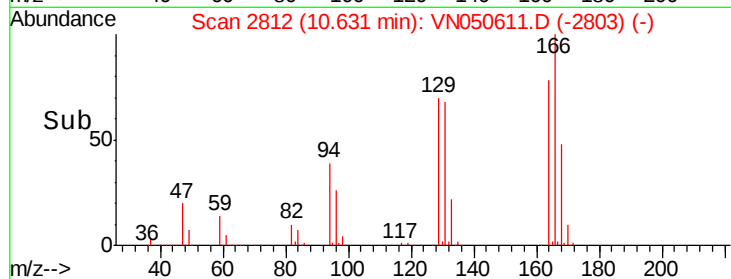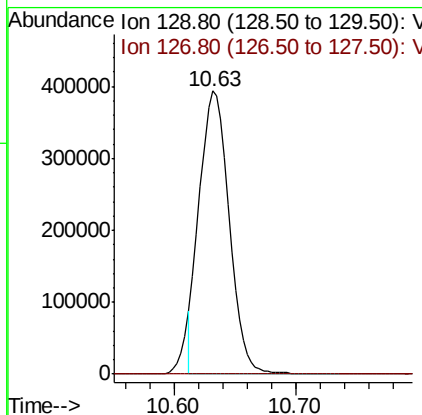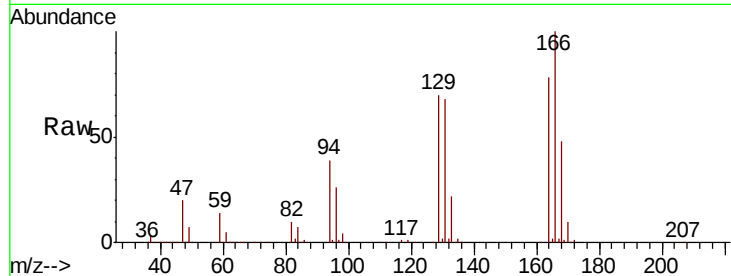

#62
 4-Bromofluorobenzene
 Concen: 37.307 ug/l
 RT: 12.40 min Scan# 3363
 Delta R.T. 0.00 min
 Lab File: VN050611.D
 Acq: 14 Aug 2018 18:53

Tgt Ion: 95 Resp: 407827
 Ion Ratio Lower Upper
 95 100
 174 91.4 0.0 177.8
 176 88.4 0.0 175.0


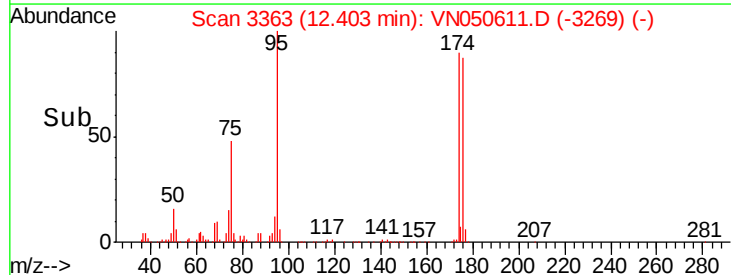
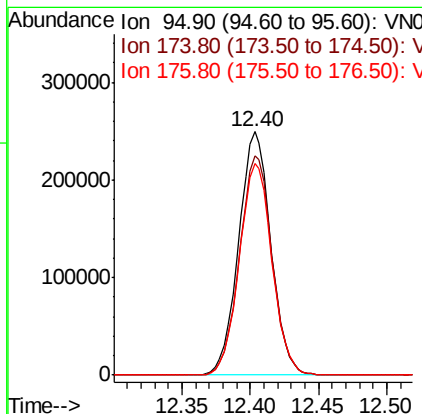
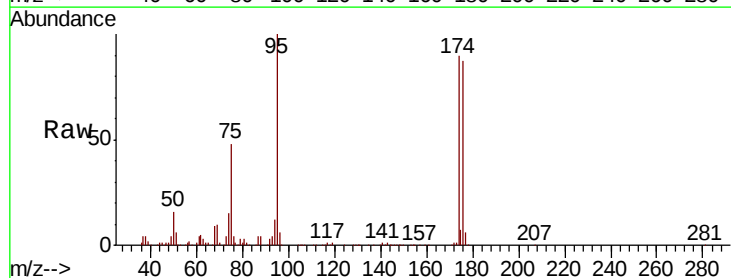


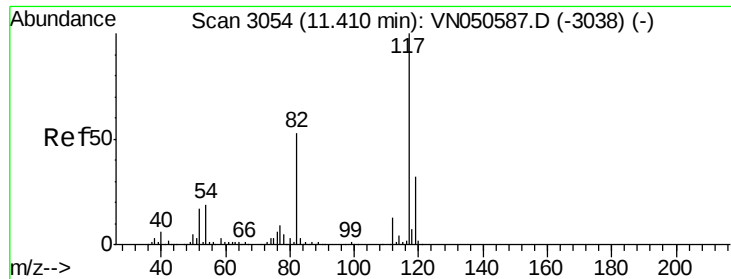

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050611.D
Acq: 14 Aug 2018 18:53




Instrument :
MSVOA_N
ClientSampleId :
958-IW-15(19)


Tgt Ion:117 Resp: 940280
Ion Ratio Lower Upper
117 100
82 52.8 42.4 63.6
119 32.2 25.8 38.8

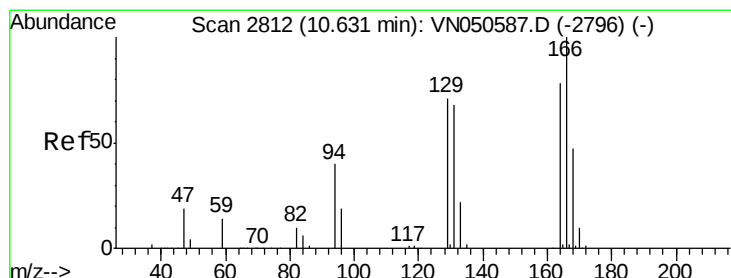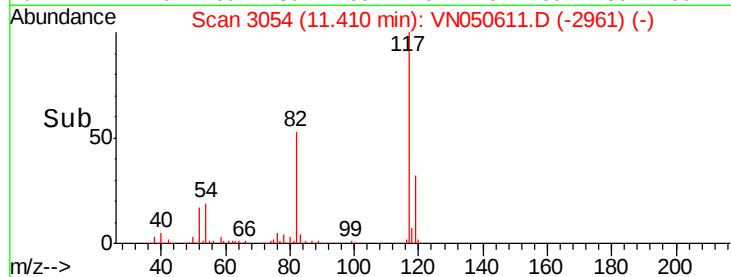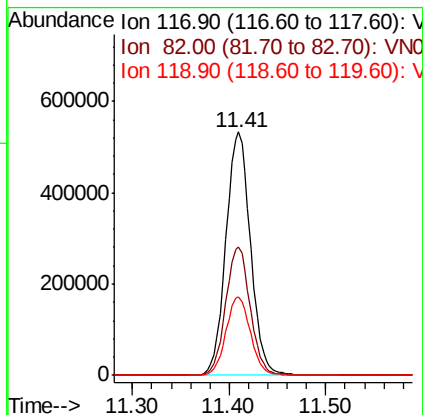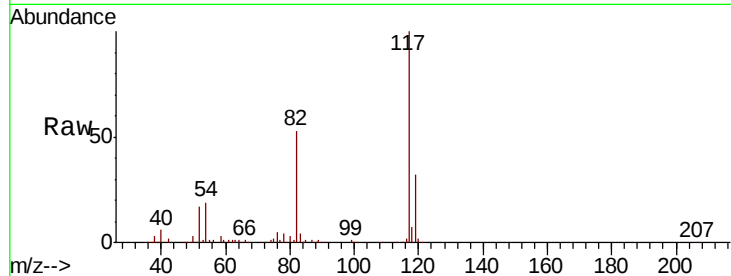

#64
Tetrachloroethene
Concen: 89.611 ug/l
RT: 10.63 min Scan# 2812
Delta R.T. 0.00 min
Lab File: VN050611.D
Acq: 14 Aug 2018 18:53

Tgt Ion:164 Resp: 782501
Ion Ratio Lower Upper
164 100
166 128.5 102.1 153.1
129 89.9 72.7 109.1
131 87.7 69.9 104.9

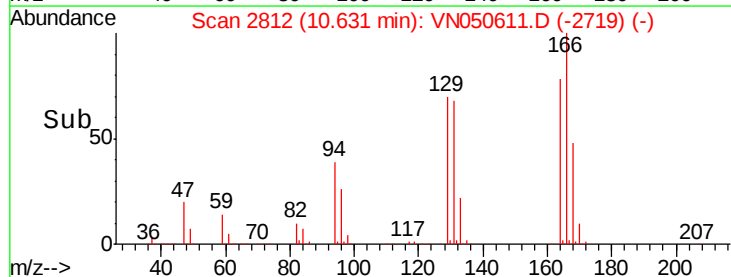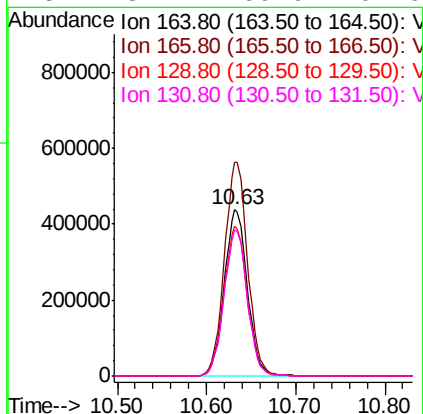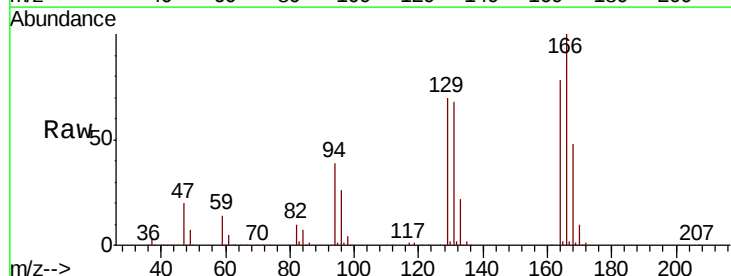

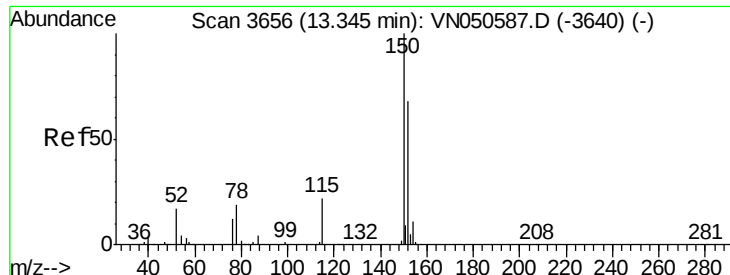

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

958-IW-15(19)


Tgt Ion:152 Resp: 337662

Ion Ratio Lower Upper

152 100

115 56.4 28.1 84.2




150 156.0 0.0 347.8

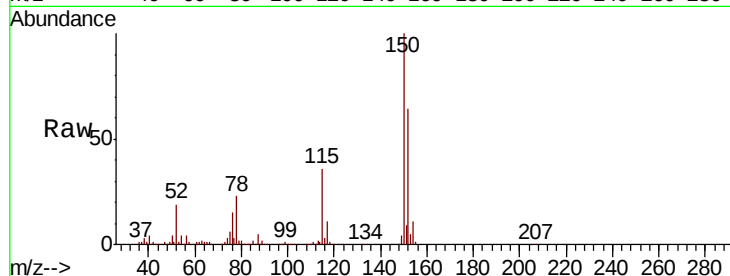

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

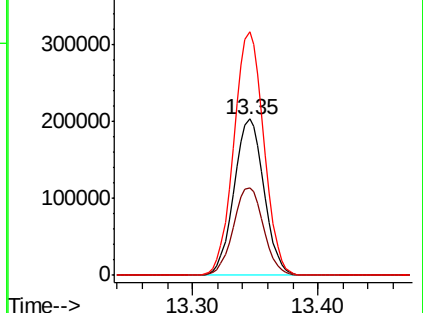

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.40 min Scan# 3362

Delta R.T. -0.10 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53


Tgt Ion: 83 Resp: 223

Ion Ratio Lower Upper

83 100

131 165.0 5.3 15.9#



85 0.0 32.1 96.5#




Abundance Ion 82.90 (82.60 to 83.60): V

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): V

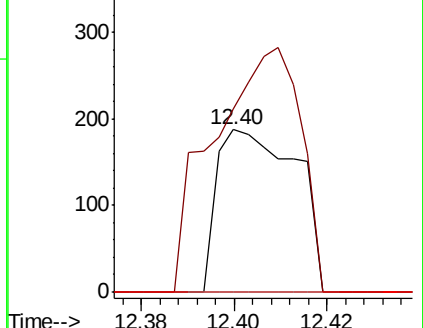



#76

1,2,3-Trichloropropane

Concen: 35.790 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53

Instrument :

MSVOA_N

ClientSampled :


958-IW-15(19)

Tgt Ion: 75 Resp: 196842

Ion Ratio Lower Upper




75 100

77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VNO

Ion 77.00 (76.70 to 77.70): VNO

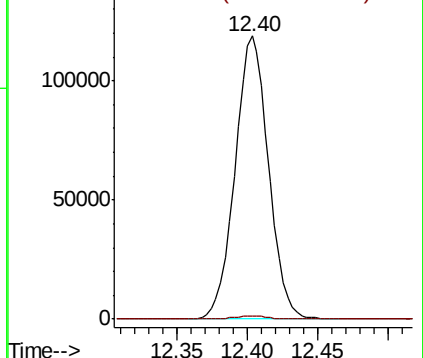

#81

trans-1,4-Dichloro-2-butene

Concen: 129.603 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.10 min

Lab File: VN050611.D

Acq: 14 Aug 2018 18:53


Tgt Ion: 75 Resp: 196842

Ion Ratio Lower Upper

75 100

53 0.1 72.2 108.2#



89 0.0 36.3 54.5#




Abundance Ion 74.90 (74.60 to 75.60): VNO

Ion 53.00 (52.70 to 53.70): VNO

Ion 88.90 (88.60 to 89.60): VNO

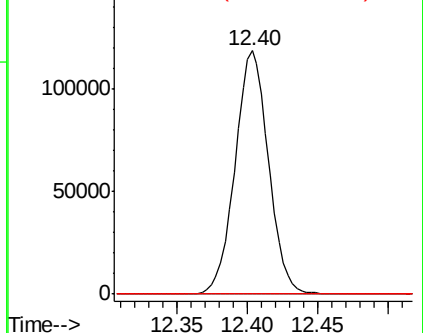


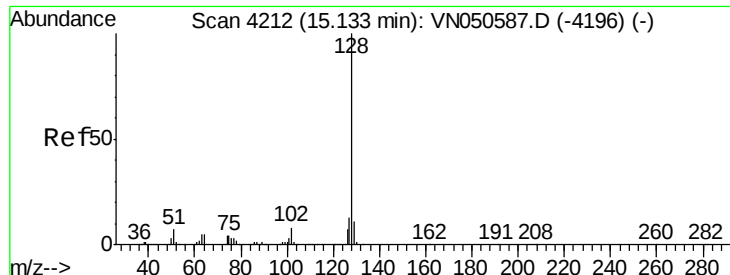

#95
Naphthalene
Concen: 3.912 ug/l
RT: 15.14 min Scan# 4214
Delta R.T. 0.01 min
Lab File: VN050611.D
Acq: 14 Aug 2018 18:53

Instrument :
MSVOA_N
ClientSampleId :
958-IW-15(19)

Tgt Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.5	12.7#



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

