



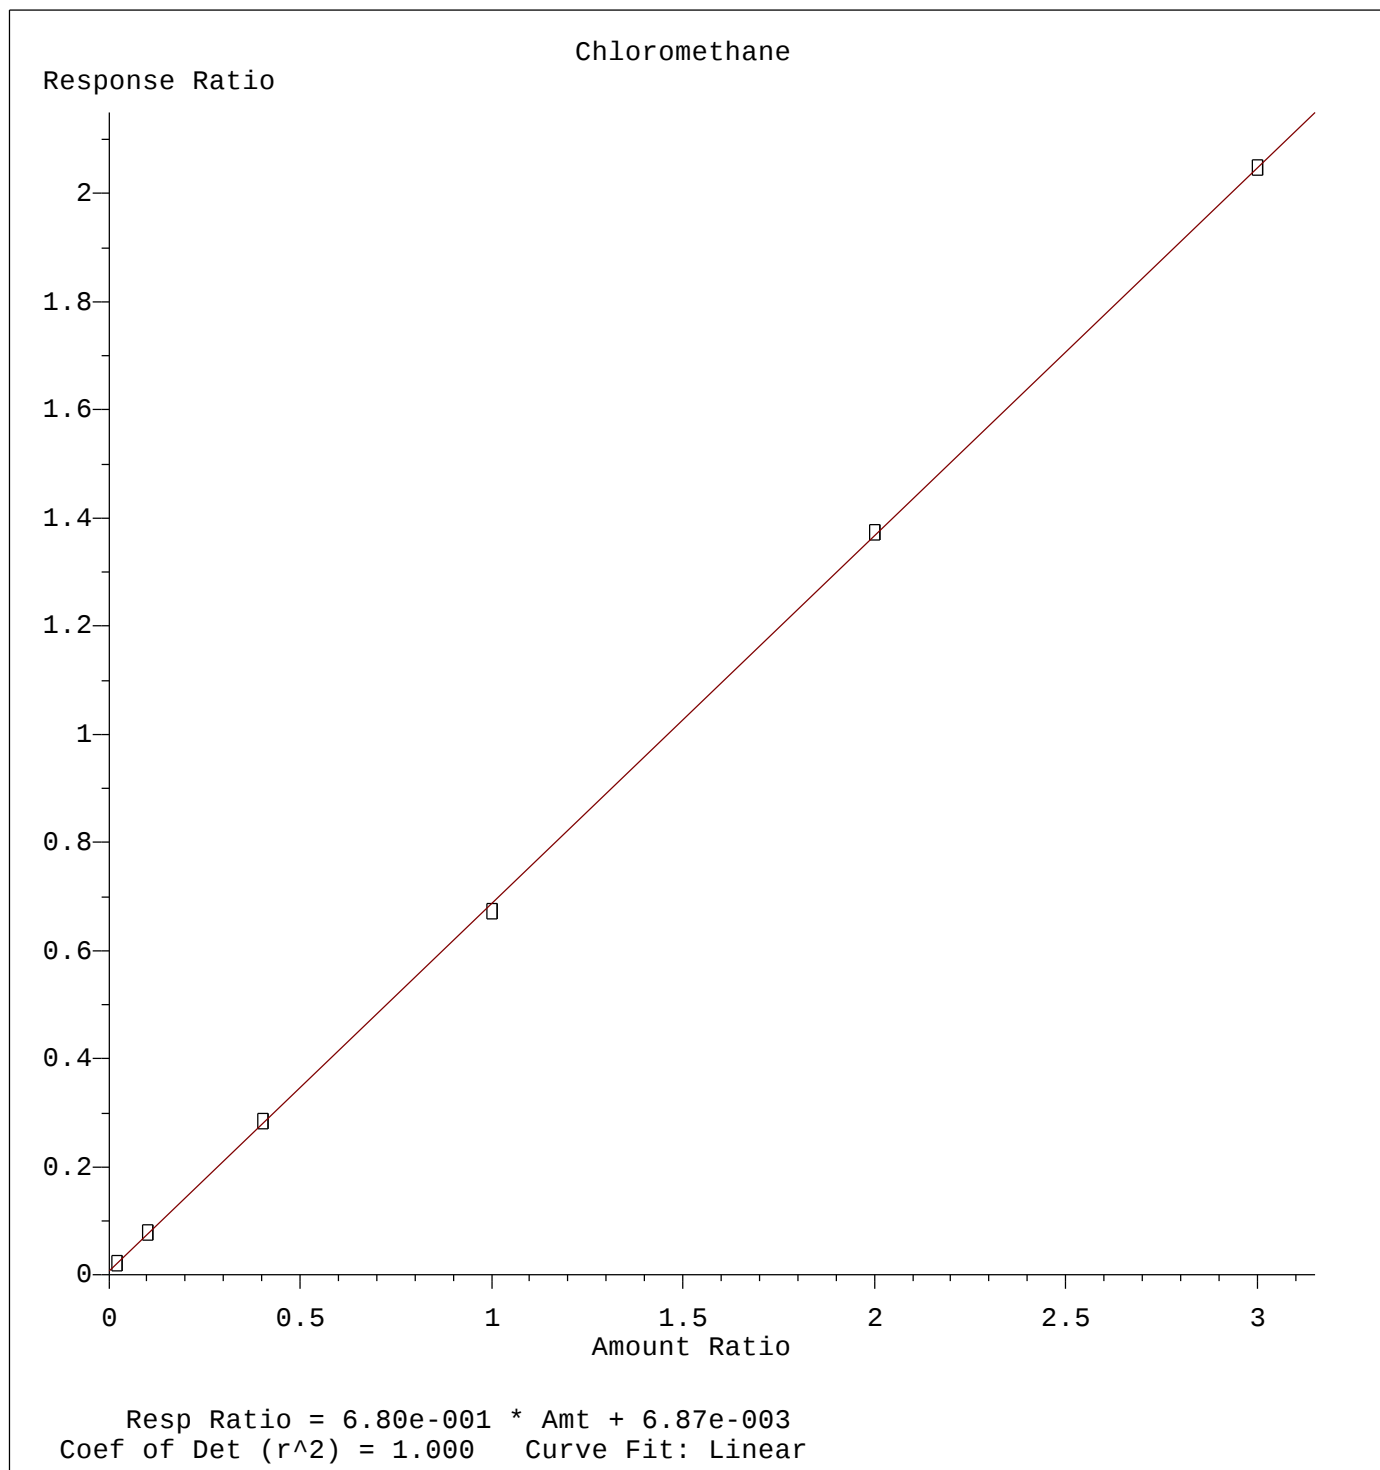


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

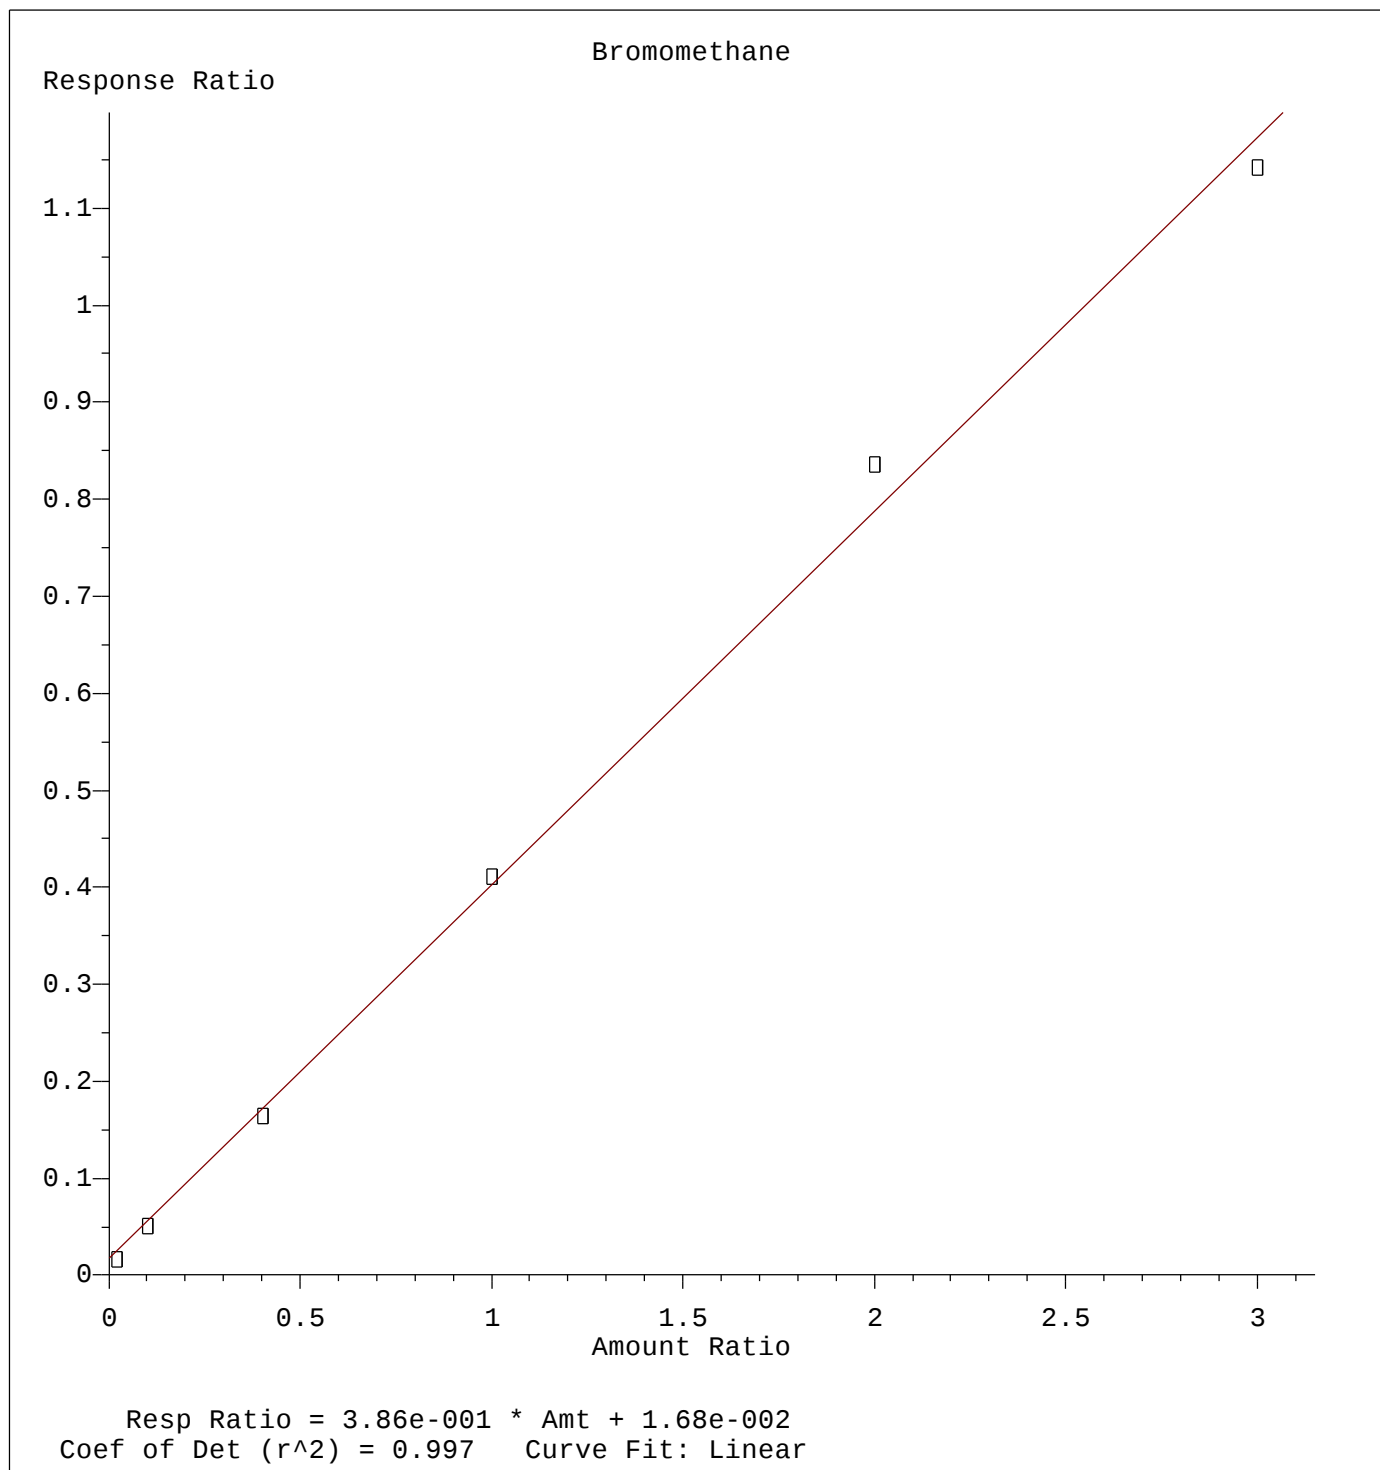

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018


# Chloroethane

Response Ratio

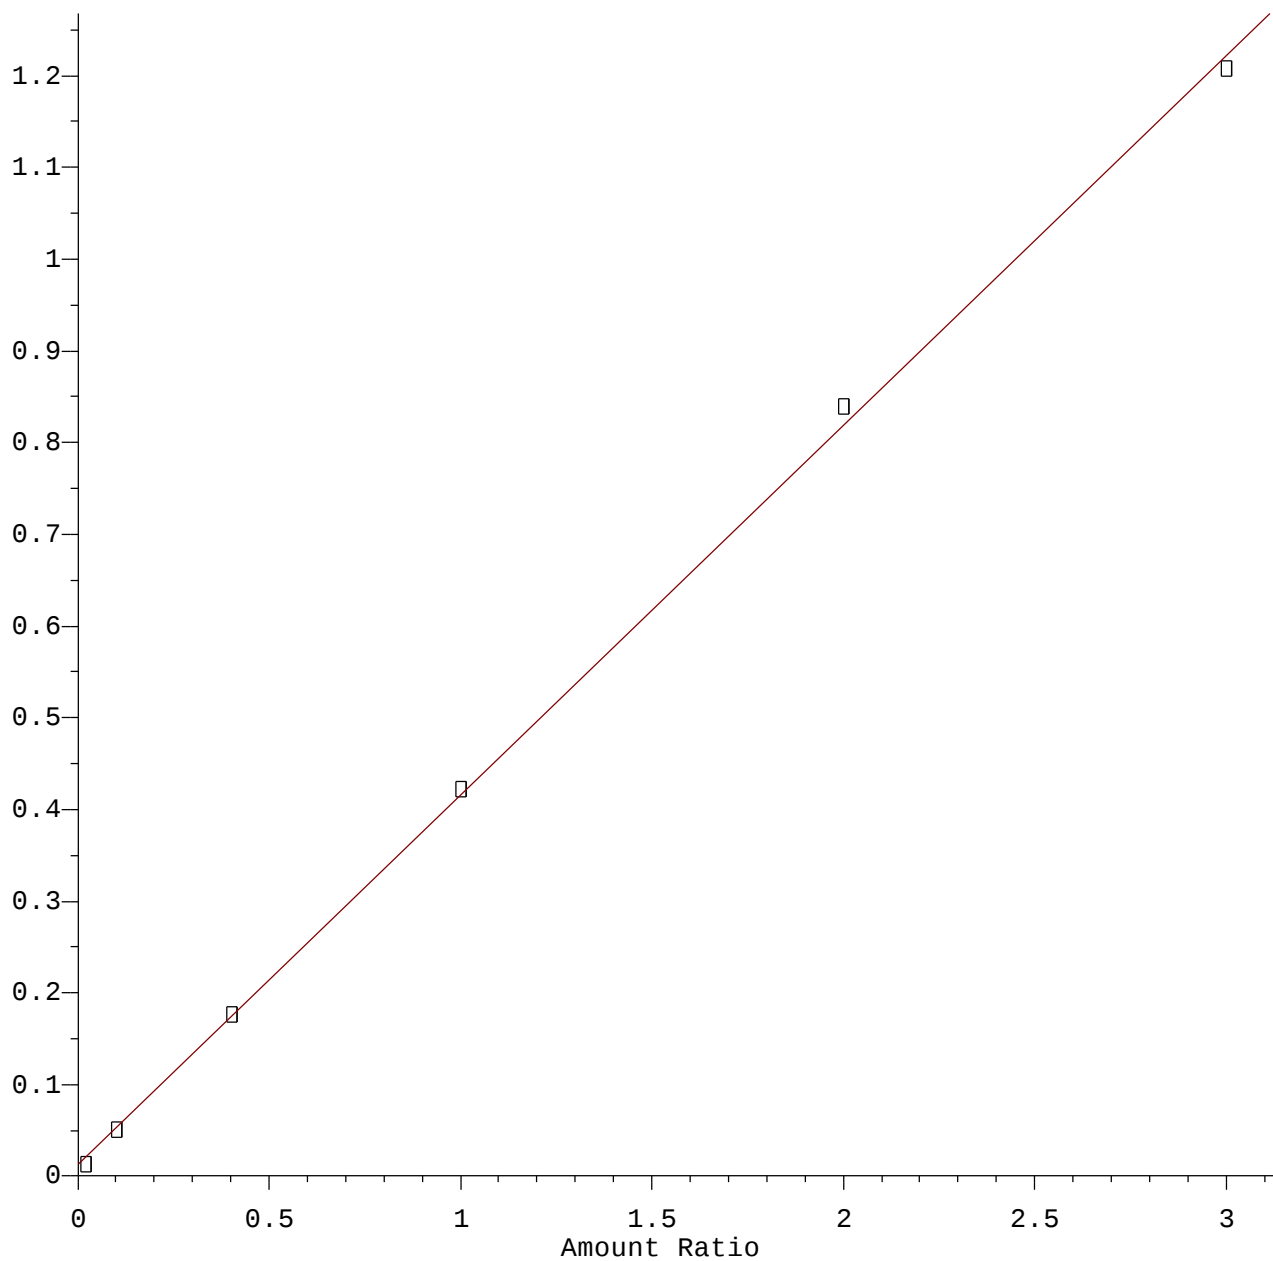


Resp Ratio =  $4.03 \times 10^{-1} \times \text{Amt} + 1.32 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

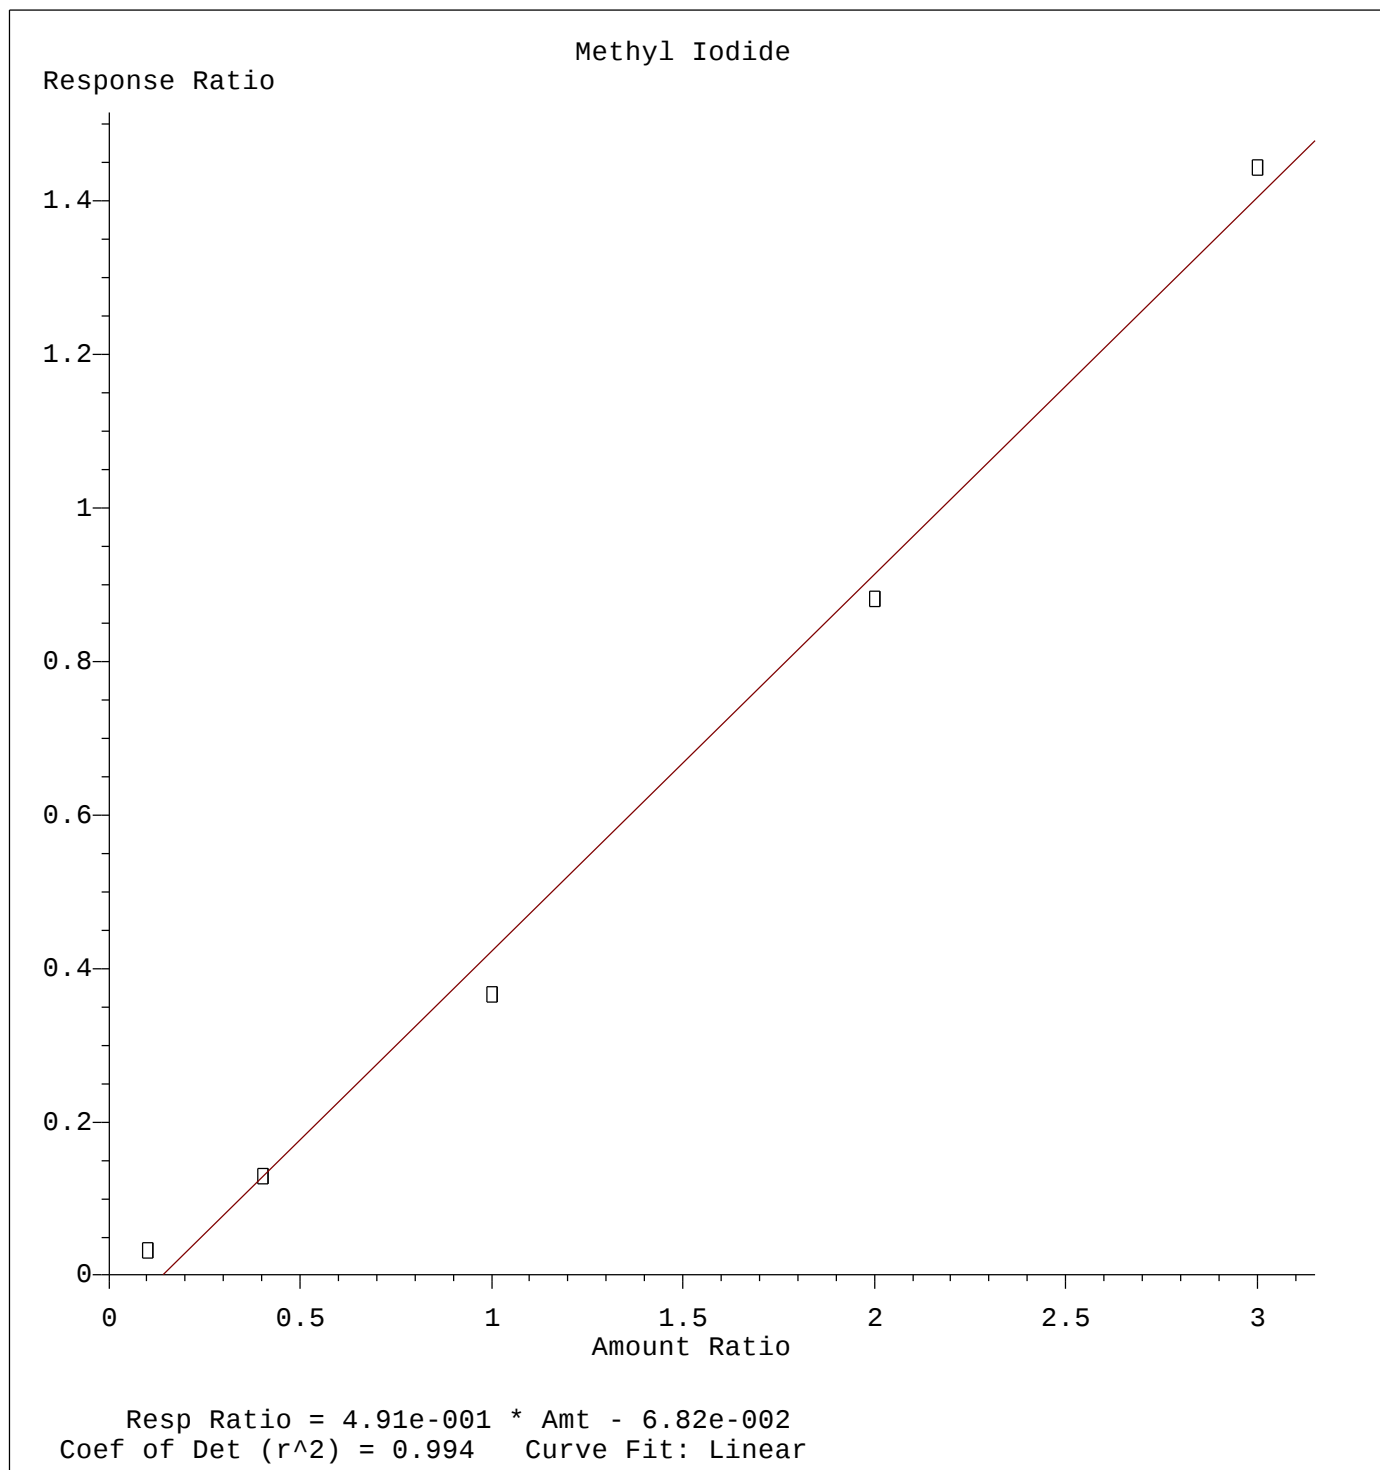


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

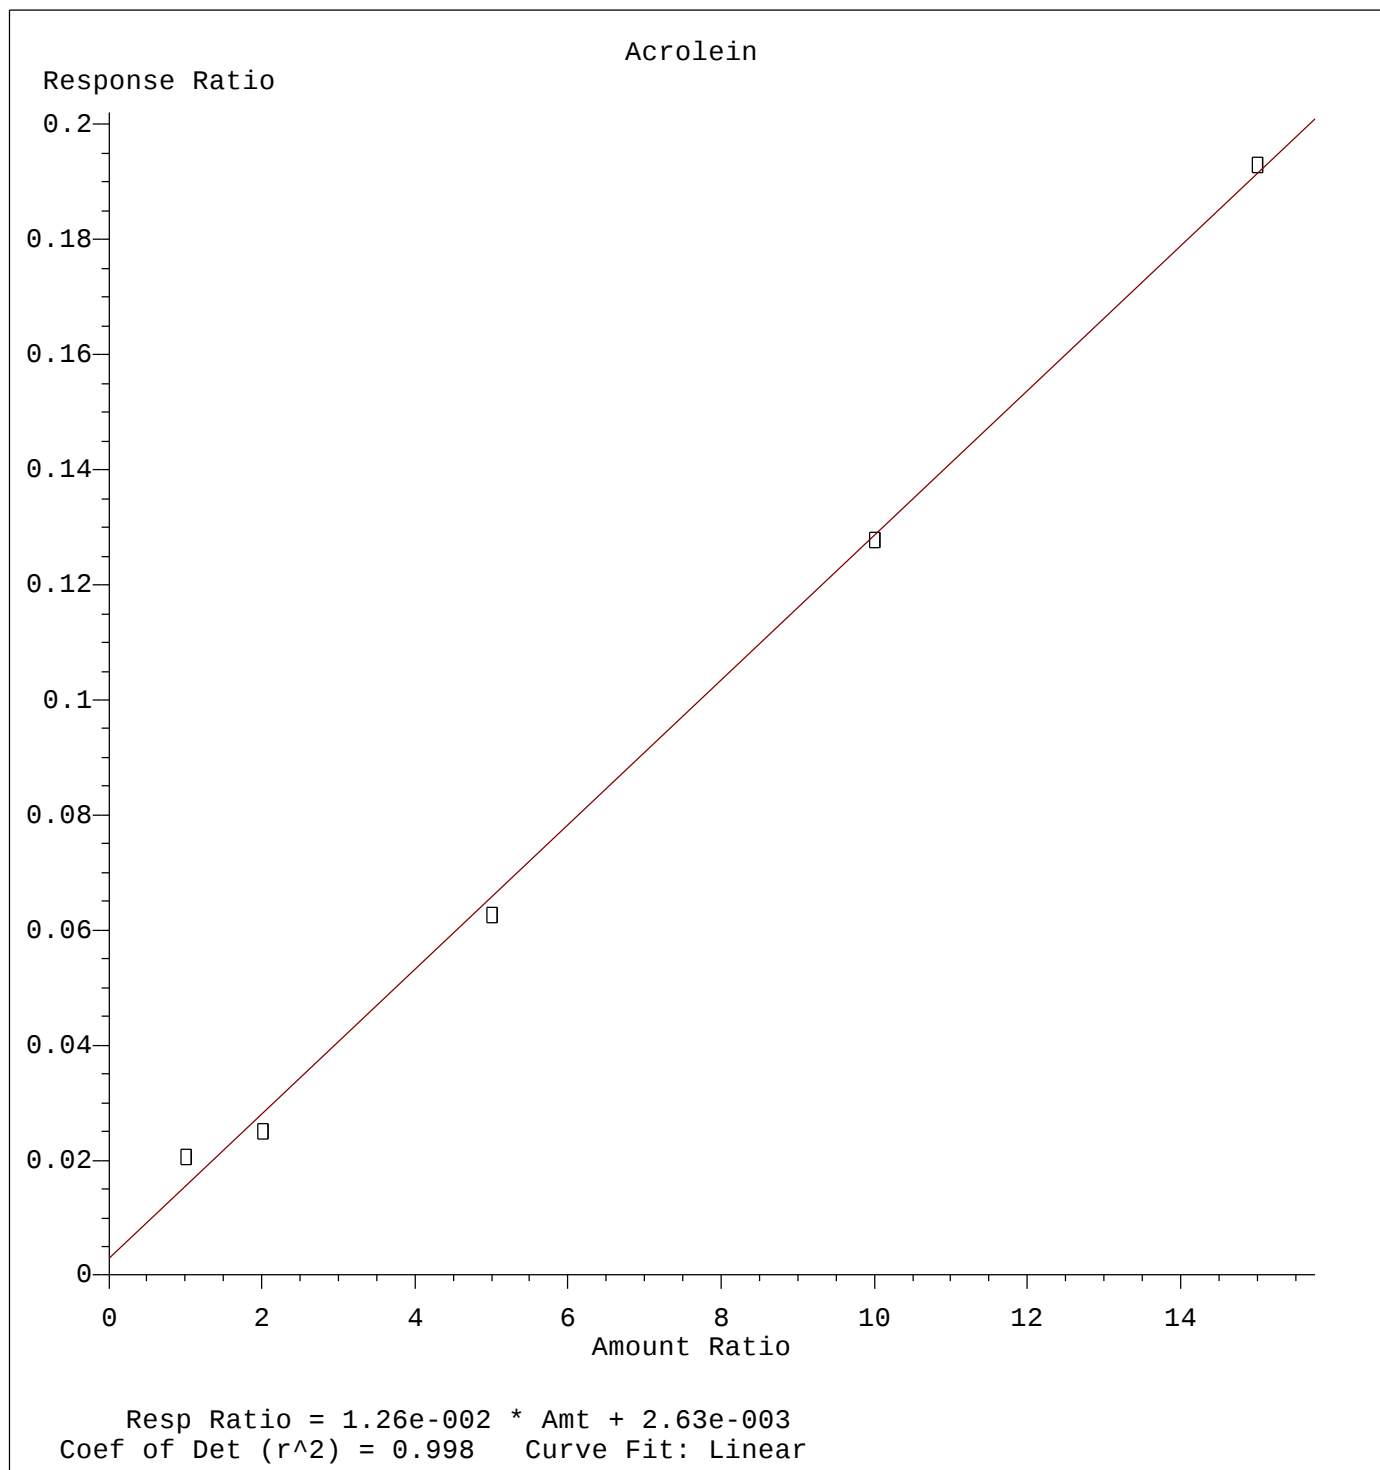

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

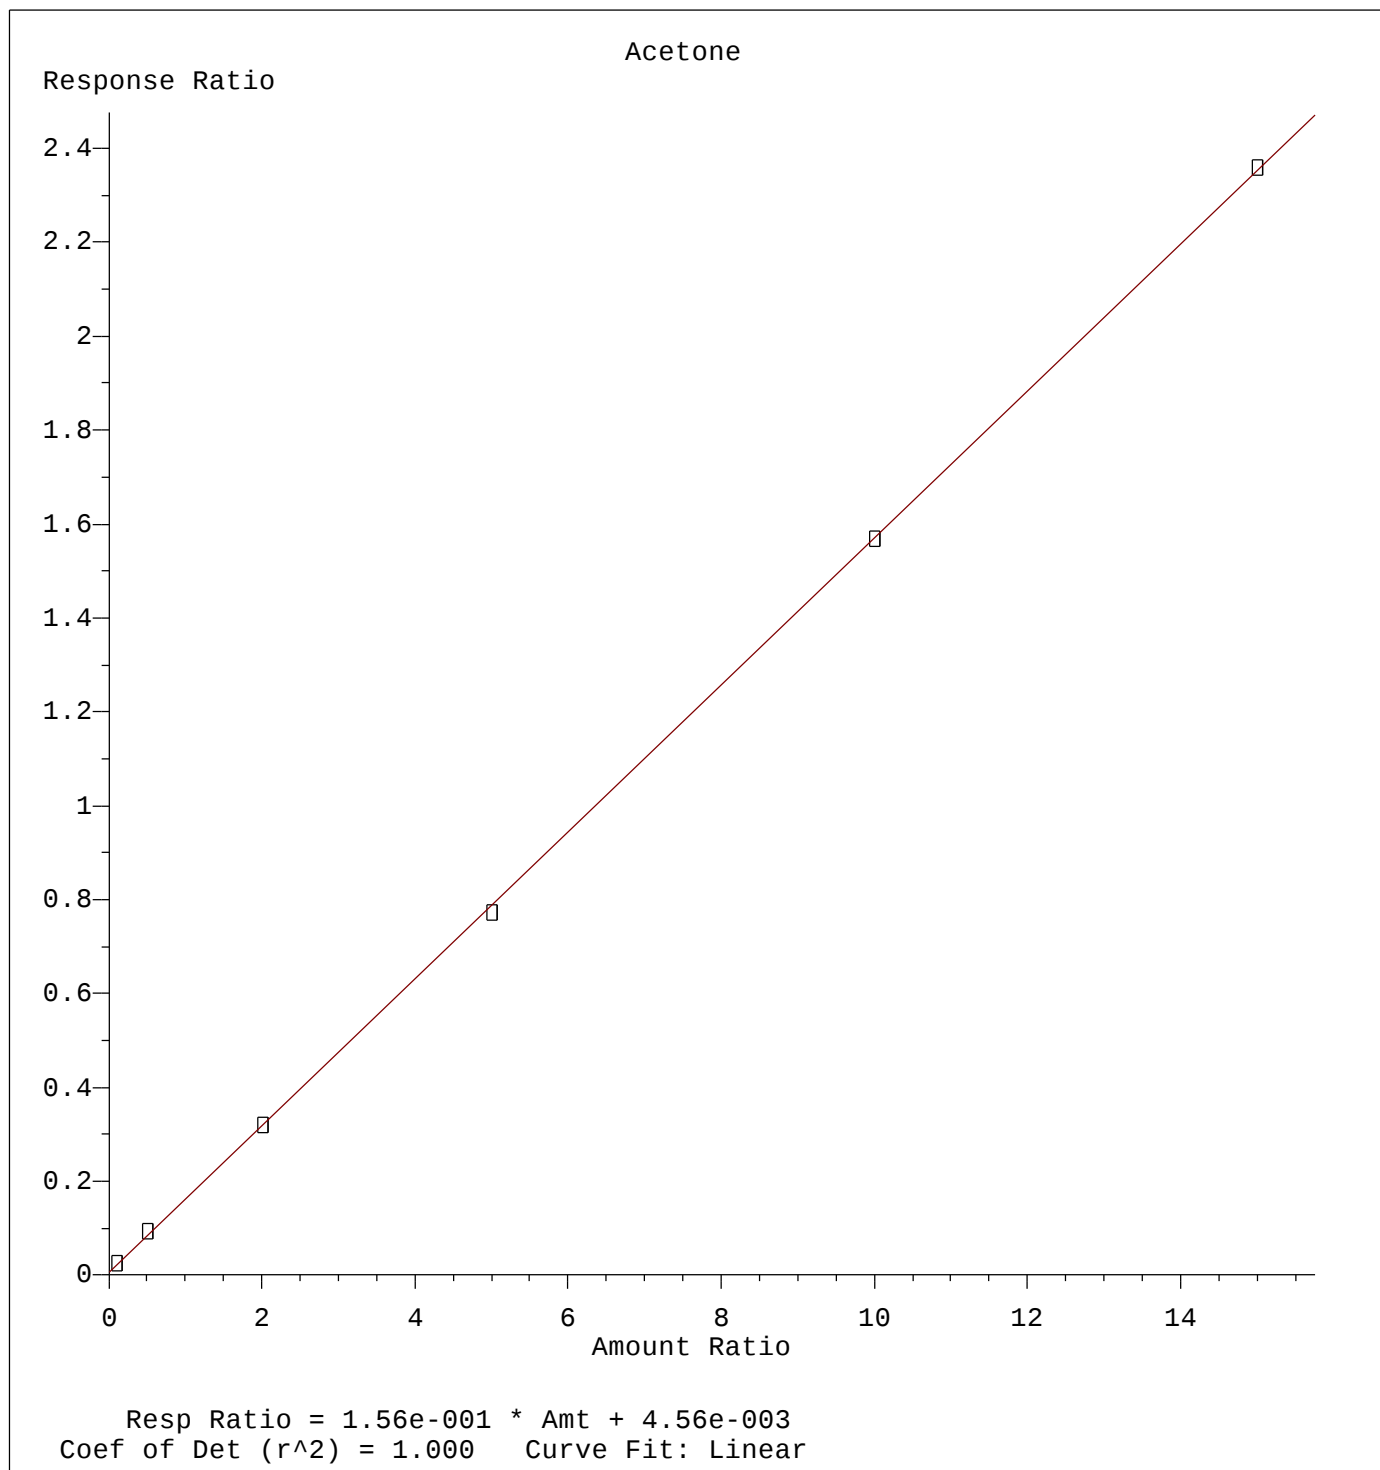


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

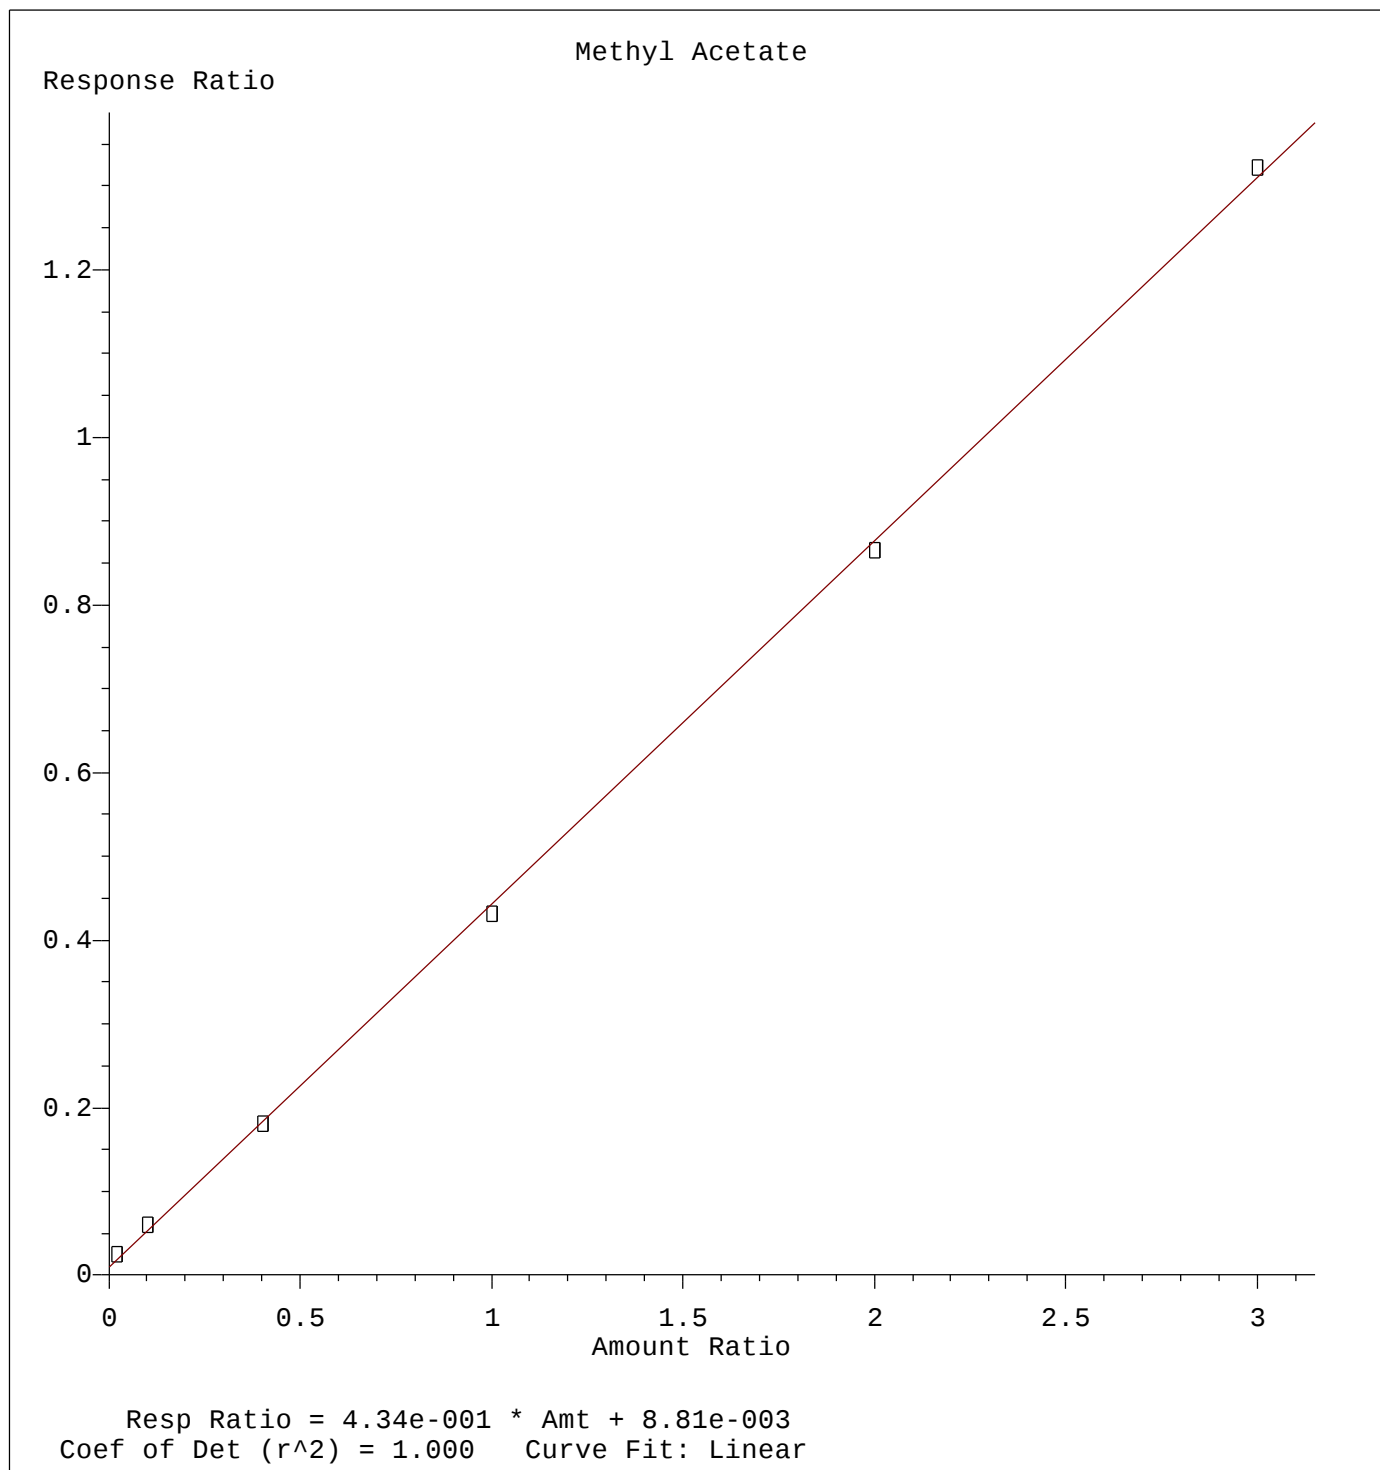

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018


# Methylene Chloride

Response Ratio

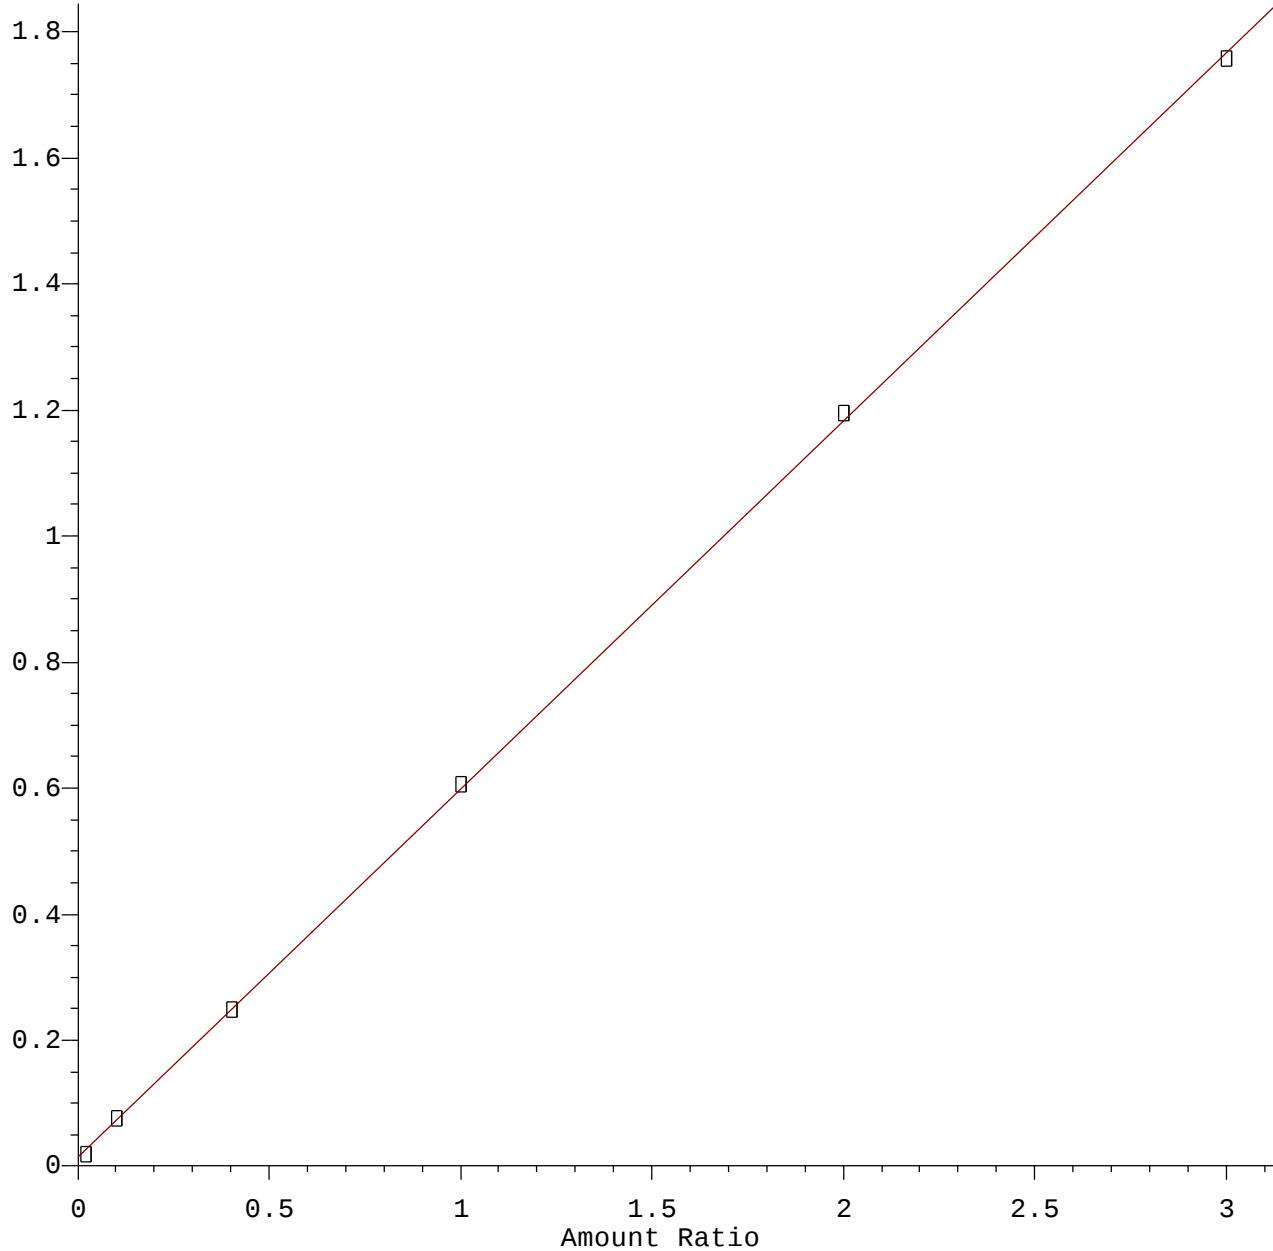


Resp Ratio = 5.84e-001 \* Amt + 1.52e-002  
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

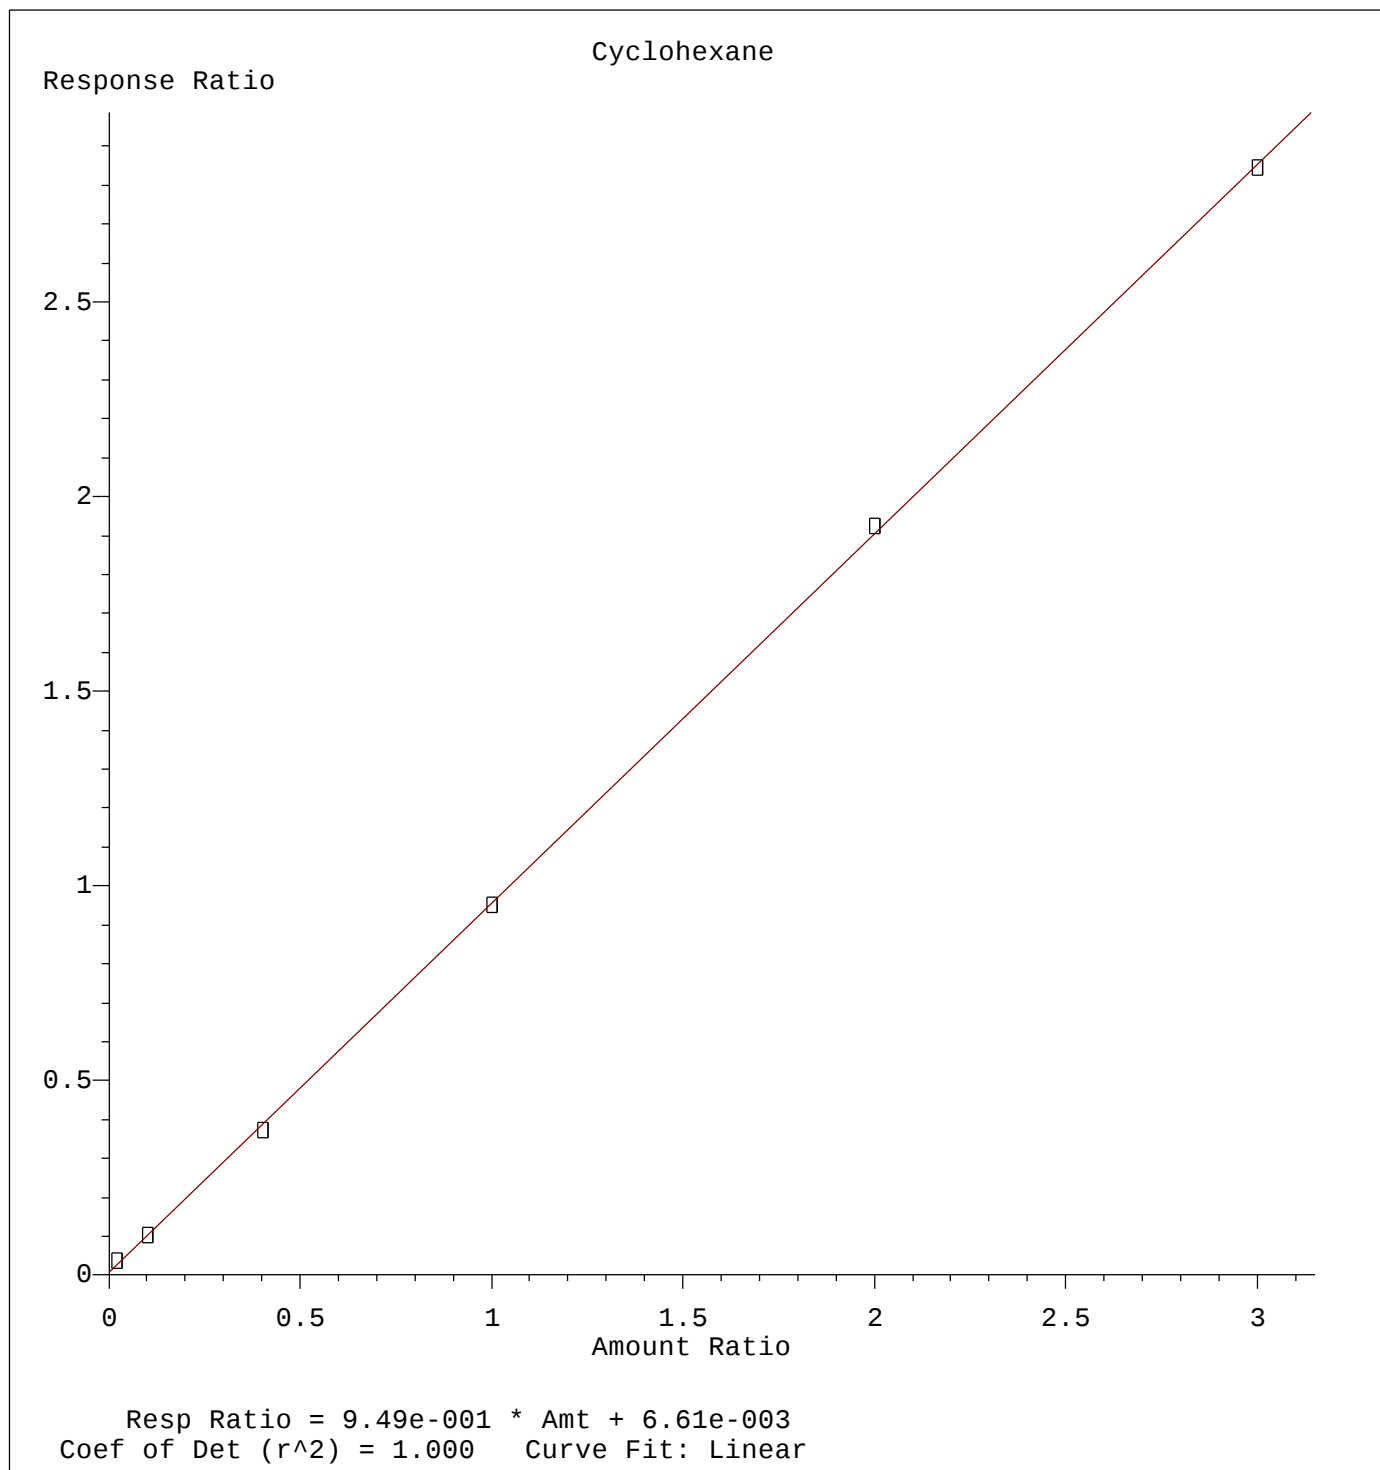


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

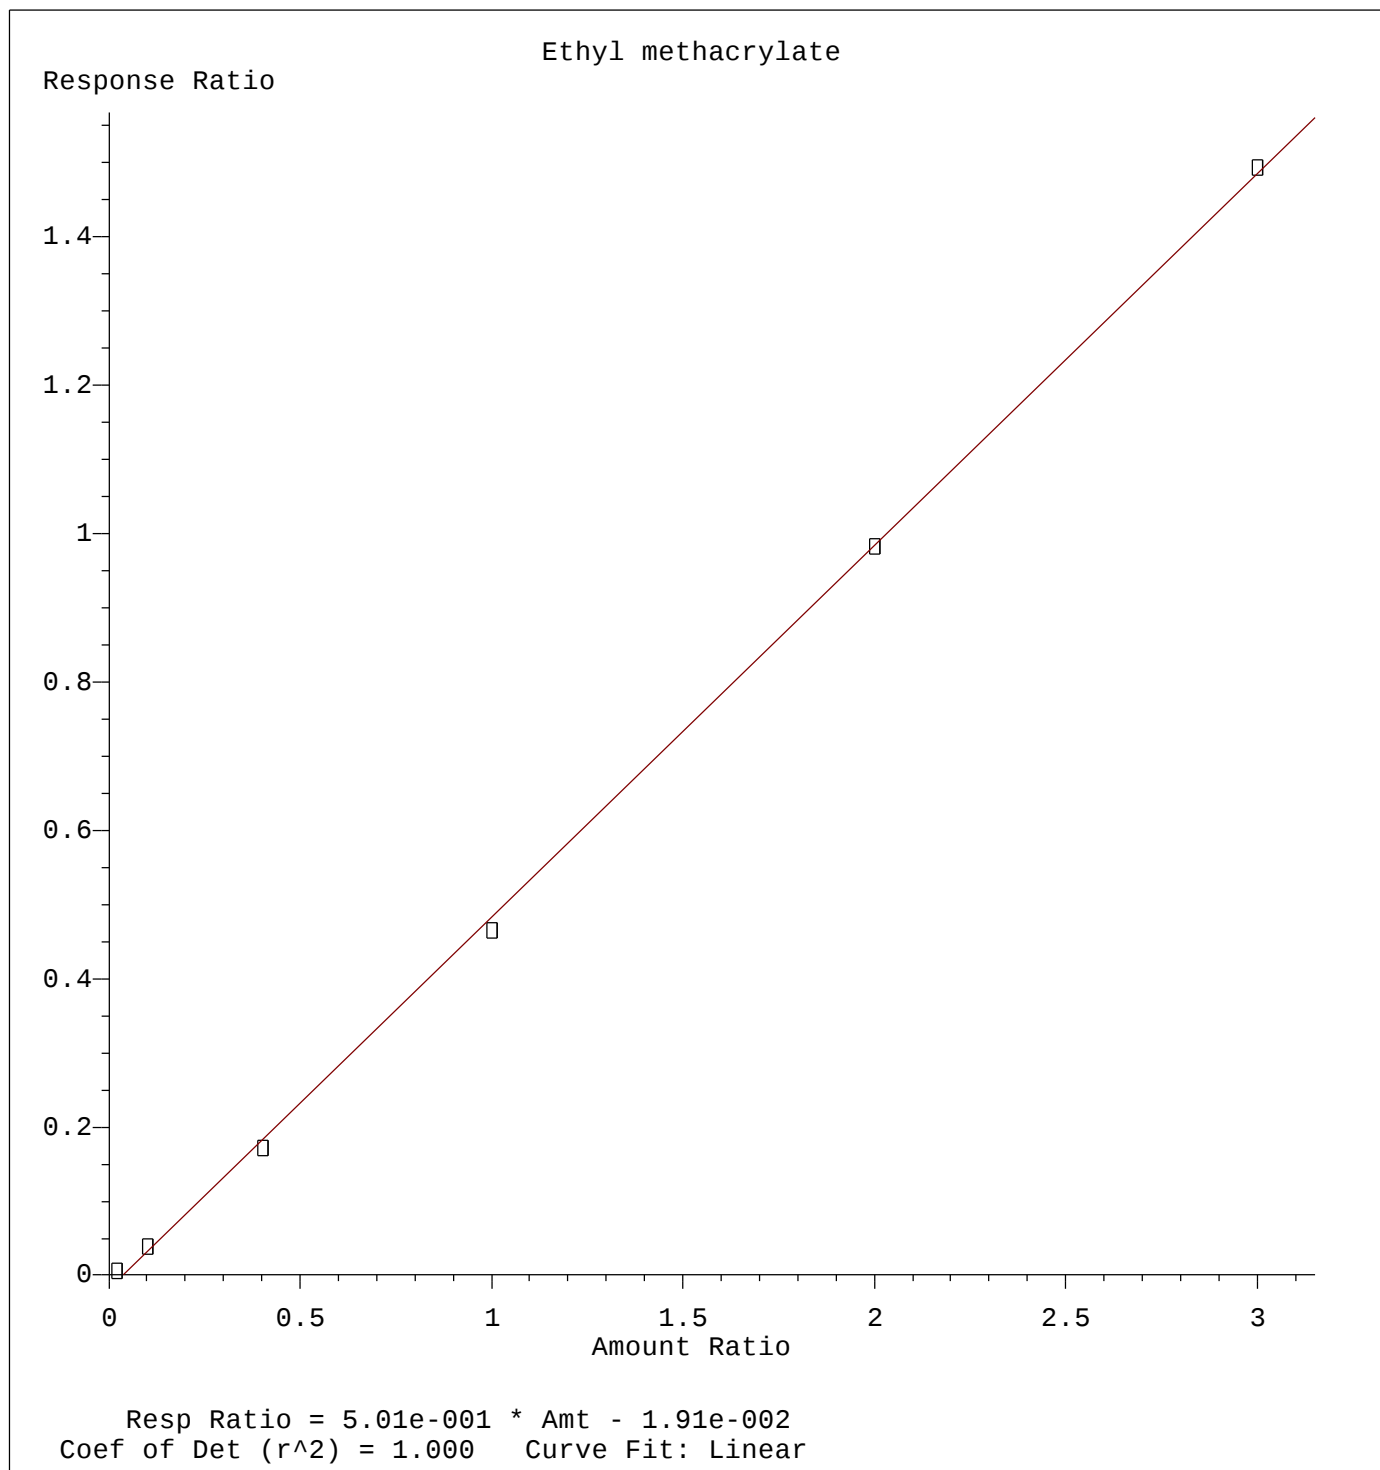

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018


2-Chloroethyl Vinyl ether

Response Ratio

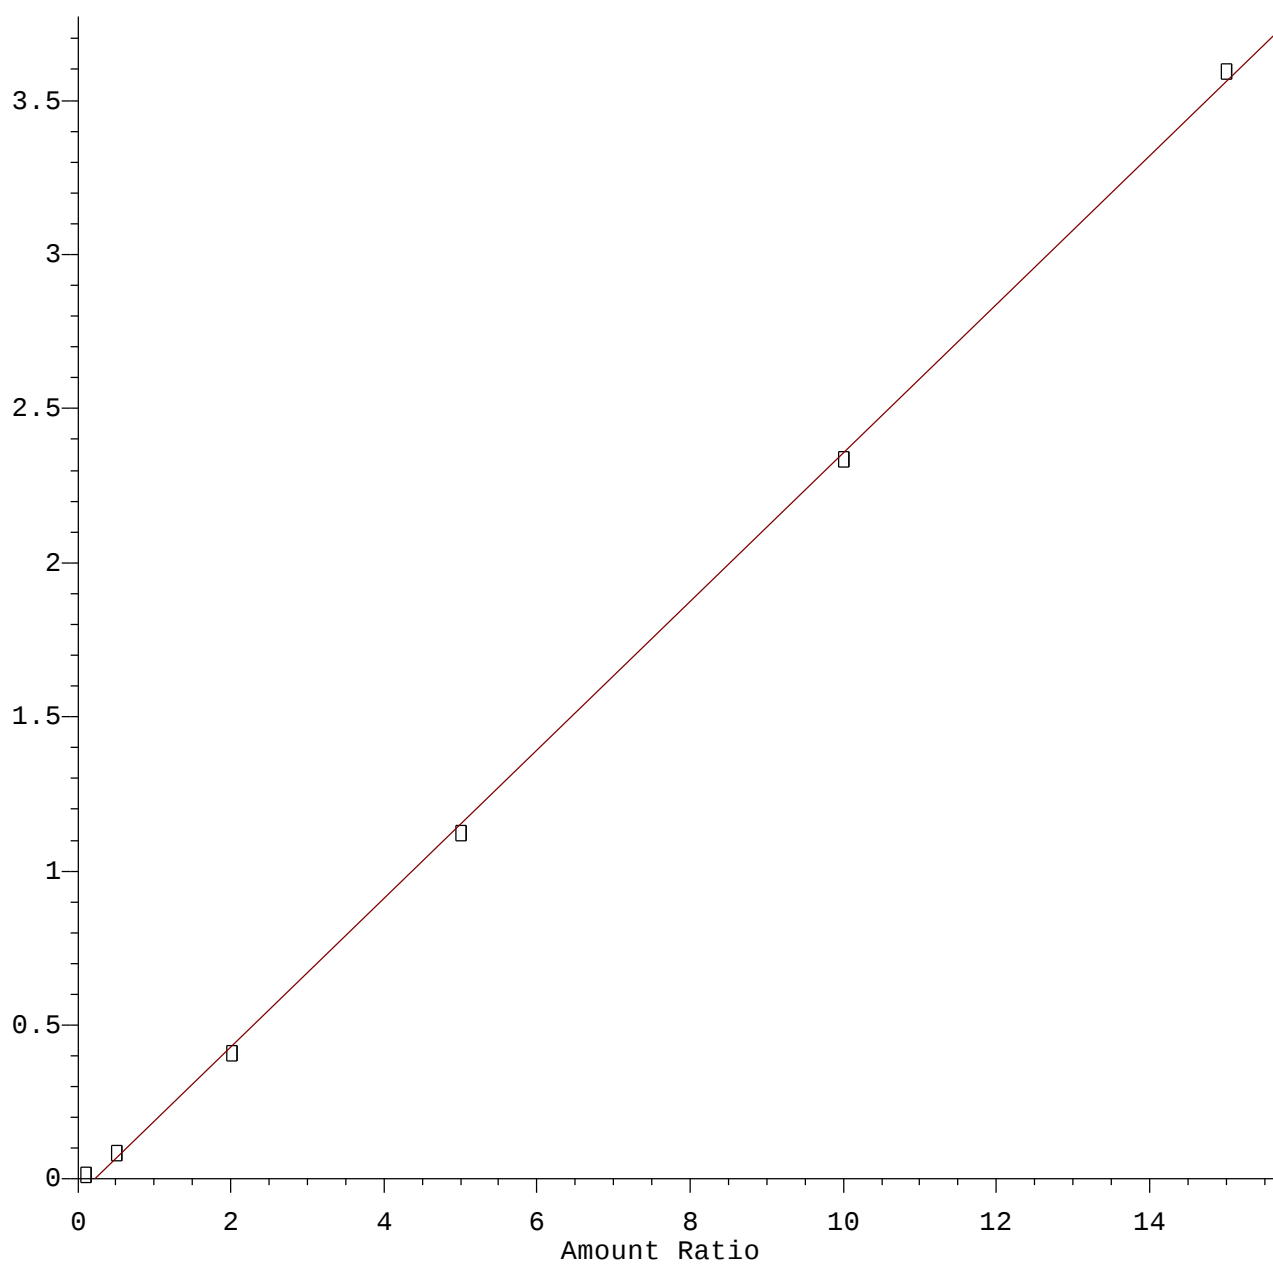

Resp Ratio =  $2.41 \times 10^{-1} \times \text{Amt} - 5.02 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 1.000    Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

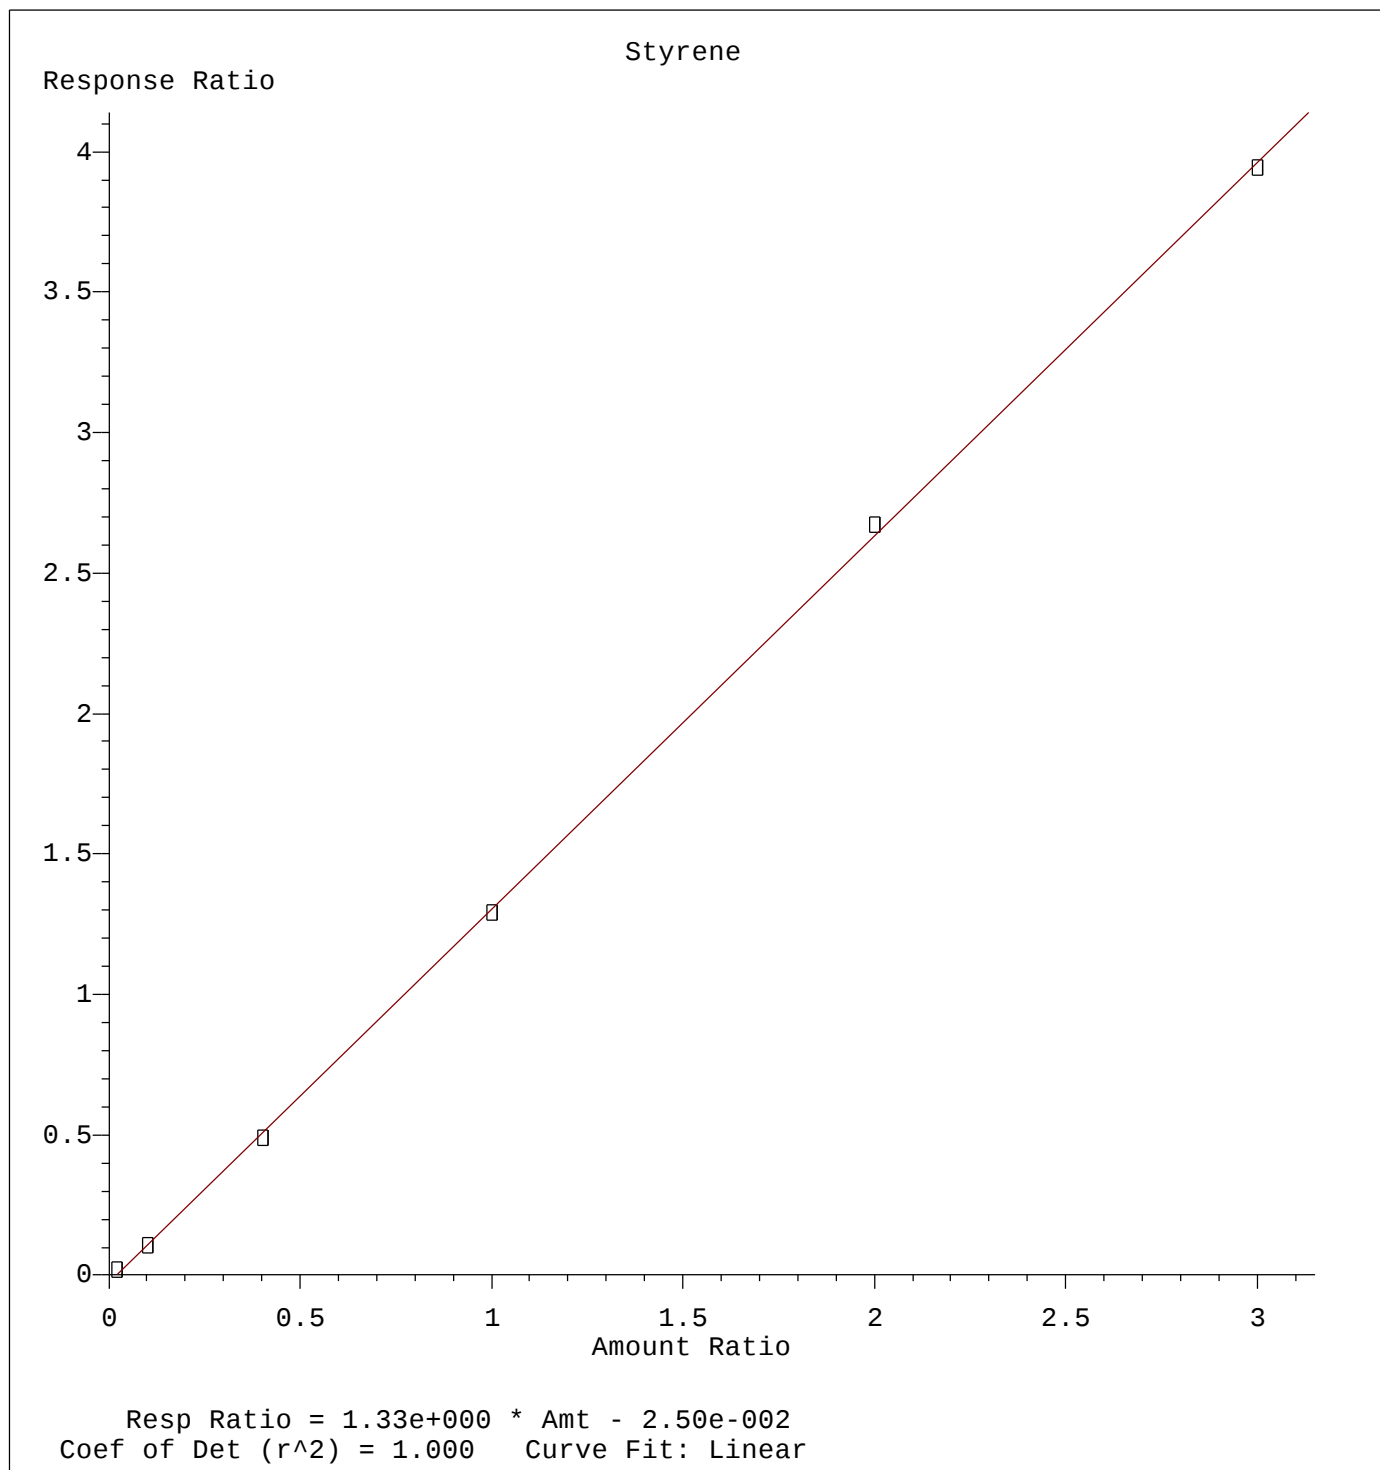

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

1,1,2,2-Tetrachloroethane

Response Ratio

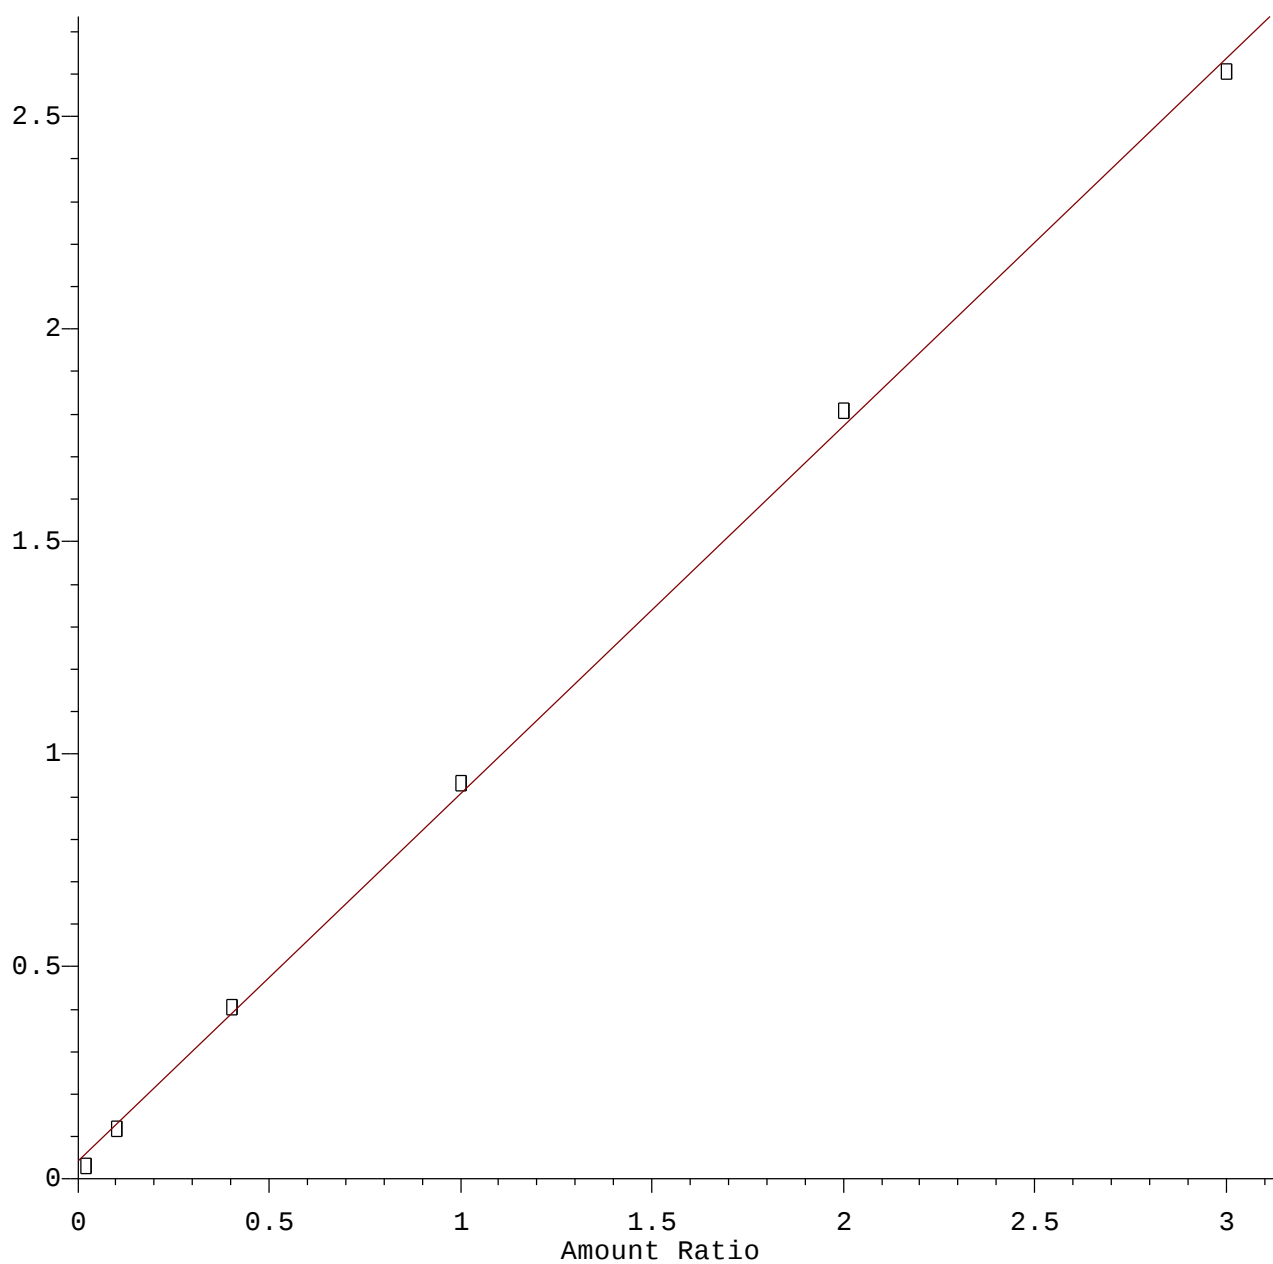


Resp Ratio = 8.65e-001 \* Amt + 4.22e-002  
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

# 1,2,3-Trichloropropane

Response Ratio

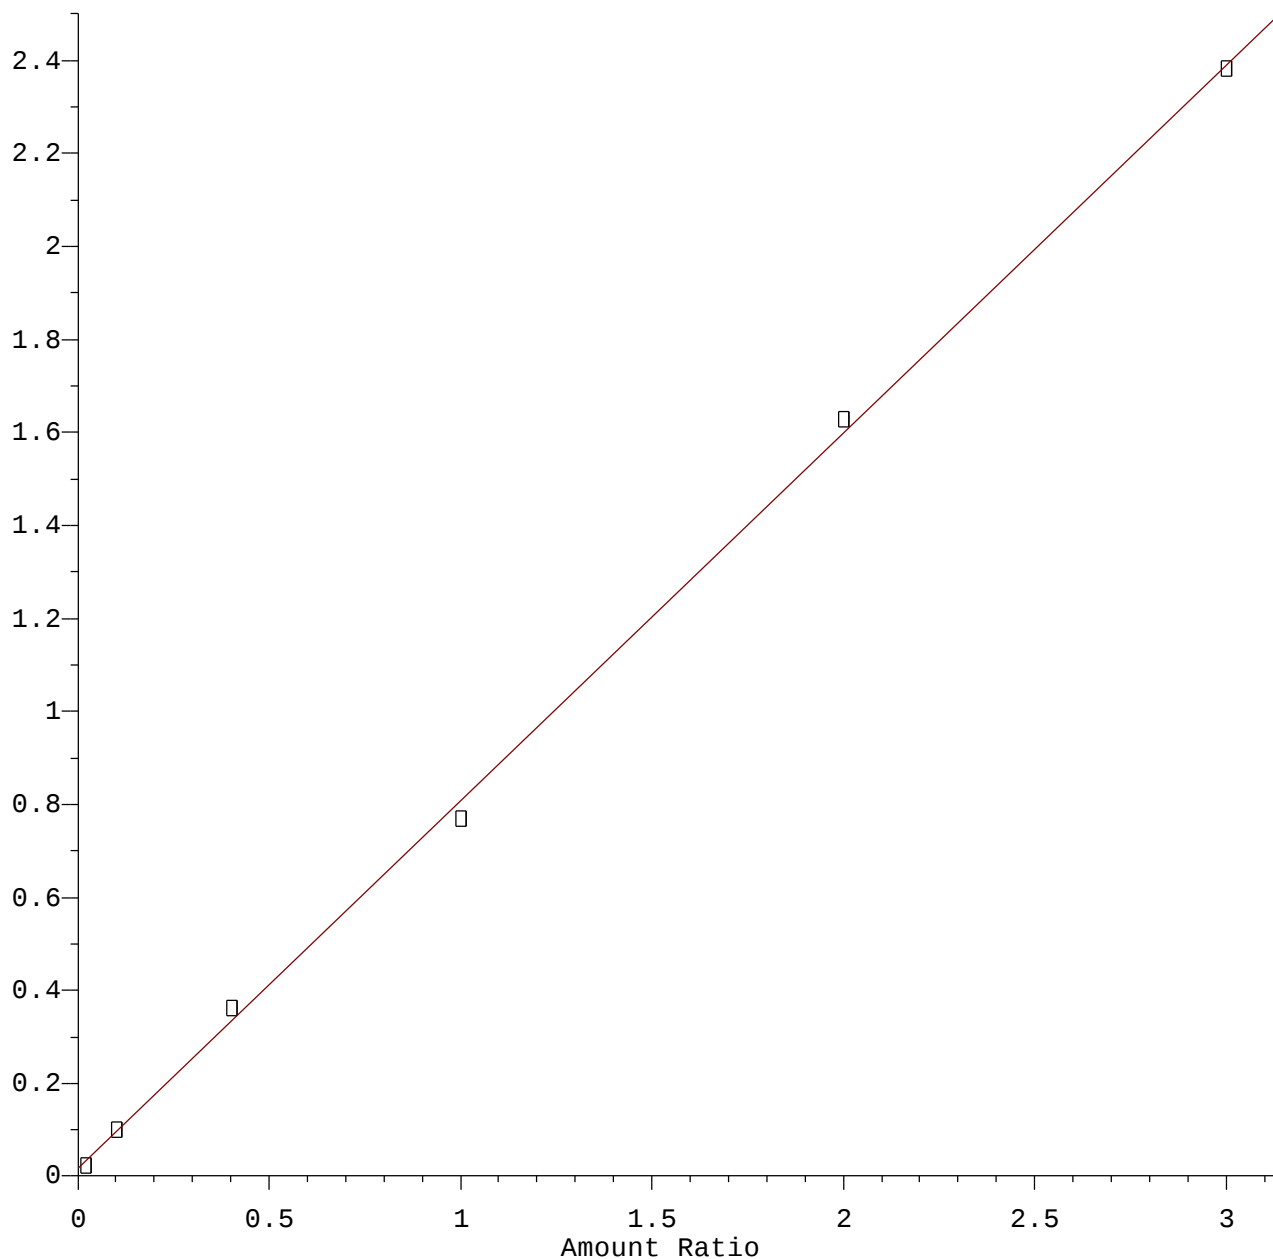


Resp Ratio =  $7.91 \times 10^{-1} \times \text{Amt} + 1.66 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

# 1,2,4-Trichlorobenzene

Response Ratio

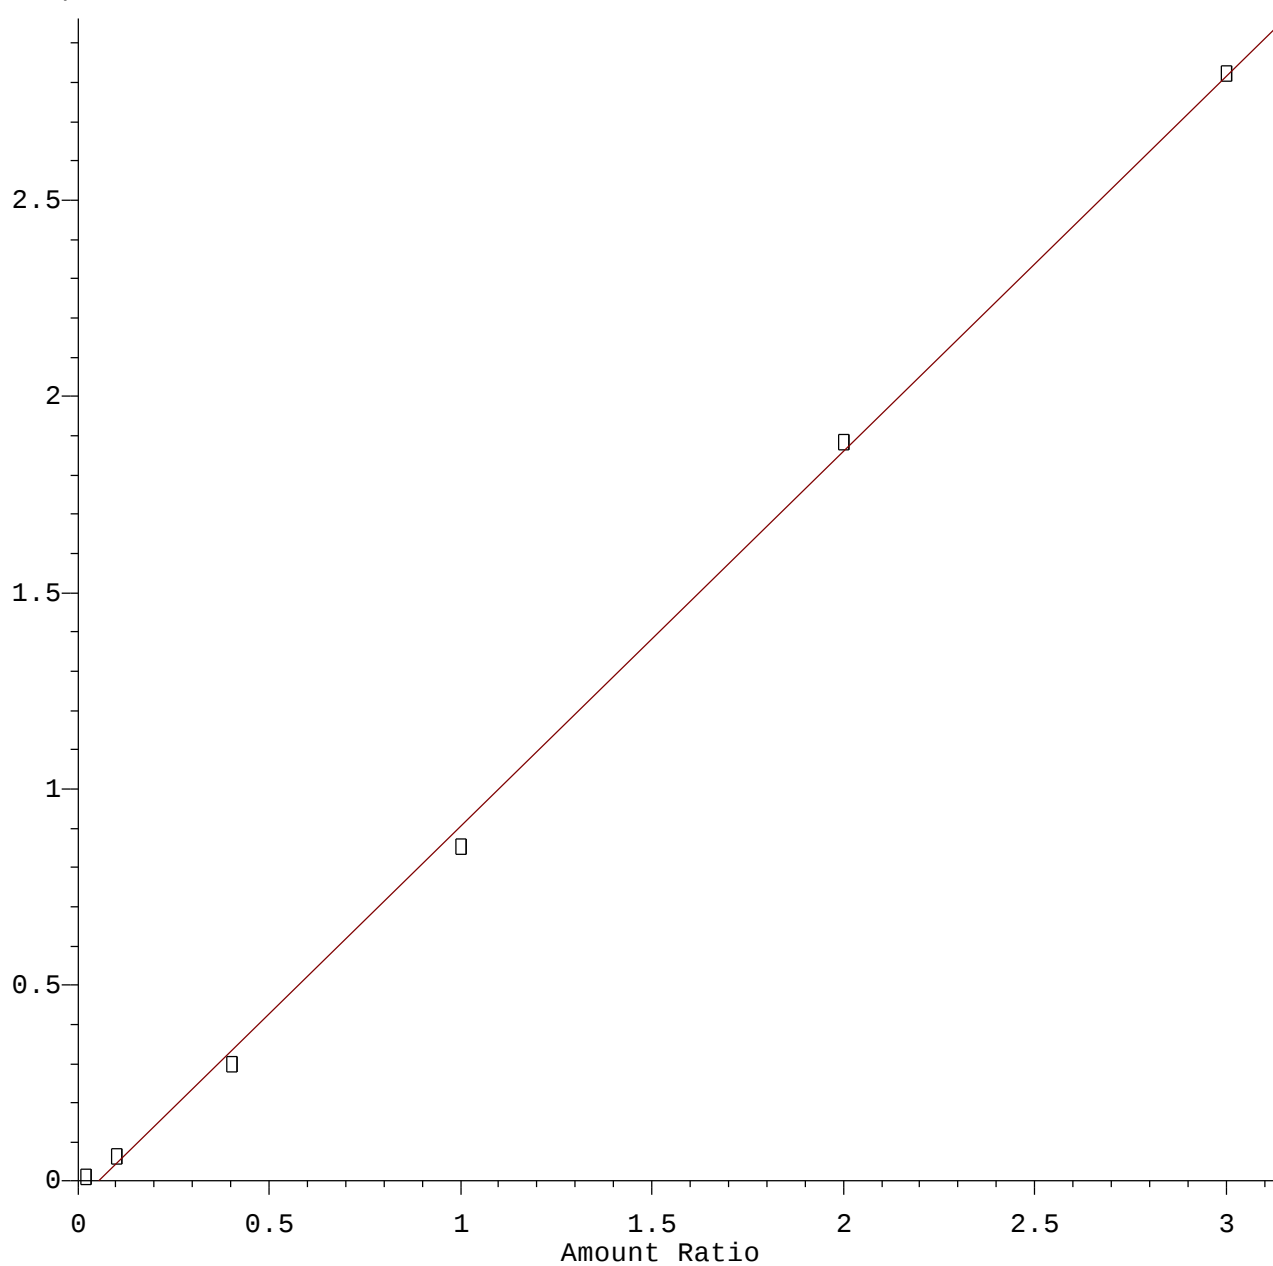


Resp Ratio = 9.55e-001 \* Amt - 5.11e-002  
Coef of Det ( $r^2$ ) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

# Naphthalene

Response Ratio

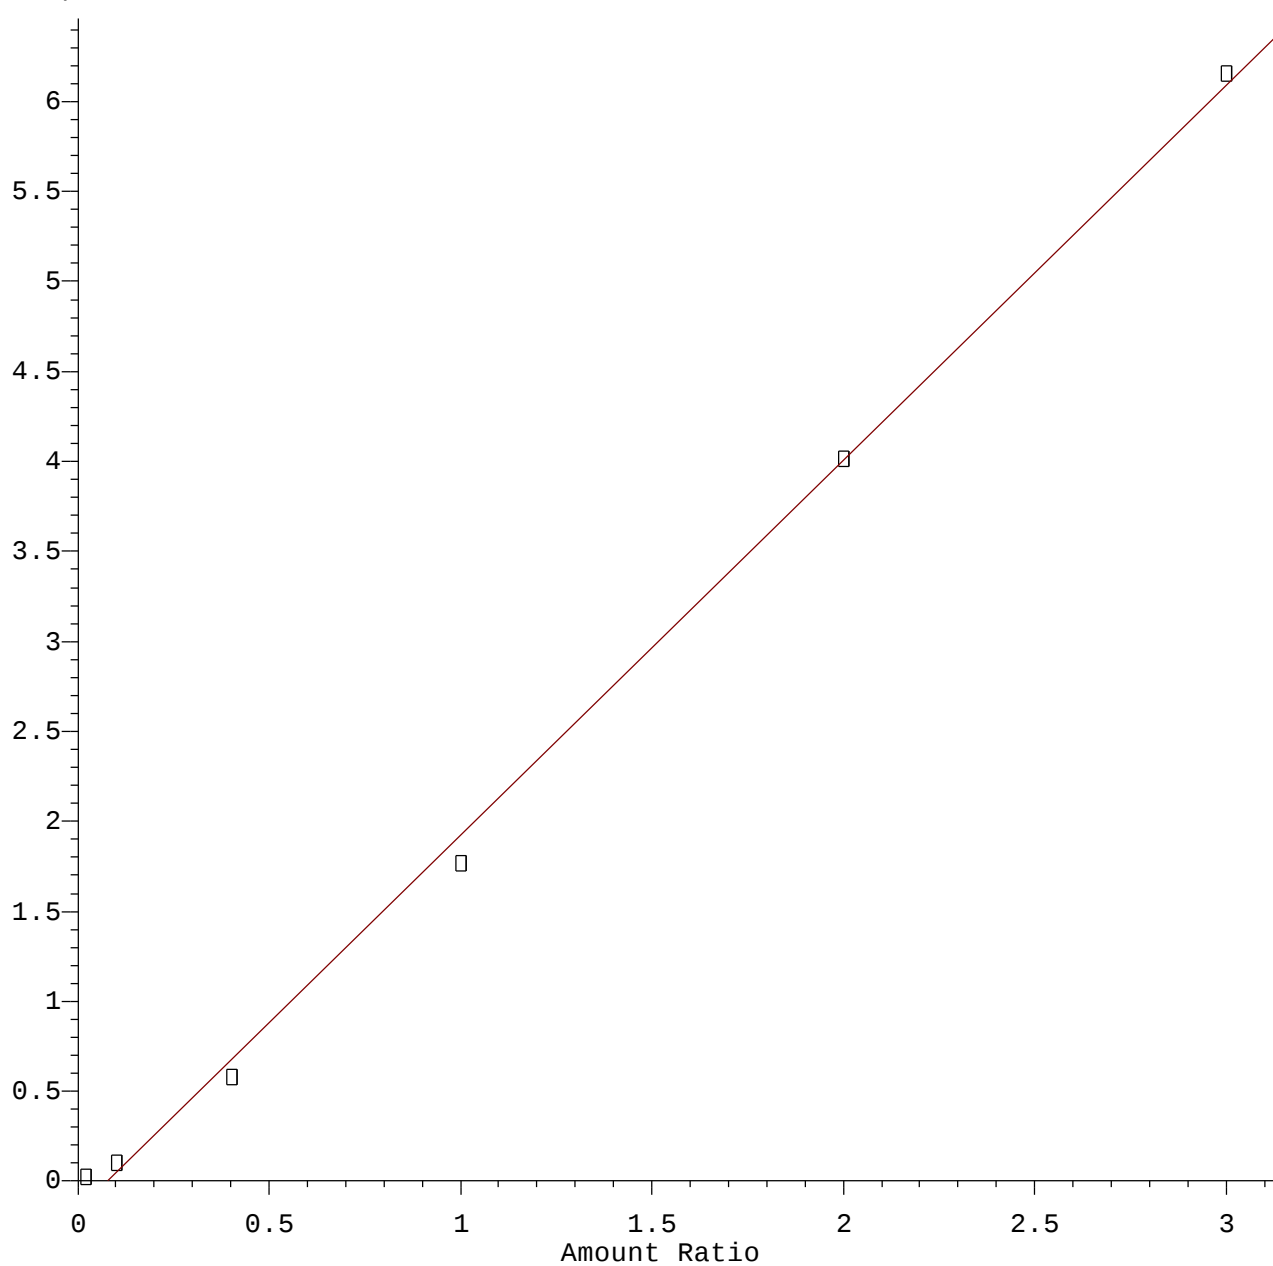


Resp Ratio = 2.08e+000 \* Amt - 1.61e-001  
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018

# 1,2,3-Trichlorobenzene

Response Ratio

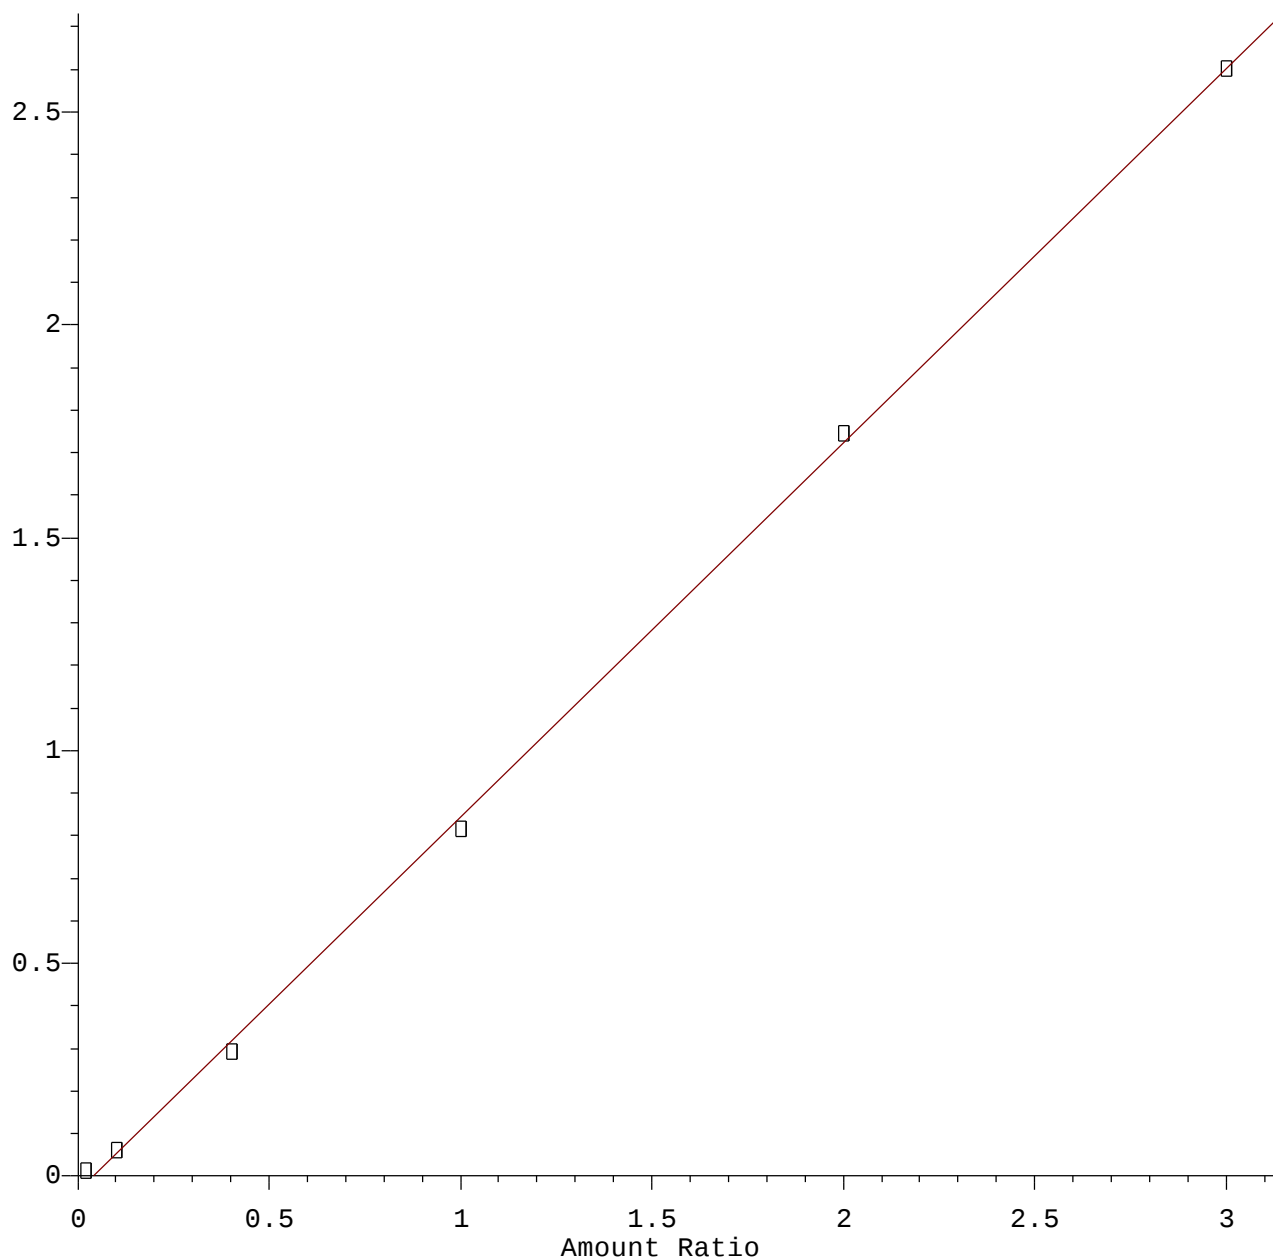

Resp Ratio = 8.78e-001 \* Amt - 3.41e-002  
Coef of Det (r<sup>2</sup>) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081418W.M  
Calibration Table Last Updated: Tue Aug 14 08:07:08 2018