


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081418\
Data File : VN050583.D
Acq On : 13 Aug 2018 22:57
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 08:07:08 2018

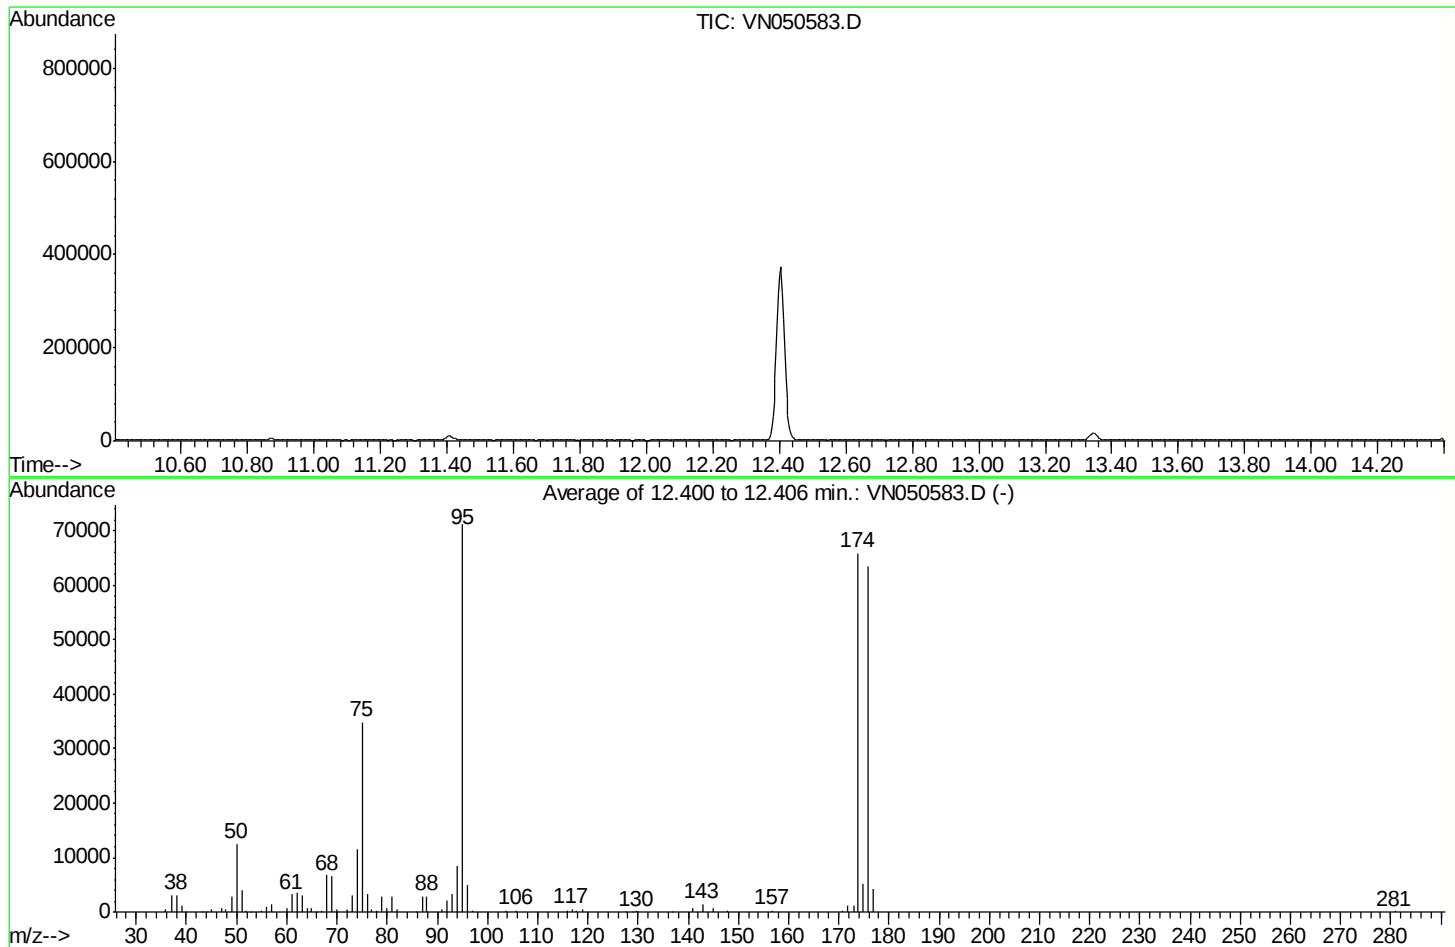

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12584	PASS
75	95	30	60	49.0	34869	PASS
95	95	100	100	100.0	71216	PASS
96	95	5	9	6.9	4919	PASS
173	174	0.00	2	1.6	1083	PASS
174	95	50	100	92.5	65901	PASS
175	174	5	9	8.0	5274	PASS
176	174	95	101	96.2	63424	PASS
177	176	5	9	6.5	4125	PASS