


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081418\
Data File : VN050591.D
Acq On : 14 Aug 2018 10:11
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 08:07:08 2018

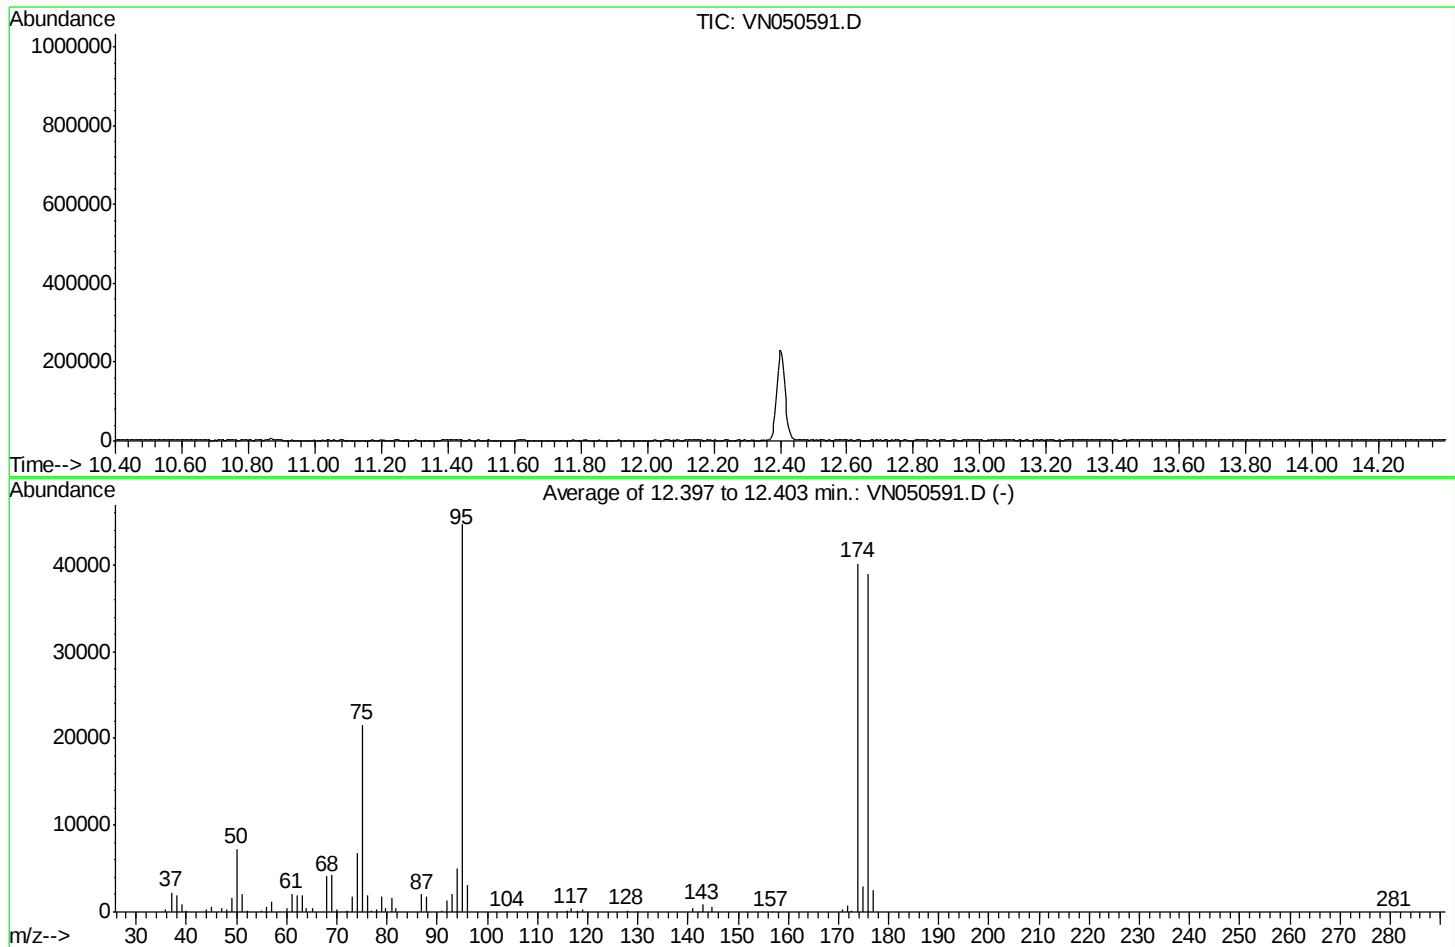

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7249	PASS
75	95	30	60	48.4	21621	PASS
95	95	100	100	100.0	44688	PASS
96	95	5	9	6.9	3096	PASS
173	174	0.00	2	0.4	163	PASS
174	95	50	100	89.8	40136	PASS
175	174	5	9	7.5	3011	PASS
176	174	95	101	97.2	39005	PASS
177	176	5	9	6.4	2494	PASS