


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081418\
 Data File : VN050616.D
 Acq On : 14 Aug 2018 21:21
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Title : SW846 8260
 Last Update : Tue Aug 14 08:07:08 2018

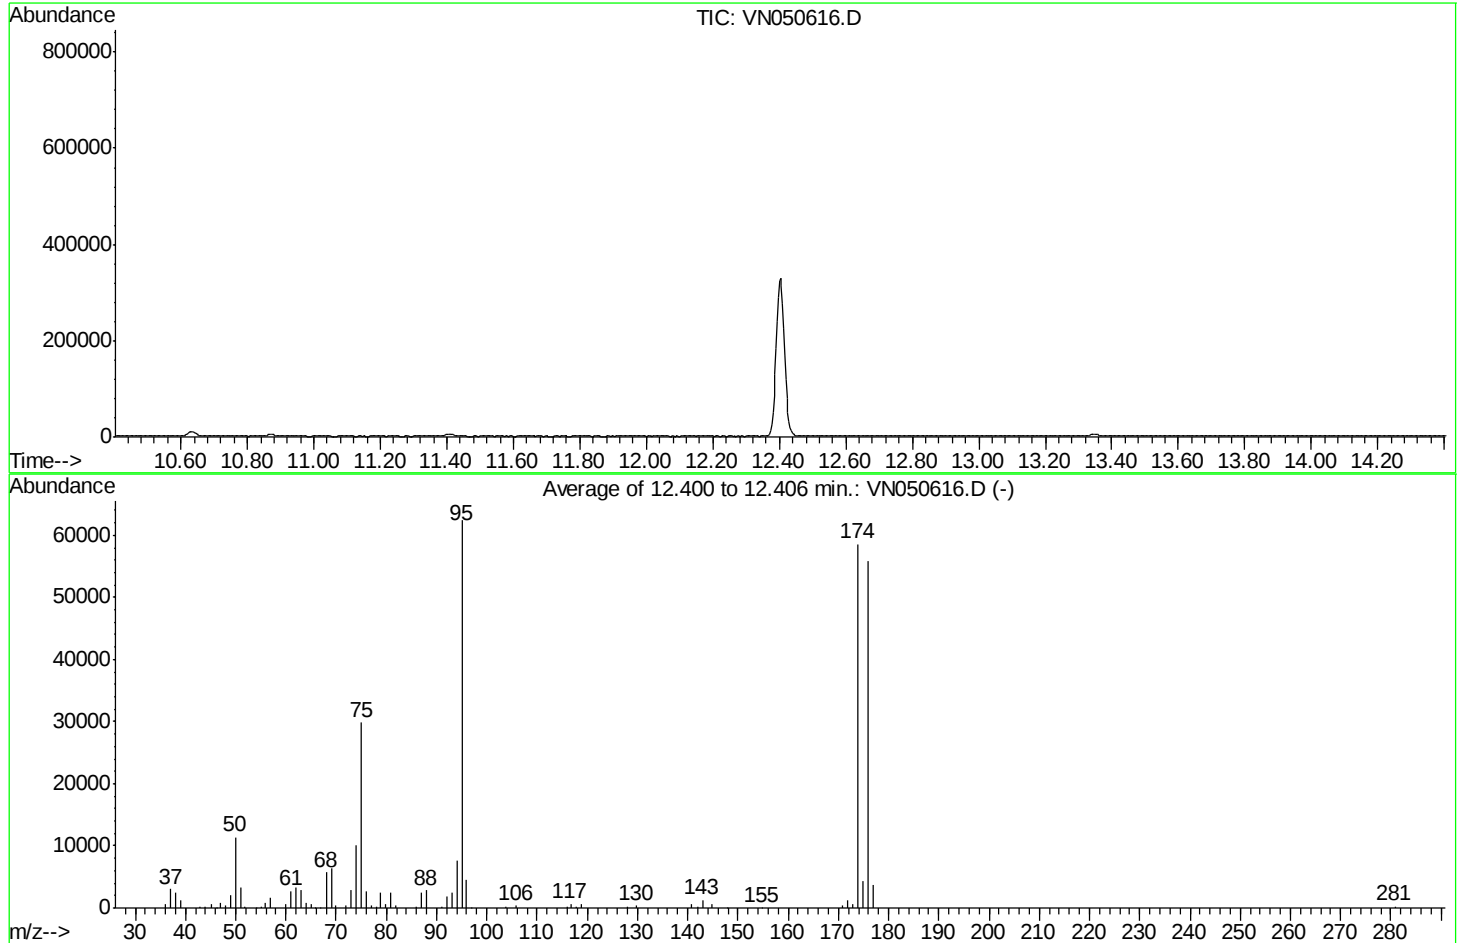

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	11436	PASS
75	95	30	60	47.8	29858	PASS
95	95	100	100	100.0	62400	PASS
96	95	5	9	7.2	4462	PASS
173	174	0.00	2	1.2	686	PASS
174	95	50	100	93.9	58597	PASS
175	174	5	9	7.4	4345	PASS
176	174	95	101	95.4	55880	PASS
177	176	5	9	6.8	3808	PASS