


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081420\
 Data File : VN062926.D
 Acq On : 13 Aug 2020 21:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N081420W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Aug 14 06:20:27 2020

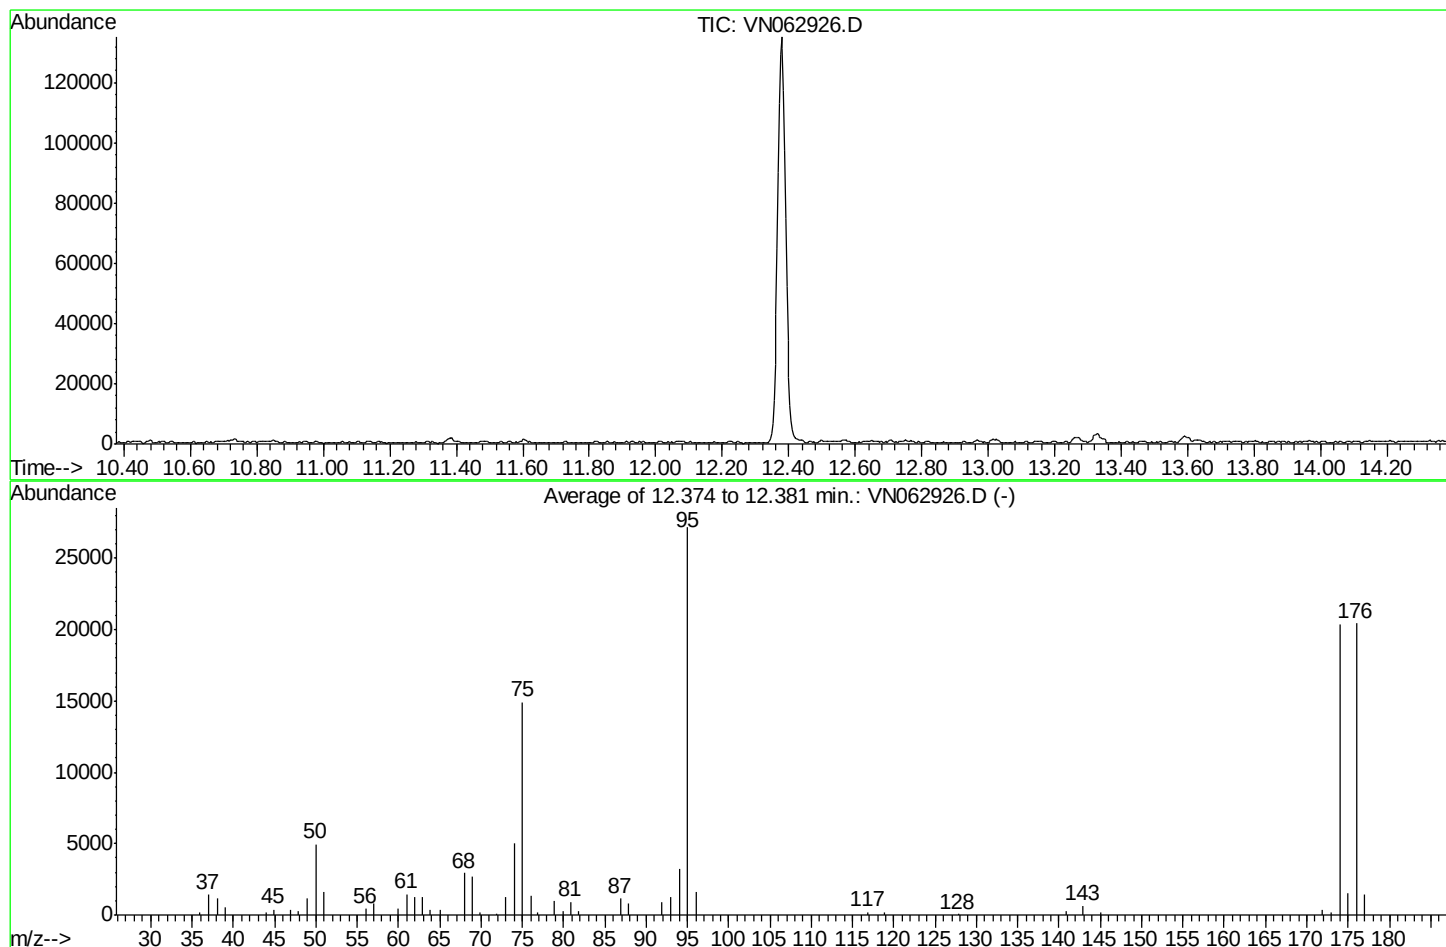

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3286

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	4967	PASS
75	95	30	60	54.9	14915	PASS
95	95	100	100	100.0	27165	PASS
96	95	5	9	5.9	1614	PASS
173	174	0.00	2	0.8	159	PASS
174	95	50	100	75.0	20384	PASS
175	174	5	9	7.7	1569	PASS
176	174	95	101	100.3	20440	PASS
177	176	5	9	7.1	1449	PASS