


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081420\
 Data File : VN062933.D
 Acq On : 14 Aug 2020 11:06
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N081420W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Aug 14 06:20:27 2020

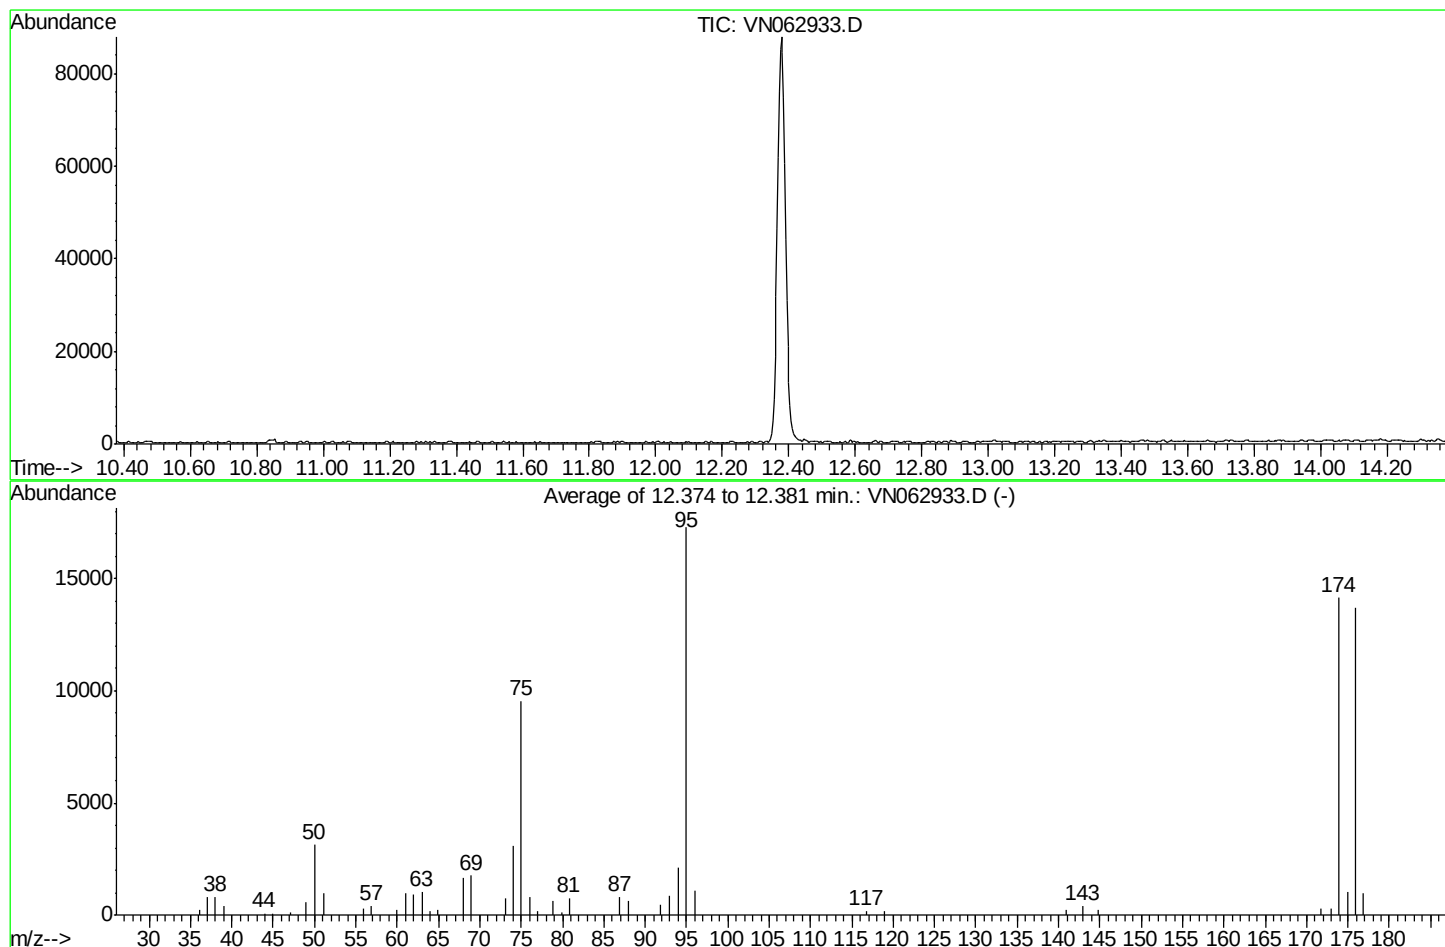

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3286

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	3139	PASS
75	95	30	60	55.3	9561	PASS
95	95	100	100	100.0	17301	PASS
96	95	5	9	6.4	1100	PASS
173	174	0.00	2	1.9	263	PASS
174	95	50	100	81.8	14151	PASS
175	174	5	9	7.3	1039	PASS
176	174	95	101	96.7	13689	PASS
177	176	5	9	7.0	956	PASS