


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081420\
 Data File : VN062941.D
 Acq On : 14 Aug 2020 17:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
 Title : SW846 8260
 Last Update : Wed Aug 05 13:26:42 2020

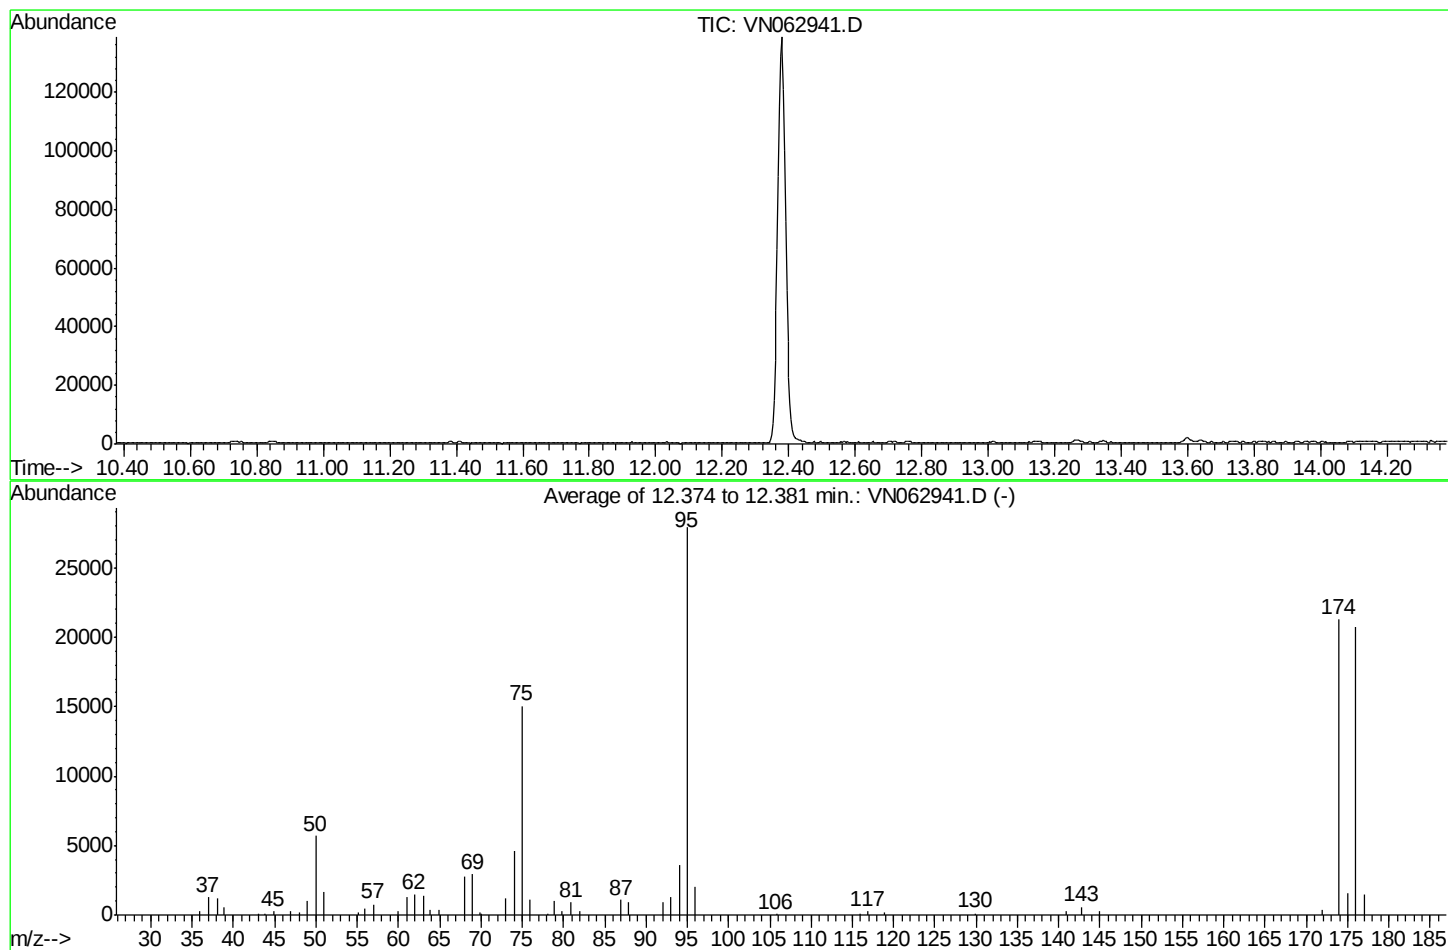

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	5704	PASS
75	95	30	60	54.0	15066	PASS
95	95	100	100	100.0	27909	PASS
96	95	5	9	7.2	1997	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.2	21277	PASS
175	174	5	9	7.3	1545	PASS
176	174	95	101	97.5	20749	PASS
177	176	5	9	6.9	1438	PASS