

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081425\
 Data File : VN087565.D
 Acq On : 14 Aug 2025 14:58
 Operator : JC\MD
 Sample : Q2842-08
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB01-081225

Quant Time: Aug 14 15:25:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 17 02:56:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.212	168	224412	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	9.088	114	498664	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	458661	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	214662	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	209873	55.117	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	=	110.240%	
35) Dibromofluoromethane	8.153	113	154326	44.865	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	=	89.740%	
50) Toluene-d8	10.547	98	559384	45.589	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	=	91.180%	
62) 4-Bromofluorobenzene	12.829	95	200248	44.173	ug/l	0.00
Spiked Amount	50.000	Range 77 - 121	Recovery	=	88.340%	
Target Compounds						
16) Acetone	4.424	43	8905	4.988	ug/l	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081425\
Data File : VN087565.D
Acq On : 14 Aug 2025 14:58
Operator : JC\MD
Sample : Q2842-08
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB01-081225

Quant Time: Aug 14 15:25:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 17 02:56:13 2025
Response via : Initial Calibration




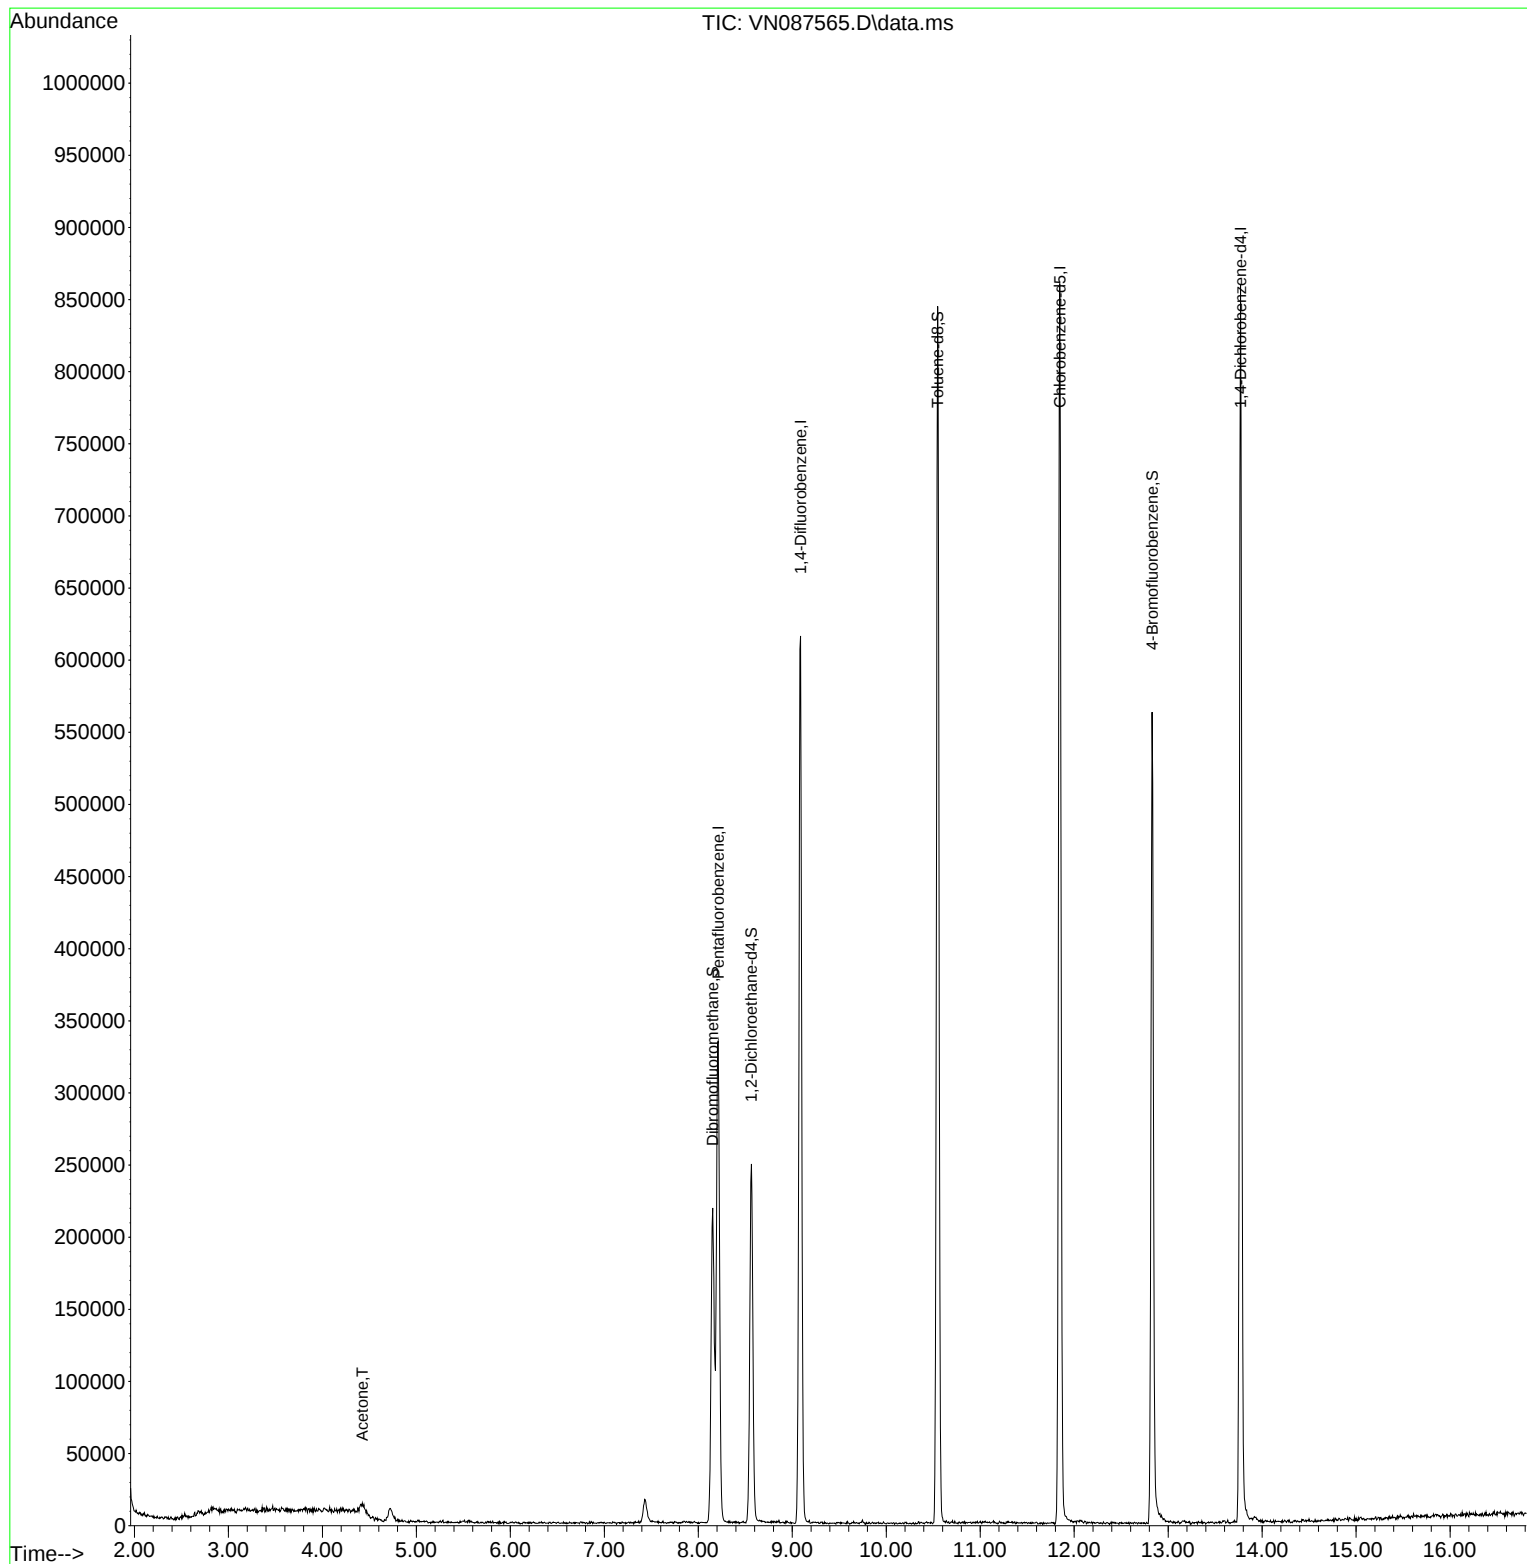


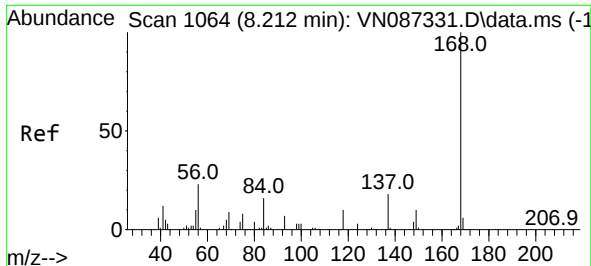

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. -0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58




Instrument :
MSVOA_N
ClientSampleId :
TB01-081225


Tgt Ion:168 Resp: 224412
Ion Ratio Lower Upper
168 100
99 72.0 47.9 71.9#

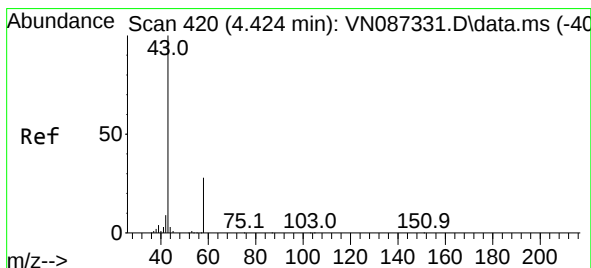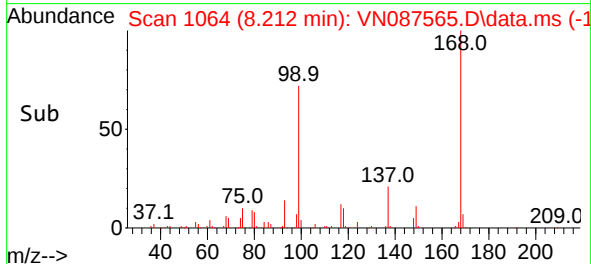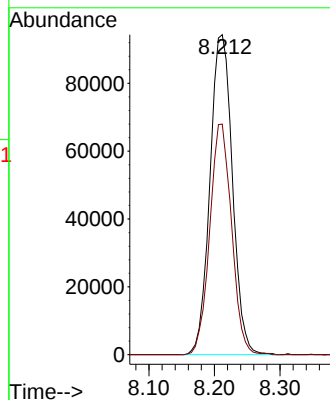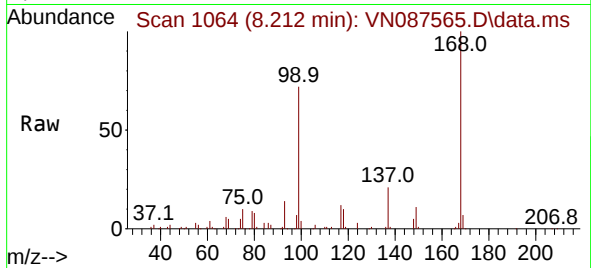

#16
Acetone
Concen: 4.988 ug/l
RT: 4.424 min Scan# 420
Delta R.T. 0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58

Tgt Ion: 43 Resp: 8905
Ion Ratio Lower Upper
43 100
58 21.4 22.3 33.5#


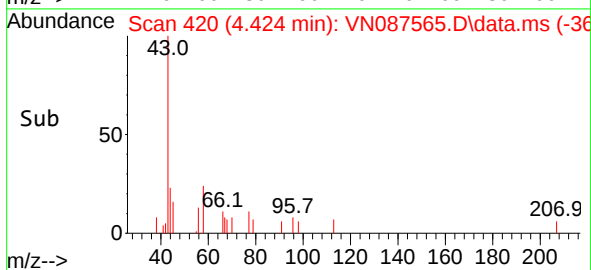
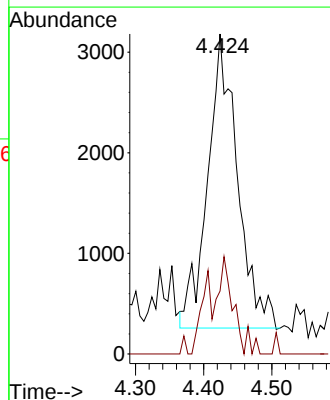
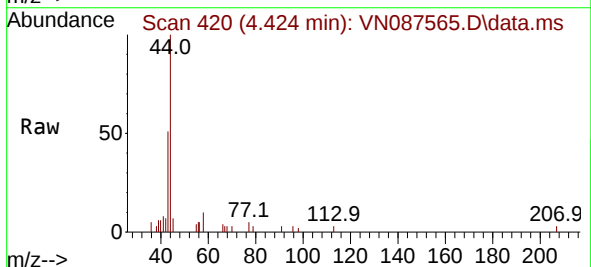


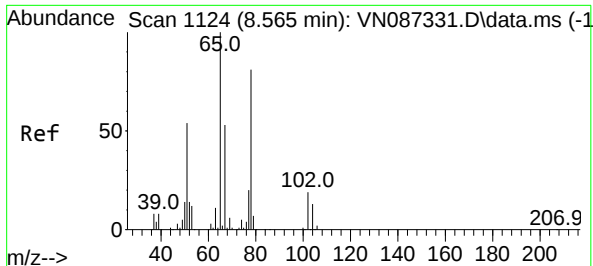

#33
1,2-Dichloroethane-d4
Concen: 55.117 ug/l
RT: 8.565 min Scan# 1124
Delta R.T. 0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58




Instrument :
MSVOA_N
ClientSampleId :
TB01-081225


Tgt Ion: 65 Resp: 209873
Ion Ratio Lower Upper
65 100
67 50.1 0.0 104.0

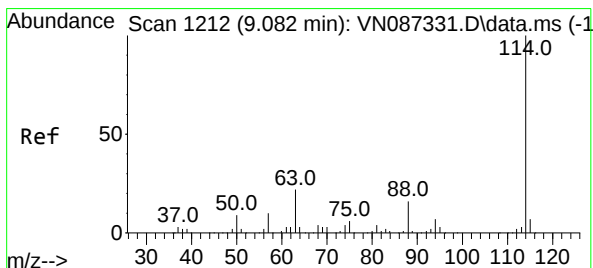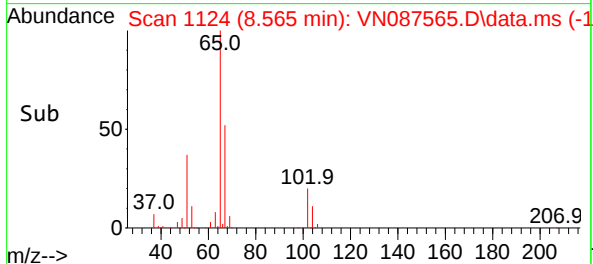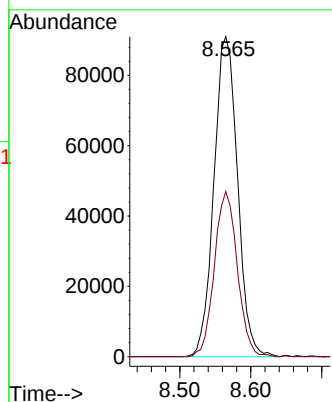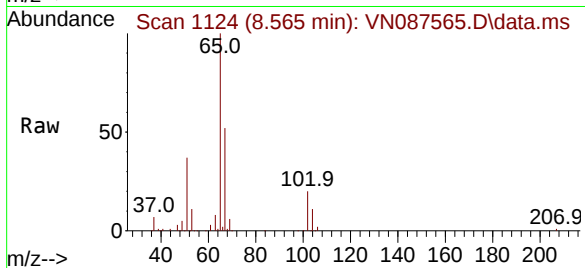

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.088 min Scan# 1213
Delta R.T. 0.006 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58

Tgt Ion: 114 Resp: 498664
Ion Ratio Lower Upper
114 100
63 23.0 0.0 44.6
88 16.0 0.0 32.8


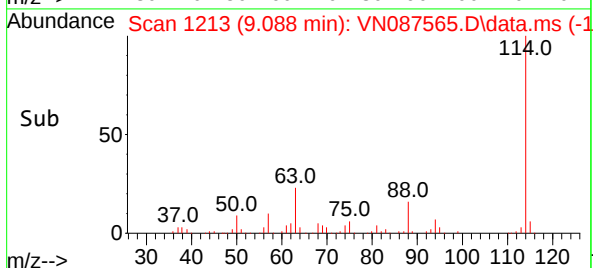
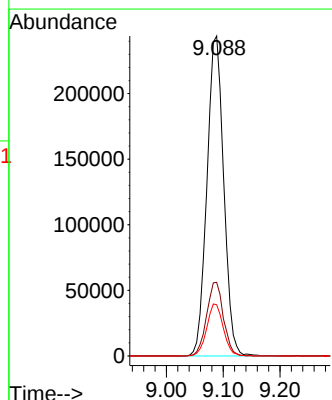
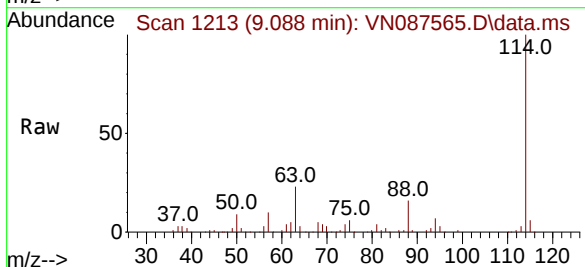


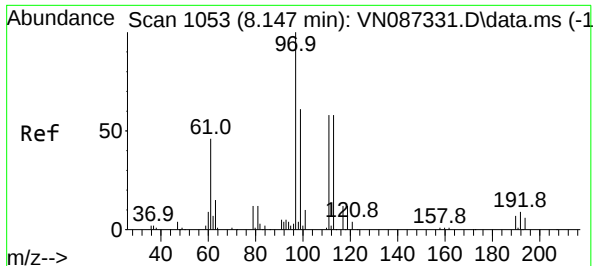

#35
Dibromofluoromethane
Concen: 44.865 ug/l
RT: 8.153 min Scan# 1054
Delta R.T. 0.006 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58




Instrument :
MSVOA_N
ClientSampleId :
TB01-081225


Tgt Ion:113 Resp: 154326
Ion Ratio Lower Upper
113 100
111 103.2 82.5 123.7
192 15.9 13.7 20.5

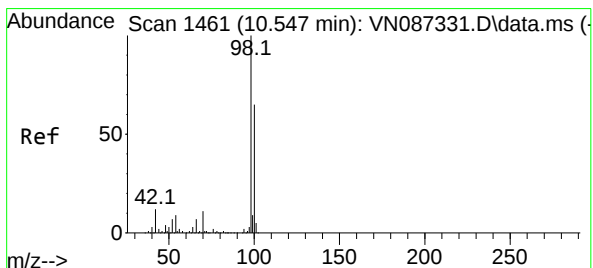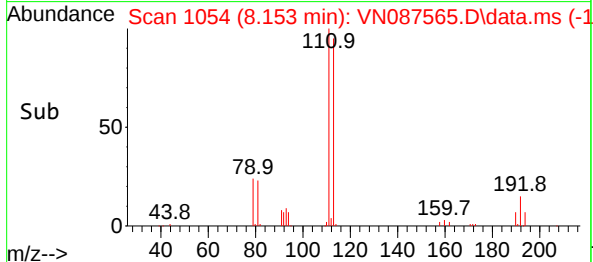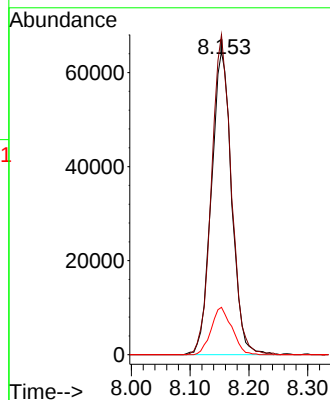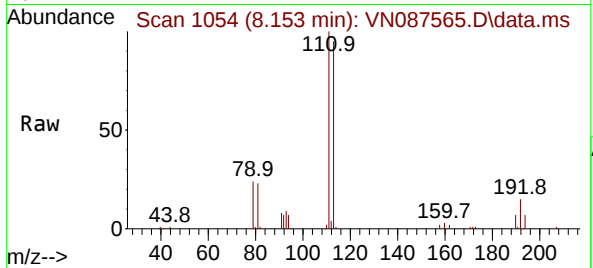

#50
Toluene-d8
Concen: 45.589 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. 0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58

Tgt Ion: 98 Resp: 559384
Ion Ratio Lower Upper
98 100
100 64.6 52.1 78.1


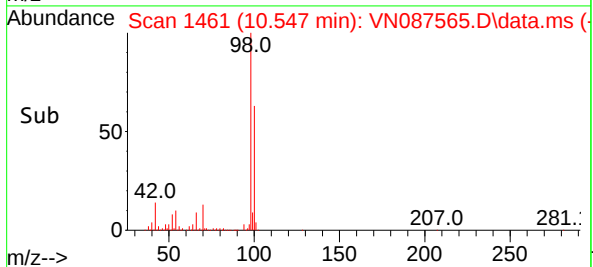
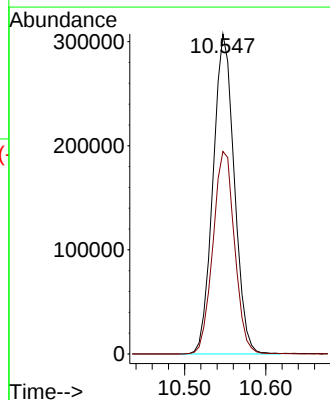
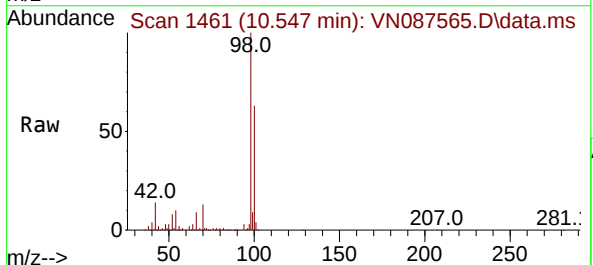


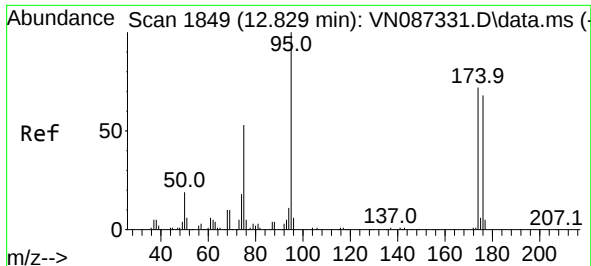

#62
4-Bromofluorobenzene
Concen: 44.173 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58




Instrument :
MSVOA_N
ClientSampleId :
TB01-081225


Tgt Ion: 95 Resp: 200248
Ion Ratio Lower Upper
95 100
174 68.6 0.0 149.4
176 63.7 0.0 141.2

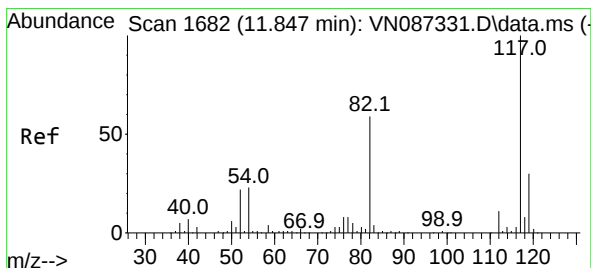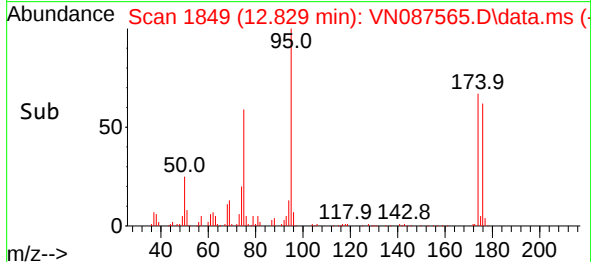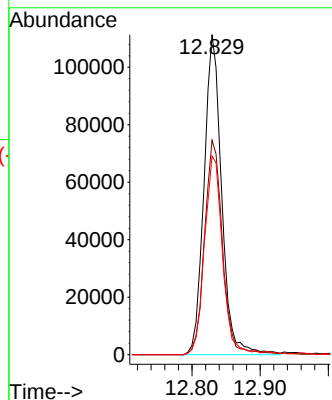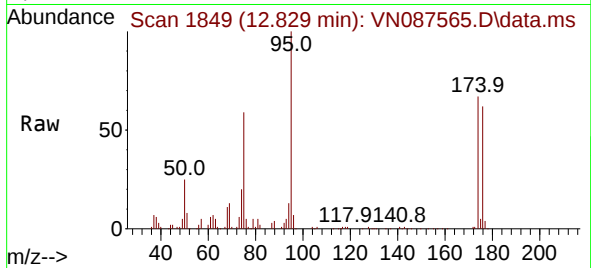

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 1682
Delta R.T. -0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58


Tgt Ion: 117 Resp: 458661
Ion Ratio Lower Upper
117 100
82 63.8 47.4 71.2
119 32.1 23.8 35.8

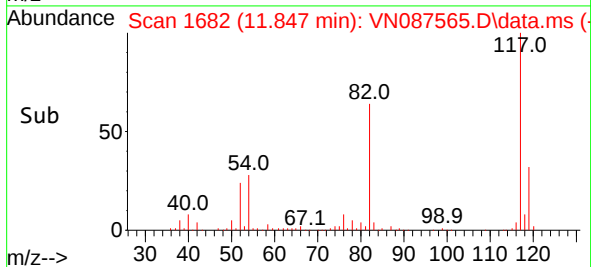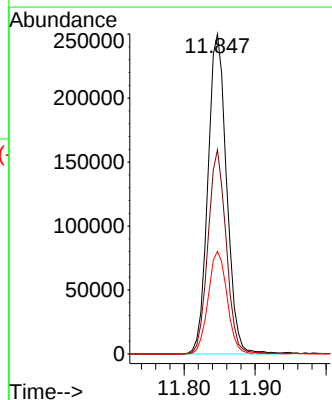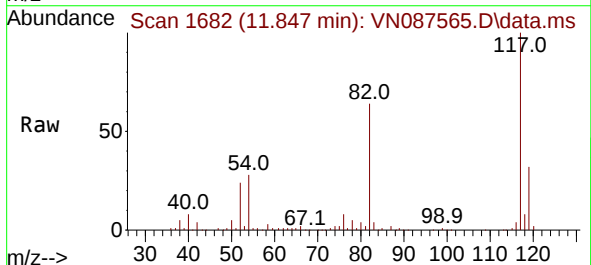

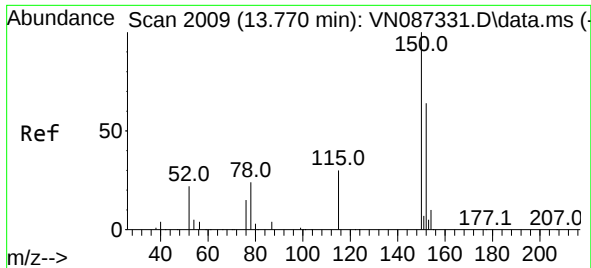

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 20
Delta R.T. 0.000 min
Lab File: VN087565.D
Acq: 14 Aug 2025 14:58

Instrument :
MSVOA_N
ClientSampleId :
TB01-081225

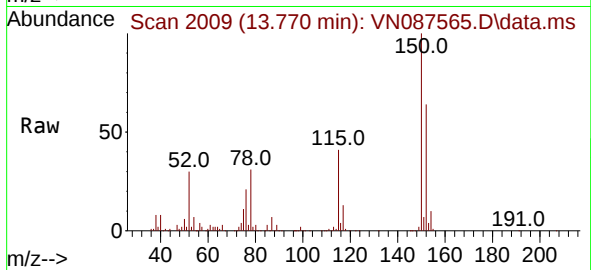

Tgt Ion	Ratio	Lower	Upper
152	100		
115	64.0	31.1	93.5
150	156.9	0.0	349.0

