
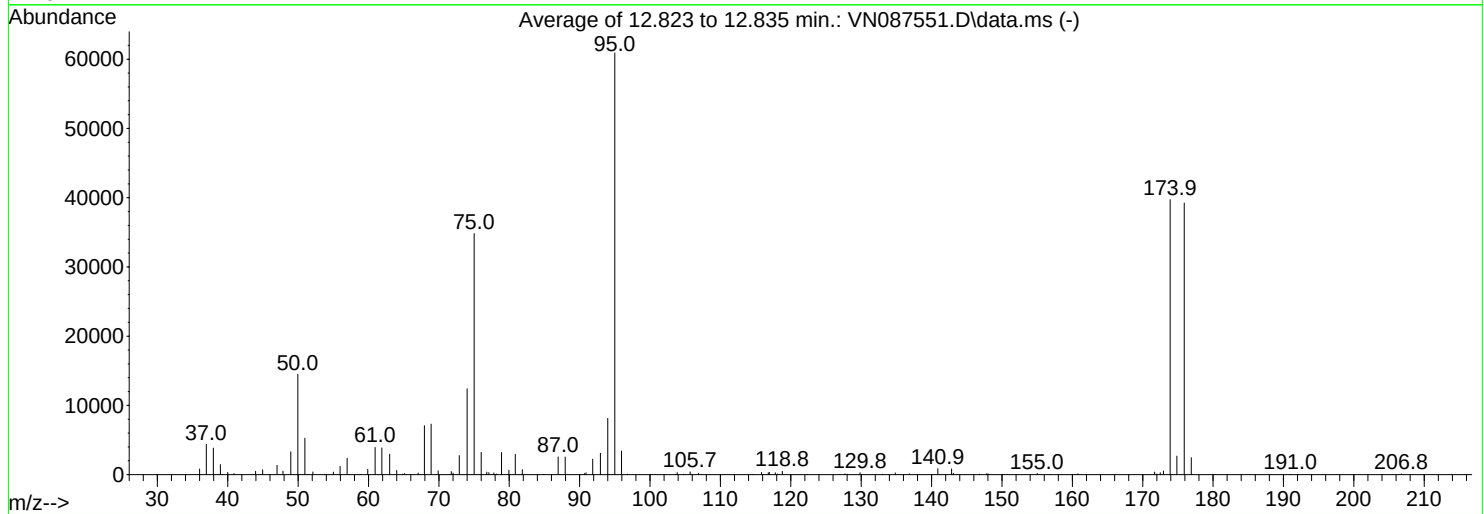


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081425\
Data File : VN087551.D
Acq On : 14 Aug 2025 09:01
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

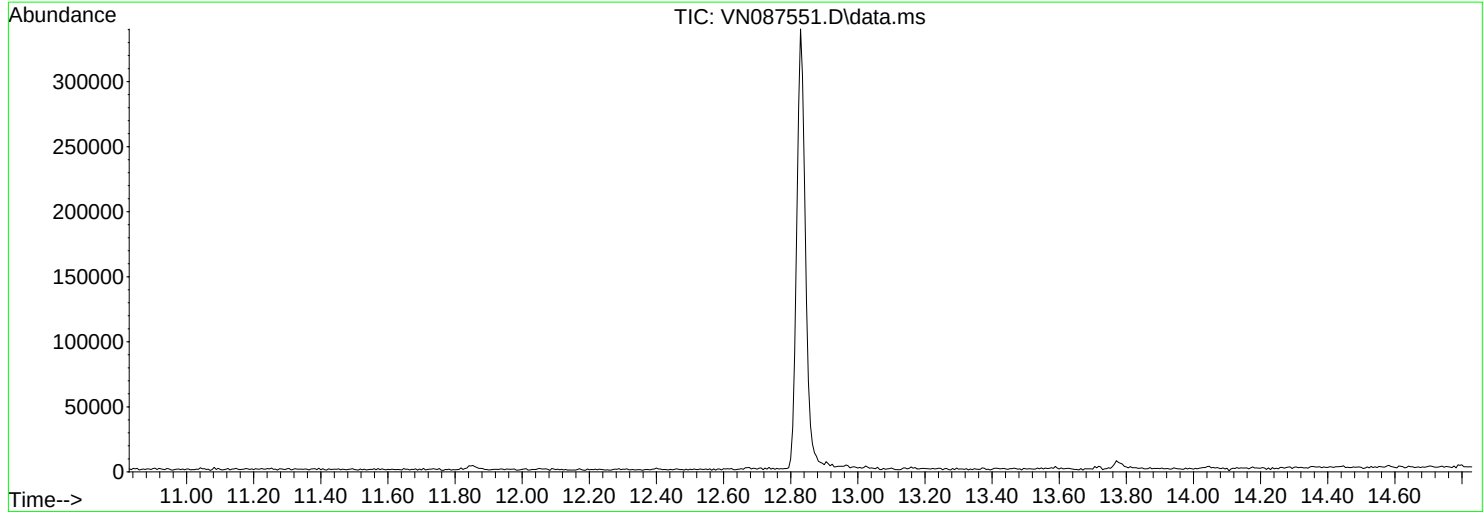

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.8	14484	PASS
75	95	30	60	57.2	34829	PASS
95	95	100	100	100.0	60920	PASS
96	95	5	9	5.6	3407	PASS
173	174	0.00	2	1.3	536	PASS
174	95	50	100	65.2	39723	PASS
175	174	5	9	6.8	2685	PASS
176	174	95	101	98.8	39240	PASS
177	176	5	9	6.2	2451	PASS

Average of 12.823 to 12.835 min.: VN087551.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	805	49.95	14484	63.00	2963	74.00	1241
36.95	4361	50.95	5265	64.00	607	75.00	3482
37.95	3826	52.10	400	64.80	64	76.00	321
38.95	1459	53.80	50	65.10	174	76.80	37
40.00	321	55.00	367	67.05	225	77.10	310
40.90	158	55.95	1213	67.95	7067	77.80	254
43.95	478	56.95	2372	68.90	7296	78.20	87
44.95	699	58.80	53	69.90	564	78.90	3182
47.00	1337	59.90	752	71.75	448	79.95	646
47.85	509	60.95	3931	72.00	227	80.85	2939
48.95	3305	61.90	3852	72.90	2741	81.85	729

Average of 12.823 to 12.835 min.: VN087551.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
84.90	53	103.60	56	118.80	492	143.70	53
86.95	2577	103.85	295	122.40	52	146.80	70
87.95	2550	104.80	79	127.70	126	147.80	109
90.70	164	105.70	404	128.10	73	148.00	129
90.90	275	106.90	186	129.85	282	155.00	182
91.85	2248	114.60	54	133.00	81	156.90	53
92.95	3098	115.85	328	134.85	244	160.80	136
94.00	8132	116.80	285	136.85	122	171.70	369
95.00	60920	116.95	325	140.90	863	172.00	97
95.95	3407	117.80	270	142.85	826	172.50	283
96.80	81	118.10	99	143.10	183	172.95	536

Average of 12.823 to 12.835 min.: VN087551.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	39723						
174.85	2685						
175.90	39240						
176.90	2451						
191.00	51						
206.75	119						

Instrument :

MSVOA_N

ClientSampleId :

BFB